

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS020119\  
 Data File : PS002998.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 Feb 2019 12:01  
 Operator : EI\SJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 01 12:57:45 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS012819.M  
 Quant Title : 8080.M  
 QLast Update : Tue Jan 29 06:11:45 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1  | Resp#2  | ng/ml | ng/ml     |
|-----------------------------|--------------|--------|--------|---------|---------|-------|-----------|
| -----                       |              |        |        |         |         |       |           |
| System Monitoring Compounds |              |        |        |         |         |       |           |
| 4) S                        | 2,4-DCAA     | 0.000  | 10.782 | 0       | 193.4E6 | N.D.  | 452.437 # |
| Target Compounds            |              |        |        |         |         |       |           |
| 10) T                       | Pentachlo... | 13.510 | 13.196 | 4425637 | 2686761 | 0.690 | 0.435 #   |
| 16) T                       | DCPA         | 0.000  | 16.635 | 0       | 2074328 | N.D.  | 0.670 #   |
| -----                       |              |        |        |         |         |       |           |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS020119\  
Data File : PS002998.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 01 Feb 2019 12:01  
Operator : EI\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 01 12:57:45 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS012819.M  
Quant Title : 8080.M  
QLast Update : Tue Jan 29 06:11:45 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

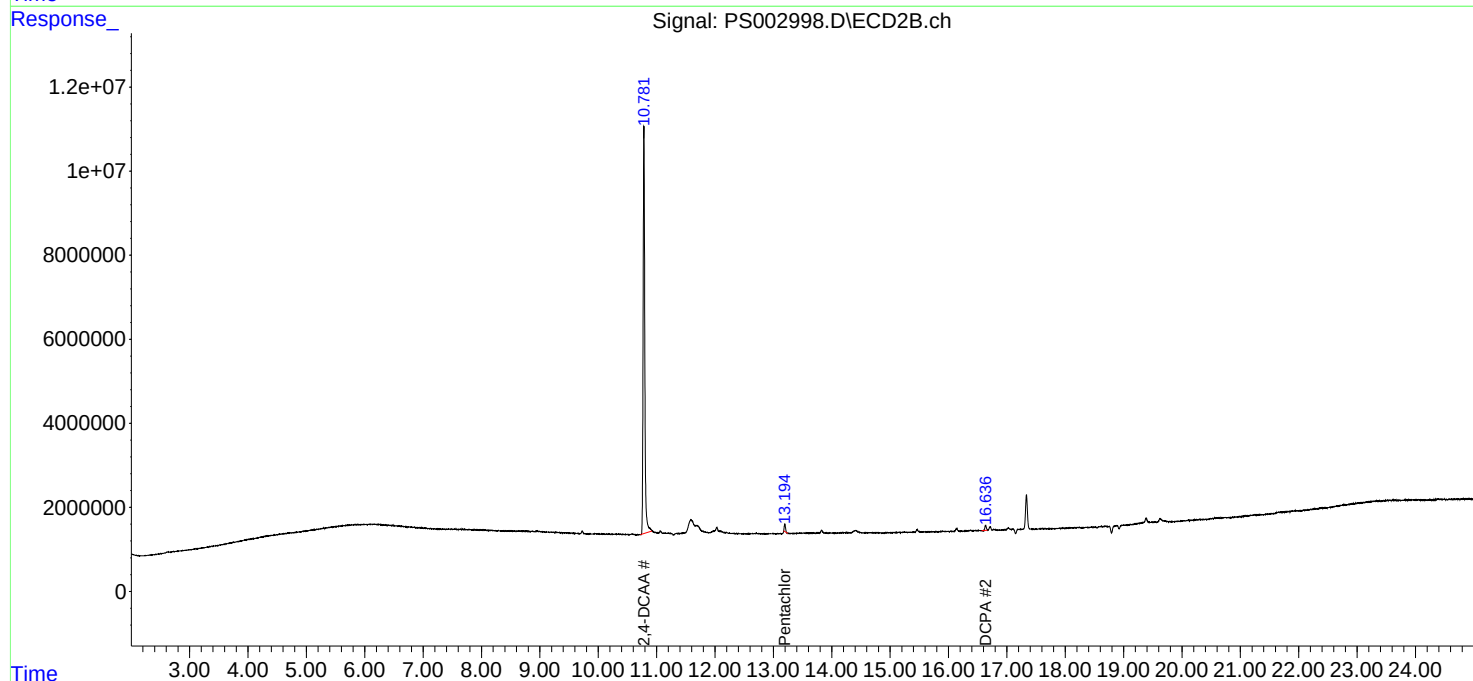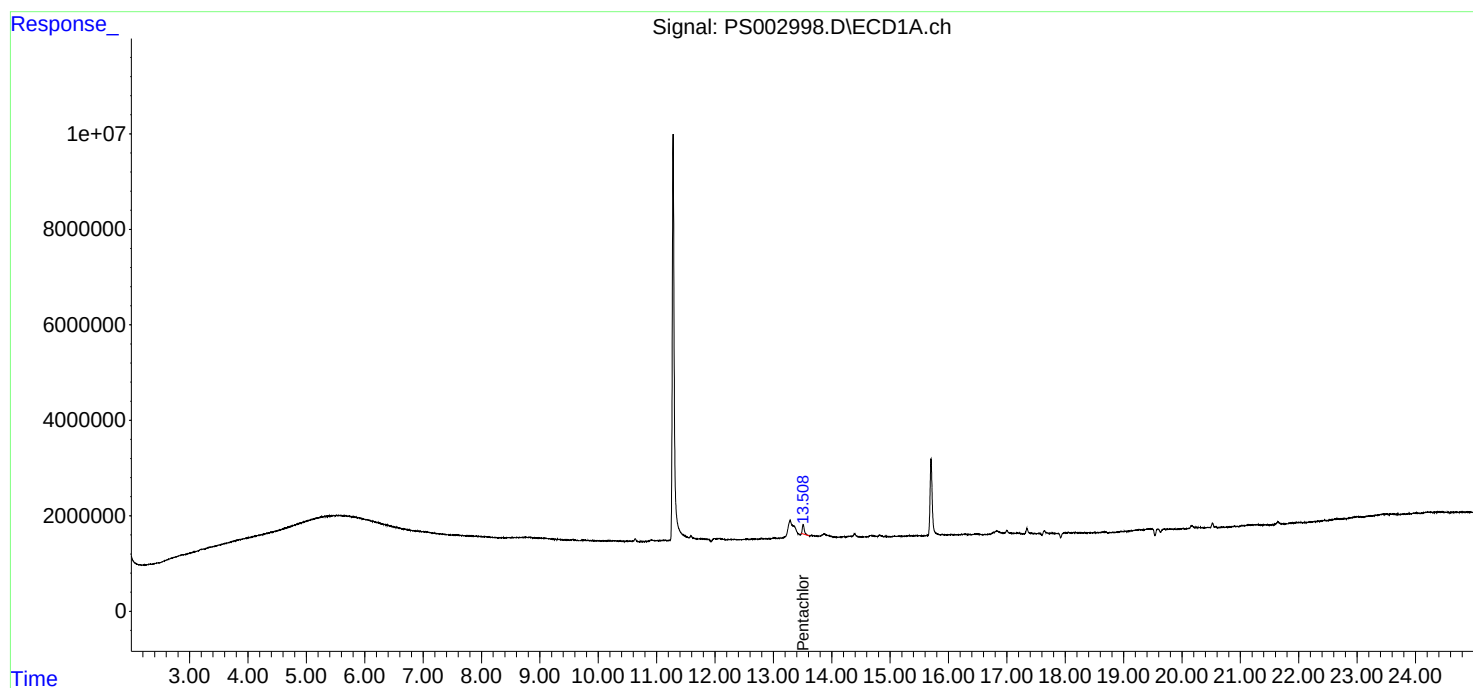


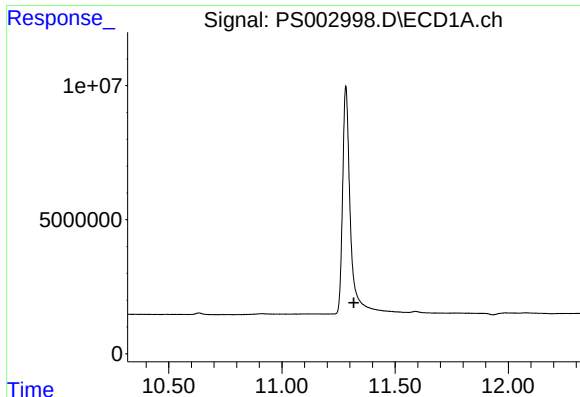

#4 2,4-DCAA


R.T.: 0.000 min  
Exp R.T.: 11.318 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

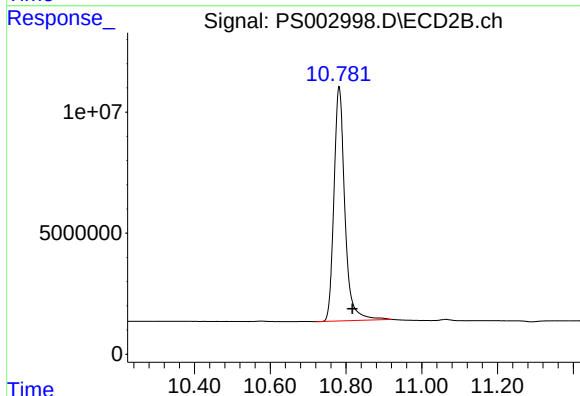


#4 2,4-DCAA

R.T.: 10.782 min  
Delta R.T.: -0.035 min  
Response: 193437332  
Conc: 452.44 ng/ml

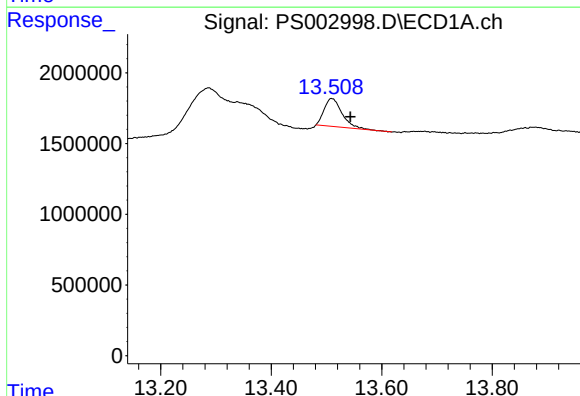


#10 Pentachlorophenol

R.T.: 13.510 min  
Delta R.T.: -0.034 min  
Response: 4425637  
Conc: 0.69 ng/ml

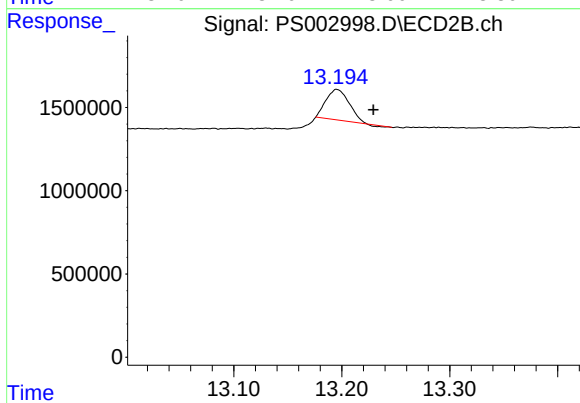

#10 Pentachlorophenol


R.T.: 13.196 min  
Delta R.T.: -0.034 min  
Response: 2686761  
Conc: 0.43 ng/ml

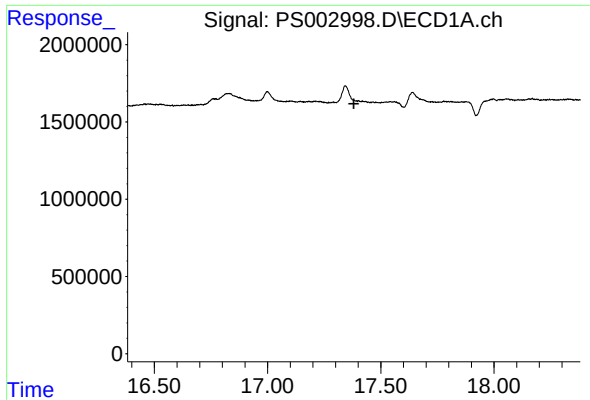

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 17.382 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

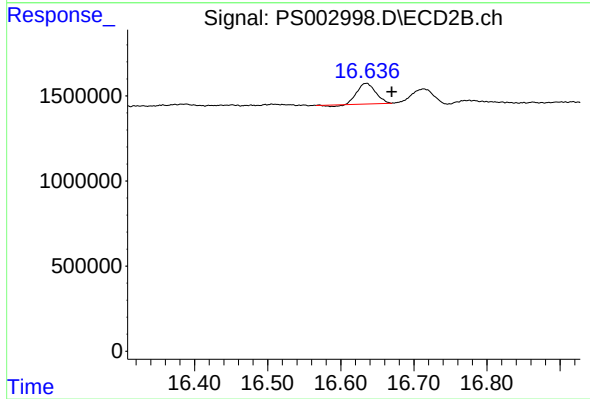

#16 DCPA

R.T.: 16.635 min  
Delta R.T.: -0.035 min  
Response: 2074328  
Conc: 0.67 ng/ml