

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020122\
 Data File : PS018203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2022 19:53
 Operator : AJ\MA
 Sample : N1325-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 00:19:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.040	6.647	565.4E6	219.6E6	391.176	378.373
Target Compounds							
1) T	Dalapon	0.000	2.376f	0 18800867	N.D.	24.586	
2) T	3,5-DICHL...	6.320	5.887	11836332	124.3E6	5.502	140.539 #
3) T	4-Nitroph...	6.886	6.327	332.4E6	70623225	411.528	230.402 #
5) T	DICAMBA	7.237	6.769	3414333	109.8E6	<MDL	41.765 #
6) T	MCP	7.392	6.896	12791949	22607322	2.740	10.510 #
7) T	MCPA	7.541	7.110	44976156	37488790	6.741	12.564 #
8) T	DICHLORPROP	7.935	7.433	61987014	49153762	39.406	73.647 #
9) T	2,4-D	8.151	7.728	112.4E6	118.9E6	61.717	161.529 #
10) T	Pentachlo...	8.460	8.085	615.7E6	18038609	29.143	2.142 #
11) T	2,4,5-TP ...	8.985	8.509	27573815	544.0E6	3.258	152.614 #
12) T	2,4,5-T	9.334f	8.849	962.6E6	63140128	108.596	19.303 #
13) T	2,4-DB	9.804	9.371	1568.5E6	721.1E6	948.834	1629.735 #
14) T	DINOSEB	10.930	9.672	4080.8E6	594.0E6	621.420	238.081 #
15) T	Picloram	10.767	10.674	47114.1E6	4622.7E6	3947.254	988.581 #
16) T	DCPA	11.218	10.597	438.3E6	206.7E6	40.565	46.816



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020122\
Data File : PS018203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2022 19:53
Operator : AJ\MA
Sample : N1325-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 00:19:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

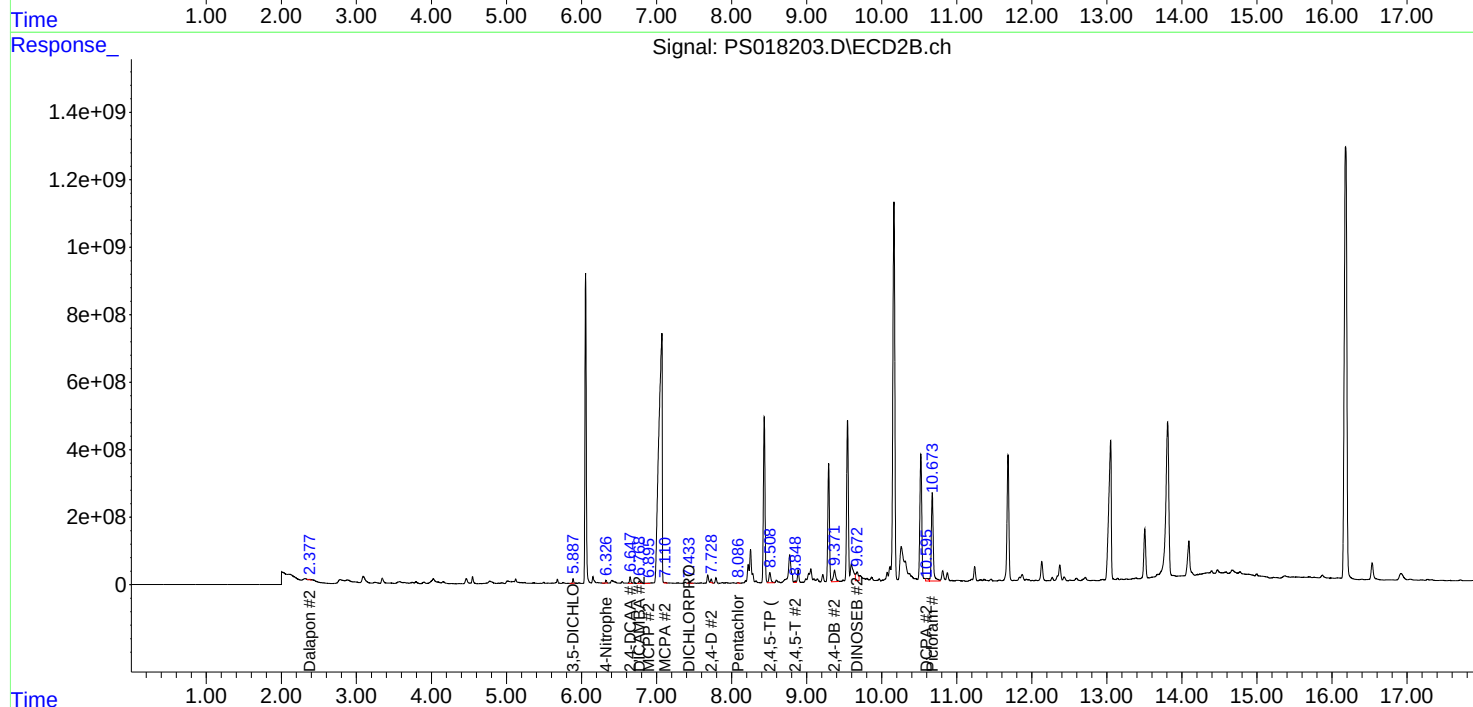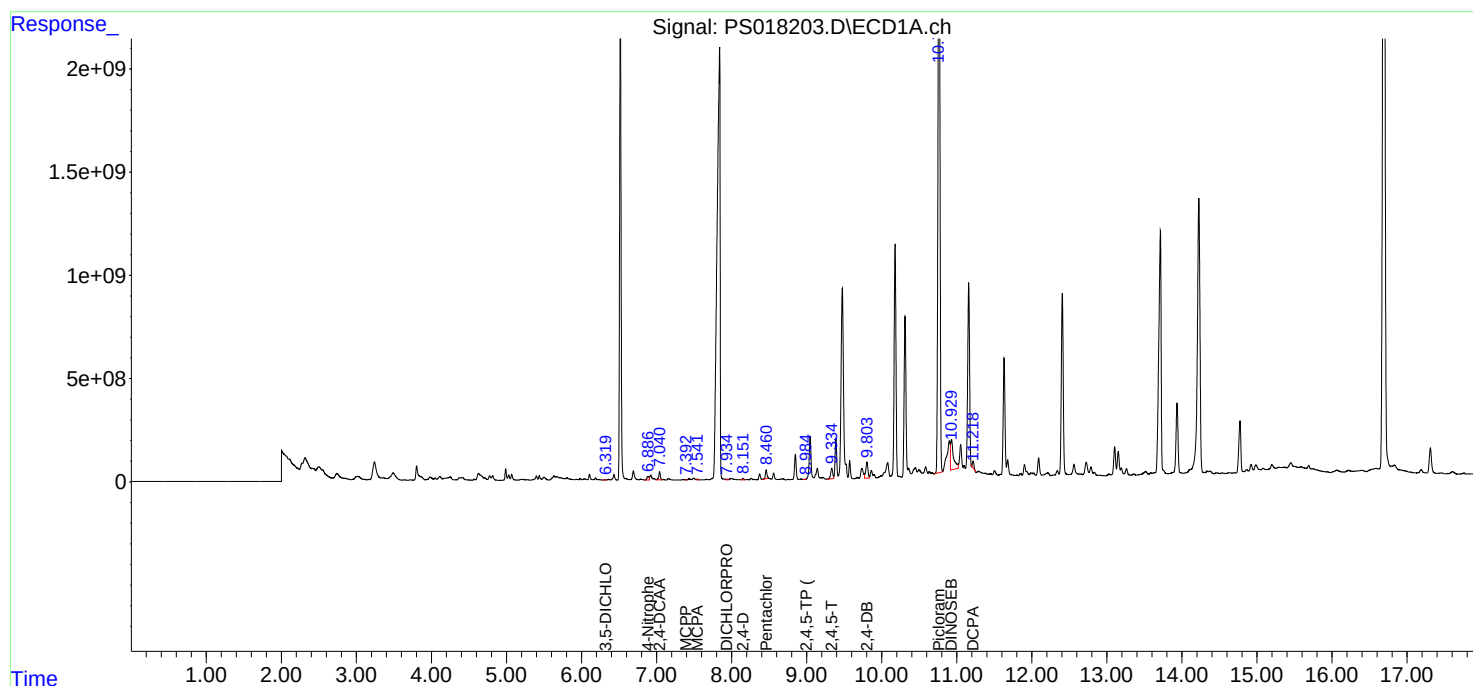


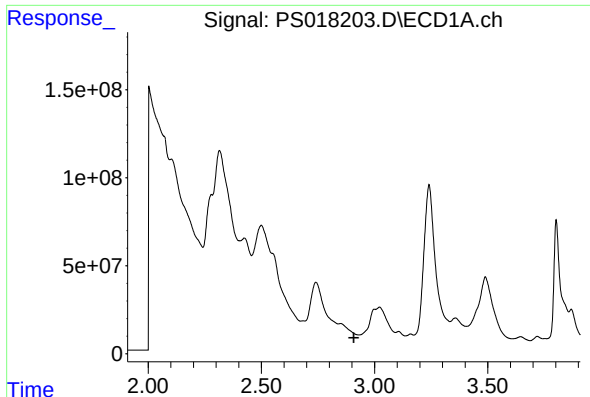

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

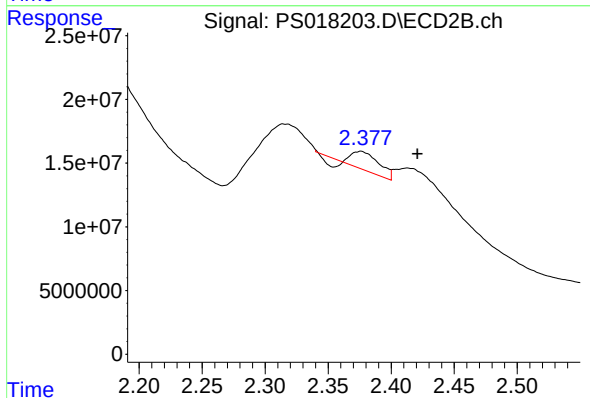


#1 Dalapon

R.T.: 2.376 min
Delta R.T.: -0.045 min
Response: 18800867
Conc: 24.59 ng/ml

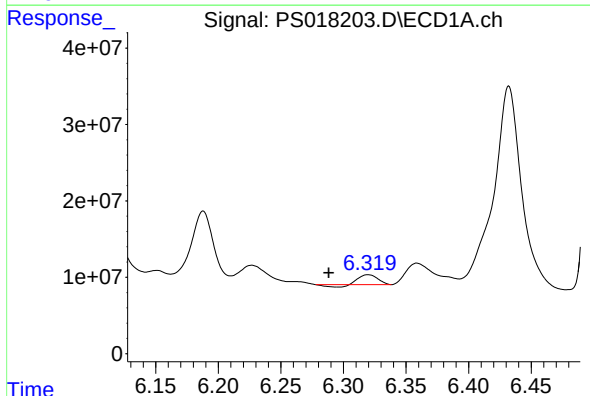


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.320 min
Delta R.T.: 0.032 min
Response: 11836332
Conc: 5.50 ng/ml

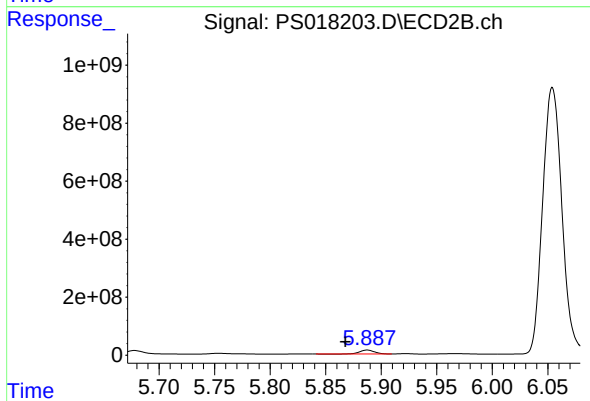

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.887 min
Delta R.T.: 0.019 min
Response: 124324952
Conc: 140.54 ng/ml

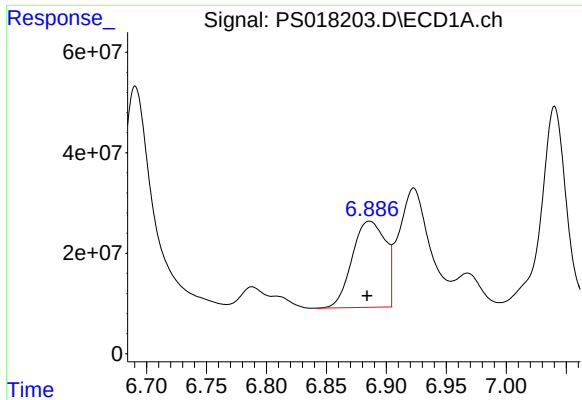

#3 4-Nitrophenol


R.T.: 6.886 min
Delta R.T.: 0.002 min
Response: 332384559
Conc: 411.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

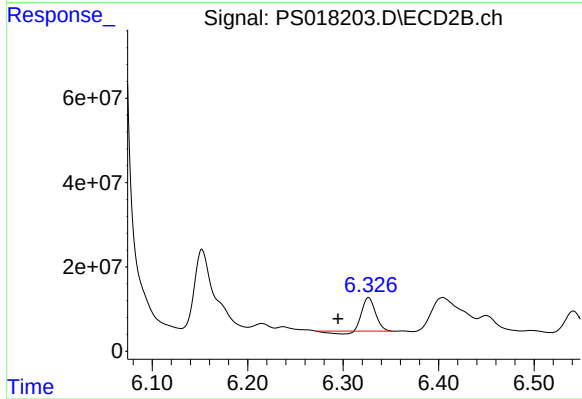


#3 4-Nitrophenol

R.T.: 6.327 min
Delta R.T.: 0.032 min
Response: 70623225
Conc: 230.40 ng/ml

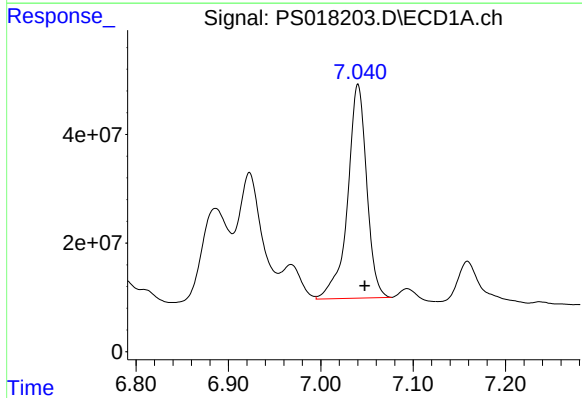


#4 2,4-DCAA

R.T.: 7.040 min
Delta R.T.: -0.007 min
Response: 565440347
Conc: 391.18 ng/ml

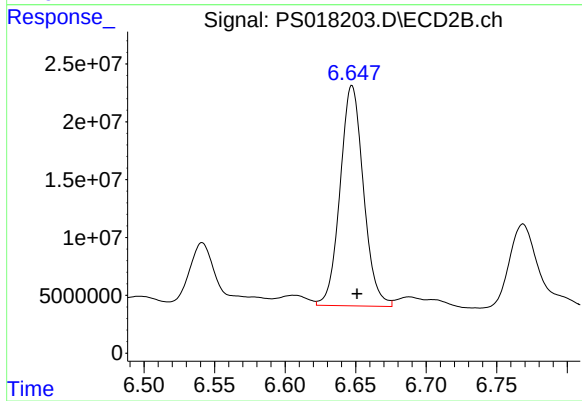

#4 2,4-DCAA


R.T.: 6.647 min
Delta R.T.: -0.003 min
Response: 219550748
Conc: 378.37 ng/ml

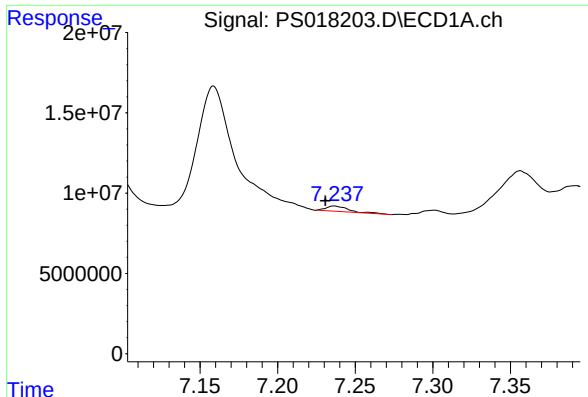

#5 DICAMBA


R.T.: 7.237 min
Delta R.T.: 0.006 min
Response: 3414333
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

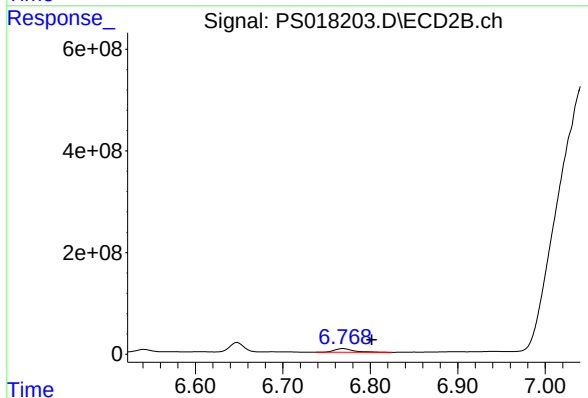


#5 DICAMBA

R.T.: 6.769 min
Delta R.T.: -0.033 min
Response: 109802776
Conc: 41.77 ng/ml

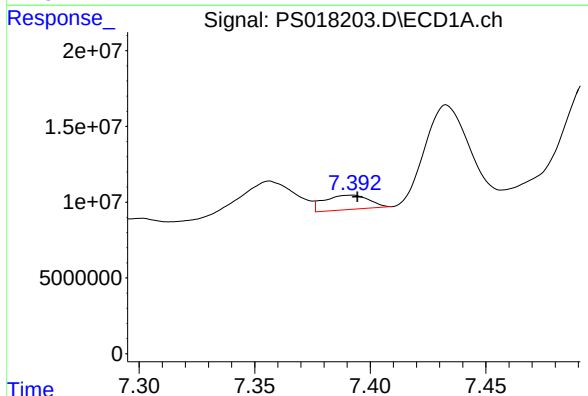


#6 MCP

R.T.: 7.392 min
Delta R.T.: -0.003 min
Response: 12791949
Conc: 2.74 ug/ml

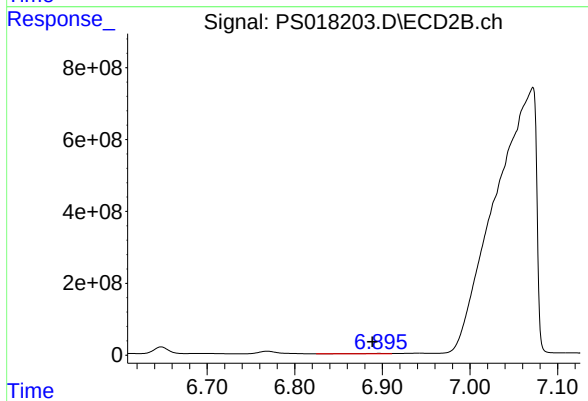

#6 MCP


R.T.: 6.896 min
Delta R.T.: 0.008 min
Response: 22607322
Conc: 10.51 ug/ml

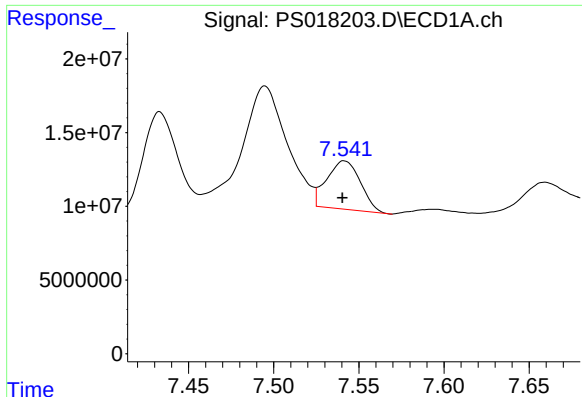

#7 MCPA


R.T.: 7.541 min
Delta R.T.: 0.001 min
Response: 44976156
Conc: 6.74 ug/ml

Instrument :
ECD_S
ClientSampleId :

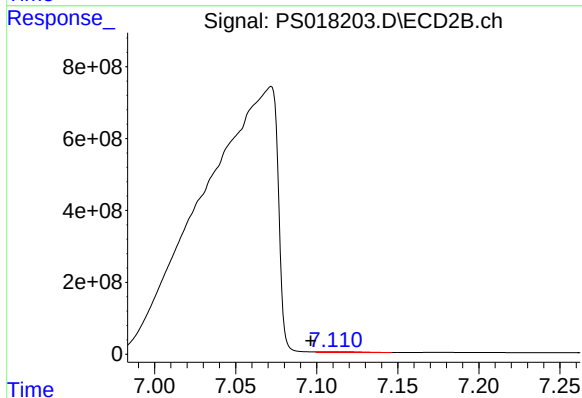


#7 MCPA

R.T.: 7.110 min
Delta R.T.: 0.014 min
Response: 37488790
Conc: 12.56 ug/ml

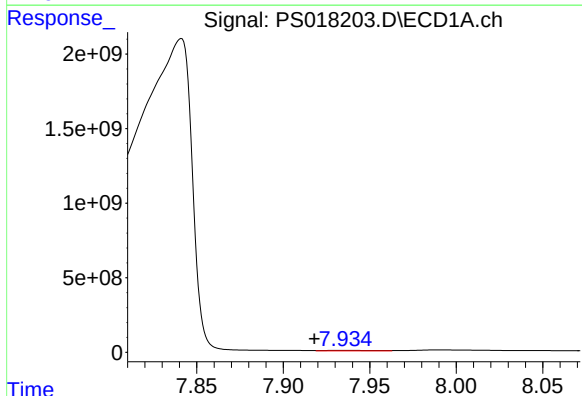


#8 DICHLORPROP

R.T.: 7.935 min
Delta R.T.: 0.017 min
Response: 61987014
Conc: 39.41 ng/ml

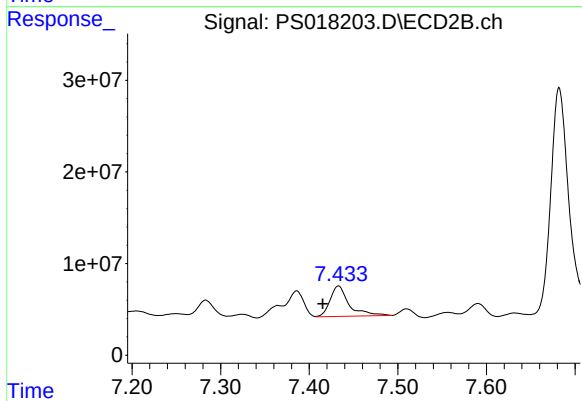

#8 DICHLORPROP


R.T.: 7.433 min
Delta R.T.: 0.018 min
Response: 49153762
Conc: 73.65 ng/ml

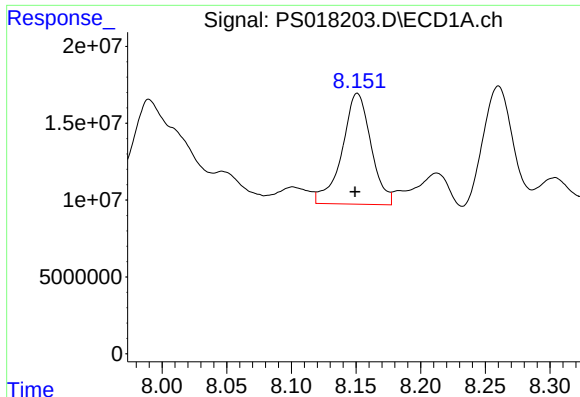

#9 2,4-D


R.T.: 8.151 min
Delta R.T.: 0.002 min
Response: 112382397
Conc: 61.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

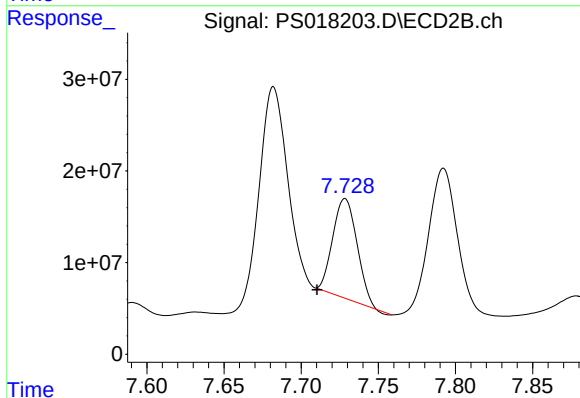


#9 2,4-D

R.T.: 7.728 min
Delta R.T.: 0.018 min
Response: 118876484
Conc: 161.53 ng/ml

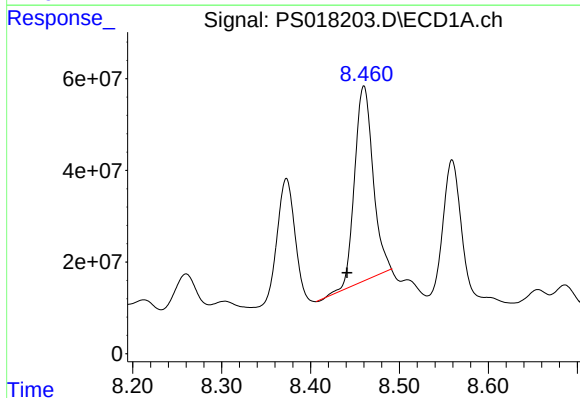


#10 Pentachlorophenol

R.T.: 8.460 min
Delta R.T.: 0.019 min
Response: 615682443
Conc: 29.14 ng/ml

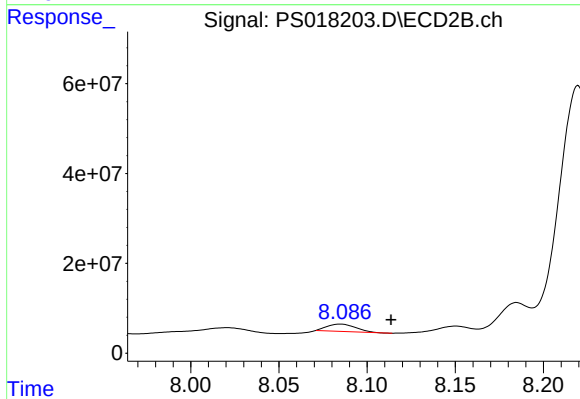

#10 Pentachlorophenol


R.T.: 8.085 min
Delta R.T.: -0.029 min
Response: 18038609
Conc: 2.14 ng/ml

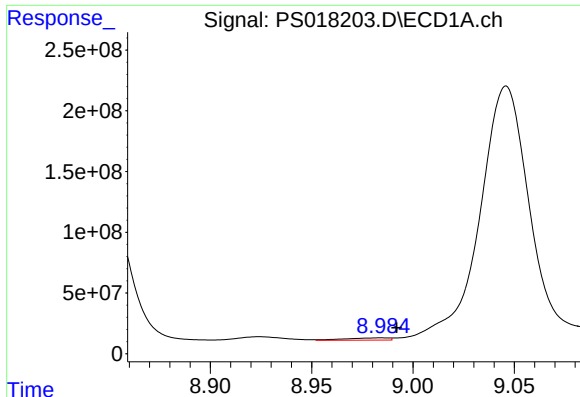

#11 2,4,5-TP (SILVEX)


R.T.: 8.985 min
Delta R.T.: -0.007 min
Response: 27573815
Conc: 3.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

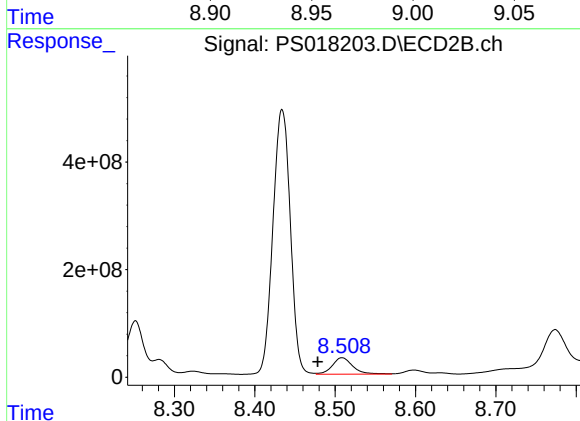


#11 2,4,5-TP (SILVEX)

R.T.: 8.509 min
Delta R.T.: 0.030 min
Response: 544021263
Conc: 152.61 ng/ml

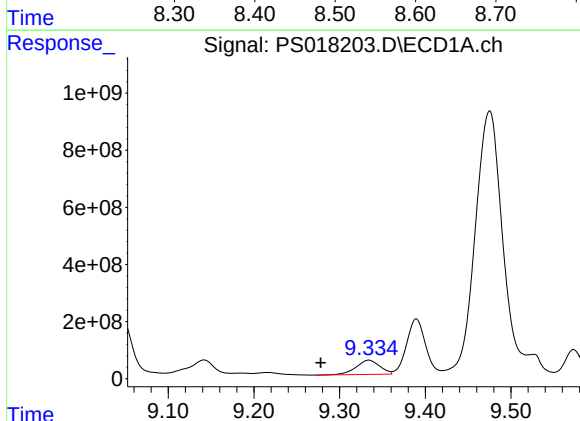


#12 2,4,5-T

R.T.: 9.334 min
Delta R.T.: 0.056 min
Response: 962606523
Conc: 108.60 ng/ml

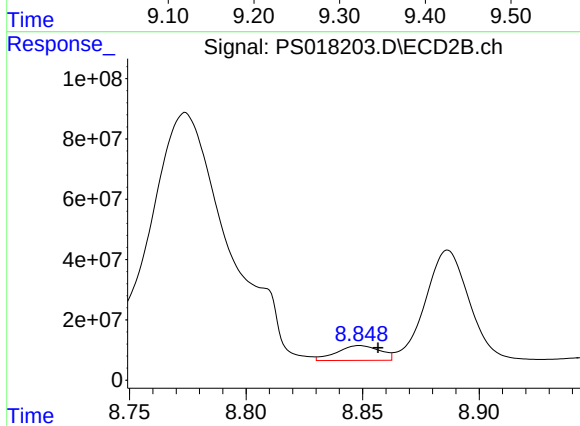

#12 2,4,5-T


R.T.: 8.849 min
Delta R.T.: -0.008 min
Response: 63140128
Conc: 19.30 ng/ml

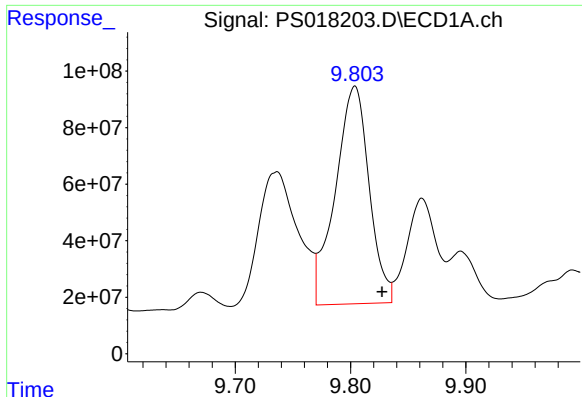

#13 2,4-DB


R.T.: 9.804 min
Delta R.T.: -0.024 min
Response: 1568454466
Conc: 948.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

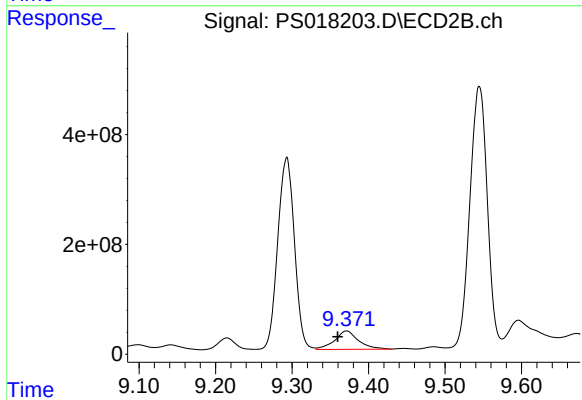


#13 2,4-DB

R.T.: 9.371 min
Delta R.T.: 0.011 min
Response: 721088087
Conc: 1629.74 ng/ml

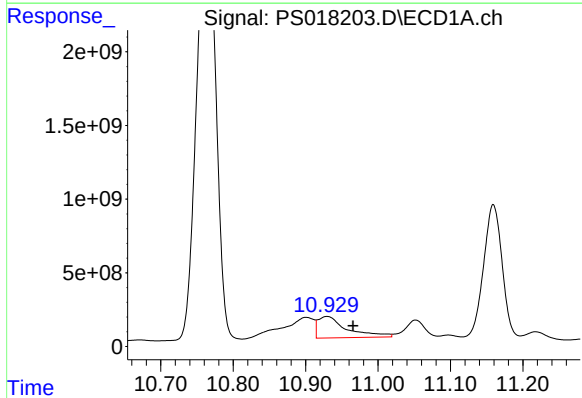


#14 DINOSEB

R.T.: 10.930 min
Delta R.T.: -0.036 min
Response: 4080830798
Conc: 621.42 ng/ml

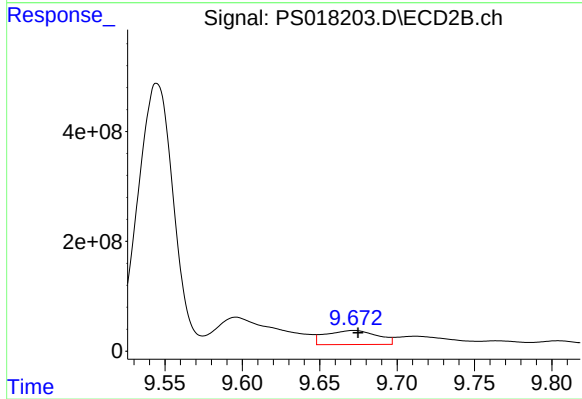

#14 DINOSEB


R.T.: 9.672 min
Delta R.T.: -0.003 min
Response: 594015758
Conc: 238.08 ng/ml

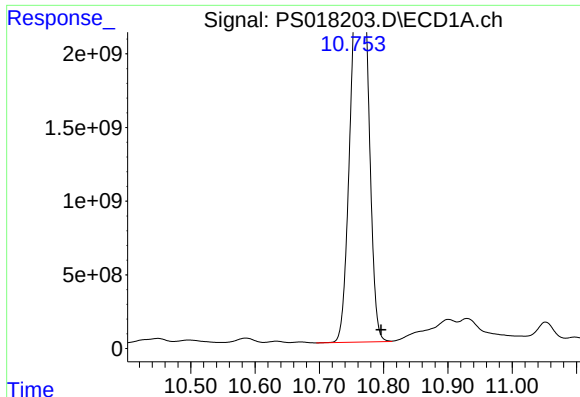

#15 Picloram


R.T.: 10.767 min
Delta R.T.: -0.029 min
Response: 47114080830
Conc: 3947.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

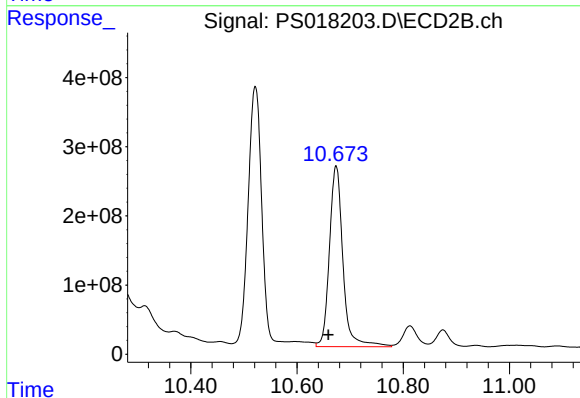


#15 Picloram

R.T.: 10.674 min
Delta R.T.: 0.015 min
Response: 4622748338
Conc: 988.58 ng/ml

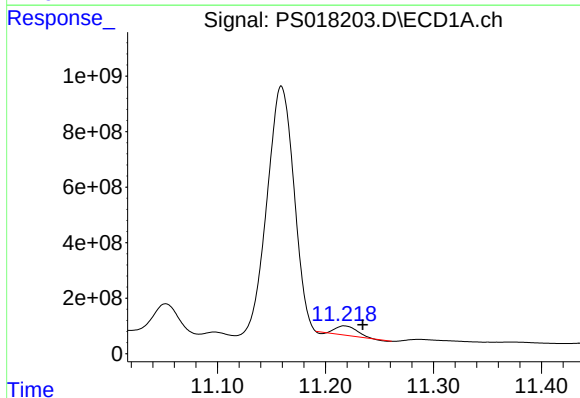

#16 DCPA

R.T.: 11.218 min
Delta R.T.: -0.017 min
Response: 438295507
Conc: 40.56 ng/ml

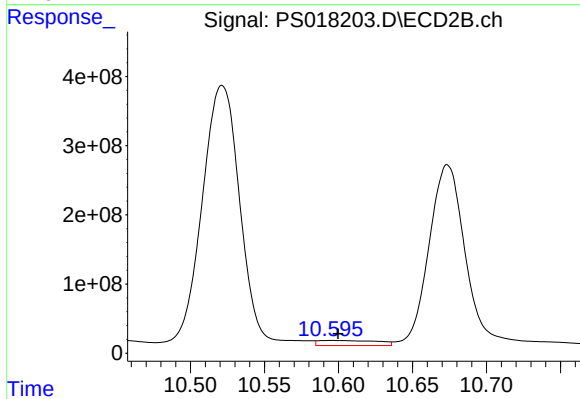

#16 DCPA

R.T.: 10.597 min
Delta R.T.: -0.003 min
Response: 206717329
Conc: 46.82 ng/ml