

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020122\
 Data File : PS018206.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2022 21:11
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 00:21:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.042	6.649	658.5E6	291.2E6	455.557	501.874
Target Compounds							
7) T	MCPA	7.490f	0.000	9518267	0	1.427	N.D. #
9) T	2,4-D	8.200f	0.000	889178	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.048f	8.439	19983006	15046446	2.361	4.221 #
12) T	2,4,5-T	9.336f	0.000	32510289	0	3.668	N.D. #
13) T	2,4-DB	9.793	0.000	11417390	0	6.907	N.D. #
14) T	DINOSEB	10.902f	0.000	27326863	0	4.161	N.D. #
15) T	Picloram	10.821	10.697	37141333	27210493	3.112	5.819 #
16) T	DCPA	11.222	0.000	13639141	0	1.262	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020122\
Data File : PS018206.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2022 21:11
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 00:21:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

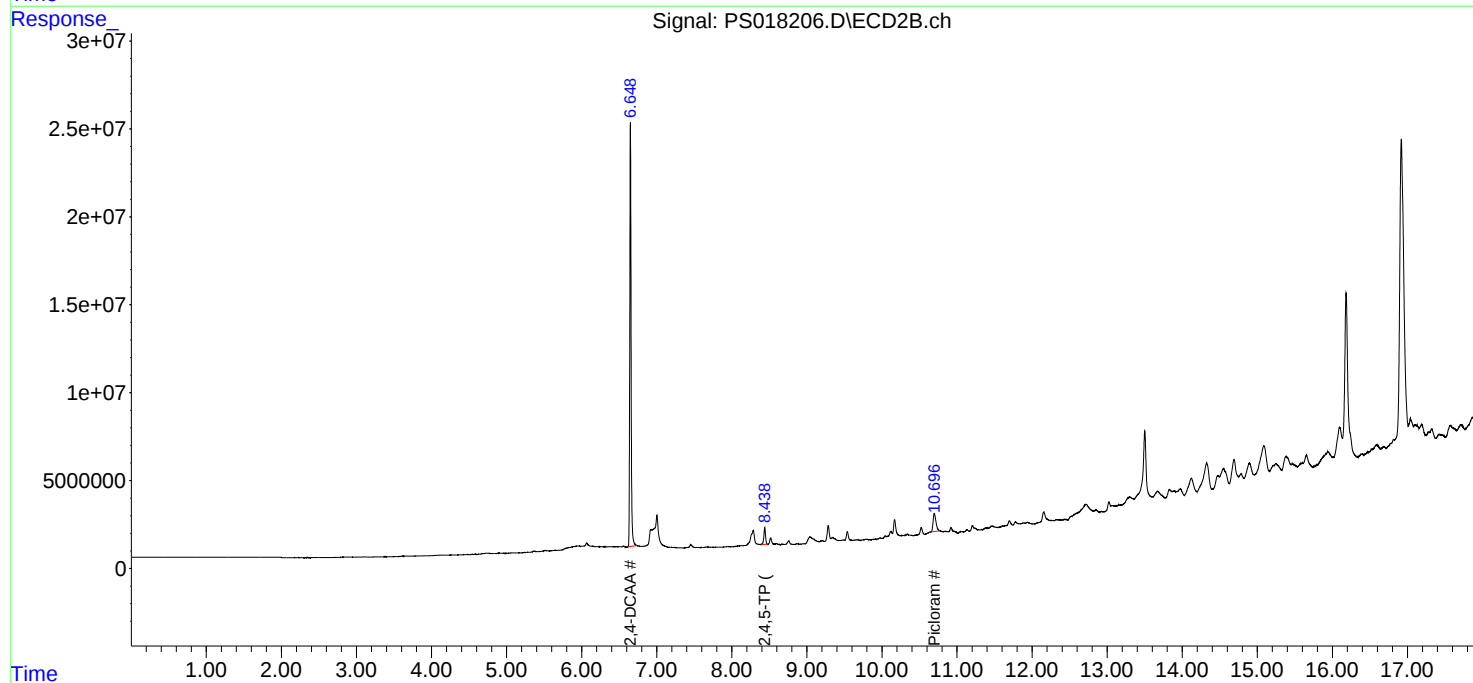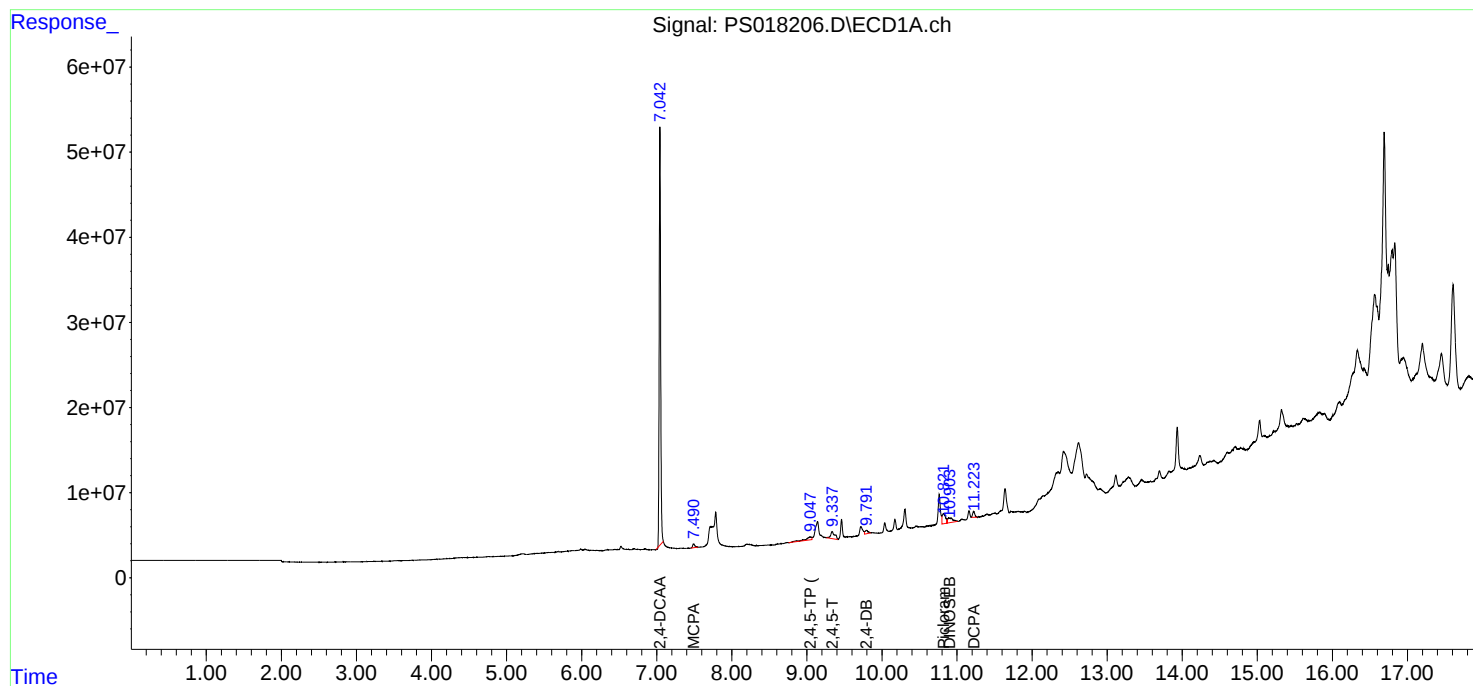


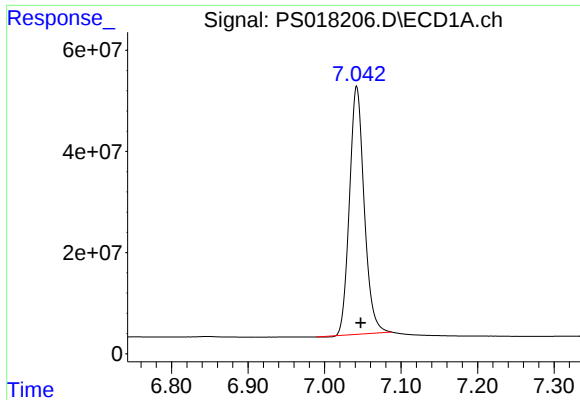

#4 2,4-DCAA


R.T.: 7.042 min
Delta R.T.: -0.005 min
Response: 658501964
Conc: 455.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

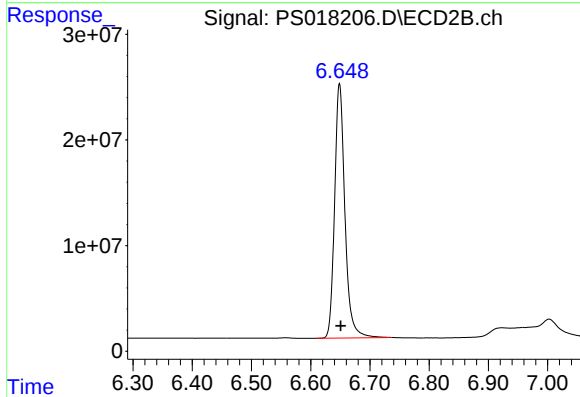


#4 2,4-DCAA

R.T.: 6.649 min
Delta R.T.: -0.002 min
Response: 291211677
Conc: 501.87 ng/ml

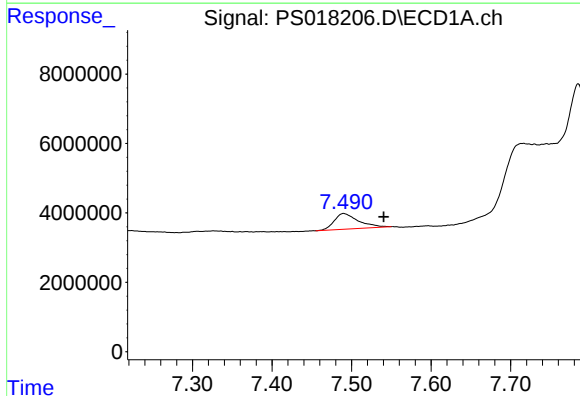


#7 MCPA

R.T.: 7.490 min
Delta R.T.: -0.050 min
Response: 9518267
Conc: 1.43 ug/ml

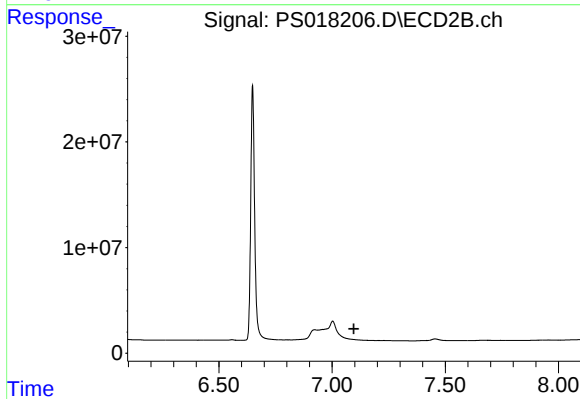

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.096 min
Response: 0
Conc: N.D.

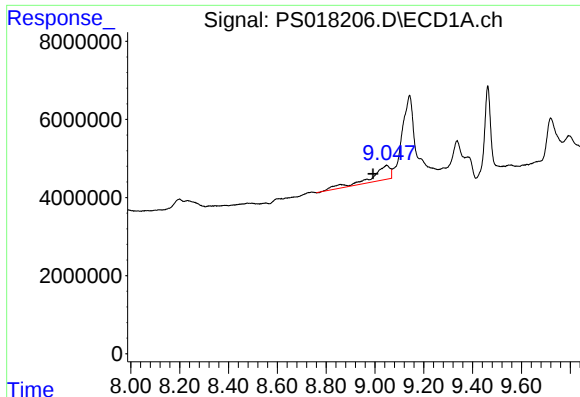

#11 2,4,5-TP (SILVEX)


R.T.: 9.048 min
Delta R.T.: 0.056 min
Response: 19983006
Conc: 2.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

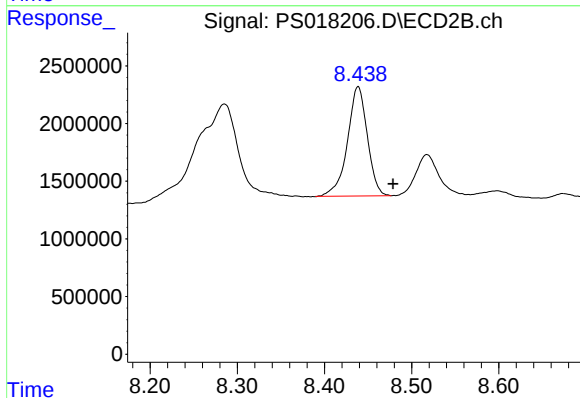


#11 2,4,5-TP (SILVEX)

R.T.: 8.439 min
Delta R.T.: -0.040 min
Response: 15046446
Conc: 4.22 ng/ml

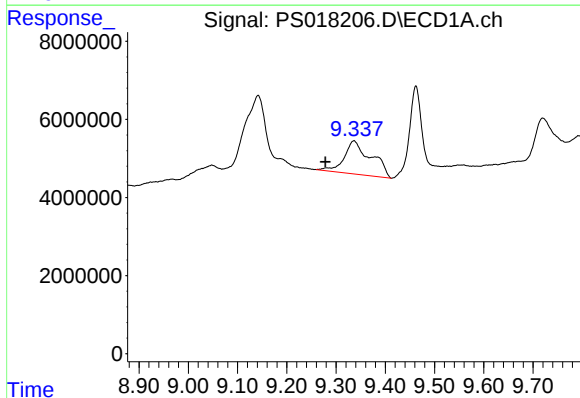


#12 2,4,5-T

R.T.: 9.336 min
Delta R.T.: 0.058 min
Response: 32510289
Conc: 3.67 ng/ml

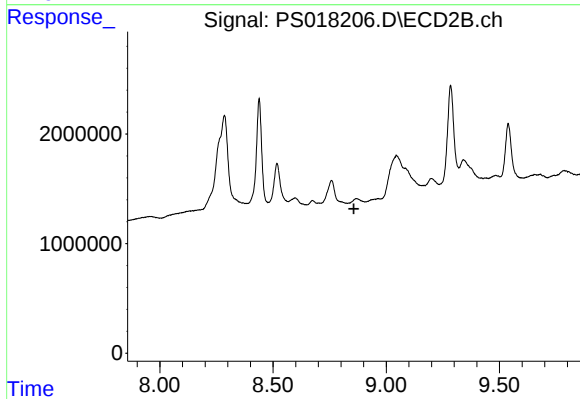

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.857 min
Response: 0
Conc: N.D.

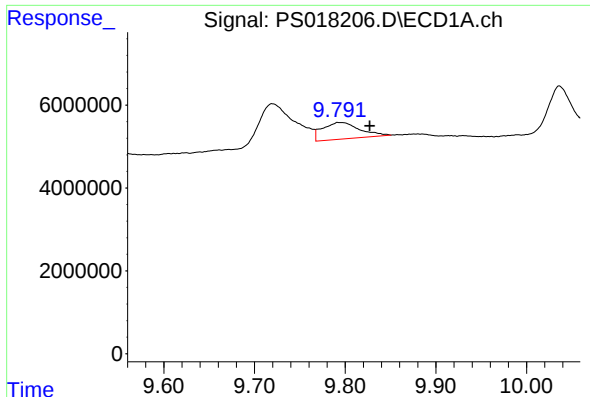

#13 2,4-DB


R.T.: 9.793 min
Delta R.T.: -0.035 min
Response: 11417390
Conc: 6.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

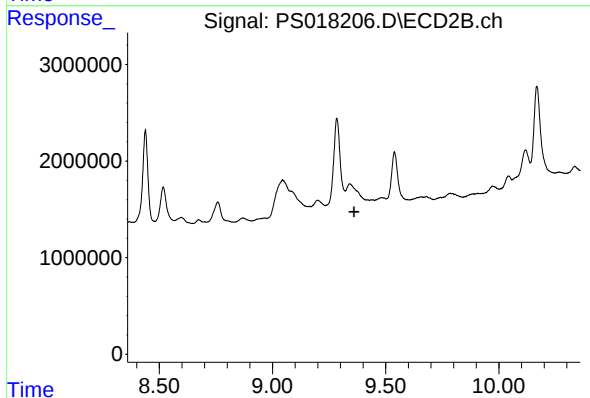


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

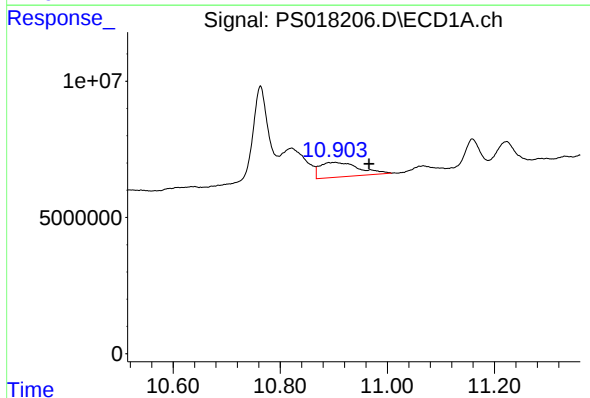


#14 DINOSEB

R.T.: 10.902 min
Delta R.T.: -0.064 min
Response: 27326863
Conc: 4.16 ng/ml

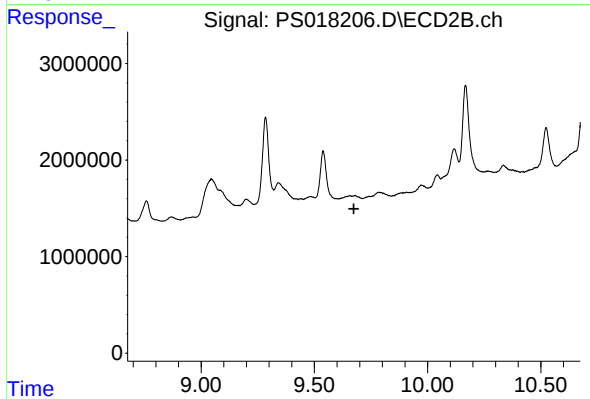

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

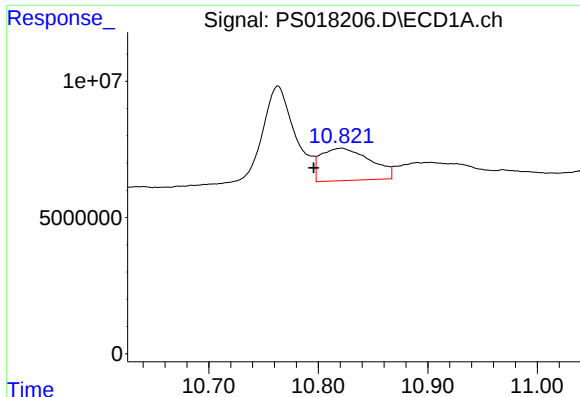

#15 Picloram


R.T.: 10.821 min
Delta R.T.: 0.025 min
Response: 37141333
Conc: 3.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

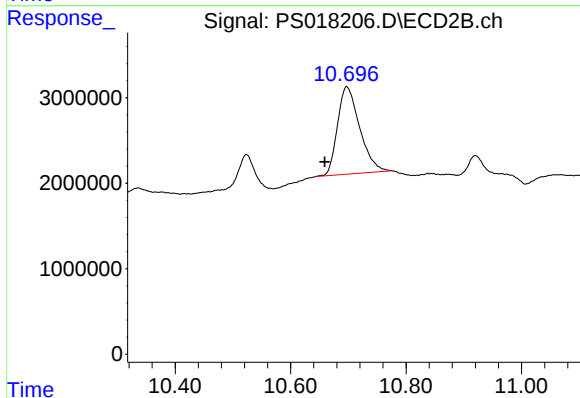


#15 Picloram

R.T.: 10.697 min
Delta R.T.: 0.038 min
Response: 27210493
Conc: 5.82 ng/ml

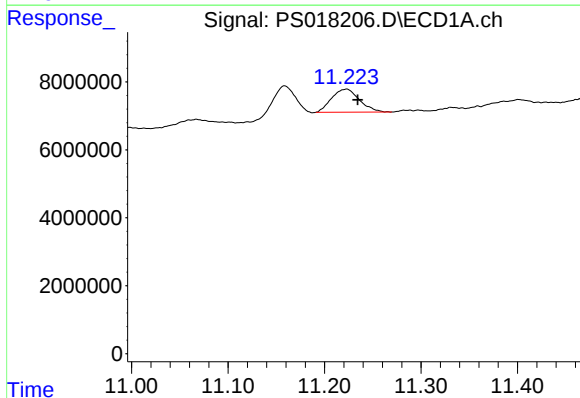

#16 DCPA

R.T.: 11.222 min
Delta R.T.: -0.012 min
Response: 13639141
Conc: 1.26 ng/ml

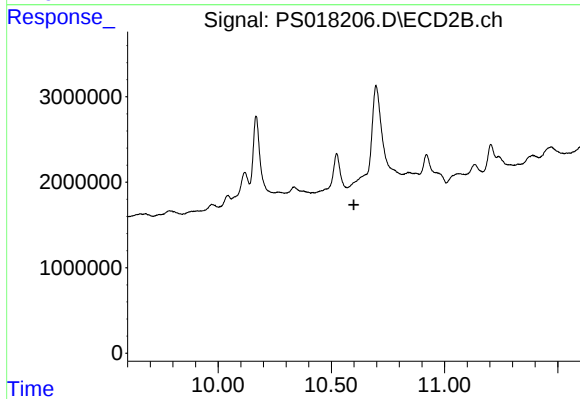

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.600 min
Response: 0
Conc: N.D.