

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020122\
 Data File : PS018211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2022 23:18
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 00:23:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.042	6.650	661.0E6	294.7E6	457.320	507.960
Target Compounds							
7) T	MCPA	7.489f	0.000	4747386	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.046f	8.442	8920424	15416055	1.054	4.325 #
12) T	2,4,5-T	9.340f	0.000	19293366	0	2.177	N.D. #
13) T	2,4-DB	9.798	0.000	5465083	0	3.306	N.D. #
14) T	DINOSEB	10.970	0.000	1407332	0	<MDL	N.D. #
15) T	Picloram	10.767	10.708f	58699092	24357214	4.918	5.209
16) T	DCPA	11.223	0.000	10509751	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020122\
Data File : PS018211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2022 23:18
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 00:23:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

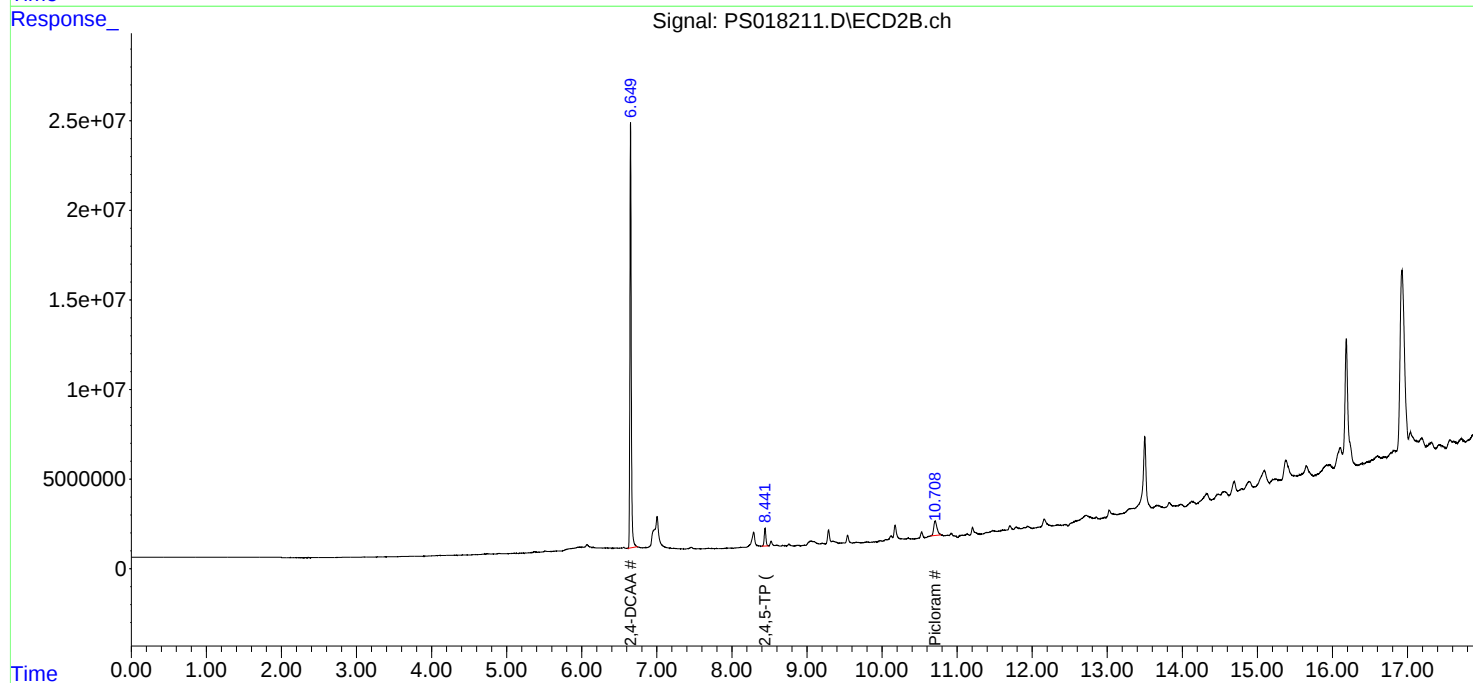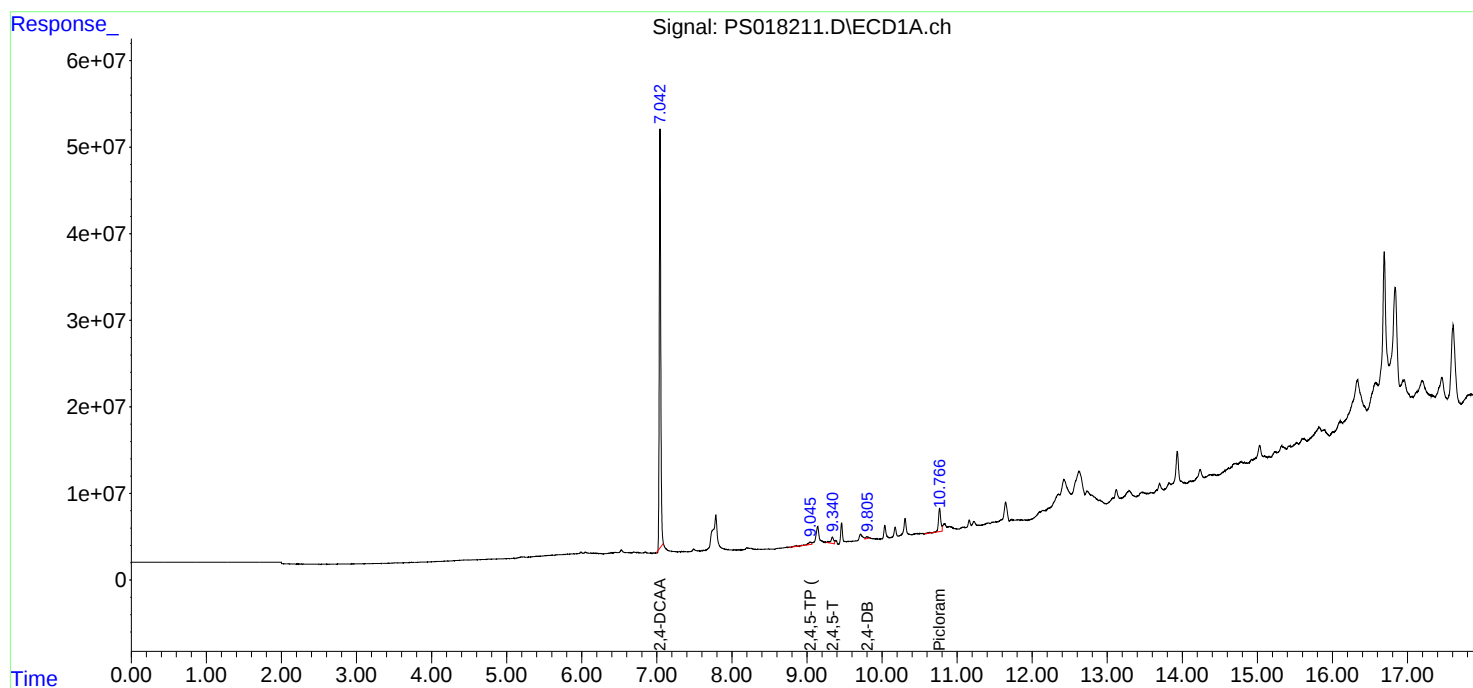


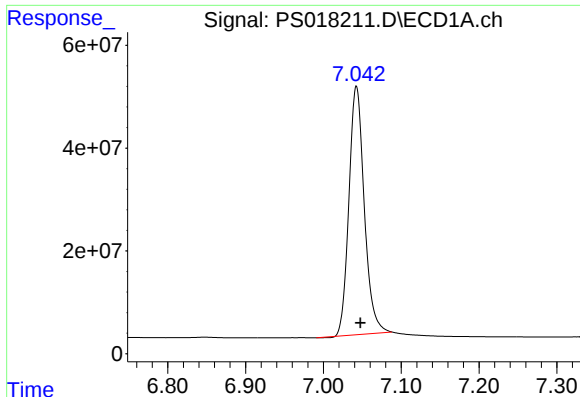

#4 2,4-DCAA


R.T.: 7.042 min
Delta R.T.: -0.005 min
Response: 661049893
Conc: 457.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

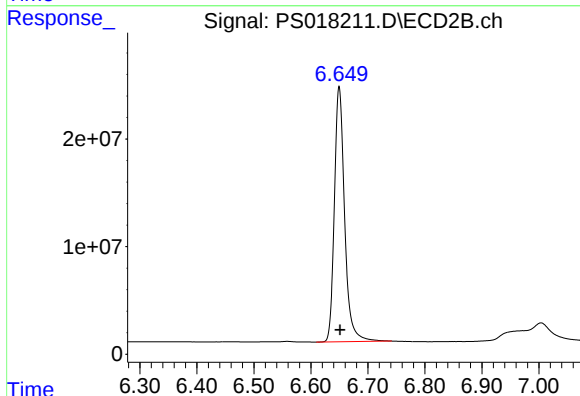


#4 2,4-DCAA

R.T.: 6.650 min
Delta R.T.: -0.001 min
Response: 294743154
Conc: 507.96 ng/ml

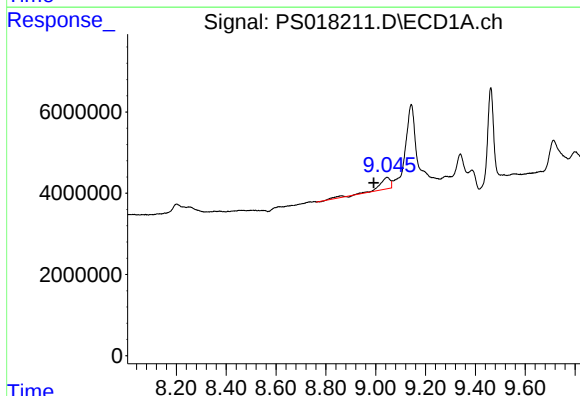


#11 2,4,5-TP (SILVEX)

R.T.: 9.046 min
Delta R.T.: 0.053 min
Response: 8920424
Conc: 1.05 ng/ml

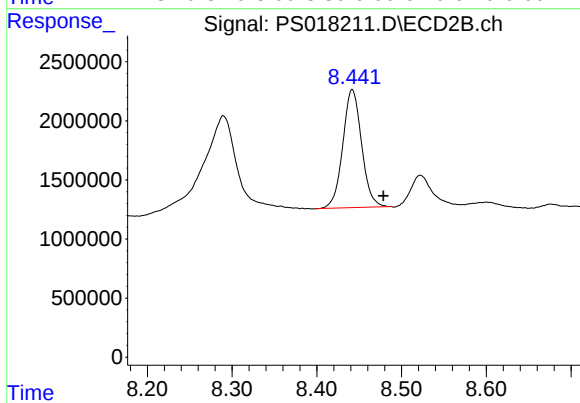

#11 2,4,5-TP (SILVEX)


R.T.: 8.442 min
Delta R.T.: -0.037 min
Response: 15416055
Conc: 4.32 ng/ml

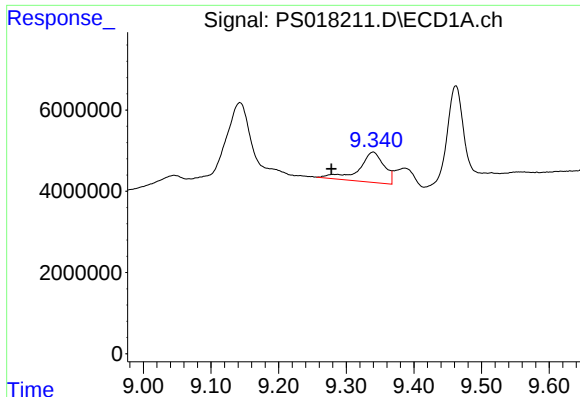

#12 2,4,5-T


R.T.: 9.340 min
Delta R.T.: 0.062 min
Response: 19293366
Conc: 2.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

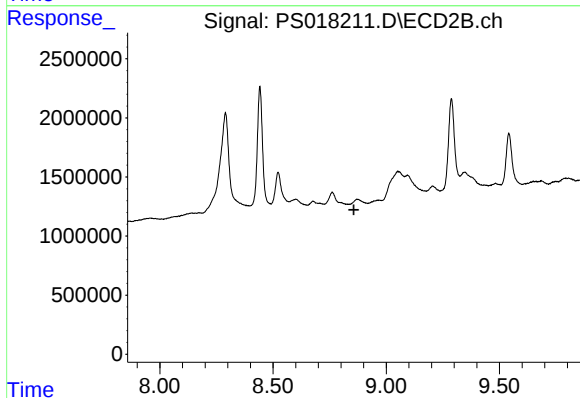


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.857 min
Response: 0
Conc: N.D.

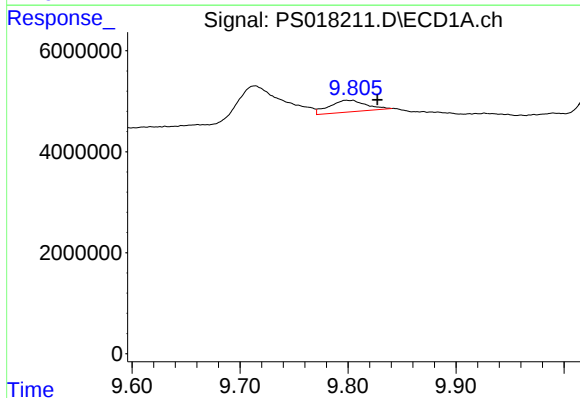


#13 2,4-DB

R.T.: 9.798 min
Delta R.T.: -0.029 min
Response: 5465083
Conc: 3.31 ng/ml

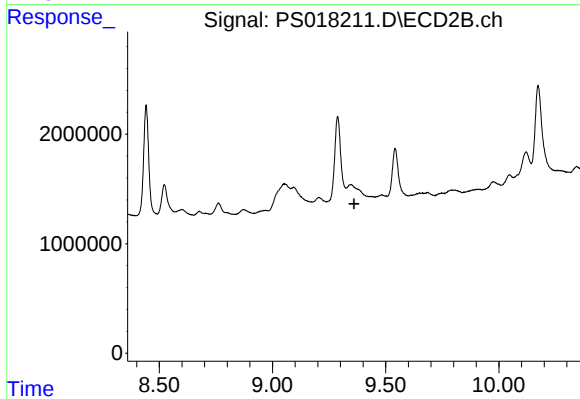

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

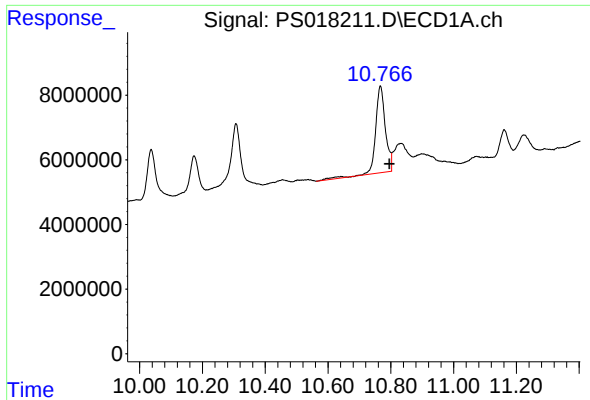

#15 Picloram

R.T.: 10.767 min
Delta R.T.: -0.029 min
Response: 58699092
Conc: 4.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

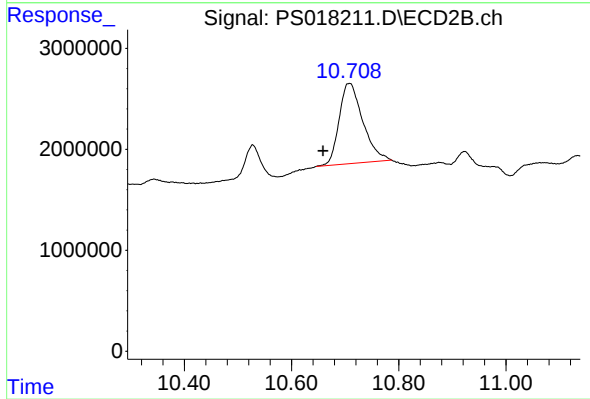

#15 Picloram

R.T.: 10.708 min
Delta R.T.: 0.049 min
Response: 24357214
Conc: 5.21 ng/ml