

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020123\
 Data File : PS021965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2023 10:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 00:09:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.390	6.818	1192.5E6	1190.3E6	428.408	662.513 #
Target Compounds							
1) T	Dalapon	2.494	0.000	271879	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.758	0.000	11825420	0	3.057	N.D. #
3) T	4-Nitroph...	6.247	6.449	7057048	1772517	4.841	1.617 #
6) T	MCP	0.000	7.046	0	49090178	N.D.	7.402
7) T	MCPA	0.000	7.246f	0	12181213	N.D.	1.343
9) T	2,4-D	7.315	0.000	42549	0	<MDL	N.D. #
12) T	2,4,5-T	8.295f	0.000	238384	0	<MDL	N.D. #
14) T	DINOSEB	9.877	0.000	319232	0	<MDL	N.D. #
15) T	Picloram	9.748	10.825	188280	6622954	<MDL	<MDL #
16) T	DCPA	10.177	10.825	150414	6622954	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020123\
Data File : PS021965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2023 10:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 00:09:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

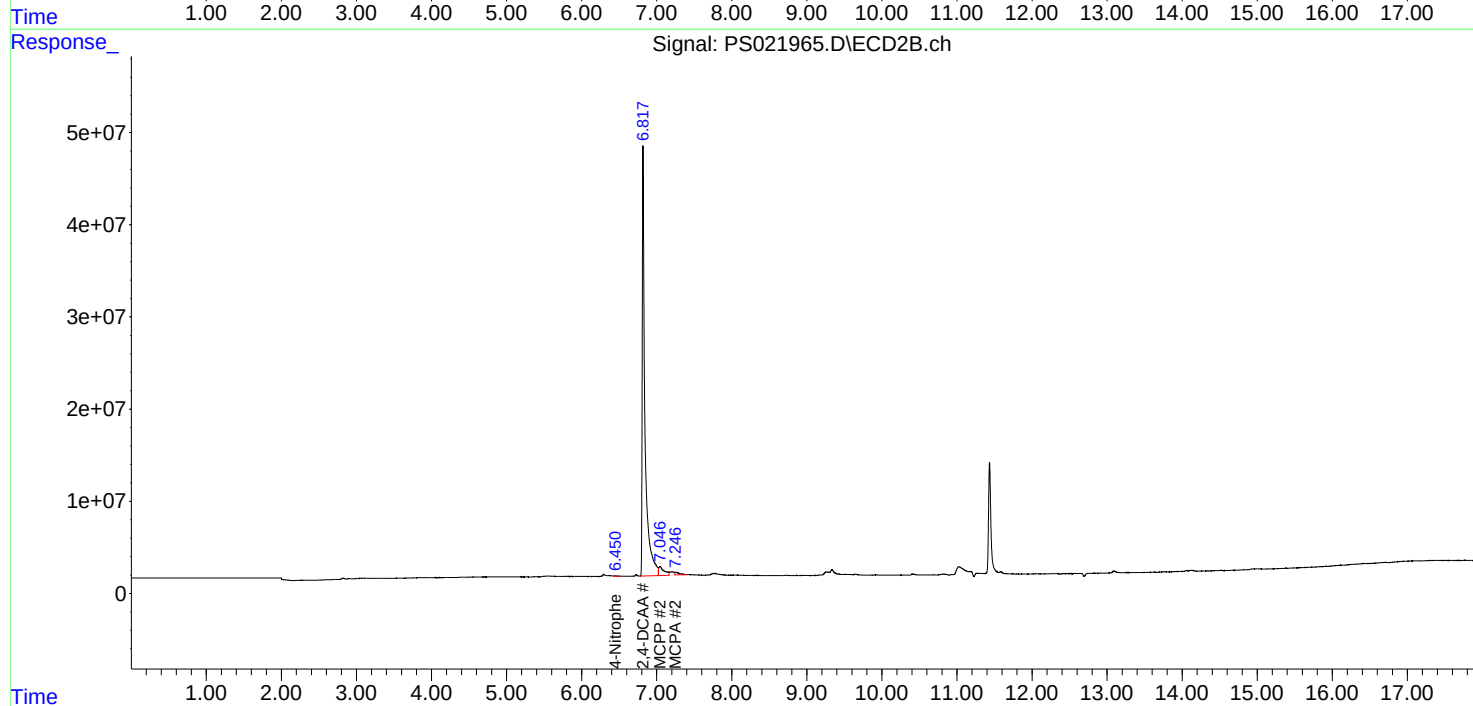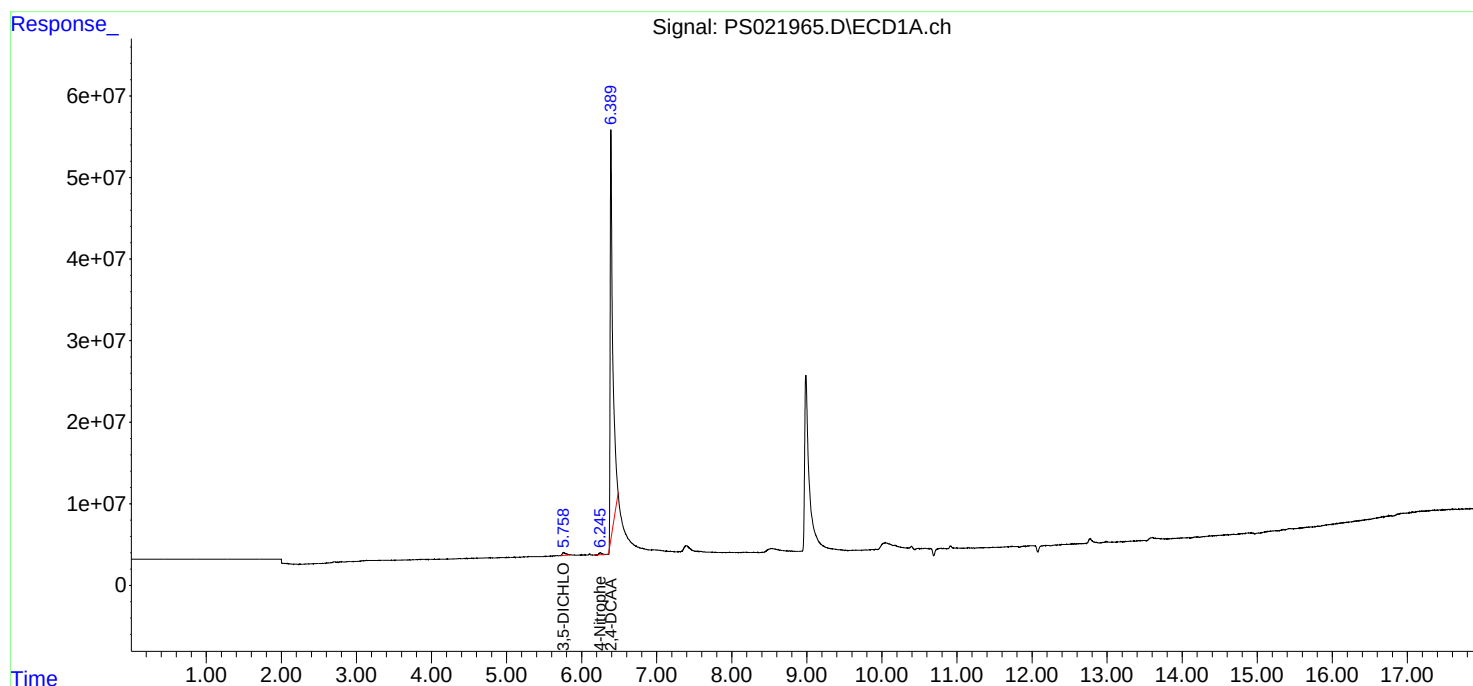


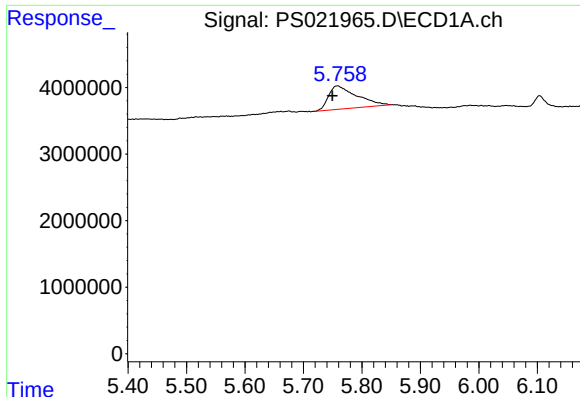

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.758 min
Delta R.T.: 0.009 min
Response: 11825420
Conc: 3.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

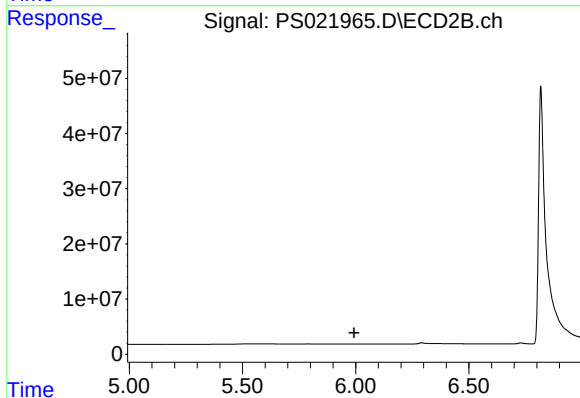


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.992 min
Response: 0
Conc: N.D.

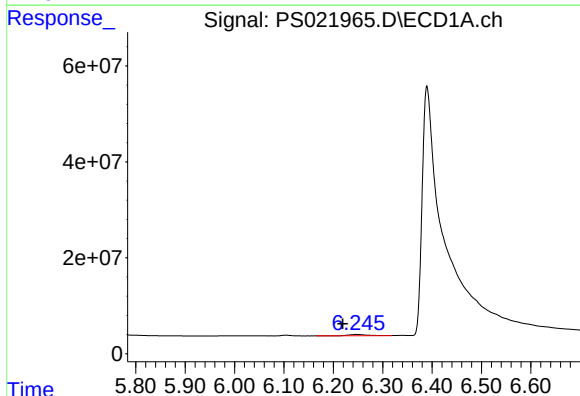


#3 4-Nitrophenol

R.T.: 6.247 min
Delta R.T.: 0.027 min
Response: 7057048
Conc: 4.84 ng/ml

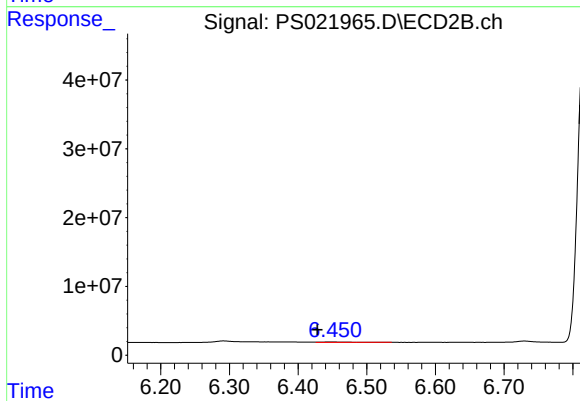

#3 4-Nitrophenol


R.T.: 6.449 min
Delta R.T.: 0.021 min
Response: 1772517
Conc: 1.62 ng/ml

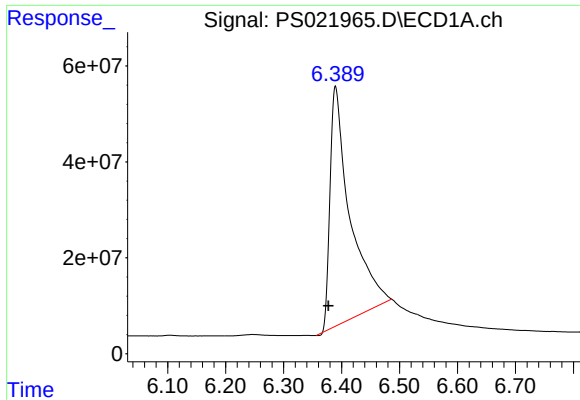

#4 2,4-DCAA


R.T.: 6.390 min
Delta R.T.: 0.012 min
Response: 1192502755
Conc: 428.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

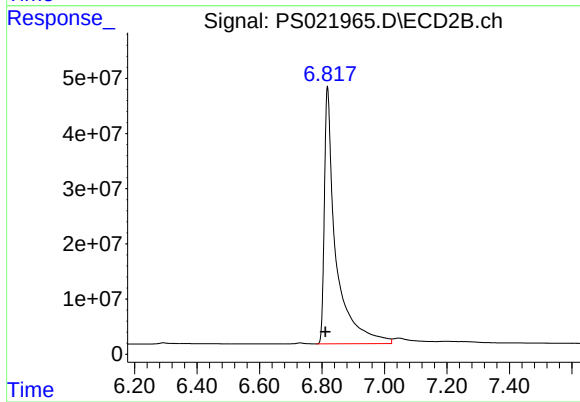


#4 2,4-DCAA

R.T.: 6.818 min
Delta R.T.: 0.006 min
Response: 1190330552
Conc: 662.51 ng/ml

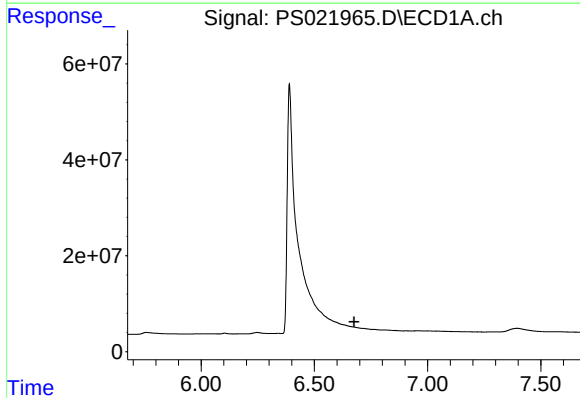


#6 MCP

R.T.: 0.000 min
Exp R.T. : 6.675 min
Response: 0
Conc: N.D.

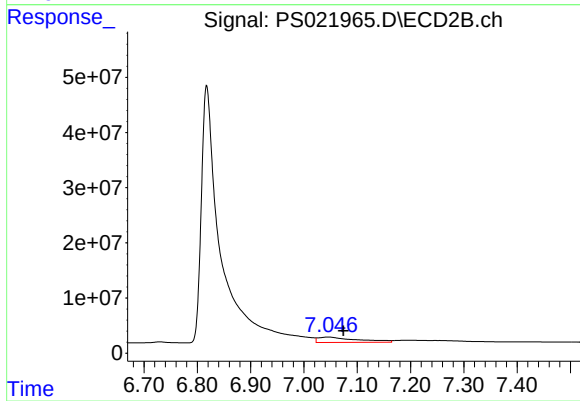

#6 MCP


R.T.: 7.046 min
Delta R.T.: -0.028 min
Response: 49090178
Conc: 7.40 ug/ml

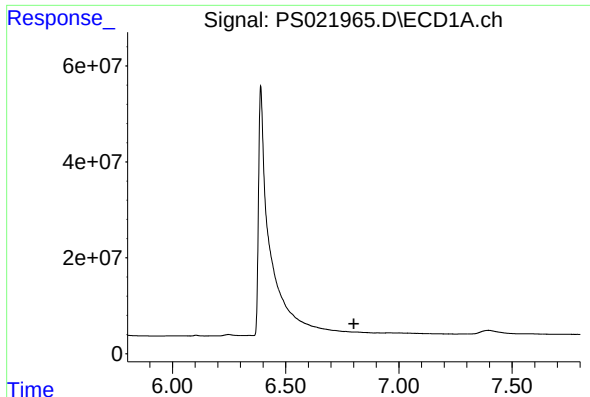

#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

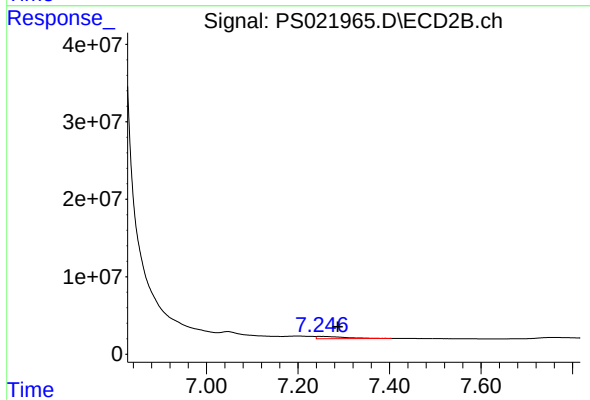

#7 MCPA

R.T.: 7.246 min
Delta R.T.: -0.040 min
Response: 12181213
Conc: 1.34 ug/ml