

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020419\
 Data File : PS003009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2019 21:33
 Operator : EI\SJ
 Sample : K1284-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:16:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.782	0	277.7E6	N.D.	649.447 #
Target Compounds							
1) T	Dalapon	0.000	2.290	0	112.1E6	N.D.	209.179 #
2) T	3,5-DICHL...	0.000	8.942	0	2453041	N.D.	4.353 #
3) T	4-Nitroph...	0.000	10.004	0	3055696	N.D.	14.619 #
5) T	DICAMBA	11.610	0.000	6316416	0	3.941	N.D. #
7) T	MCPA	12.249	11.722	1703944	1487118	0.963	0.945
8) T	DICHLORPROP	12.851	12.242	2675697	2062320	6.976	5.394
11) T	2,4,5-TP ...	14.368	0.000	5380863	0	2.137	N.D. #
12) T	2,4,5-T	14.752	14.384	10093817	2881241	4.138	1.506 #
13) T	2,4-DB	15.554	0.000	33921079	0	129.753	N.D. #
15) T	Picloram	16.802	16.696	10451954	28083880	3.304	9.341 #
16) T	DCPA	0.000	16.696	0	28083880	N.D.	9.066 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020419\
Data File : PS003009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2019 21:33
Operator : EI\SJ
Sample : K1284-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:16:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

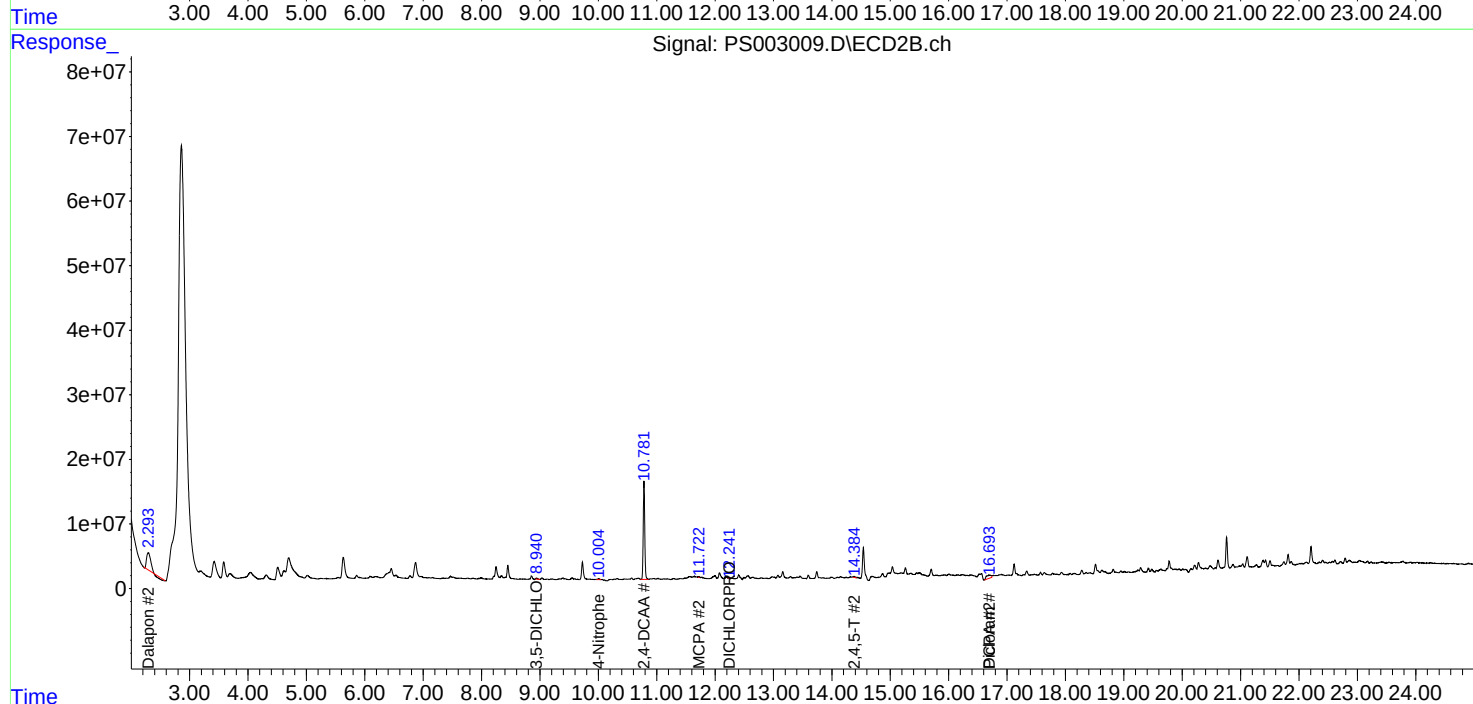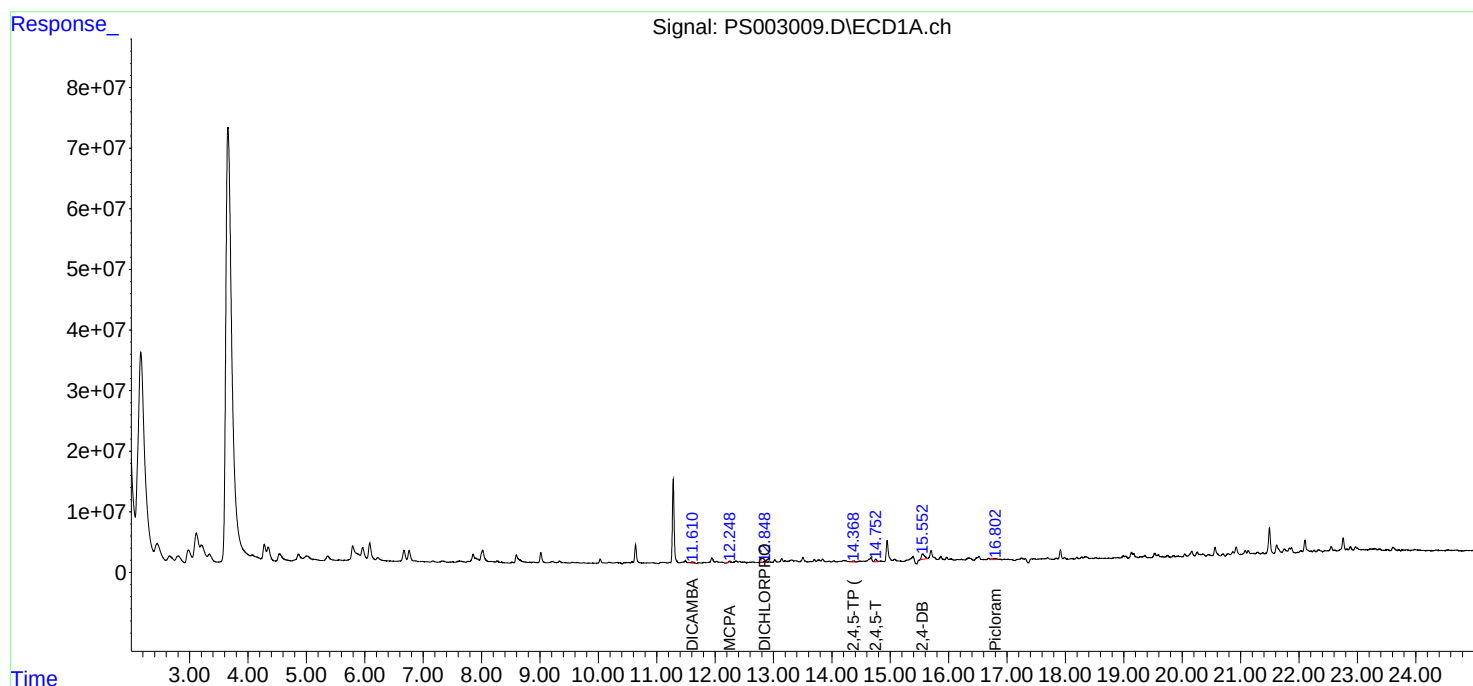


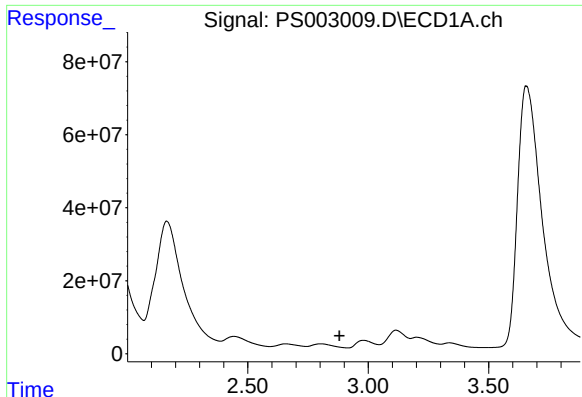

#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

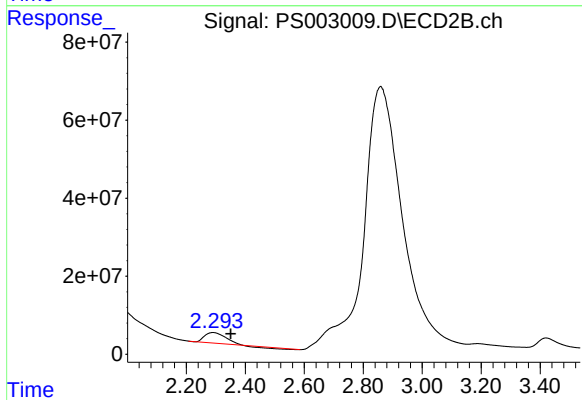


#1 Dalapon

R.T.: 2.290 min
Delta R.T.: -0.060 min
Response: 112103499
Conc: 209.18 ng/ml


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

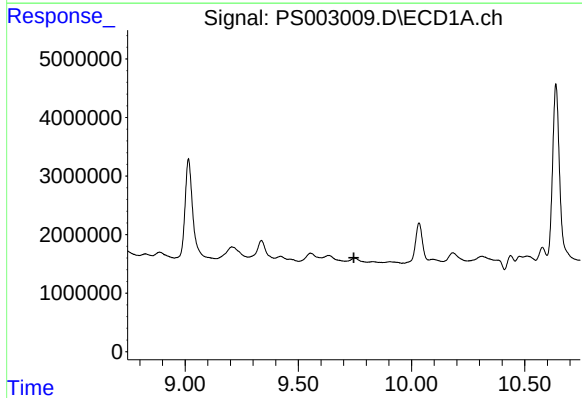

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.942 min
Delta R.T.: -0.034 min
Response: 2453041
Conc: 4.35 ng/ml

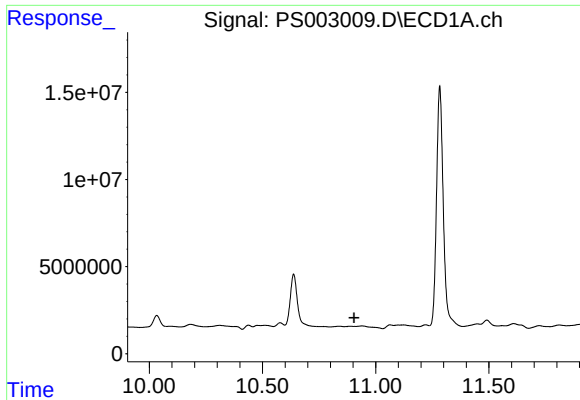

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

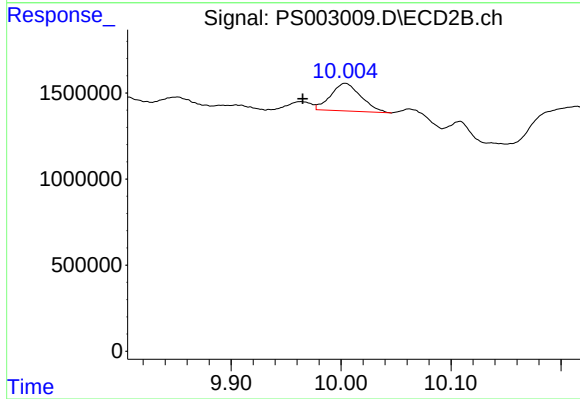


#3 4-Nitrophenol

R.T.: 10.004 min
Delta R.T.: 0.039 min
Response: 3055696
Conc: 14.62 ng/ml

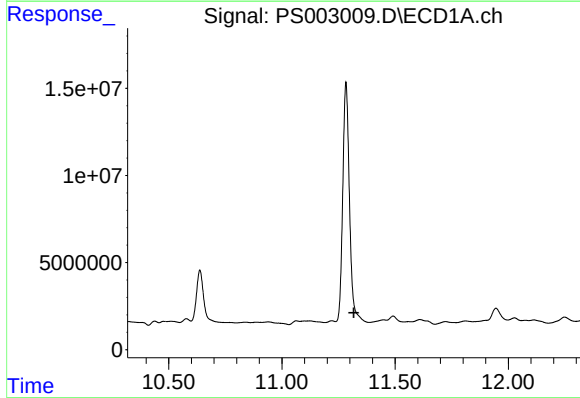


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.318 min
Response: 0
Conc: N.D.

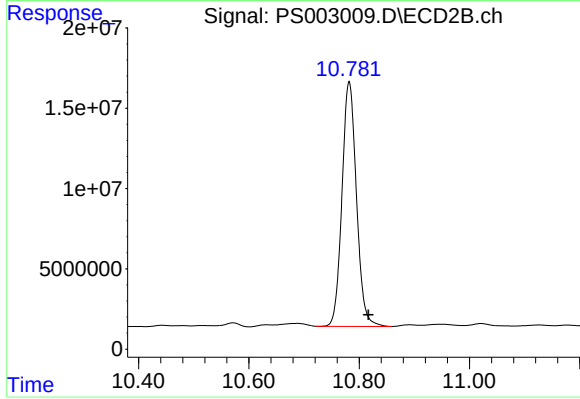

#4 2,4-DCAA


R.T.: 10.782 min
Delta R.T.: -0.035 min
Response: 277668105
Conc: 649.45 ng/ml

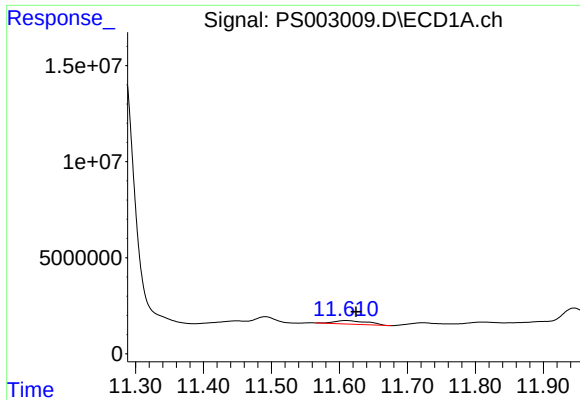

#5 DICAMBA


R.T.: 11.610 min
Delta R.T.: -0.014 min
Response: 6316416
Conc: 3.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

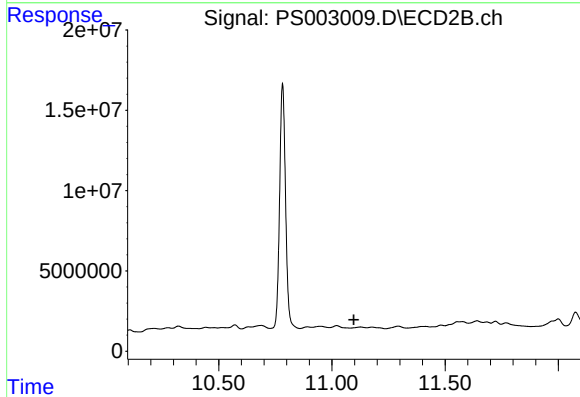


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.097 min
Response: 0
Conc: N.D.

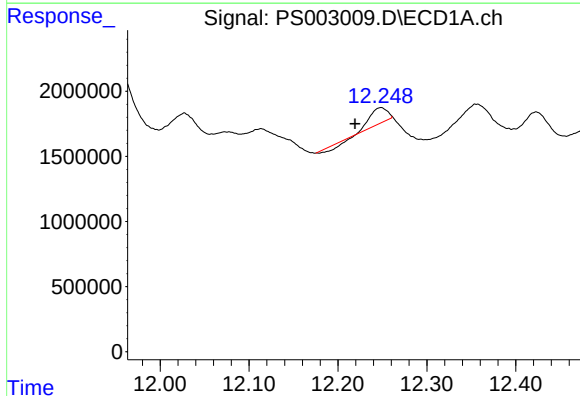


#7 MCPA

R.T.: 12.249 min
Delta R.T.: 0.029 min
Response: 1703944
Conc: 0.96 ug/ml

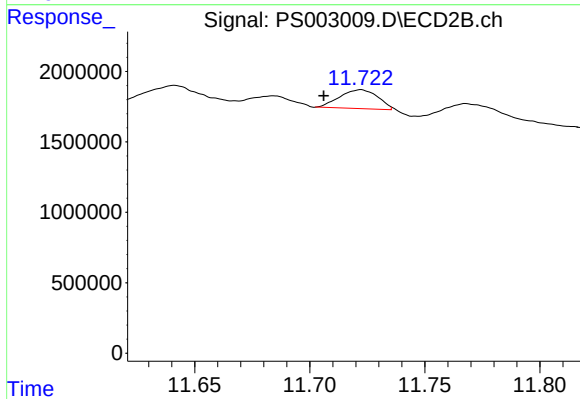

#7 MCPA


R.T.: 11.722 min
Delta R.T.: 0.016 min
Response: 1487118
Conc: 0.95 ug/ml

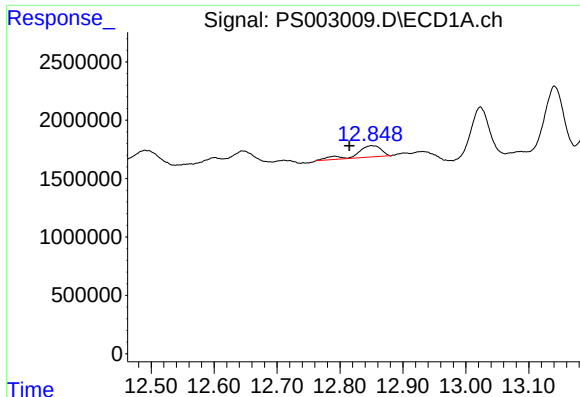

#8 DICHLORPROP


R.T.: 12.851 min
Delta R.T.: 0.036 min
Response: 2675697
Conc: 6.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

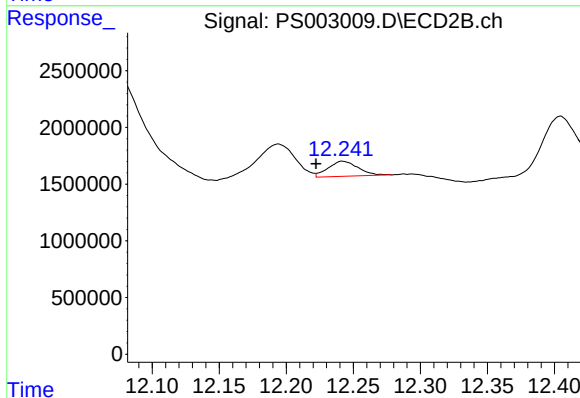


#8 DICHLORPROP

R.T.: 12.242 min
Delta R.T.: 0.020 min
Response: 2062320
Conc: 5.39 ng/ml

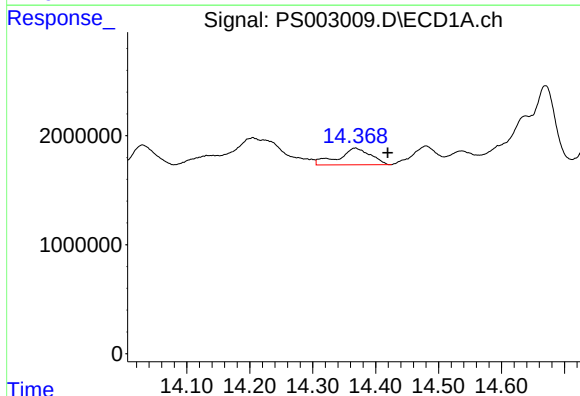


#11 2,4,5-TP (SILVEX)

R.T.: 14.368 min
Delta R.T.: -0.051 min
Response: 5380863
Conc: 2.14 ng/ml

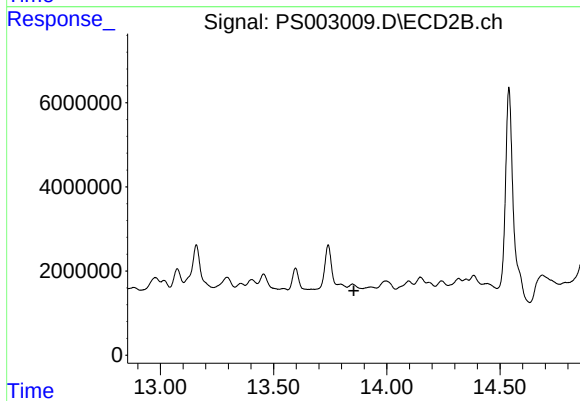

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

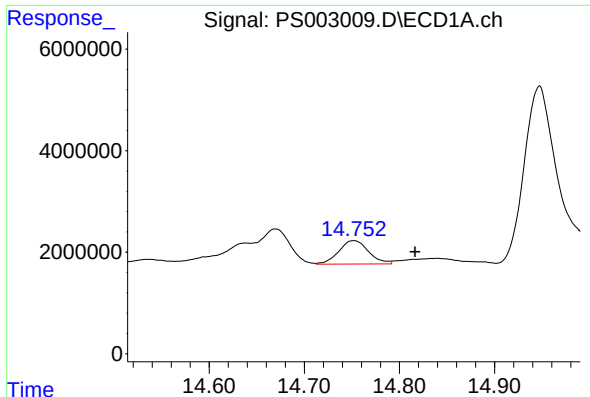

#12 2,4,5-T


R.T.: 14.752 min
Delta R.T.: -0.065 min
Response: 10093817
Conc: 4.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

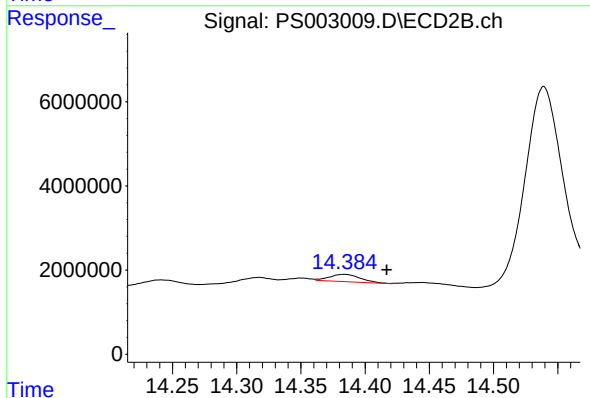


#12 2,4,5-T

R.T.: 14.384 min
Delta R.T.: -0.033 min
Response: 2881241
Conc: 1.51 ng/ml

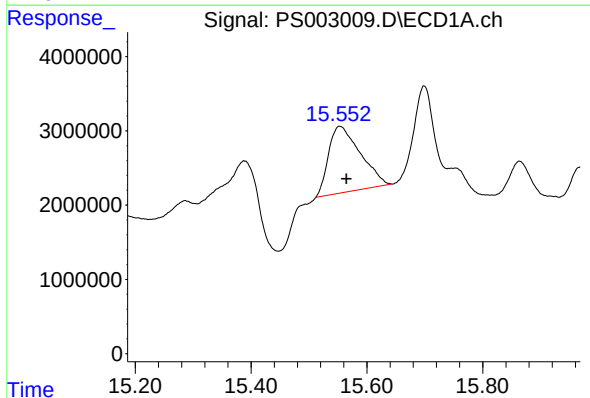


#13 2,4-DB

R.T.: 15.554 min
Delta R.T.: -0.011 min
Response: 33921079
Conc: 129.75 ng/ml

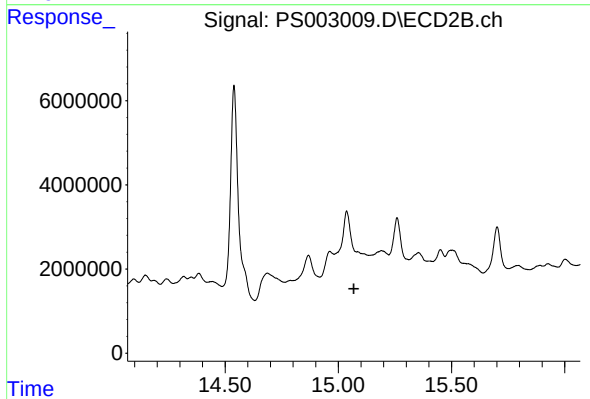

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.069 min
Response: 0
Conc: N.D.

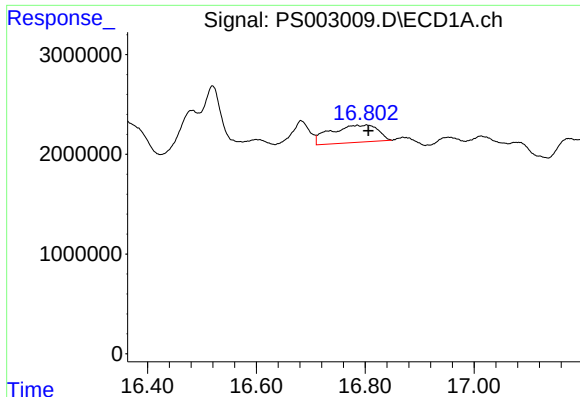

#15 Picloram


R.T.: 16.802 min
Delta R.T.: -0.003 min
Response: 10451954
Conc: 3.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

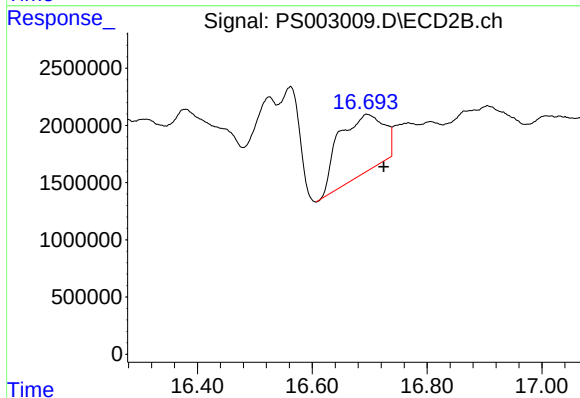


#15 Picloram

R.T.: 16.696 min
Delta R.T.: -0.029 min
Response: 28083880
Conc: 9.34 ng/ml

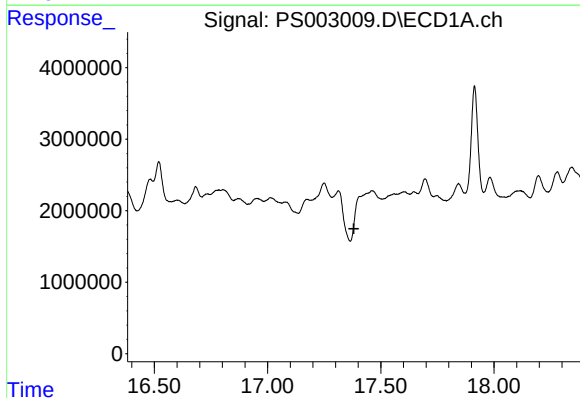

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

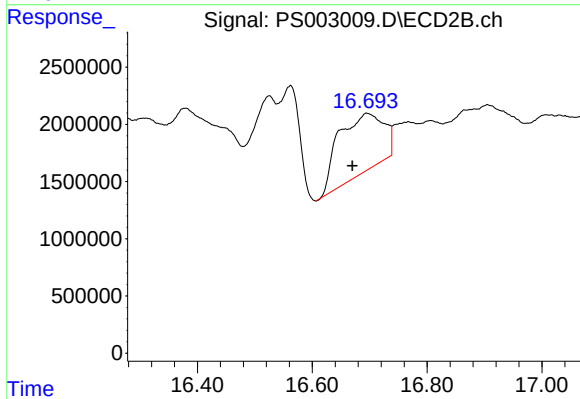

#16 DCPA

R.T.: 16.696 min
Delta R.T.: 0.026 min
Response: 28083880
Conc: 9.07 ng/ml