

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020419\
 Data File : PS003010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2019 22:04
 Operator : EI\SJ
 Sample : K1361-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:16:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.780	0	213.0E6	N.D.	498.133 #
Target Compounds							
1) T	Dalapon	0.000	2.283	0	25162631	N.D.	46.952 #
2) T	3,5-DICHL...	0.000	8.944	0	2173995	N.D.	3.858 #
3) T	4-Nitroph...	0.000	9.999	0	3757665	N.D.	17.977 #
7) T	MCPA	12.246	0.000	2397041	0	1.354	N.D. #
8) T	DICHLORPROP	12.838	12.241	3934591	1405515	10.259	3.676 #
10) T	Pentachlo...	13.508	13.291	9145736	-6634086	1.426	N.D. #
11) T	2,4,5-TP ...	14.479	0.000	5696172	0	2.262	N.D. #
12) T	2,4,5-T	14.842	14.382	3940111	3788762	1.615	1.980
13) T	2,4-DB	15.558	0.000	22904020	0	87.611	N.D. #
14) T	DINOSEB	17.016	15.495	22264395	10685831	11.834	6.096 #
15) T	Picloram	16.793	16.697	23372985	32410952	7.388	10.781 #
16) T	DCPA	0.000	16.697	0	32410952	N.D.	10.463 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020419\
Data File : PS003010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2019 22:04
Operator : EI\SJ
Sample : K1361-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:16:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

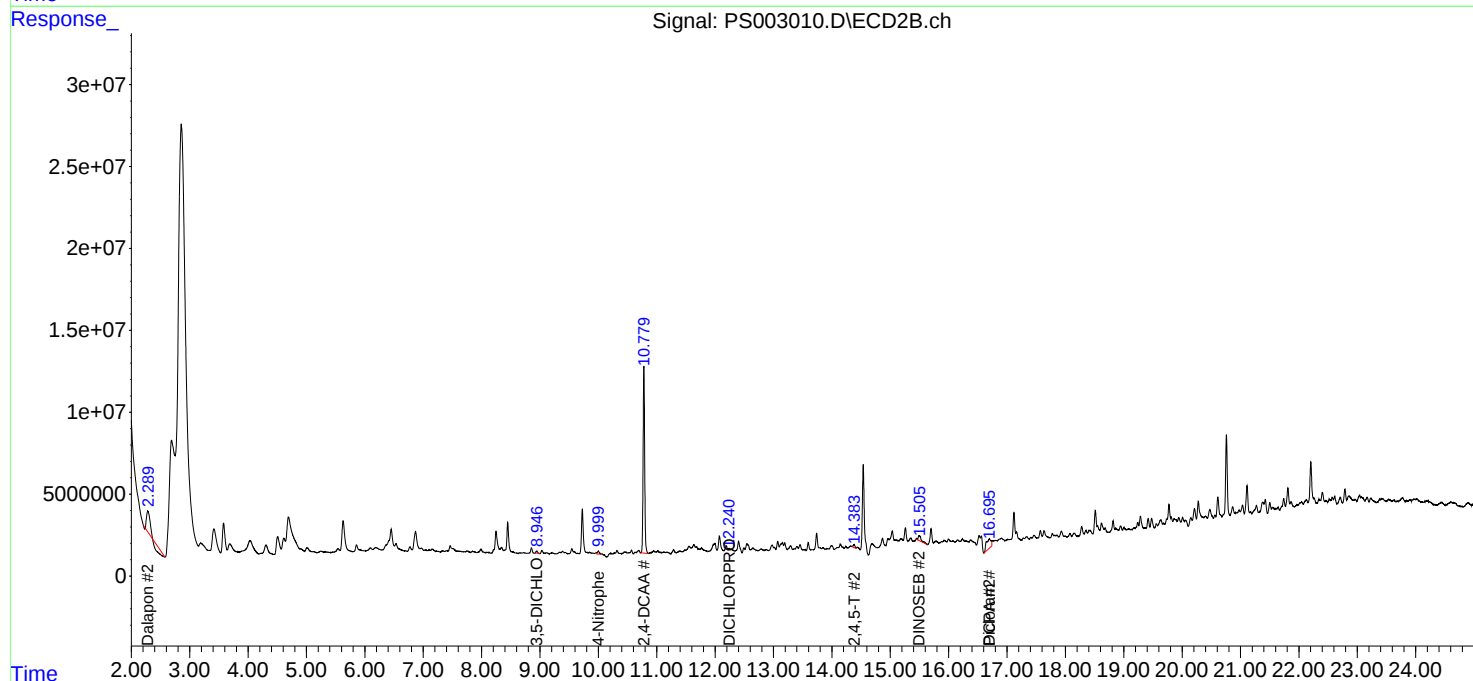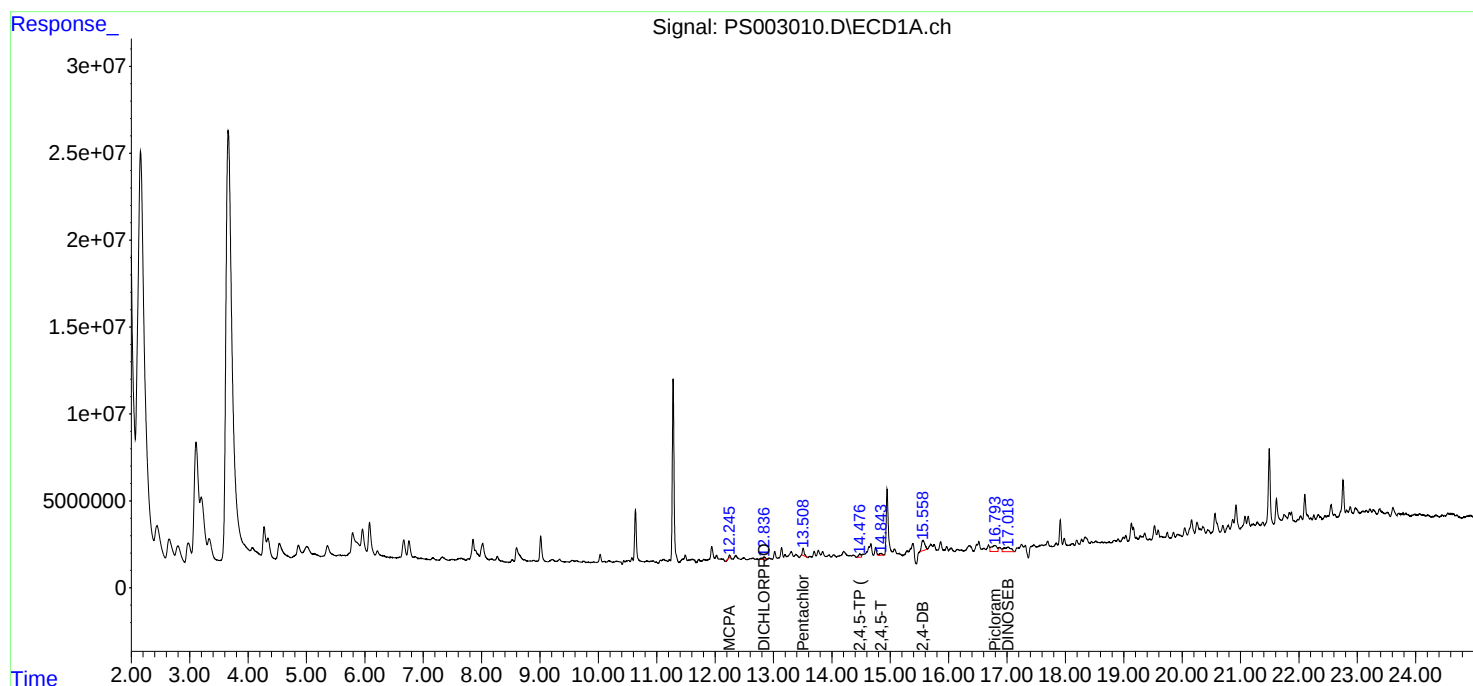


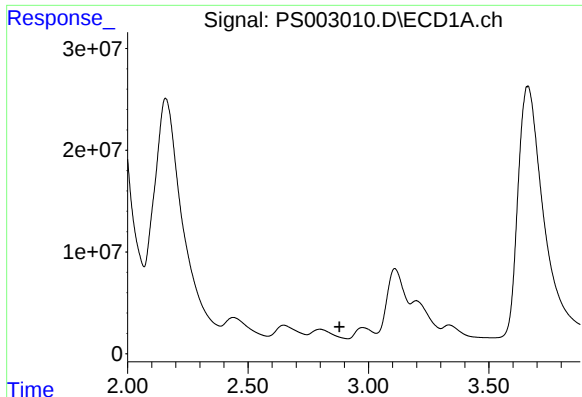

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

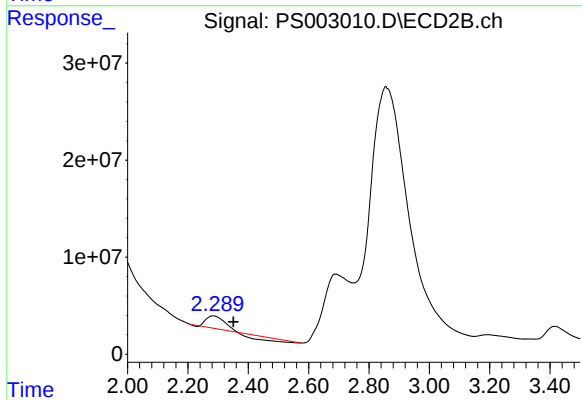


#1 Dalapon

R.T.: 2.283 min
Delta R.T.: -0.067 min
Response: 25162631
Conc: 46.95 ng/ml

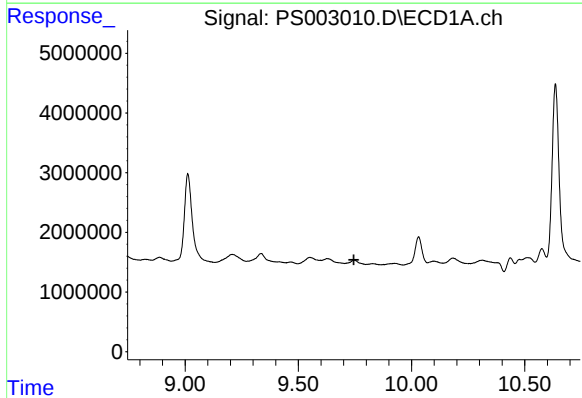


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

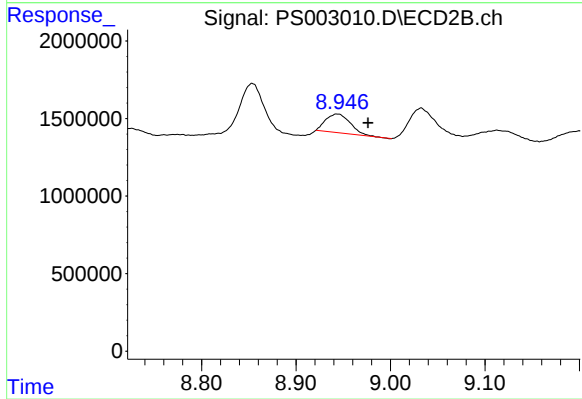

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.944 min
Delta R.T.: -0.033 min
Response: 2173995
Conc: 3.86 ng/ml

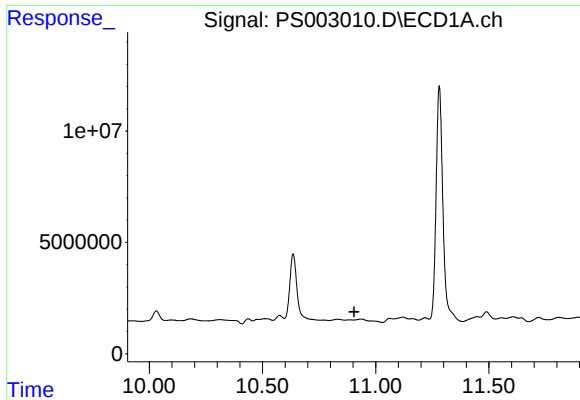

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

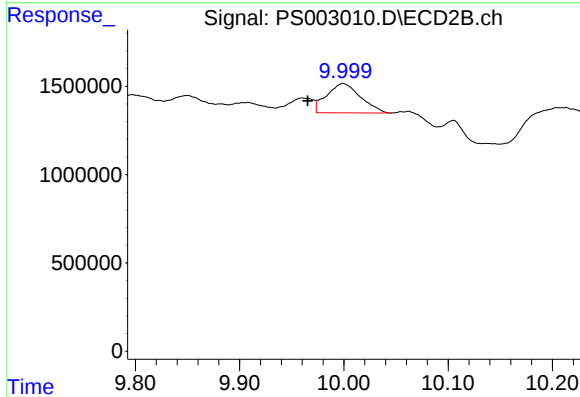


#3 4-Nitrophenol

R.T.: 9.999 min
Delta R.T.: 0.034 min
Response: 3757665
Conc: 17.98 ng/ml

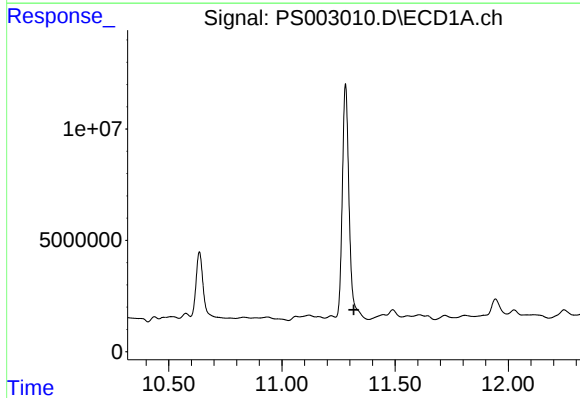


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.318 min
Response: 0
Conc: N.D.

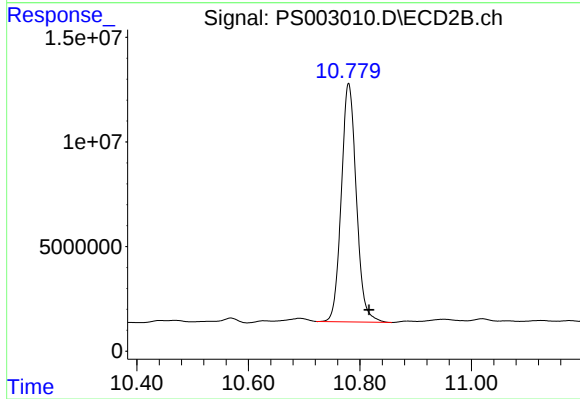

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: -0.037 min
Response: 212974540
Conc: 498.13 ng/ml

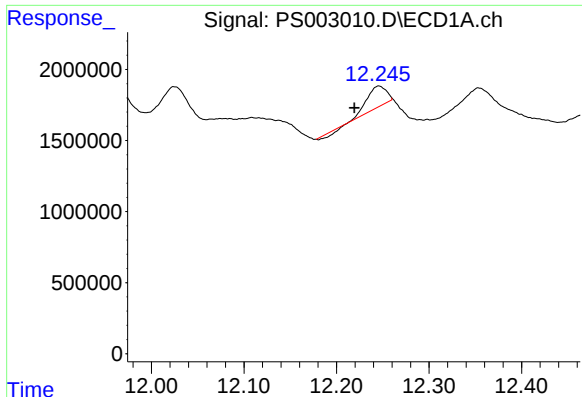

#7 MCPA


R.T.: 12.246 min
Delta R.T.: 0.027 min
Response: 2397041
Conc: 1.35 ug/ml

Instrument :
ECD_S
ClientSampleId :

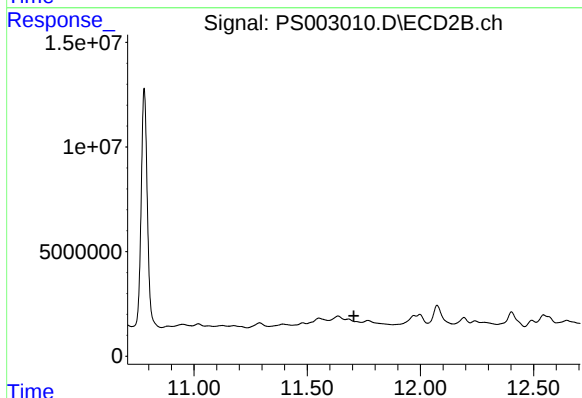


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

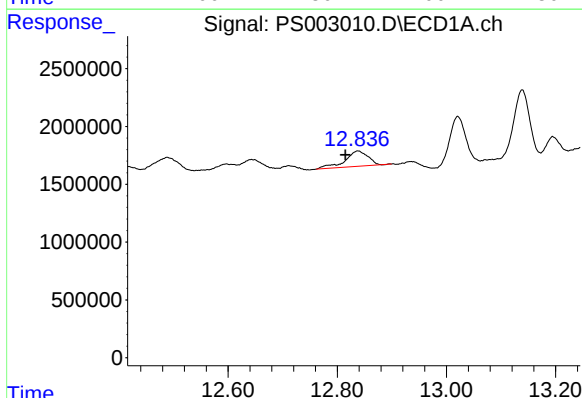


#8 DICHLORPROP

R.T.: 12.838 min
Delta R.T.: 0.023 min
Response: 3934591
Conc: 10.26 ng/ml

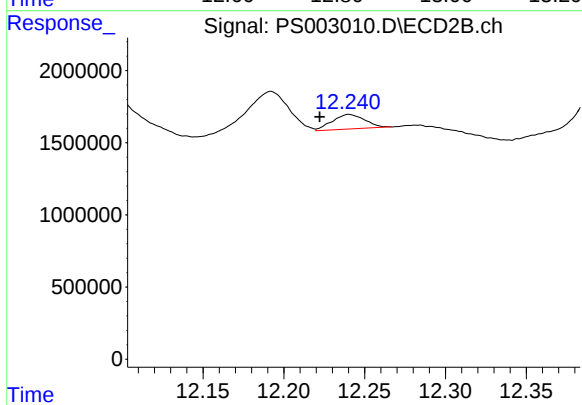

#8 DICHLORPROP


R.T.: 12.241 min
Delta R.T.: 0.019 min
Response: 1405515
Conc: 3.68 ng/ml

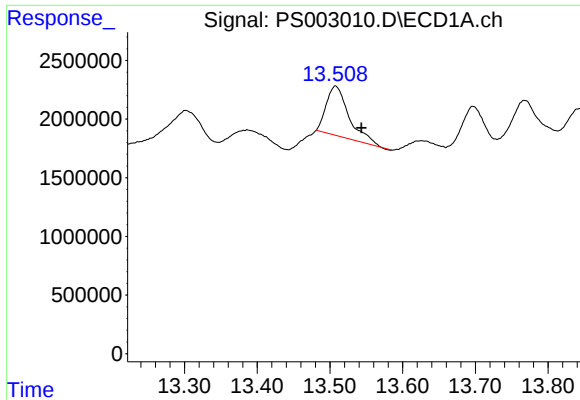

#10 Pentachlorophenol


R.T.: 13.508 min
Delta R.T.: -0.036 min
Response: 9145736
Conc: 1.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

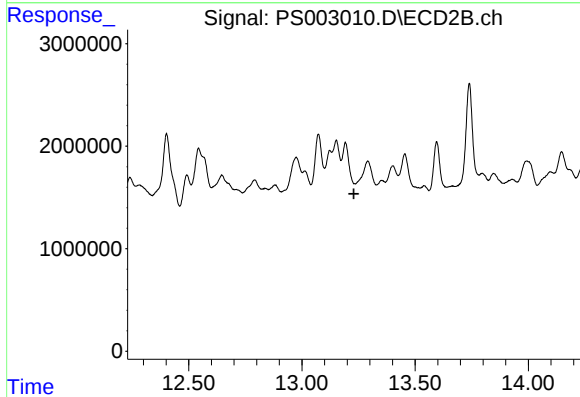


#10 Pentachlorophenol

R.T.: 13.291 min
Delta R.T.: 0.062 min
Response: -6634086
Conc: N.D.

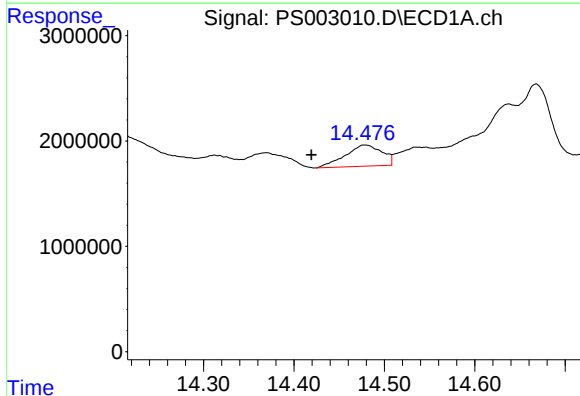


#11 2,4,5-TP (SILVEX)

R.T.: 14.479 min
Delta R.T.: 0.060 min
Response: 5696172
Conc: 2.26 ng/ml

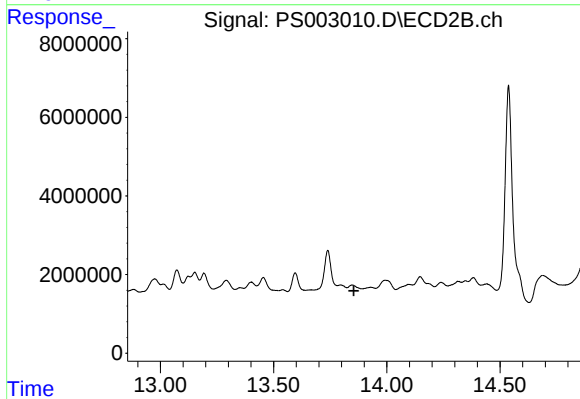

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

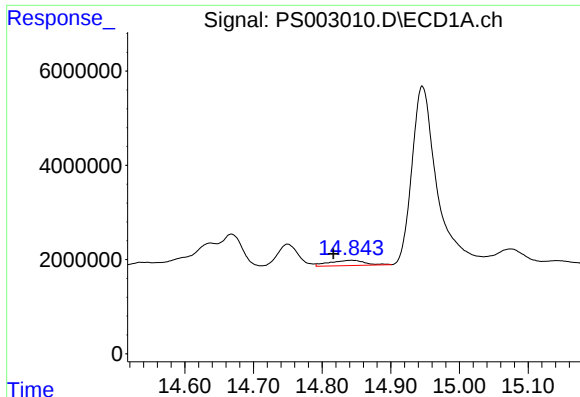

#12 2,4,5-T


R.T.: 14.842 min
Delta R.T.: 0.026 min
Response: 3940111
Conc: 1.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

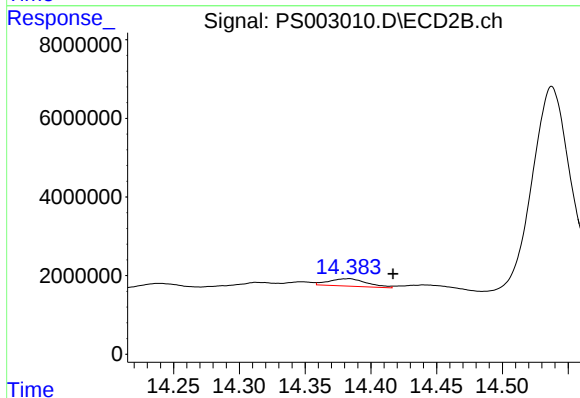


#12 2,4,5-T

R.T.: 14.382 min
Delta R.T.: -0.035 min
Response: 3788762
Conc: 1.98 ng/ml

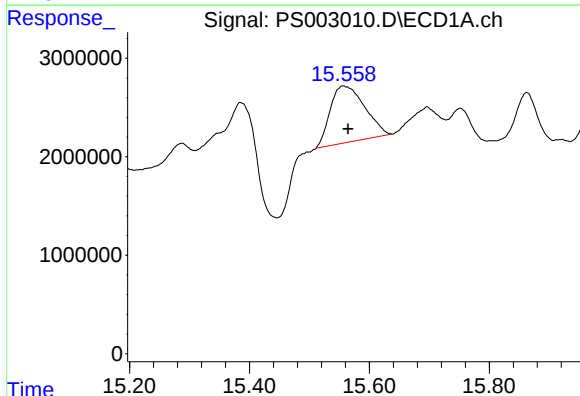


#13 2,4-DB

R.T.: 15.558 min
Delta R.T.: -0.006 min
Response: 22904020
Conc: 87.61 ng/ml

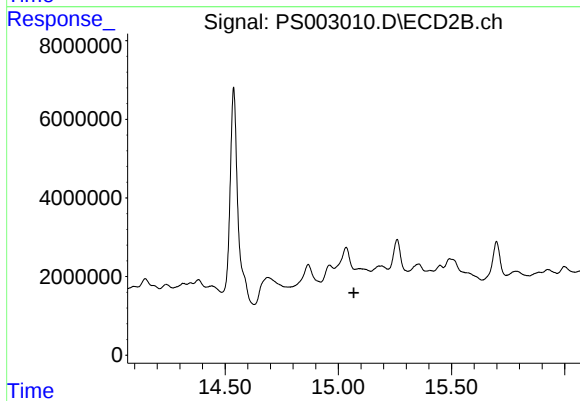

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.069 min
Response: 0
Conc: N.D.

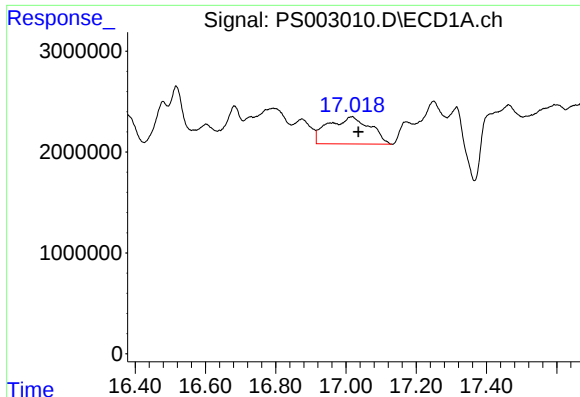

#14 DINOSEB


R.T.: 17.016 min
Delta R.T.: -0.020 min
Response: 22264395
Conc: 11.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

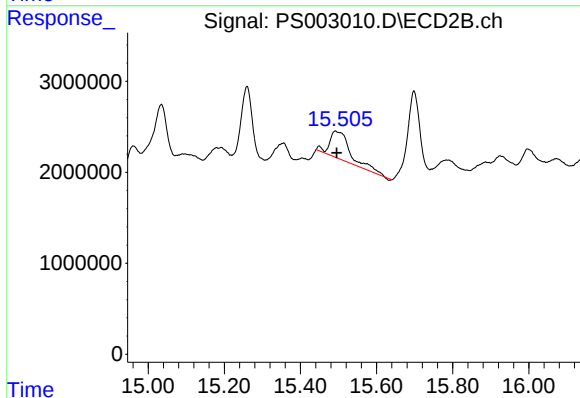


#14 DINOSEB

R.T.: 15.495 min
Delta R.T.: 0.000 min
Response: 10685831
Conc: 6.10 ng/ml

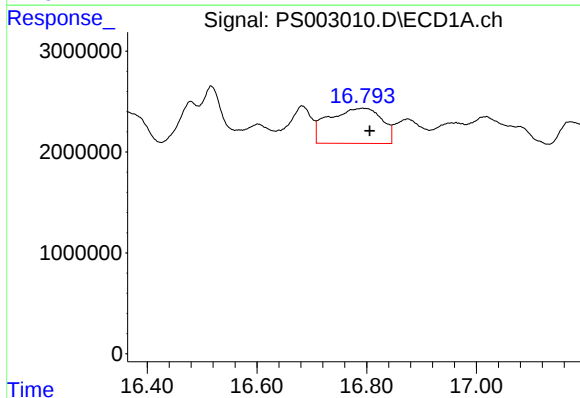


#15 Picloram

R.T.: 16.793 min
Delta R.T.: -0.013 min
Response: 23372985
Conc: 7.39 ng/ml

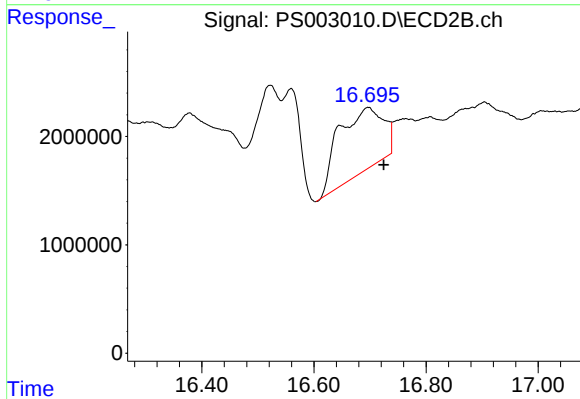

#15 Picloram


R.T.: 16.697 min
Delta R.T.: -0.028 min
Response: 32410952
Conc: 10.78 ng/ml

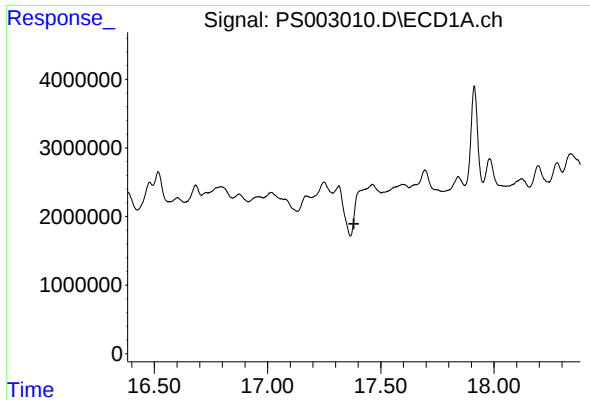

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

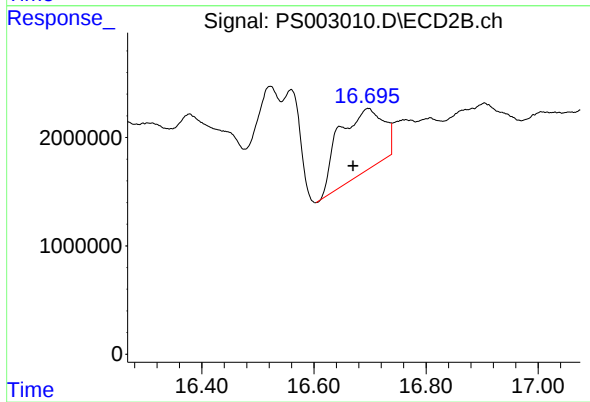

#16 DCPA

R.T.: 16.697 min
Delta R.T.: 0.027 min
Response: 32410952
Conc: 10.46 ng/ml