

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020420\
 Data File : PS008708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2020 16:37
 Operator : DD\AJ
 Sample : PB126575BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB126575BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 02:38:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.252	6.946	1038.6E6	487.2E6	483.912	525.709
Target Compounds							
1) T	Dalapon	0.000	2.595	0	248.1E6	N.D.	206.846
2) T	3,5-DICHL...	0.000	6.119	0	102.8E6	N.D.	74.709
7) T	MCPA	7.805	0.000	56288046	0	6.552	N.D. #
15) T	Picloram	11.050	11.040	278.3E6	177.8E6	18.379	23.553 #
16) T	DCPA	0.000	11.040	0	177.8E6	N.D.	27.333



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020420\
Data File : PS008708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2020 16:37
Operator : DD\AJ
Sample : PB126575BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB126575BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 02:38:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

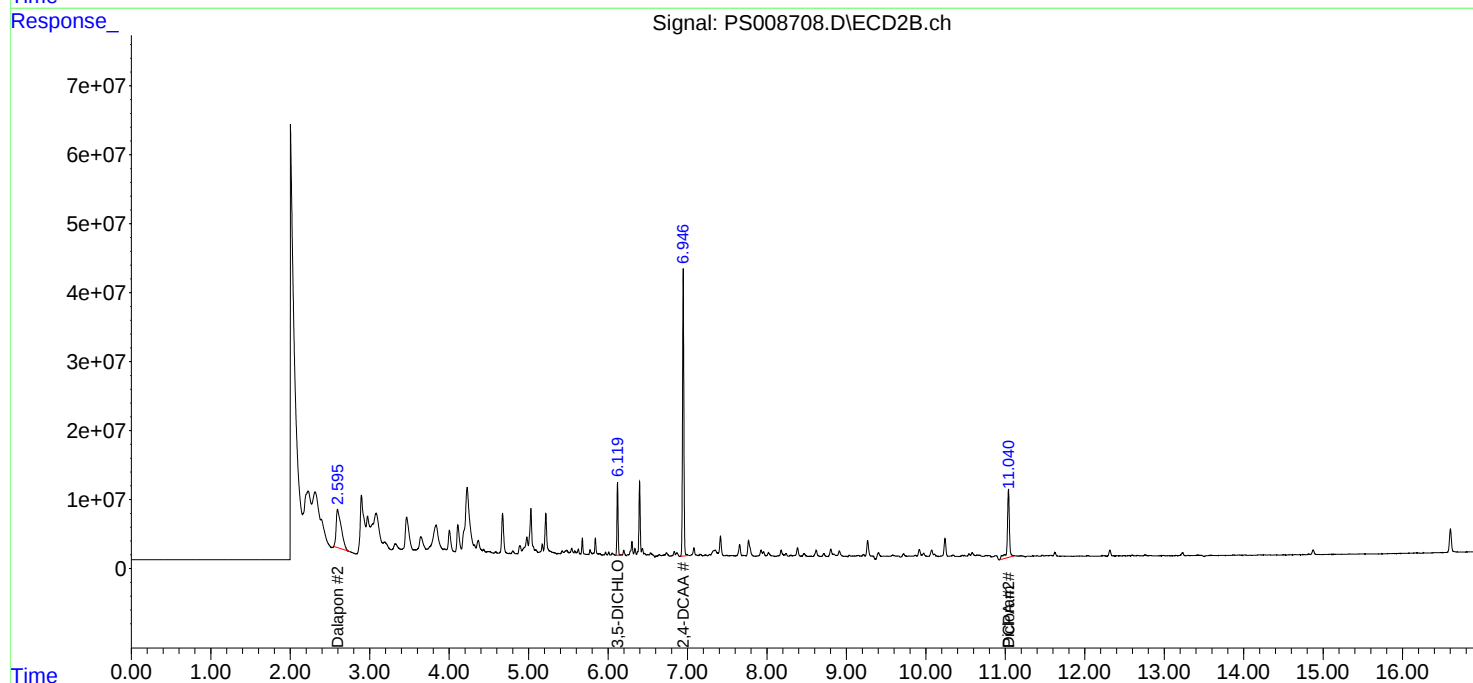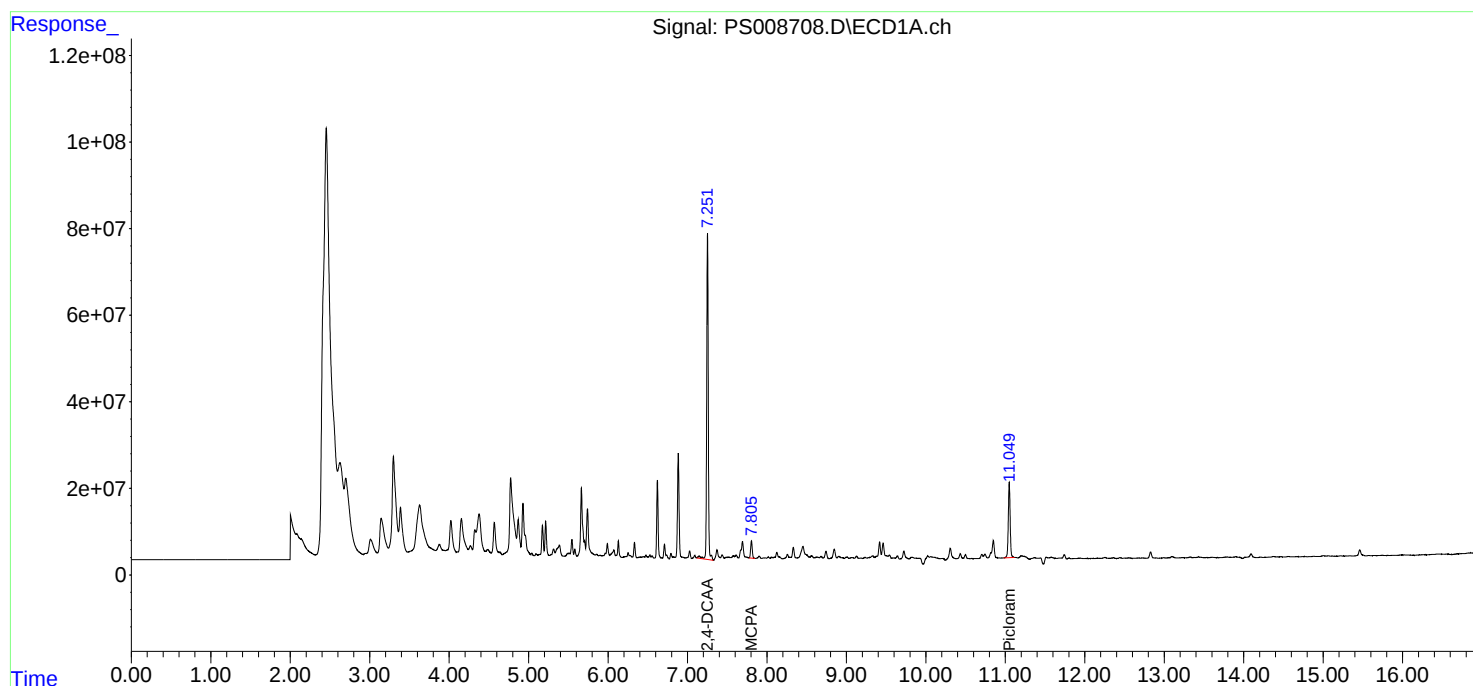


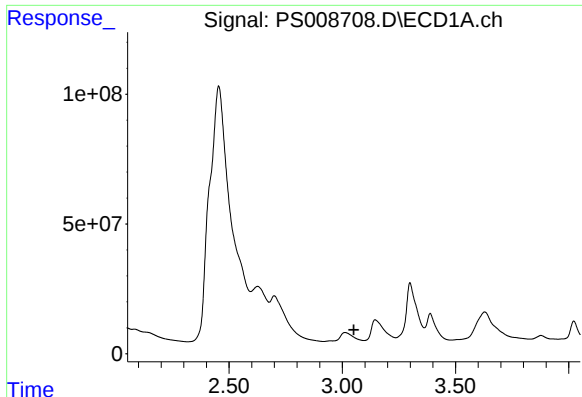

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB126575BL

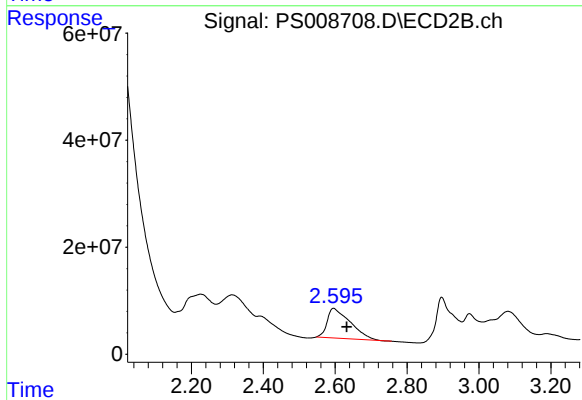


#1 Dalapon

R.T.: 2.595 min
Delta R.T.: -0.036 min
Response: 248074353
Conc: 206.85 ng/ml

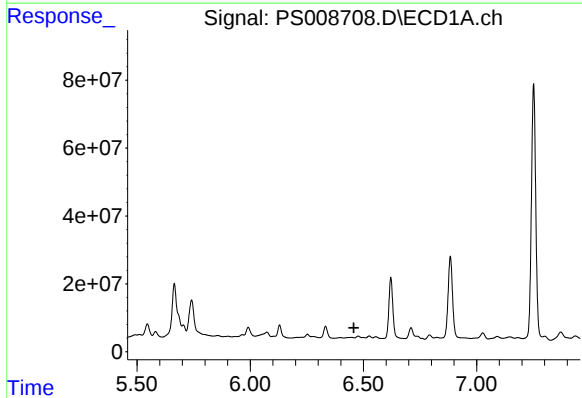


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

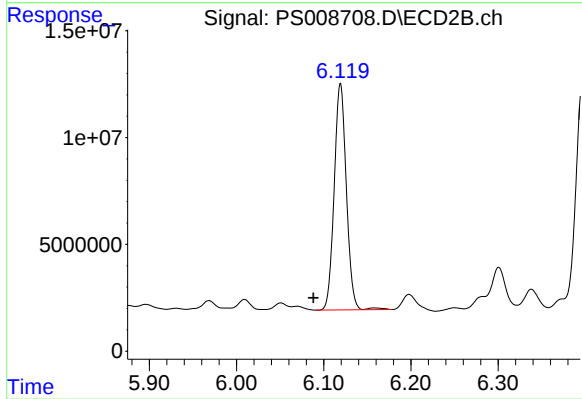

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.119 min
Delta R.T.: 0.031 min
Response: 102790448
Conc: 74.71 ng/ml

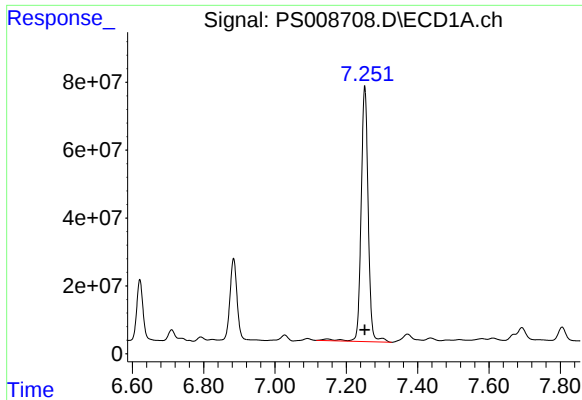

#4 2,4-DCAA


R.T.: 7.252 min
Delta R.T.: 0.000 min
Response: 1038624508
Conc: 483.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126575BL

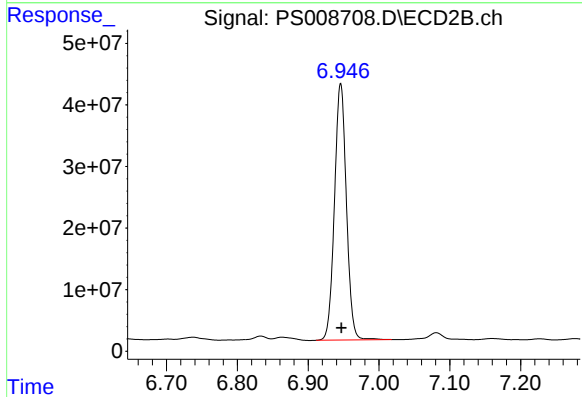


#4 2,4-DCAA

R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 487239324
Conc: 525.71 ng/ml

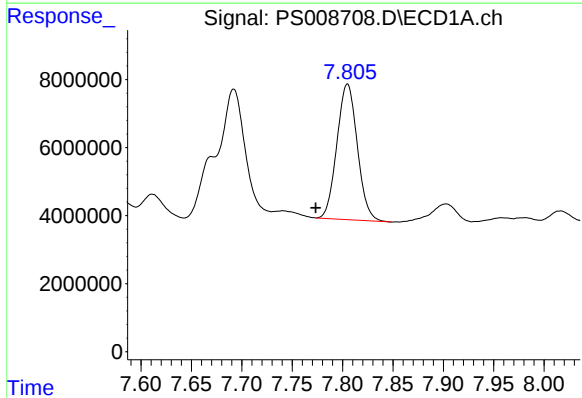


#7 MCPA

R.T.: 7.805 min
Delta R.T.: 0.032 min
Response: 56288046
Conc: 6.55 ug/ml

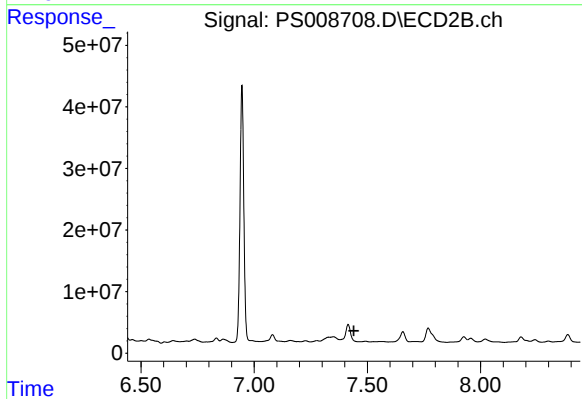

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.441 min
Response: 0
Conc: N.D.

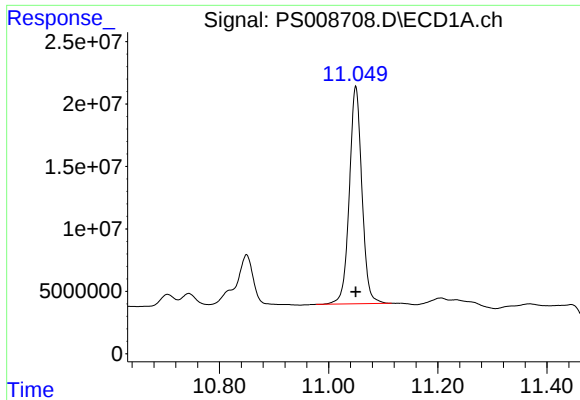

#15 Picloram


R.T.: 11.050 min
Delta R.T.: 0.000 min
Response: 278327128
Conc: 18.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126575BL

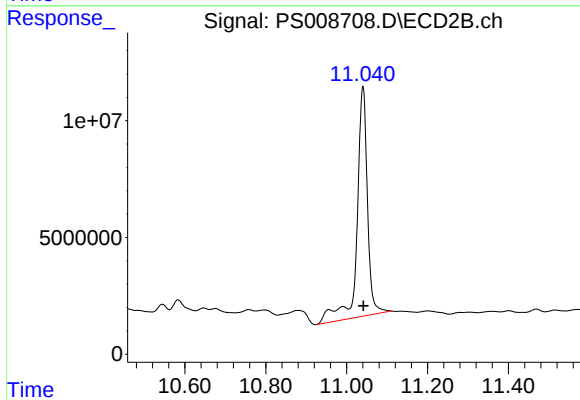


#15 Picloram

R.T.: 11.040 min
Delta R.T.: -0.001 min
Response: 177778159
Conc: 23.55 ng/ml

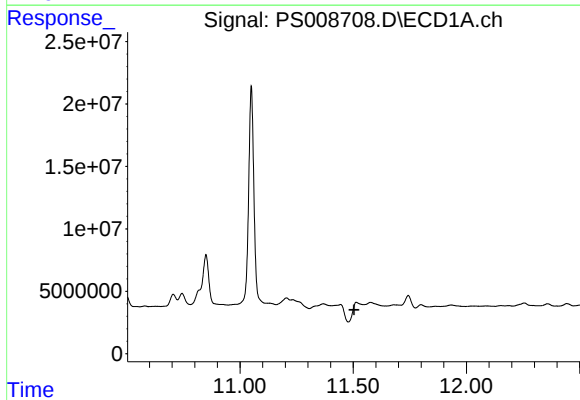

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.503 min
Response: 0
Conc: N.D.

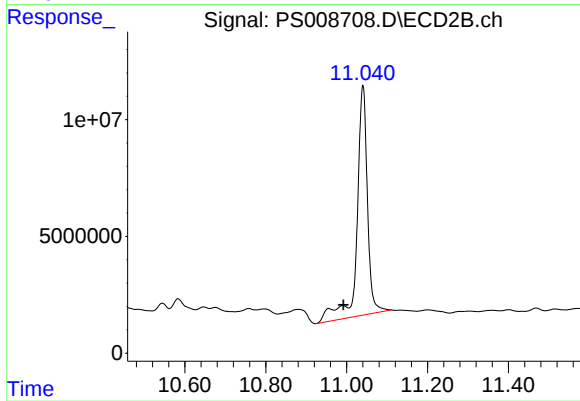

#16 DCPA

R.T.: 11.040 min
Delta R.T.: 0.048 min
Response: 177778159
Conc: 27.33 ng/ml