

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020420\
 Data File : PS008710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2020 17:22
 Operator : DD\AJ
 Sample : PB126575TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB126575TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 02:39:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.250	6.946	681.5E6	337.1E6	317.518	363.694
Target Compounds							
1) T	Dalapon	3.010	2.596	128.2E6	186.5E6	50.534	155.518 #
2) T	3,5-DICHL...	0.000	6.119	0	129.5E6	N.D.	94.116
8) T	DICHLORPROP	0.000	7.768	0	46106367	N.D.	48.395
12) T	2,4,5-T	9.460	0.000	73629729	0	6.690	N.D. #
15) T	Picloram	11.049	0.000	71023543	0	4.690	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020420\
Data File : PS008710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2020 17:22
Operator : DD\AJ
Sample : PB126575TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB126575TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 02:39:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

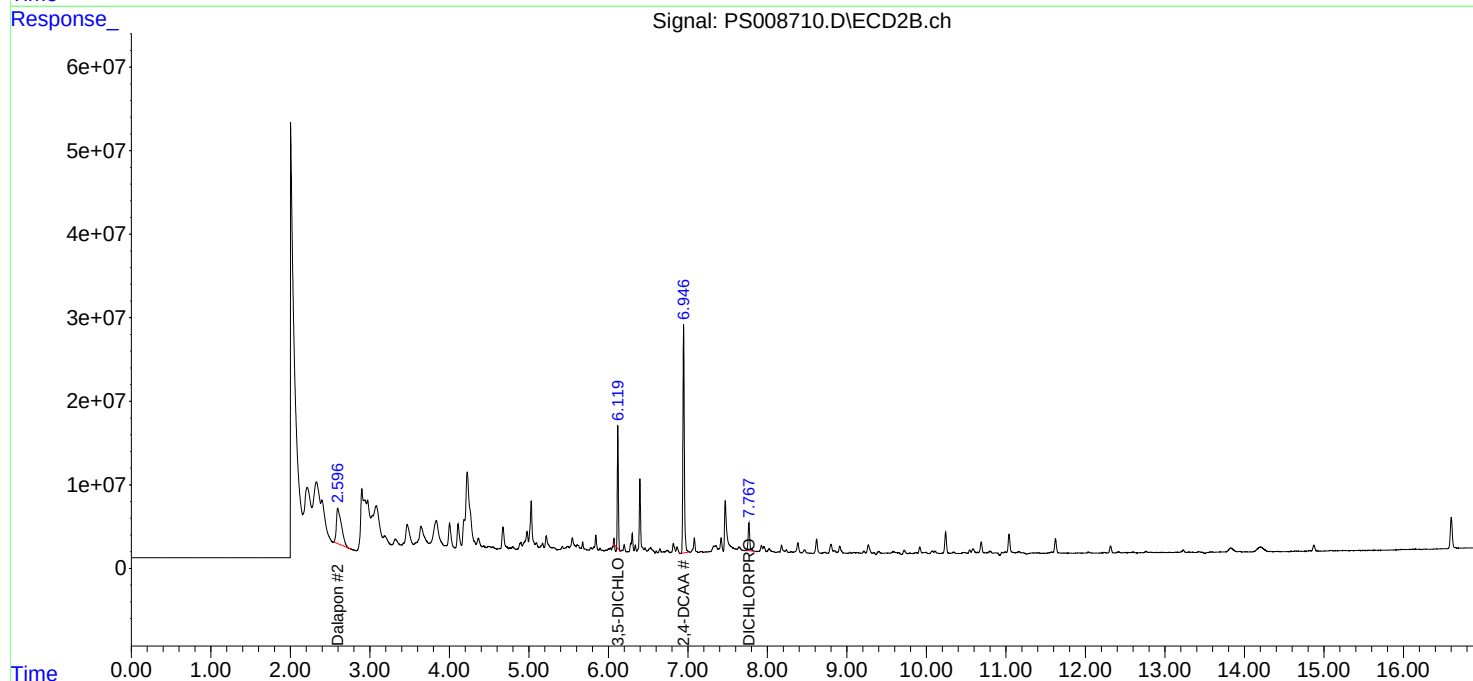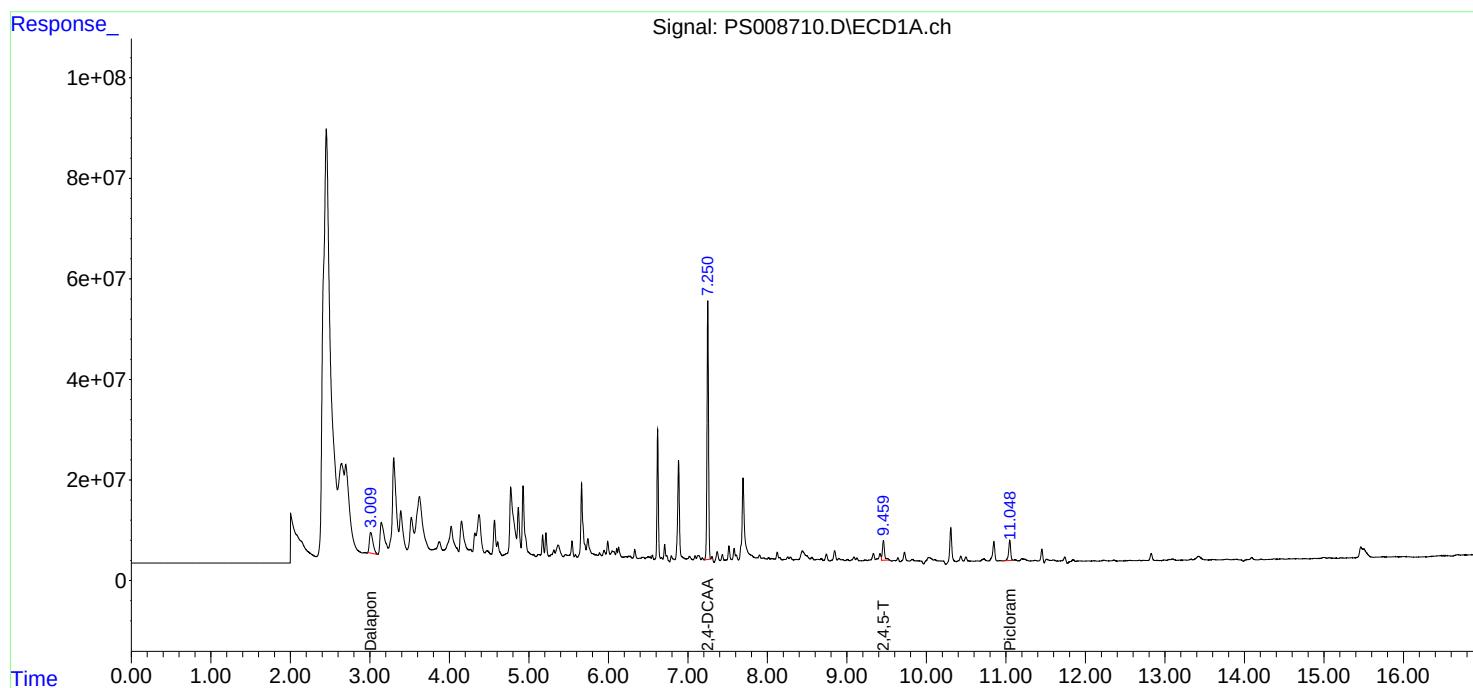


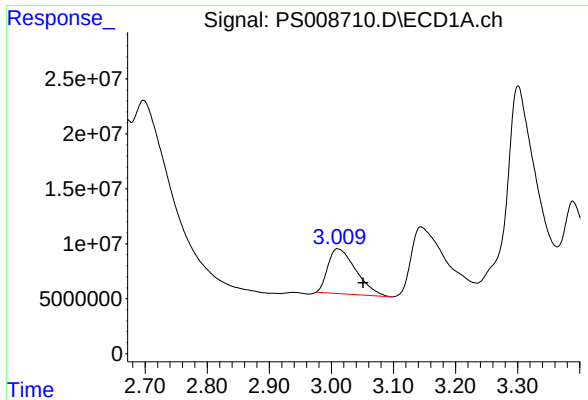

#1 Dalapon


R.T.: 3.010 min
Delta R.T.: -0.041 min
Response: 128168738
Conc: 50.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126575TB

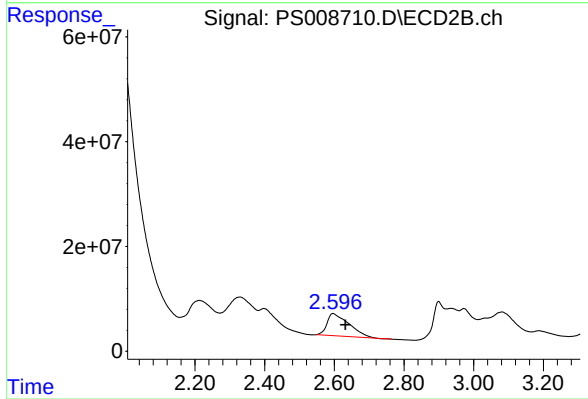


#1 Dalapon

R.T.: 2.596 min
Delta R.T.: -0.036 min
Response: 186515467
Conc: 155.52 ng/ml

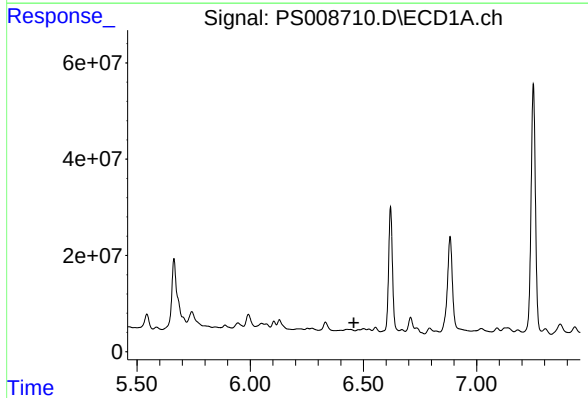


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.458 min
Response: 0
Conc: N.D.

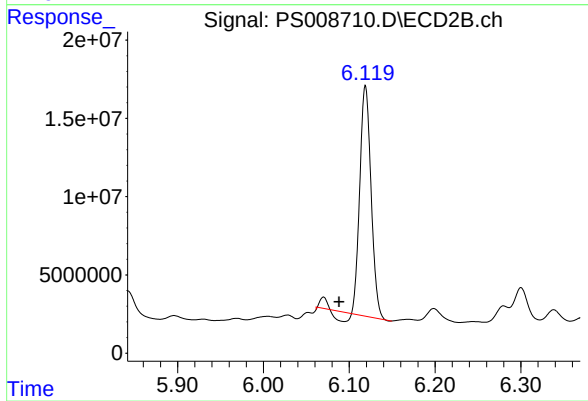

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.119 min
Delta R.T.: 0.031 min
Response: 129492118
Conc: 94.12 ng/ml

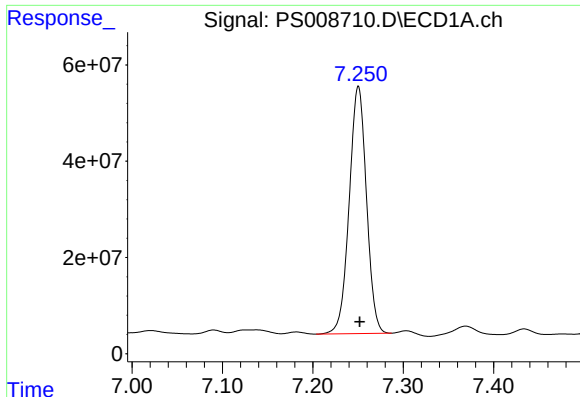

#4 2,4-DCAA


R.T.: 7.250 min
Delta R.T.: -0.001 min
Response: 681491239
Conc: 317.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126575TB

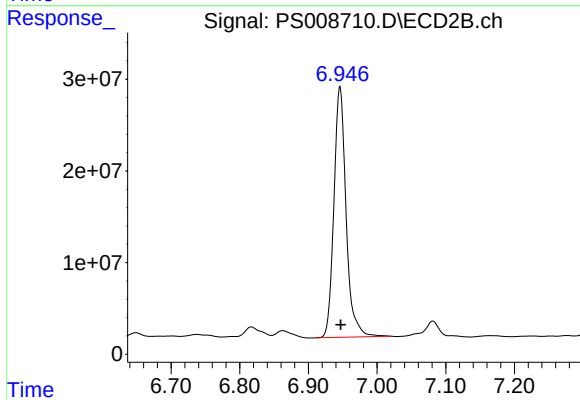


#4 2,4-DCAA

R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 337080084
Conc: 363.69 ng/ml

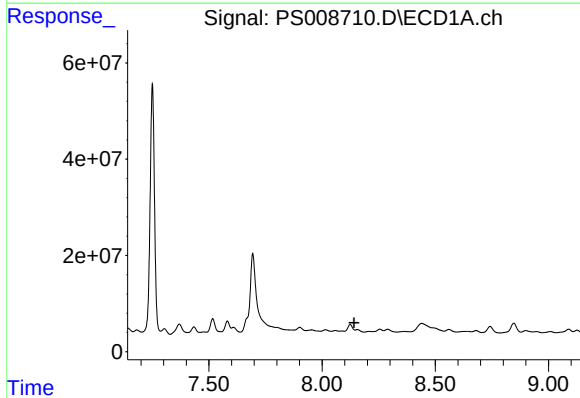


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.141 min
Response: 0
Conc: N.D.

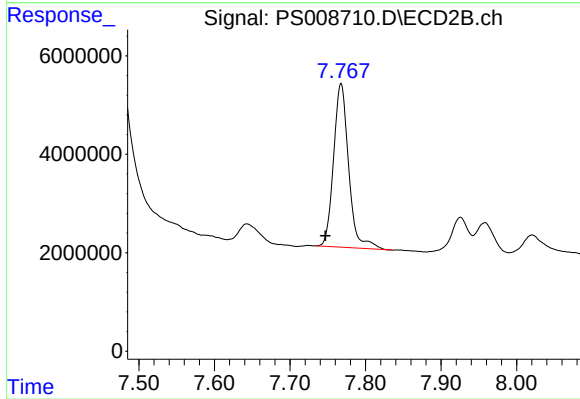

#8 DICHLORPROP


R.T.: 7.768 min
Delta R.T.: 0.021 min
Response: 46106367
Conc: 48.40 ng/ml

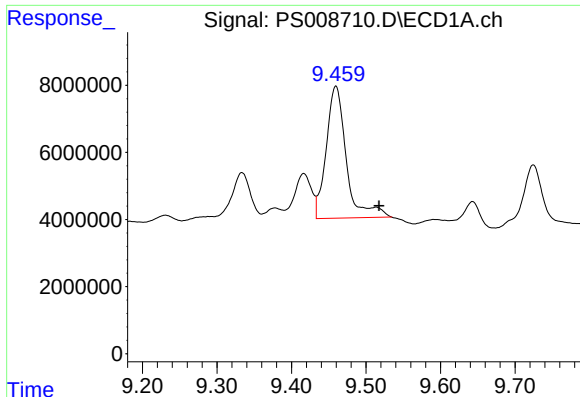

#12 2,4,5-T


R.T.: 9.460 min
Delta R.T.: -0.058 min
Response: 73629729
Conc: 6.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126575TB

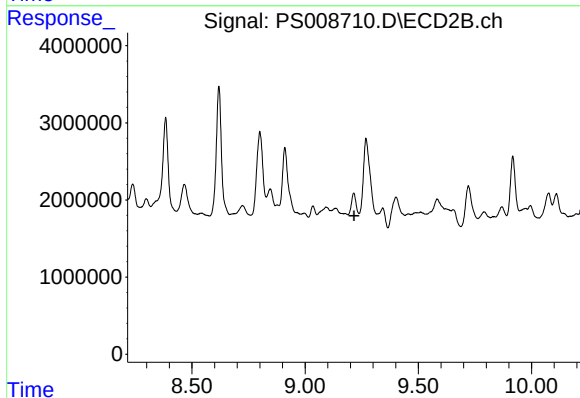


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

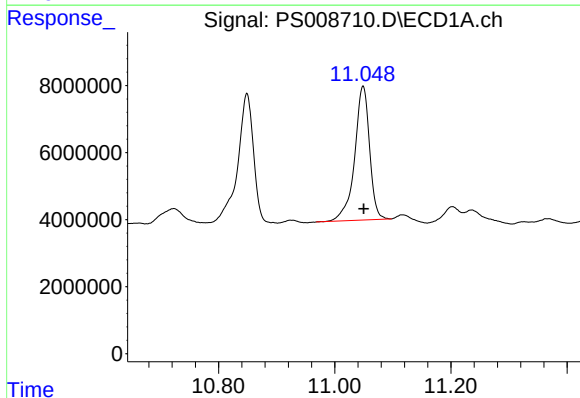

#15 Picloram

R.T.: 11.049 min
Delta R.T.: -0.001 min
Response: 71023543
Conc: 4.69 ng/ml

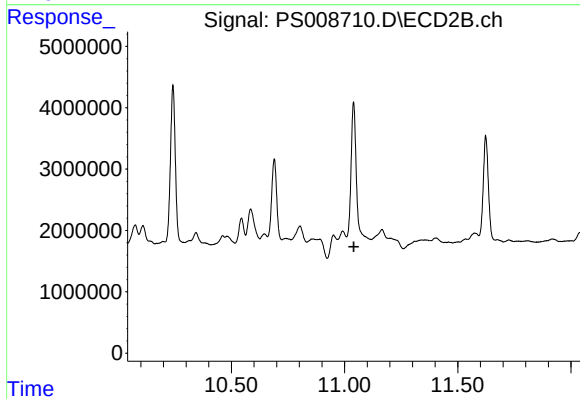

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.041 min
Response: 0
Conc: N.D.