

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020420\
 Data File : PS008720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2020 21:11
 Operator : DD\AJ
 Sample : L1383-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-B-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 02:42:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.250	6.946	978.2E6	468.7E6	455.744	505.698
Target Compounds							
1) T	Dalapon	0.000	2.596	0	300.1E6	N.D.	250.213
2) T	3,5-DICHL...	0.000	6.120	0	134.3E6	N.D.	97.640
12) T	2,4,5-T	9.460	0.000	63391606	0	5.760	N.D. #
15) T	Picloram	11.048	11.040	150.7E6	95404350	9.949	12.640 #
16) T	DCPA	0.000	11.040	0	95404350	N.D.	14.668



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020420\
Data File : PS008720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2020 21:11
Operator : DD\AJ
Sample : L1383-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-B-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 02:42:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

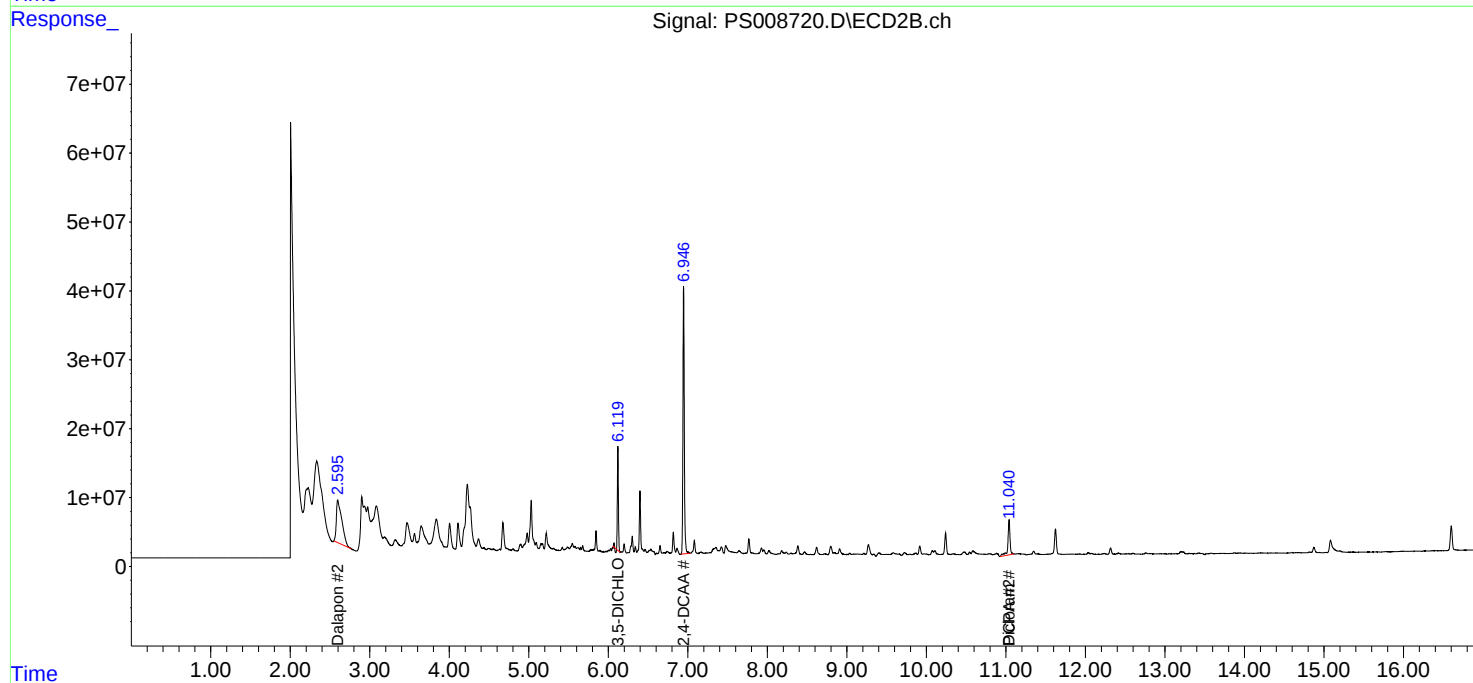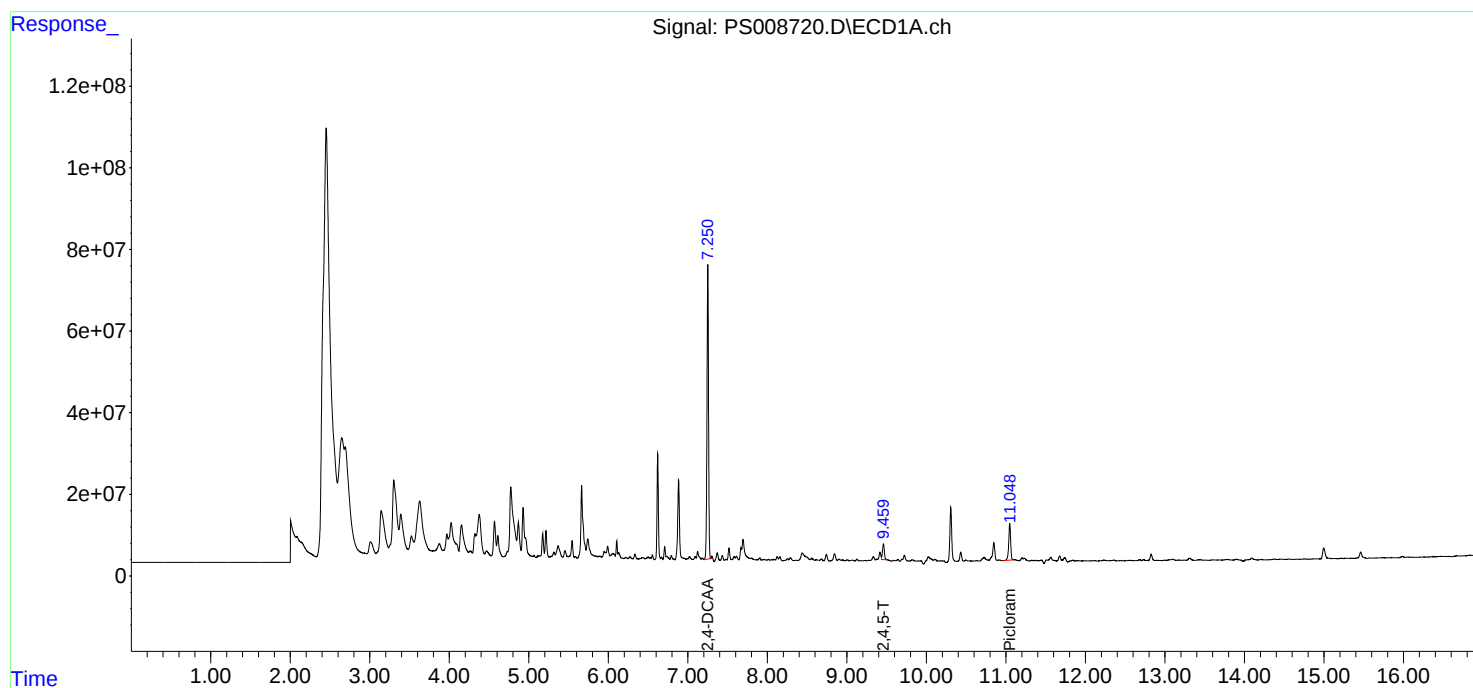


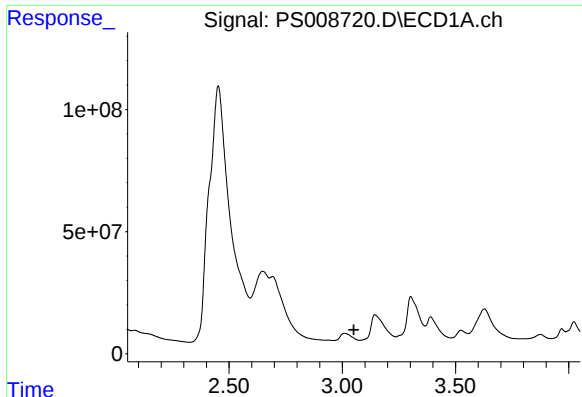

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-B-1

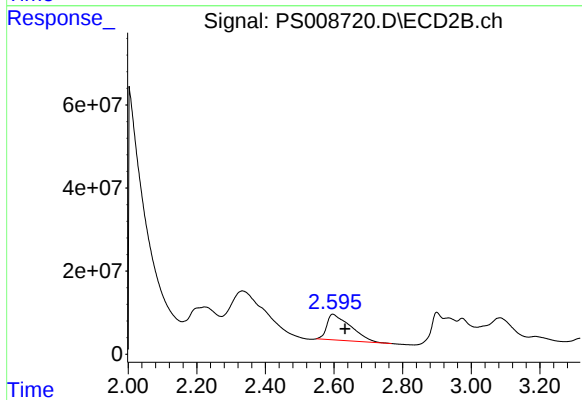


#1 Dalapon

R.T.: 2.596 min
Delta R.T.: -0.035 min
Response: 300084487
Conc: 250.21 ng/ml

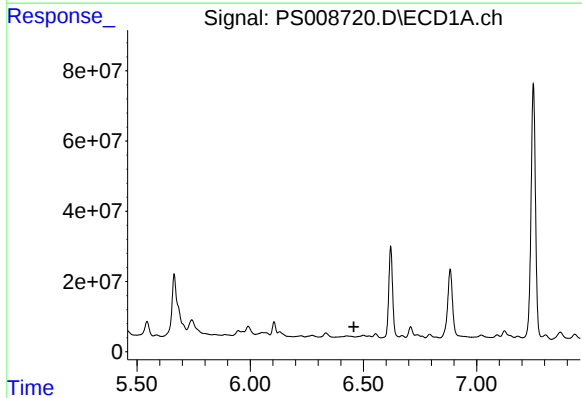


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

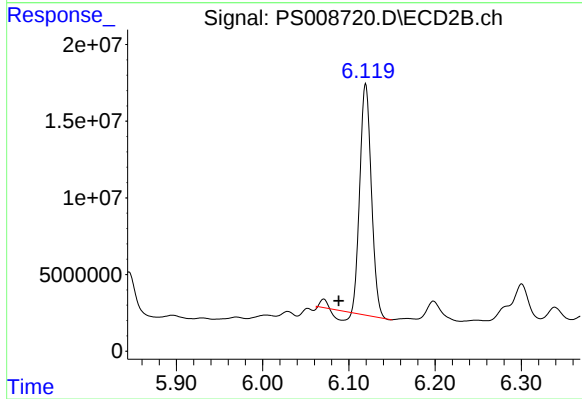

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.120 min
Delta R.T.: 0.031 min
Response: 134341289
Conc: 97.64 ng/ml

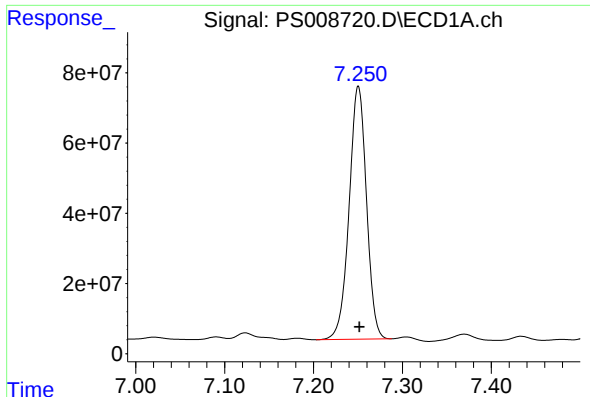

#4 2,4-DCAA


R.T.: 7.250 min
Delta R.T.: -0.001 min
Response: 978168462
Conc: 455.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-B-1

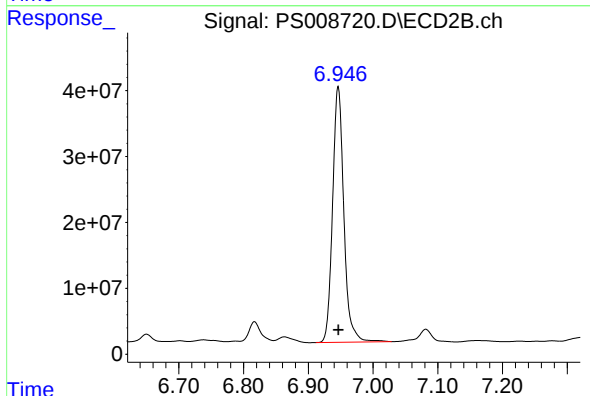


#4 2,4-DCAA

R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 468693341
Conc: 505.70 ng/ml

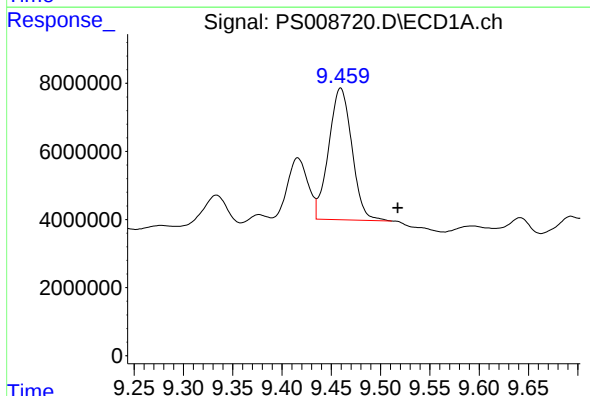


#12 2,4,5-T

R.T.: 9.460 min
Delta R.T.: -0.058 min
Response: 63391606
Conc: 5.76 ng/ml

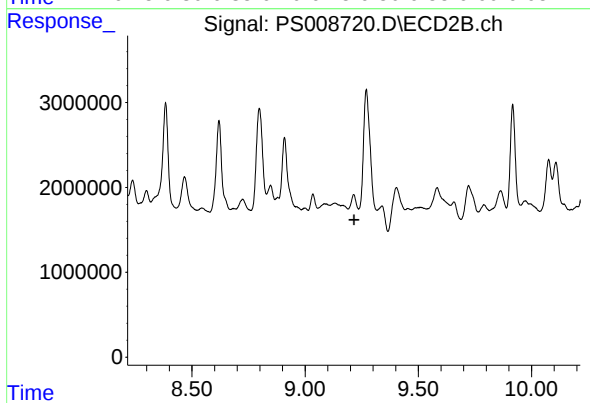

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.216 min
Response: 0
Conc: N.D.

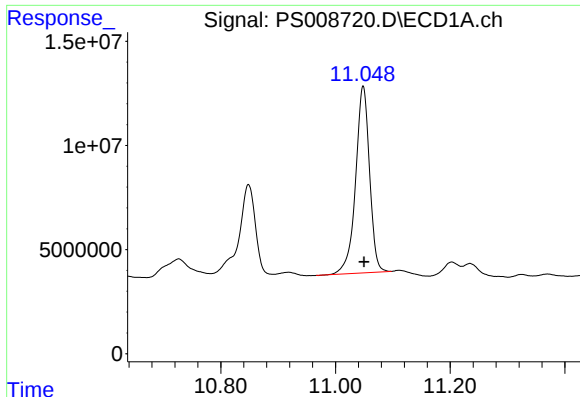

#15 Picloram


R.T.: 11.048 min
Delta R.T.: -0.002 min
Response: 150672671
Conc: 9.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-B-1

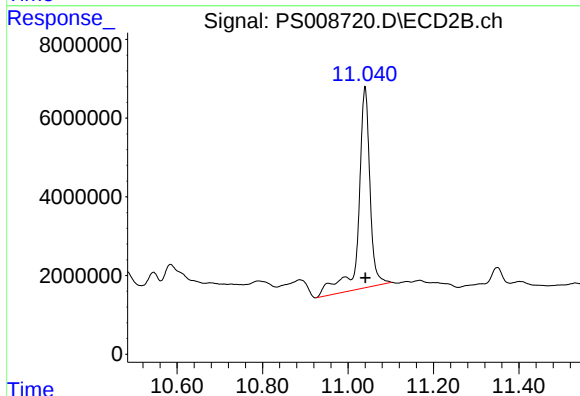


#15 Picloram

R.T.: 11.040 min
Delta R.T.: -0.001 min
Response: 95404350
Conc: 12.64 ng/ml

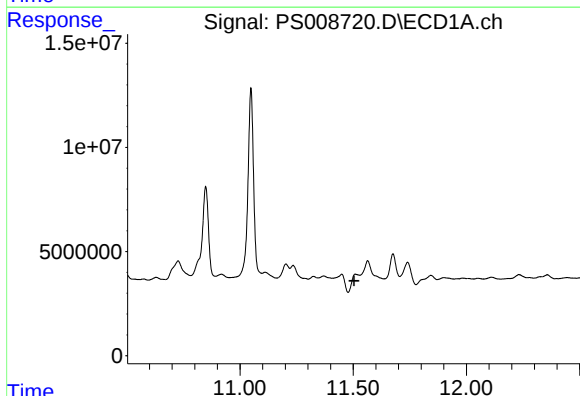

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.503 min
Response: 0
Conc: N.D.

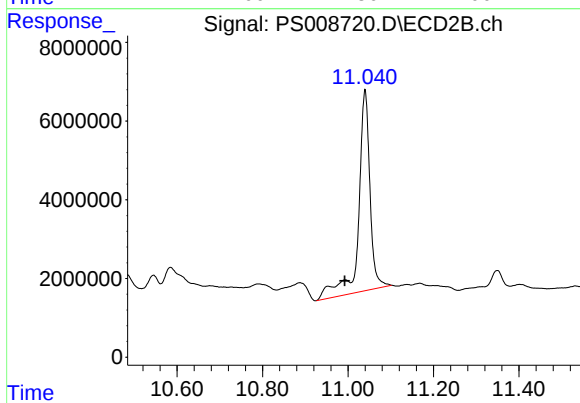

#16 DCPA

R.T.: 11.040 min
Delta R.T.: 0.048 min
Response: 95404350
Conc: 14.67 ng/ml