

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020420\
 Data File : PS008702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2020 13:56
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 15:34:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 04 15:33:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.251	6.947	1604.4E6	692.4E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.050	2.632	1766.4E6	842.5E6	682.500	682.500
2) T	3,5-DICHL...	6.458	6.088	1954.9E6	957.6E6	697.500	697.500
3) T	4-Nitroph...	7.080	6.546	738.2E6	387.4E6	682.500	682.500
5) T	DICAMBA	7.446	7.118	5713.0E6	2773.0E6	705.000	705.000
6) T	MCPD	7.616	7.216	442.2E6	211.0E6	70.500	70.500
7) T	MCPA	7.766	7.432	608.4E6	293.5E6	69.750	69.750
8) T	DICHLORPROP	8.140	7.747	1389.0E6	665.7E6	705.000	705.000
9) T	2,4-D	8.369	8.041	1514.5E6	807.0E6	705.000	705.000
10) T	Pentachlo...	8.683	8.475	20136.7E6	9372.7E6	712.500	712.500
11) T	2,4,5-TP ...	9.234	8.837	7942.7E6	3643.0E6	712.500	712.500
12) T	2,4,5-T	9.518	9.217	7931.2E6	3641.9E6	712.500	712.500
13) T	2,4-DB	10.072	9.725	1156.6E6	494.0E6	712.500	712.500
14) T	DINOSEB	11.239	10.061	5969.1E6	2607.6E6	705.000	705.000
15) T	Picloram	11.051	11.042	10977.3E6	5473.5E6	712.500	712.500
16) T	DCPA	11.503	10.993	10130.2E6	4684.5E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020420\
Data File : PS008702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2020 13:56
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 15:34:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Tue Feb 04 15:33:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

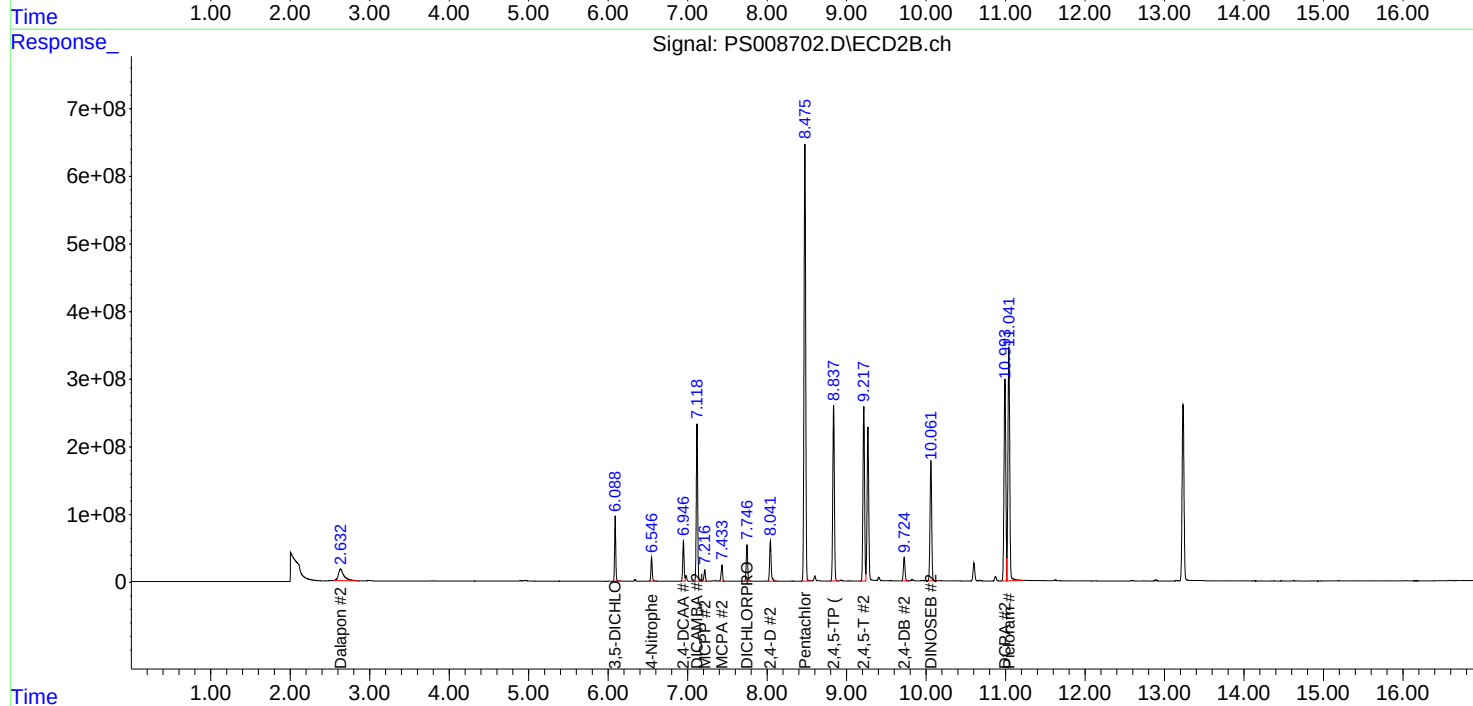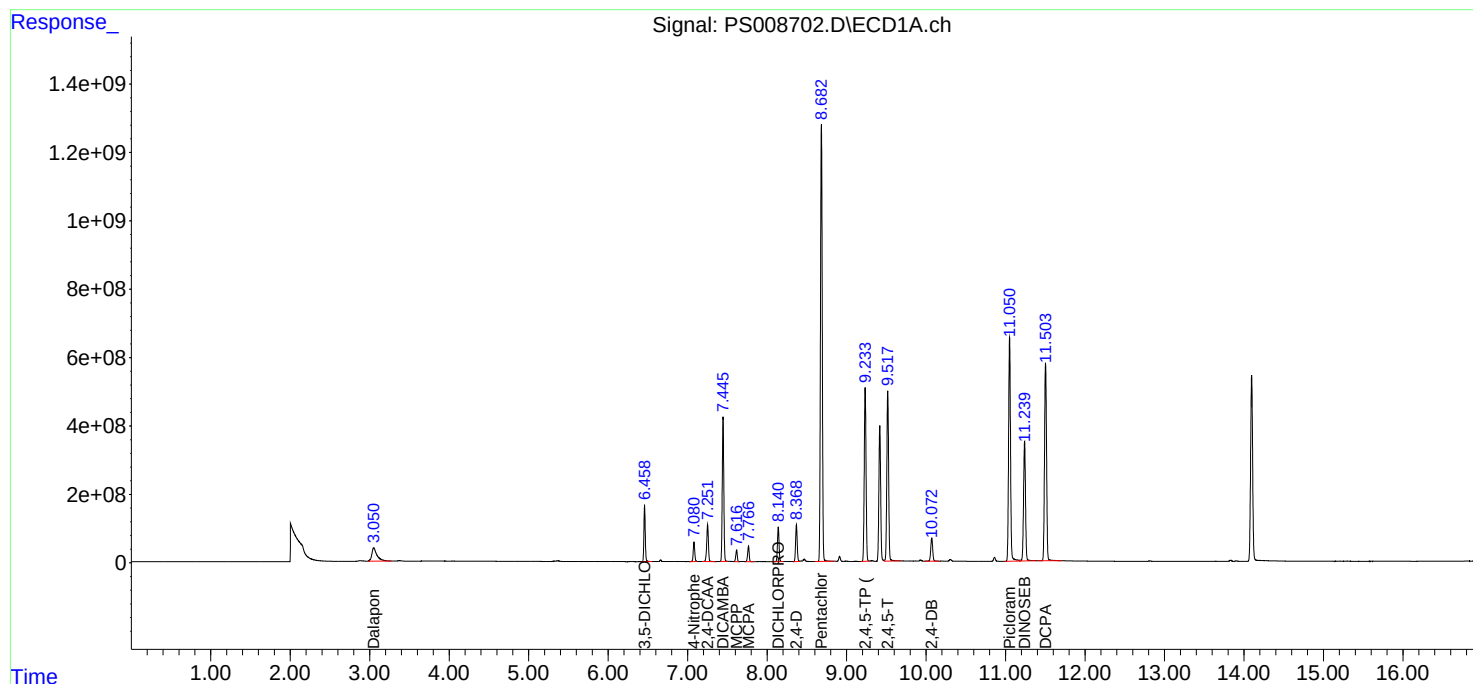


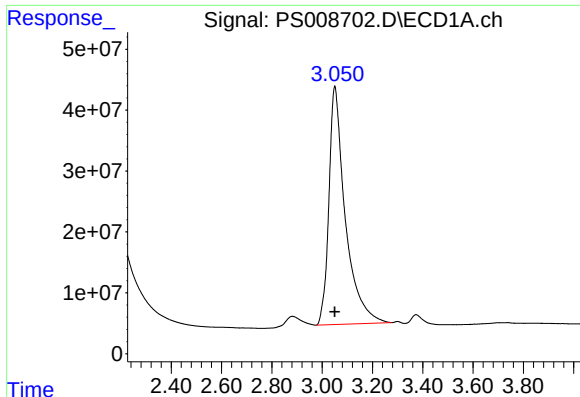

#1 Dalapon


R.T.: 3.050 min
Delta R.T.: 0.000 min
Response: 1766431025
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

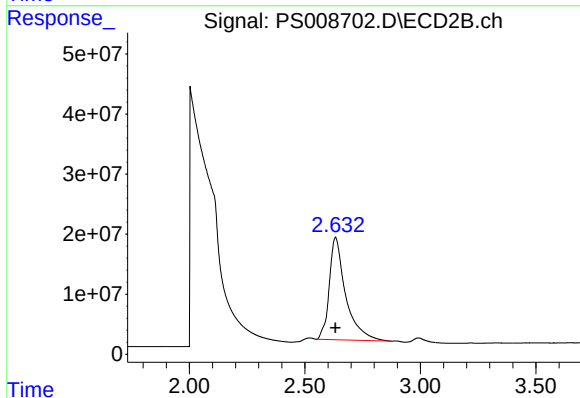


#1 Dalapon

R.T.: 2.632 min
Delta R.T.: 0.000 min
Response: 842525301
Conc: 682.50 ng/ml

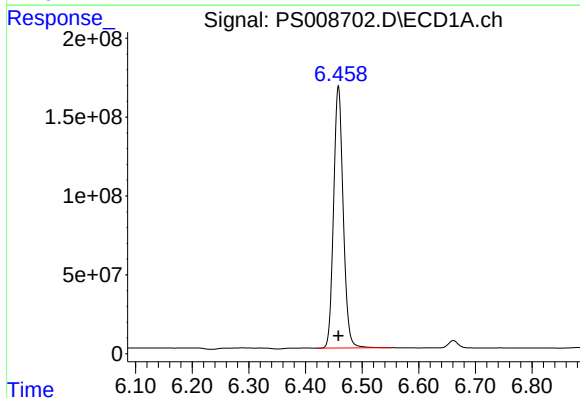


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.458 min
Delta R.T.: 0.000 min
Response: 1954886068
Conc: 697.50 ng/ml

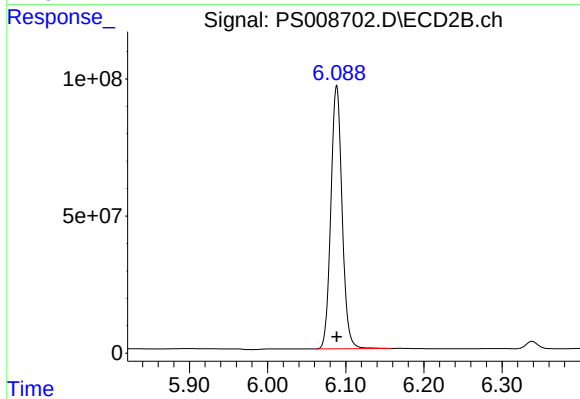

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 957584617
Conc: 697.50 ng/ml

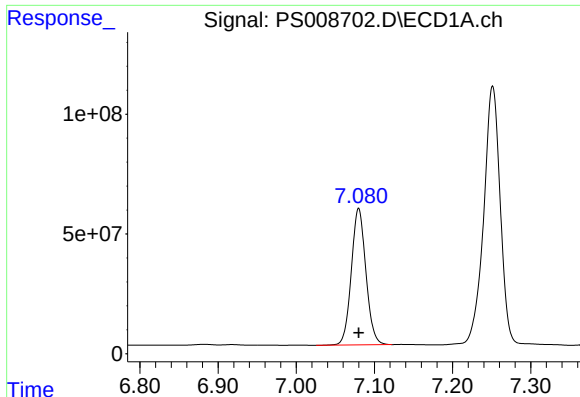

#3 4-Nitrophenol


R.T.: 7.080 min
Delta R.T.: 0.000 min
Response: 738178182
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

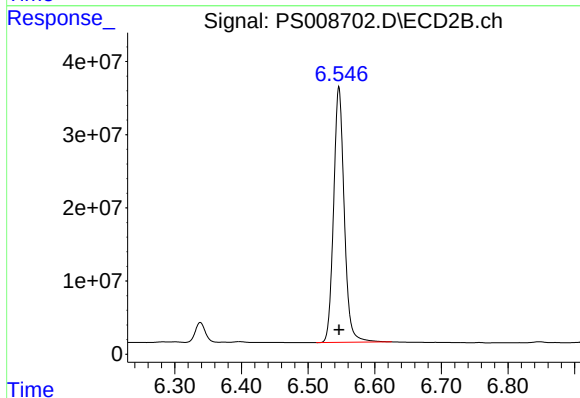


#3 4-Nitrophenol

R.T.: 6.546 min
Delta R.T.: 0.000 min
Response: 387409559
Conc: 682.50 ng/ml

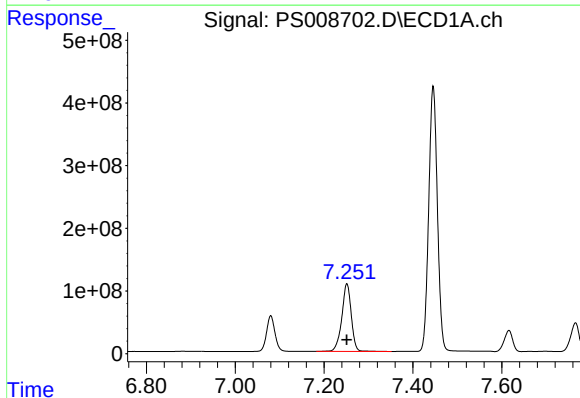


#4 2,4-DCAA

R.T.: 7.251 min
Delta R.T.: 0.000 min
Response: 1604427644
Conc: 750.00 ng/ml

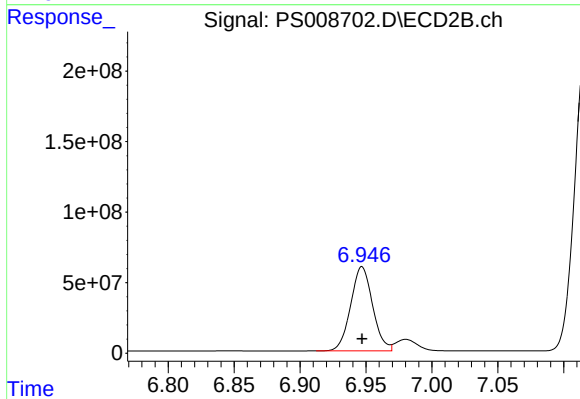

#4 2,4-DCAA


R.T.: 6.947 min
Delta R.T.: 0.000 min
Response: 692433339
Conc: 750.00 ng/ml

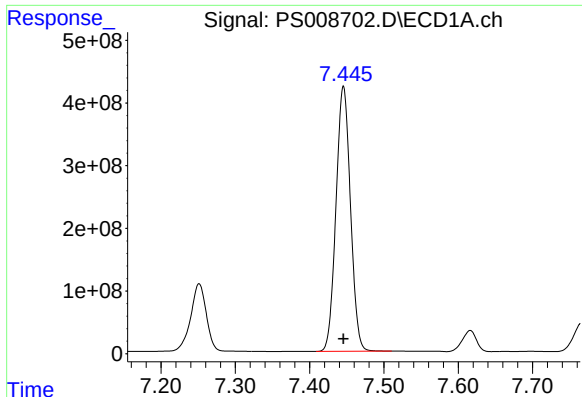

#5 DICAMBA


R.T.: 7.446 min
Delta R.T.: 0.000 min
Response: 5713045394
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

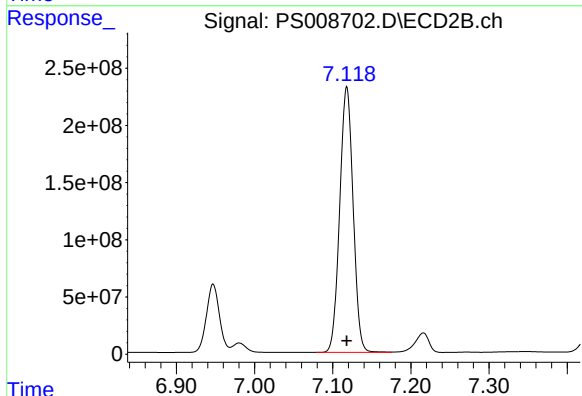


#5 DICAMBA

R.T.: 7.118 min
Delta R.T.: 0.000 min
Response: 2772998351
Conc: 705.00 ng/ml

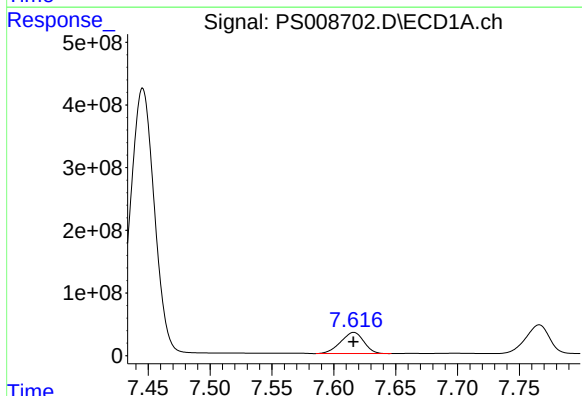


#6 MCP

R.T.: 7.616 min
Delta R.T.: 0.000 min
Response: 442249265
Conc: 70.50 ug/ml

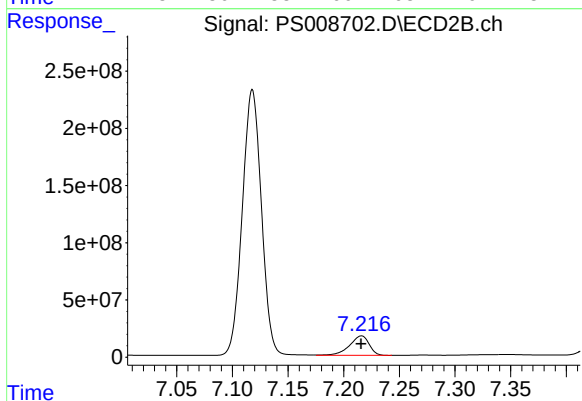

#6 MCP


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 211013321
Conc: 70.50 ug/ml

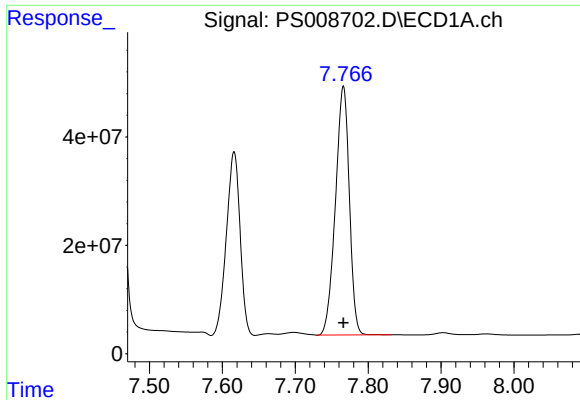

#7 MCPA


R.T.: 7.766 min
Delta R.T.: 0.000 min
Response: 608399304
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

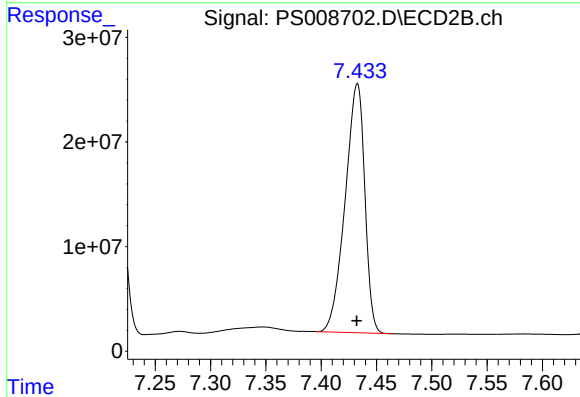


#7 MCPA

R.T.: 7.432 min
Delta R.T.: 0.000 min
Response: 293537689
Conc: 69.75 ug/ml

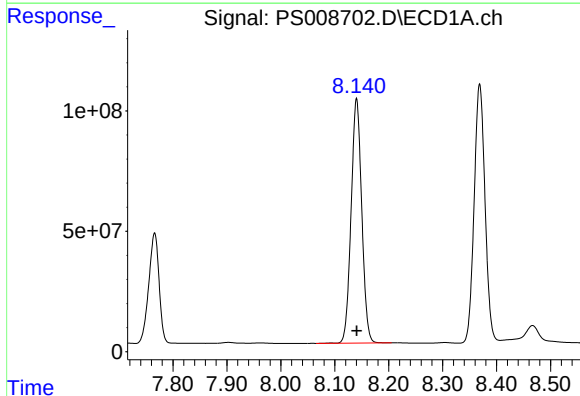


#8 DICHLORPROP

R.T.: 8.140 min
Delta R.T.: 0.000 min
Response: 1388952929
Conc: 705.00 ng/ml

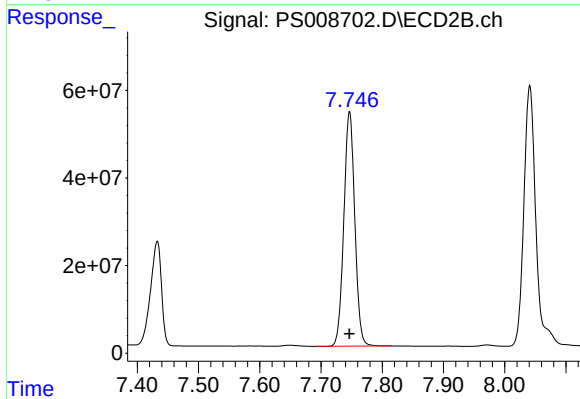

#8 DICHLORPROP


R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 665708918
Conc: 705.00 ng/ml

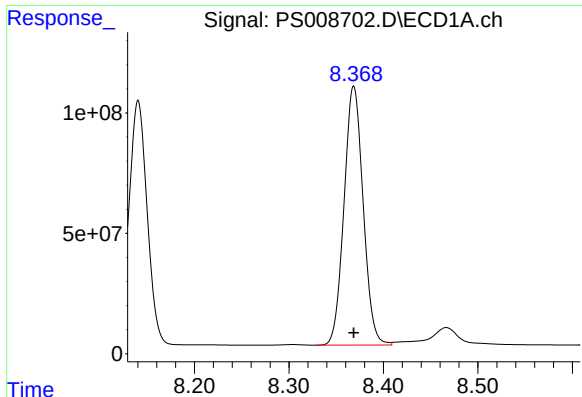

#9 2,4-D


R.T.: 8.369 min
Delta R.T.: 0.000 min
Response: 1514499366
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

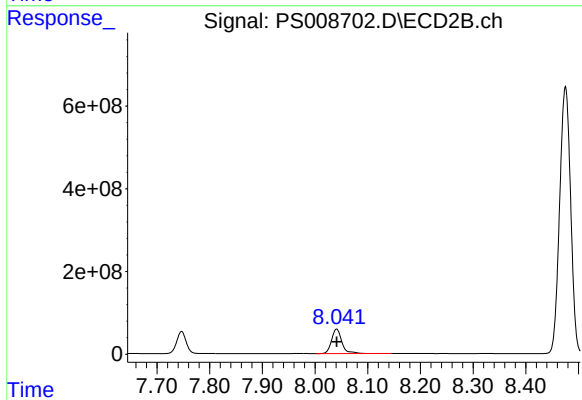


#9 2,4-D

R.T.: 8.041 min
Delta R.T.: 0.000 min
Response: 807037957
Conc: 705.00 ng/ml

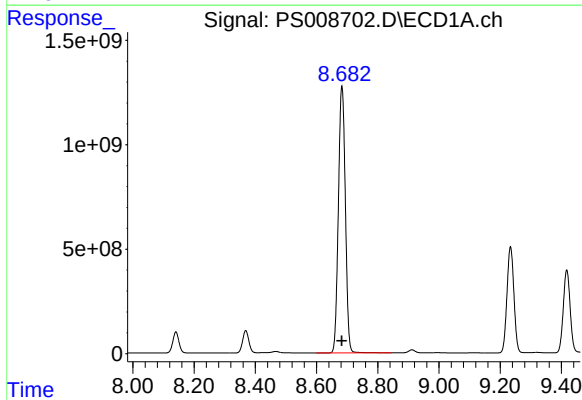


#10 Pentachlorophenol

R.T.: 8.683 min
Delta R.T.: 0.000 min
Response: 20136671152
Conc: 712.50 ng/ml

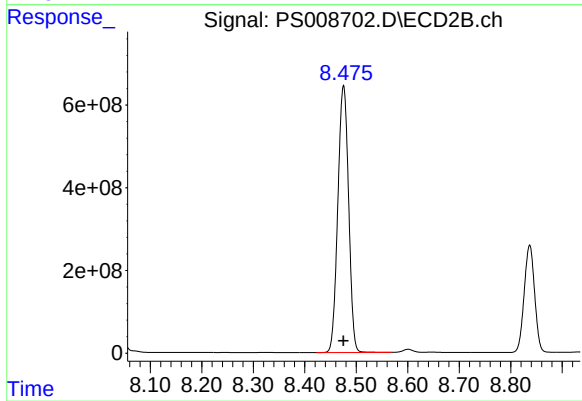

#10 Pentachlorophenol


R.T.: 8.475 min
Delta R.T.: 0.000 min
Response: 9372704784
Conc: 712.50 ng/ml

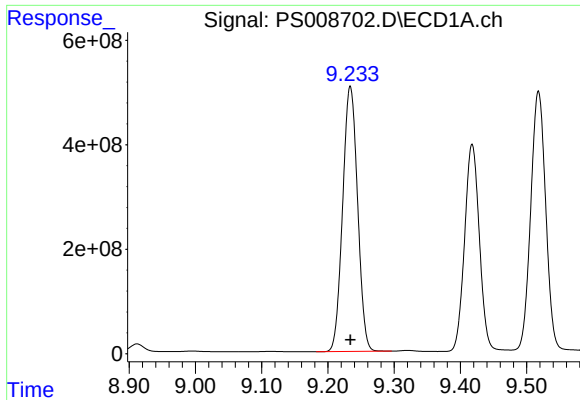

#11 2,4,5-TP (SILVEX)


R.T.: 9.234 min
Delta R.T.: 0.000 min
Response: 7942651208
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

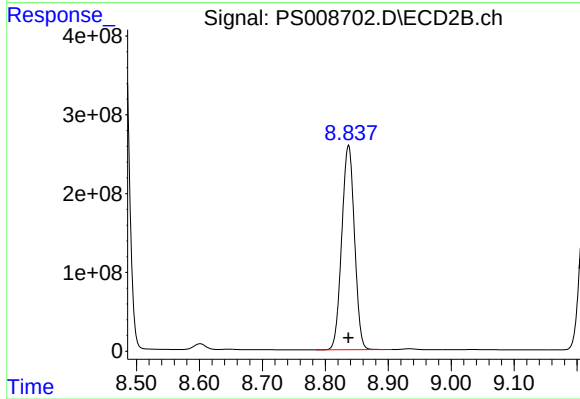


#11 2,4,5-TP (SILVEX)

R.T.: 8.837 min
Delta R.T.: 0.000 min
Response: 3642982348
Conc: 712.50 ng/ml

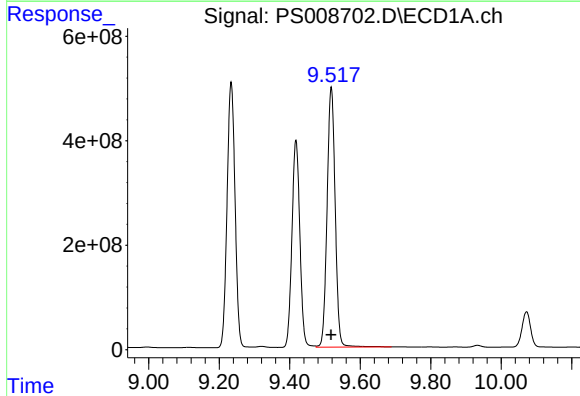


#12 2,4,5-T

R.T.: 9.518 min
Delta R.T.: 0.000 min
Response: 7931227860
Conc: 712.50 ng/ml

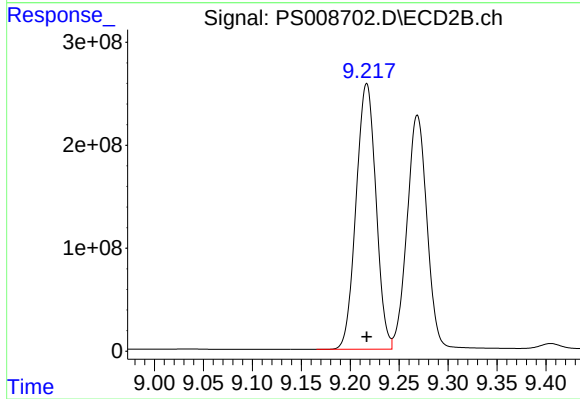

#12 2,4,5-T


R.T.: 9.217 min
Delta R.T.: 0.000 min
Response: 3641851885
Conc: 712.50 ng/ml

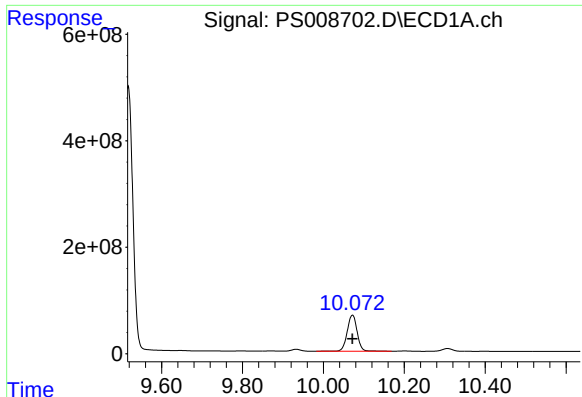

#13 2,4-DB


R.T.: 10.072 min
Delta R.T.: 0.000 min
Response: 1156646077
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

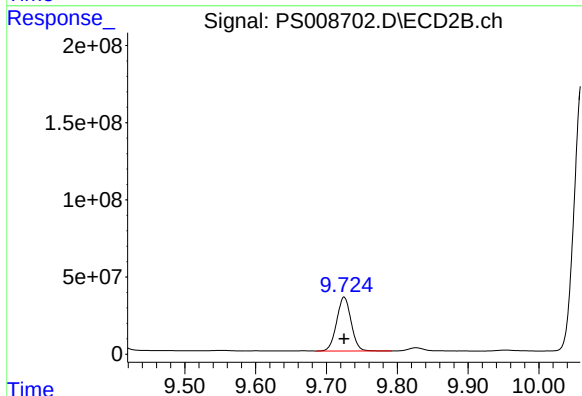


#13 2,4-DB

R.T.: 9.725 min
Delta R.T.: 0.000 min
Response: 493970938
Conc: 712.50 ng/ml

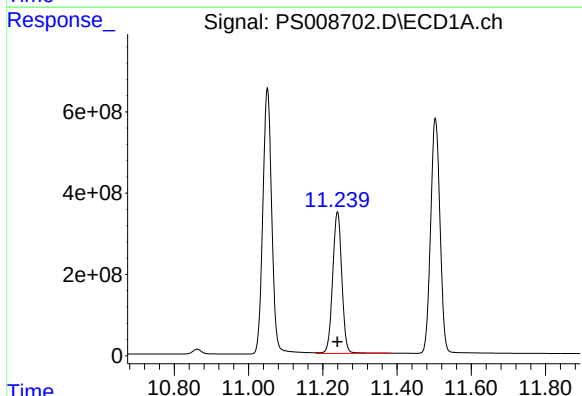


#14 DINOSEB

R.T.: 11.239 min
Delta R.T.: 0.000 min
Response: 5969065330
Conc: 705.00 ng/ml

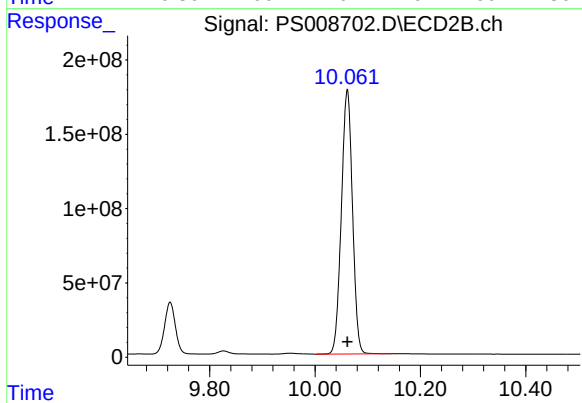

#14 DINOSEB


R.T.: 10.061 min
Delta R.T.: 0.000 min
Response: 2607598549
Conc: 705.00 ng/ml

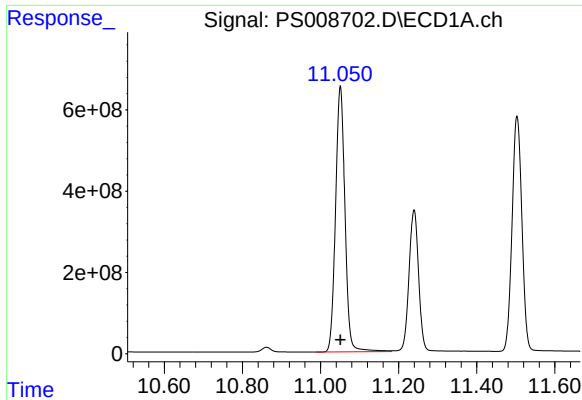

#15 Picloram


R.T.: 11.051 min
Delta R.T.: 0.000 min
Response: 10977328241
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

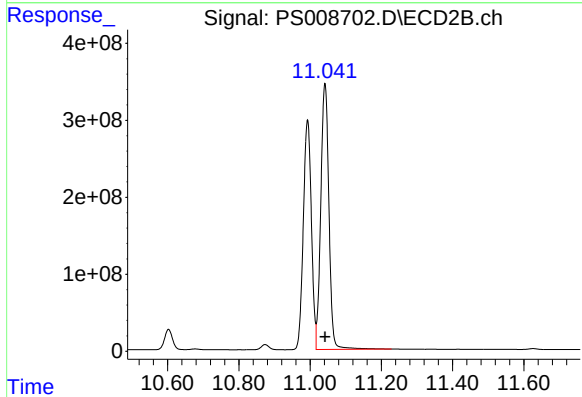


#15 Picloram

R.T.: 11.042 min
Delta R.T.: 0.000 min
Response: 5473512754
Conc: 712.50 ng/ml

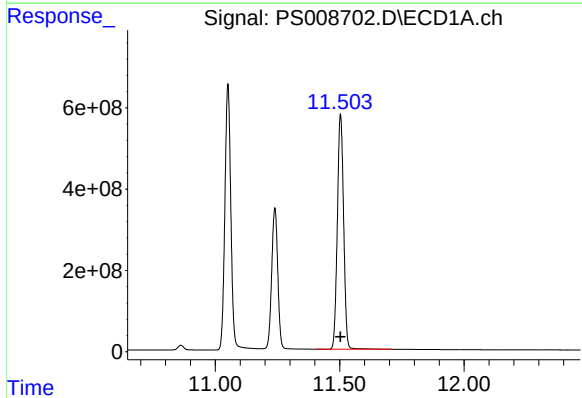

#16 DCPA

R.T.: 11.503 min
Delta R.T.: 0.000 min
Response: 10130175976
Conc: 720.00 ng/ml

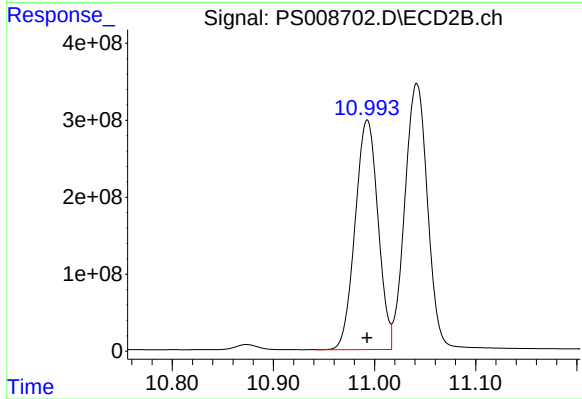

#16 DCPA

R.T.: 10.993 min
Delta R.T.: 0.000 min
Response: 4684487246
Conc: 720.00 ng/ml