

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020422\
 Data File : PS018244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 16:25
 Operator : AJ\MA
 Sample : N1357-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 21:37:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.044	6.651	658.9E6	282.0E6	455.836	486.008
Target Compounds							
1) T	Dalapon	2.861f	2.378f	77891782	11793230	31.751	15.422 #
2) T	3,5-DICHL...	6.253	5.890	362391	71044657	<MDL	80.310 #
3) T	4-Nitroph...	6.877	0.000	5942388	0	7.357	N.D. #
5) T	DICAMBA	7.212	0.000	4383018	0	<MDL	N.D. #
6) T	MCPD	7.391	0.000	12191949	0	2.611	N.D. #
7) T	MCPA	7.538	0.000	5168399	0	<MDL	N.D. #
8) T	DICHLORPROP	7.857f	7.443	5737564	20717900	3.647	31.042 #
9) T	2,4-D	8.198f	0.000	10773369	0	5.916	N.D. #
10) T	Pentachlo...	8.507f	0.000	17255596	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.047f	8.443	25155078	29958373	2.973	8.404 #
12) T	2,4,5-T	9.338f	0.000	24382422	0	2.751	N.D. #
13) T	2,4-DB	9.859	9.370	37427651	11257744	22.642	25.444
14) T	DINOSEB	10.936	9.676	211.4E6	18108449	32.184	7.258 #
15) T	Picloram	10.772	0.000	48840312	0	4.092	N.D. #
16) T	DCPA	11.168f	0.000	3281633	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020422\
Data File : PS018244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 16:25
Operator : AJ\MA
Sample : N1357-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 21:37:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

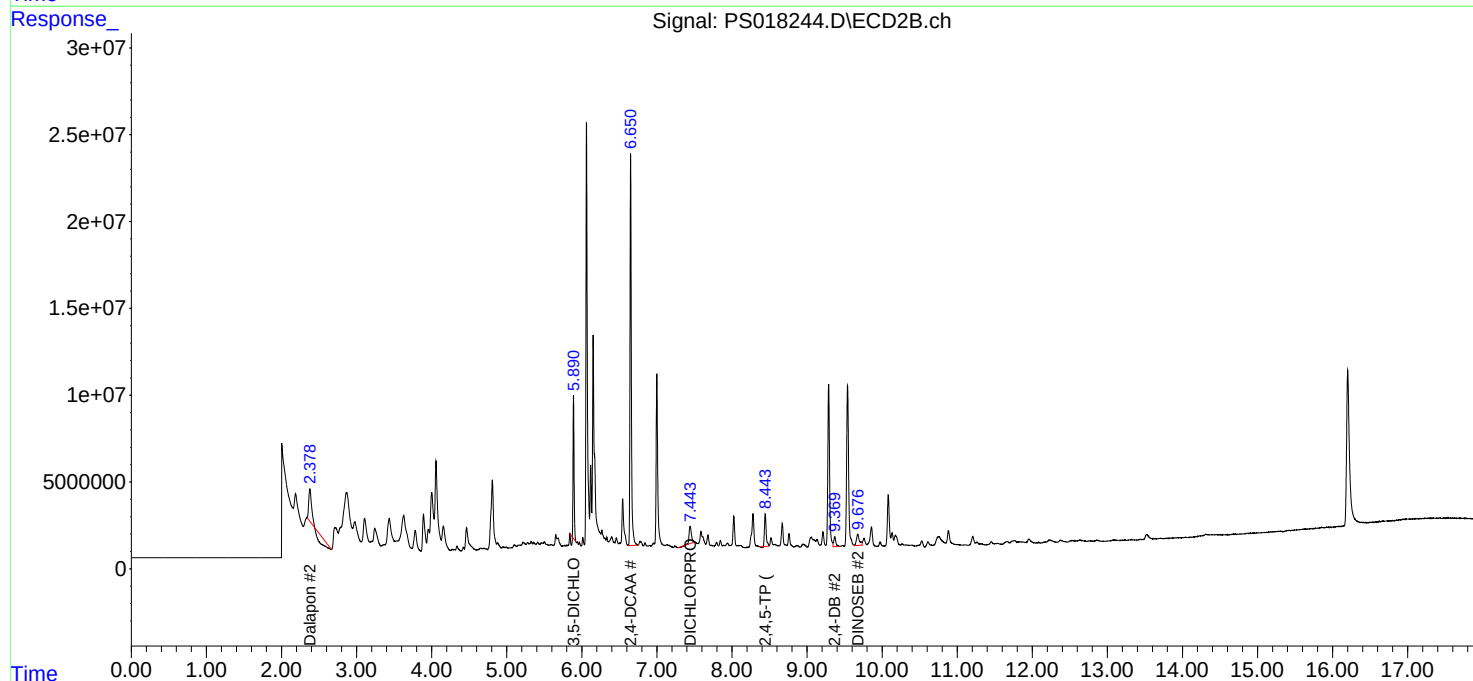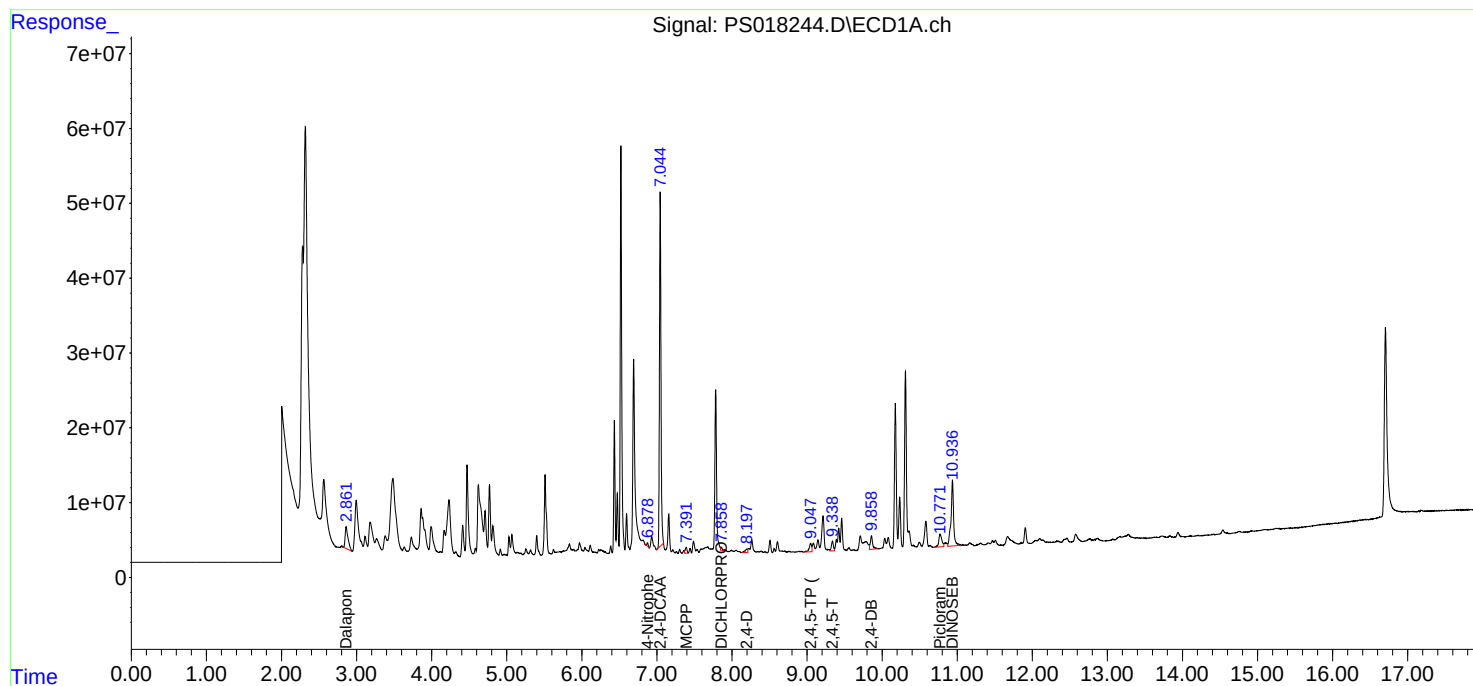


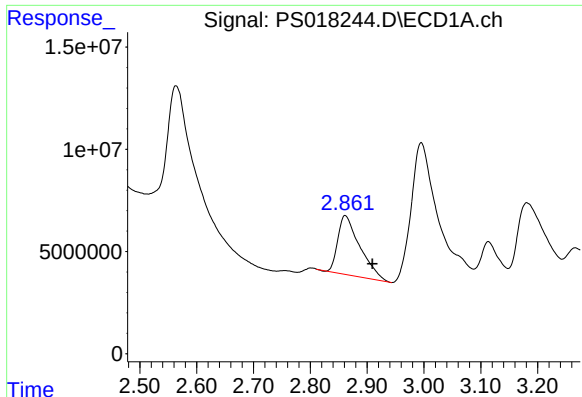

#1 Dalapon


R.T.: 2.861 min
Delta R.T.: -0.048 min
Response: 77891782
Conc: 31.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

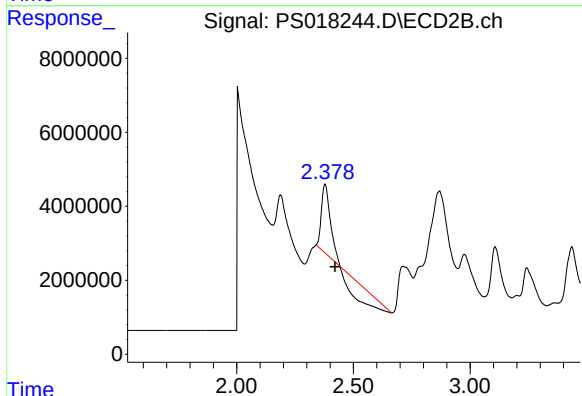


#1 Dalapon

R.T.: 2.378 min
Delta R.T.: -0.043 min
Response: 11793230
Conc: 15.42 ng/ml

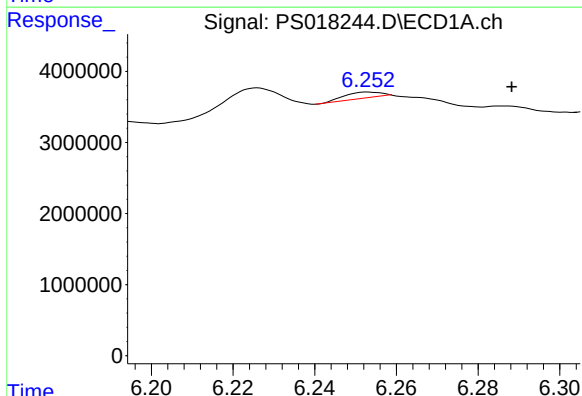


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.253 min
Delta R.T.: -0.035 min
Response: 362391
Conc: N.D.

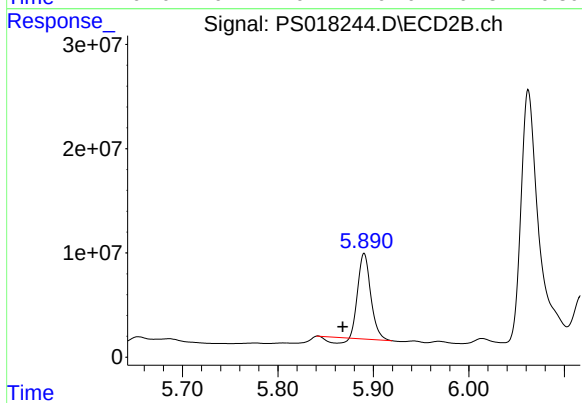

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.890 min
Delta R.T.: 0.022 min
Response: 71044657
Conc: 80.31 ng/ml

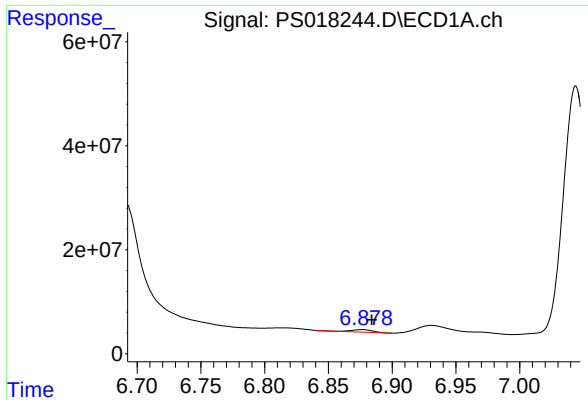

#3 4-Nitrophenol


R.T.: 6.877 min
Delta R.T.: -0.007 min
Response: 5942388
Conc: 7.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

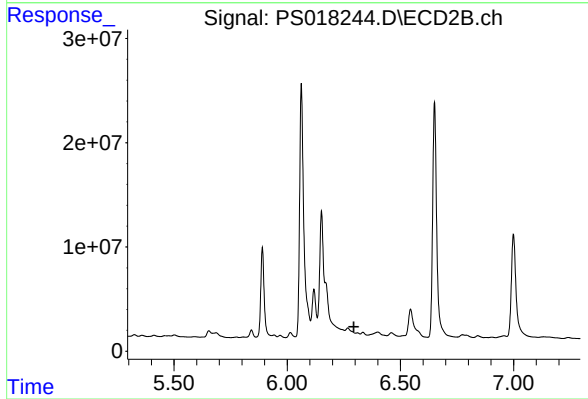


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.295 min
Response: 0
Conc: N.D.

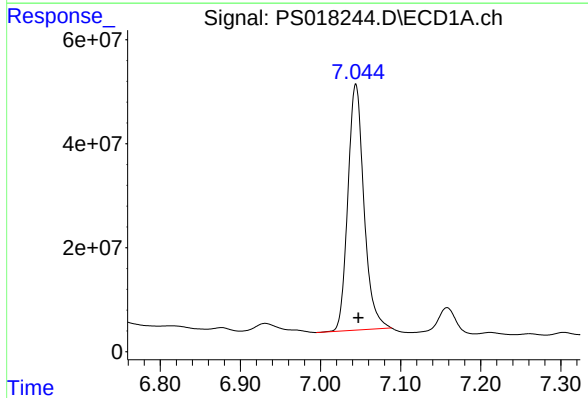


#4 2,4-DCAA

R.T.: 7.044 min
Delta R.T.: -0.003 min
Response: 658904632
Conc: 455.84 ng/ml

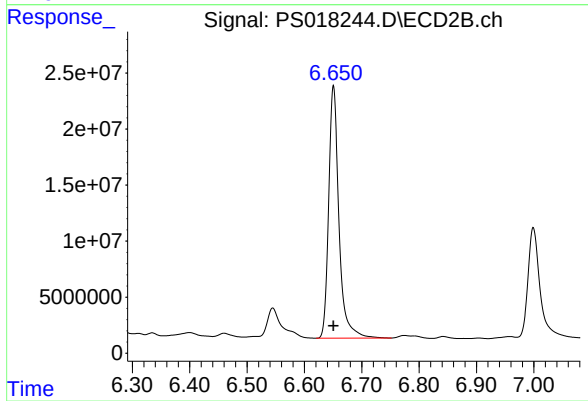

#4 2,4-DCAA


R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 282005324
Conc: 486.01 ng/ml

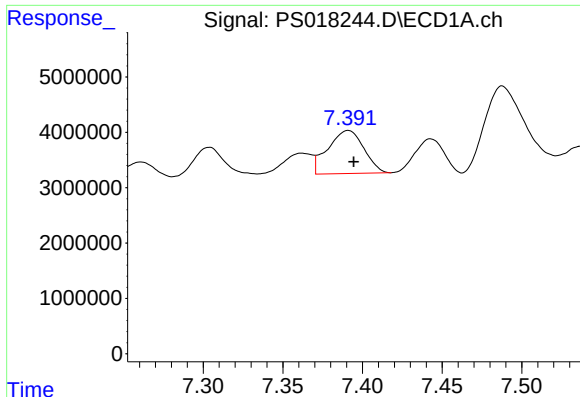

#6 MCP


R.T.: 7.391 min
Delta R.T.: -0.003 min
Response: 12191949
Conc: 2.61 ug/ml

Instrument :
ECD_S
ClientSampleId :

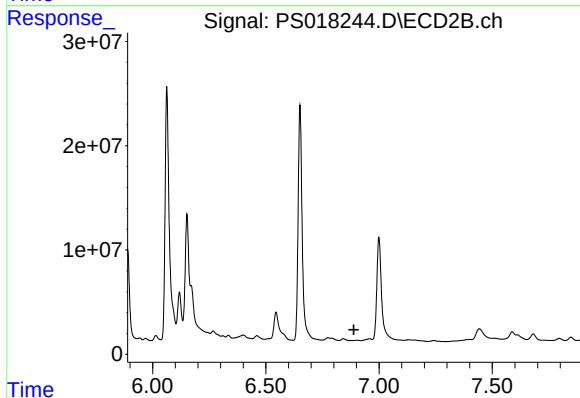


#6 MCP

R.T.: 0.000 min
Exp R.T. : 6.888 min
Response: 0
Conc: N.D.

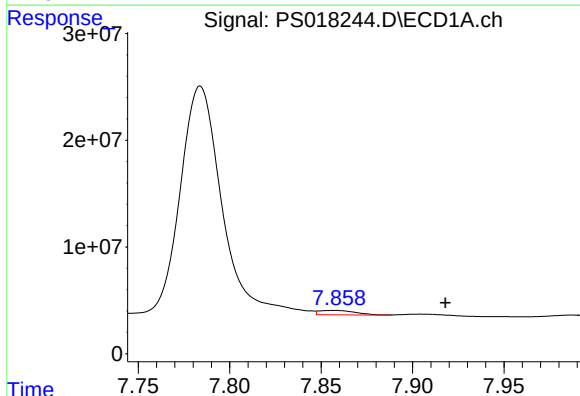


#8 DICHLORPROP

R.T.: 7.857 min
Delta R.T.: -0.061 min
Response: 5737564
Conc: 3.65 ng/ml

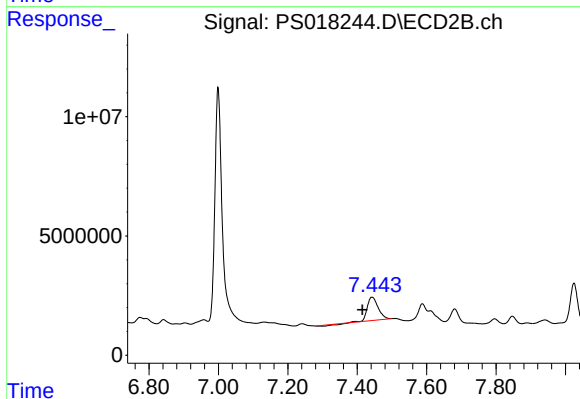

#8 DICHLORPROP


R.T.: 7.443 min
Delta R.T.: 0.027 min
Response: 20717900
Conc: 31.04 ng/ml

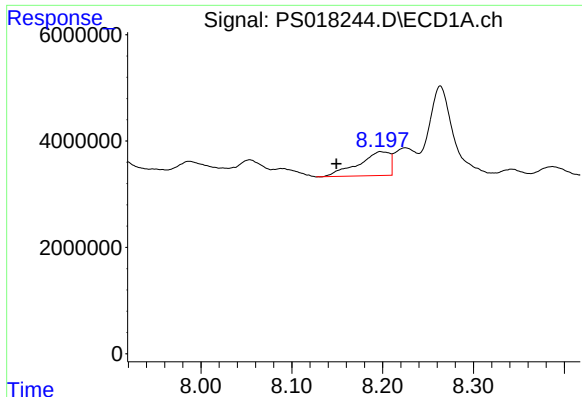

#9 2,4-D


R.T.: 8.198 min
Delta R.T.: 0.048 min
Response: 10773369
Conc: 5.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

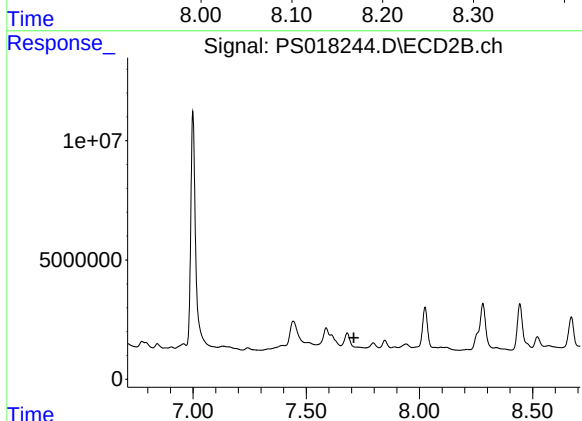


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

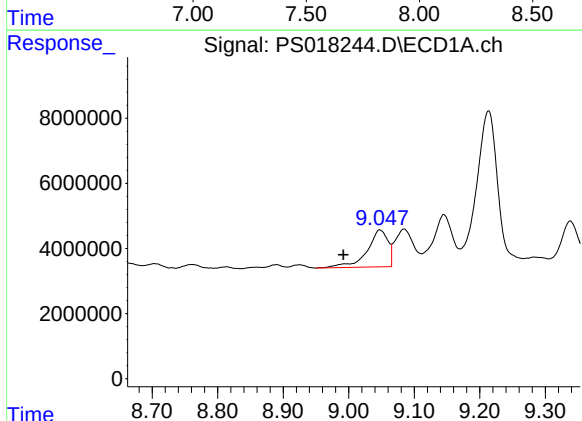


#11 2,4,5-TP (SILVEX)

R.T.: 9.047 min
Delta R.T.: 0.055 min
Response: 25155078
Conc: 2.97 ng/ml

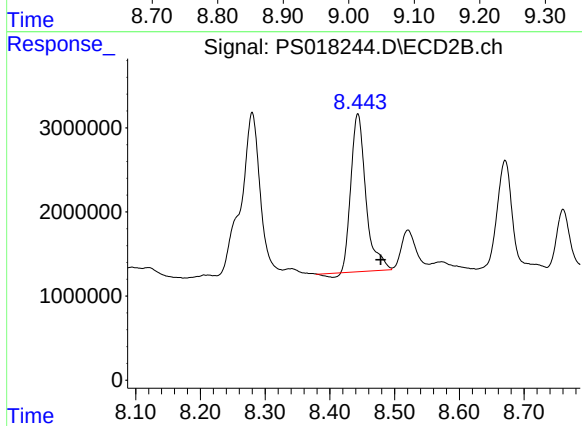

#11 2,4,5-TP (SILVEX)


R.T.: 8.443 min
Delta R.T.: -0.035 min
Response: 29958373
Conc: 8.40 ng/ml

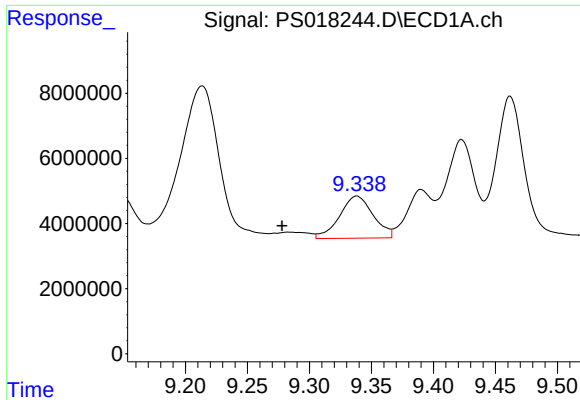

#12 2,4,5-T


R.T.: 9.338 min
Delta R.T.: 0.060 min
Response: 24382422
Conc: 2.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

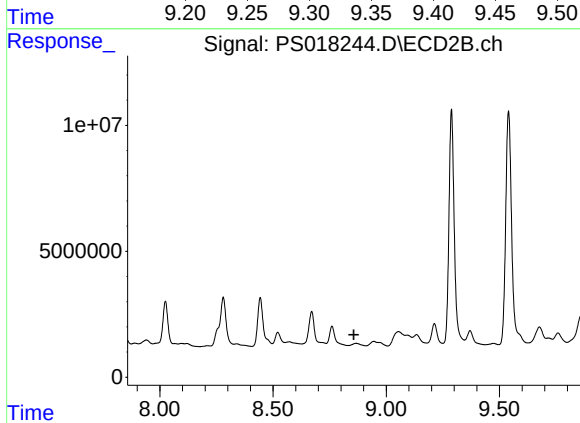


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.857 min
Response: 0
Conc: N.D.

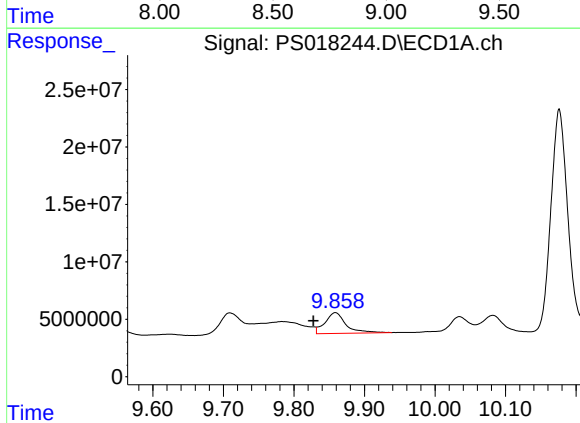


#13 2,4-DB

R.T.: 9.859 min
Delta R.T.: 0.031 min
Response: 37427651
Conc: 22.64 ng/ml

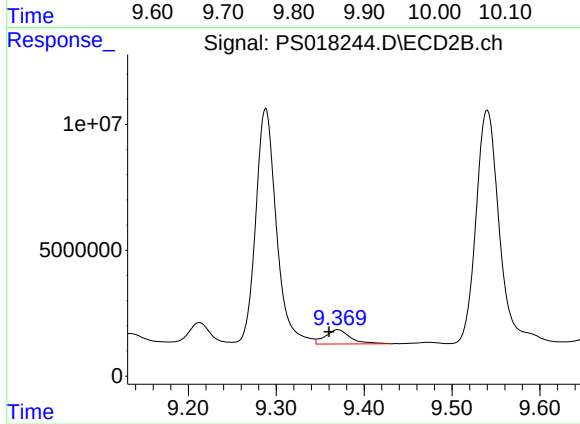

#13 2,4-DB


R.T.: 9.370 min
Delta R.T.: 0.010 min
Response: 11257744
Conc: 25.44 ng/ml

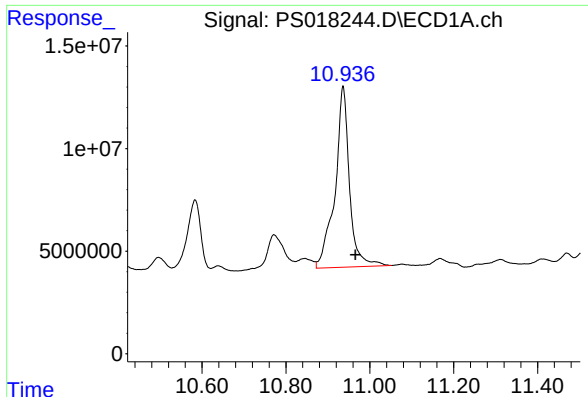

#14 DINOSEB


R.T.: 10.936 min
Delta R.T.: -0.029 min
Response: 211353122
Conc: 32.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

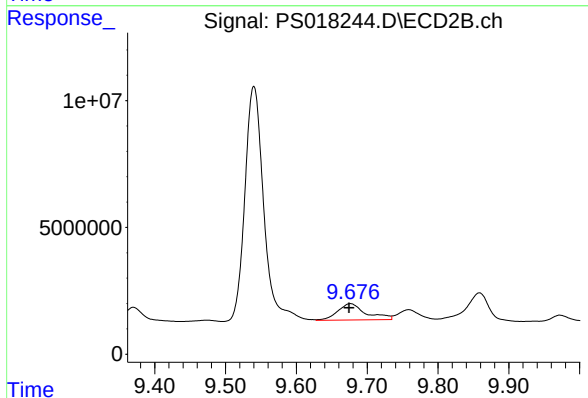


#14 DINOSEB

R.T.: 9.676 min
Delta R.T.: 0.002 min
Response: 18108449
Conc: 7.26 ng/ml

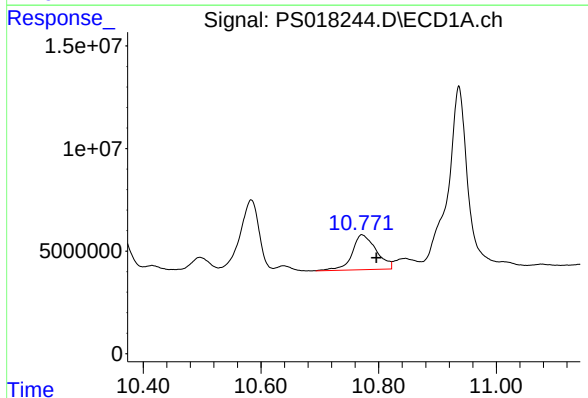

#15 Picloram

R.T.: 10.772 min
Delta R.T.: -0.024 min
Response: 48840312
Conc: 4.09 ng/ml

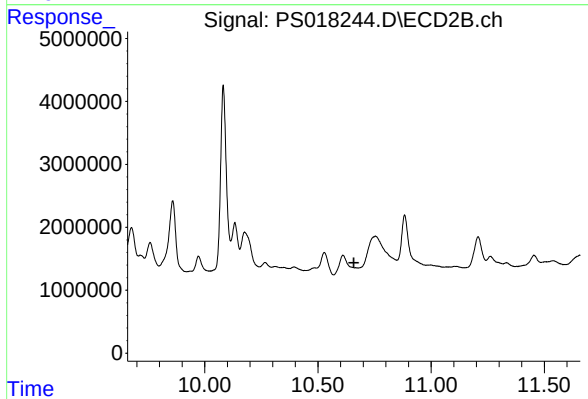

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.659 min
Response: 0
Conc: N.D.