

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
 Data File : PS003020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2019 11:53
 Operator : EI\SJ
 Sample : K1299-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 0034-FIELD-BLANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 13:25:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.284	10.783	191.5E6	223.9E6	504.340	523.653
Target Compounds							
1) T	Dalapon	0.000	2.287	0	54486279	N.D.	101.668 #
2) T	3,5-DICHL...	0.000	9.033	0	2137180	N.D.	3.792 #
6) T	MCPD	11.954	11.346	14781250	2228940	12.337	2.021 #
7) T	MCPA	12.241	0.000	2701145	0	1.526	N.D. #
10) T	Pentachlo...	13.512	13.196	3652027	1968482	0.569	0.318 #
14) T	DINOSEB	0.000	15.513	0	9199124	N.D.	5.248 #
15) T	Picloram	0.000	16.706	0	16124306	N.D.	5.363 #
16) T	DCPA	0.000	16.706	0	16124306	N.D.	5.205 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
Data File : PS003020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2019 11:53
Operator : EI\SJ
Sample : K1299-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
0034-FIELD-BLANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 13:25:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

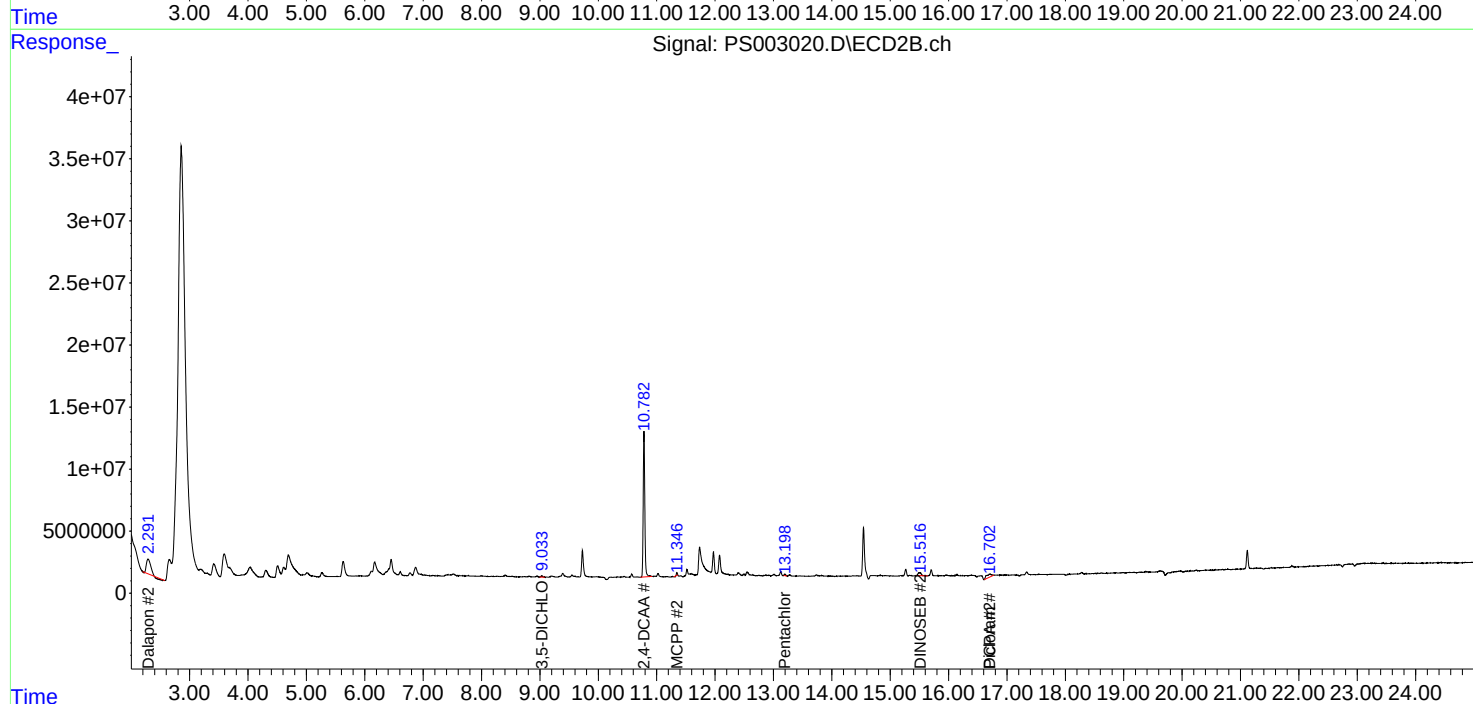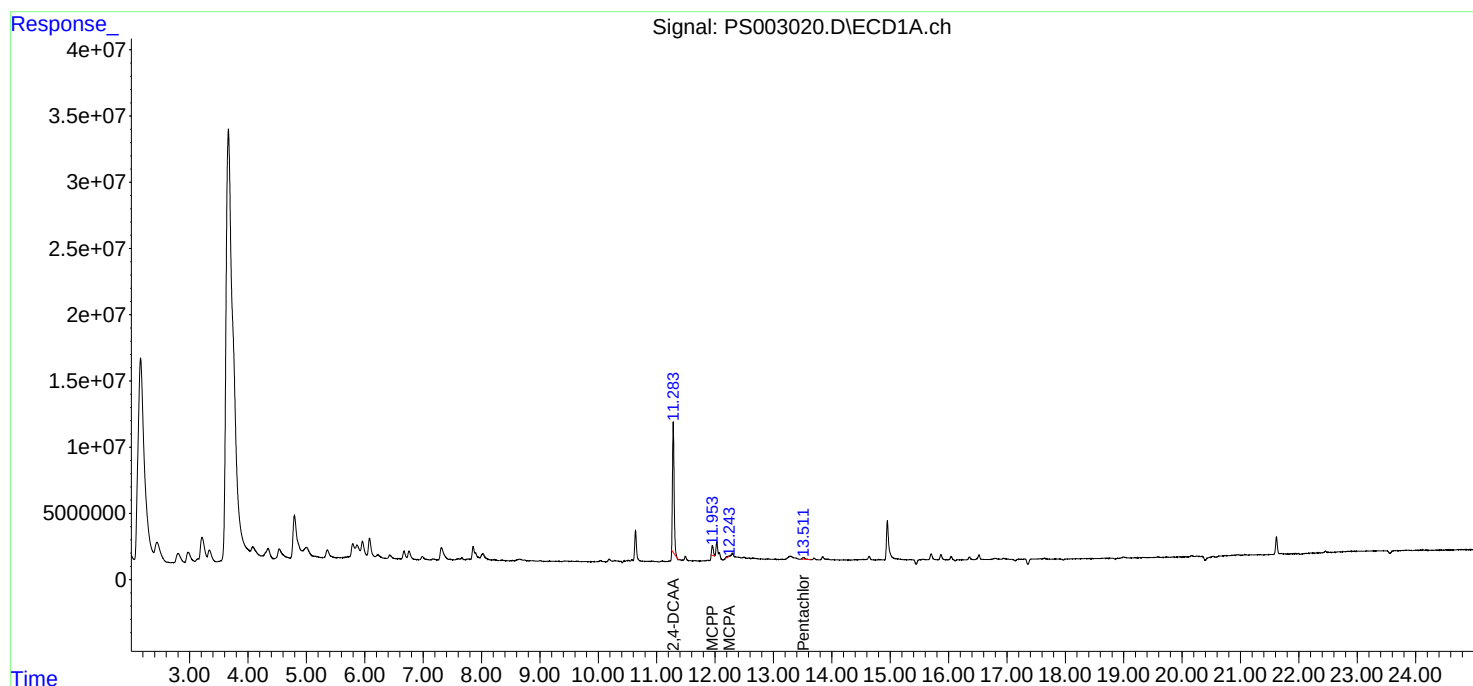


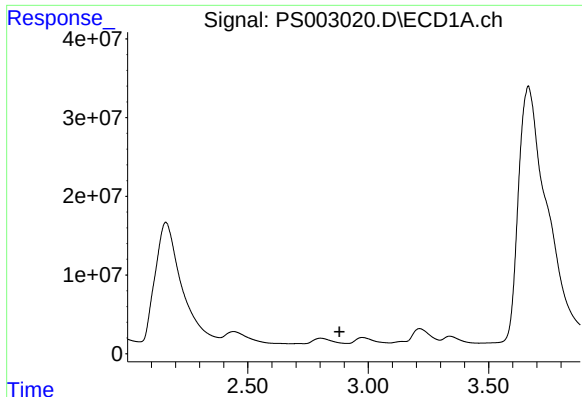

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
0034-FIELD-BLANK

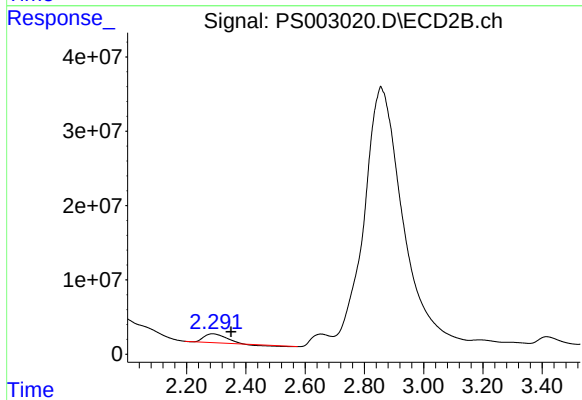


#1 Dalapon

R.T.: 2.287 min
Delta R.T.: -0.064 min
Response: 54486279
Conc: 101.67 ng/ml

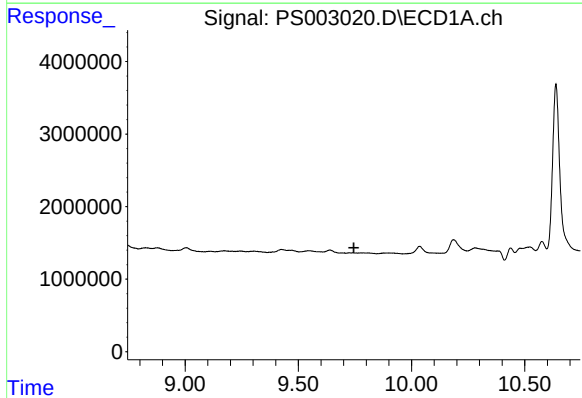


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

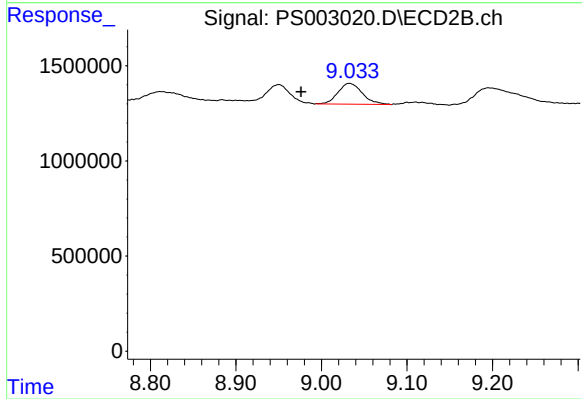

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.033 min
Delta R.T.: 0.057 min
Response: 2137180
Conc: 3.79 ng/ml

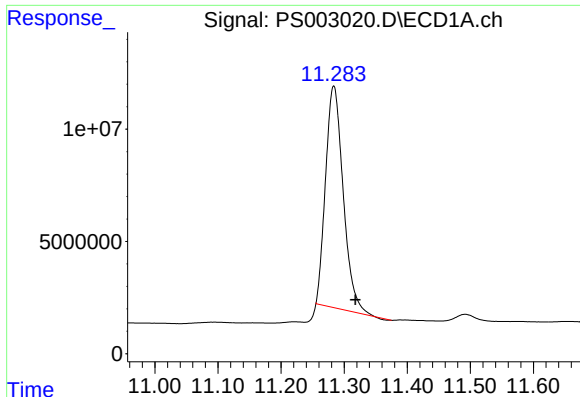

#4 2,4-DCAA


R.T.: 11.284 min
Delta R.T.: -0.034 min
Response: 191468146
Conc: 504.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
0034-FIELD-BLANK

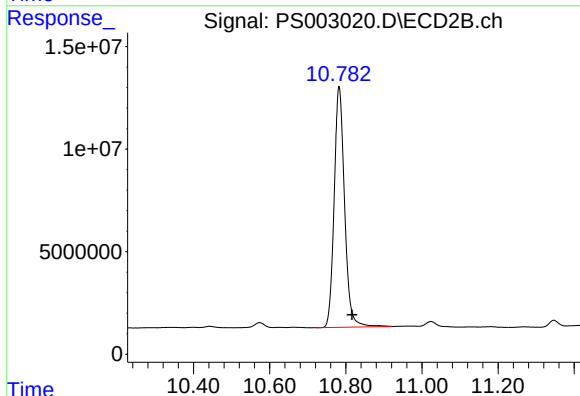


#4 2,4-DCAA

R.T.: 10.783 min
Delta R.T.: -0.034 min
Response: 223885693
Conc: 523.65 ng/ml

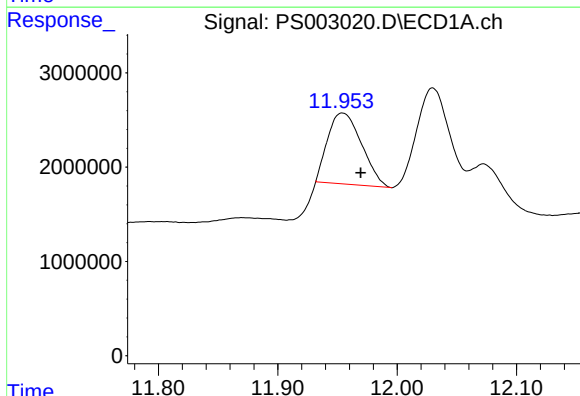


#6 MCP

R.T.: 11.954 min
Delta R.T.: -0.015 min
Response: 14781250
Conc: 12.34 ug/ml

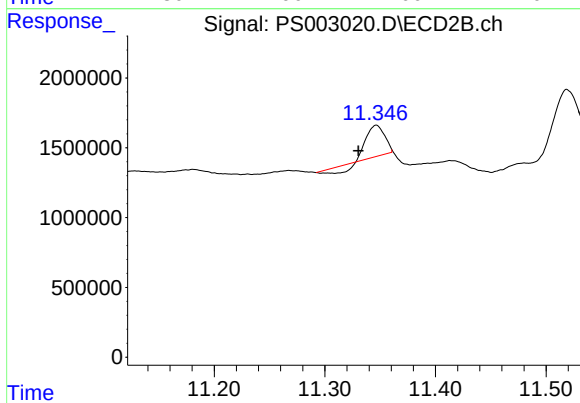

#6 MCP


R.T.: 11.346 min
Delta R.T.: 0.016 min
Response: 2228940
Conc: 2.02 ug/ml

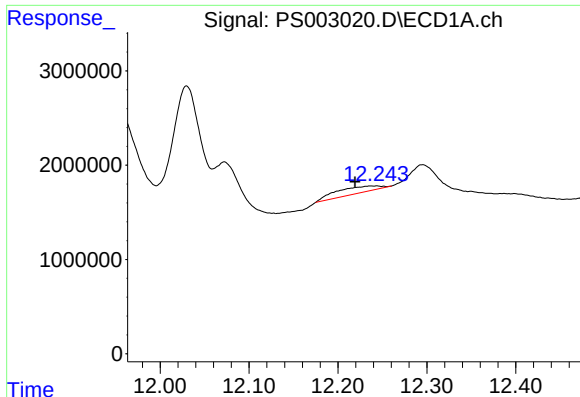

#7 MCPA


R.T.: 12.241 min
Delta R.T.: 0.022 min
Response: 2701145
Conc: 1.53 ug/ml

Instrument :
ECD_S
ClientSampleId :
0034-FIELD-BLANK

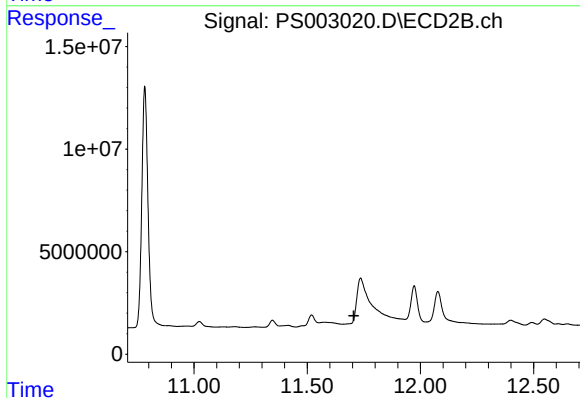


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

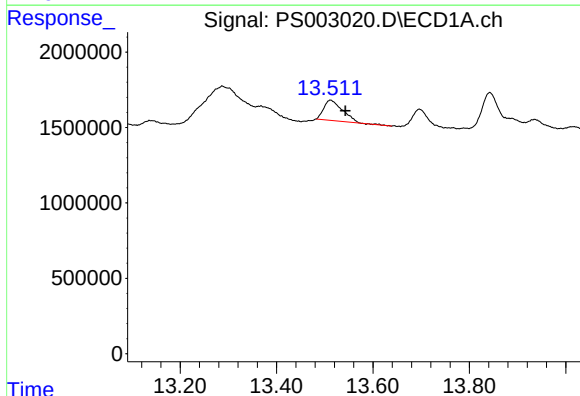


#10 Pentachlorophenol

R.T.: 13.512 min
Delta R.T.: -0.031 min
Response: 3652027
Conc: 0.57 ng/ml

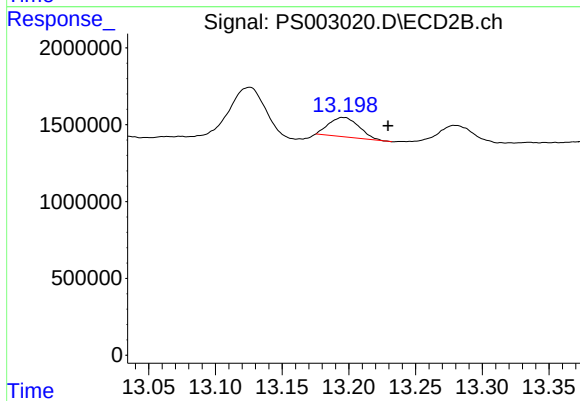

#10 Pentachlorophenol


R.T.: 13.196 min
Delta R.T.: -0.034 min
Response: 1968482
Conc: 0.32 ng/ml

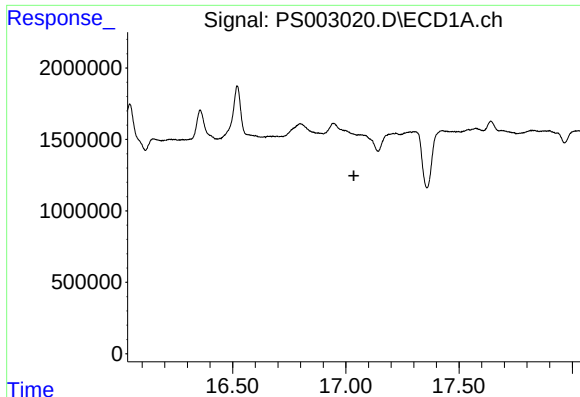

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
0034-FIELD-BLANK

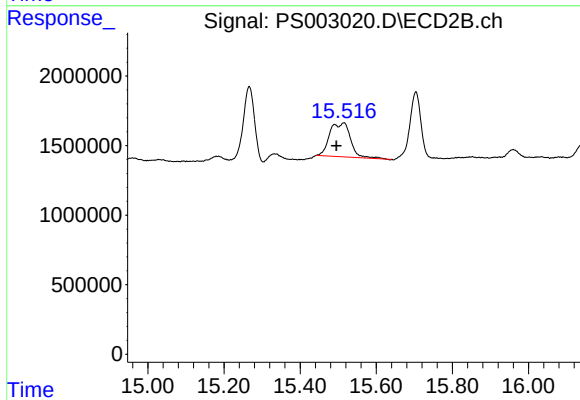


#14 DINOSEB

R.T.: 15.513 min
Delta R.T.: 0.018 min
Response: 9199124
Conc: 5.25 ng/ml

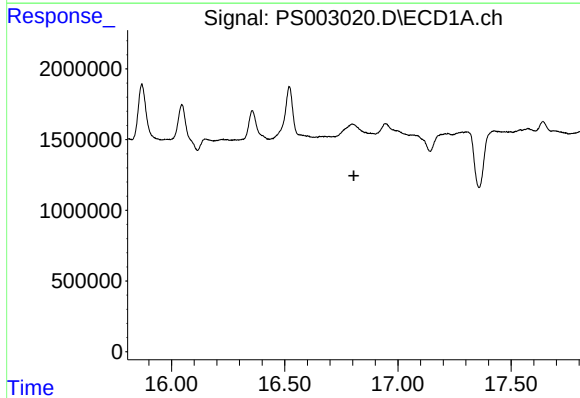


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

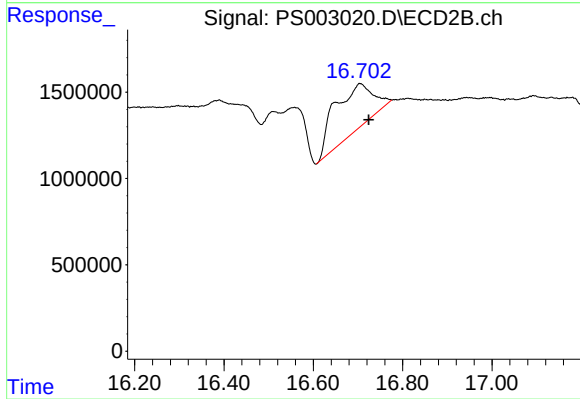

#15 Picloram


R.T.: 16.706 min
Delta R.T.: -0.019 min
Response: 16124306
Conc: 5.36 ng/ml

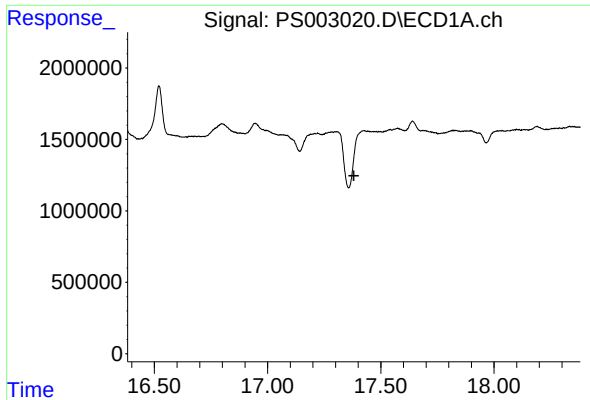

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
0034-FIELD-BLANK

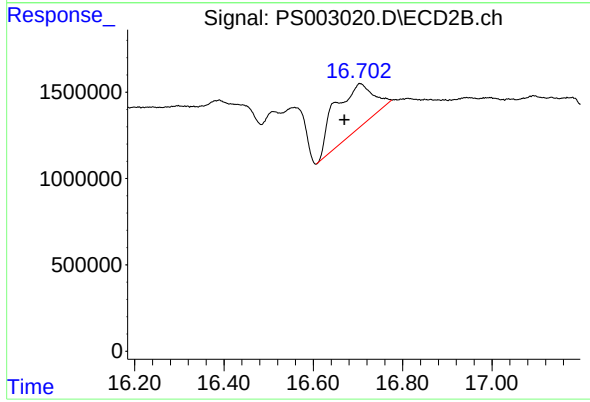

#16 DCPA

R.T.: 16.706 min
Delta R.T.: 0.036 min
Response: 16124306
Conc: 5.21 ng/ml