

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
 Data File : PS003021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2019 12:24
 Operator : EI\SJ
 Sample : PB116790BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116790BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 13:25:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.298	10.781	214.8E6	215.8E6	565.763	504.808
Target Compounds							
1) T	Dalapon	0.000	2.285	0 46986772		N.D.	87.675 #
6) T	MCP	11.971	11.346	15927076	1593773	13.293	1.445 #
14) T	DINOSEB	0.000	15.509	0 8226817		N.D.	4.693 #
15) T	Picloram	0.000	16.707	0 15351454		N.D.	5.106 #
16) T	DCPA	0.000	16.707	0 15351454		N.D.	4.956 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
Data File : PS003021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2019 12:24
Operator : EI\SJ
Sample : PB116790BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB116790BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 13:25:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

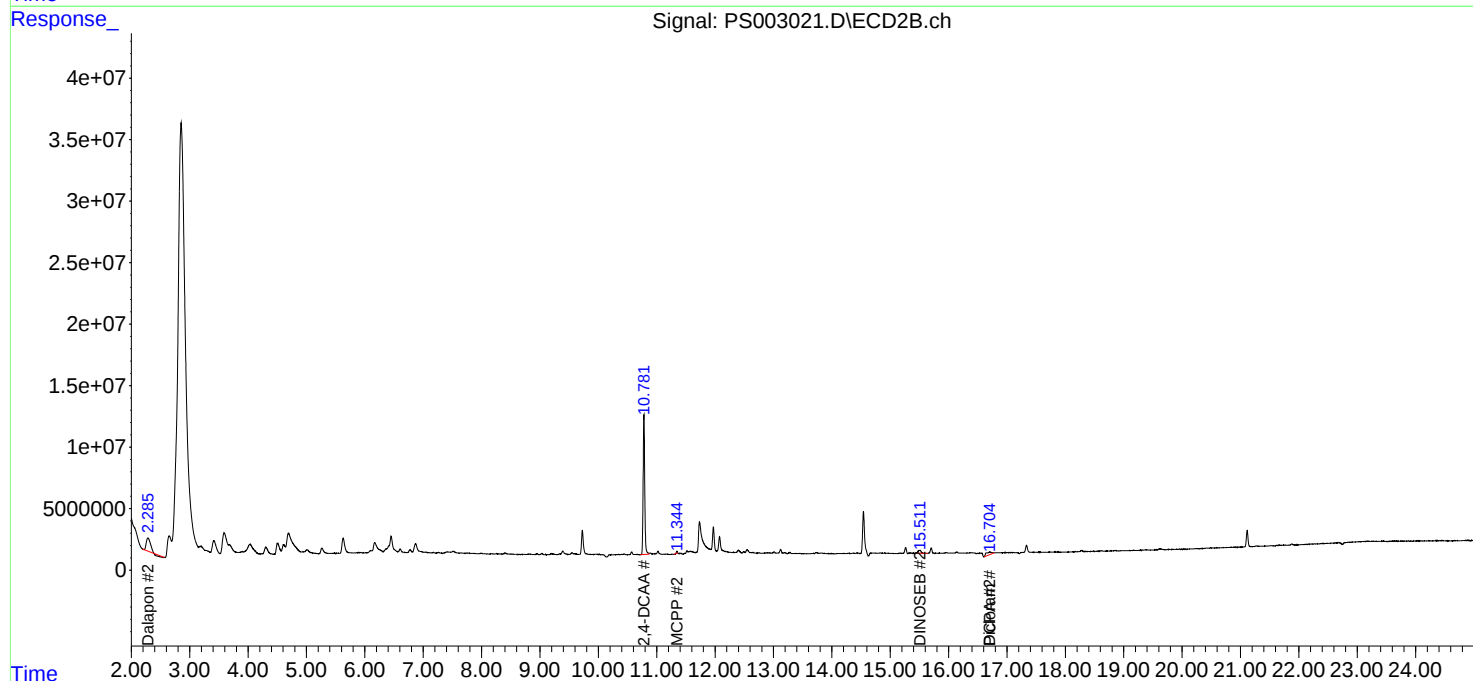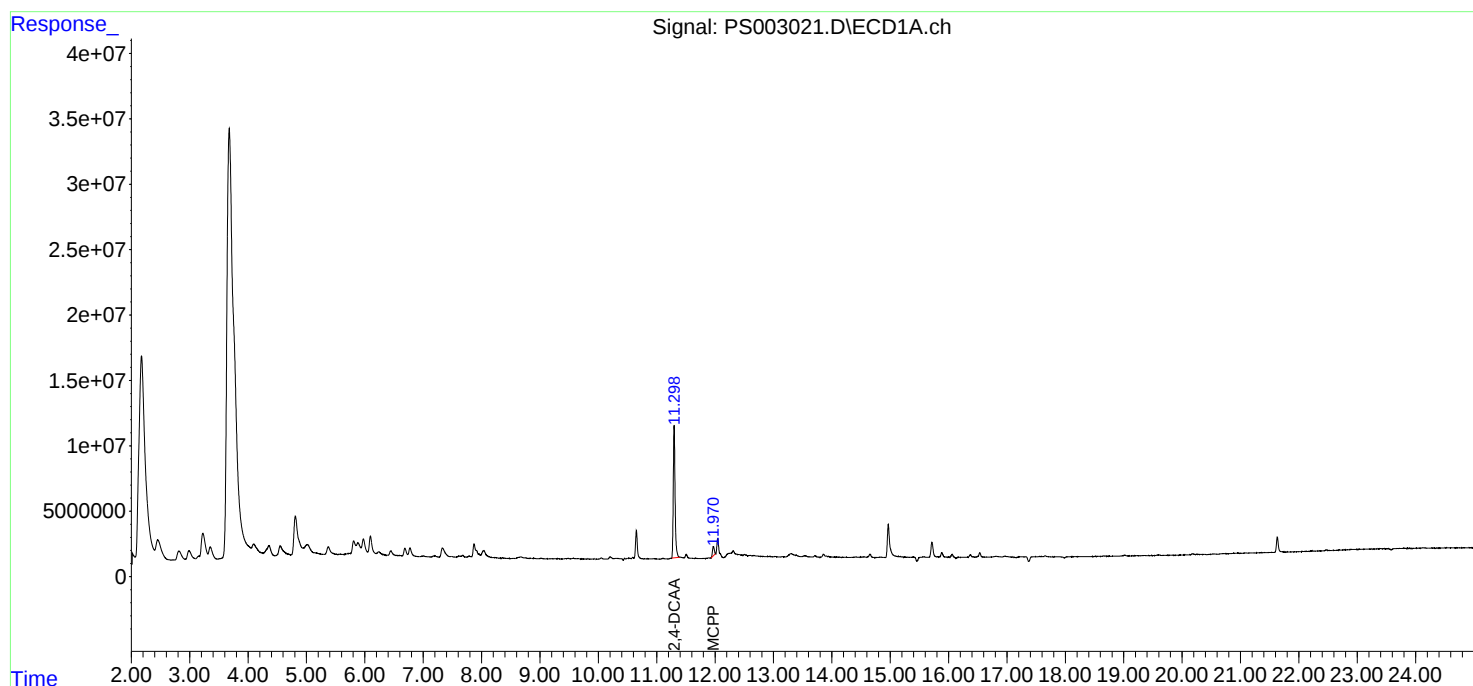


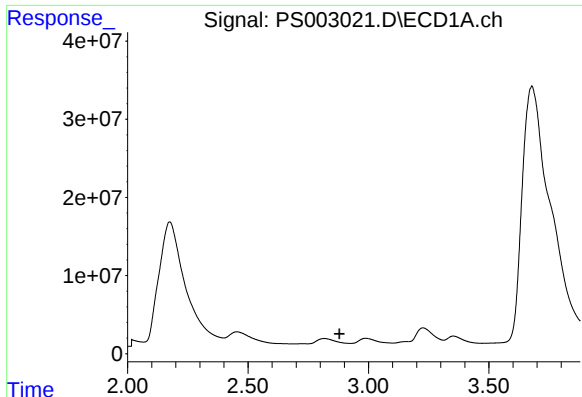

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116790BL

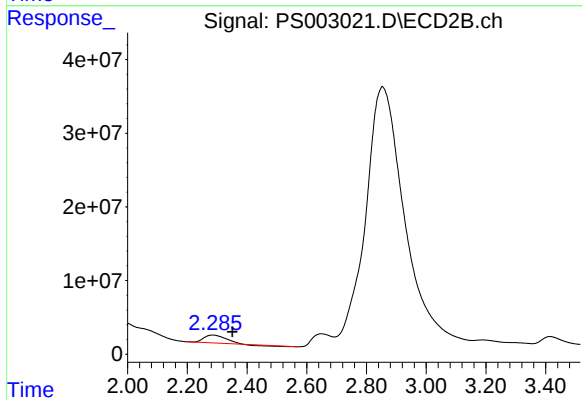


#1 Dalapon

R.T.: 2.285 min
Delta R.T.: -0.066 min
Response: 46986772
Conc: 87.67 ng/ml

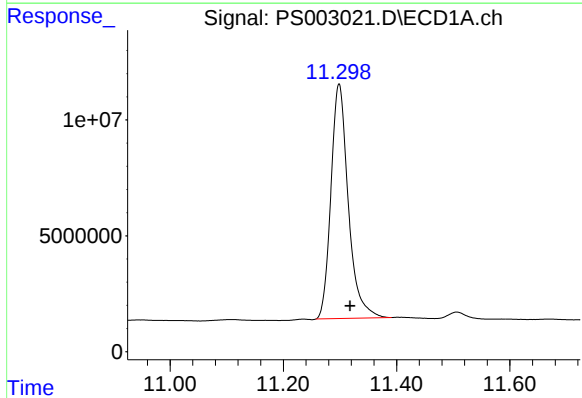


#4 2,4-DCAA

R.T.: 11.298 min
Delta R.T.: -0.019 min
Response: 214786726
Conc: 565.76 ng/ml

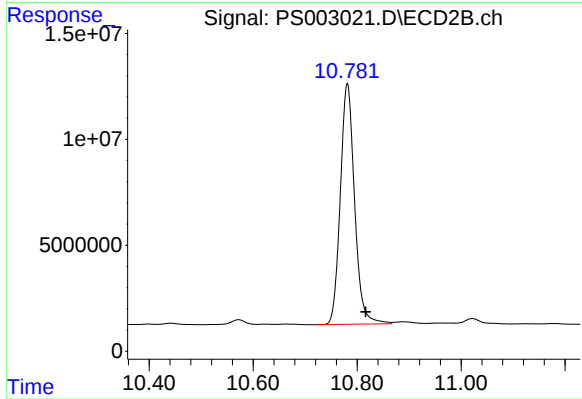

#4 2,4-DCAA


R.T.: 10.781 min
Delta R.T.: -0.035 min
Response: 215828595
Conc: 504.81 ng/ml

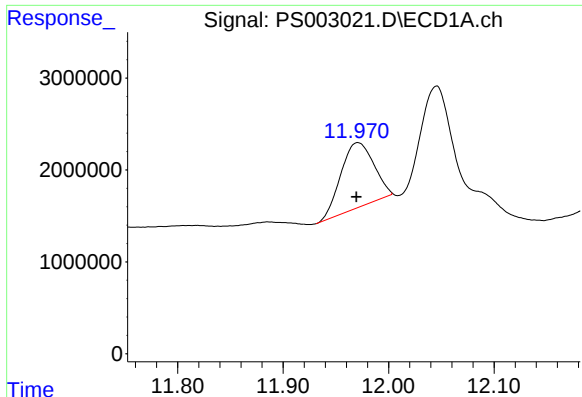

#6 MCP


R.T.: 11.971 min
Delta R.T.: 0.002 min
Response: 15927076
Conc: 13.29 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB116790BL

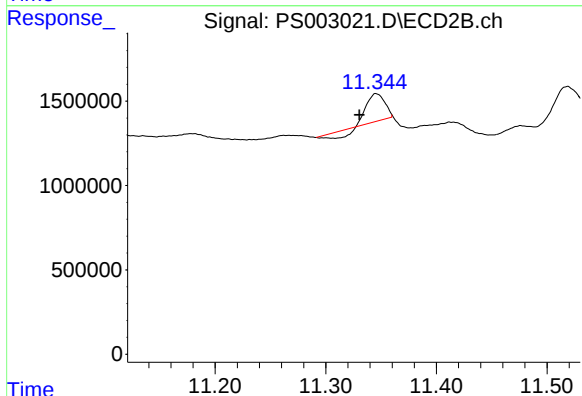


#6 MCP

R.T.: 11.346 min
Delta R.T.: 0.016 min
Response: 1593773
Conc: 1.45 ug/ml

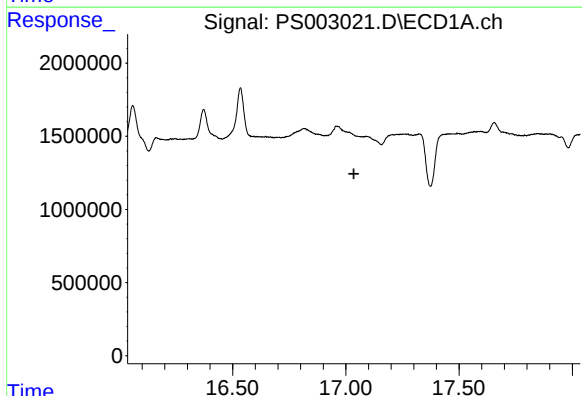


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

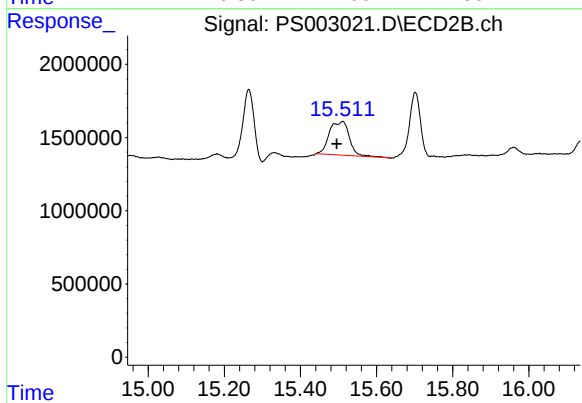

#14 DINOSEB


R.T.: 15.509 min
Delta R.T.: 0.014 min
Response: 8226817
Conc: 4.69 ng/ml

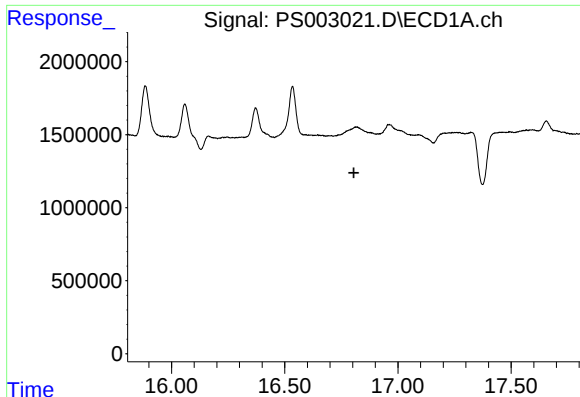

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116790BL

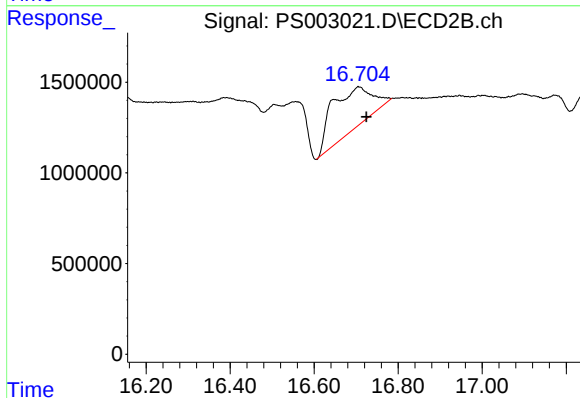


#15 Picloram

R.T.: 16.707 min
Delta R.T.: -0.018 min
Response: 15351454
Conc: 5.11 ng/ml

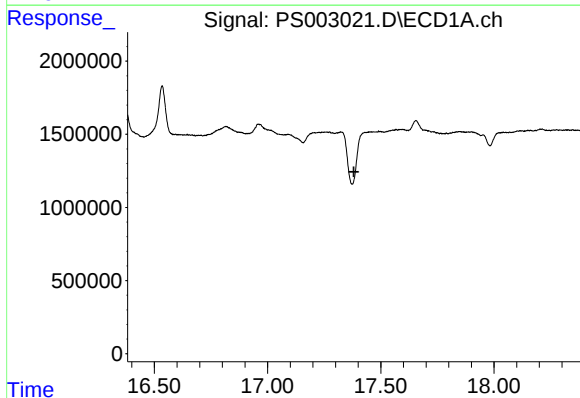

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

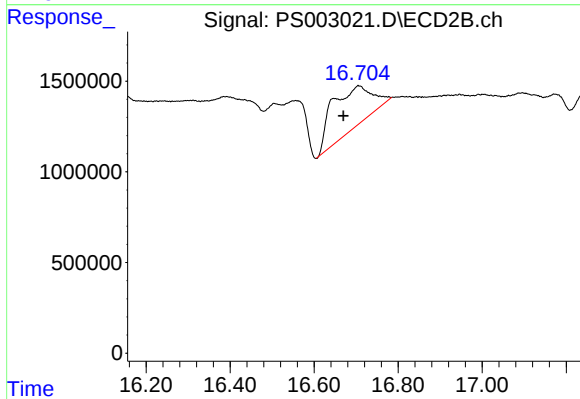

#16 DCPA

R.T.: 16.707 min
Delta R.T.: 0.037 min
Response: 15351454
Conc: 4.96 ng/ml