

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
 Data File : PS003027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2019 15:30
 Operator : EI\SJ
 Sample : PB116800TB
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116800TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:13:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.302	10.800	91767294	94293201	241.721	220.545
Target Compounds							
1) T	Dalapon	0.000	2.304	0	104.9E6	N.D.	195.755 #
2) T	3,5-DICHL...	0.000	8.966	0	9434103	N.D.	16.740 #
6) T	MCP	11.972	0.000	20058946	0	16.742	N.D. #
14) T	DINOSEB	0.000	15.504	0	5900017	N.D.	3.366 #
15) T	Picloram	0.000	16.724	0	7601703	N.D.	2.529 #
16) T	DCPA	0.000	16.665	0	3704040	N.D.	1.196 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
Data File : PS003027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2019 15:30
Operator : EI\SJ
Sample : PB116800TB
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB116800TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:13:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

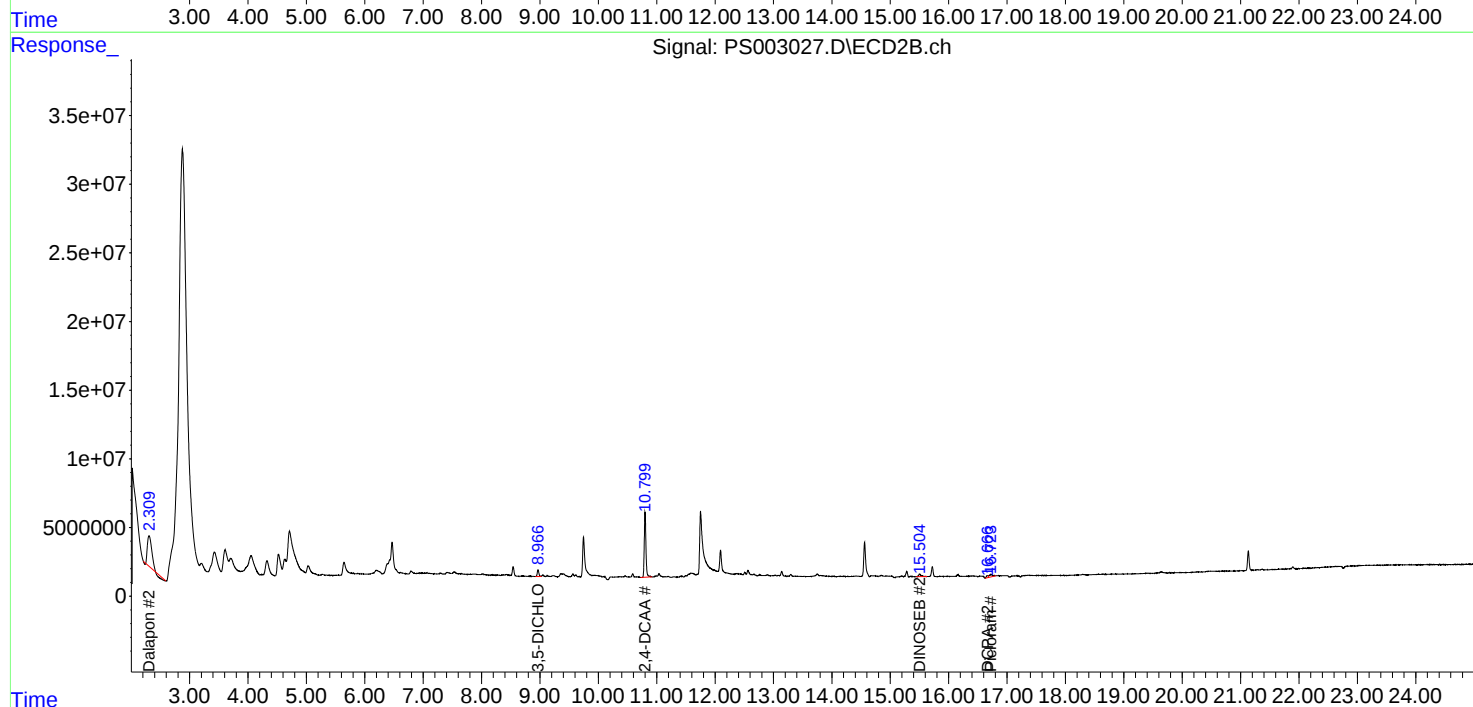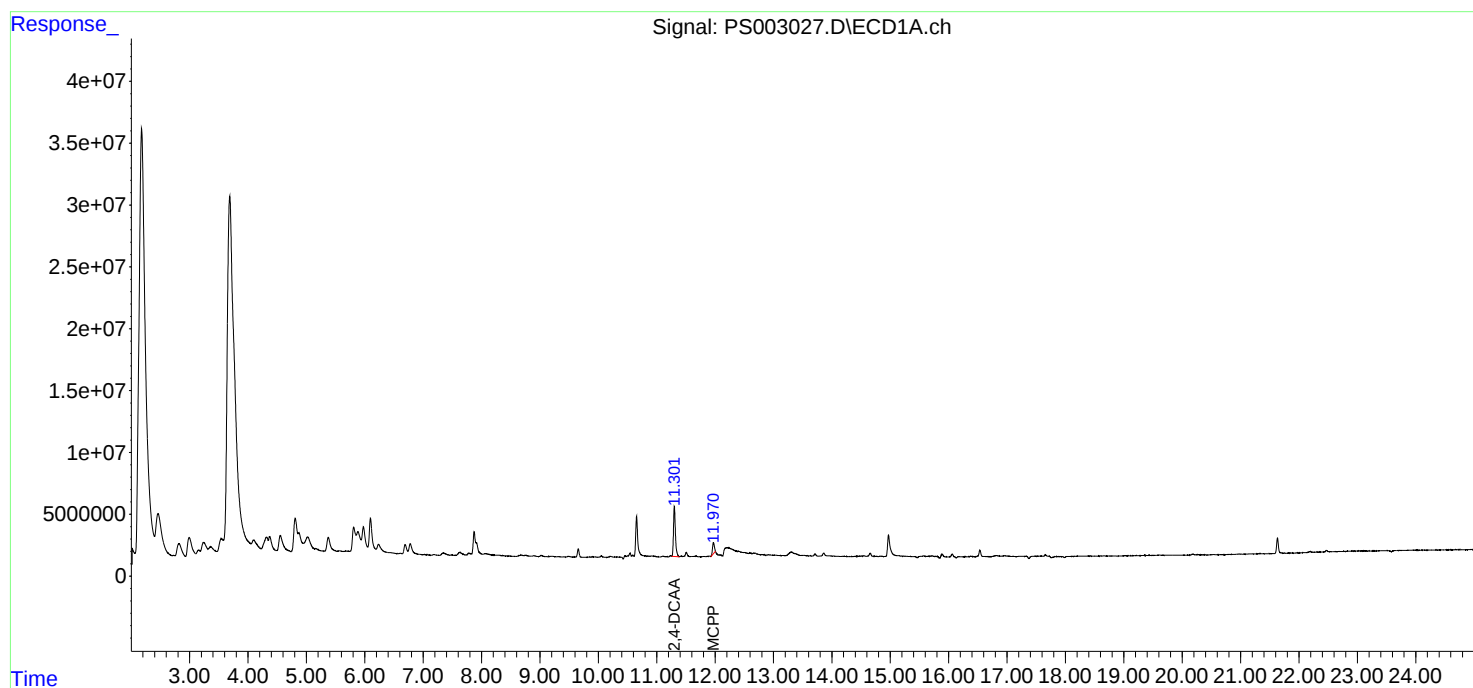


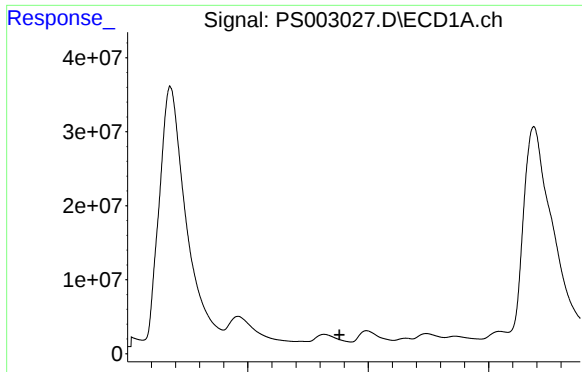

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116800TB

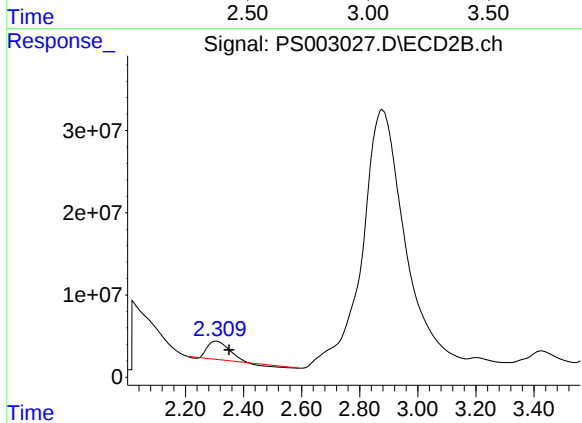


#1 Dalapon

R.T.: 2.304 min
Delta R.T.: -0.046 min
Response: 104909387
Conc: 195.76 ng/ml

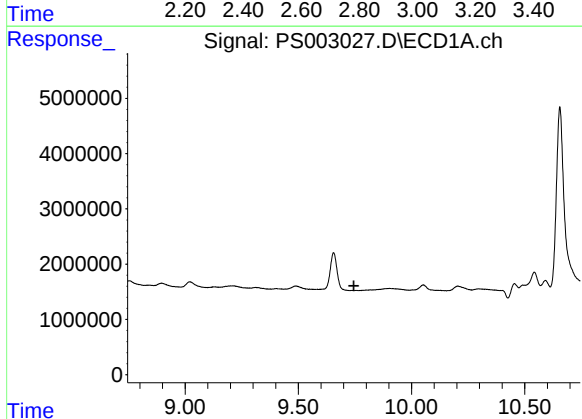


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

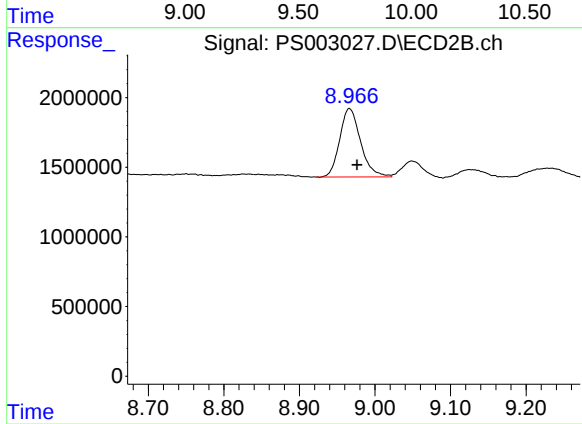

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.966 min
Delta R.T.: -0.010 min
Response: 9434103
Conc: 16.74 ng/ml

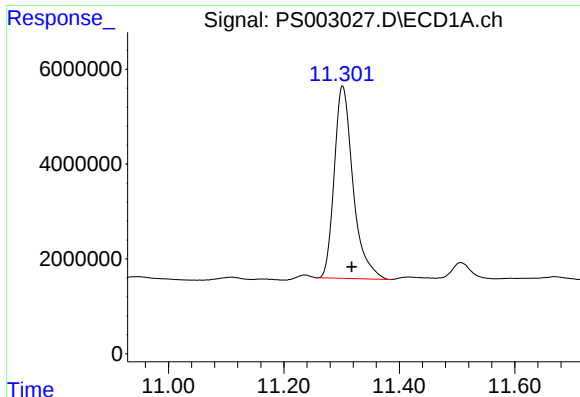

#4 2,4-DCAA


R.T.: 11.302 min
Delta R.T.: -0.016 min
Response: 91767294
Conc: 241.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116800TB

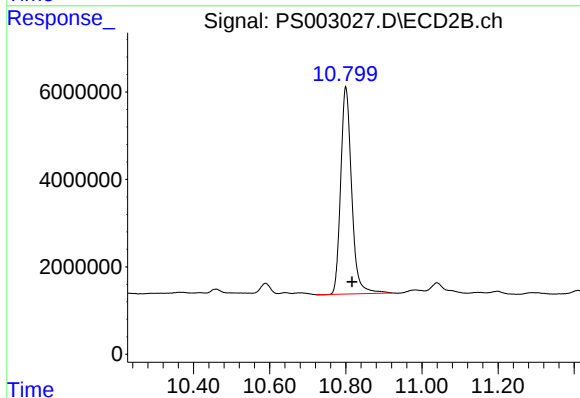


#4 2,4-DCAA

R.T.: 10.800 min
Delta R.T.: -0.017 min
Response: 94293201
Conc: 220.55 ng/ml

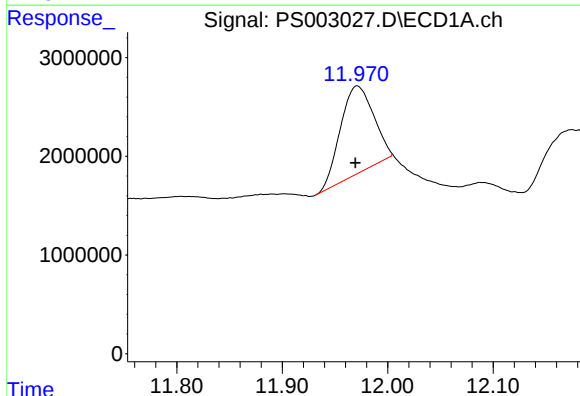


#6 MCP

R.T.: 11.972 min
Delta R.T.: 0.002 min
Response: 20058946
Conc: 16.74 ug/ml

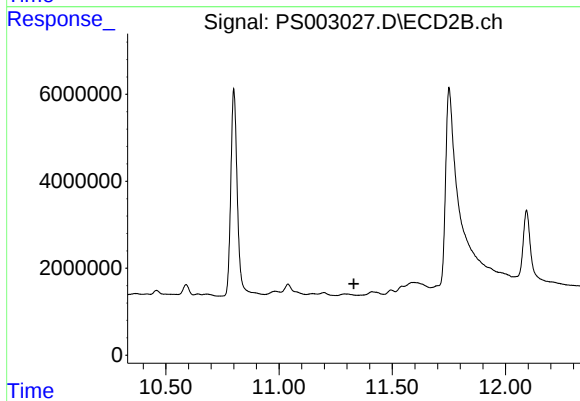

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

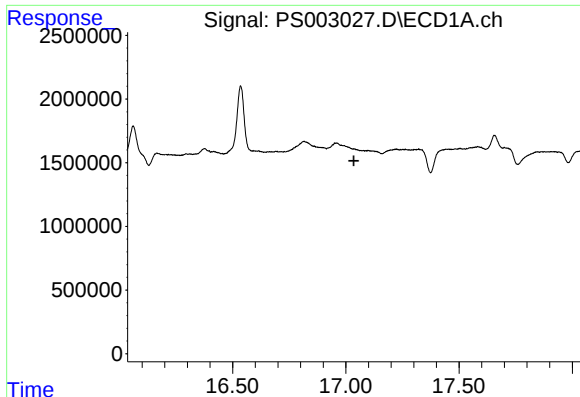

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116800TB

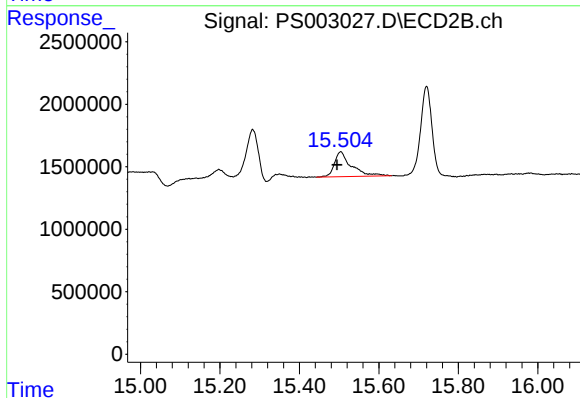


#14 DINOSEB

R.T.: 15.504 min
Delta R.T.: 0.009 min
Response: 5900017
Conc: 3.37 ng/ml

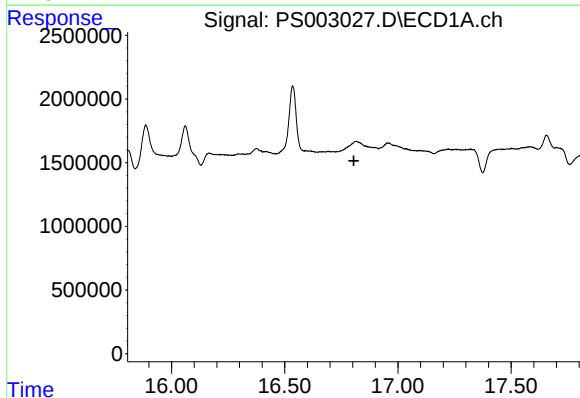


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.806 min
Response: 0
Conc: N.D.

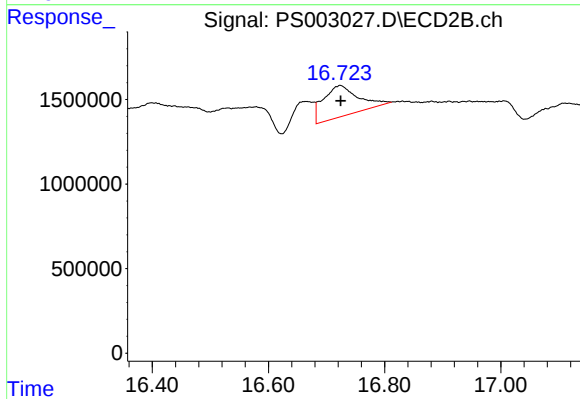

#15 Picloram


R.T.: 16.724 min
Delta R.T.: 0.000 min
Response: 7601703
Conc: 2.53 ng/ml

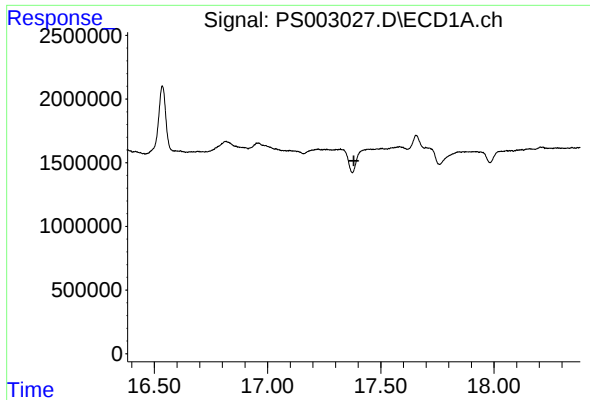

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116800TB

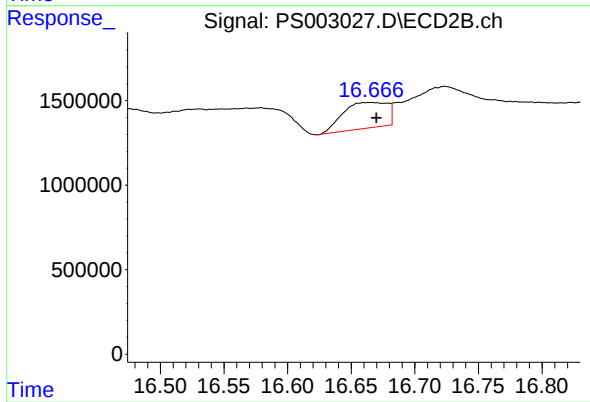

#16 DCPA

R.T.: 16.665 min
Delta R.T.: -0.005 min
Response: 3704040
Conc: 1.20 ng/ml