

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
 Data File : PS003035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2019 19:39
 Operator : EI\SJ
 Sample : K1346-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-020419-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:15:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.297	10.781	196.8E6	204.7E6	518.307	478.812
Target Compounds							
1) T	Dalapon	0.000	2.284	0	94688916	N.D.	176.684 #
2) T	3,5-DICHL...	0.000	8.949	0	9298123	N.D.	16.499 #
3) T	4-Nitroph...	0.000	10.003	0	6398071	N.D.	30.609 #
6) T	MCP	11.968	0.000	14054204	0	11.730	N.D. #
9) T	2,4-D	13.156	0.000	5713418	0	12.392	N.D. #
10) T	Pentachlo...	0.000	13.278	0	2159700	N.D.	0.349 #
11) T	2,4,5-TP ...	14.482	0.000	9170265	0	3.641	N.D. #
12) T	2,4,5-T	0.000	14.434	0	3674488	N.D.	1.920 #
14) T	DINOSEB	0.000	15.489	0	7668980	N.D.	4.375 #
15) T	Picloram	16.780	16.703	7402730	9950145	2.340	3.310 #
16) T	DCPA	17.436	16.703	-6942626	9950145	N.D.	3.212



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
Data File : PS003035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2019 19:39
Operator : EI\SJ
Sample : K1346-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:15:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

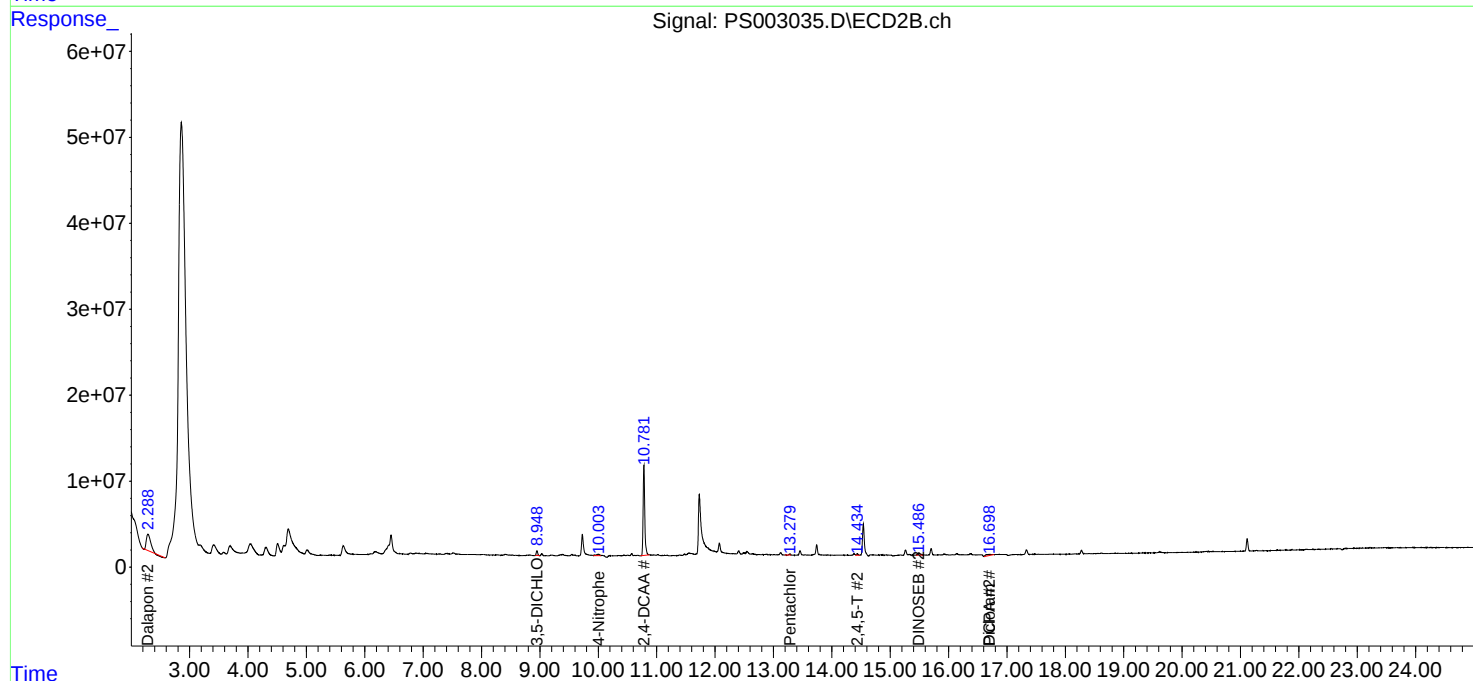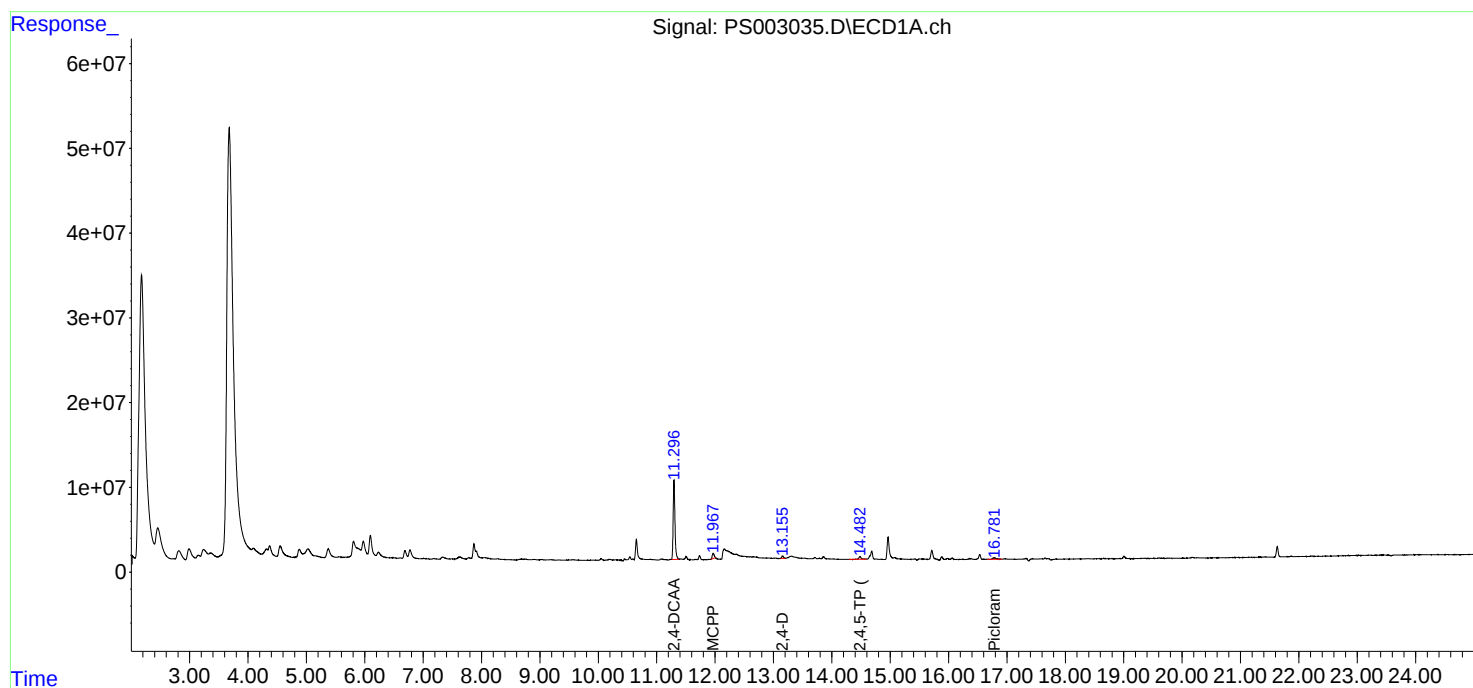


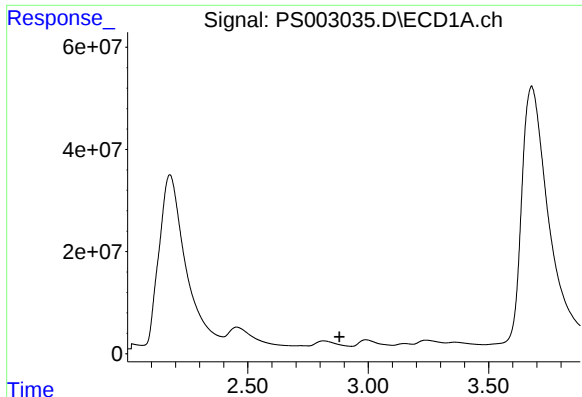

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-B

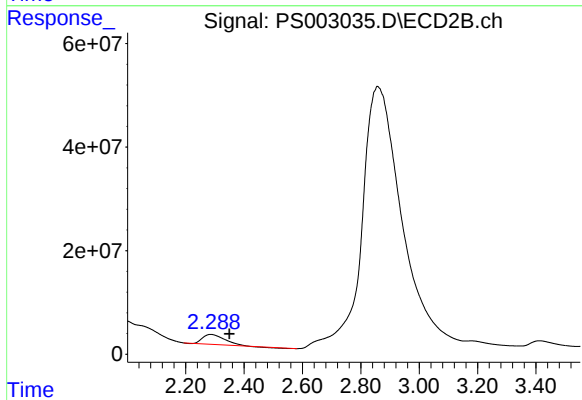


#1 Dalapon

R.T.: 2.284 min
Delta R.T.: -0.066 min
Response: 94688916
Conc: 176.68 ng/ml

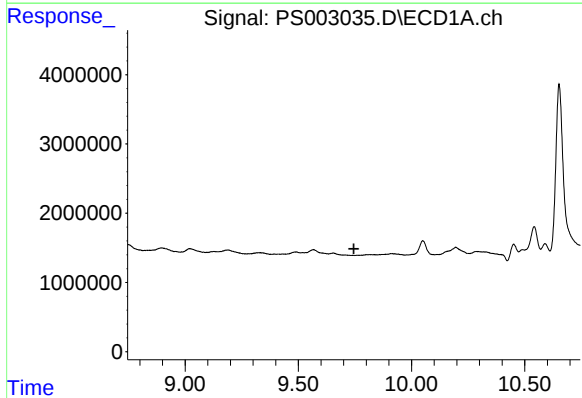


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

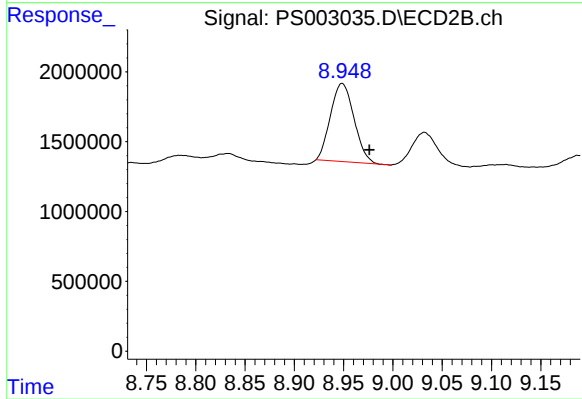

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.949 min
Delta R.T.: -0.028 min
Response: 9298123
Conc: 16.50 ng/ml

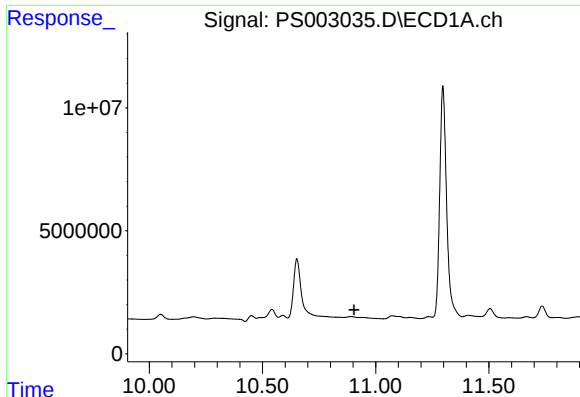

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-B

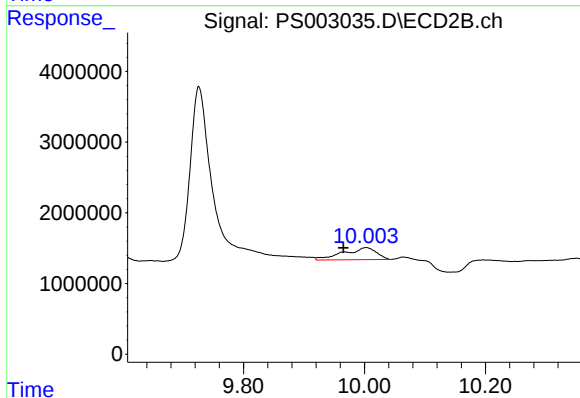


#3 4-Nitrophenol

R.T.: 10.003 min
Delta R.T.: 0.037 min
Response: 6398071
Conc: 30.61 ng/ml

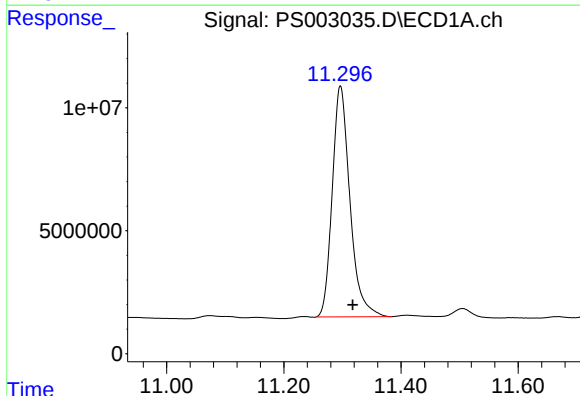


#4 2,4-DCAA

R.T.: 11.297 min
Delta R.T.: -0.021 min
Response: 196770424
Conc: 518.31 ng/ml

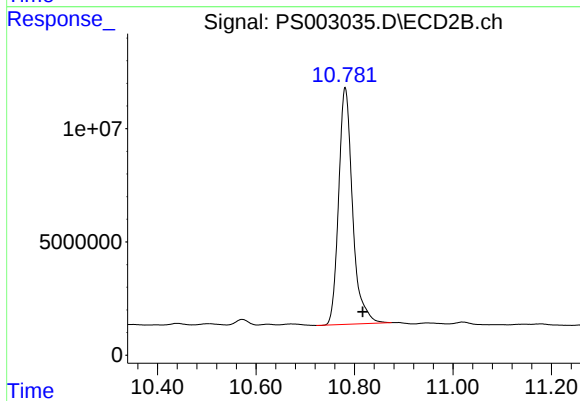

#4 2,4-DCAA


R.T.: 10.781 min
Delta R.T.: -0.035 min
Response: 204714206
Conc: 478.81 ng/ml

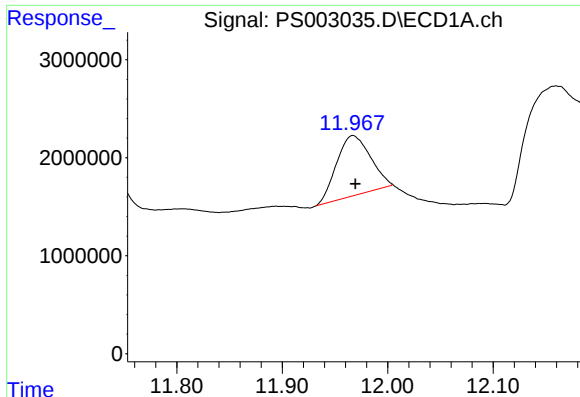

#6 MCP


R.T.: 11.968 min
Delta R.T.: -0.002 min
Response: 14054204
Conc: 11.73 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-B

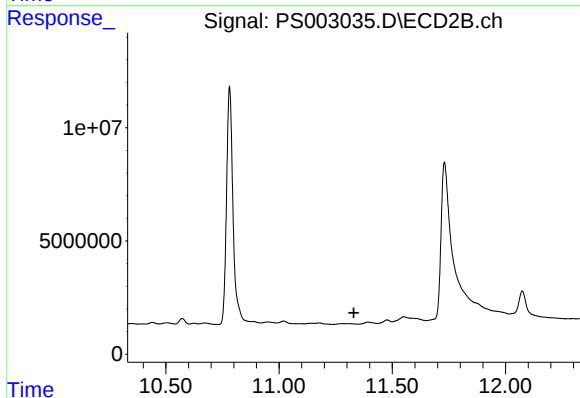


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

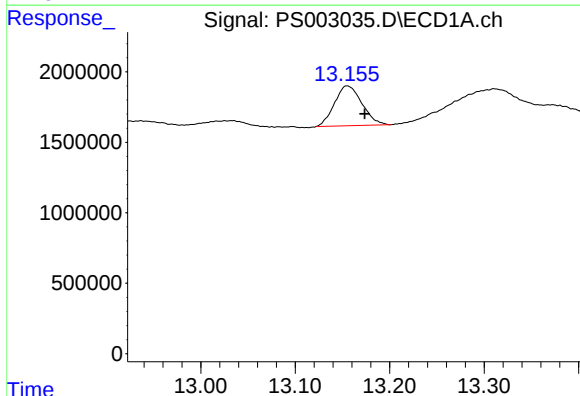


#9 2,4-D

R.T.: 13.156 min
Delta R.T.: -0.018 min
Response: 5713418
Conc: 12.39 ng/ml

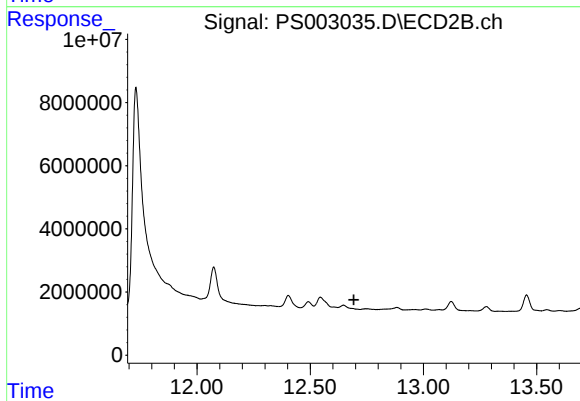

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

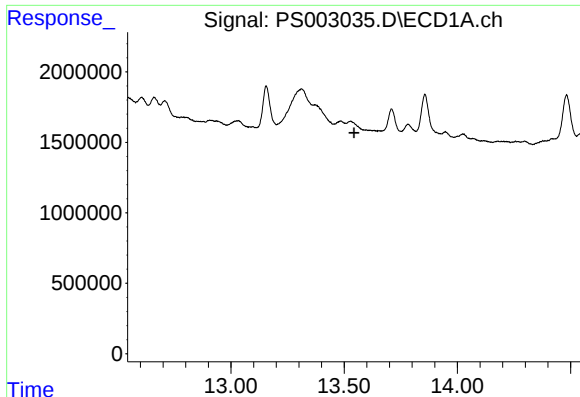

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-B

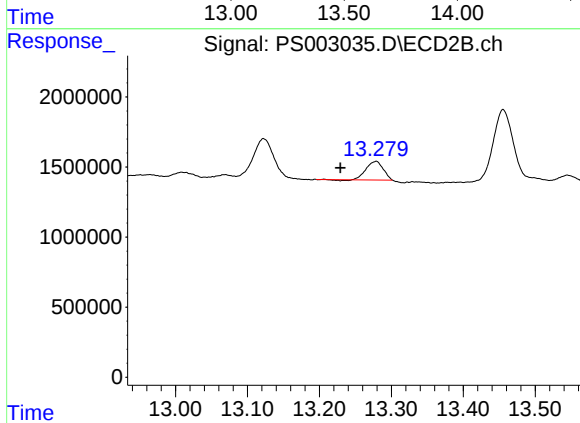


#10 Pentachlorophenol

R.T.: 13.278 min
Delta R.T.: 0.049 min
Response: 2159700
Conc: 0.35 ng/ml

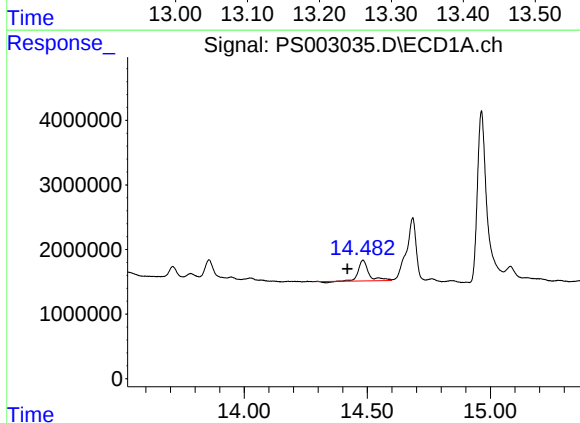


#11 2,4,5-TP (SILVEX)

R.T.: 14.482 min
Delta R.T.: 0.063 min
Response: 9170265
Conc: 3.64 ng/ml

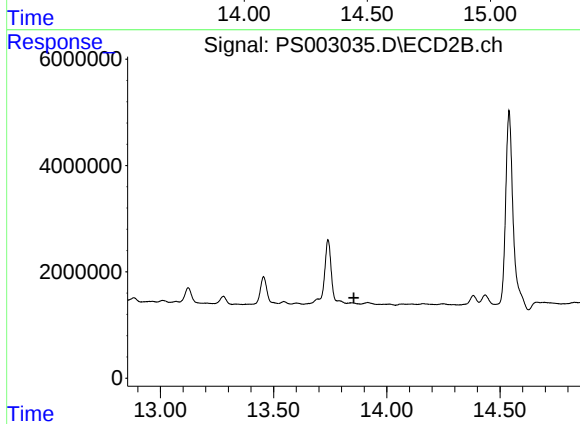

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.854 min
Response: 0
Conc: N.D.

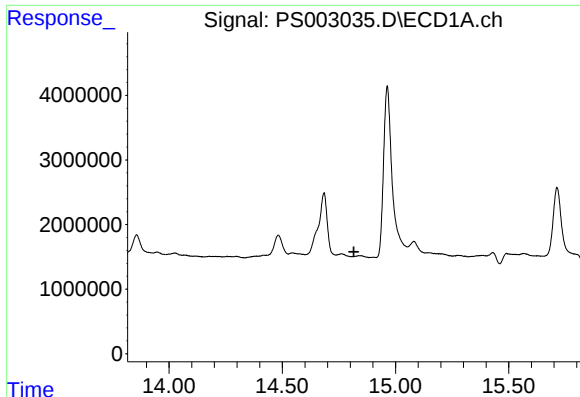

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-B

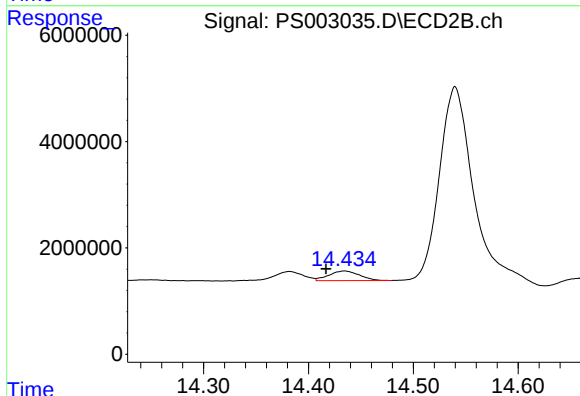


#12 2,4,5-T

R.T.: 14.434 min
Delta R.T.: 0.017 min
Response: 3674488
Conc: 1.92 ng/ml

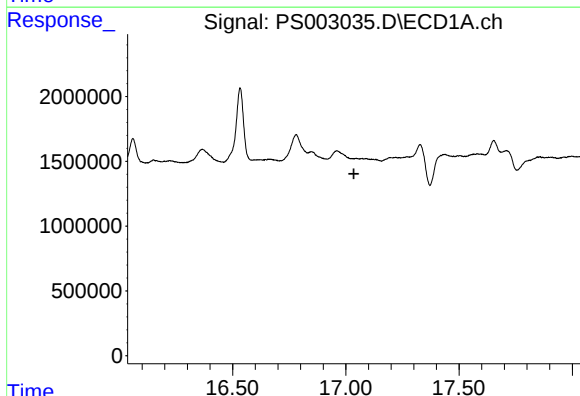


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

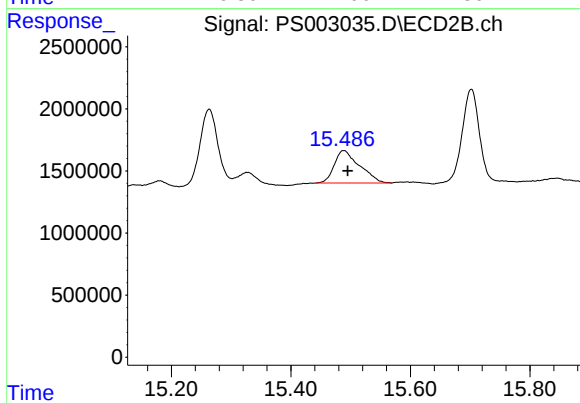

#14 DINOSEB


R.T.: 15.489 min
Delta R.T.: -0.006 min
Response: 7668980
Conc: 4.37 ng/ml

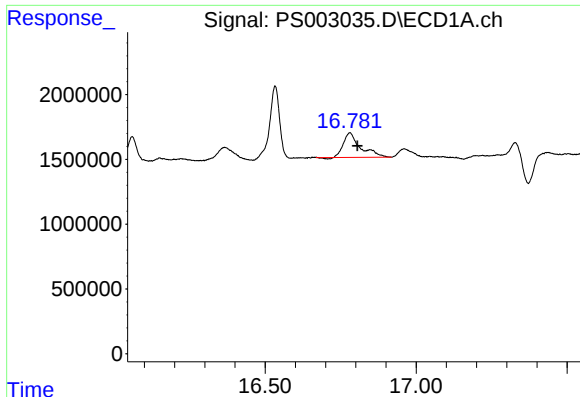

#15 Picloram


R.T.: 16.780 min
Delta R.T.: -0.026 min
Response: 7402730
Conc: 2.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-B

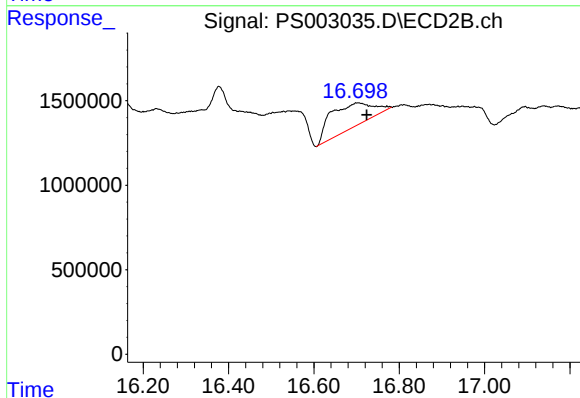


#15 Picloram

R.T.: 16.703 min
Delta R.T.: -0.021 min
Response: 9950145
Conc: 3.31 ng/ml

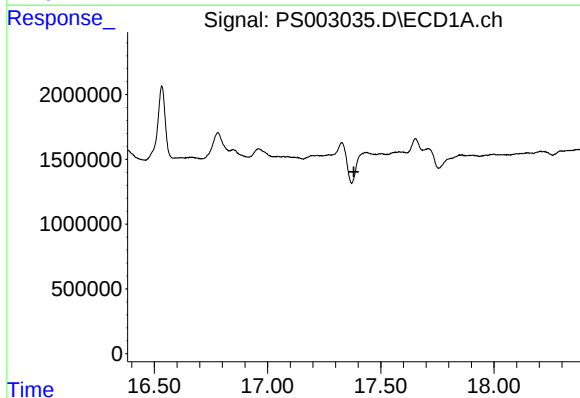

#16 DCPA

R.T.: 17.436 min
Delta R.T.: 0.054 min
Response: -6942626
Conc: N.D.

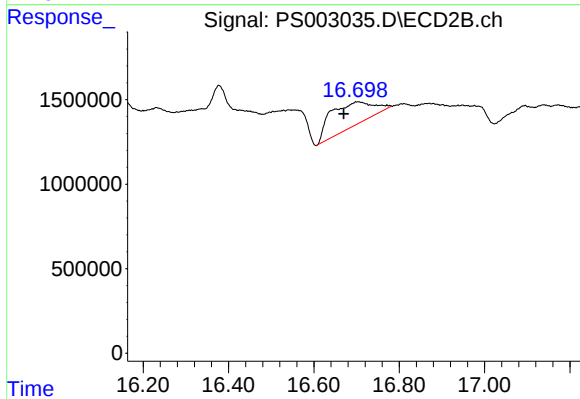

#16 DCPA

R.T.: 16.703 min
Delta R.T.: 0.033 min
Response: 9950145
Conc: 3.21 ng/ml