

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
 Data File : PS003036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2019 20:10
 Operator : EI\SJ
 Sample : K1346-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-020419-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:16:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.299	10.799	211.8E6	218.4E6	557.872	510.871
Target Compounds							
1) T	Dalapon	0.000	2.308	0	144.5E6	N.D.	269.717 #
2) T	3,5-DICHL...	0.000	8.967	0	7154540	N.D.	12.695 #
3) T	4-Nitroph...	0.000	9.984	0	1929137	N.D.	9.229 #
6) T	MCP	11.969	0.000	13858566	0	11.567	N.D. #
9) T	2,4-D	13.159	12.665	6095087	2771856	13.220	5.528 #
11) T	2,4,5-TP ...	14.485	0.000	7228381	0	2.870	N.D. #
12) T	2,4,5-T	0.000	14.400	0	3270734	N.D.	1.709 #
14) T	DINOSEB	0.000	15.508	0	7307572	N.D.	4.169 #
15) T	Picloram	16.780	16.724	11976435	9332954	3.786	3.104
16) T	DCPA	0.000	16.724	0	9332954	N.D.	3.013 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
Data File : PS003036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2019 20:10
Operator : EI\SJ
Sample : K1346-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:16:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

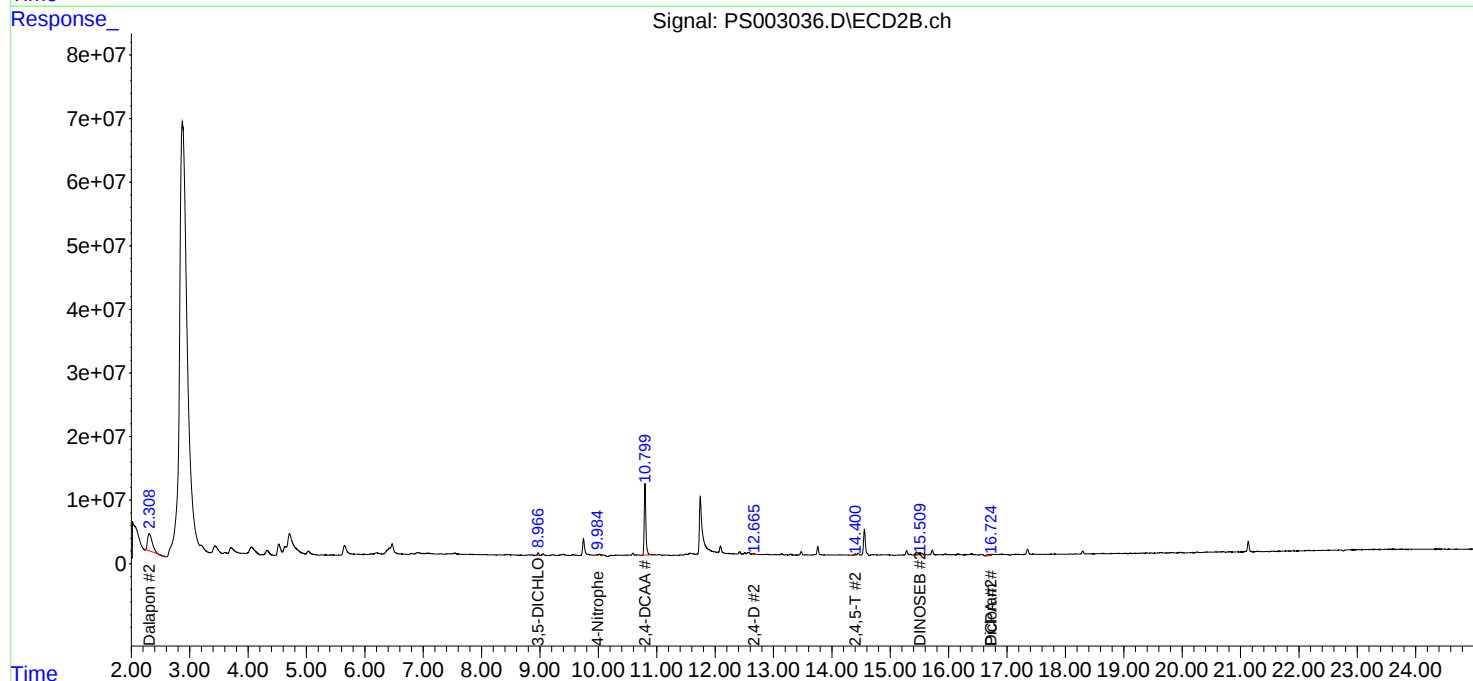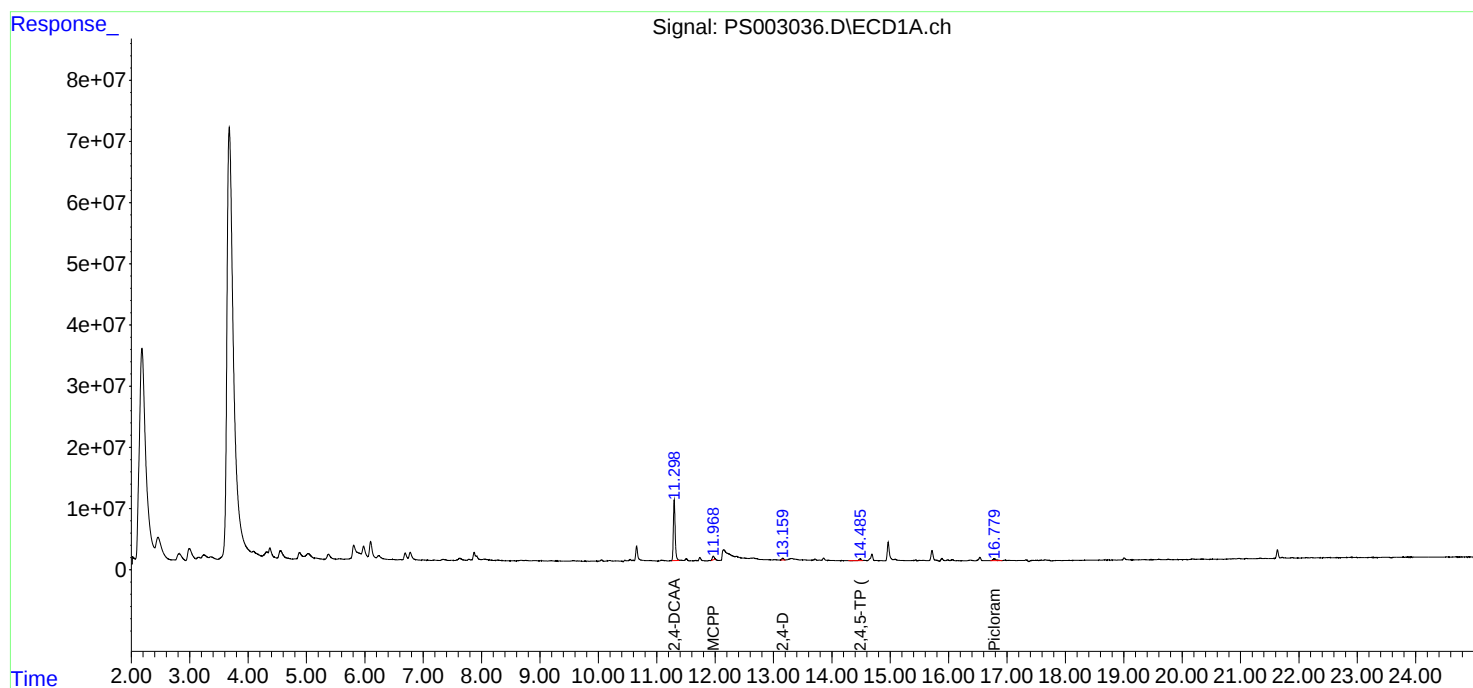


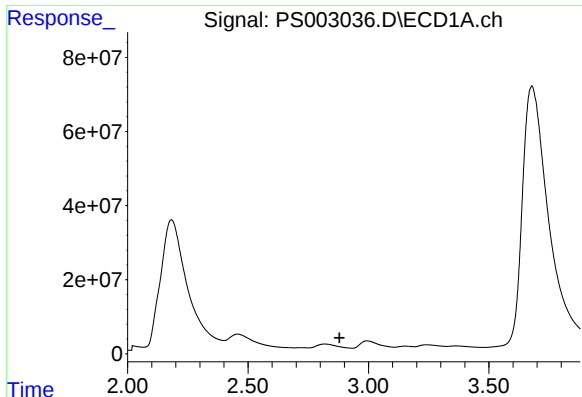

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-C

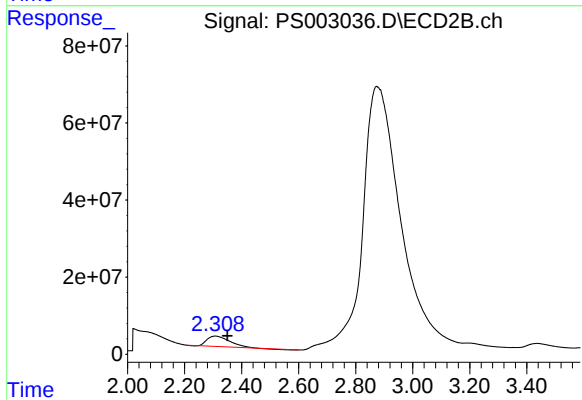


#1 Dalapon

R.T.: 2.308 min
Delta R.T.: -0.043 min
Response: 144546903
Conc: 269.72 ng/ml

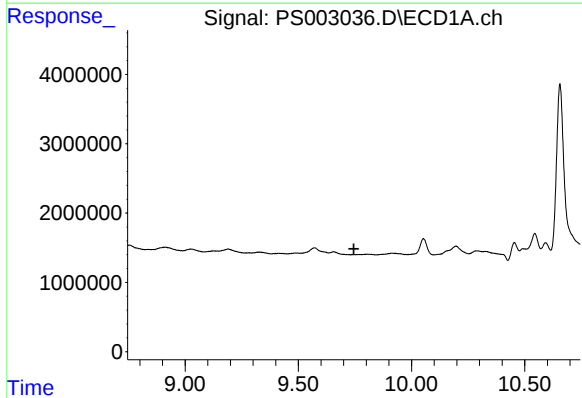


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

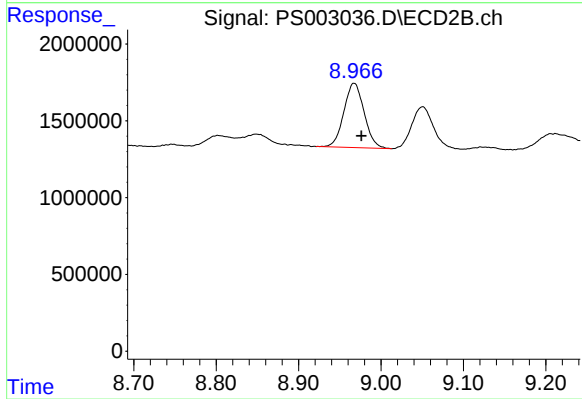

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.967 min
Delta R.T.: -0.009 min
Response: 7154540
Conc: 12.70 ng/ml

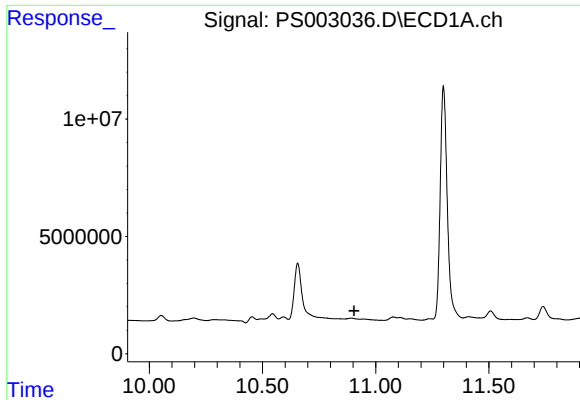

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-C

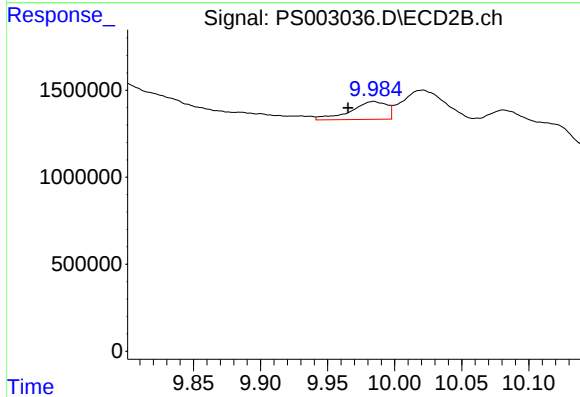


#3 4-Nitrophenol

R.T.: 9.984 min
Delta R.T.: 0.019 min
Response: 1929137
Conc: 9.23 ng/ml

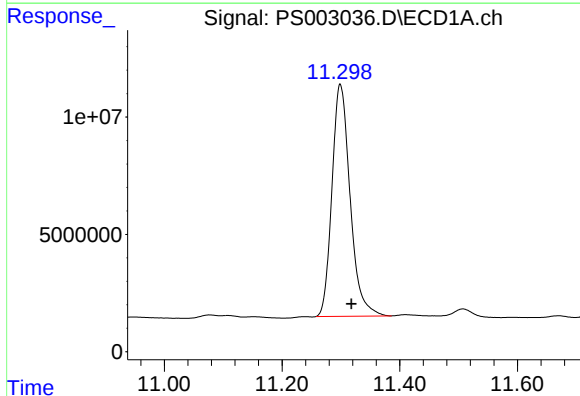


#4 2,4-DCAA

R.T.: 11.299 min
Delta R.T.: -0.018 min
Response: 211790780
Conc: 557.87 ng/ml

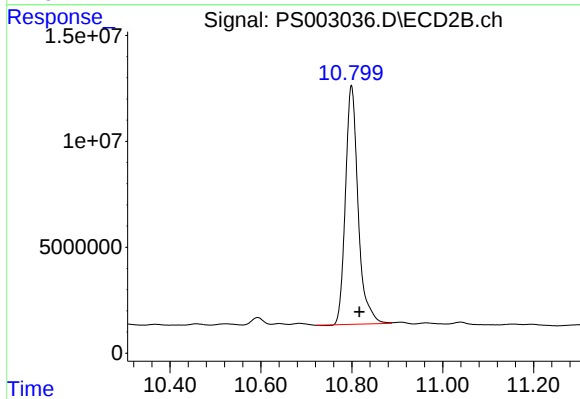

#4 2,4-DCAA


R.T.: 10.799 min
Delta R.T.: -0.017 min
Response: 218420914
Conc: 510.87 ng/ml

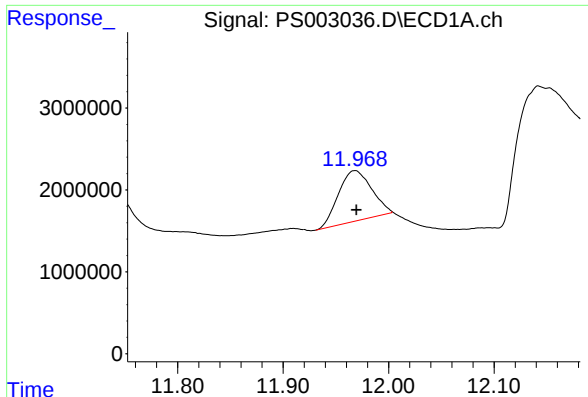

#6 MCP


R.T.: 11.969 min
Delta R.T.: 0.000 min
Response: 13858566
Conc: 11.57 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-C

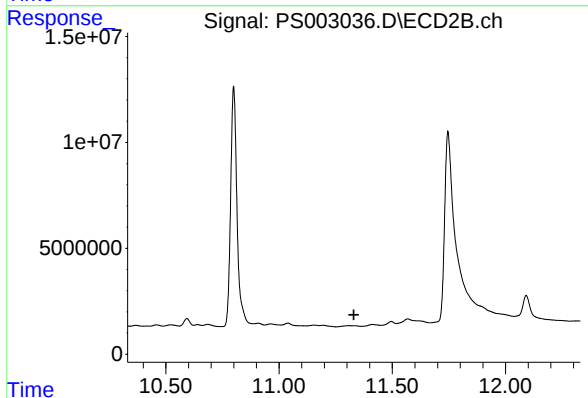


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

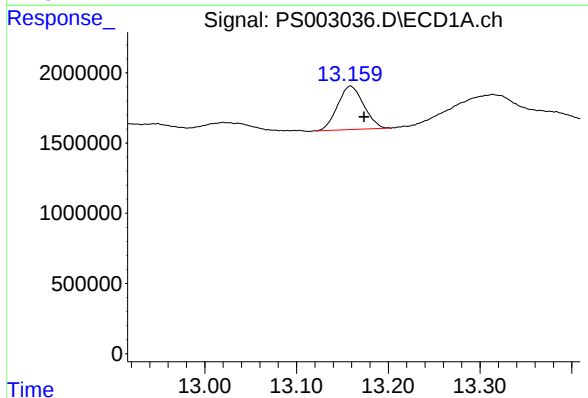


#9 2,4-D

R.T.: 13.159 min
Delta R.T.: -0.014 min
Response: 6095087
Conc: 13.22 ng/ml

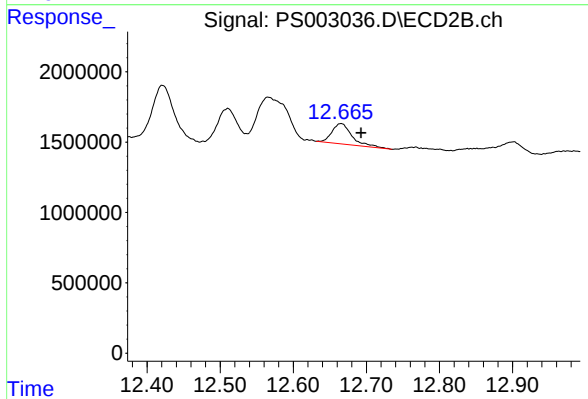

#9 2,4-D


R.T.: 12.665 min
Delta R.T.: -0.028 min
Response: 2771856
Conc: 5.53 ng/ml

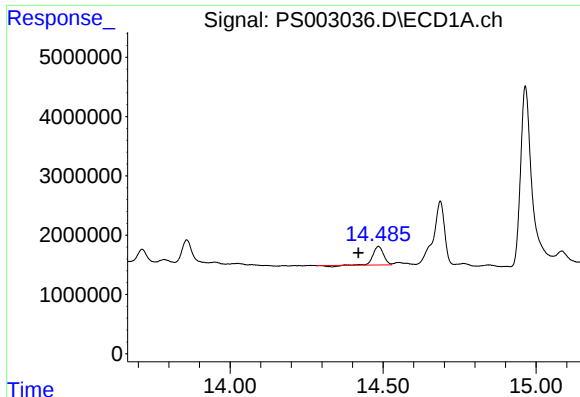

#11 2,4,5-TP (SILVEX)


R.T.: 14.485 min
Delta R.T.: 0.065 min
Response: 7228381
Conc: 2.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-C

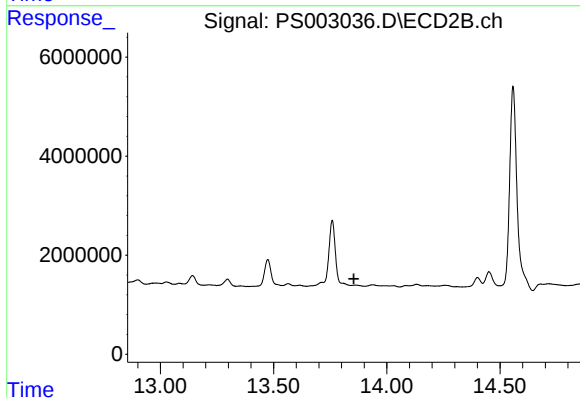


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

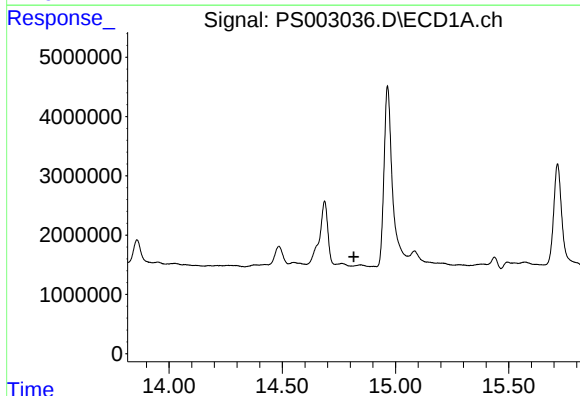


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

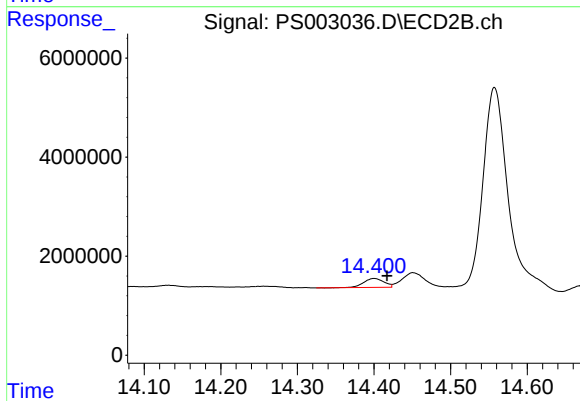

#12 2,4,5-T


R.T.: 14.400 min
Delta R.T.: -0.017 min
Response: 3270734
Conc: 1.71 ng/ml

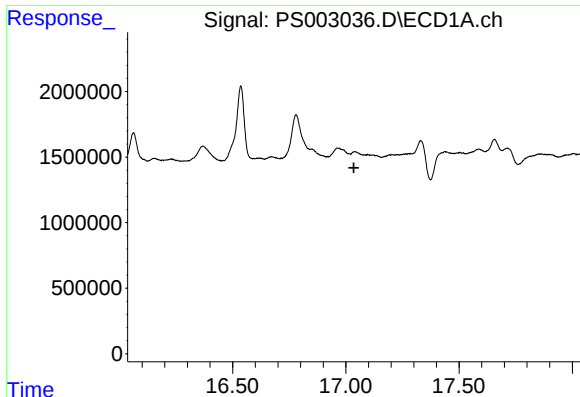

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-C

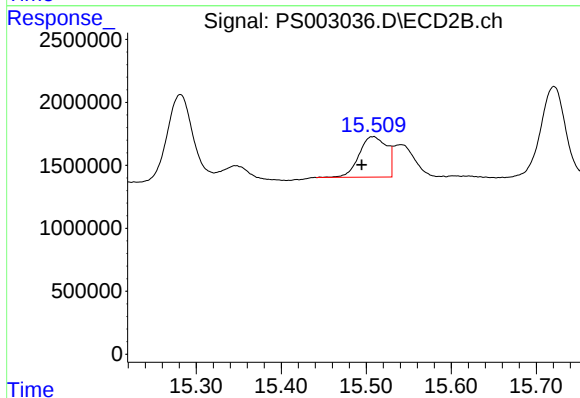


#14 DINOSEB

R.T.: 15.508 min
Delta R.T.: 0.013 min
Response: 7307572
Conc: 4.17 ng/ml

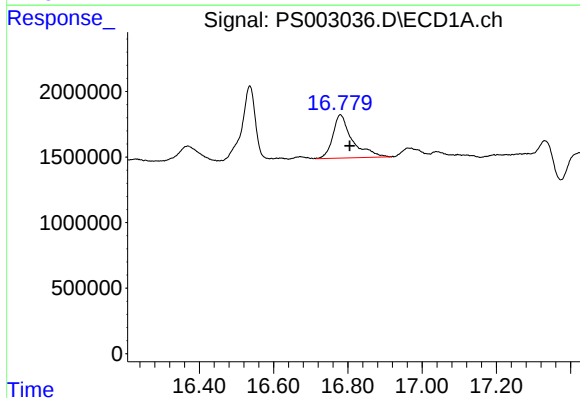


#15 Picloram

R.T.: 16.780 min
Delta R.T.: -0.026 min
Response: 11976435
Conc: 3.79 ng/ml

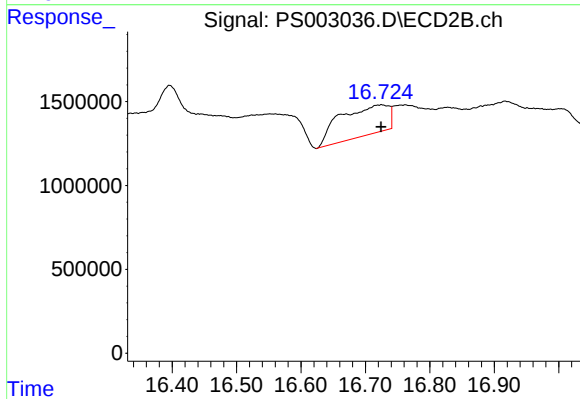

#15 Picloram


R.T.: 16.724 min
Delta R.T.: 0.000 min
Response: 9332954
Conc: 3.10 ng/ml

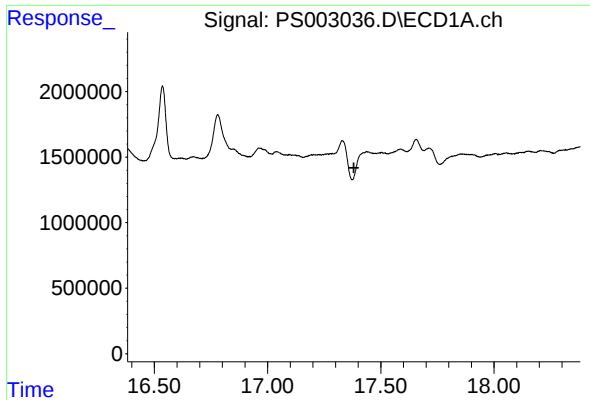

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-020419-C

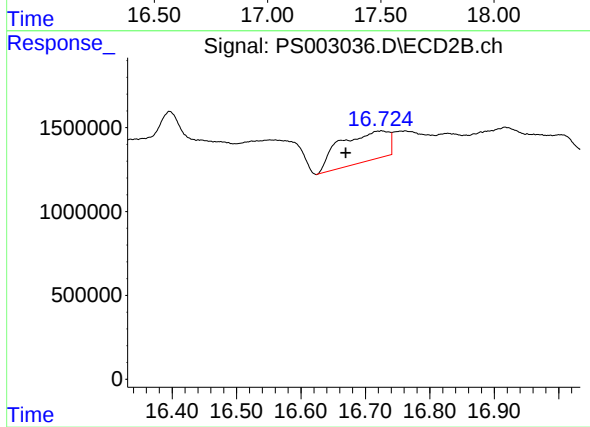

#16 DCPA

R.T.: 16.724 min
Delta R.T.: 0.055 min
Response: 9332954
Conc: 3.01 ng/ml