

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
 Data File : PS003037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2019 20:41
 Operator : EI\SJ
 Sample : K1350-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-03-020419-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:16:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.283	10.783	181.0E6	222.4E6	476.734	520.203
Target Compounds							
1) T	Dalapon	0.000	2.289	0	116.6E6	N.D.	217.575 #
2) T	3,5-DICHL...	0.000	8.951	0	8815461	N.D.	15.642 #
3) T	4-Nitroph...	0.000	9.970	0	3928539	N.D.	18.795 #
9) T	2,4-D	13.141	0.000	3580905	0	7.767	N.D. #
10) T	Pentachlo...	0.000	13.279	0	2629236	N.D.	0.425 #
11) T	2,4,5-TP ...	14.468	0.000	11398672	0	4.526	N.D. #
12) T	2,4,5-T	0.000	14.434	0	4116419	N.D.	2.151 #
14) T	DINOSEB	0.000	15.490	0	6959760	N.D.	3.970 #
15) T	Picloram	16.763	16.737	11688925	11161063	3.695	3.712
16) T	DCPA	17.427	16.737	-4105418	11161063	N.D.	3.603



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
Data File : PS003037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2019 20:41
Operator : EI\SJ
Sample : K1350-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:16:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

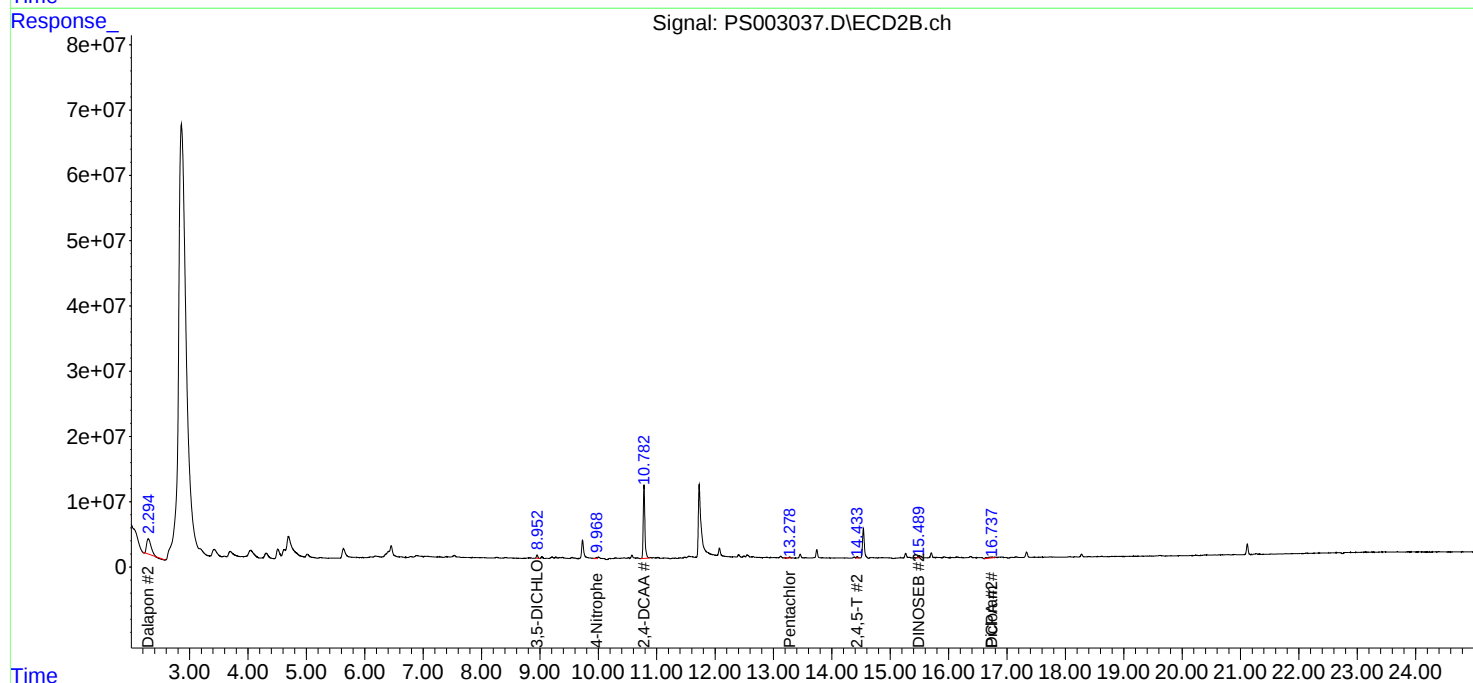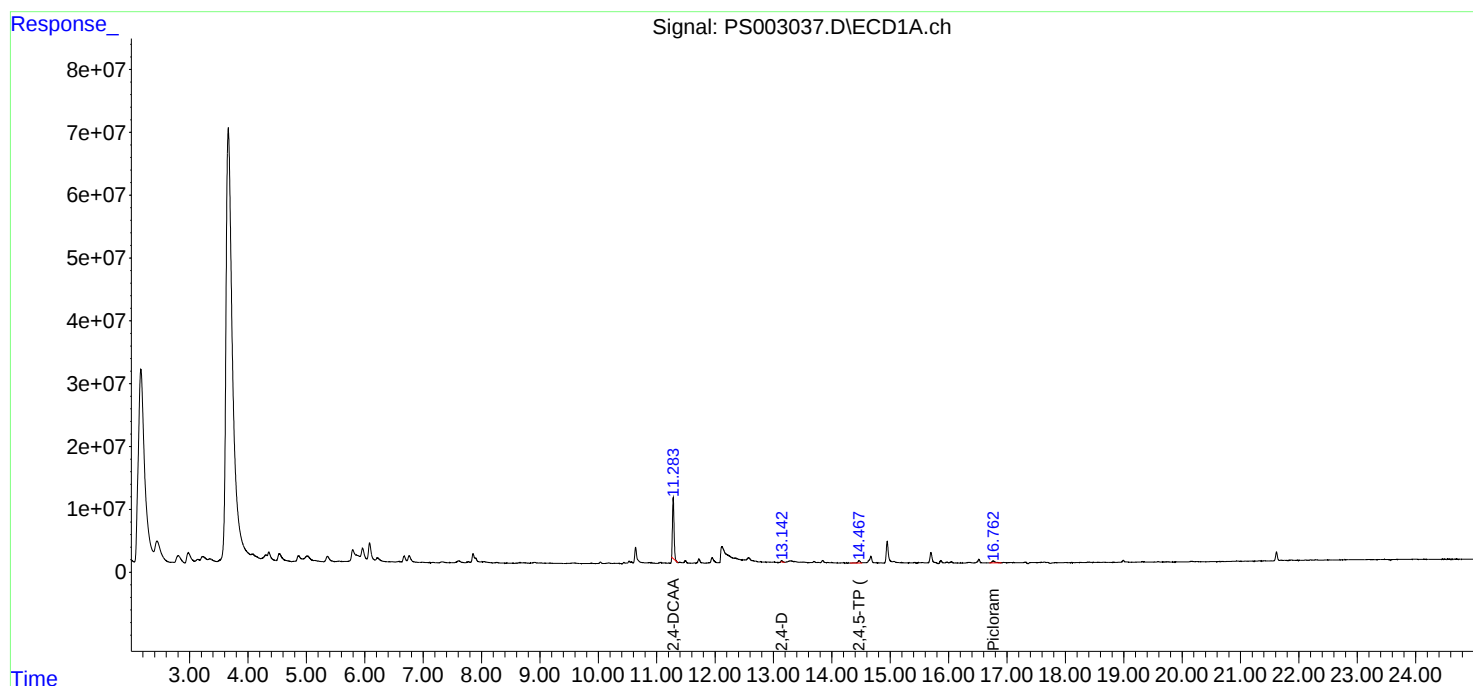


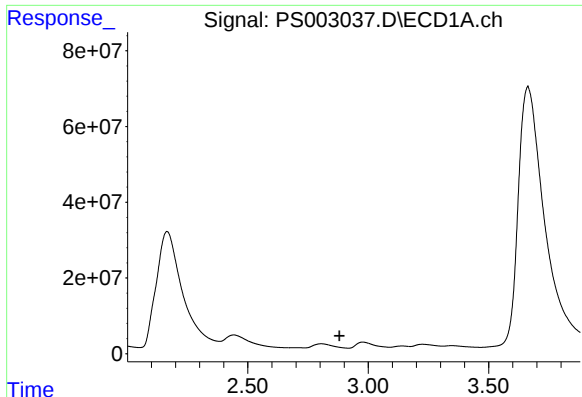

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-A

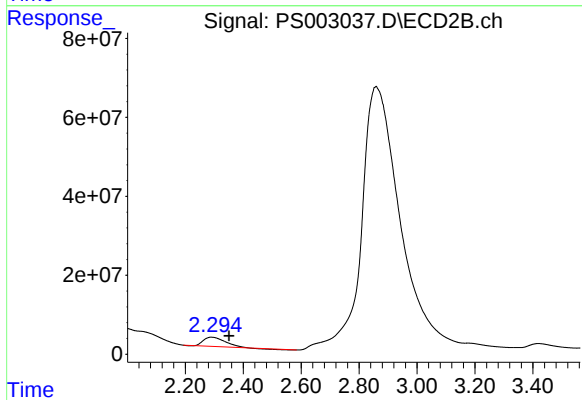


#1 Dalapon

R.T.: 2.289 min
Delta R.T.: -0.061 min
Response: 116603205
Conc: 217.58 ng/ml

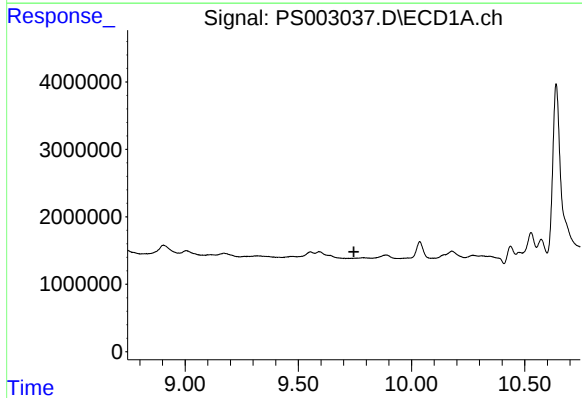


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

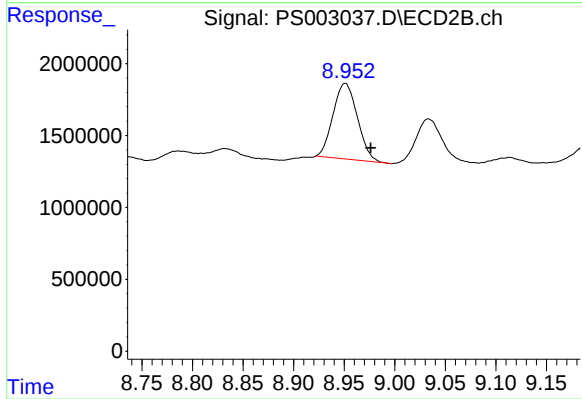

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.951 min
Delta R.T.: -0.025 min
Response: 8815461
Conc: 15.64 ng/ml

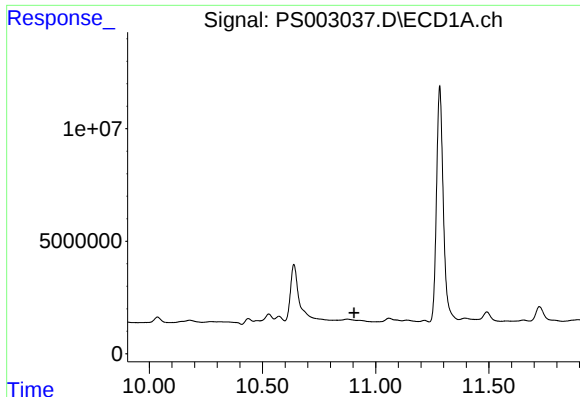

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-A

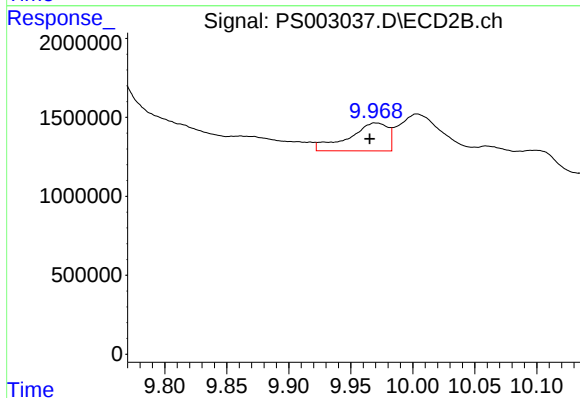


#3 4-Nitrophenol

R.T.: 9.970 min
Delta R.T.: 0.005 min
Response: 3928539
Conc: 18.79 ng/ml

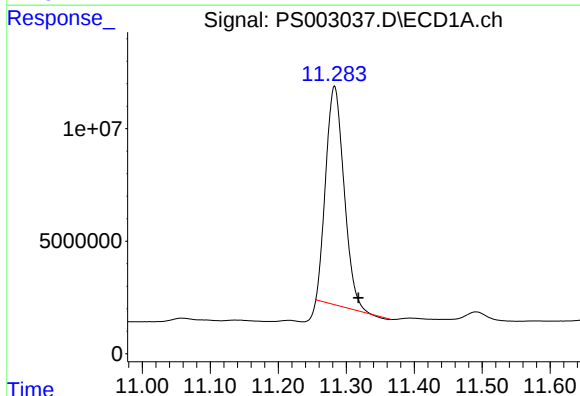


#4 2,4-DCAA

R.T.: 11.283 min
Delta R.T.: -0.035 min
Response: 180987829
Conc: 476.73 ng/ml

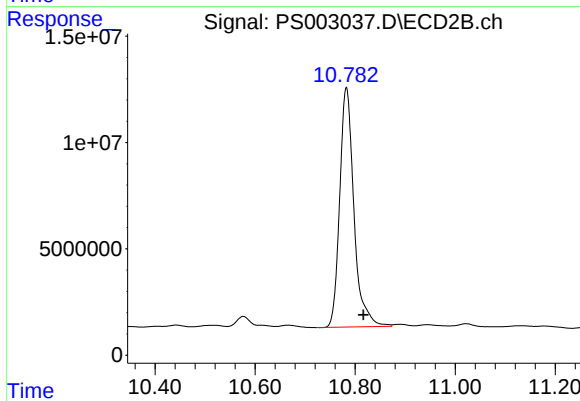

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: -0.034 min
Response: 222410424
Conc: 520.20 ng/ml

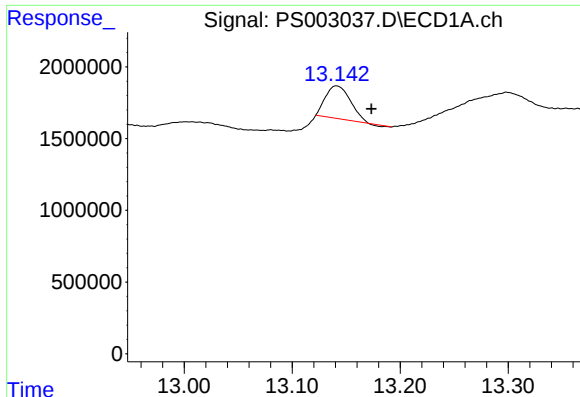

#9 2,4-D


R.T.: 13.141 min
Delta R.T.: -0.032 min
Response: 3580905
Conc: 7.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-A

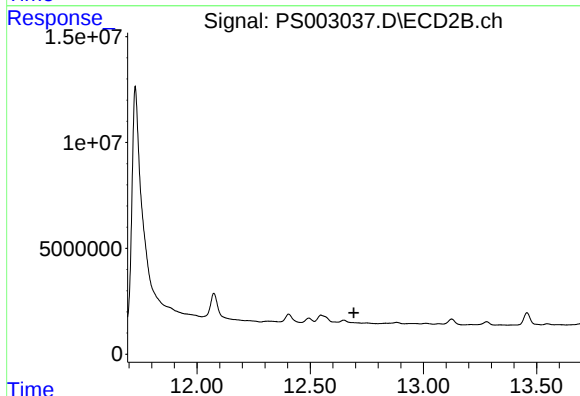


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

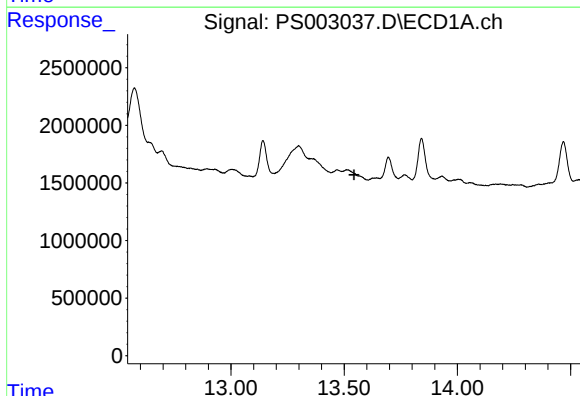


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.543 min
Response: 0
Conc: N.D.

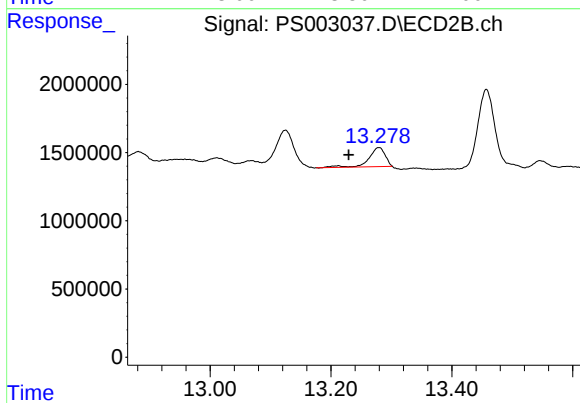

#10 Pentachlorophenol


R.T.: 13.279 min
Delta R.T.: 0.050 min
Response: 2629236
Conc: 0.43 ng/ml

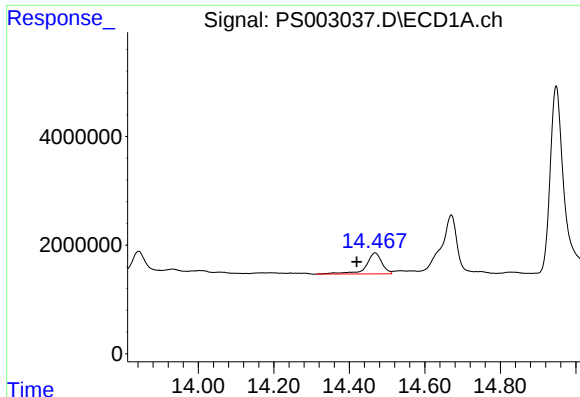

#11 2,4,5-TP (SILVEX)


R.T.: 14.468 min
Delta R.T.: 0.049 min
Response: 11398672
Conc: 4.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-A

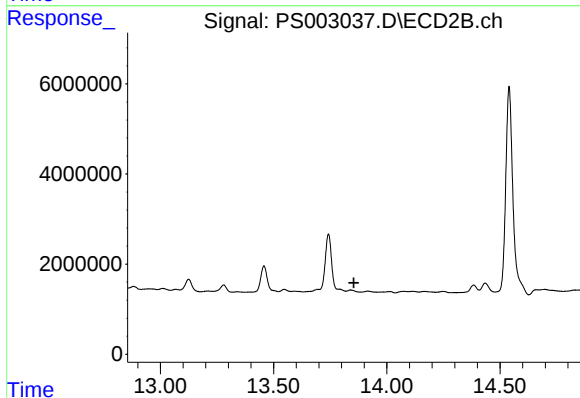


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

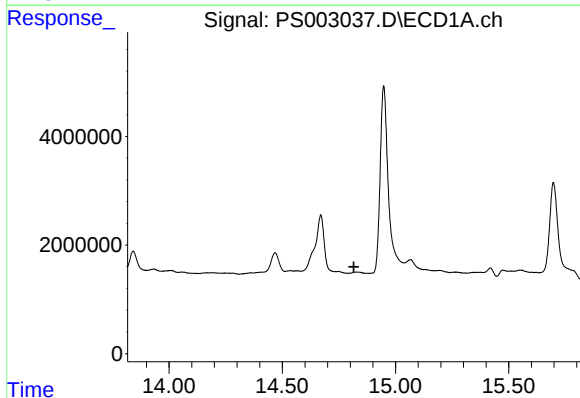


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

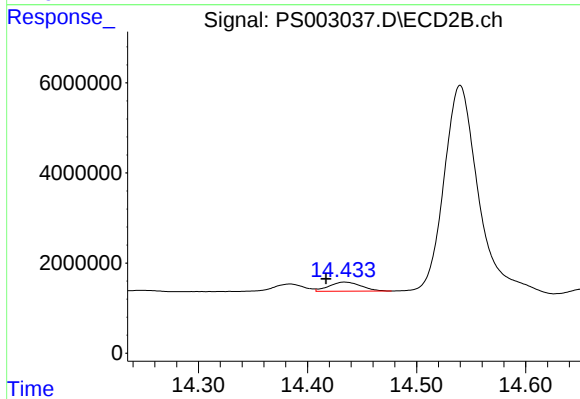

#12 2,4,5-T


R.T.: 14.434 min
Delta R.T.: 0.017 min
Response: 4116419
Conc: 2.15 ng/ml

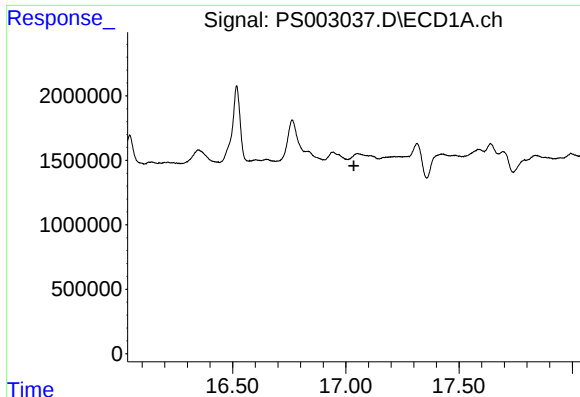

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-A

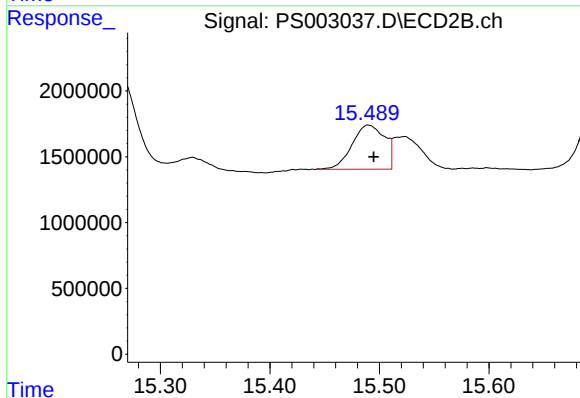


#14 DINOSEB

R.T.: 15.490 min
Delta R.T.: -0.005 min
Response: 6959760
Conc: 3.97 ng/ml

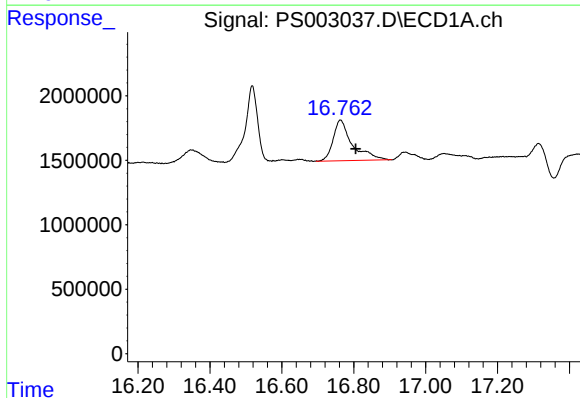


#15 Picloram

R.T.: 16.763 min
Delta R.T.: -0.043 min
Response: 11688925
Conc: 3.69 ng/ml

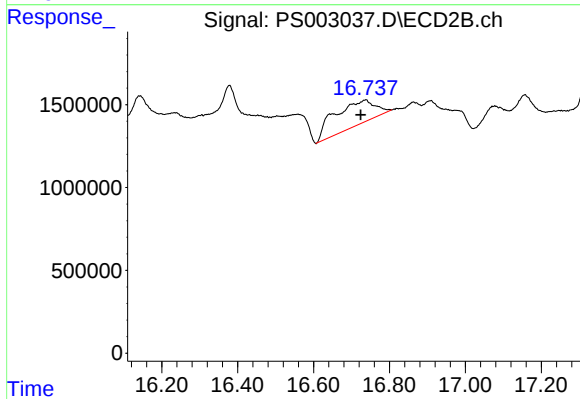

#15 Picloram


R.T.: 16.737 min
Delta R.T.: 0.013 min
Response: 11161063
Conc: 3.71 ng/ml

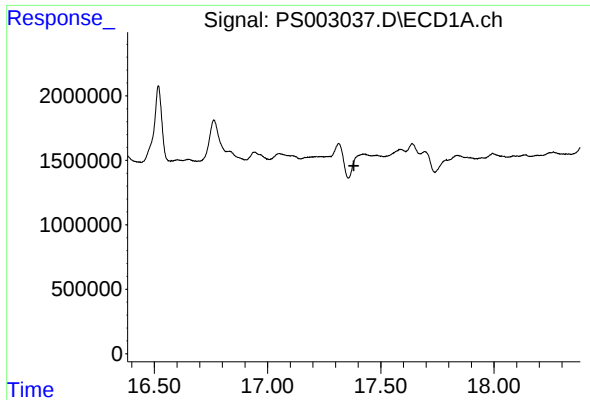

#16 DCPA

R.T.: 17.427 min
Delta R.T.: 0.046 min
Response: -4105418
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-A

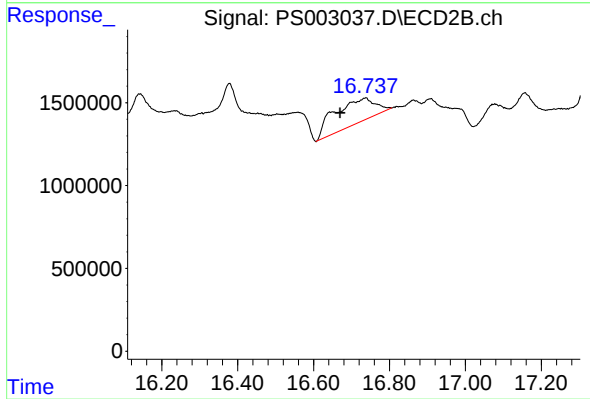

#16 DCPA

R.T.: 16.737 min
Delta R.T.: 0.067 min
Response: 11161063
Conc: 3.60 ng/ml