

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
 Data File : PS003038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2019 21:12
 Operator : EI\SJ
 Sample : K1350-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-03-020419-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:16:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.316	10.815	210.4E6	216.1E6	554.193	505.434
Target Compounds							
1) T	Dalapon	2.836	2.325	27490764	131.5E6	49.834	245.461 #
2) T	3,5-DICHL...	0.000	8.983	0	9009886	N.D.	15.987 #
3) T	4-Nitroph...	0.000	10.001	0	2392402	N.D.	11.446 #
6) T	MCP	11.985	0.000	6108150	0	5.098	N.D. #
7) T	MCPA	12.156	11.761	-28285195	155.8E6	N.D.	99.044
9) T	2,4-D	13.175	0.000	6713862	0	14.562	N.D. #
12) T	2,4,5-T	0.000	14.417	0	3287238	N.D.	1.718 #
14) T	DINOSEB	0.000	15.523	0	8666420	N.D.	4.944 #
15) T	Picloram	16.801	16.735	9653928	14208584	3.052	4.726 #
16) T	DCPA	0.000	16.735	0	14208584	N.D.	4.587 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
Data File : PS003038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2019 21:12
Operator : EI\SJ
Sample : K1350-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:16:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

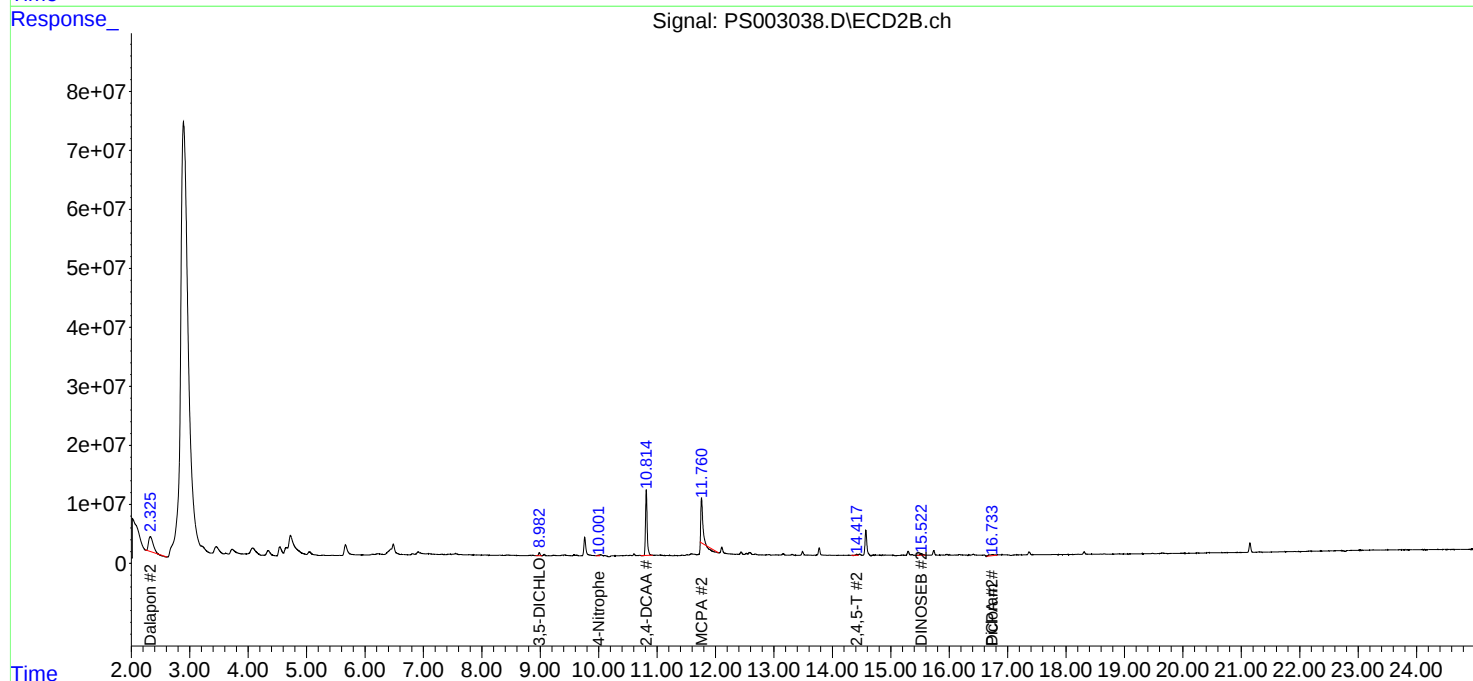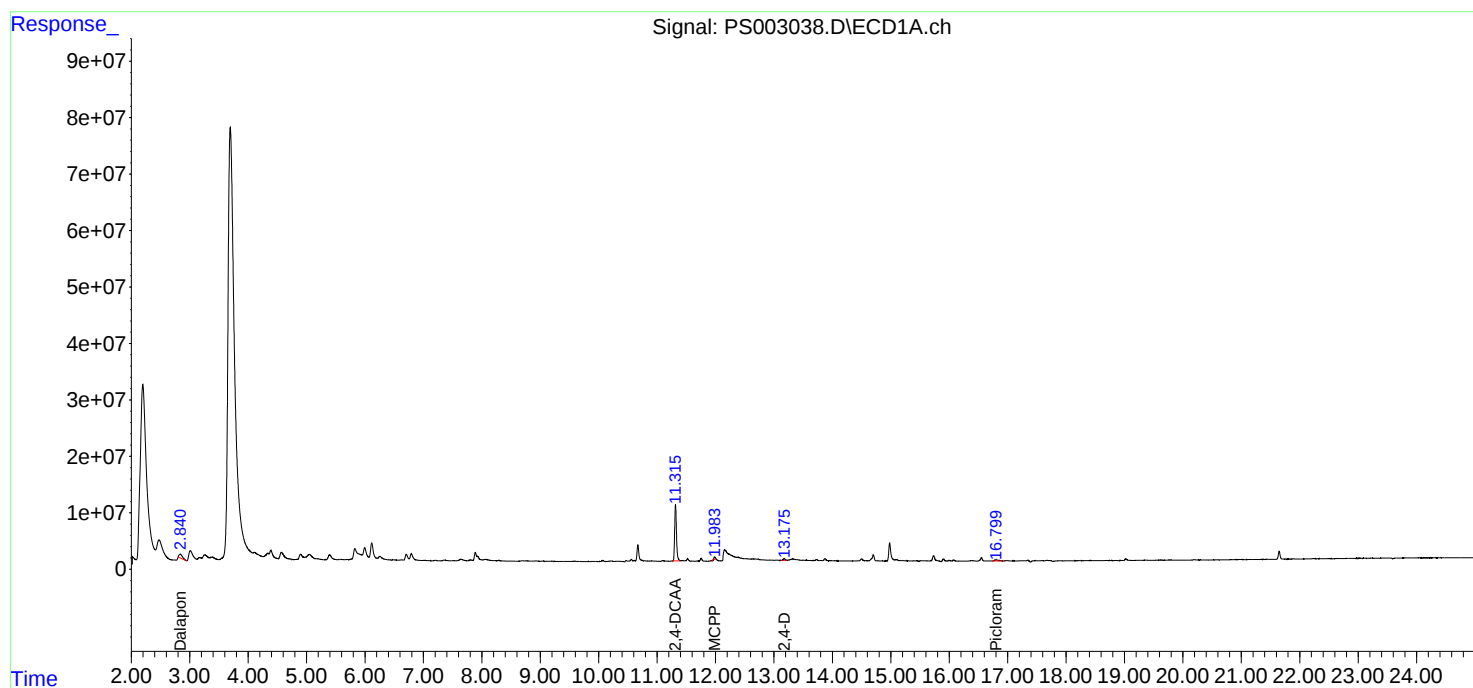


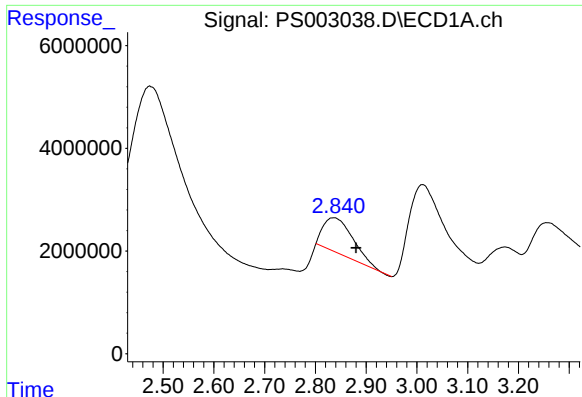

#1 Dalapon


R.T.: 2.836 min
Delta R.T.: -0.044 min
Response: 27490764
Conc: 49.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-B

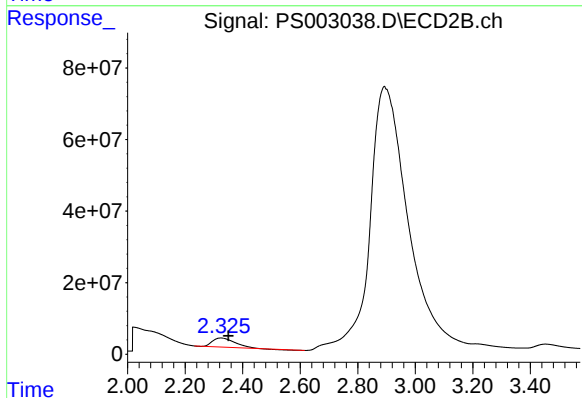


#1 Dalapon

R.T.: 2.325 min
Delta R.T.: -0.026 min
Response: 131547947
Conc: 245.46 ng/ml

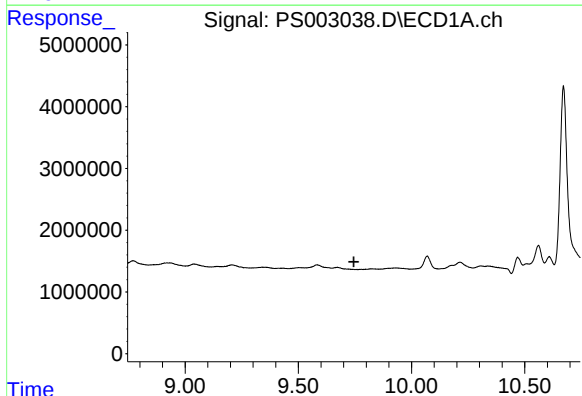


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

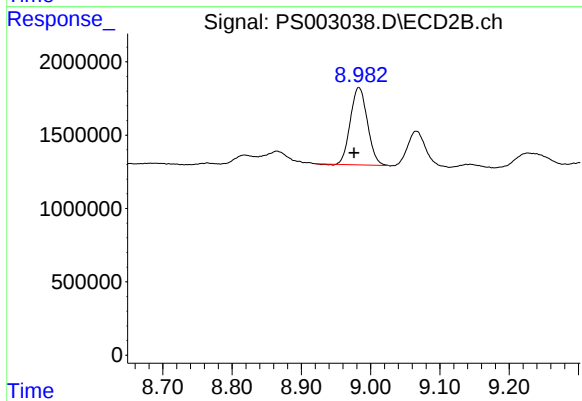

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.983 min
Delta R.T.: 0.007 min
Response: 9009886
Conc: 15.99 ng/ml

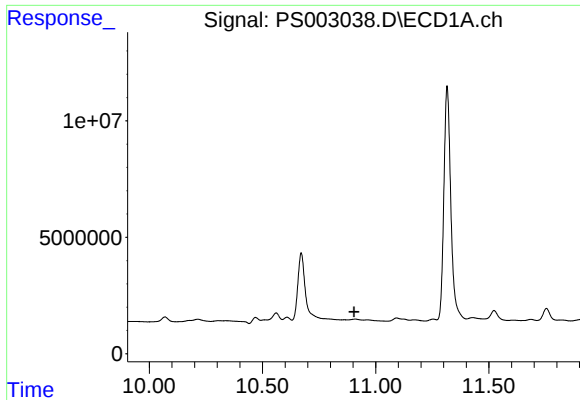

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-B

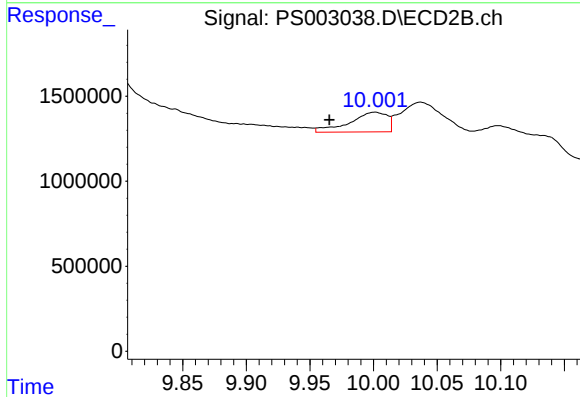


#3 4-Nitrophenol

R.T.: 10.001 min
Delta R.T.: 0.036 min
Response: 2392402
Conc: 11.45 ng/ml

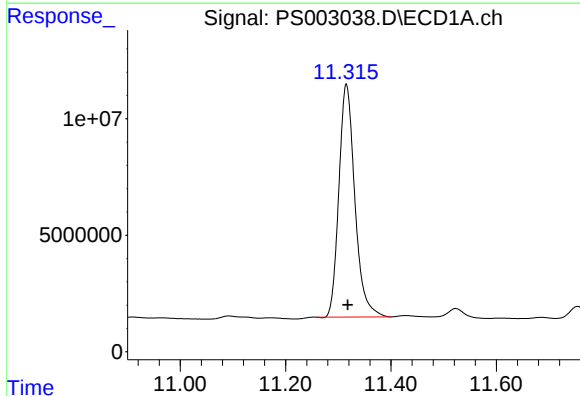


#4 2,4-DCAA

R.T.: 11.316 min
Delta R.T.: -0.002 min
Response: 210394355
Conc: 554.19 ng/ml

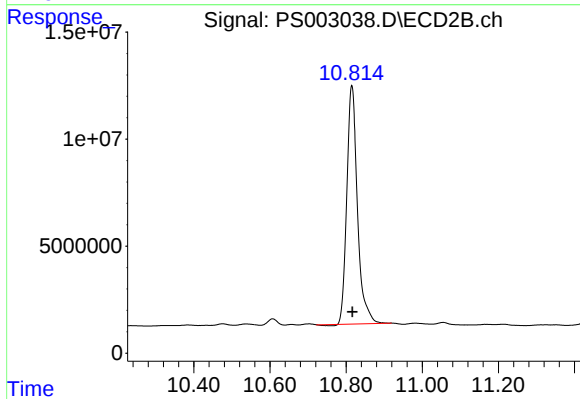

#4 2,4-DCAA


R.T.: 10.815 min
Delta R.T.: -0.002 min
Response: 216096033
Conc: 505.43 ng/ml

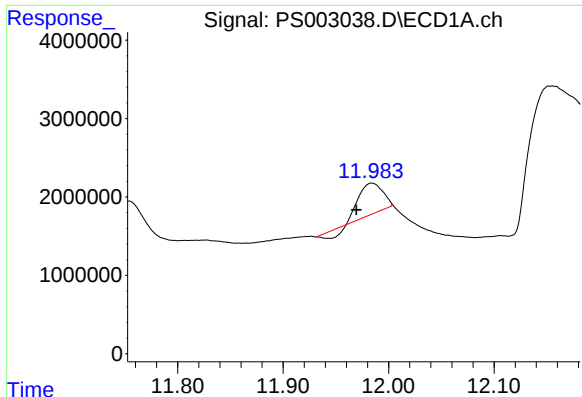

#6 MCP


R.T.: 11.985 min
Delta R.T.: 0.015 min
Response: 6108150
Conc: 5.10 ug/ml

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-B

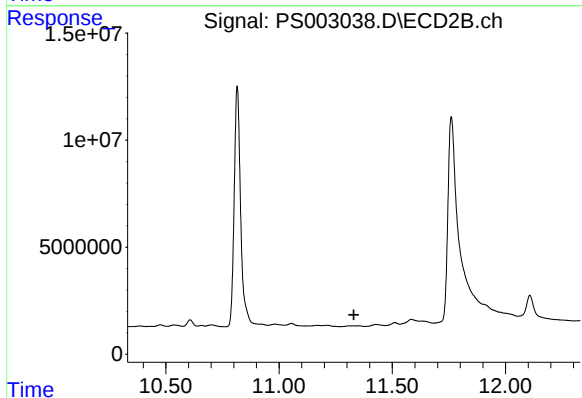


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

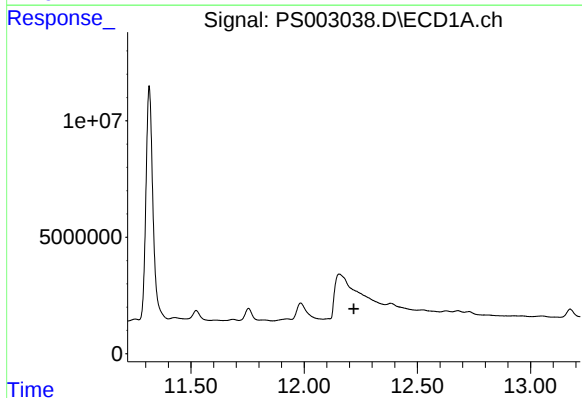


#7 MCP

R.T.: 12.156 min
Delta R.T.: -0.063 min
Response: -28285195
Conc: N.D.

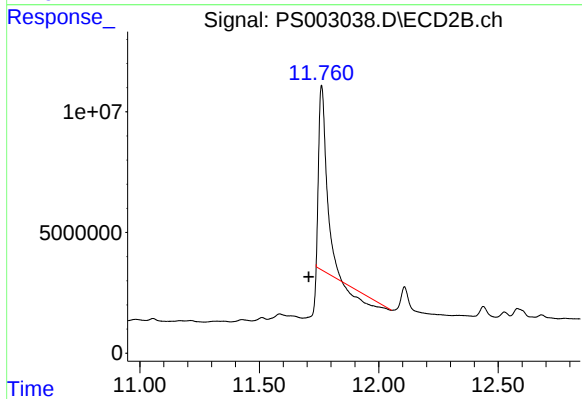

#7 MCP


R.T.: 11.761 min
Delta R.T.: 0.055 min
Response: 155801793
Conc: 99.04 ug/ml

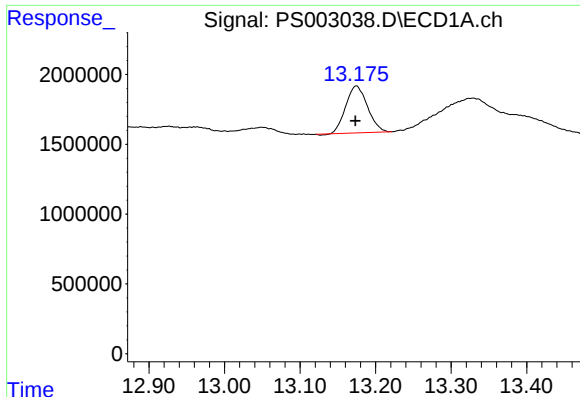

#9 2,4-D


R.T.: 13.175 min
Delta R.T.: 0.001 min
Response: 6713862
Conc: 14.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-B

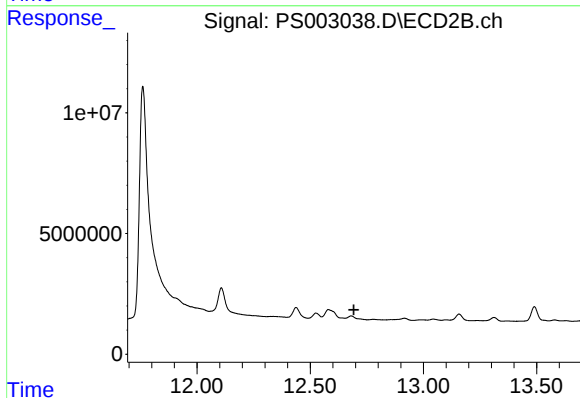


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

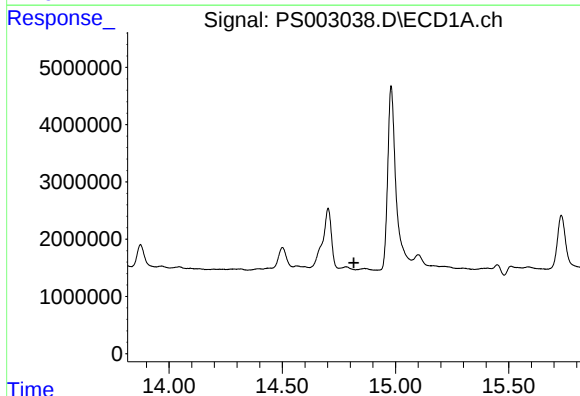


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

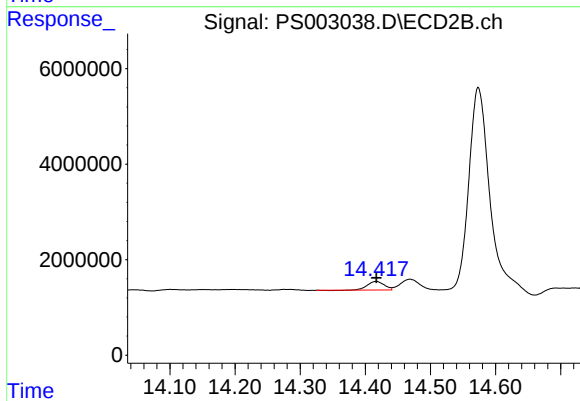

#12 2,4,5-T


R.T.: 14.417 min
Delta R.T.: 0.000 min
Response: 3287238
Conc: 1.72 ng/ml

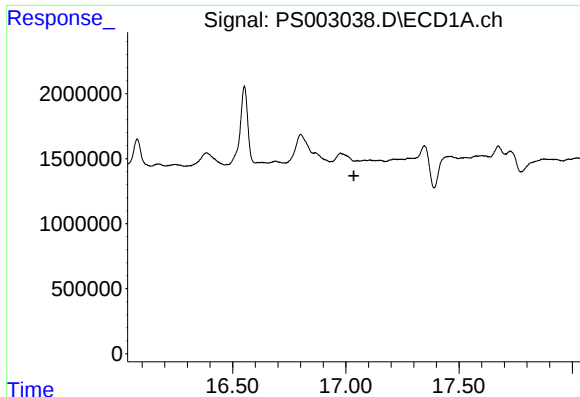

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-B

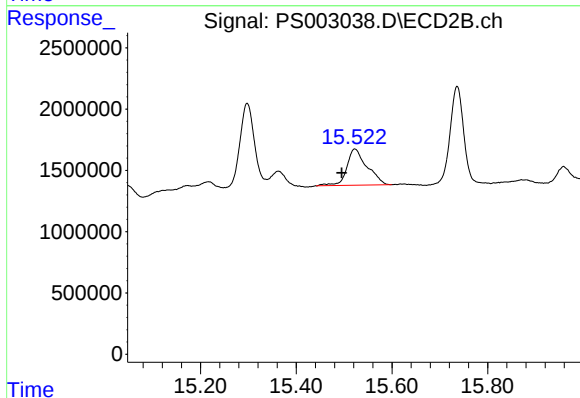


#14 DINOSEB

R.T.: 15.523 min
Delta R.T.: 0.028 min
Response: 8666420
Conc: 4.94 ng/ml

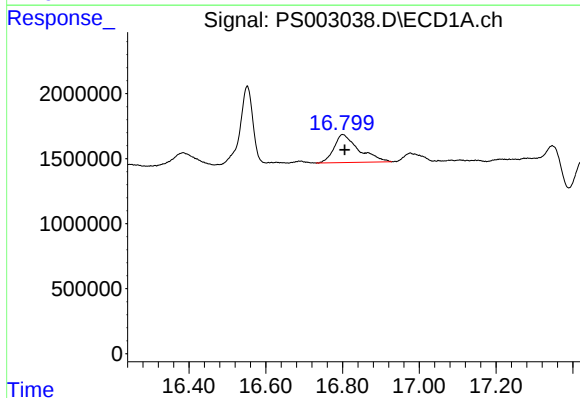


#15 Picloram

R.T.: 16.801 min
Delta R.T.: -0.005 min
Response: 9653928
Conc: 3.05 ng/ml

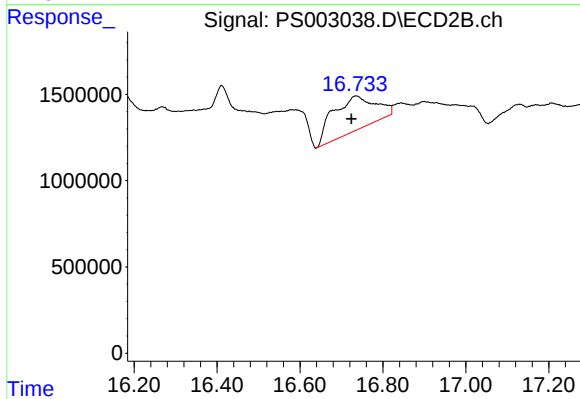

#15 Picloram


R.T.: 16.735 min
Delta R.T.: 0.011 min
Response: 14208584
Conc: 4.73 ng/ml

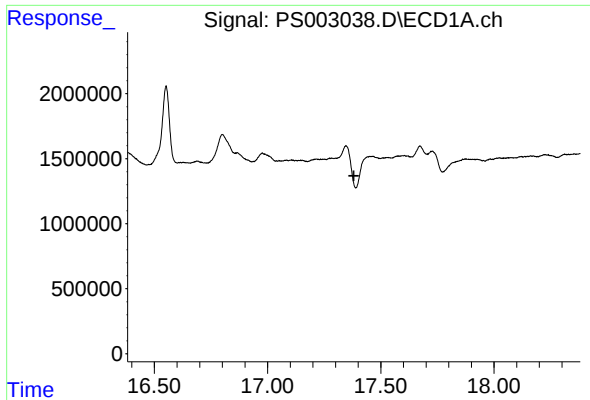

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-03-020419-B

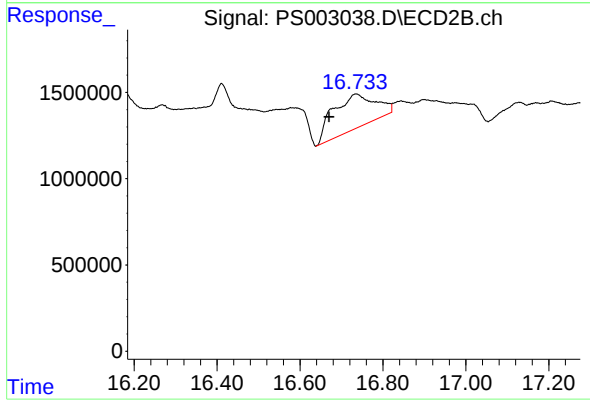

#16 DCPA

R.T.: 16.735 min
Delta R.T.: 0.065 min
Response: 14208584
Conc: 4.59 ng/ml