

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
 Data File : PS003043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2019 23:47
 Operator : EI\SJ
 Sample : PB116851TB
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116851TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:18:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.278	10.799	124.7E6	204.0E6	328.388	477.033 #
Target Compounds							
1) T	Dalapon	0.000	2.306	0	127.1E6	N.D.	237.237 #
2) T	3,5-DICHL...	0.000	8.966	0	7272565	N.D.	12.904 #
3) T	4-Nitroph...	0.000	10.020	0	6600518	N.D.	31.578 #
11) T	2,4,5-TP ...	14.463	0.000	9916982	0	3.938	N.D. #
12) T	2,4,5-T	0.000	14.401	0	3599286	N.D.	1.881 #
14) T	DINOSEB	0.000	15.517	0	13042840	N.D.	7.440 #
15) T	Picloram	16.756	16.719	14982537	12348045	4.736	4.107
16) T	DCPA	0.000	16.719	0	12348045	N.D.	3.986 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
Data File : PS003043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2019 23:47
Operator : EI\SJ
Sample : PB116851TB
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB116851TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:18:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

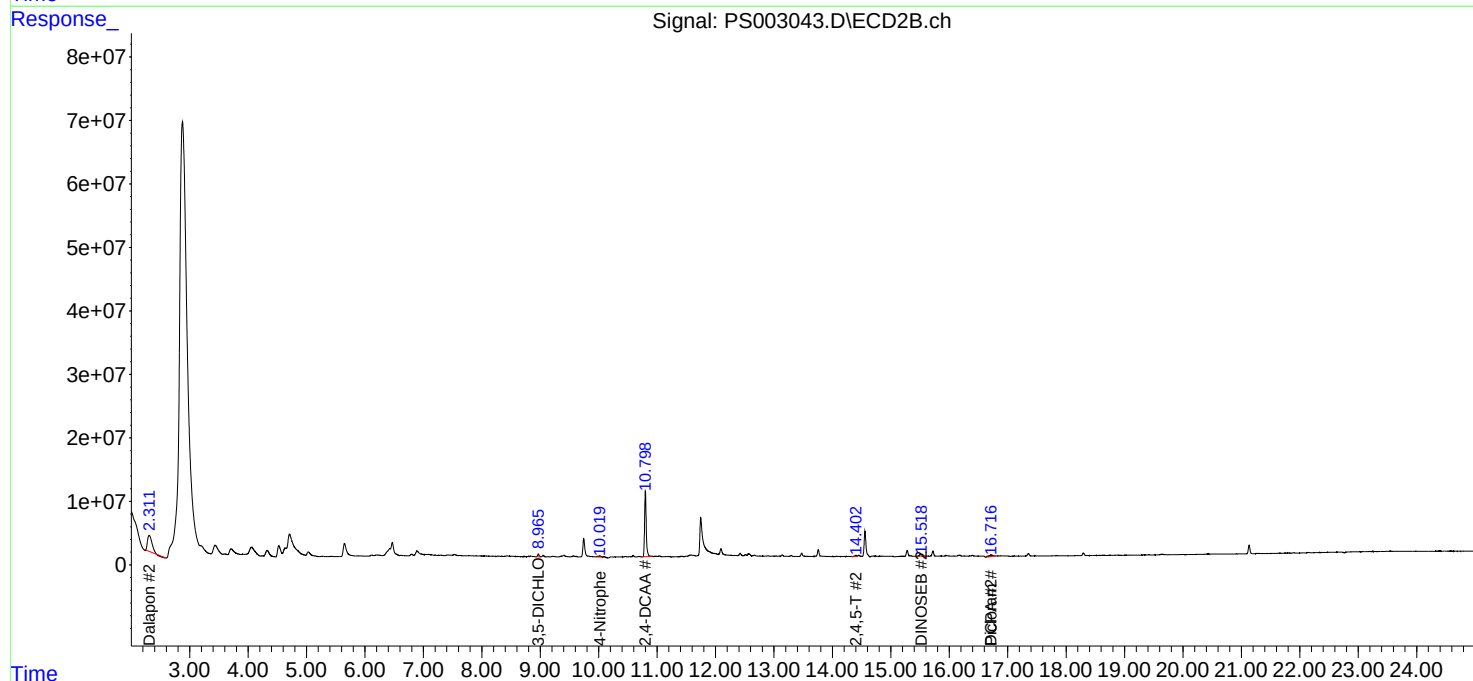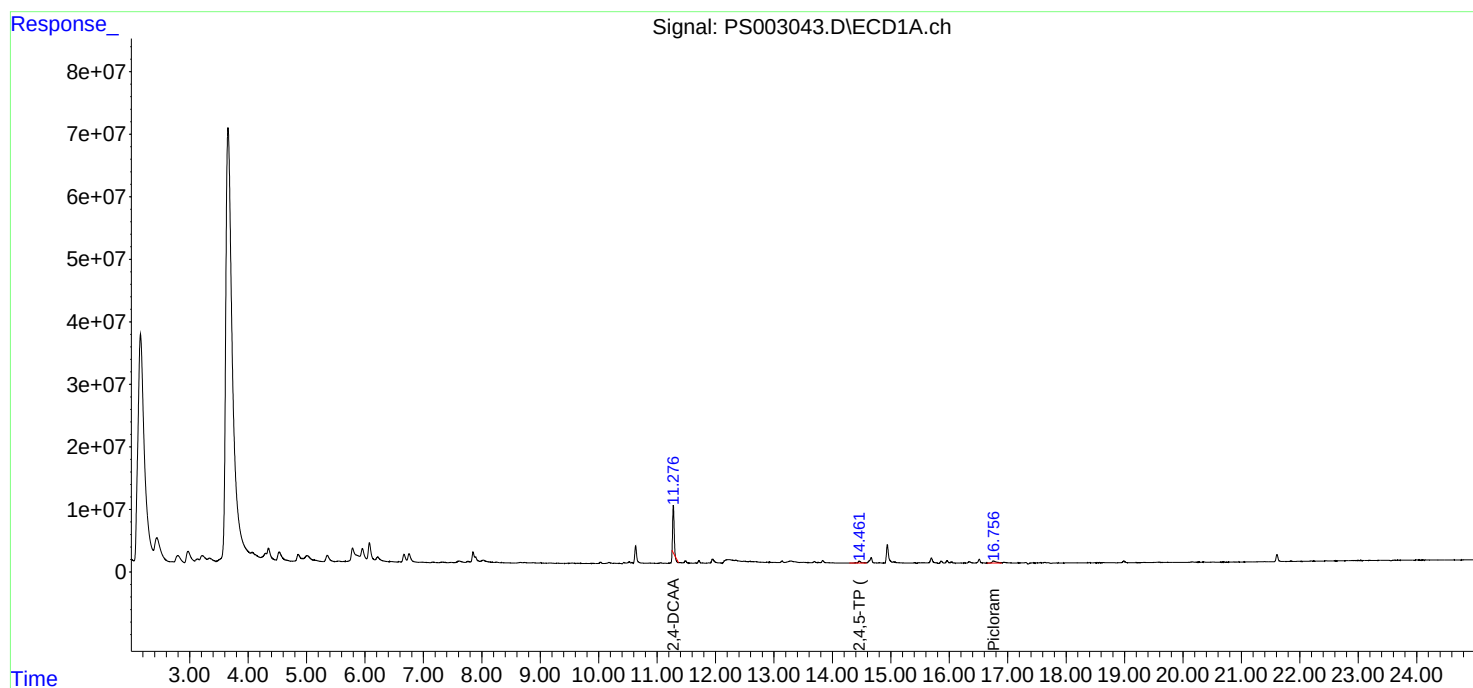


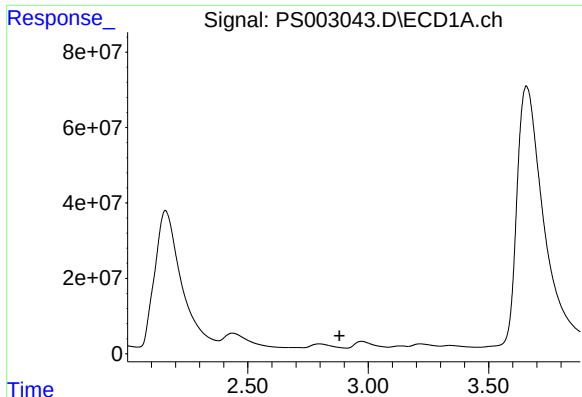

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116851TB

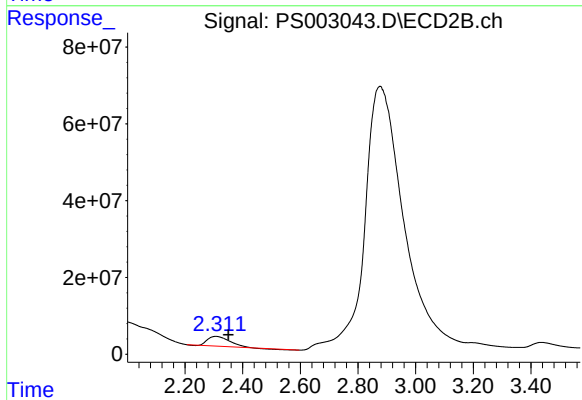


#1 Dalapon

R.T.: 2.306 min
Delta R.T.: -0.044 min
Response: 127140182
Conc: 237.24 ng/ml

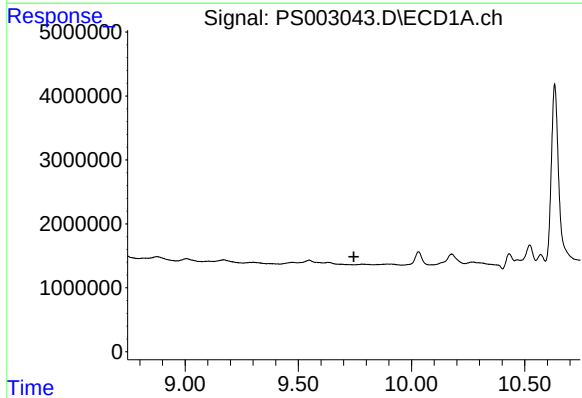


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

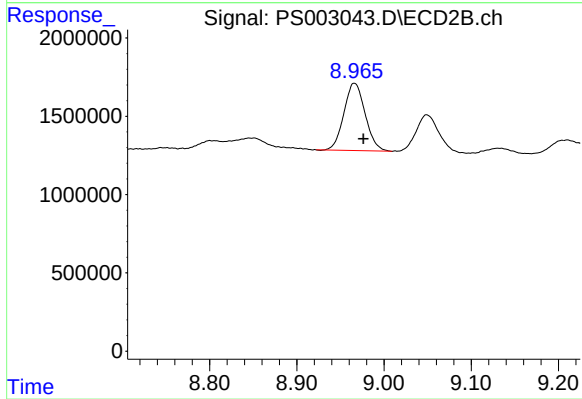

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.966 min
Delta R.T.: -0.010 min
Response: 7272565
Conc: 12.90 ng/ml

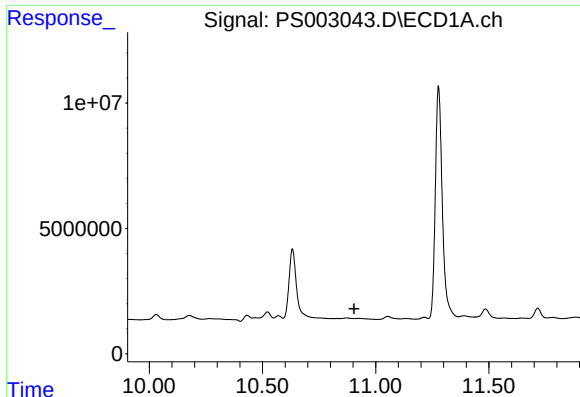

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116851TB

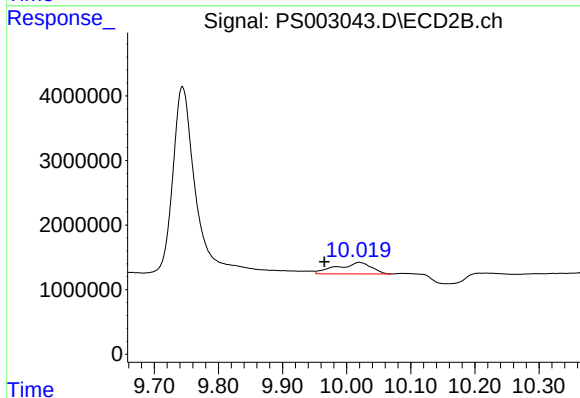


#3 4-Nitrophenol

R.T.: 10.020 min
Delta R.T.: 0.054 min
Response: 6600518
Conc: 31.58 ng/ml

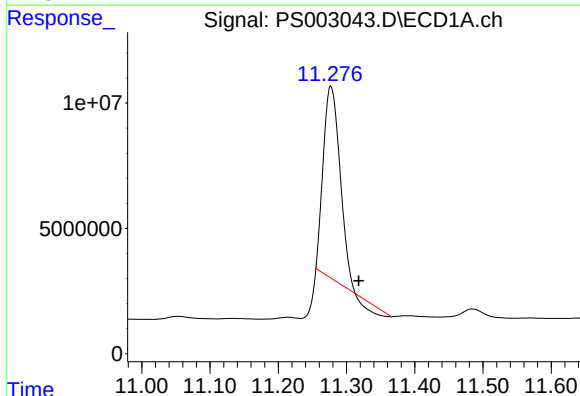


#4 2,4-DCAA

R.T.: 11.278 min
Delta R.T.: -0.040 min
Response: 124669355
Conc: 328.39 ng/ml

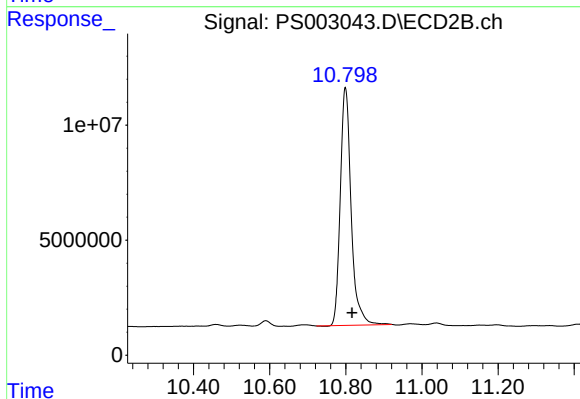

#4 2,4-DCAA


R.T.: 10.799 min
Delta R.T.: -0.018 min
Response: 203953299
Conc: 477.03 ng/ml

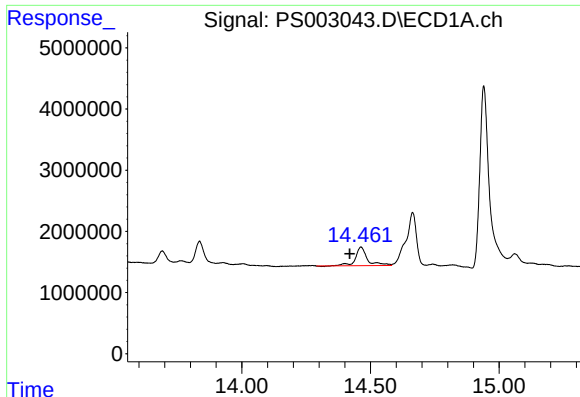

#11 2,4,5-TP (SILVEX)


R.T.: 14.463 min
Delta R.T.: 0.043 min
Response: 9916982
Conc: 3.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116851TB

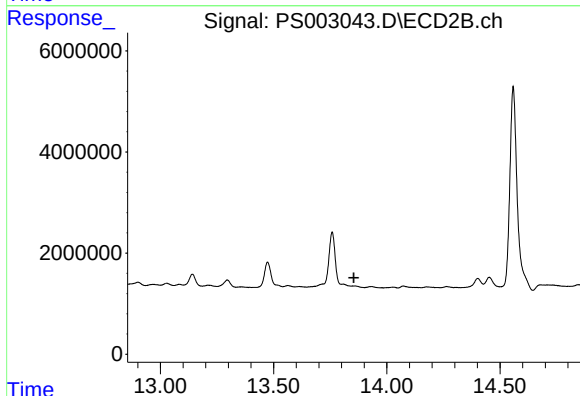


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

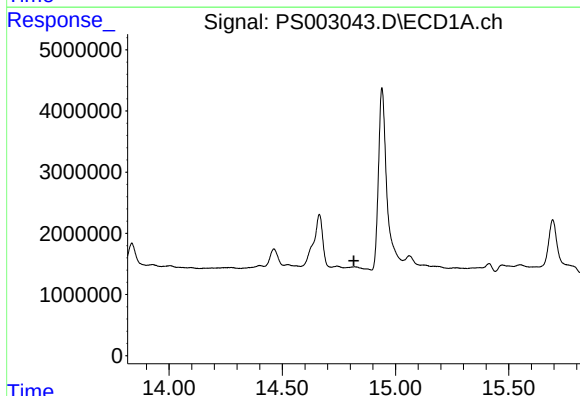


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

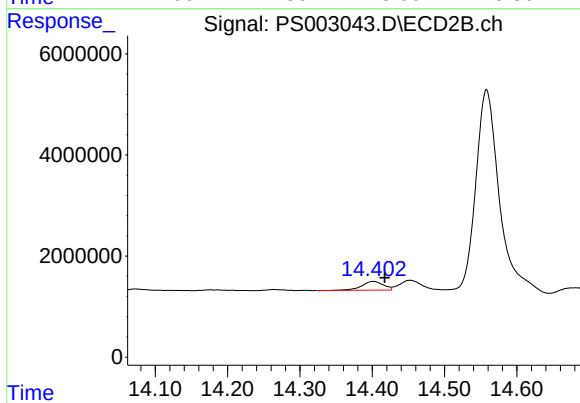

#12 2,4,5-T


R.T.: 14.401 min
Delta R.T.: -0.016 min
Response: 3599286
Conc: 1.88 ng/ml

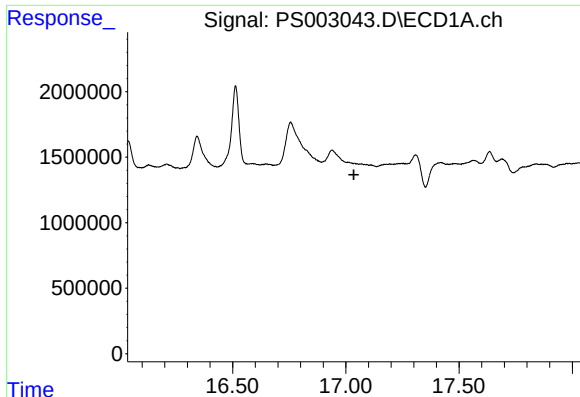

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116851TB

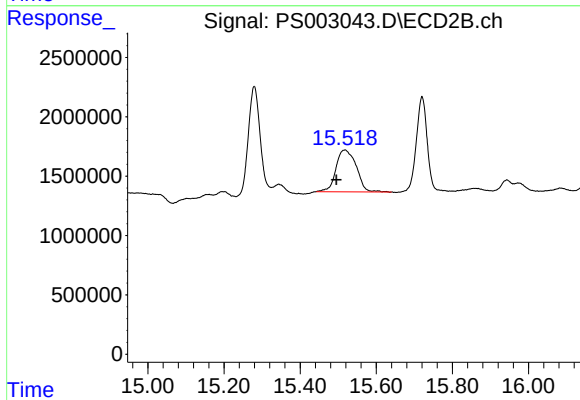


#14 DINOSEB

R.T.: 15.517 min
Delta R.T.: 0.022 min
Response: 13042840
Conc: 7.44 ng/ml

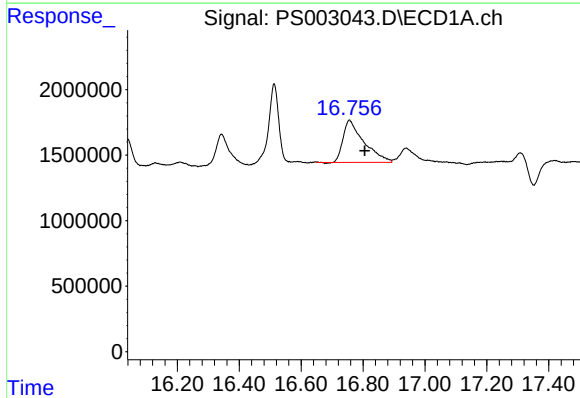


#15 Picloram

R.T.: 16.756 min
Delta R.T.: -0.049 min
Response: 14982537
Conc: 4.74 ng/ml

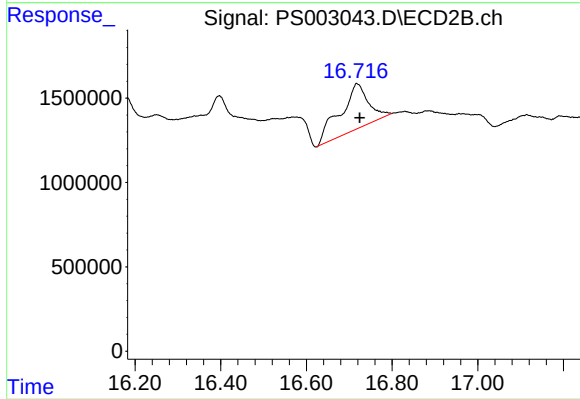

#15 Picloram


R.T.: 16.719 min
Delta R.T.: -0.005 min
Response: 12348045
Conc: 4.11 ng/ml

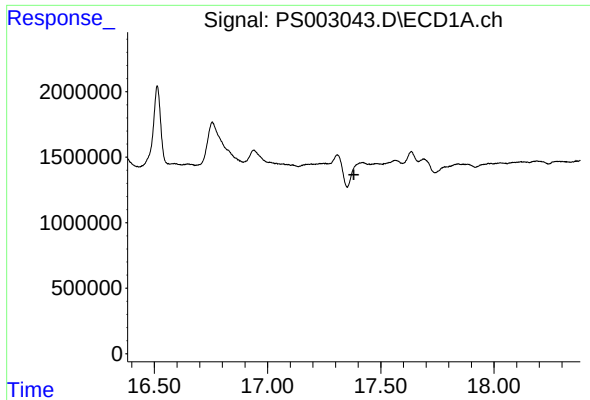

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116851TB

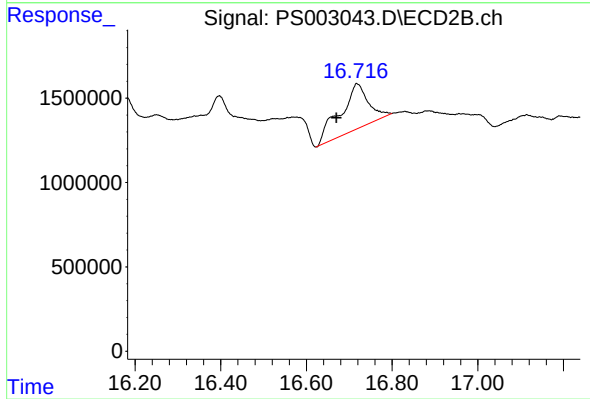

#16 DCPA

R.T.: 16.719 min
Delta R.T.: 0.049 min
Response: 12348045
Conc: 3.99 ng/ml