

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
 Data File : PS003044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 00:18
 Operator : EI\SJ
 Sample : K1341-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HR-05-020419-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 02:12:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.294	10.794	177.7E6	183.2E6	467.982	428.473
Target Compounds							
1) T	Dalapon	0.000	2.299	0 47414390		N.D.	88.473 #
2) T	3,5-DICHL...	0.000	8.962	0 11158891		N.D.	19.800 #
3) T	4-Nitroph...	0.000	9.980	0 2756205		N.D.	13.186 #
6) T	MCP	11.963	0.000	14252369	0	11.896	N.D. #
9) T	2,4-D	13.152	0.000	4167668	0	9.039	N.D. #
11) T	2,4,5-TP ...	14.478	0.000	7395992	0	2.937	N.D. #
12) T	2,4,5-T	0.000	14.395	0 2843462		N.D.	1.486 #
14) T	DINOSEB	0.000	15.501	0 6783462		N.D.	3.870 #
15) T	Picloram	16.784	16.713	8639335 11008068		2.731	3.662 #
16) T	DCPA	17.438	16.713	-5435581 11008068		N.D.	3.554



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
Data File : PS003044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 00:18
Operator : EI\SJ
Sample : K1341-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 02:12:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

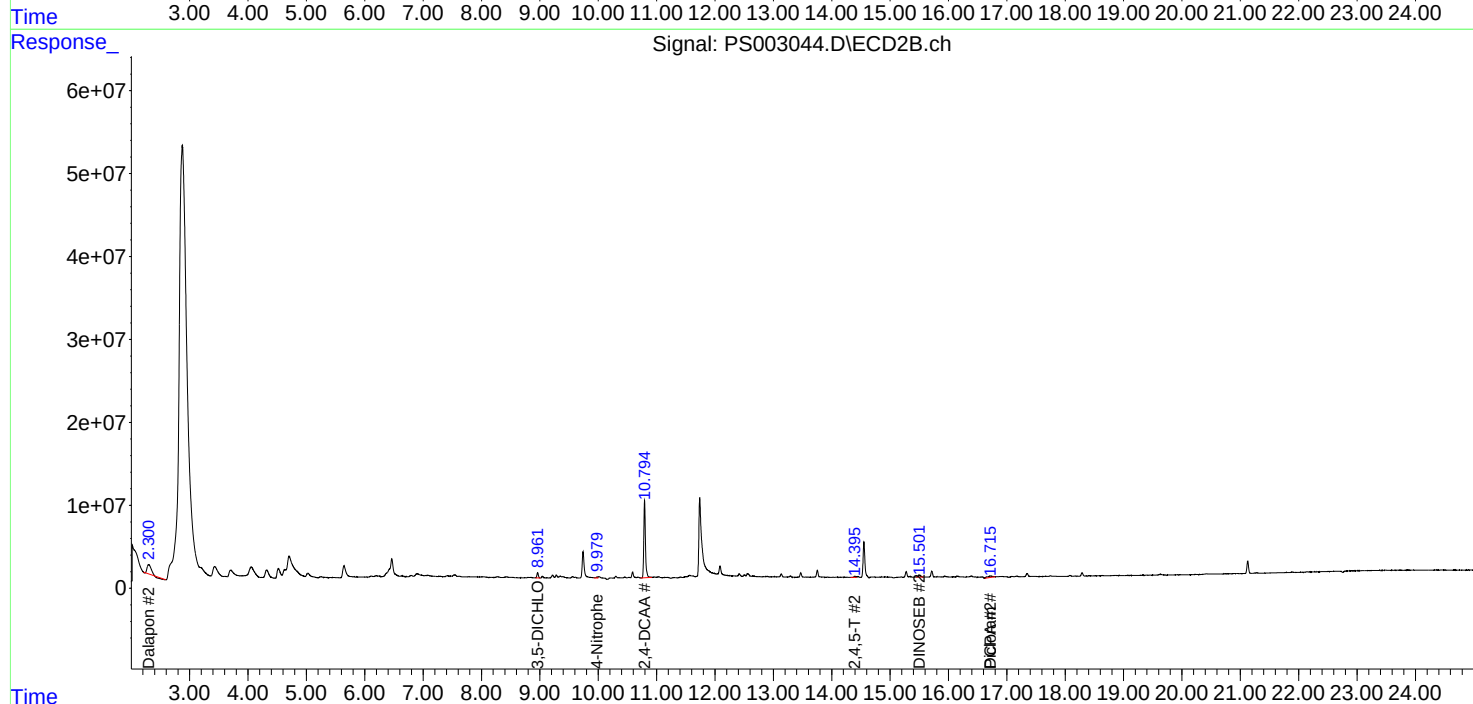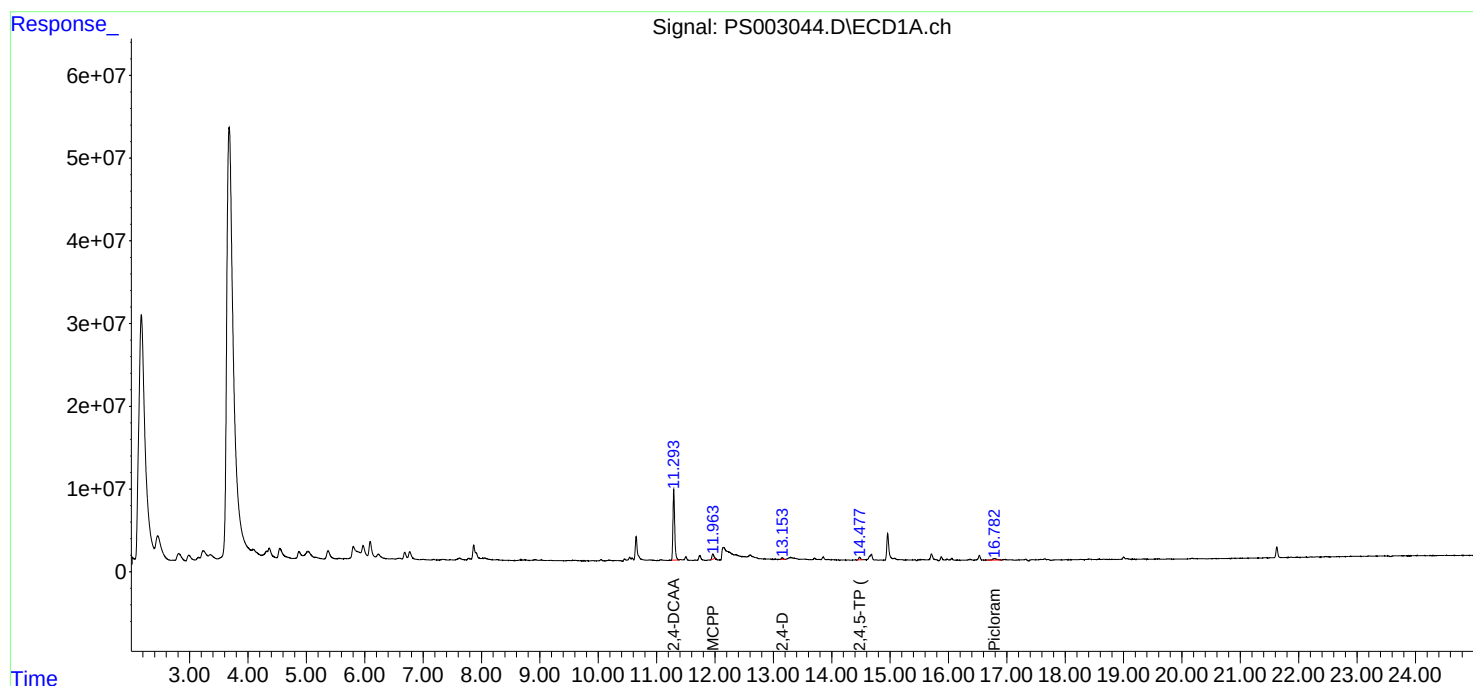


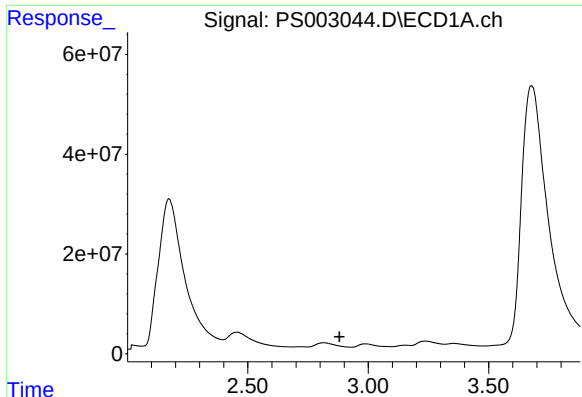

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-A

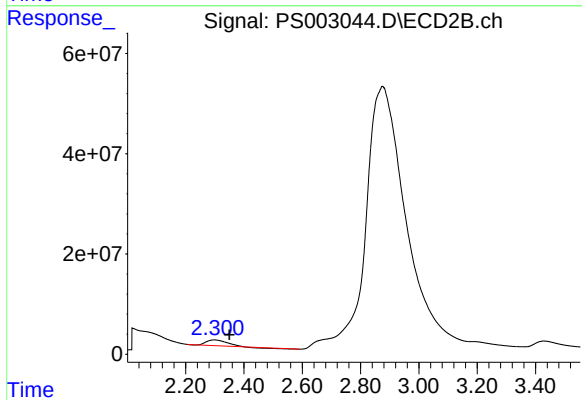


#1 Dalapon

R.T.: 2.299 min
Delta R.T.: -0.052 min
Response: 47414390
Conc: 88.47 ng/ml

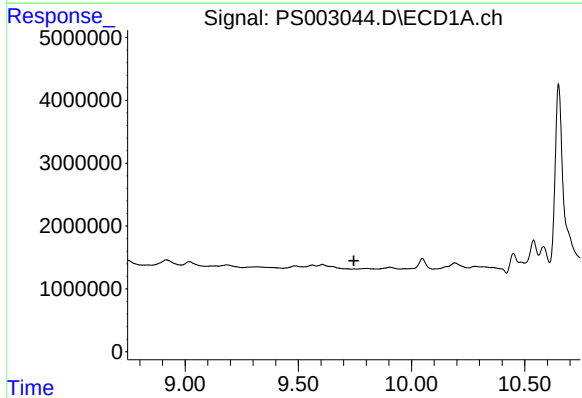


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

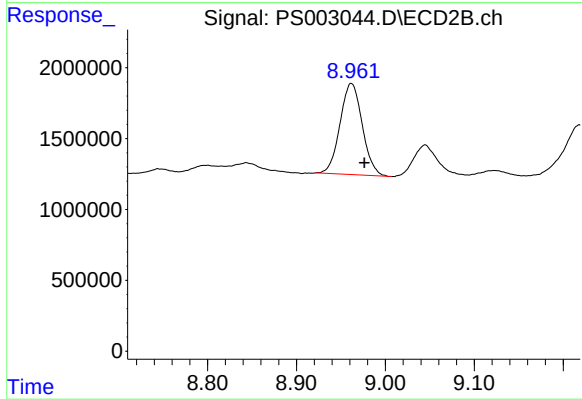

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.962 min
Delta R.T.: -0.015 min
Response: 11158891
Conc: 19.80 ng/ml

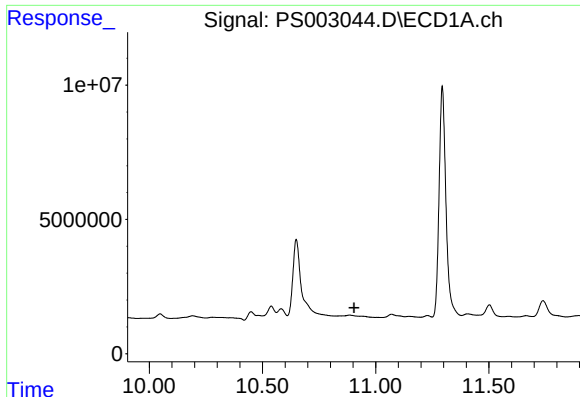

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-A

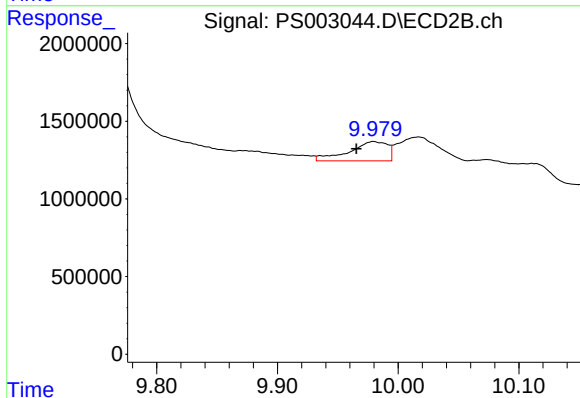


#3 4-Nitrophenol

R.T.: 9.980 min
Delta R.T.: 0.015 min
Response: 2756205
Conc: 13.19 ng/ml

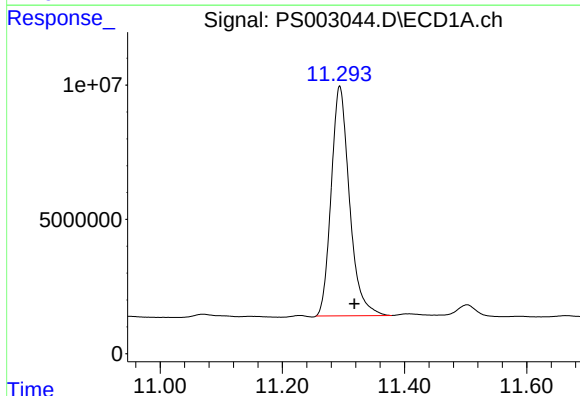


#4 2,4-DCAA

R.T.: 11.294 min
Delta R.T.: -0.024 min
Response: 177665088
Conc: 467.98 ng/ml

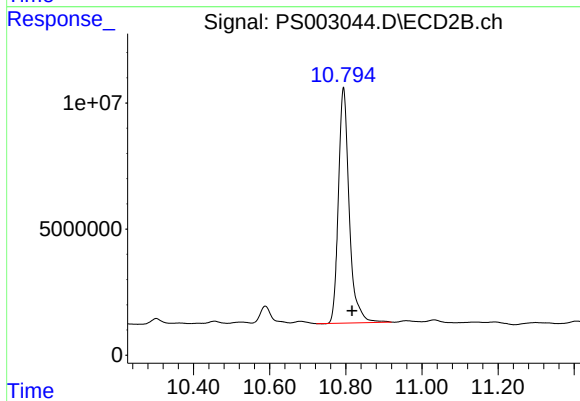

#4 2,4-DCAA


R.T.: 10.794 min
Delta R.T.: -0.023 min
Response: 183191874
Conc: 428.47 ng/ml

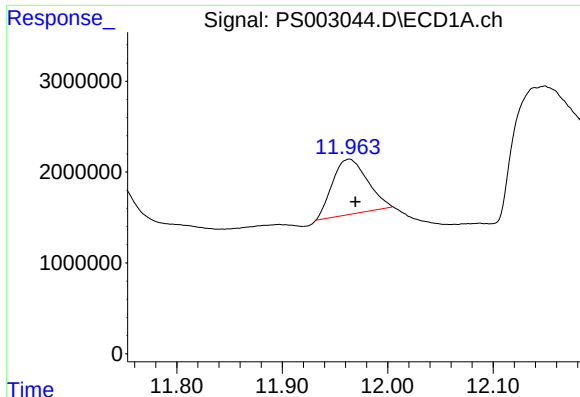

#6 MCP


R.T.: 11.963 min
Delta R.T.: -0.006 min
Response: 14252369
Conc: 11.90 ug/ml

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-A

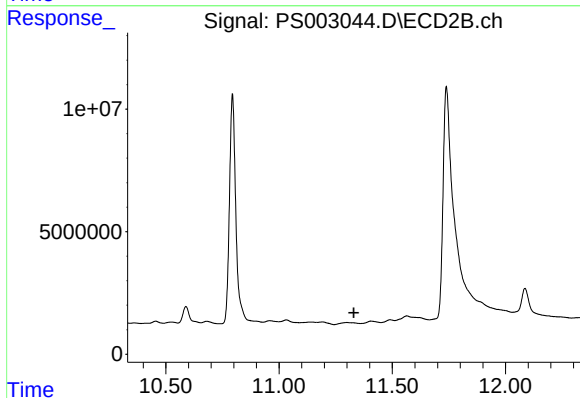


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

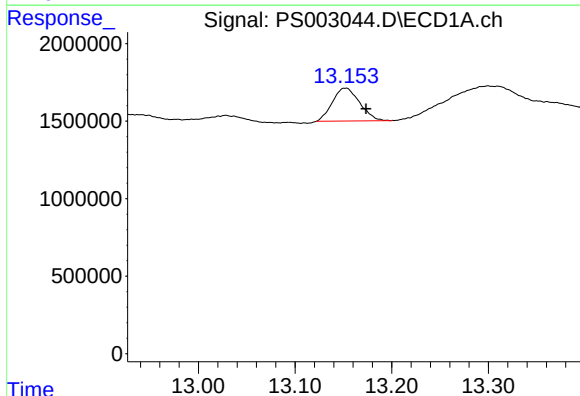


#9 2,4-D

R.T.: 13.152 min
Delta R.T.: -0.021 min
Response: 4167668
Conc: 9.04 ng/ml

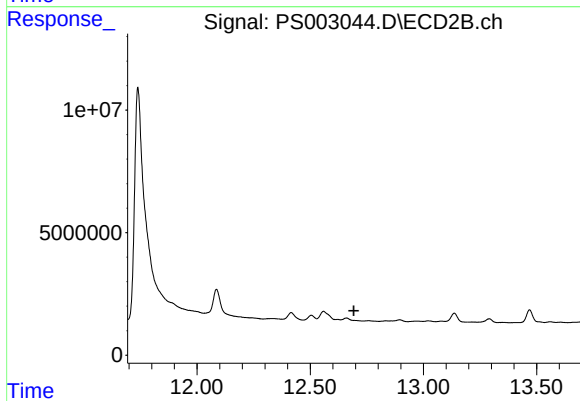

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

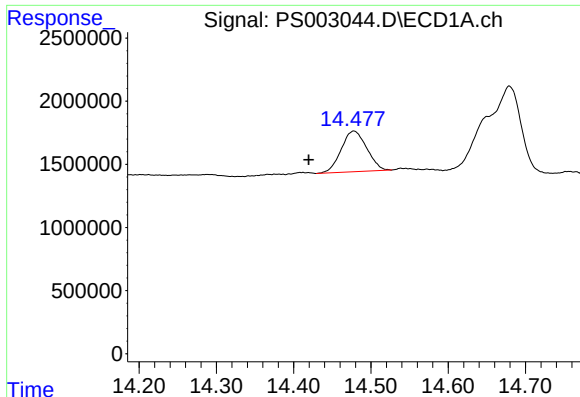

#11 2,4,5-TP (SILVEX)


R.T.: 14.478 min
Delta R.T.: 0.058 min
Response: 7395992
Conc: 2.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-A

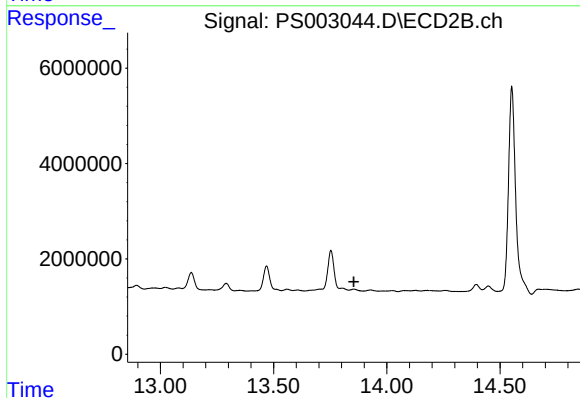


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

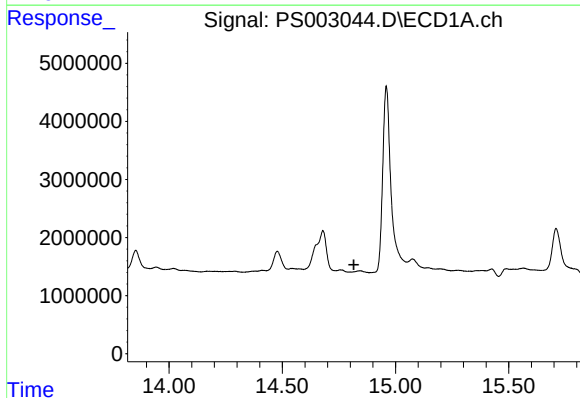


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

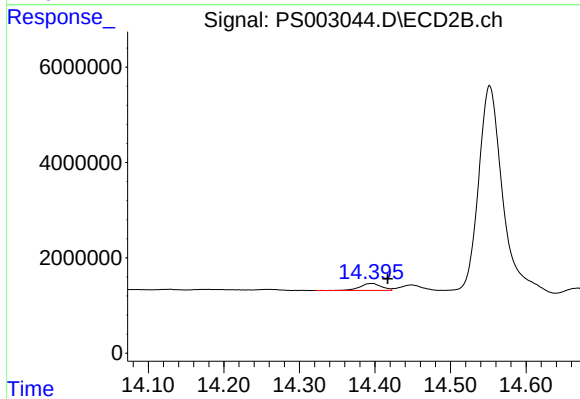

#12 2,4,5-T


R.T.: 14.395 min
Delta R.T.: -0.022 min
Response: 2843462
Conc: 1.49 ng/ml

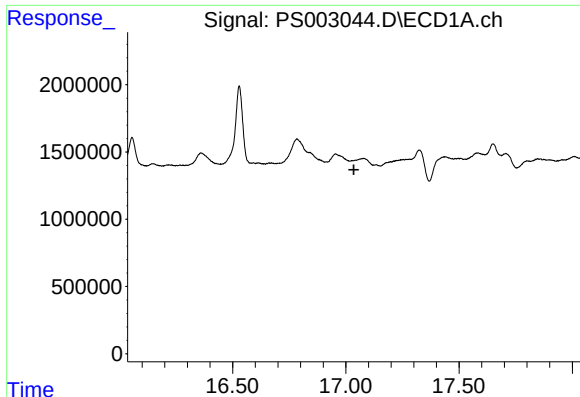

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-A

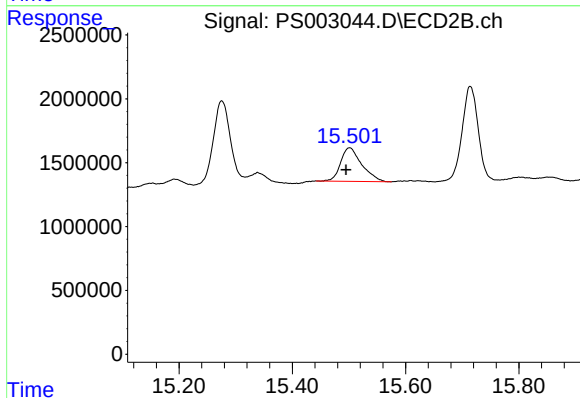


#14 DINOSEB

R.T.: 15.501 min
Delta R.T.: 0.006 min
Response: 6783462
Conc: 3.87 ng/ml

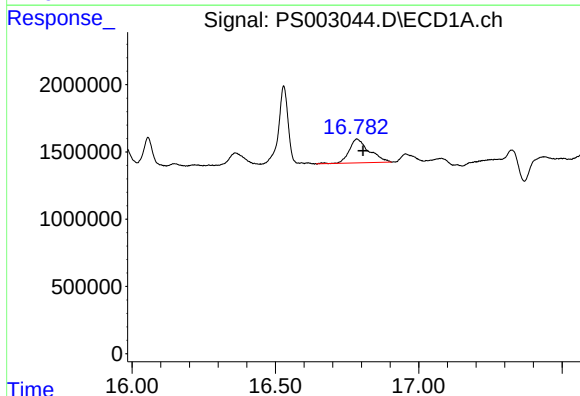


#15 Picloram

R.T.: 16.784 min
Delta R.T.: -0.022 min
Response: 8639335
Conc: 2.73 ng/ml

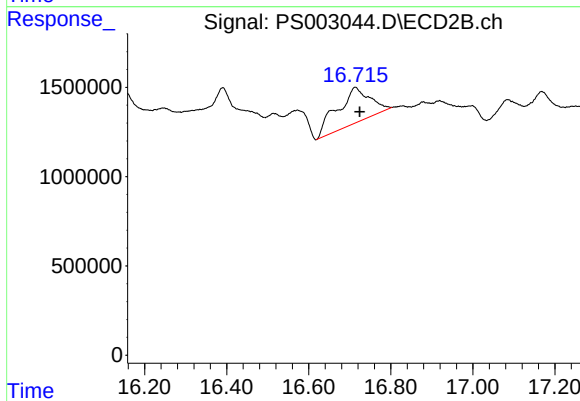

#15 Picloram


R.T.: 16.713 min
Delta R.T.: -0.011 min
Response: 11008068
Conc: 3.66 ng/ml

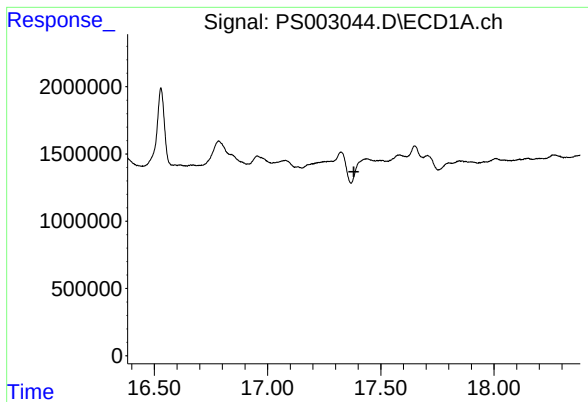

#16 DCPA

R.T.: 17.438 min
Delta R.T.: 0.056 min
Response: -5435581
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-A

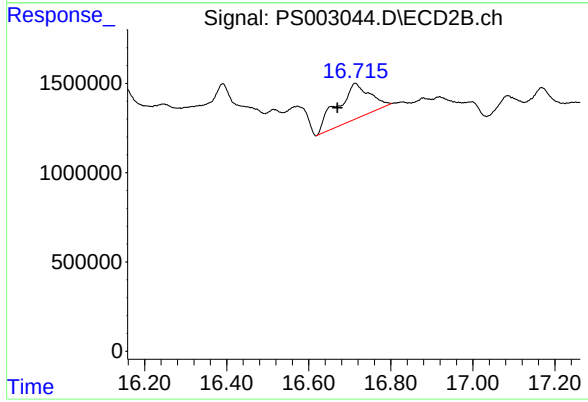

#16 DCPA

R.T.: 16.713 min
Delta R.T.: 0.044 min
Response: 11008068
Conc: 3.55 ng/ml