

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
 Data File : PS003047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 01:51
 Operator : EI\SJ
 Sample : K1341-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HR-05-020419-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 02:16:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.759	0	205.1E6	N.D.	479.818 #
Target Compounds							
3) T	4-Nitroph...	0.000	9.980	0	3295804	N.D.	15.768 #
5) T	DICAMBA	11.628	0.000	1643715	0	1.025	N.D. #
7) T	MCPA	0.000	11.702	0	171.7E6	N.D.	109.123 #
10) T	Pentachlo...	0.000	13.255	0	2029419	N.D.	0.328 #
11) T	2,4,5-TP ...	14.444	0.000	10655362	0	4.231	N.D. #
12) T	2,4,5-T	0.000	14.410	0	5589967	N.D.	2.921 #
14) T	DINOSEB	0.000	15.472	0	9639638	N.D.	5.499 #
15) T	Picloram	16.744	16.674	13230440	16879802	4.182	5.615 #
16) T	DCPA	17.403	16.674	3166415	16879802	1.053	5.449 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020519\
Data File : PS003047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 01:51
Operator : EI\SJ
Sample : K1341-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 02:16:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

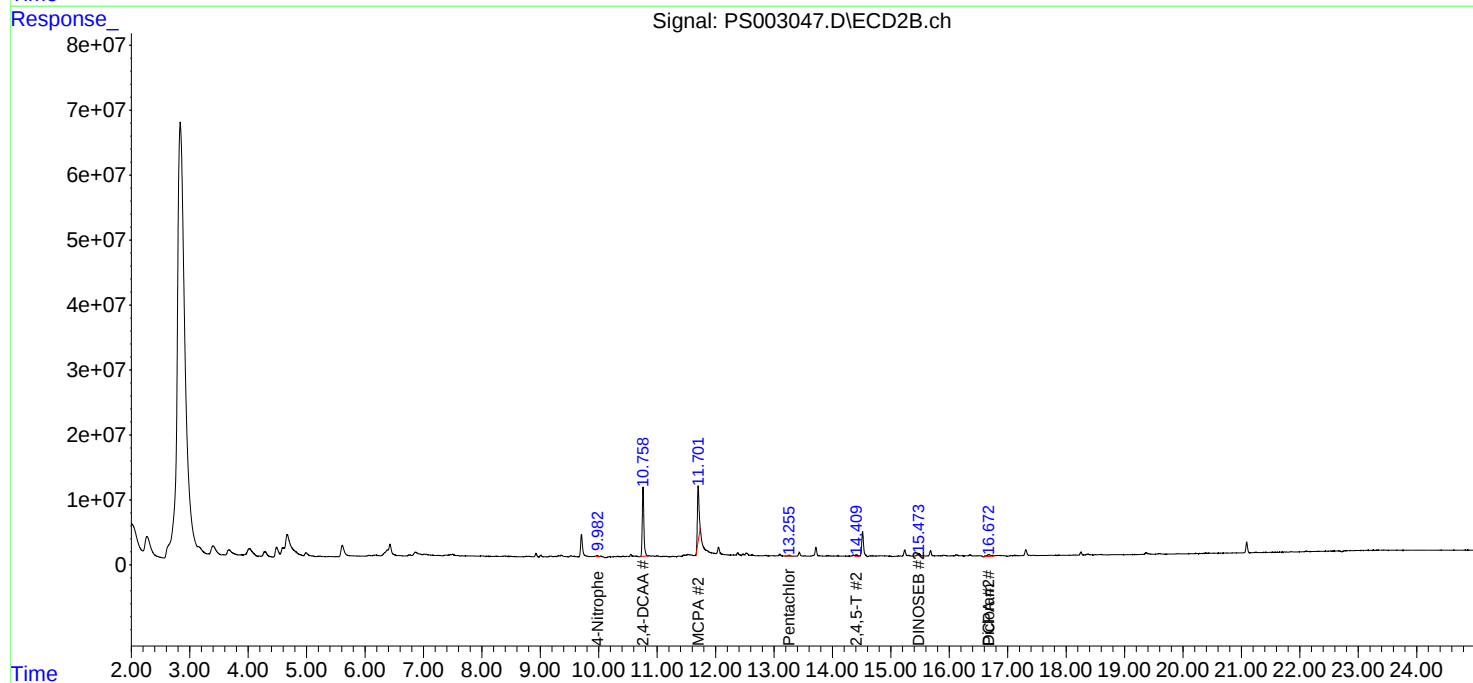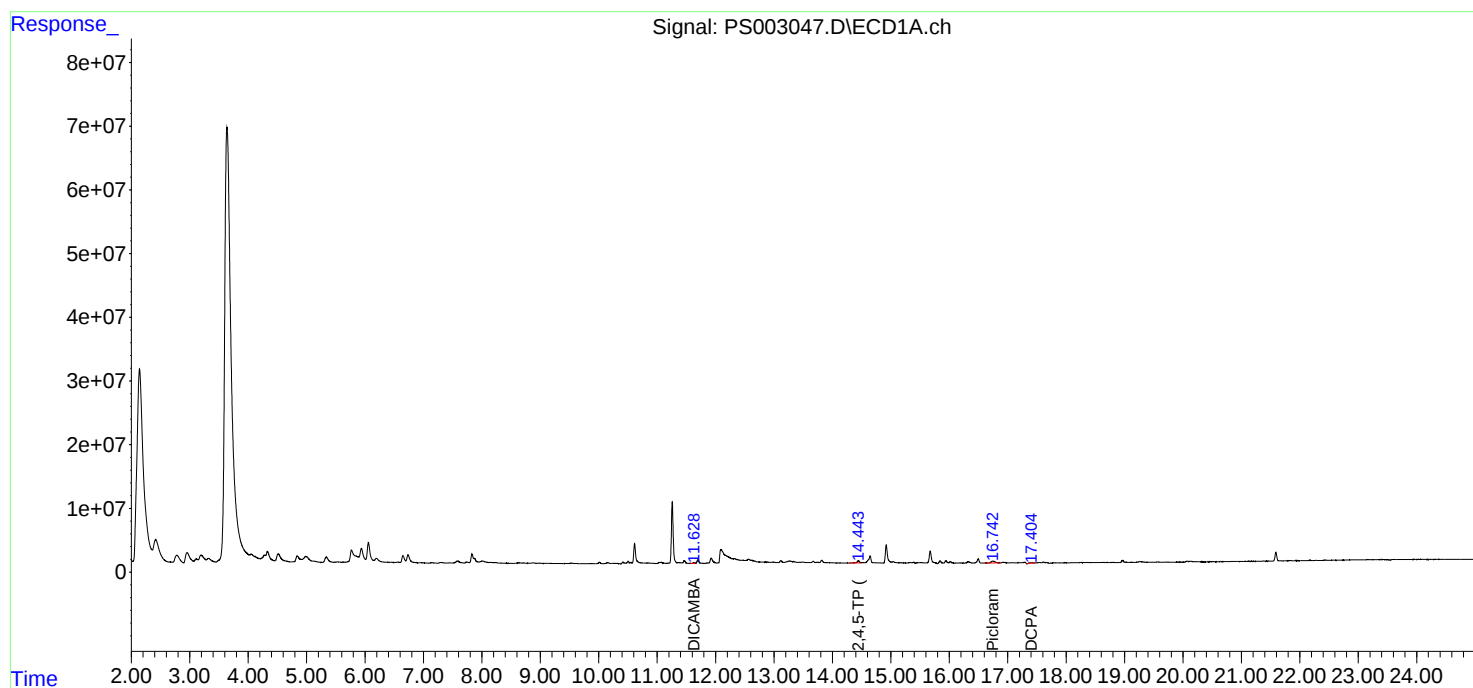


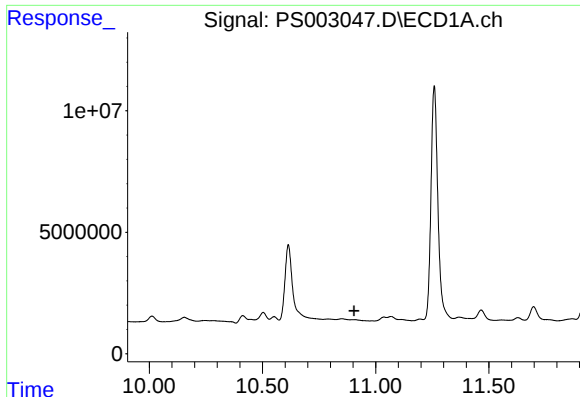

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-B

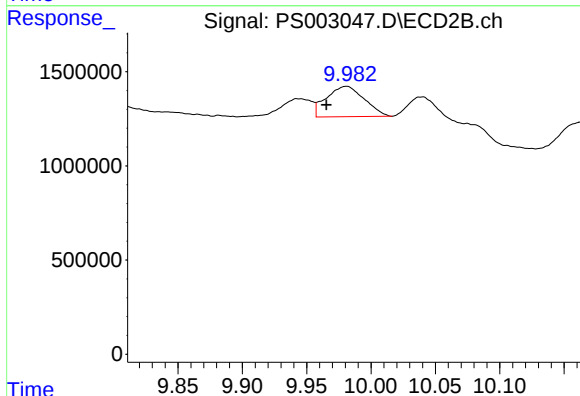


#3 4-Nitrophenol

R.T.: 9.980 min
Delta R.T.: 0.015 min
Response: 3295804
Conc: 15.77 ng/ml

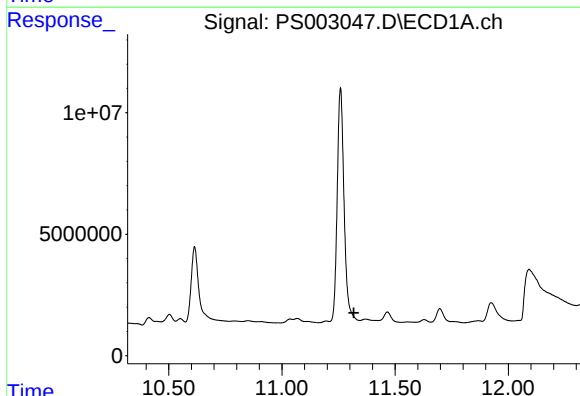


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

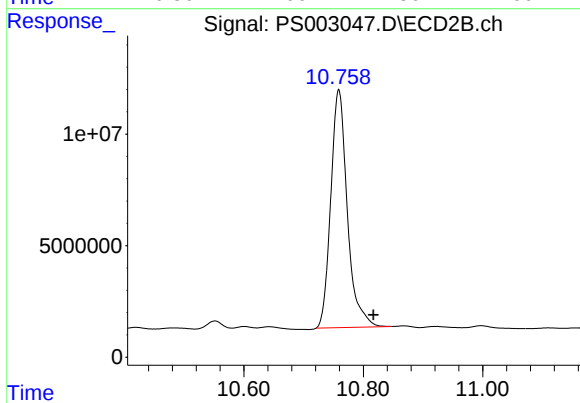

#4 2,4-DCAA


R.T.: 10.759 min
Delta R.T.: -0.058 min
Response: 205144096
Conc: 479.82 ng/ml

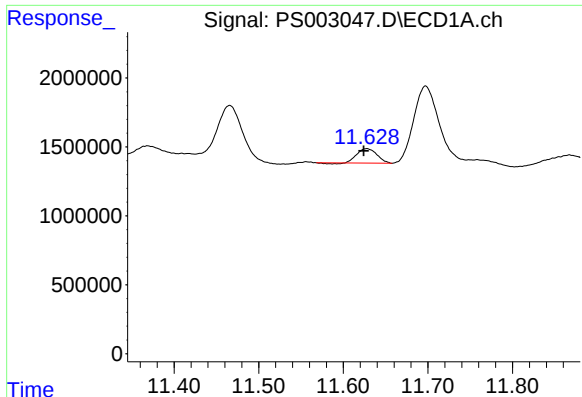

#5 DICAMBA


R.T.: 11.628 min
Delta R.T.: 0.004 min
Response: 1643715
Conc: 1.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-B

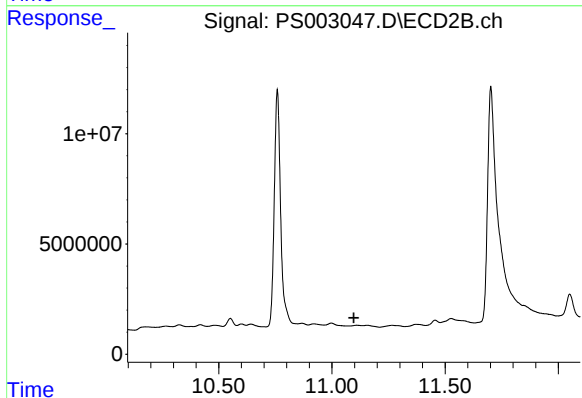


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.097 min
Response: 0
Conc: N.D.

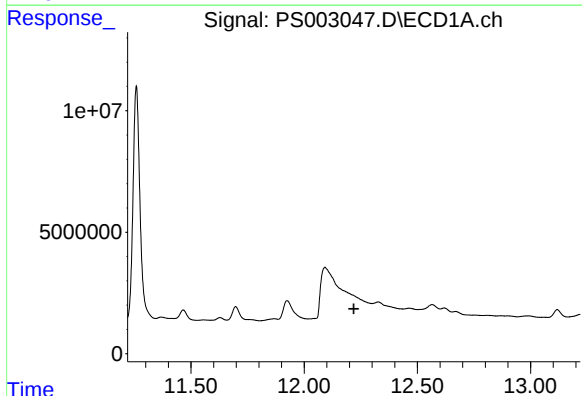


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.219 min
Response: 0
Conc: N.D.

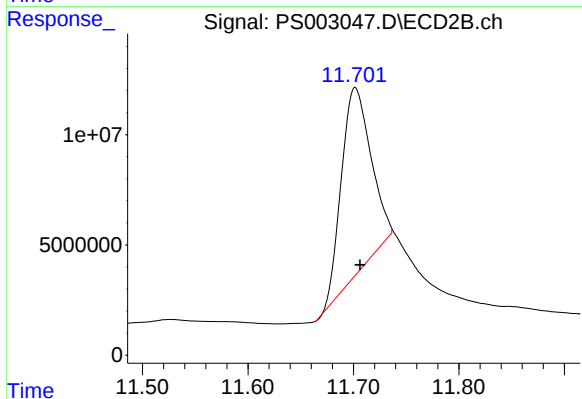

#7 MCPA


R.T.: 11.702 min
Delta R.T.: -0.004 min
Response: 171658131
Conc: 109.12 ug/ml

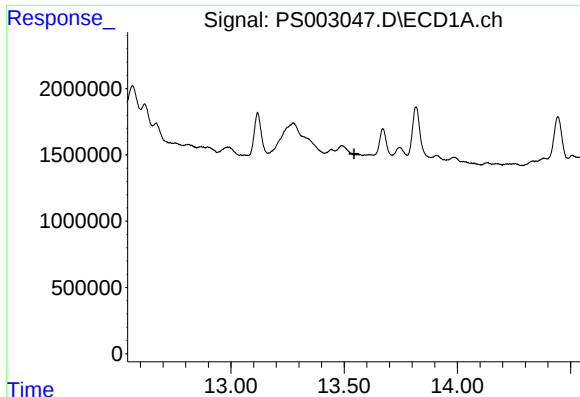

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-B

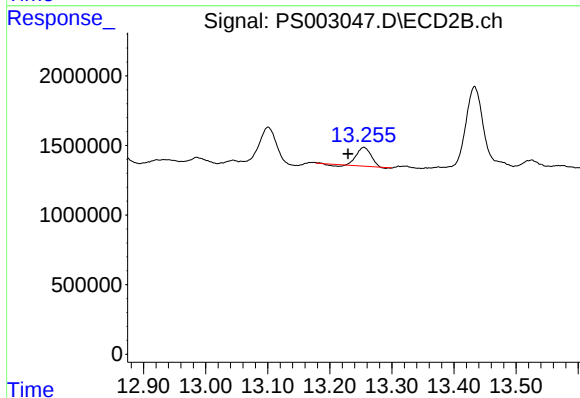


#10 Pentachlorophenol

R.T.: 13.255 min
Delta R.T.: 0.025 min
Response: 2029419
Conc: 0.33 ng/ml

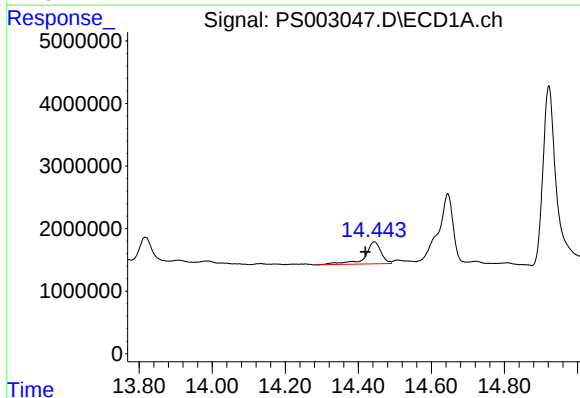


#11 2,4,5-TP (SILVEX)

R.T.: 14.444 min
Delta R.T.: 0.024 min
Response: 10655362
Conc: 4.23 ng/ml

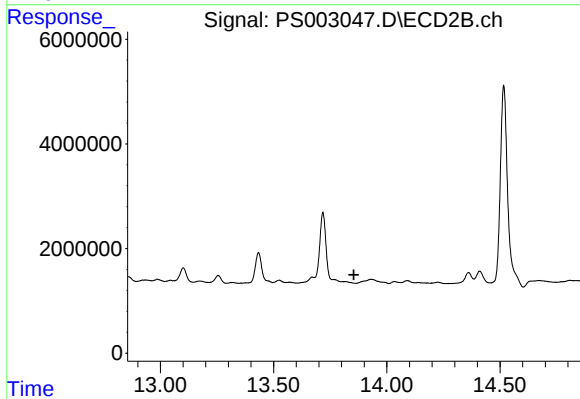

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.854 min
Response: 0
Conc: N.D.

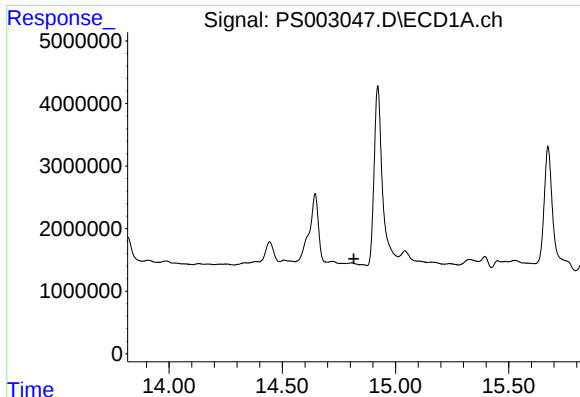

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-B

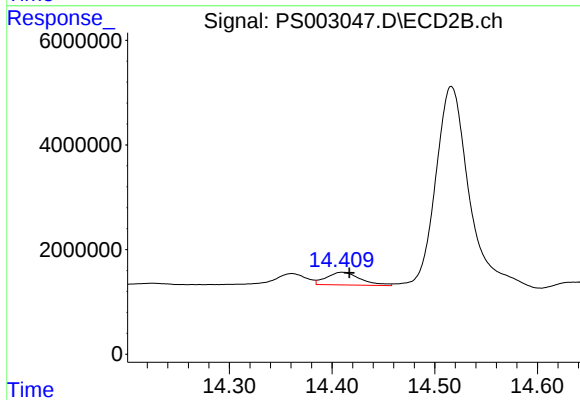


#12 2,4,5-T

R.T.: 14.410 min
Delta R.T.: -0.007 min
Response: 5589967
Conc: 2.92 ng/ml

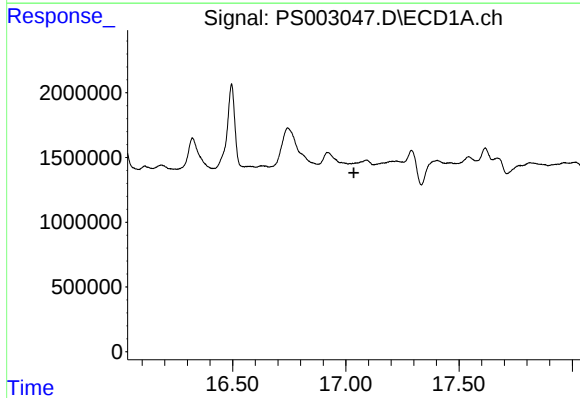


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

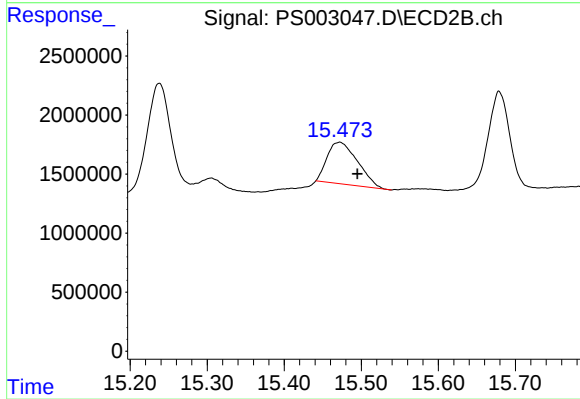

#14 DINOSEB


R.T.: 15.472 min
Delta R.T.: -0.023 min
Response: 9639638
Conc: 5.50 ng/ml

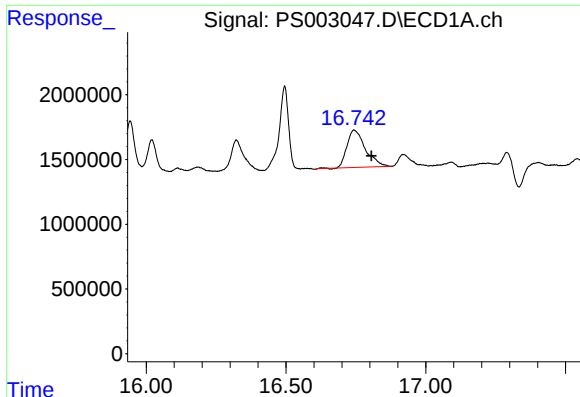

#15 Picloram


R.T.: 16.744 min
Delta R.T.: -0.061 min
Response: 13230440
Conc: 4.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
HR-05-020419-B

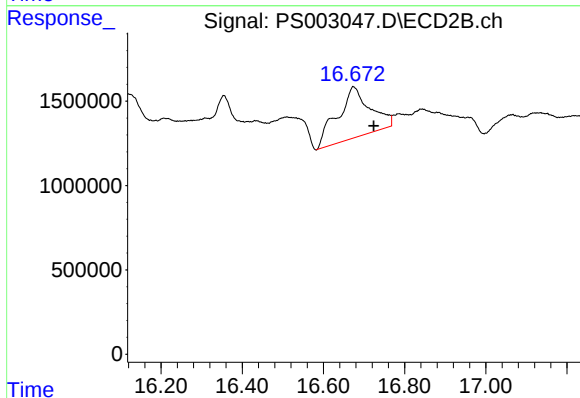


#15 Picloram

R.T.: 16.674 min
Delta R.T.: -0.050 min
Response: 16879802
Conc: 5.61 ng/ml

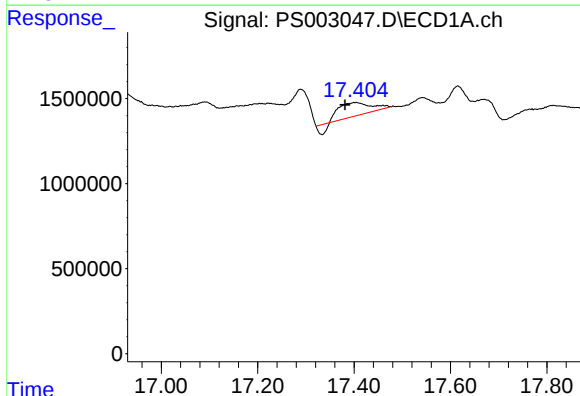

#16 DCPA

R.T.: 17.403 min
Delta R.T.: 0.021 min
Response: 3166415
Conc: 1.05 ng/ml

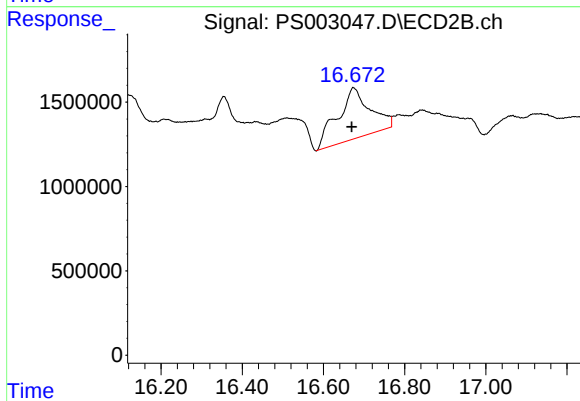

#16 DCPA

R.T.: 16.674 min
Delta R.T.: 0.004 min
Response: 16879802
Conc: 5.45 ng/ml