

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020520\
 Data File : PS008734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2020 16:28
 Operator : DD\AJ
 Sample : PB126600BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:41:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.251	6.945	969.6E6	464.0E6	451.741	500.620
Target Compounds							
1) T	Dalapon	0.000	2.595	0	239.6E6	N.D.	199.793
2) T	3,5-DICHL...	0.000	6.119	0	80248754	N.D.	58.325
7) T	MCPA	7.804	0.000	58536247	0	6.814	N.D. #
15) T	Picloram	11.048	11.039	185.1E6	126.2E6	12.222	16.714 #
16) T	DCPA	0.000	11.039	0	126.2E6	N.D.	19.396



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020520\
Data File : PS008734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2020 16:28
Operator : DD\AJ
Sample : PB126600BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:41:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

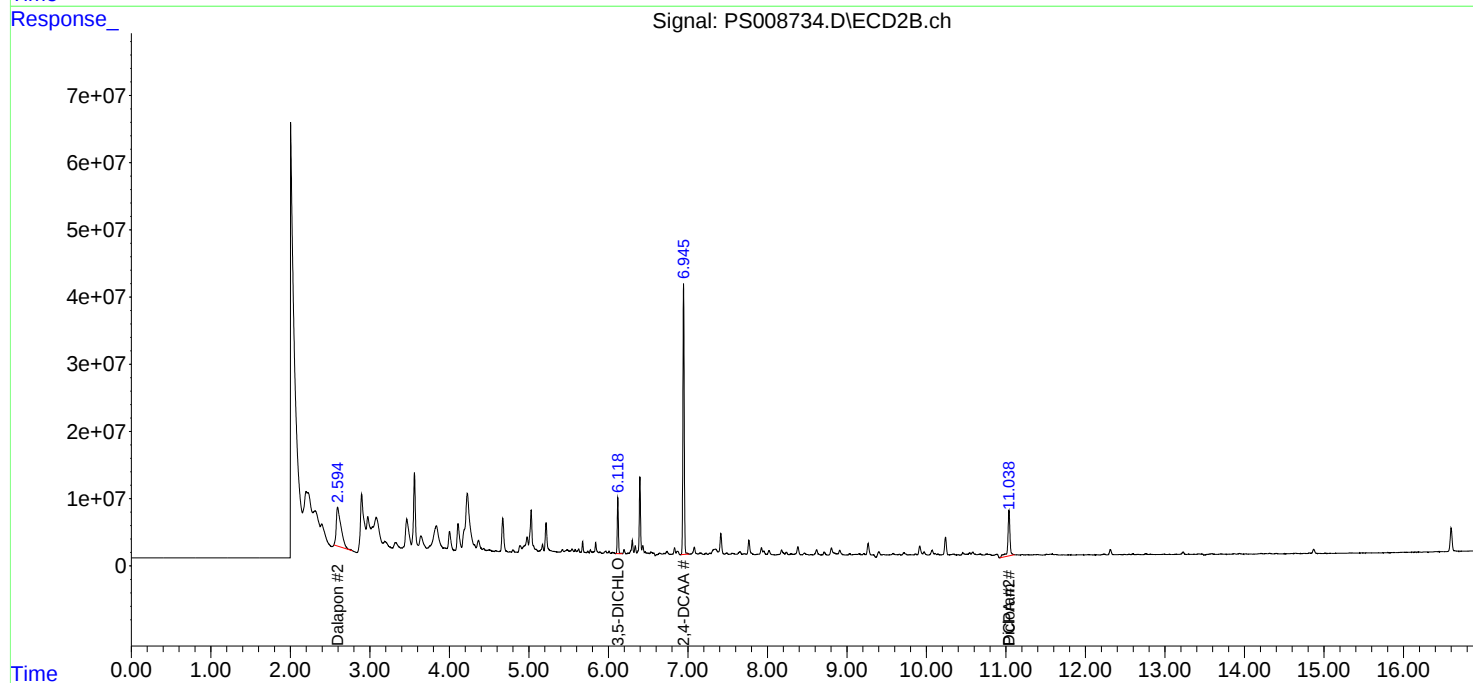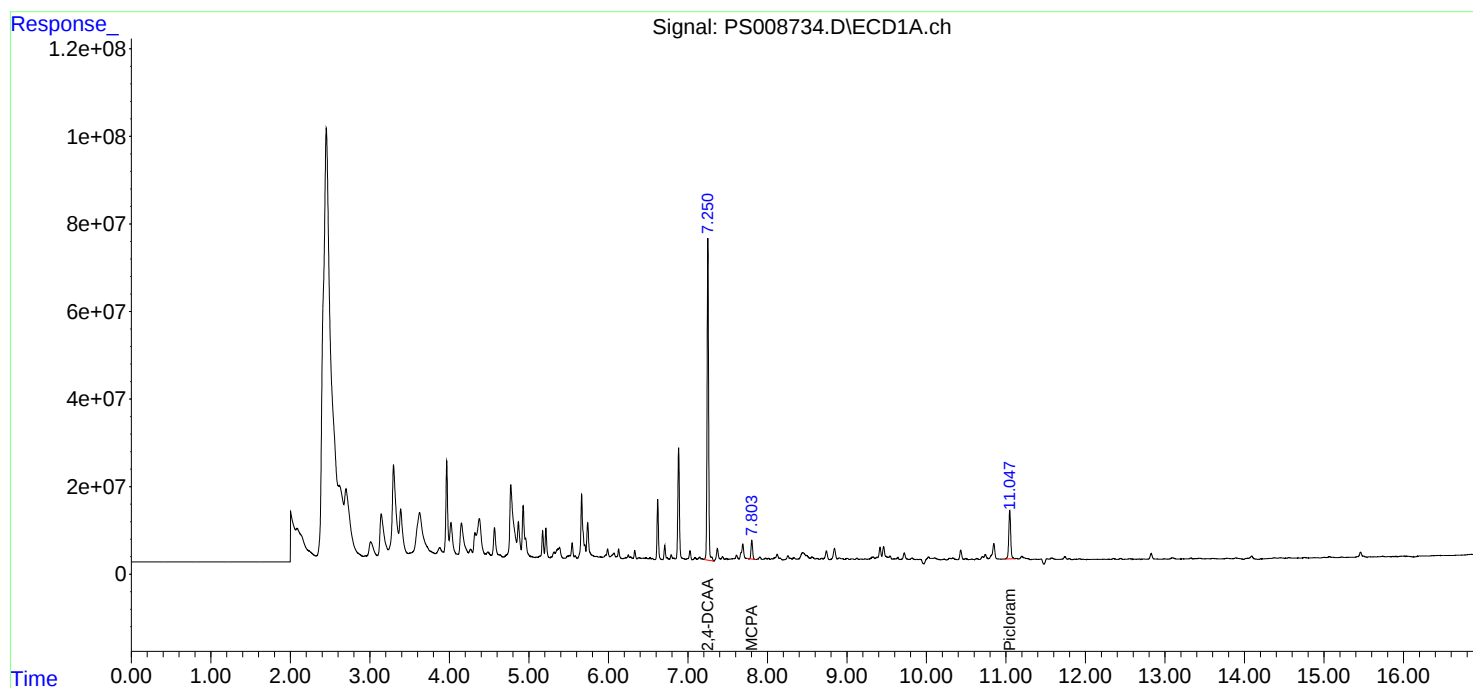


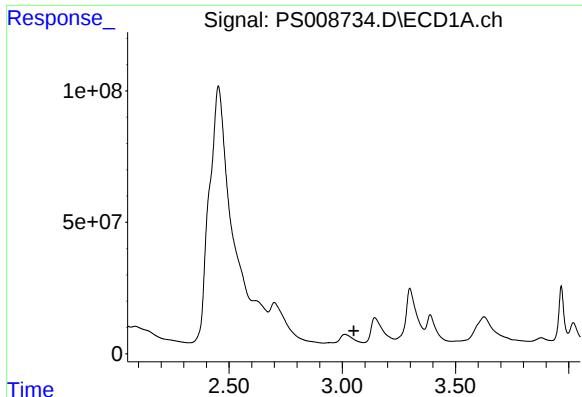

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

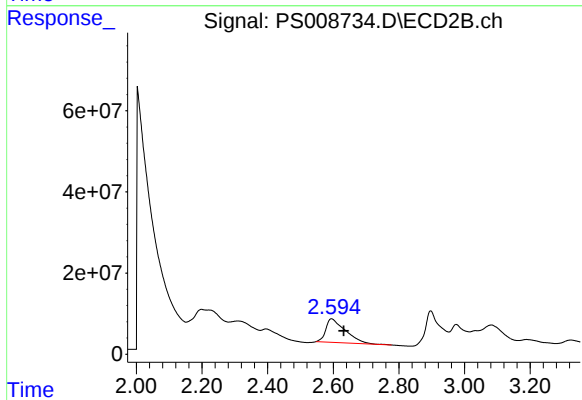


#1 Dalapon

R.T.: 2.595 min
Delta R.T.: -0.037 min
Response: 239615598
Conc: 199.79 ng/ml

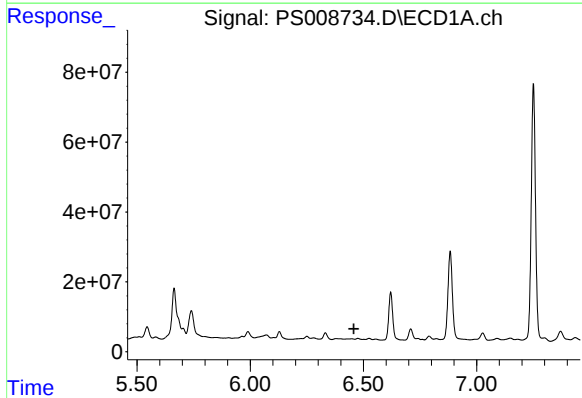


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

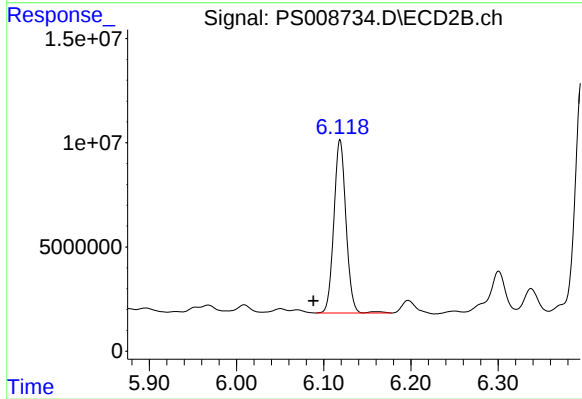

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.119 min
Delta R.T.: 0.031 min
Response: 80248754
Conc: 58.33 ng/ml

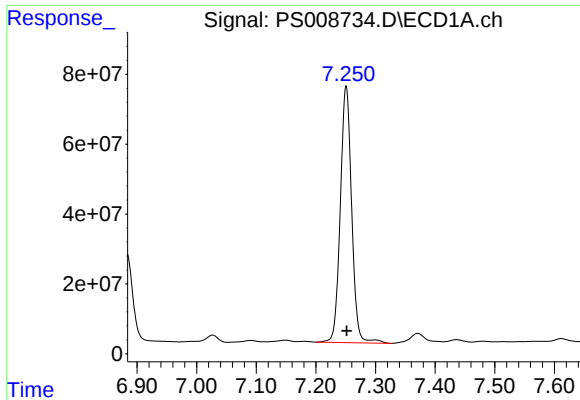

#4 2,4-DCAA


R.T.: 7.251 min
Delta R.T.: -0.001 min
Response: 969576782
Conc: 451.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

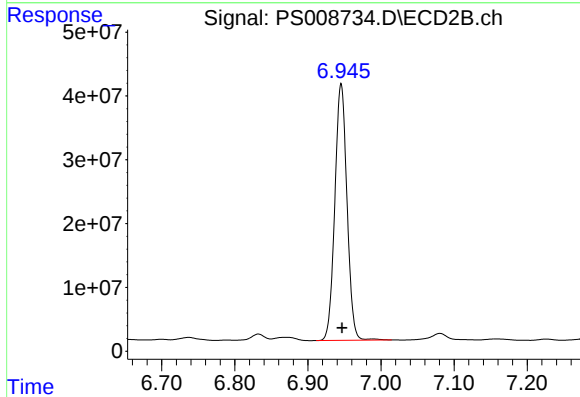


#4 2,4-DCAA

R.T.: 6.945 min
Delta R.T.: -0.001 min
Response: 463986503
Conc: 500.62 ng/ml

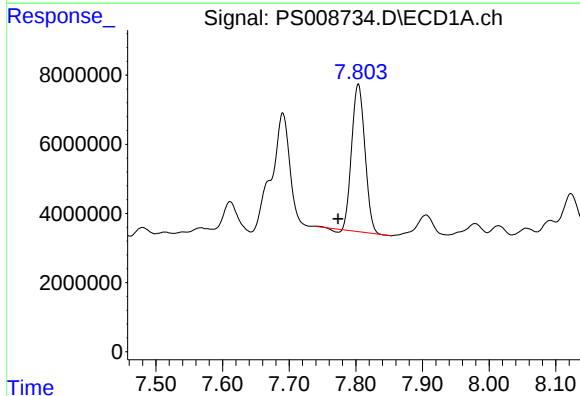


#7 MCPA

R.T.: 7.804 min
Delta R.T.: 0.030 min
Response: 58536247
Conc: 6.81 ug/ml

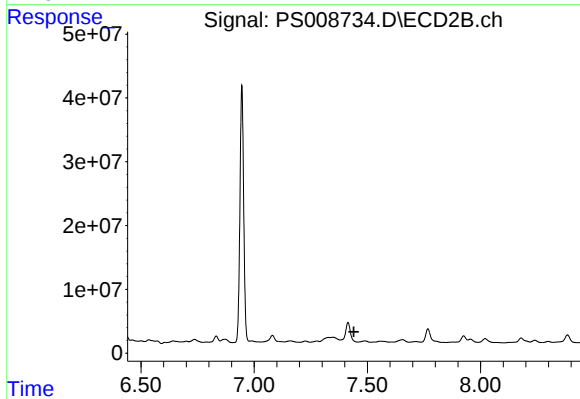

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.441 min
Response: 0
Conc: N.D.

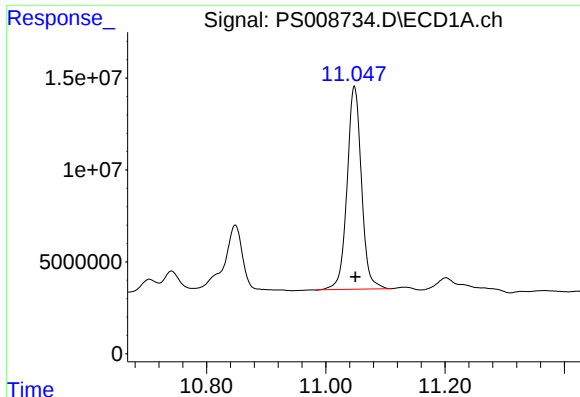

#15 Picloram


R.T.: 11.048 min
Delta R.T.: -0.002 min
Response: 185090245
Conc: 12.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

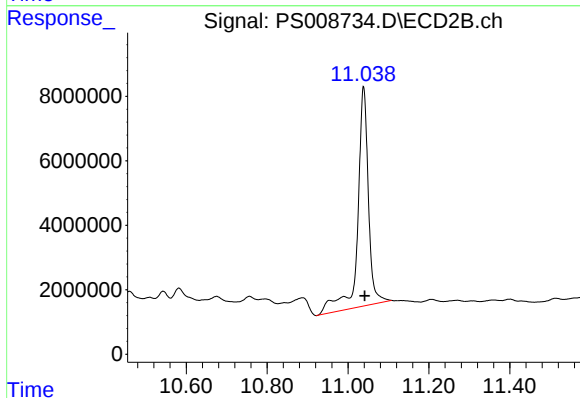


#15 Picloram

R.T.: 11.039 min
Delta R.T.: -0.003 min
Response: 126156406
Conc: 16.71 ng/ml

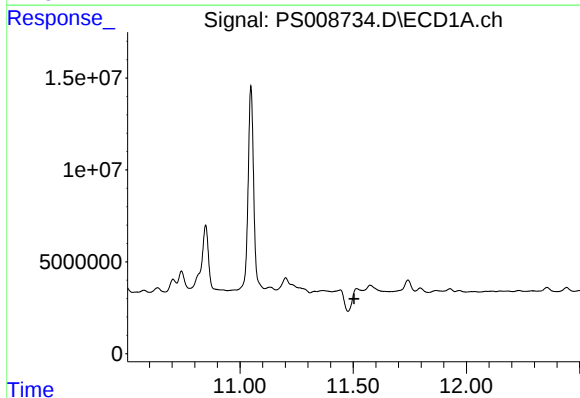

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.503 min
Response: 0
Conc: N.D.

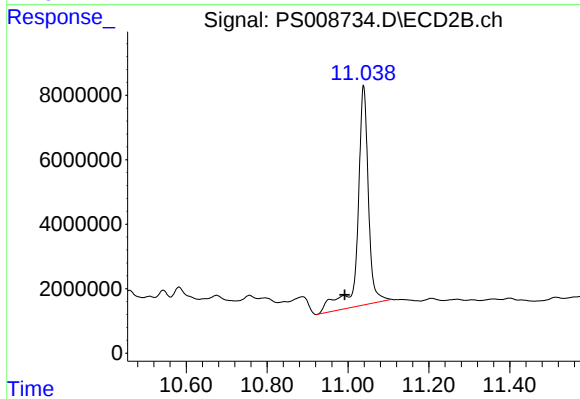

#16 DCPA

R.T.: 11.039 min
Delta R.T.: 0.046 min
Response: 126156406
Conc: 19.40 ng/ml