

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020521\
 Data File : PS013942.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2021 10:48
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 14:45:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 28 01:00:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.468f	0.000	94674644	0	63.709	N.D.	#
5) T	DICAMBA	0.000	7.140f	0	53115361	N.D.	32.231	
6) T	MCPP	0.000	7.140	0	53115361	N.D.	39.547	
15) T	Picloram	10.977	11.058f	36134992	25375208	4.256	7.436	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020521\
Data File : PS013942.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2021 10:48
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 14:45:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
Quant Title : 8080.M
QLast Update : Thu Jan 28 01:00:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

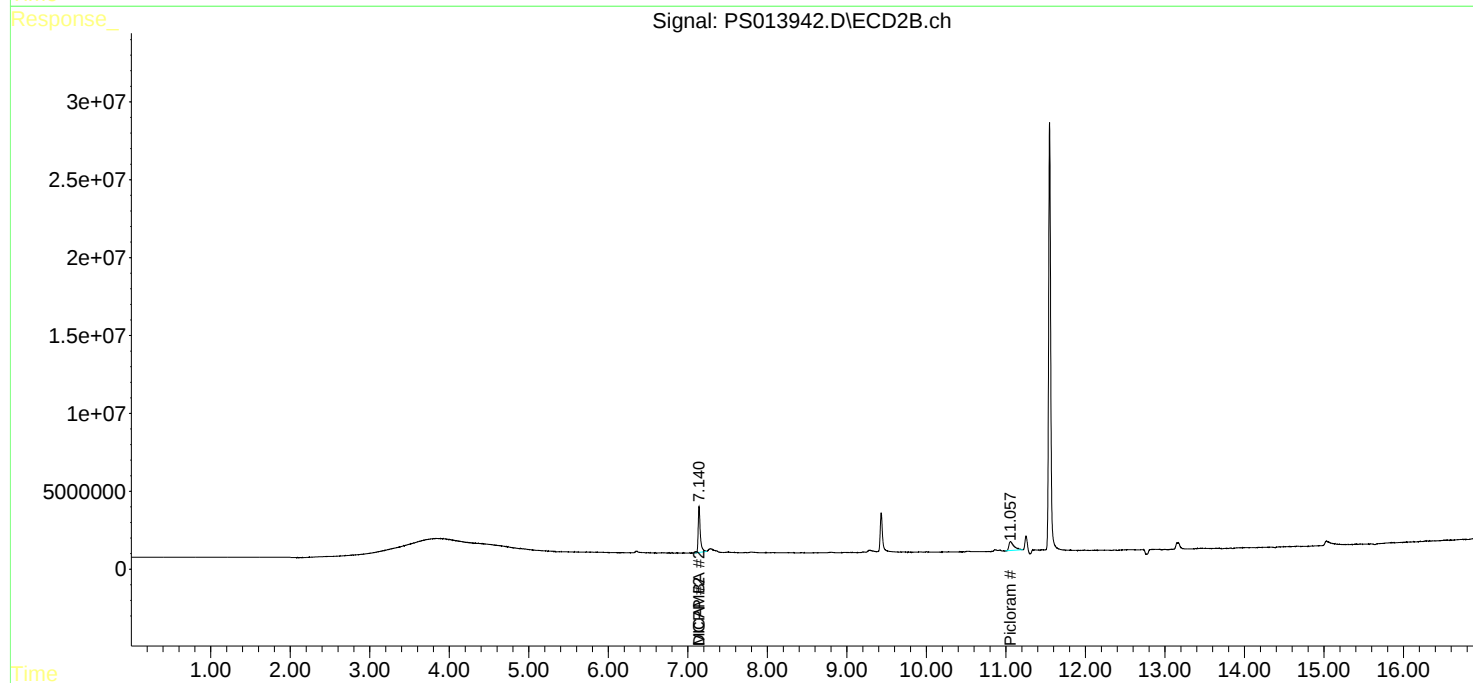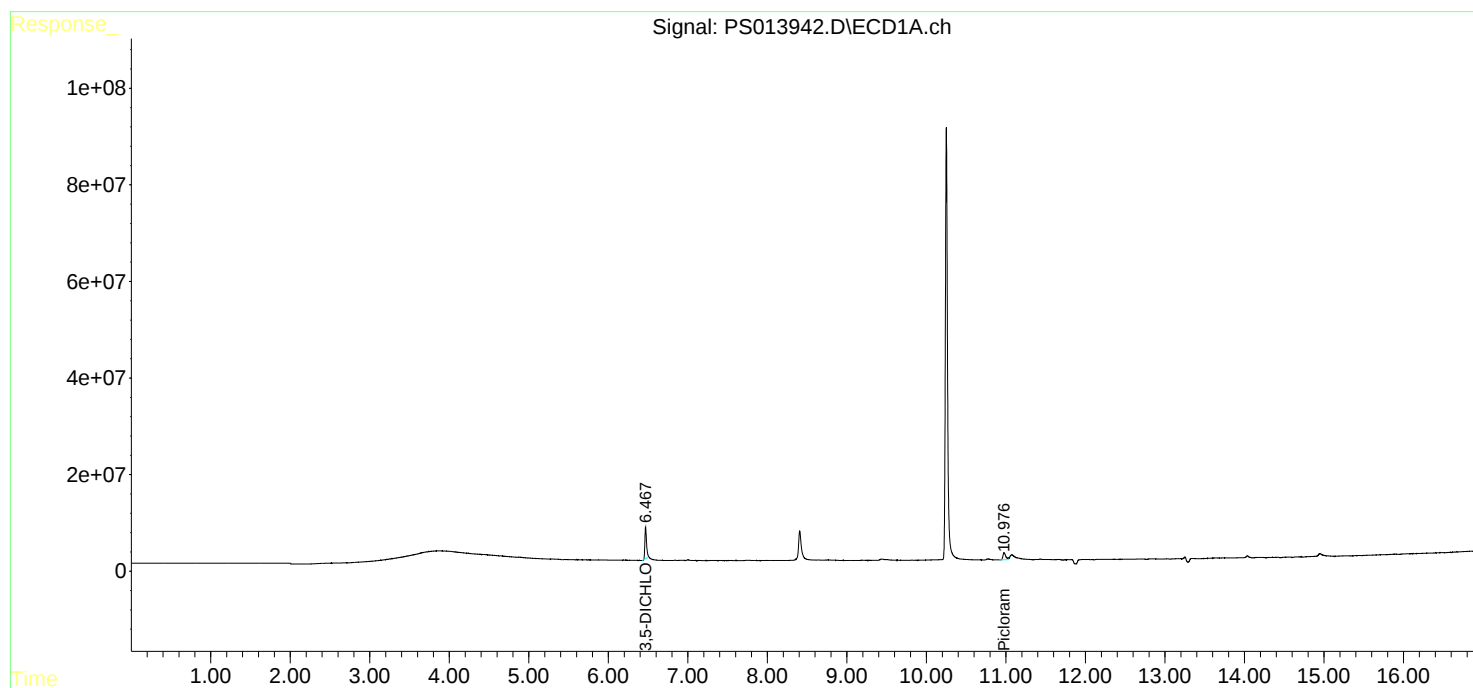


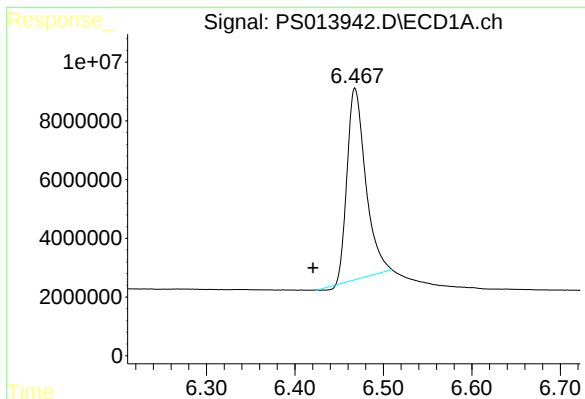

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.468 min
Delta R.T.: 0.048 min
Response: 94674644
Conc: 63.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

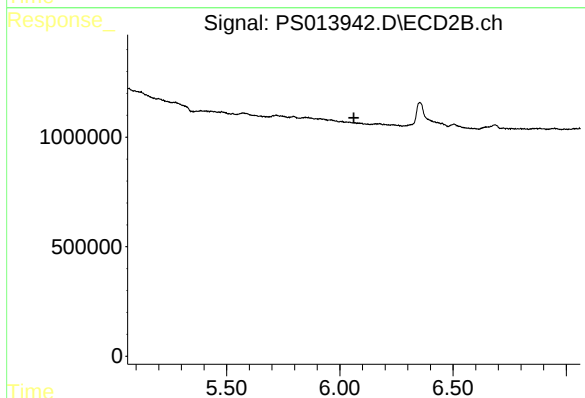


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.062 min
Response: 0
Conc: N.D.

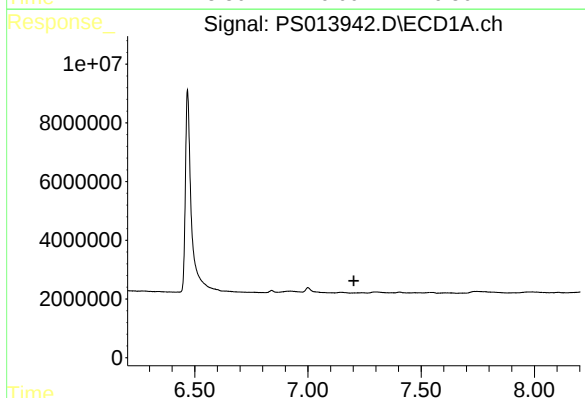


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.203 min
Response: 0
Conc: N.D.

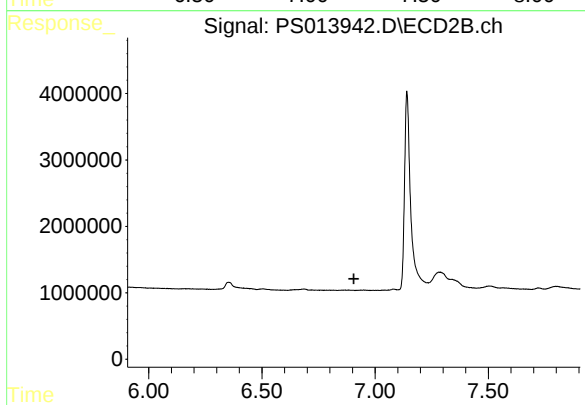

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.906 min
Response: 0
Conc: N.D.

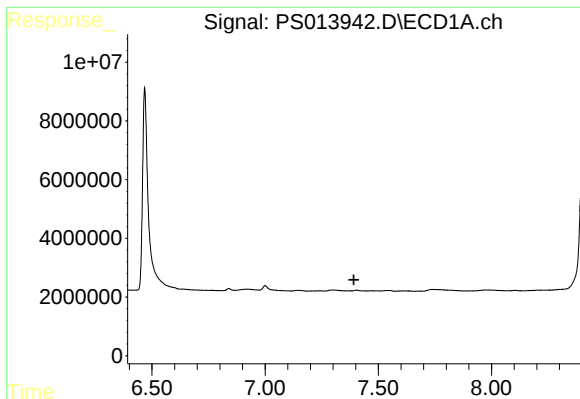

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

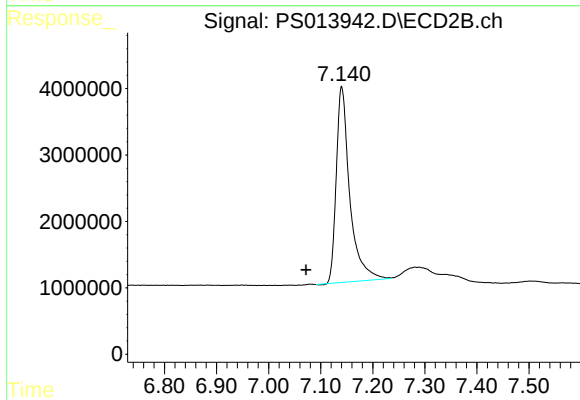


#5 DICAMBA

R.T.: 7.140 min
Delta R.T.: 0.068 min
Response: 53115361
Conc: 32.23 ng/ml

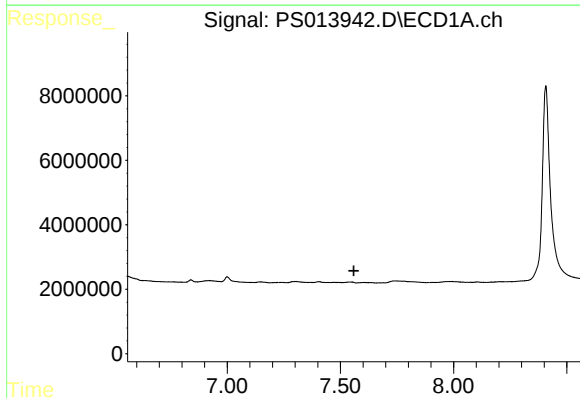


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.559 min
Response: 0
Conc: N.D.

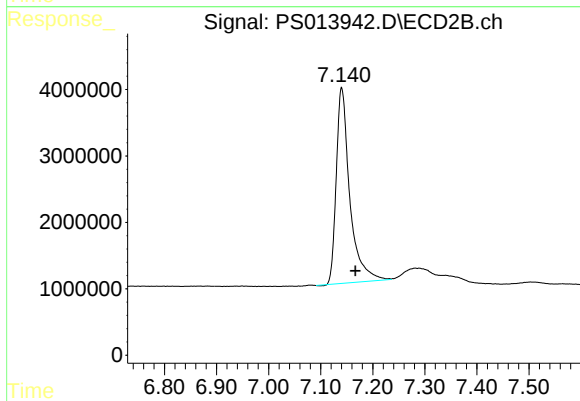

#6 MCP


R.T.: 7.140 min
Delta R.T.: -0.026 min
Response: 53115361
Conc: 39.55 ug/ml

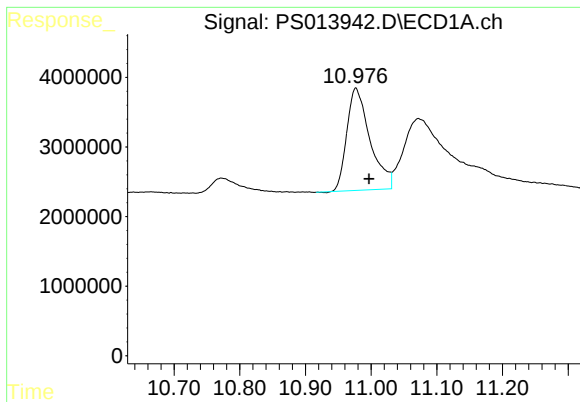

#15 Picloram

R.T.: 10.977 min
Delta R.T.: -0.020 min
Response: 36134992
Conc: 4.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

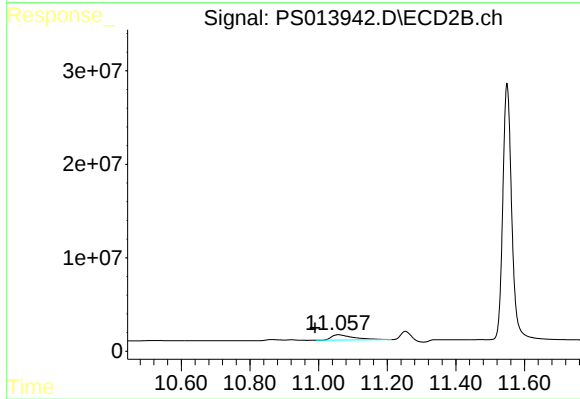

#15 Picloram

R.T.: 11.058 min
Delta R.T.: 0.068 min
Response: 25375208
Conc: 7.44 ng/ml