

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020524\
 Data File : PS025720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2024 08:53
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 14:08:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.553	0	3416970	N.D. 2.908
2) T	3,5-DICHL...	5.691	0.000	4763131	0	2.081 N.D. #
5) T	DICAMBA	0.000	6.951	0	3248177	N.D. <MDL
6) T	MCP	0.000	6.951f	0	3248177	N.D. 1.400
7) T	MCPA	0.000	7.278f	0	350756	N.D. <MDL
8) T	DICHLORPROP	0.000	7.535	0	1773466	N.D. 2.052
9) T	2,4-D	7.241	0.000	11977613	0	6.505 N.D. #
11) T	2,4,5-TP ...	0.000	8.534f	0	625240	N.D. <MDL
12) T	2,4,5-T	0.000	9.001	0	339958	N.D. <MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020524\
Data File : PS025720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2024 08:53
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 14:08:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

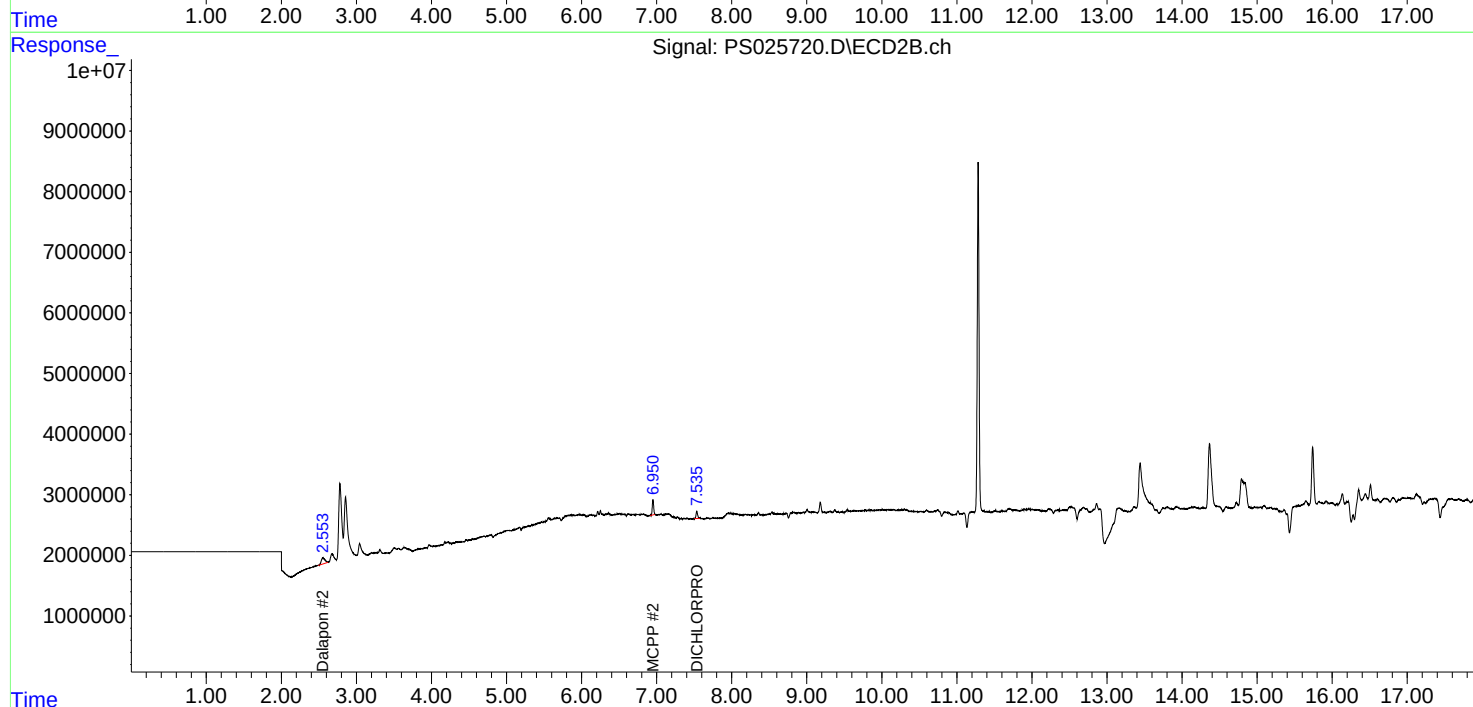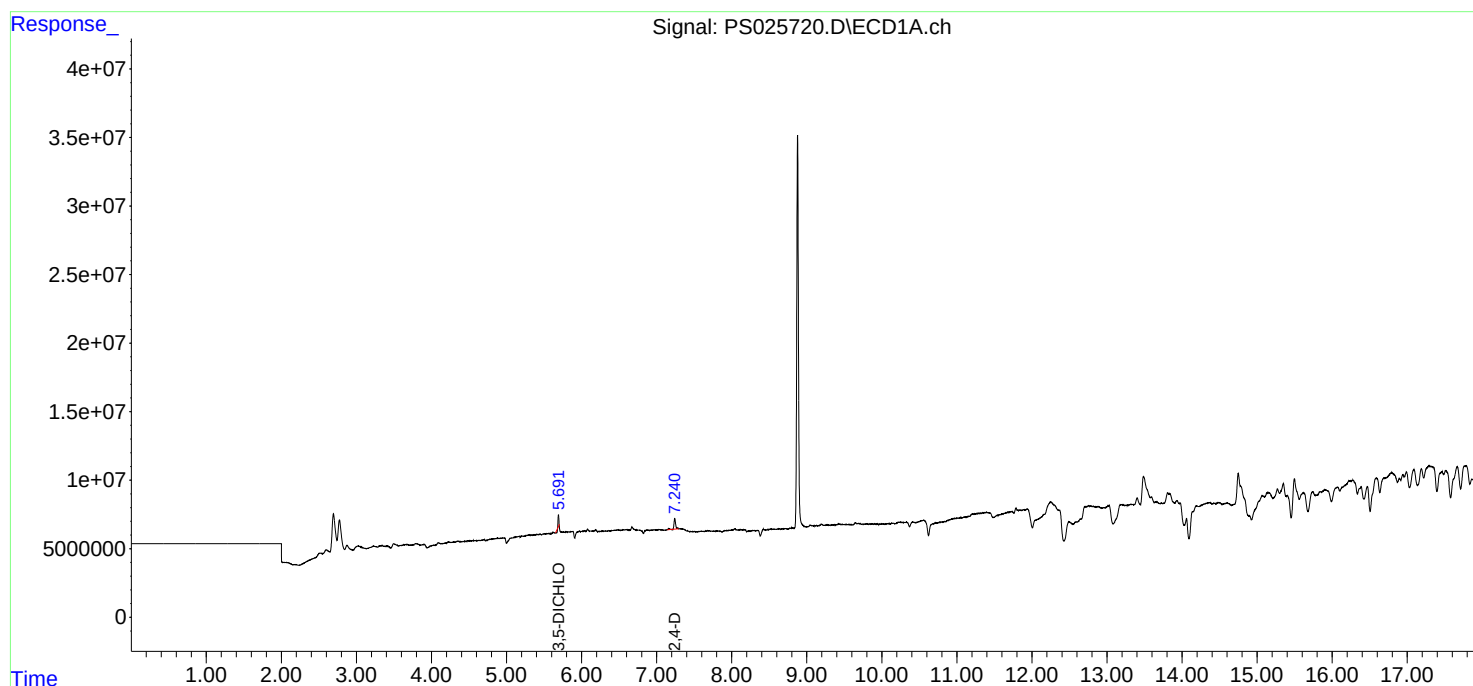


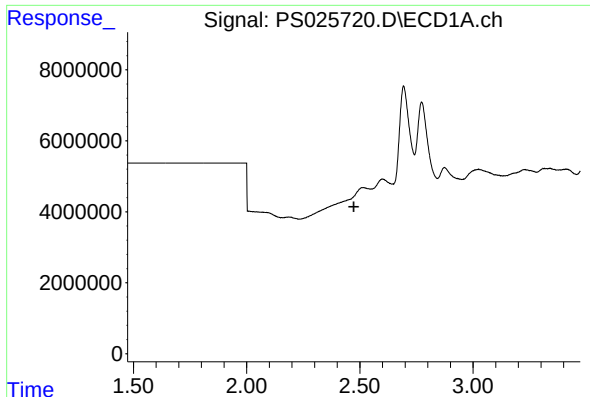

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

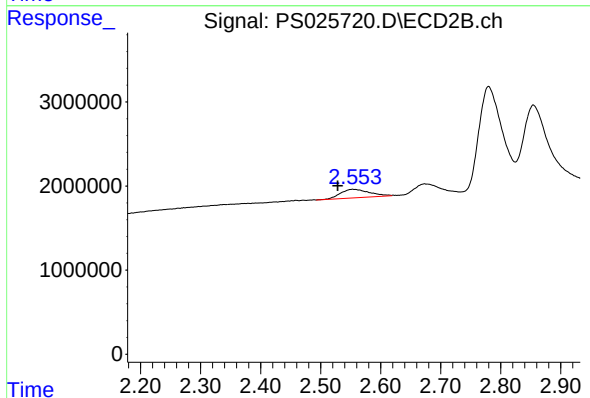


#1 Dalapon

R.T.: 2.553 min
Delta R.T.: 0.025 min
Response: 3416970
Conc: 2.91 ng/ml

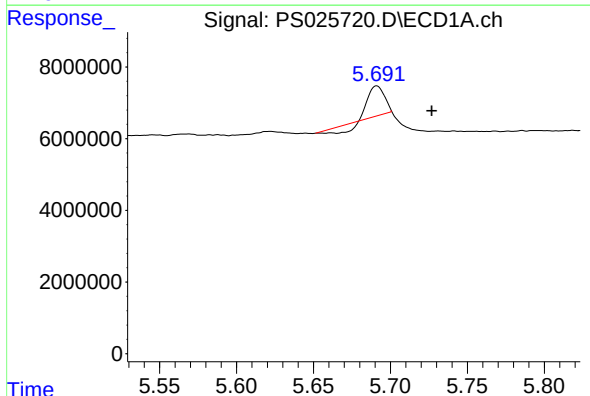


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.036 min
Response: 4763131
Conc: 2.08 ng/ml

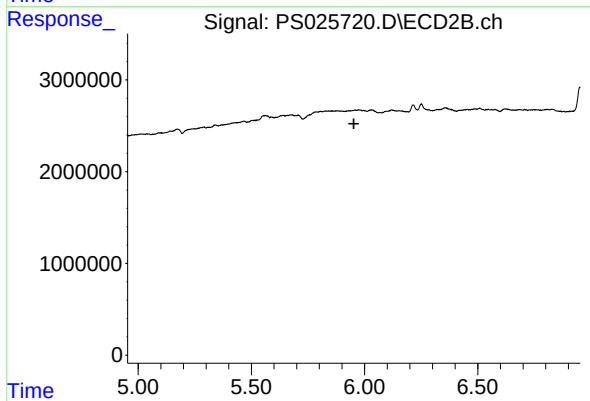

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.953 min
Response: 0
Conc: N.D.

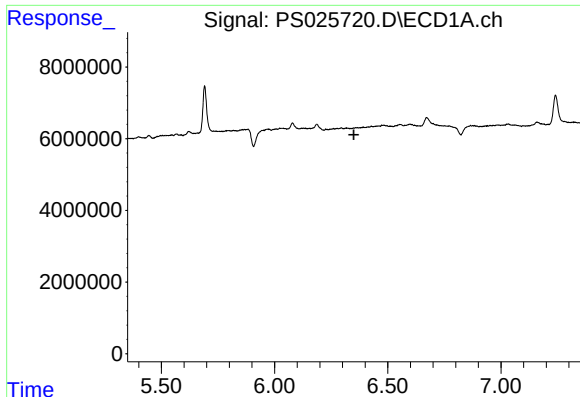

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

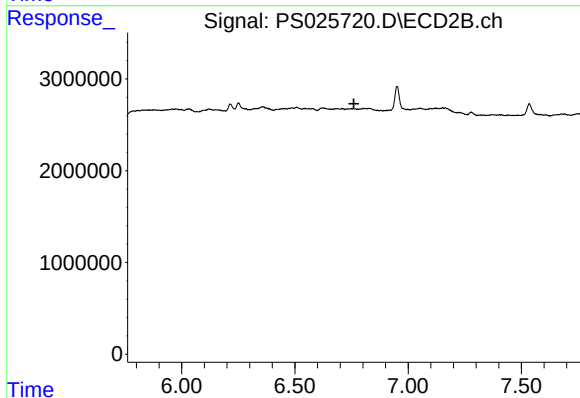


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.761 min
Response: 0
Conc: N.D.

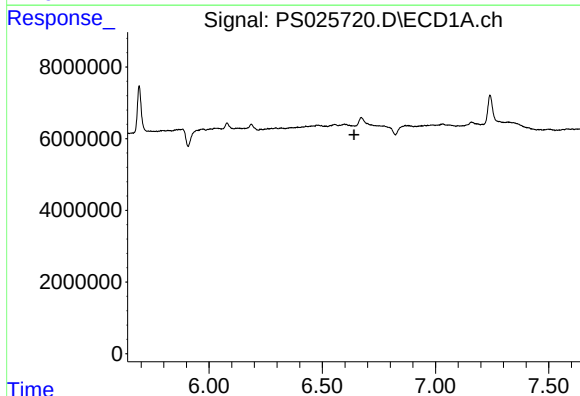


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.640 min
Response: 0
Conc: N.D.

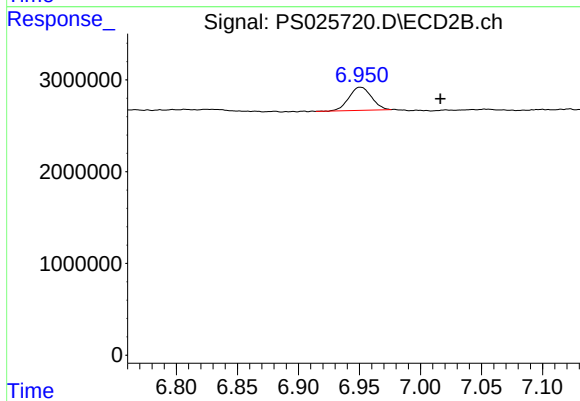

#6 MCPP


R.T.: 6.951 min
Delta R.T.: -0.066 min
Response: 3248177
Conc: 1.40 ug/ml

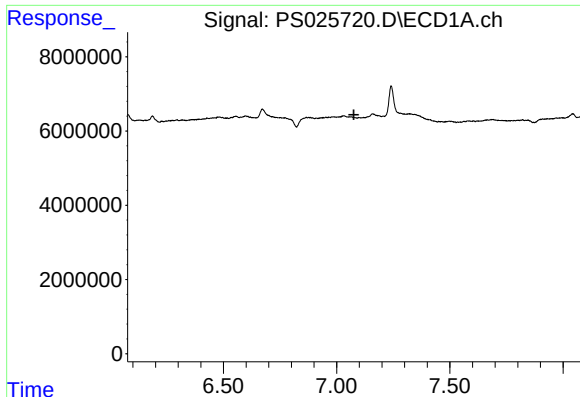

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

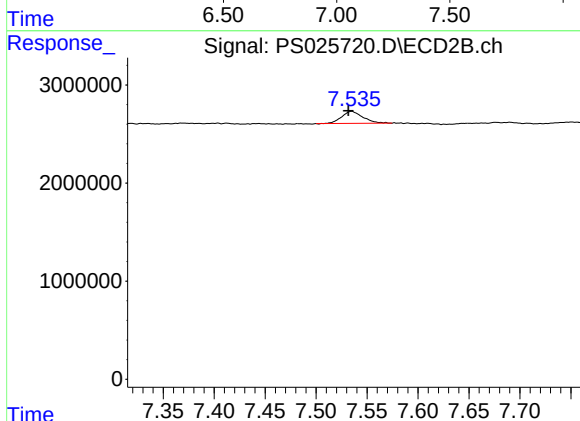


#8 DICHLORPROP

R.T.: 7.535 min
Delta R.T.: 0.003 min
Response: 1773466
Conc: 2.05 ng/ml

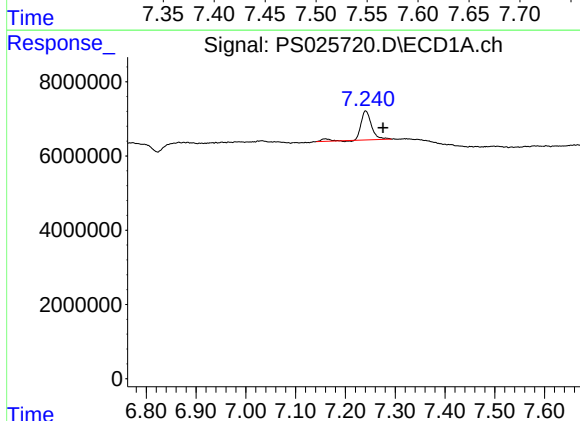

#9 2,4-D

R.T.: 7.241 min
Delta R.T.: -0.035 min
Response: 11977613
Conc: 6.50 ng/ml

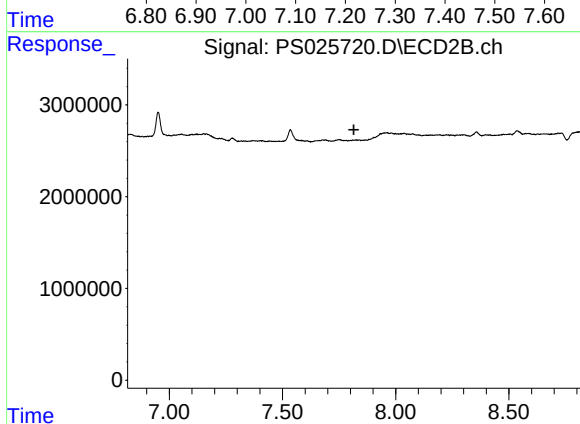

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.815 min
Response: 0
Conc: N.D.