

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 19:34
 Operator : EI\SJ
 Sample : PB116874TB
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB116874TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:52:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.315	10.814	212.4E6	217.6E6	559.402	508.854
Target Compounds							
1) T	Dalapon	2.834	2.315	16672148	43541570	30.222	81.246 #
2) T	3,5-DICHL...	0.000	8.982	0	9078802	N.D.	16.110 #
6) T	MCP	11.988	0.000	4819965	0	4.023	N.D. #
7) T	MCPA	0.000	11.766	0	167.5E6	N.D.	106.467 #
9) T	2,4-D	13.173	0.000	6095912	0	13.222	N.D. #
12) T	2,4,5-T	0.000	14.417	0	4852082	N.D.	2.536 #
14) T	DINOSEB	0.000	15.520	0	8922861	N.D.	5.090 #
15) T	Picloram	16.806	16.738	8766623	17181081	2.771	5.715 #
16) T	DCPA	0.000	16.738	0	17181081	N.D.	5.547 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 19:34
Operator : EI\SJ
Sample : PB116874TB
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB116874TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 23:52:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

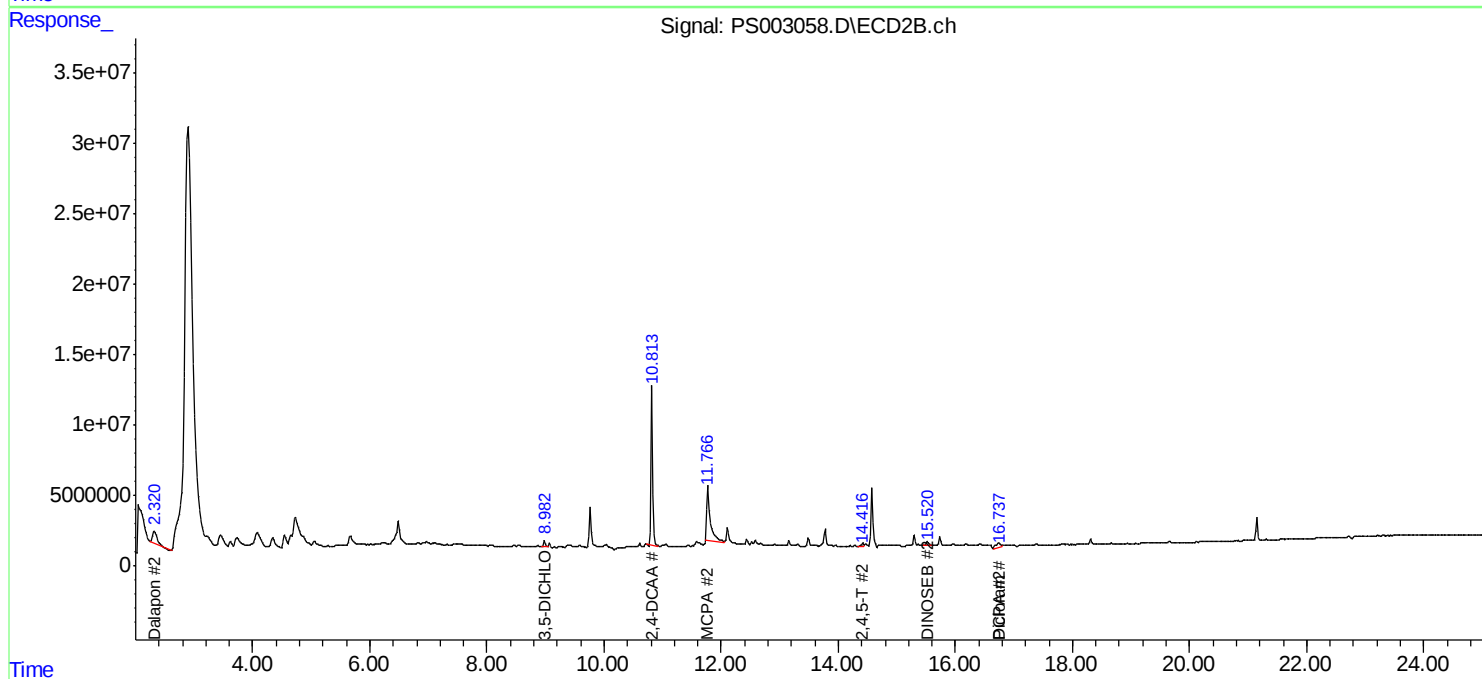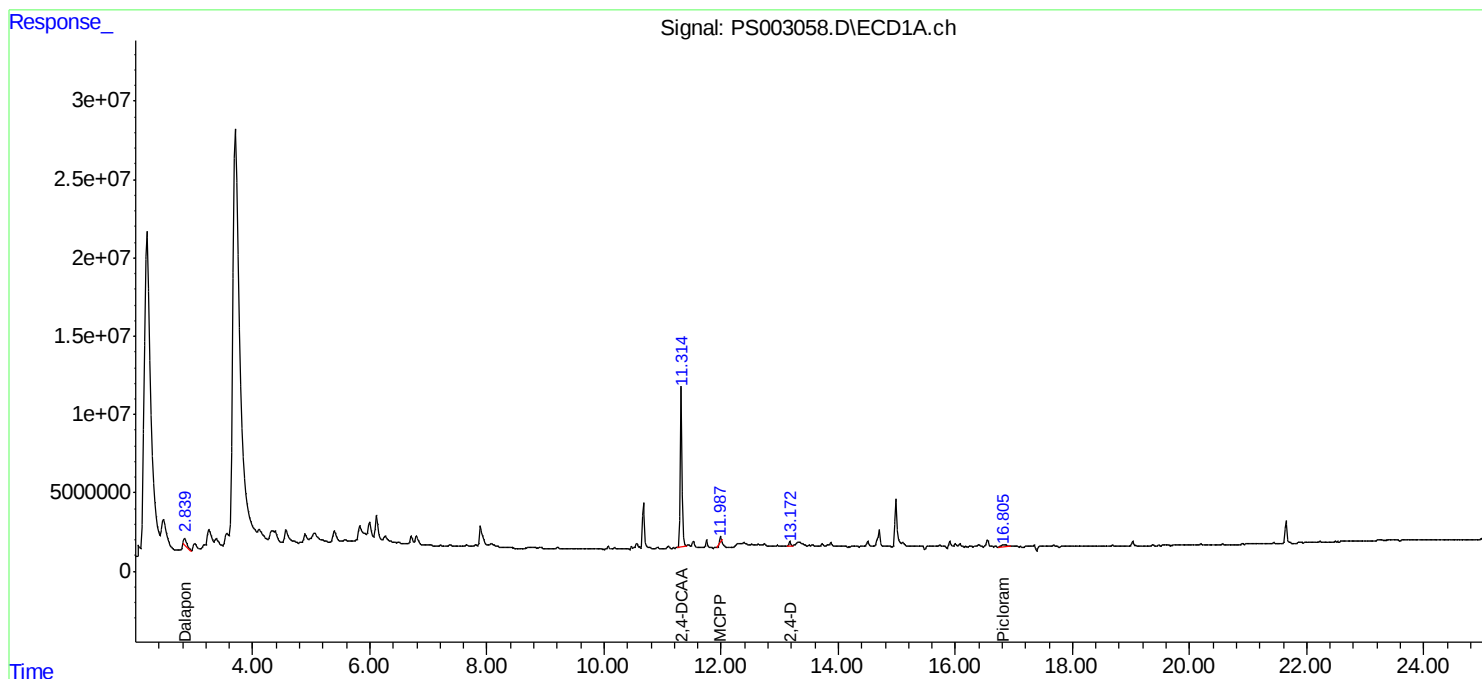


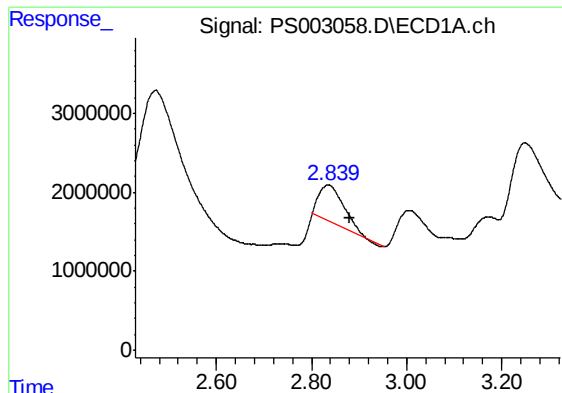

#1 Dalapon


R.T.: 2.834 min
Delta R.T.: -0.046 min
Response: 16672148
Conc: 30.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116874TB

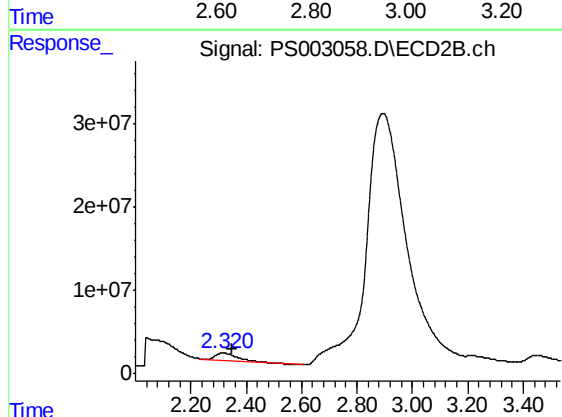


#1 Dalapon

R.T.: 2.315 min
Delta R.T.: -0.036 min
Response: 43541570
Conc: 81.25 ng/ml

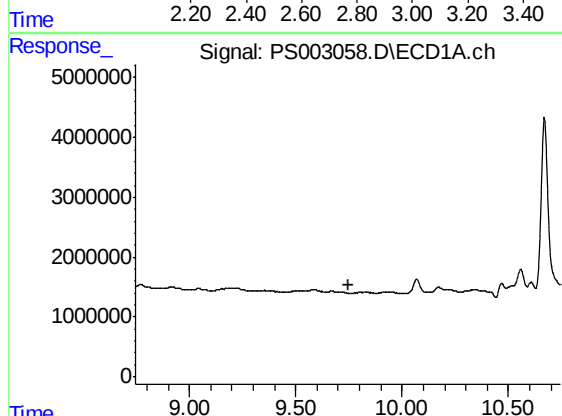


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

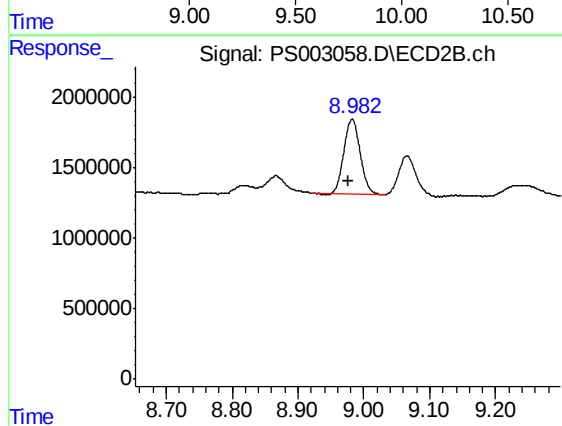

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.982 min
Delta R.T.: 0.006 min
Response: 9078802
Conc: 16.11 ng/ml

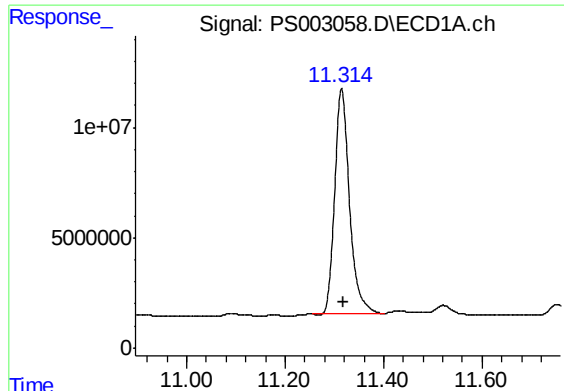

#4 2,4-DCAA


R.T.: 11.315 min
Delta R.T.: -0.003 min
Response: 212371908
Conc: 559.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116874TB

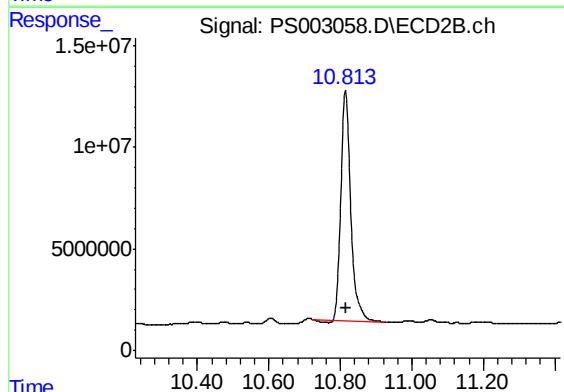


#4 2,4-DCAA

R.T.: 10.814 min
Delta R.T.: -0.002 min
Response: 217558346
Conc: 508.85 ng/ml

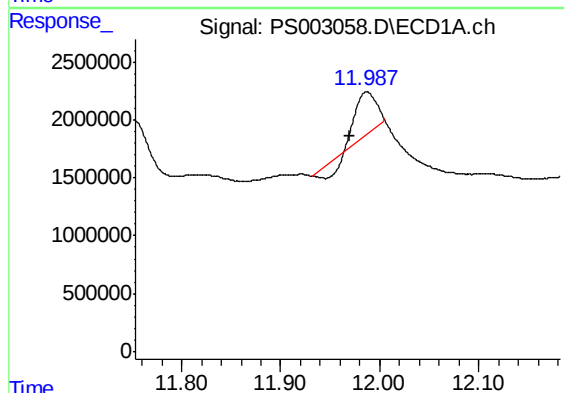


#6 MCP

R.T.: 11.988 min
Delta R.T.: 0.018 min
Response: 4819965
Conc: 4.02 ug/ml

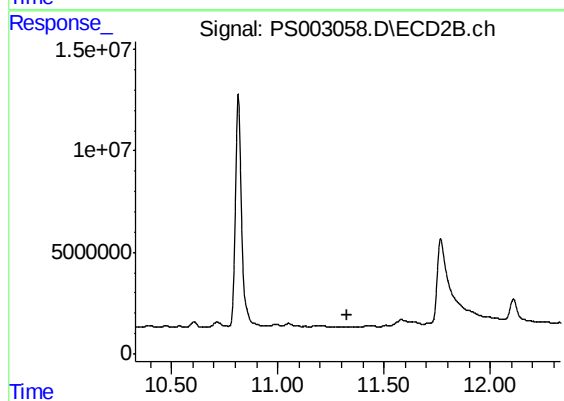

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

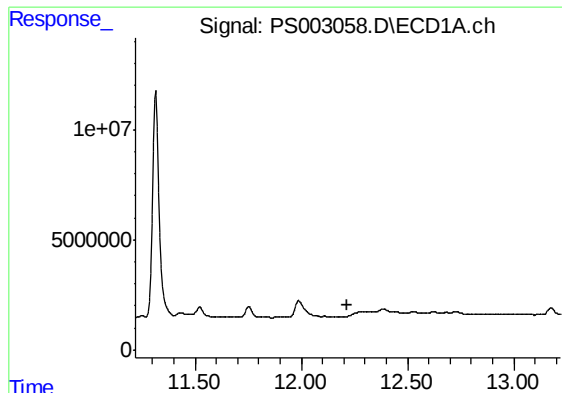

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116874TB

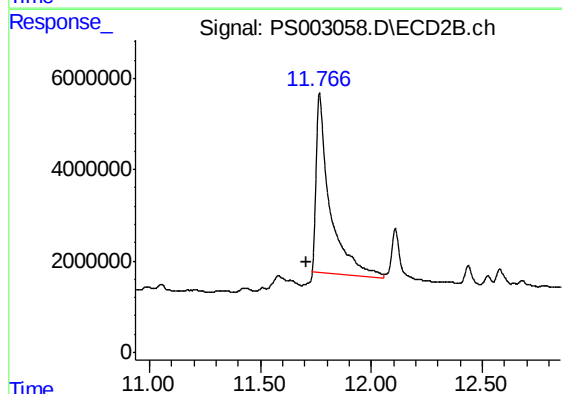


#7 MCPA

R.T.: 11.766 min
Delta R.T.: 0.060 min
Response: 167479870
Conc: 106.47 ug/ml

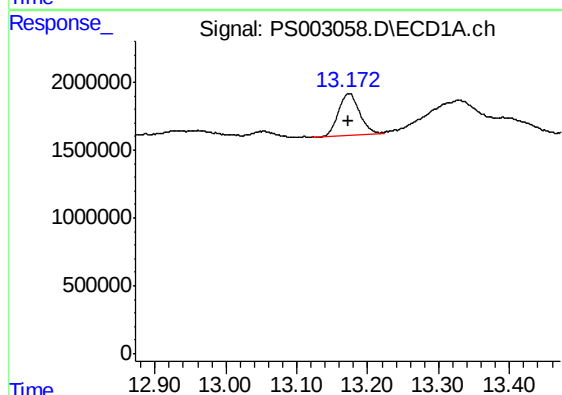


#9 2,4-D

R.T.: 13.173 min
Delta R.T.: 0.000 min
Response: 6095912
Conc: 13.22 ng/ml

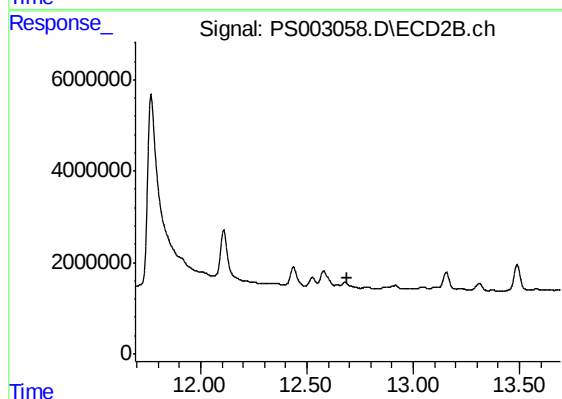

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.693 min
Response: 0
Conc: N.D.

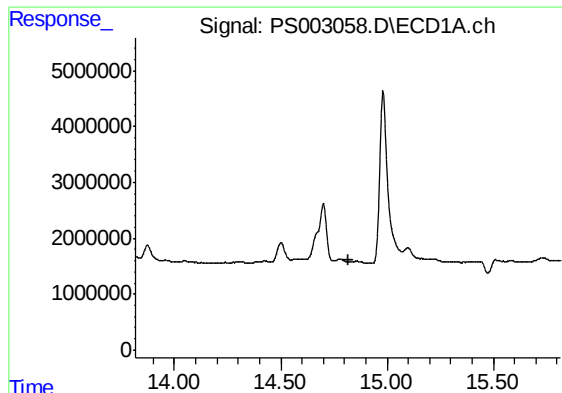

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB116874TB

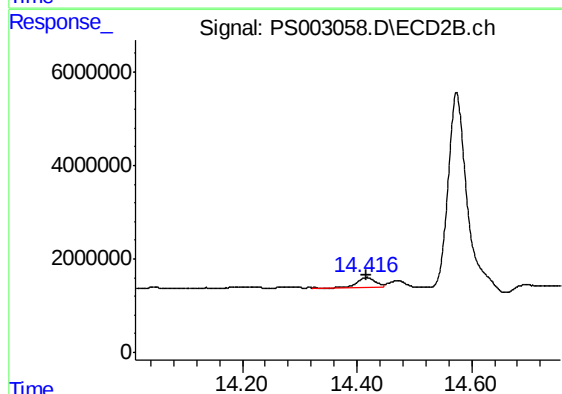


#12 2,4,5-T

R.T.: 14.417 min
Delta R.T.: 0.000 min
Response: 4852082
Conc: 2.54 ng/ml

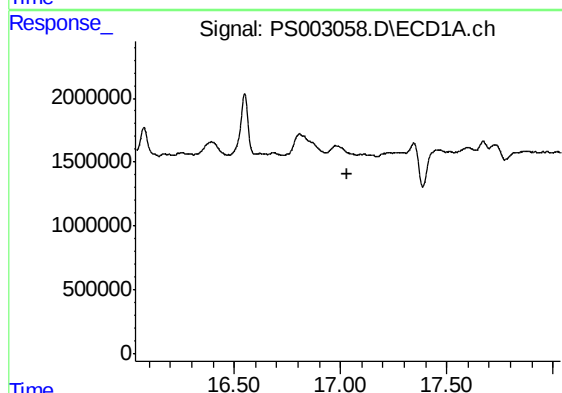


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

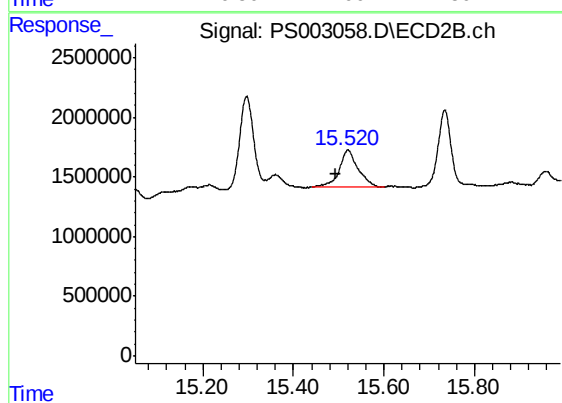

#14 DINOSEB


R.T.: 15.520 min
Delta R.T.: 0.025 min
Response: 8922861
Conc: 5.09 ng/ml

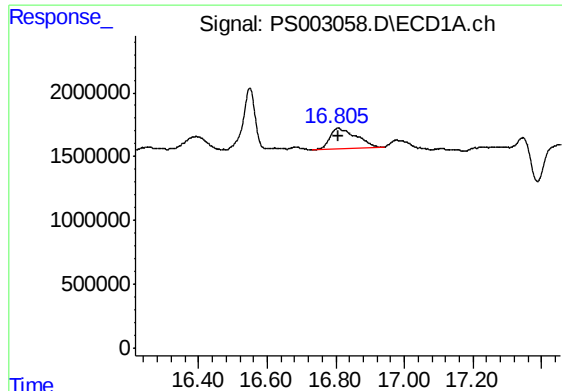

#15 Picloram


R.T.: 16.806 min
Delta R.T.: 0.000 min
Response: 8766623
Conc: 2.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB116874TB

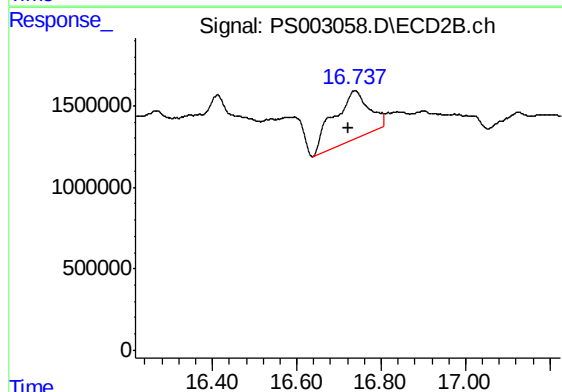


#15 Picloram

R.T.: 16.738 min
Delta R.T.: 0.013 min
Response: 17181081
Conc: 5.71 ng/ml

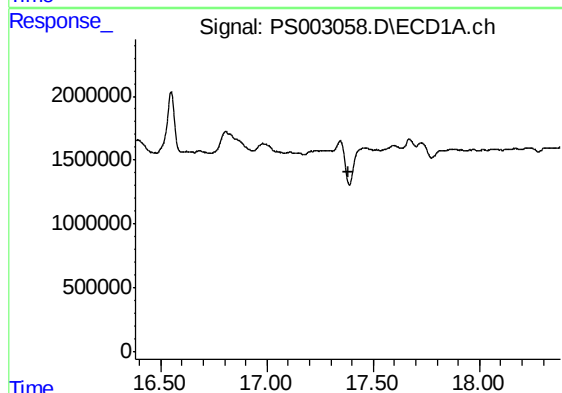

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

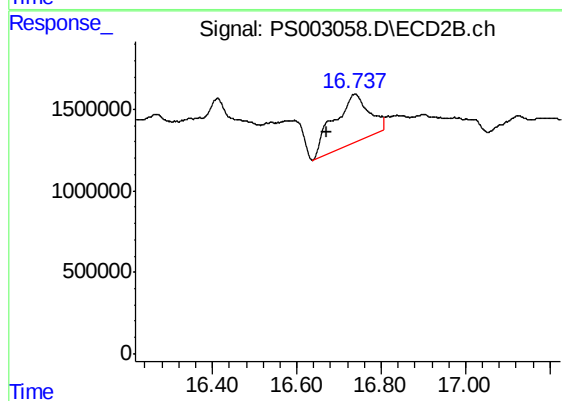

#16 DCPA

R.T.: 16.738 min
Delta R.T.: 0.068 min
Response: 17181081
Conc: 5.55 ng/ml