

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 20:06
 Operator : EI\SJ
 Sample : K1338-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-06-020519-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:52:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.774	84288392	186.0E6	222.021	435.017 #
Target Compounds							
1) T	Dalapon	0.000	2.281	0 77917054	N.D.	145.389	#
3) T	4-Nitroph...	0.000	9.997	0 23353246	N.D.	111.726	#
7) T	MCPA	0.000	11.721	0 50764525	N.D.	32.271	#
10) T	Pentachlo...	0.000	13.270	0 3501886	N.D.	0.567	#
11) T	2,4,5-TP ...	14.461	0.000	12744891	0	5.061	N.D. #
12) T	2,4,5-T	0.000	14.429	0 2859739	N.D.	1.495	#
14) T	DINOSEB	0.000	15.480	0 8033899	N.D.	4.583	#
15) T	Picloram	16.760	16.697	9413414 10074410	2.976	3.351	
16) T	DCPA	17.424	16.697	-1367742 10074410	N.D.	3.252	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 20:06
Operator : EI\SJ
Sample : K1338-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
AU-06-020519-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 23:52:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

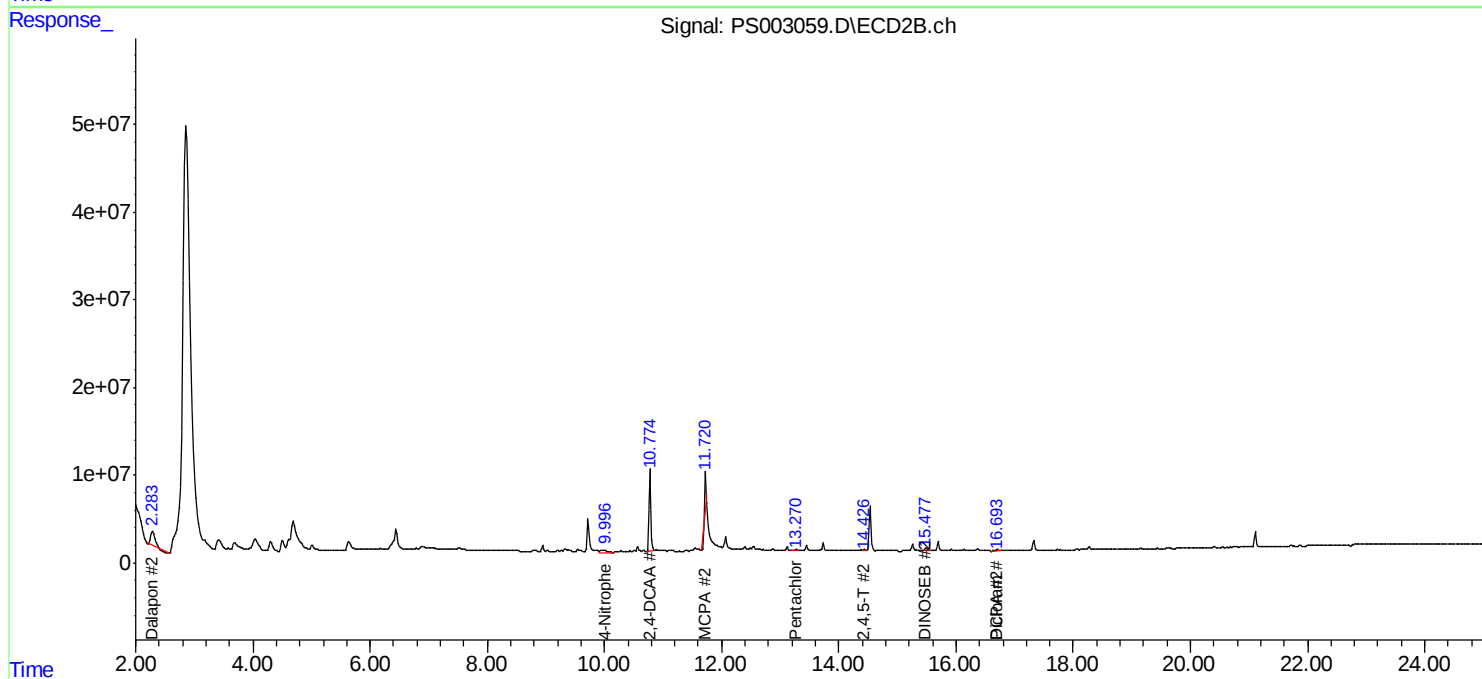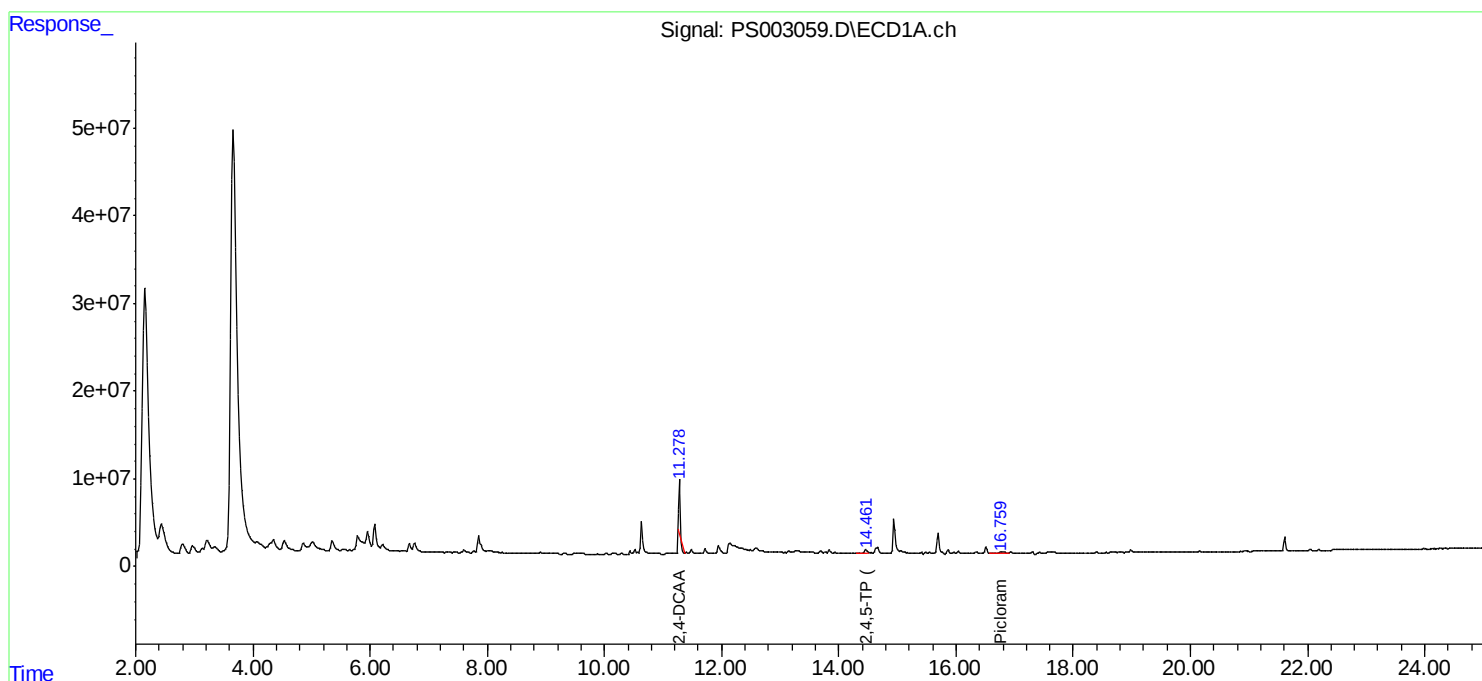


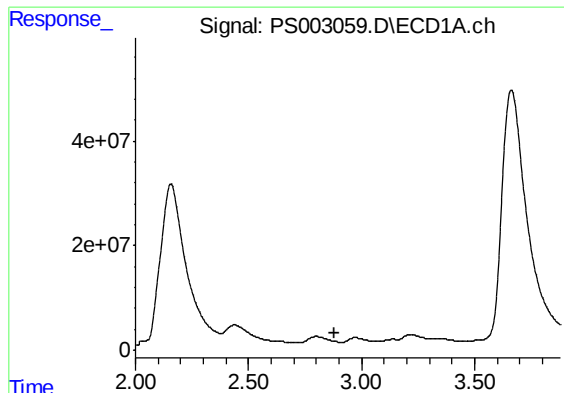

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-A

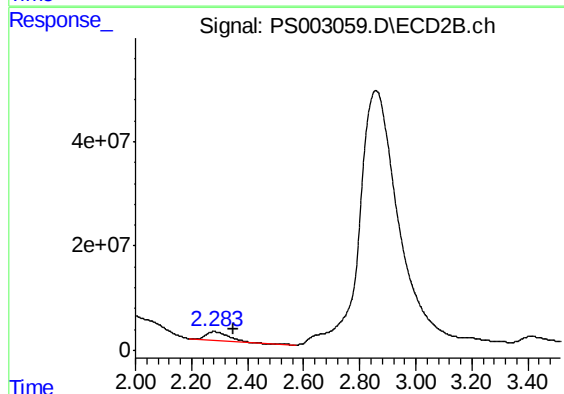


#1 Dalapon

R.T.: 2.281 min
Delta R.T.: -0.070 min
Response: 77917054
Conc: 145.39 ng/ml

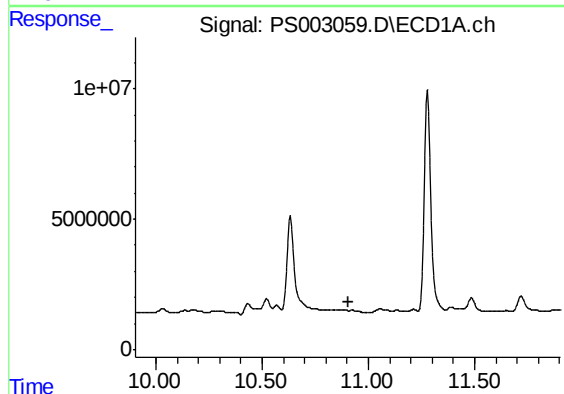


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

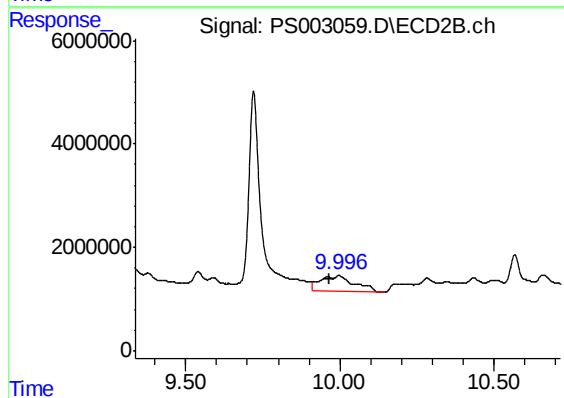

#3 4-Nitrophenol


R.T.: 9.997 min
Delta R.T.: 0.032 min
Response: 23353246
Conc: 111.73 ng/ml

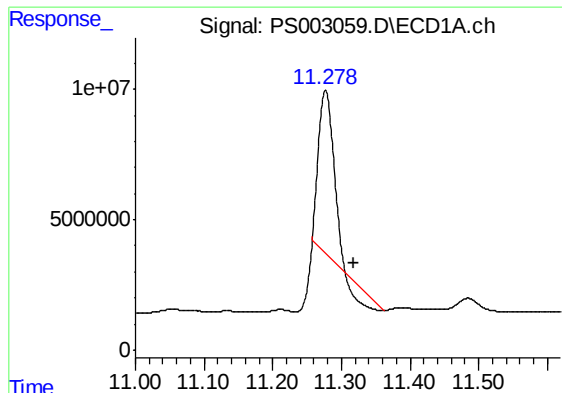

#4 2,4-DCAA


R.T.: 11.277 min
Delta R.T.: -0.041 min
Response: 84288392
Conc: 222.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-A

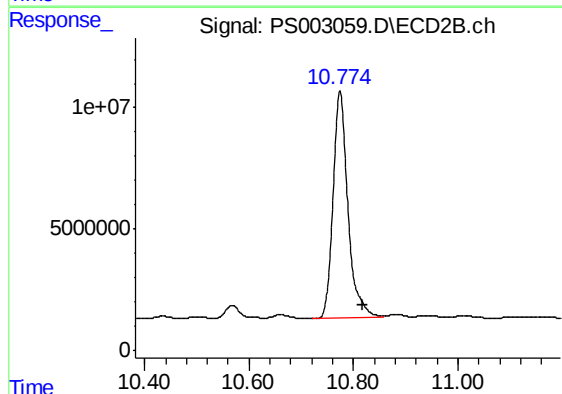


#4 2,4-DCAA

R.T.: 10.774 min
Delta R.T.: -0.042 min
Response: 185989552
Conc: 435.02 ng/ml

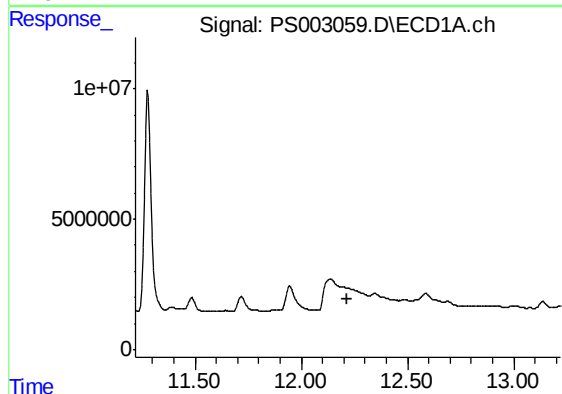


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.219 min
Response: 0
Conc: N.D.

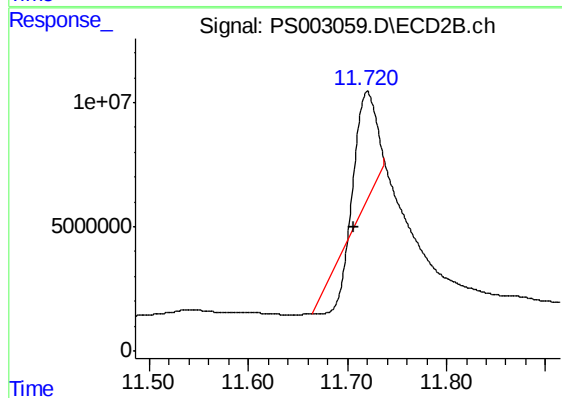

#7 MCPA


R.T.: 11.721 min
Delta R.T.: 0.015 min
Response: 50764525
Conc: 32.27 ug/ml

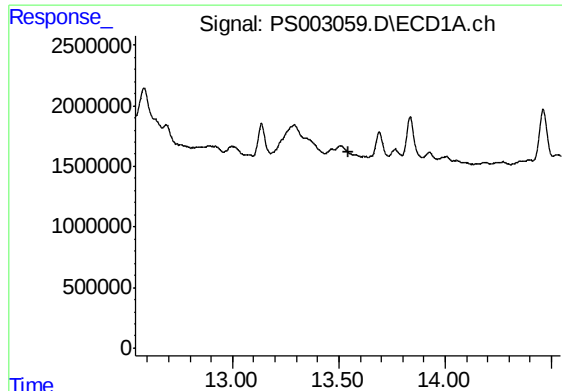

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-A

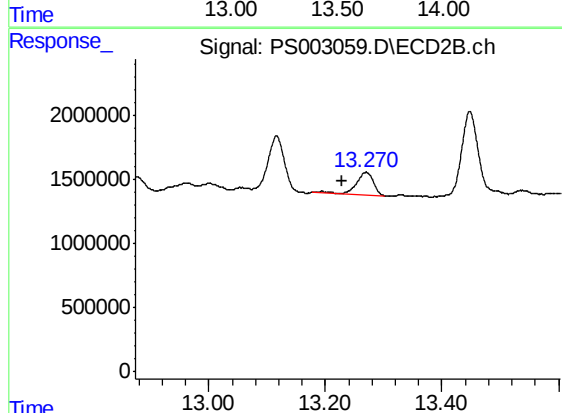


#10 Pentachlorophenol

R.T.: 13.270 min
Delta R.T.: 0.040 min
Response: 3501886
Conc: 0.57 ng/ml

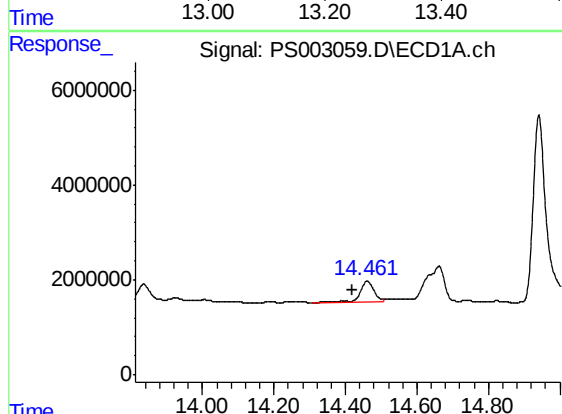


#11 2,4,5-TP (SILVEX)

R.T.: 14.461 min
Delta R.T.: 0.042 min
Response: 12744891
Conc: 5.06 ng/ml

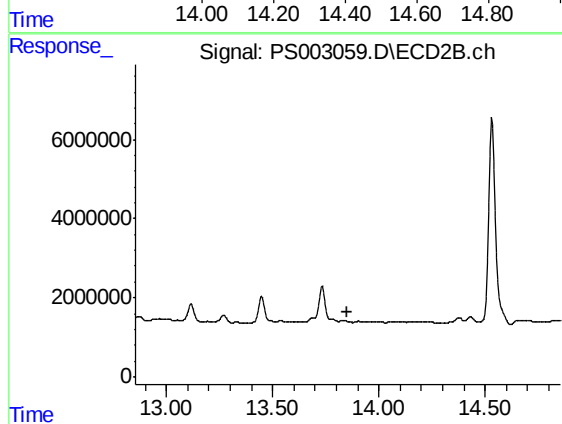

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.854 min
Response: 0
Conc: N.D.

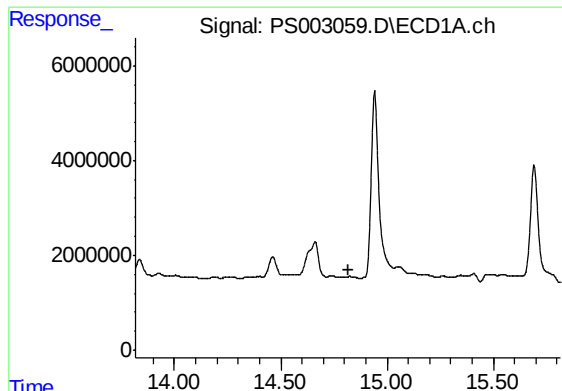

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-A

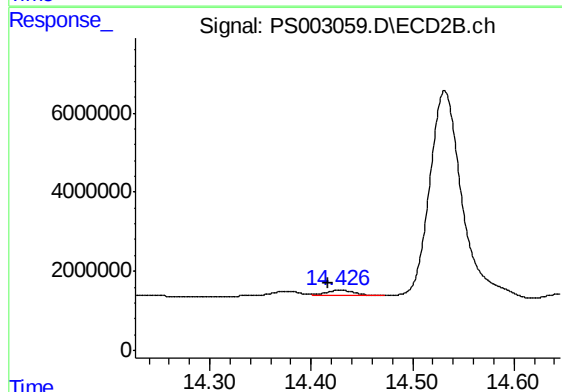


#12 2,4,5-T

R.T.: 14.429 min
Delta R.T.: 0.012 min
Response: 2859739
Conc: 1.49 ng/ml

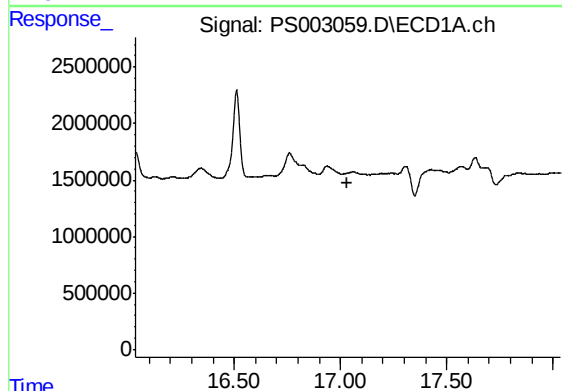


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

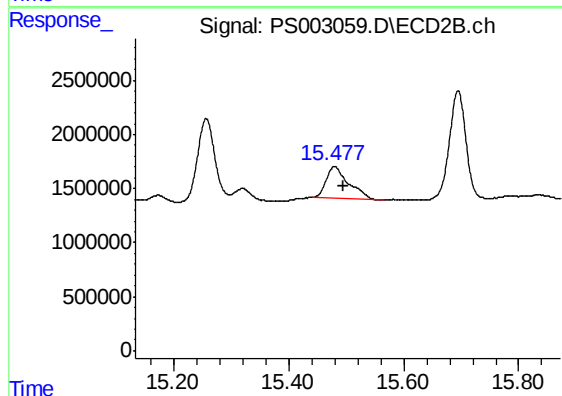

#14 DINOSEB


R.T.: 15.480 min
Delta R.T.: -0.015 min
Response: 8033899
Conc: 4.58 ng/ml

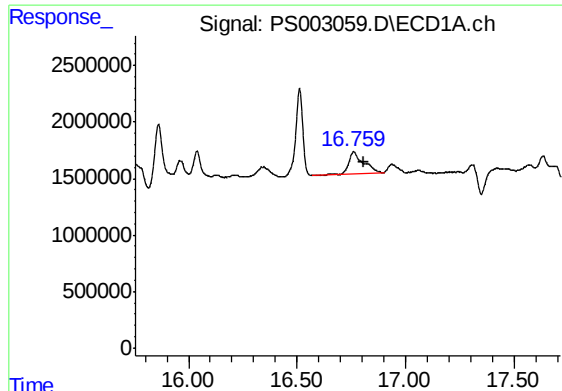

#15 Picloram


R.T.: 16.760 min
Delta R.T.: -0.046 min
Response: 9413414
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-A

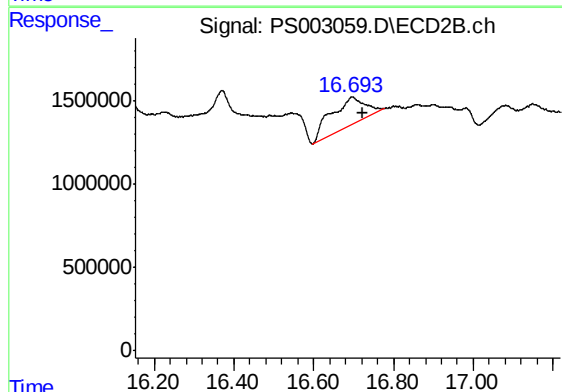


#15 Picloram

R.T.: 16.697 min
Delta R.T.: -0.027 min
Response: 10074410
Conc: 3.35 ng/ml

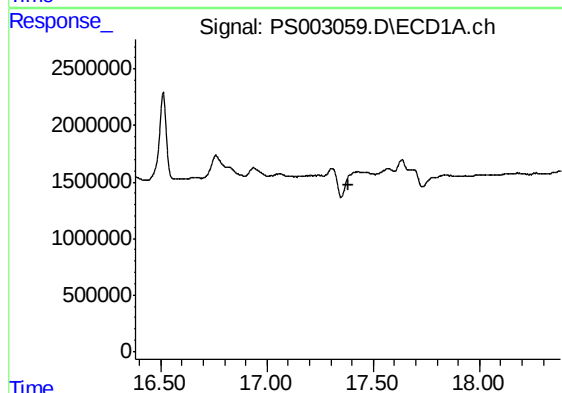

#16 DCPA

R.T.: 17.424 min
Delta R.T.: 0.043 min
Response: -1367742
Conc: N.D.

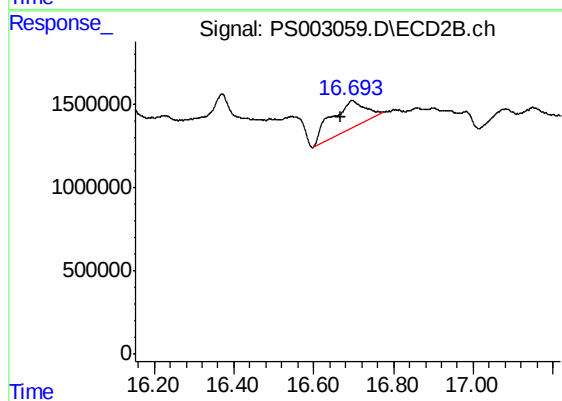

#16 DCPA

R.T.: 16.697 min
Delta R.T.: 0.027 min
Response: 10074410
Conc: 3.25 ng/ml