

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 22:10
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:53:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.281	10.775	171.1E6	294.4E6	450.570	688.549 #
Target Compounds							
1) T	Dalapon	2.844	2.307	132.6E6	352.2E6	240.358	657.148 #
3) T	4-Nitroph...	0.000	9.924	0	146.0E6	N.D.	698.492 #
5) T	DICAMBA	11.588	0.000	256.9E6	0	160.250	N.D. #
8) T	DICHLORPROP	12.778	12.181	8458195	263.5E6	22.054	689.083 #
9) T	2,4-D	0.000	12.652	0	91905756	N.D.	183.303 #
10) T	Pentachlo...	13.505	0.000	1103.1E6	0	172.013	N.D. #
11) T	2,4,5-TP ...	14.382	13.812	1773.4E6	1693.1E6	704.171	682.602
12) T	2,4,5-T	14.780	14.375	1723.9E6	-445445093	706.708	N.D. #
14) T	DINOSEB	16.996	0.000	1306.5E6	0	694.478	N.D. #
15) T	Picloram	16.766	16.682	2156.0E6	2045.2E6	681.496	680.267
16) T	DCPA	17.341	16.682	687.7E6	2045.2E6	228.672	660.241 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 22:10
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 23:53:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

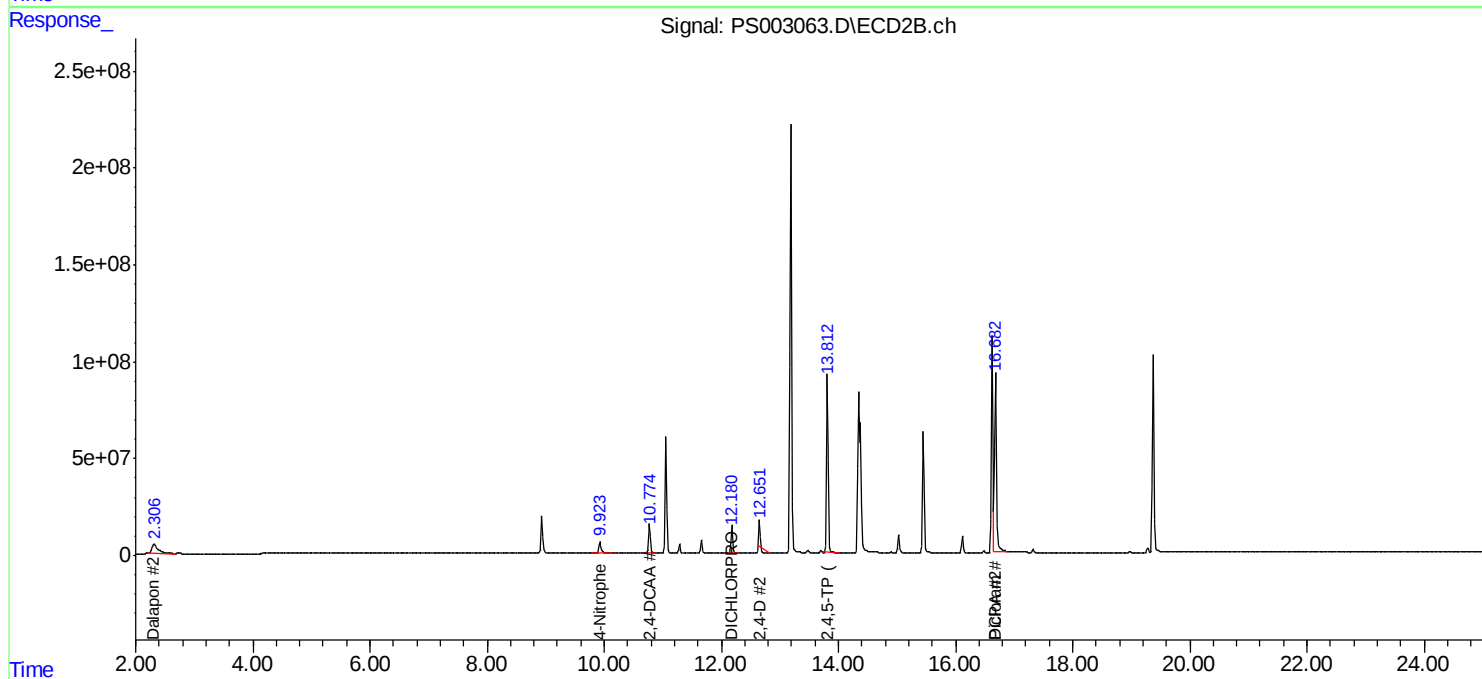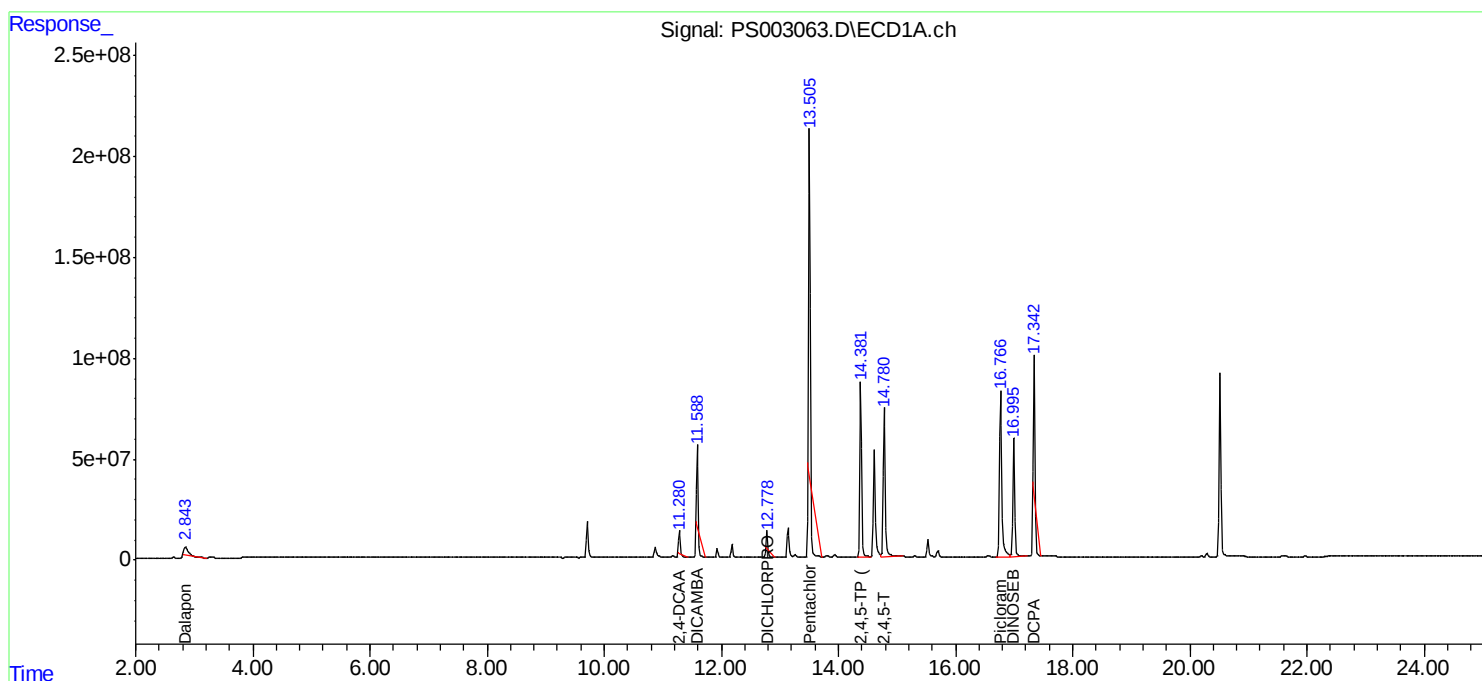


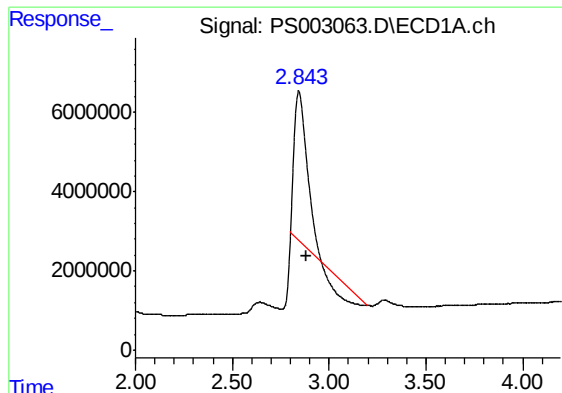

#1 Dalapon


R.T.: 2.844 min
Delta R.T.: -0.036 min
Response: 132593027
Conc: 240.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

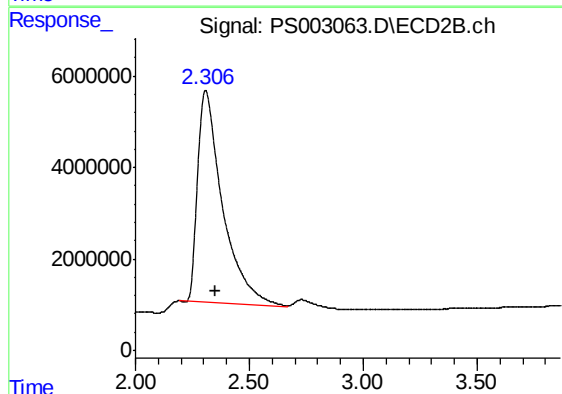


#1 Dalapon

R.T.: 2.307 min
Delta R.T.: -0.044 min
Response: 352179480
Conc: 657.15 ng/ml

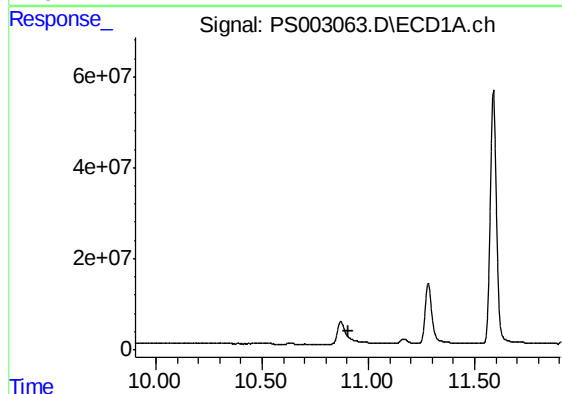


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.904 min
Response: 0
Conc: N.D.

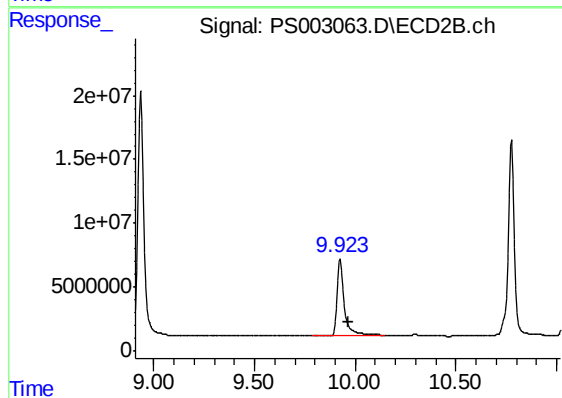

#3 4-Nitrophenol


R.T.: 9.924 min
Delta R.T.: -0.041 min
Response: 146000595
Conc: 698.49 ng/ml

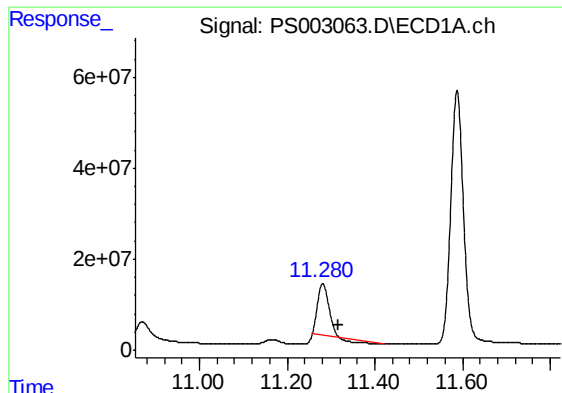

#4 2,4-DCAA


R.T.: 11.281 min
Delta R.T.: -0.037 min
Response: 171054573
Conc: 450.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

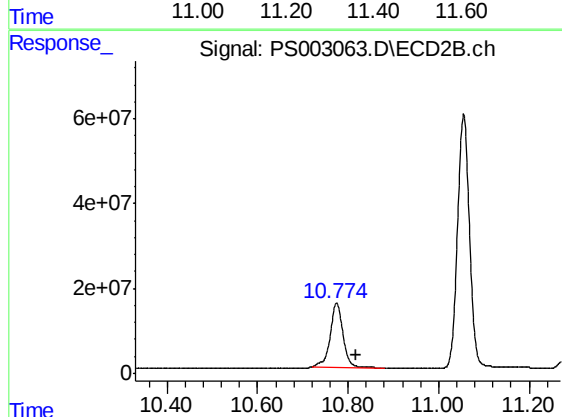


#4 2,4-DCAA

R.T.: 10.775 min
Delta R.T.: -0.042 min
Response: 294386122
Conc: 688.55 ng/ml

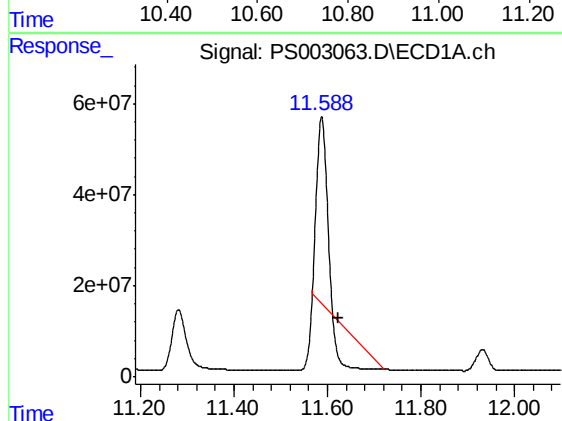


#5 DICAMBA

R.T.: 11.588 min
Delta R.T.: -0.036 min
Response: 256862300
Conc: 160.25 ng/ml

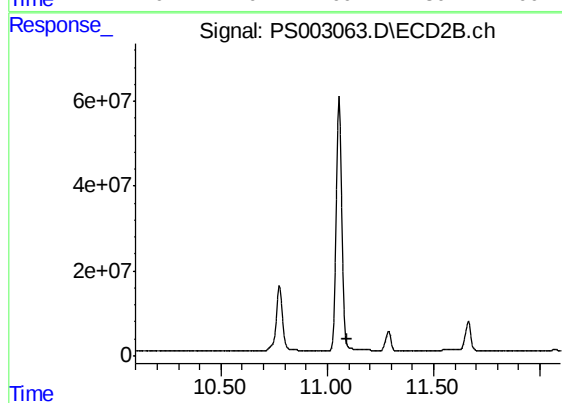

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.097 min
Response: 0
Conc: N.D.

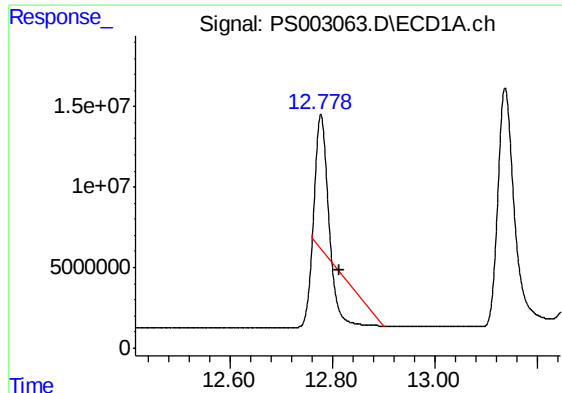

#8 DICHLORPROP


R.T.: 12.778 min
Delta R.T.: -0.037 min
Response: 8458195
Conc: 22.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

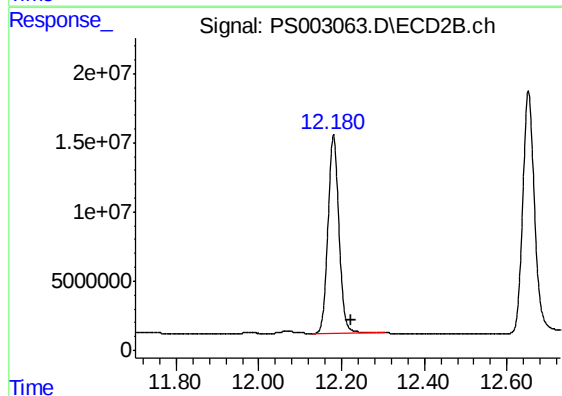


#8 DICHLORPROP

R.T.: 12.181 min
Delta R.T.: -0.042 min
Response: 263464881
Conc: 689.08 ng/ml

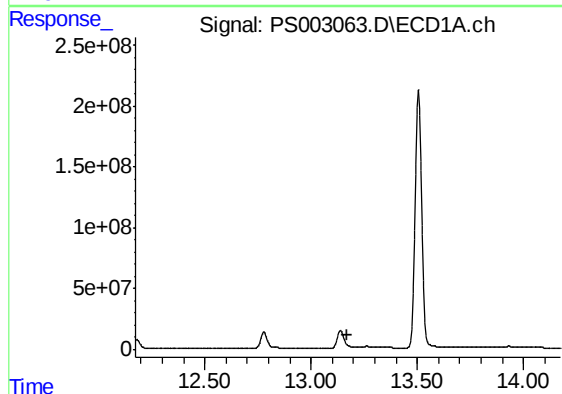


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.173 min
Response: 0
Conc: N.D.

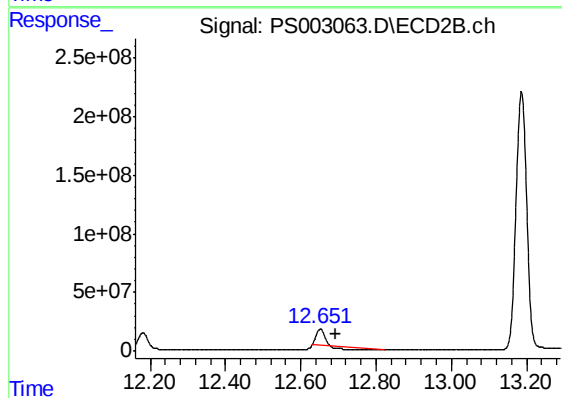

#9 2,4-D


R.T.: 12.652 min
Delta R.T.: -0.041 min
Response: 91905756
Conc: 183.30 ng/ml

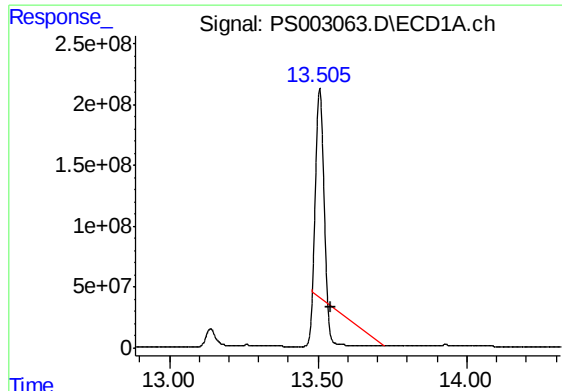

#10 Pentachlorophenol


R.T.: 13.505 min
Delta R.T.: -0.038 min
Response: 1103118650
Conc: 172.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

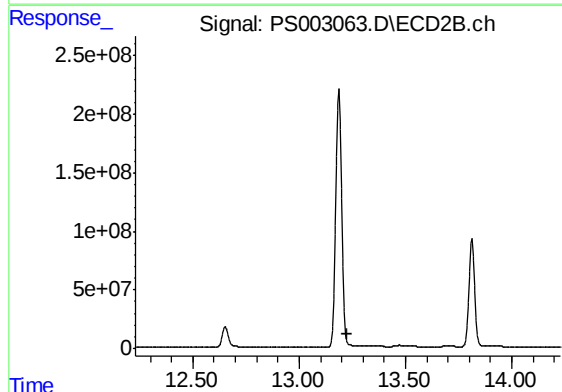


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.229 min
Response: 0
Conc: N.D.

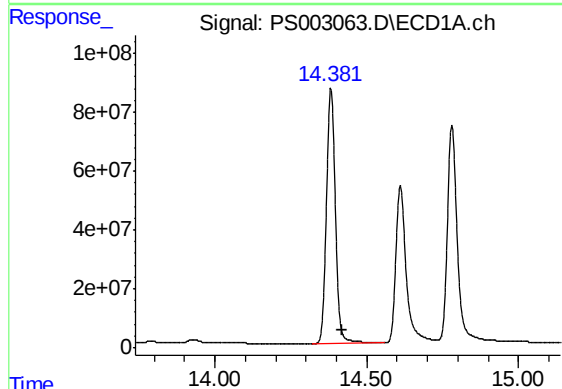


#11 2,4,5-TP (SILVEX)

R.T.: 14.382 min
Delta R.T.: -0.038 min
Response: 1773366238
Conc: 704.17 ng/ml

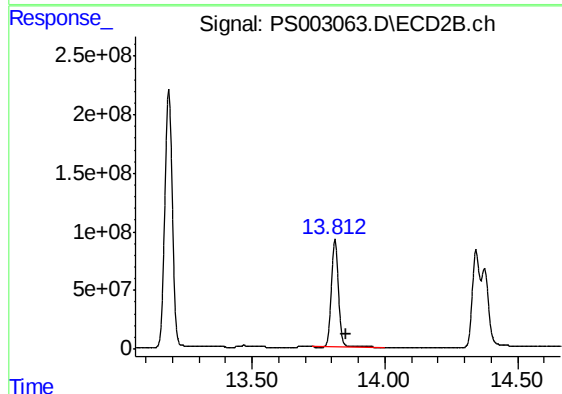

#11 2,4,5-TP (SILVEX)


R.T.: 13.812 min
Delta R.T.: -0.042 min
Response: 1693095784
Conc: 682.60 ng/ml

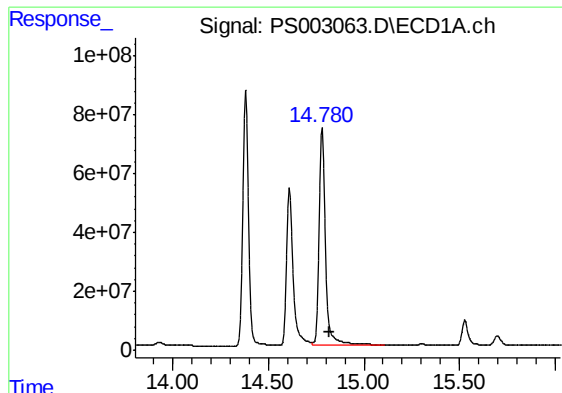

#12 2,4,5-T


R.T.: 14.780 min
Delta R.T.: -0.036 min
Response: 1723946955
Conc: 706.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

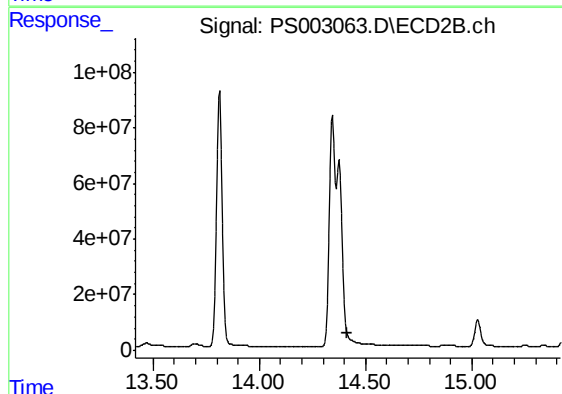


#12 2,4,5-T

R.T.: 14.375 min
Delta R.T.: -0.042 min
Response: -445445093
Conc: N.D.

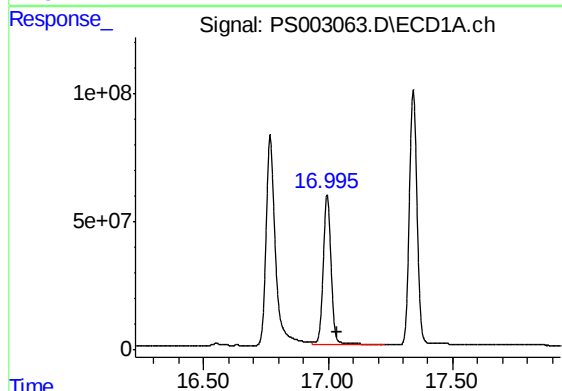


#14 DINOSEB

R.T.: 16.996 min
Delta R.T.: -0.040 min
Response: 1306539825
Conc: 694.48 ng/ml

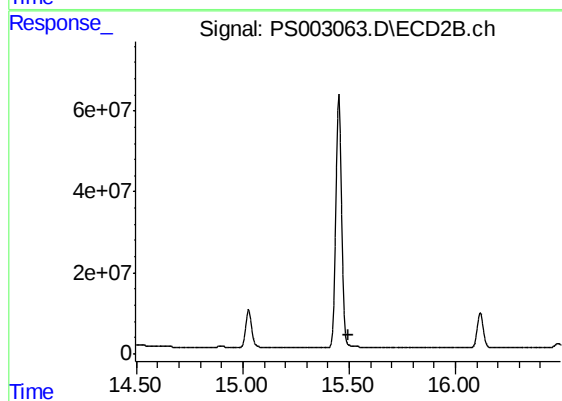

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

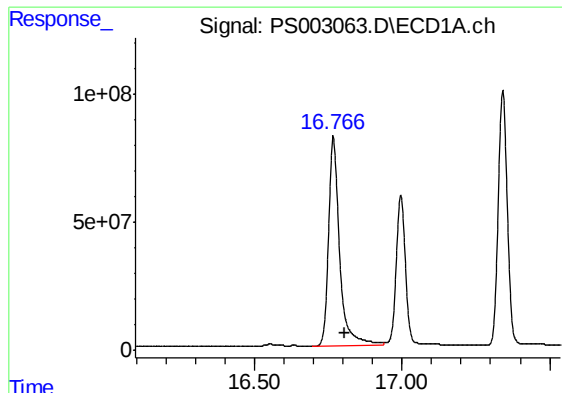

#15 Picloram


R.T.: 16.766 min
Delta R.T.: -0.039 min
Response: 2156002850
Conc: 681.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

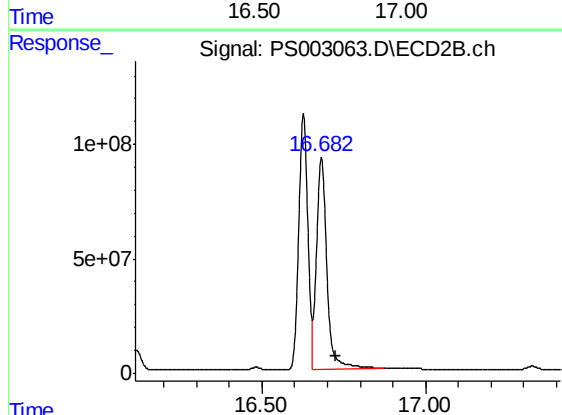


#15 Picloram

R.T.: 16.682 min
Delta R.T.: -0.042 min
Response: 2045155977
Conc: 680.27 ng/ml

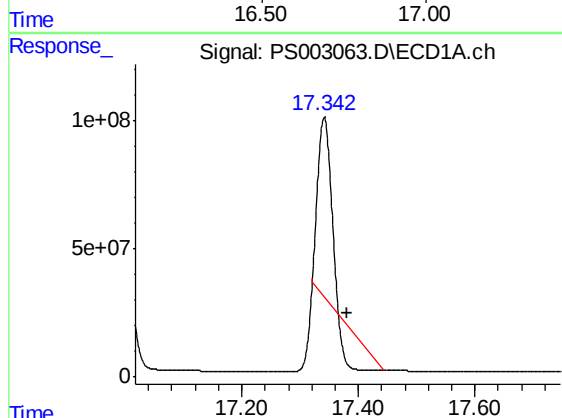

#16 DCPA

R.T.: 17.341 min
Delta R.T.: -0.040 min
Response: 687684322
Conc: 228.67 ng/ml

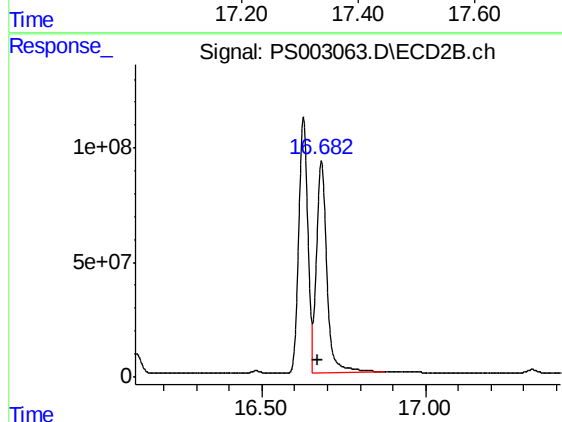

#16 DCPA

R.T.: 16.682 min
Delta R.T.: 0.012 min
Response: 2045155977
Conc: 660.24 ng/ml