

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 22:41
 Operator : EI\SJ
 Sample : K1338-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-06-020519-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:54:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.777	145.6E6	235.4E6	383.632	550.479 #
Target Compounds							
1) T	Dalapon	0.000	2.286	0	51848241	N.D.	96.746 #
2) T	3,5-DICHL...	0.000	8.945	0	8699835	N.D.	15.437 #
3) T	4-Nitroph...	0.000	9.963	0	1497362	N.D.	7.164 #
7) T	MCPA	12.243	0.000	1981751	0	1.120	N.D. #
10) T	Pentachlo...	0.000	13.274	0	2196382	N.D.	0.355 #
11) T	2,4,5-TP ...	14.463	0.000	9087745	0	3.609	N.D. #
12) T	2,4,5-T	0.000	14.432	0	2742745	N.D.	1.433 #
14) T	DINOSEB	0.000	15.484	0	7805334	N.D.	4.453 #
15) T	Picloram	16.785	16.696	12547803	19889537	3.966	6.616 #
16) T	DCPA	17.423	16.696	-3667524	19889537	N.D.	6.421



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 22:41
Operator : EI\SJ
Sample : K1338-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 23:54:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

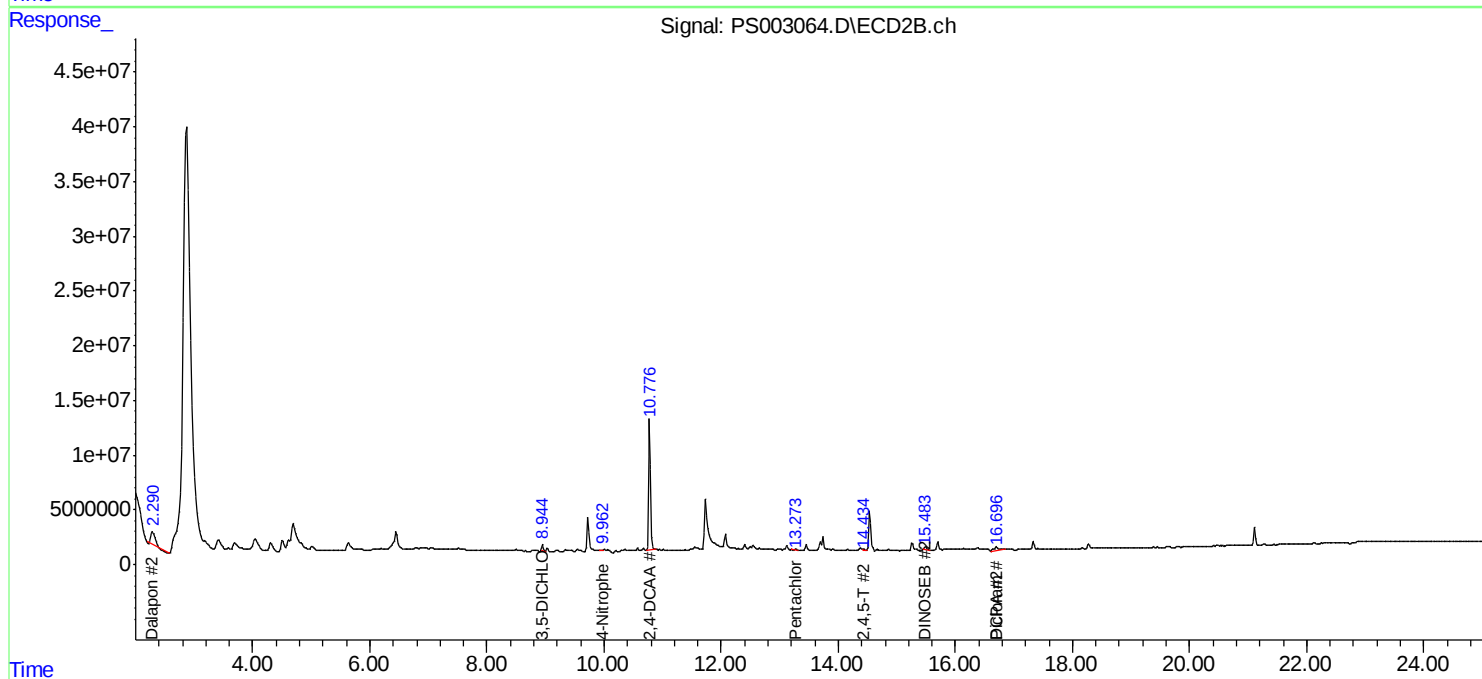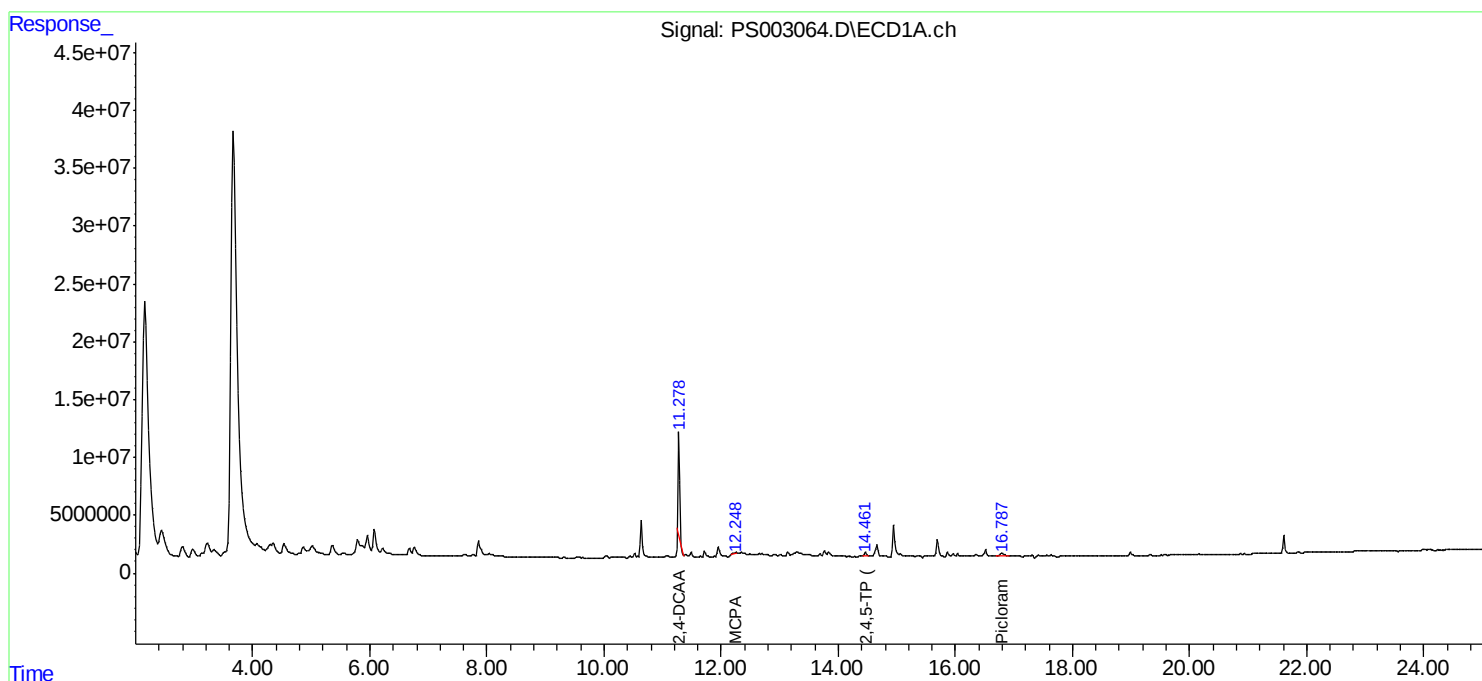


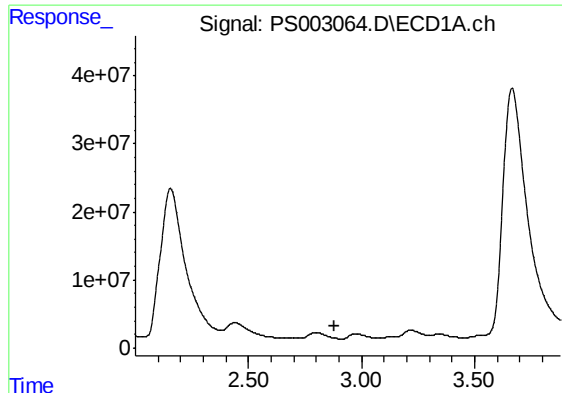

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-B

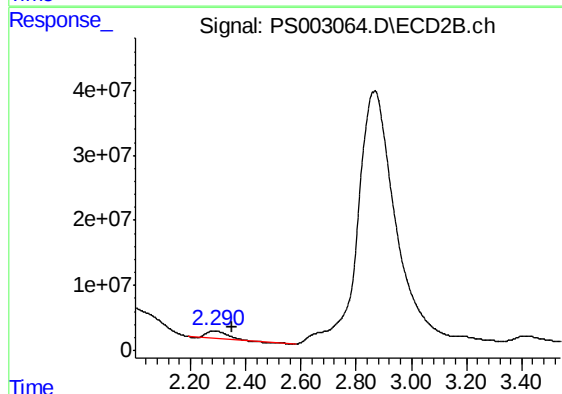


#1 Dalapon

R.T.: 2.286 min
Delta R.T.: -0.065 min
Response: 51848241
Conc: 96.75 ng/ml

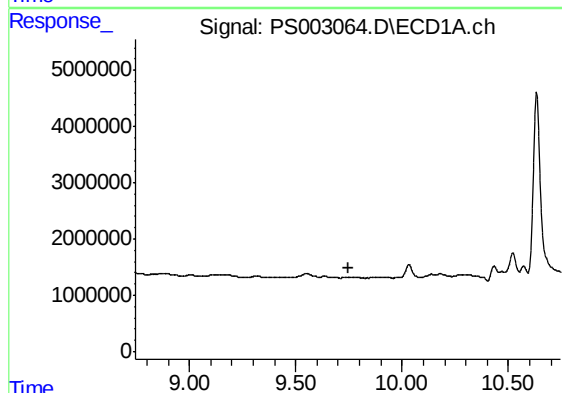


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

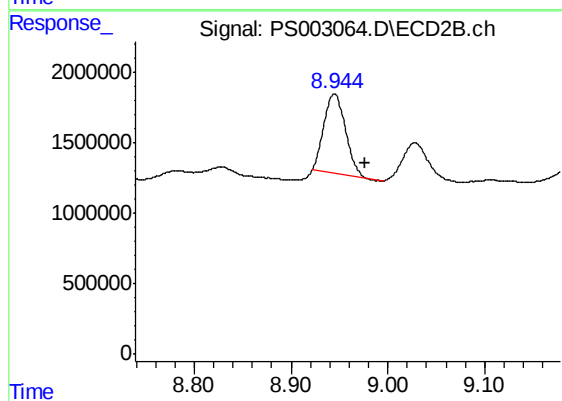

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.945 min
Delta R.T.: -0.032 min
Response: 8699835
Conc: 15.44 ng/ml

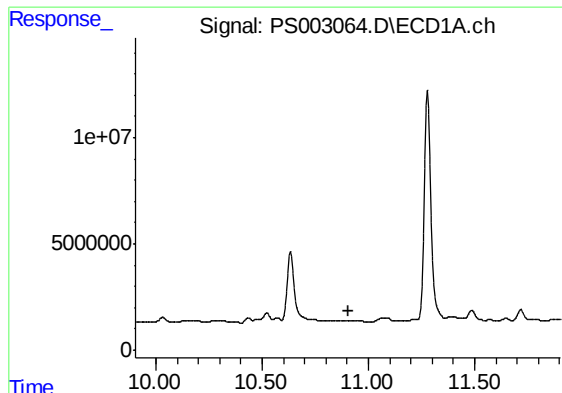

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-B

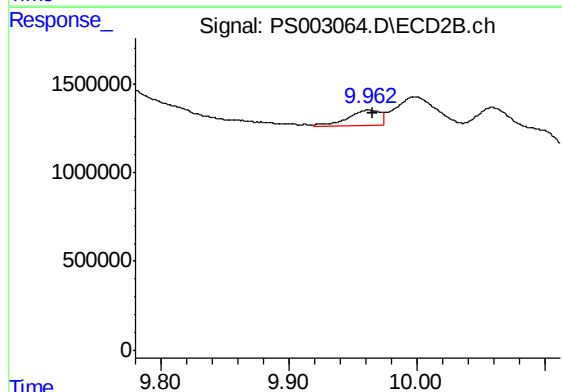


#3 4-Nitrophenol

R.T.: 9.963 min
Delta R.T.: -0.002 min
Response: 1497362
Conc: 7.16 ng/ml

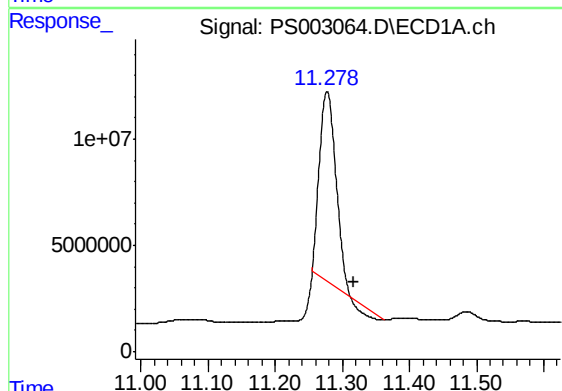


#4 2,4-DCAA

R.T.: 11.277 min
Delta R.T.: -0.040 min
Response: 145642350
Conc: 383.63 ng/ml

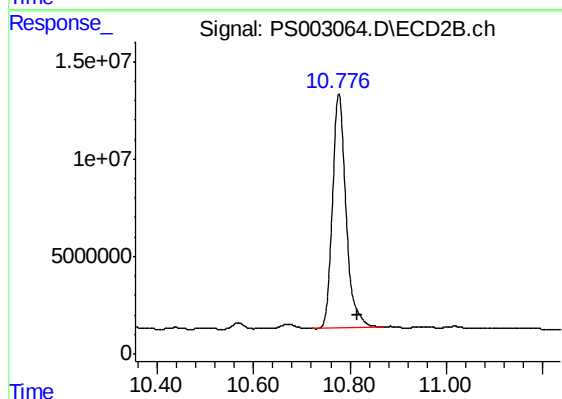

#4 2,4-DCAA


R.T.: 10.777 min
Delta R.T.: -0.040 min
Response: 235354798
Conc: 550.48 ng/ml

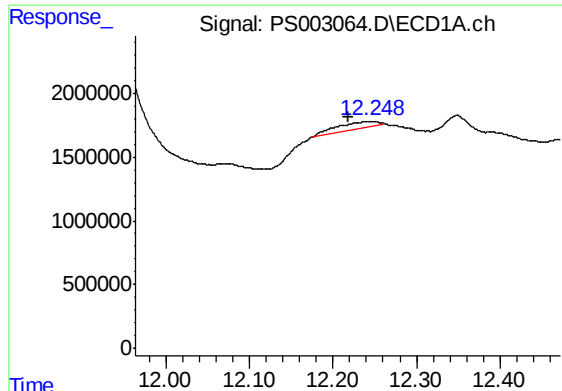

#7 MCPA


R.T.: 12.243 min
Delta R.T.: 0.024 min
Response: 1981751
Conc: 1.12 ug/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-B

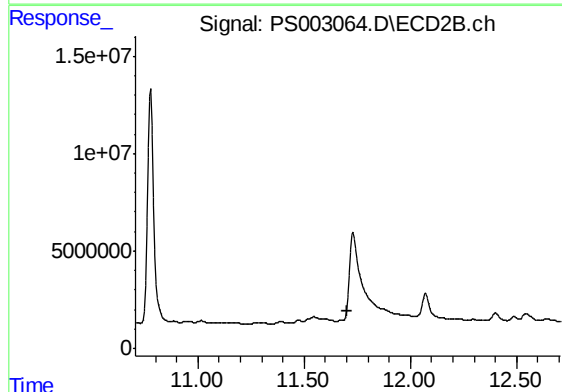


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

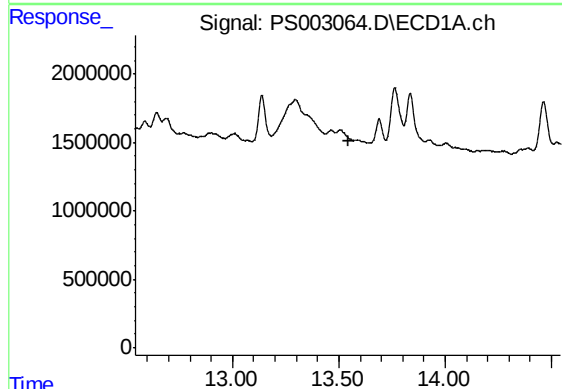


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.543 min
Response: 0
Conc: N.D.

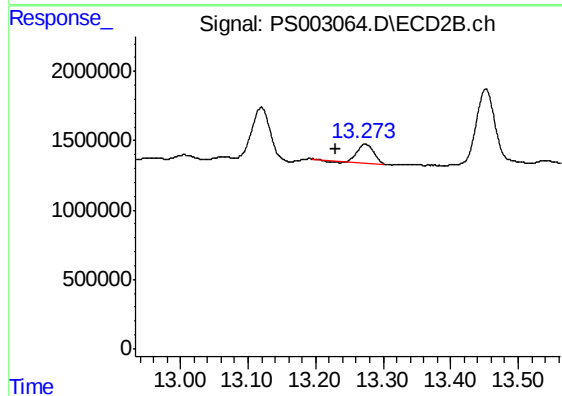

#10 Pentachlorophenol


R.T.: 13.274 min
Delta R.T.: 0.045 min
Response: 2196382
Conc: 0.36 ng/ml

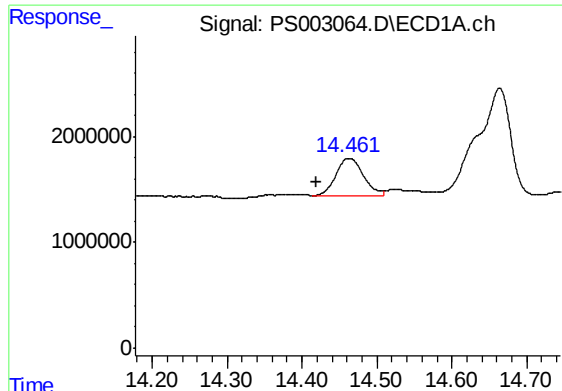

#11 2,4,5-TP (SILVEX)


R.T.: 14.463 min
Delta R.T.: 0.043 min
Response: 9087745
Conc: 3.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-B

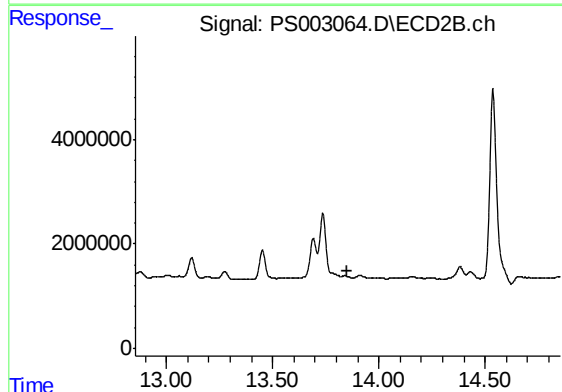


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

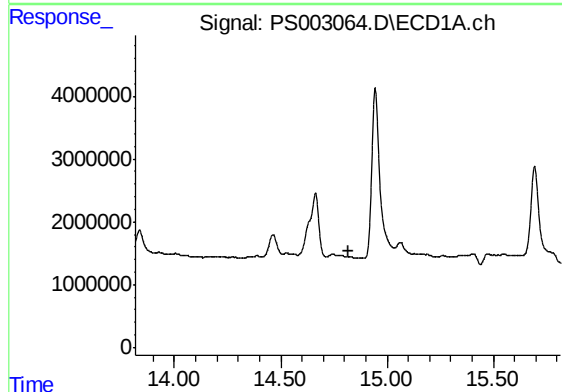


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

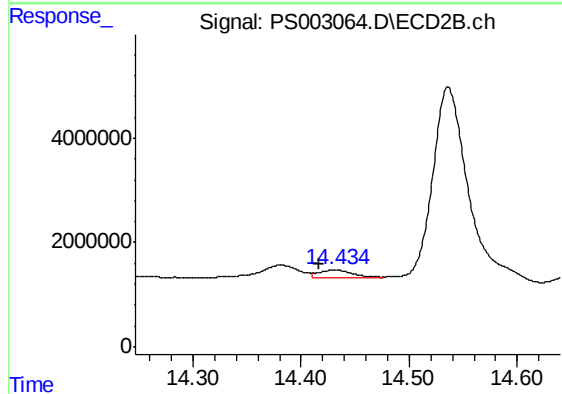

#12 2,4,5-T


R.T.: 14.432 min
Delta R.T.: 0.015 min
Response: 2742745
Conc: 1.43 ng/ml

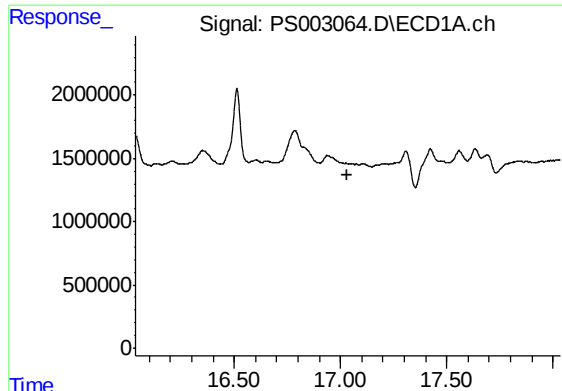

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-B

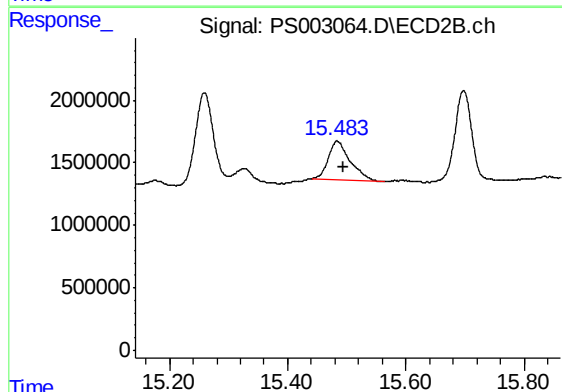


#14 DINOSEB

R.T.: 15.484 min
Delta R.T.: -0.011 min
Response: 7805334
Conc: 4.45 ng/ml

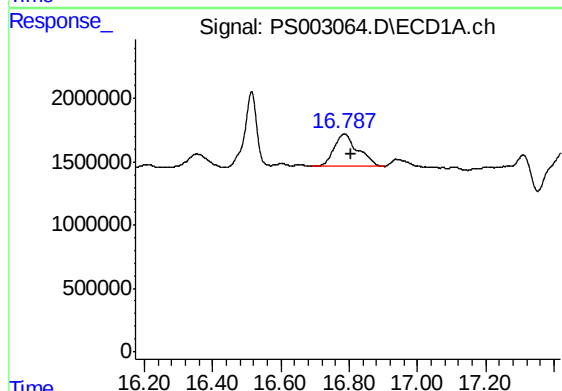


#15 Picloram

R.T.: 16.785 min
Delta R.T.: -0.020 min
Response: 12547803
Conc: 3.97 ng/ml

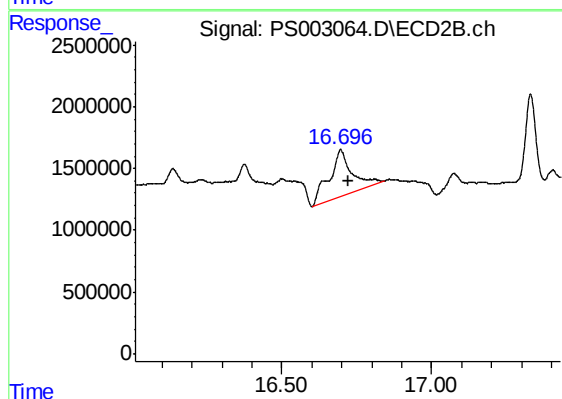

#15 Picloram


R.T.: 16.696 min
Delta R.T.: -0.028 min
Response: 19889537
Conc: 6.62 ng/ml

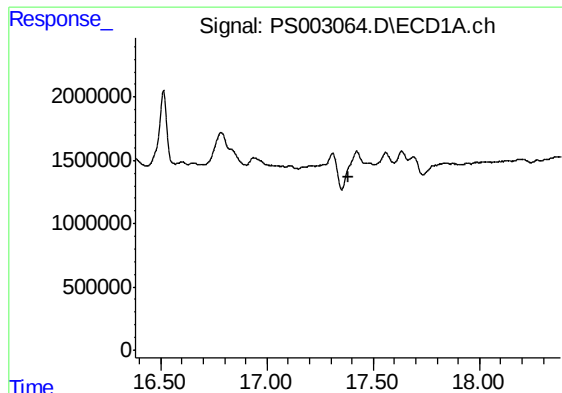

#16 DCPA

R.T.: 17.423 min
Delta R.T.: 0.041 min
Response: -3667524
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-B

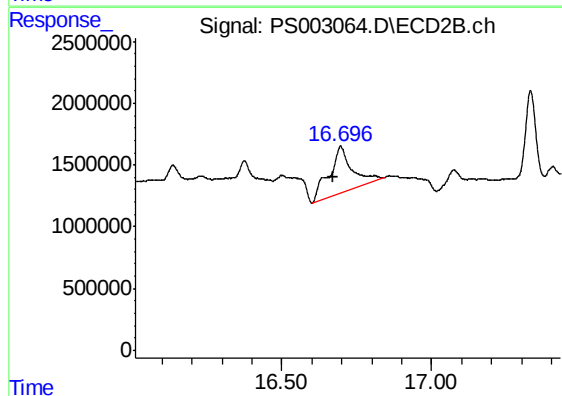

#16 DCPA

R.T.: 16.696 min
Delta R.T.: 0.026 min
Response: 19889537
Conc: 6.42 ng/ml