

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 23:12
 Operator : EI\SJ
 Sample : K1338-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-06-020519-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:54:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.776	100.4E6	235.2E6	264.584	550.193 #
Target Compounds							
1) T	Dalapon	0.000	2.285	0	44103530	N.D.	82.295 #
2) T	3,5-DICHL...	0.000	8.944	0	6807411	N.D.	12.079 #
3) T	4-Nitroph...	0.000	9.962	0	2190150	N.D.	10.478 #
10) T	Pentachlo...	0.000	13.272	0	2343271	N.D.	0.379 #
11) T	2,4,5-TP ...	14.462	0.000	7565007	0	3.004	N.D. #
12) T	2,4,5-T	0.000	14.431	0	2502909	N.D.	1.308 #
14) T	DINOSEB	0.000	15.483	0	8143081	N.D.	4.645 #
15) T	Picloram	16.766	16.699	9840348	16076718	3.110	5.347 #
16) T	DCPA	17.420	16.699	-6038200	16076718	N.D.	5.190



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 23:12
Operator : EI\SJ
Sample : K1338-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
AU-06-020519-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 23:54:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

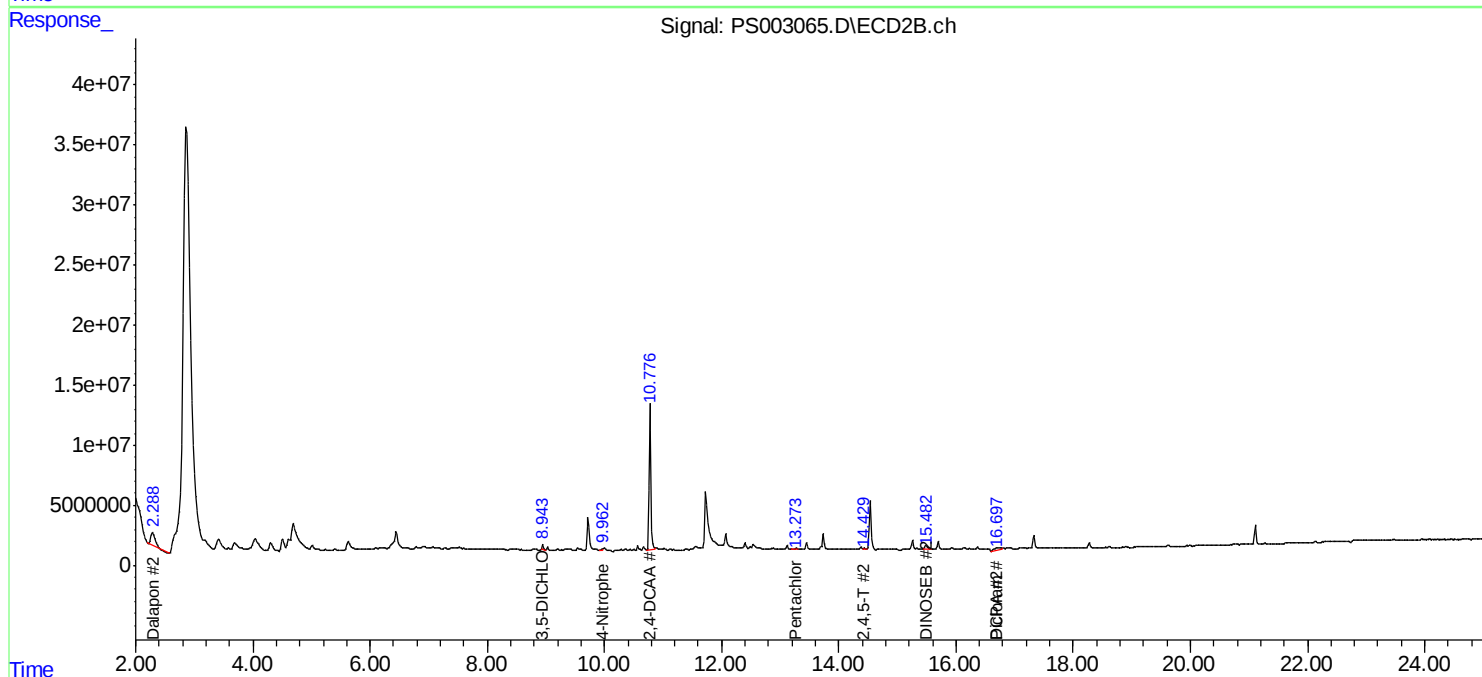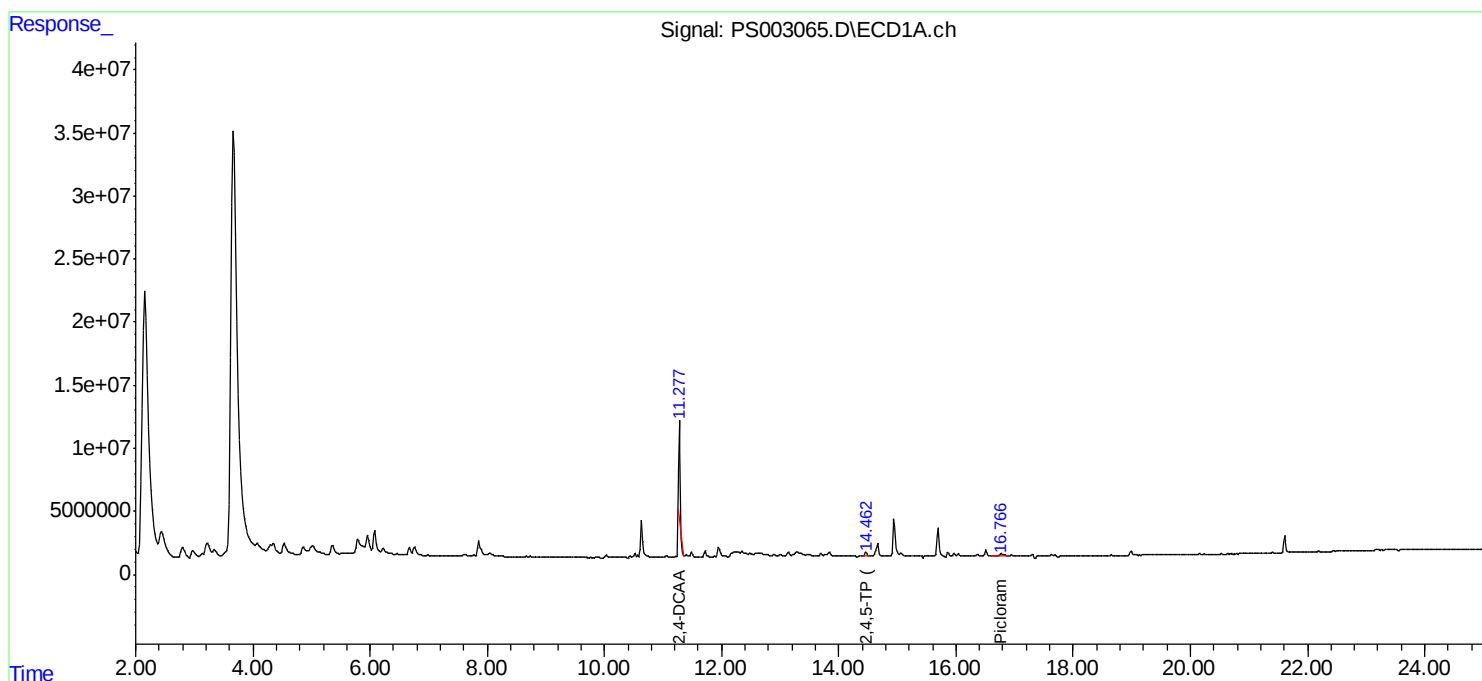


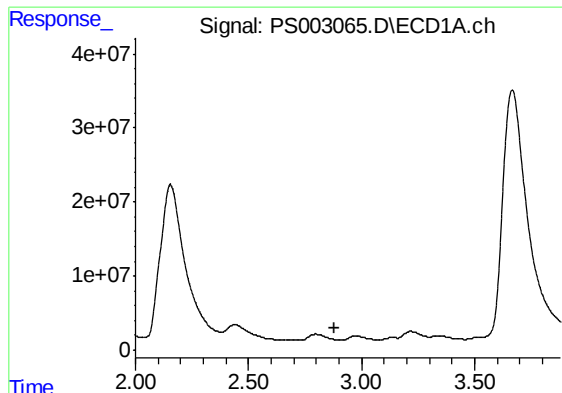

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-C

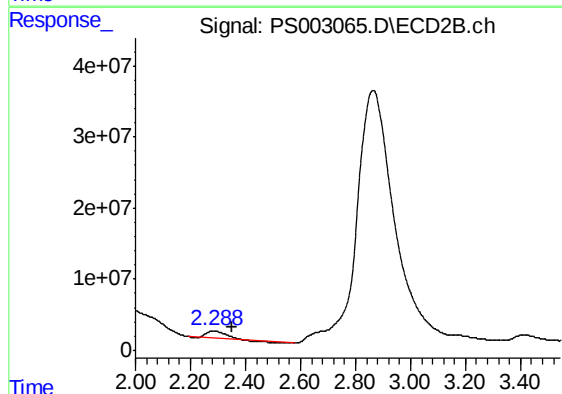


#1 Dalapon

R.T.: 2.285 min
Delta R.T.: -0.065 min
Response: 44103530
Conc: 82.29 ng/ml

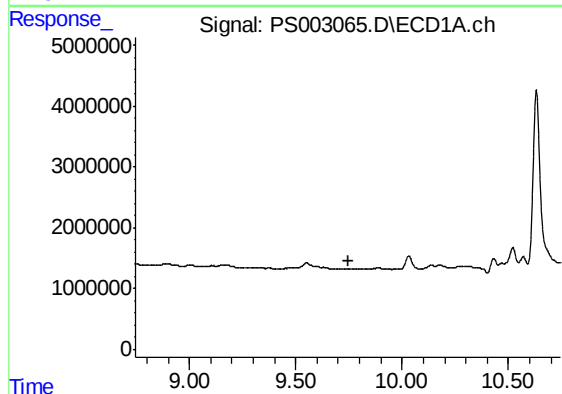


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

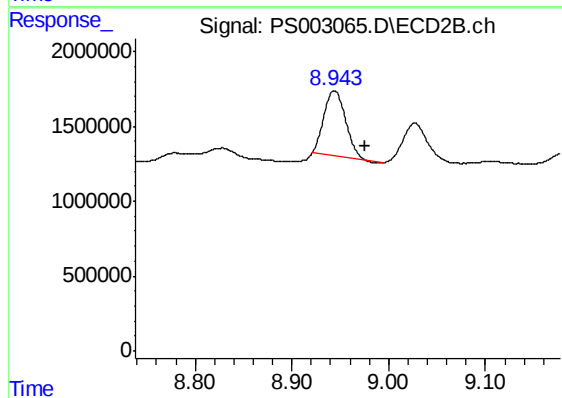

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.944 min
Delta R.T.: -0.032 min
Response: 6807411
Conc: 12.08 ng/ml

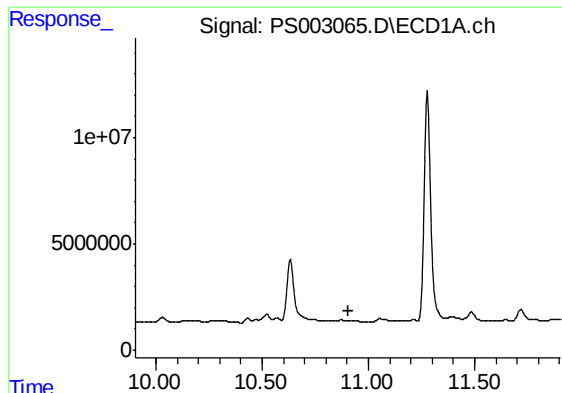

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-C

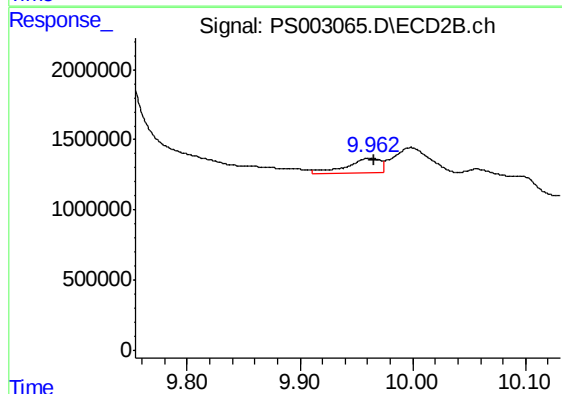


#3 4-Nitrophenol

R.T.: 9.962 min
Delta R.T.: -0.003 min
Response: 2190150
Conc: 10.48 ng/ml

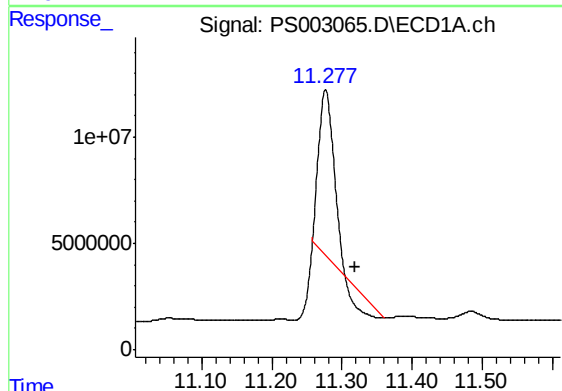


#4 2,4-DCAA

R.T.: 11.277 min
Delta R.T.: -0.041 min
Response: 100446981
Conc: 264.58 ng/ml

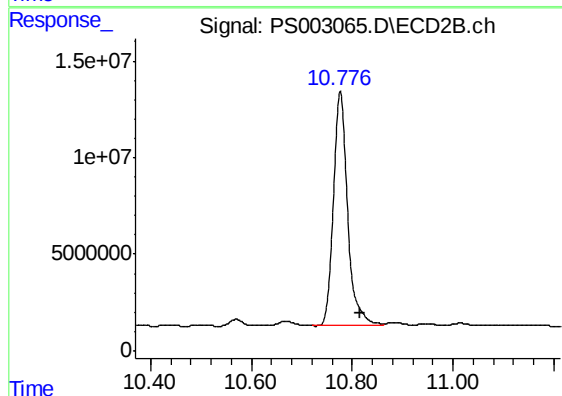

#4 2,4-DCAA


R.T.: 10.776 min
Delta R.T.: -0.040 min
Response: 235232457
Conc: 550.19 ng/ml

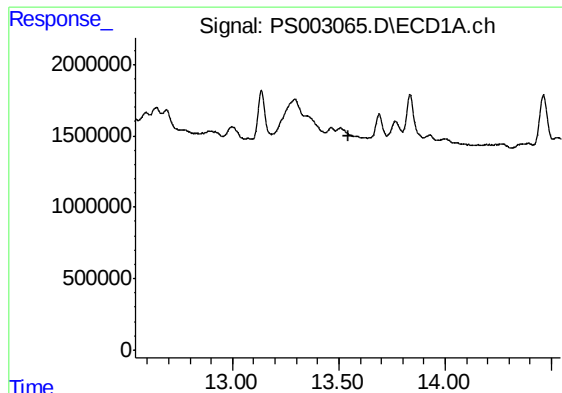

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-C

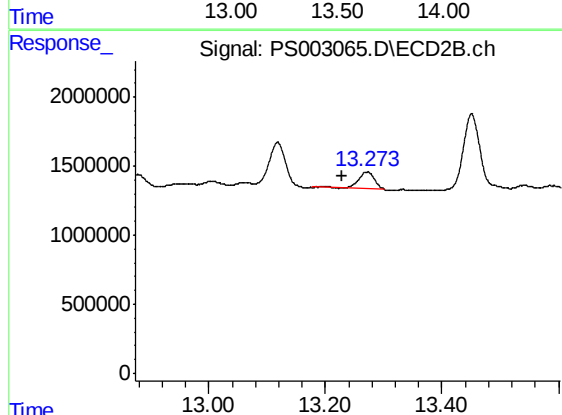


#10 Pentachlorophenol

R.T.: 13.272 min
Delta R.T.: 0.042 min
Response: 2343271
Conc: 0.38 ng/ml

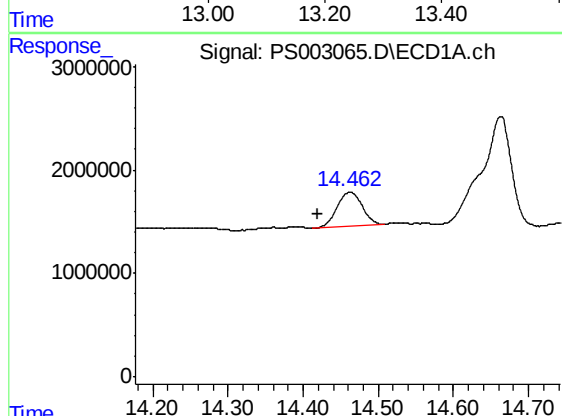


#11 2,4,5-TP (SILVEX)

R.T.: 14.462 min
Delta R.T.: 0.043 min
Response: 7565007
Conc: 3.00 ng/ml

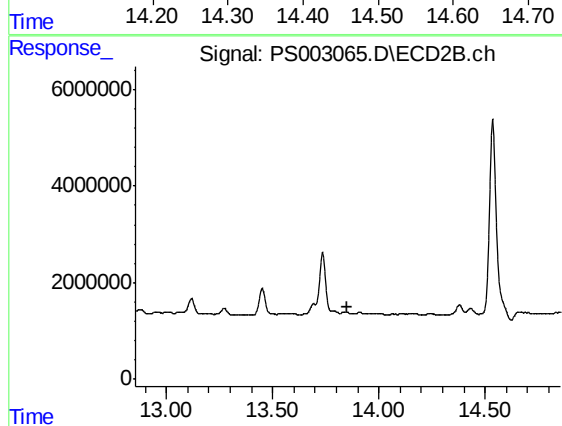

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.854 min
Response: 0
Conc: N.D.

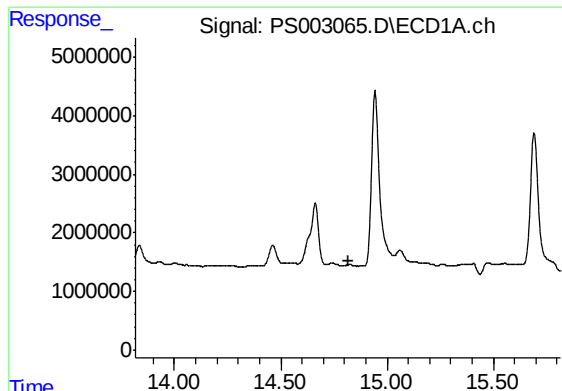

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-C

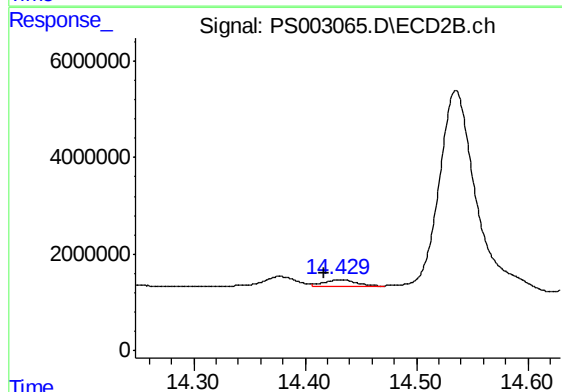


#12 2,4,5-T

R.T.: 14.431 min
Delta R.T.: 0.014 min
Response: 2502909
Conc: 1.31 ng/ml

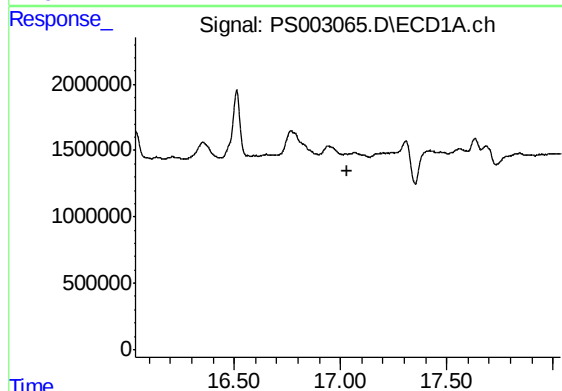


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.035 min
Response: 0
Conc: N.D.

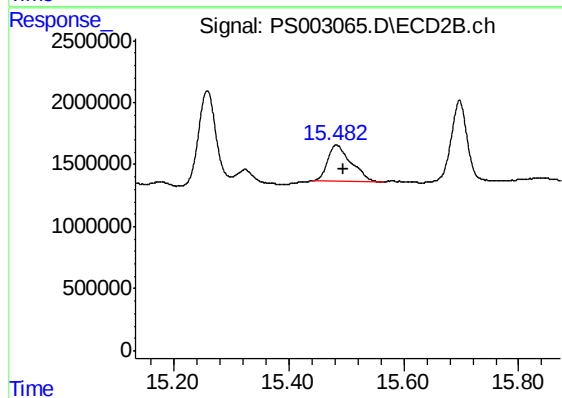

#14 DINOSEB


R.T.: 15.483 min
Delta R.T.: -0.012 min
Response: 8143081
Conc: 4.65 ng/ml

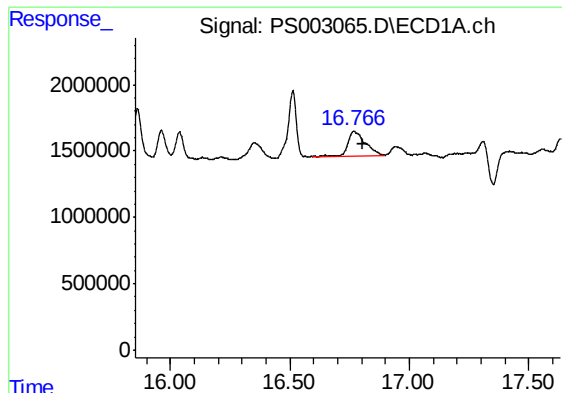

#15 Picloram


R.T.: 16.766 min
Delta R.T.: -0.039 min
Response: 9840348
Conc: 3.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-C

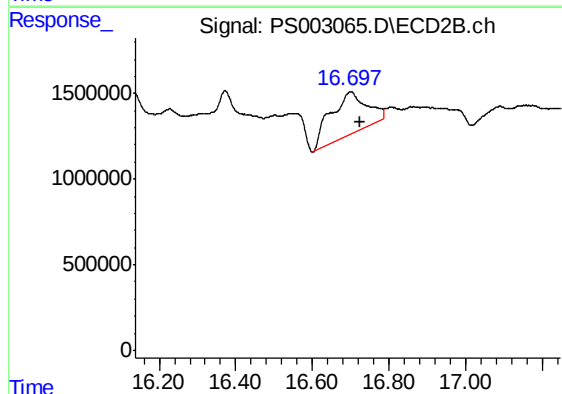


#15 Picloram

R.T.: 16.699 min
Delta R.T.: -0.026 min
Response: 16076718
Conc: 5.35 ng/ml

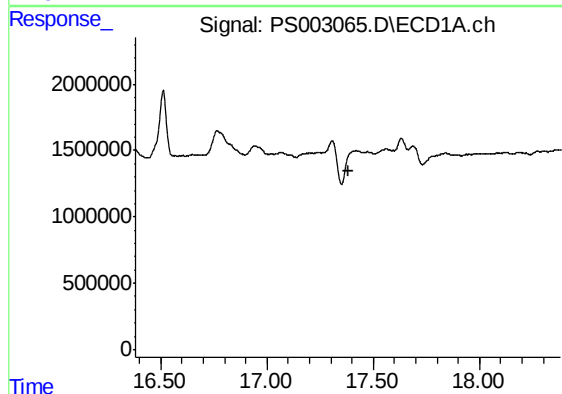

#16 DCPA

R.T.: 17.420 min
Delta R.T.: 0.039 min
Response: -6038200
Conc: N.D.

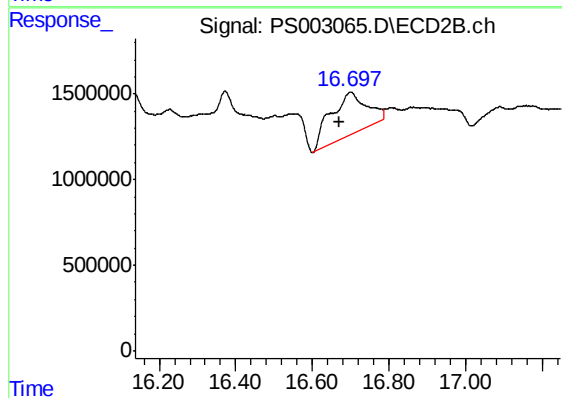

#16 DCPA

R.T.: 16.699 min
Delta R.T.: 0.029 min
Response: 16076718
Conc: 5.19 ng/ml