

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 23:43
 Operator : EI\SJ
 Sample : K1356-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 02:16:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.285	10.784	179.0E6	227.4E6	471.599	531.791
Target Compounds							
1) T	Dalapon	0.000	2.292	0	58024710	N.D.	108.271 #
2) T	3,5-DICHL...	0.000	8.952	0	9153952	N.D.	16.243 #
3) T	4-Nitroph...	0.000	9.970	0	2143174	N.D.	10.253 #
9) T	2,4-D	13.144	0.000	4781145	0	10.370	N.D. #
10) T	Pentachlo...	0.000	13.280	0	1630609	N.D.	0.264 #
11) T	2,4,5-TP ...	14.471	0.000	8173974	0	3.246	N.D. #
12) T	2,4,5-T	0.000	14.440	0	2426209	N.D.	1.268 #
14) T	DINOSEB	0.000	15.490	0	7393668	N.D.	4.218 #
15) T	Picloram	16.775	16.706	6938619	9962470	2.193	3.314 #
16) T	DCPA	17.424	16.706	-4711713	9962470	N.D.	3.216



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 23:43
Operator : EI\SJ
Sample : K1356-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 02:16:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

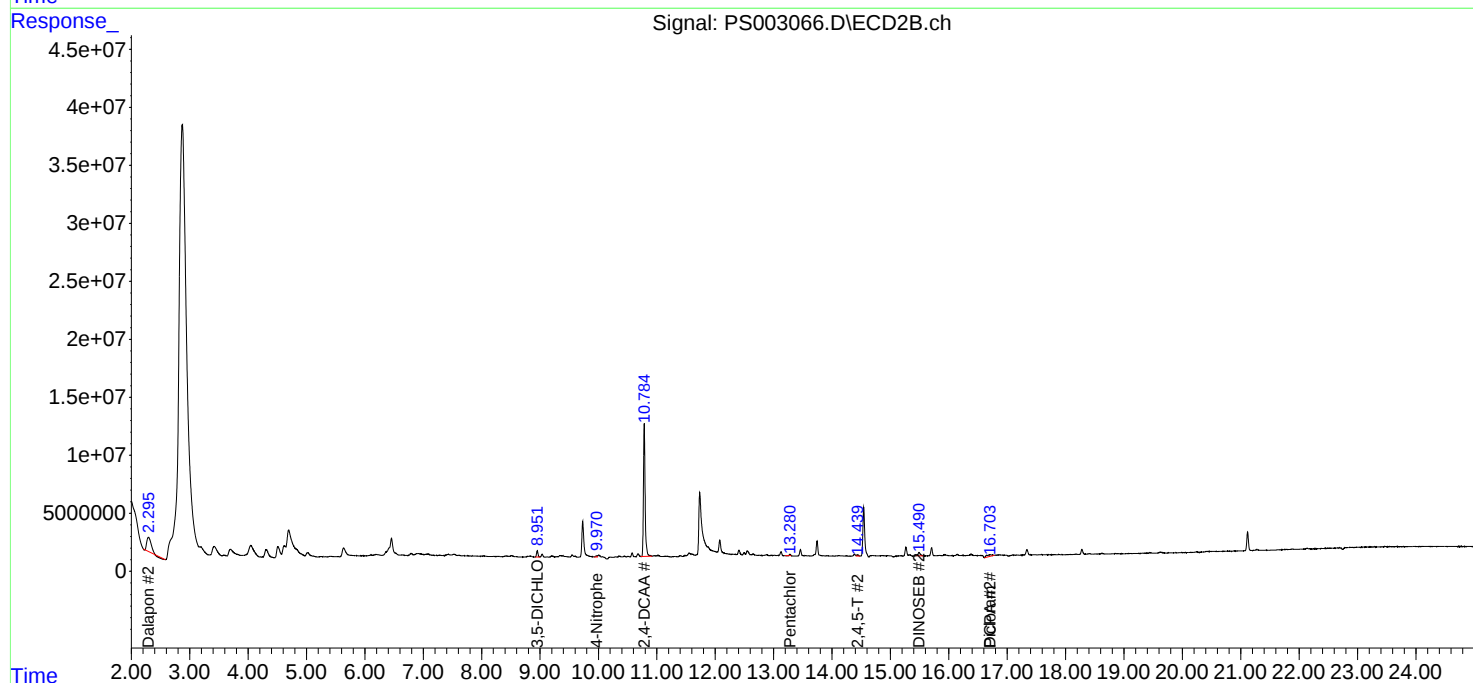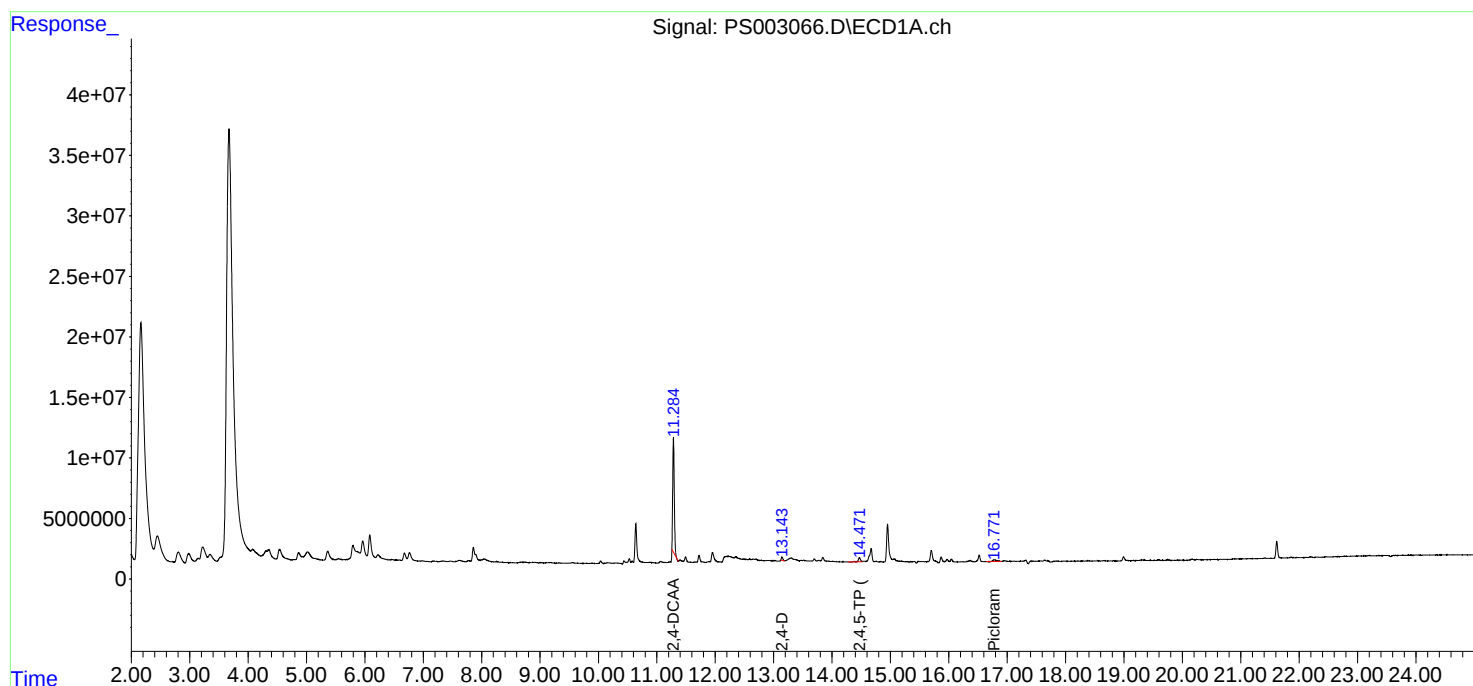


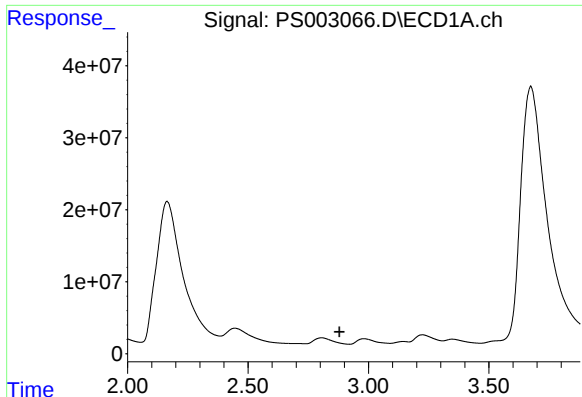

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

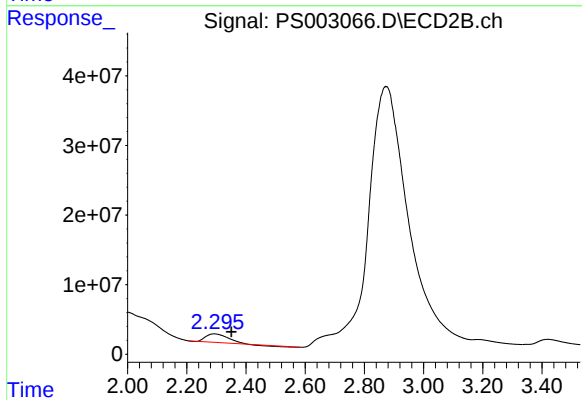


#1 Dalapon

R.T.: 2.292 min
Delta R.T.: -0.058 min
Response: 58024710
Conc: 108.27 ng/ml

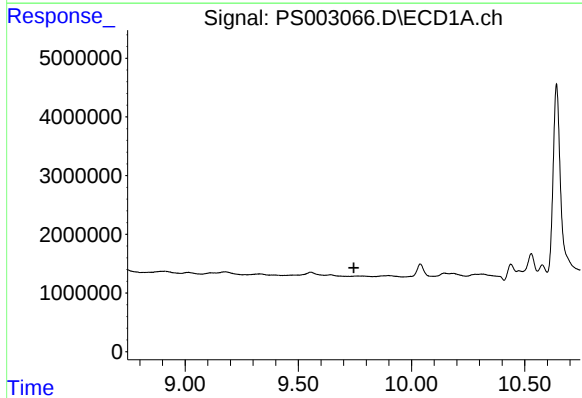


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

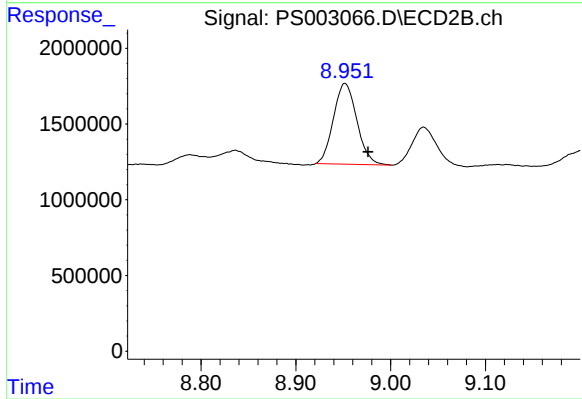

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.952 min
Delta R.T.: -0.024 min
Response: 9153952
Conc: 16.24 ng/ml

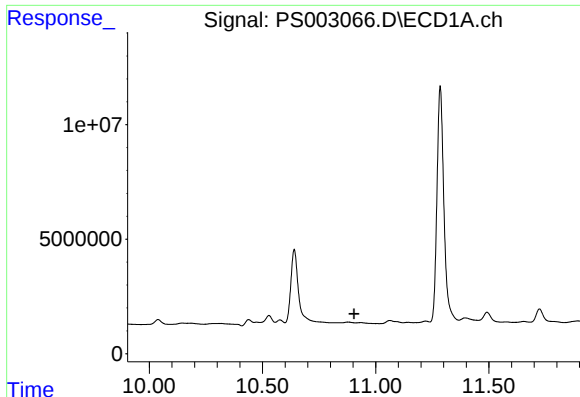

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

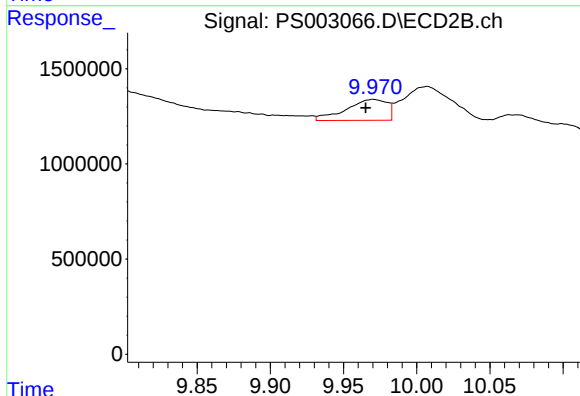


#3 4-Nitrophenol

R.T.: 9.970 min
Delta R.T.: 0.005 min
Response: 2143174
Conc: 10.25 ng/ml

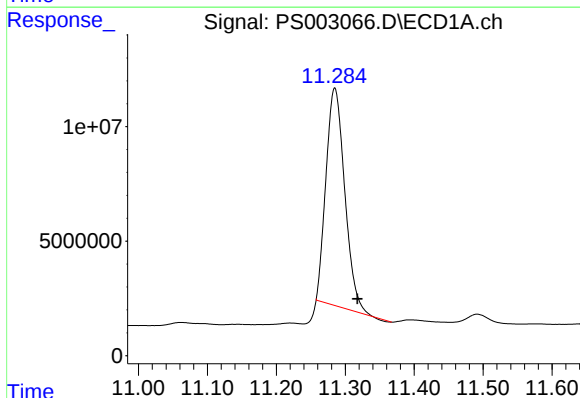


#4 2,4-DCAA

R.T.: 11.285 min
Delta R.T.: -0.033 min
Response: 179038253
Conc: 471.60 ng/ml

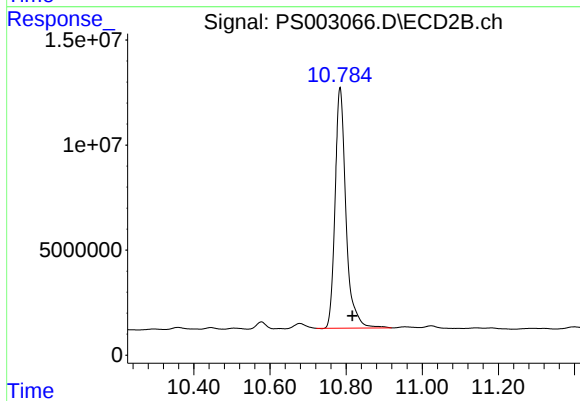

#4 2,4-DCAA


R.T.: 10.784 min
Delta R.T.: -0.032 min
Response: 227364860
Conc: 531.79 ng/ml

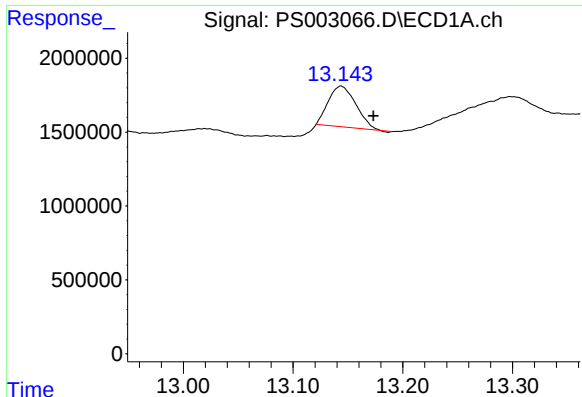

#9 2,4-D


R.T.: 13.144 min
Delta R.T.: -0.029 min
Response: 4781145
Conc: 10.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

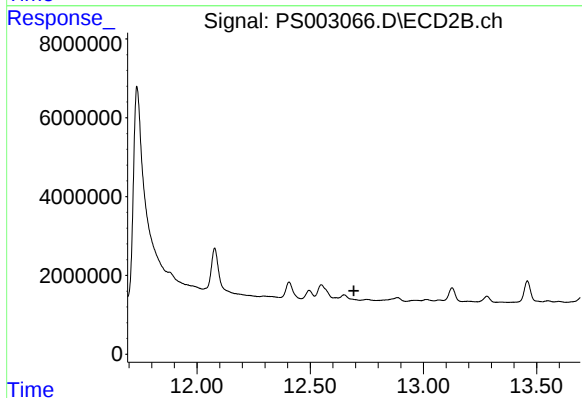


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

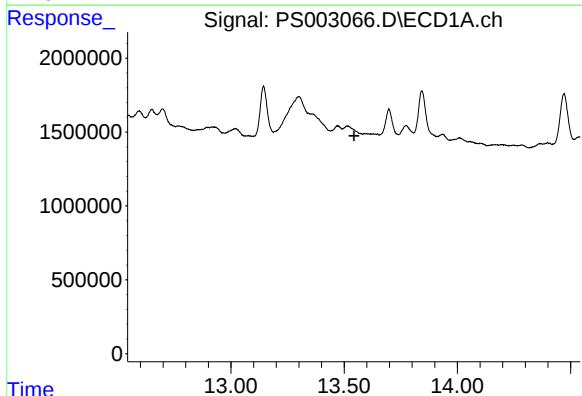


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.543 min
Response: 0
Conc: N.D.

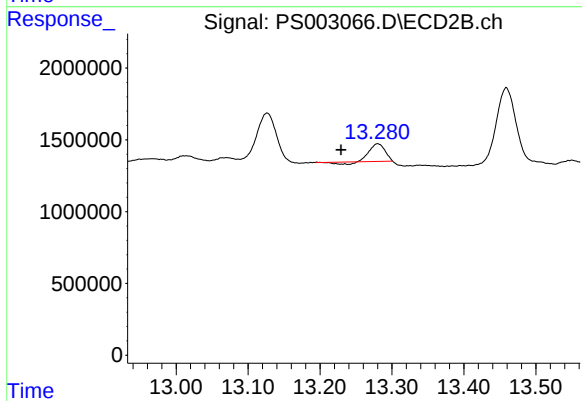

#10 Pentachlorophenol


R.T.: 13.280 min
Delta R.T.: 0.051 min
Response: 1630609
Conc: 0.26 ng/ml

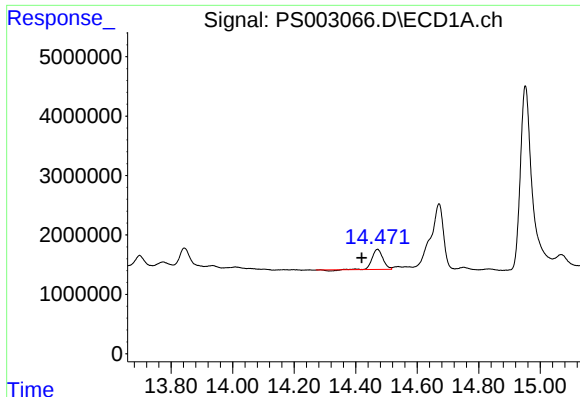

#11 2,4,5-TP (SILVEX)


R.T.: 14.471 min
Delta R.T.: 0.051 min
Response: 8173974
Conc: 3.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

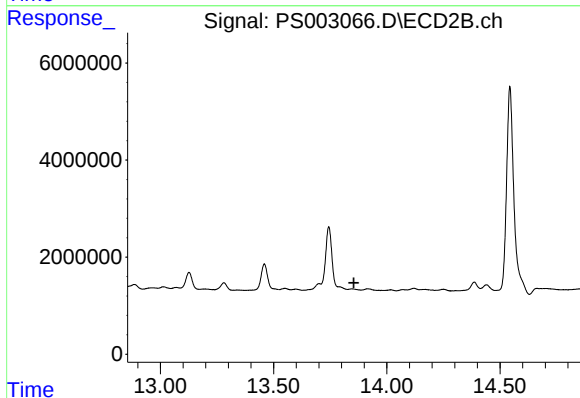


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

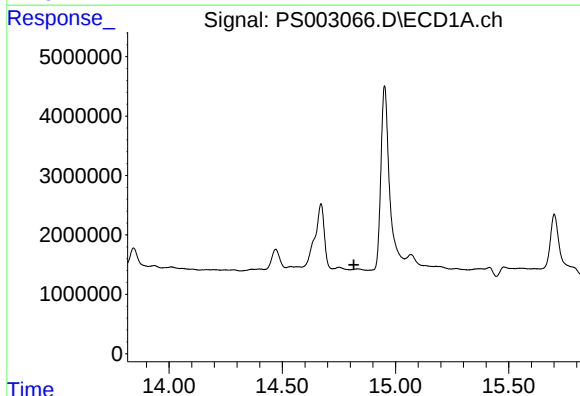


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

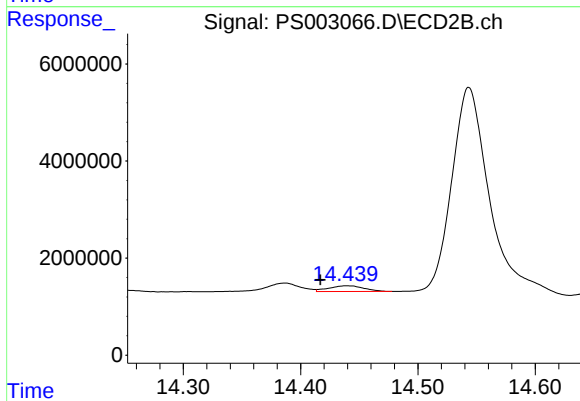

#12 2,4,5-T


R.T.: 14.440 min
Delta R.T.: 0.023 min
Response: 2426209
Conc: 1.27 ng/ml

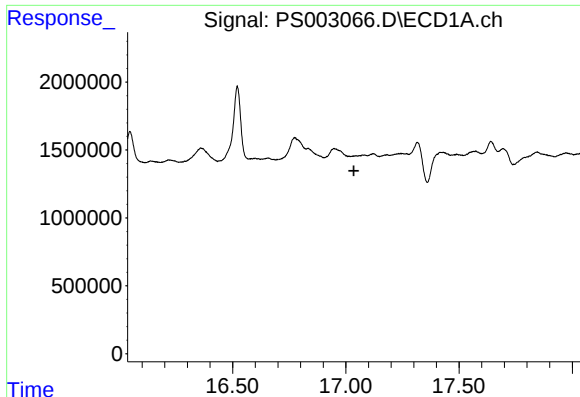

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

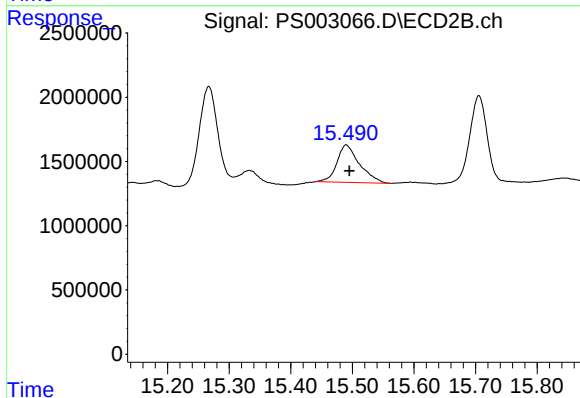


#14 DINOSEB

R.T.: 15.490 min
Delta R.T.: -0.005 min
Response: 7393668
Conc: 4.22 ng/ml

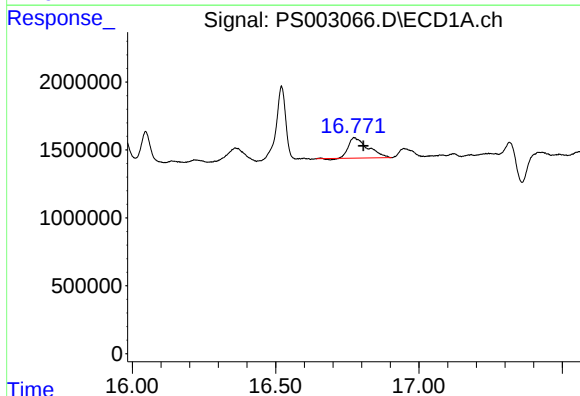


#15 Picloram

R.T.: 16.775 min
Delta R.T.: -0.031 min
Response: 6938619
Conc: 2.19 ng/ml

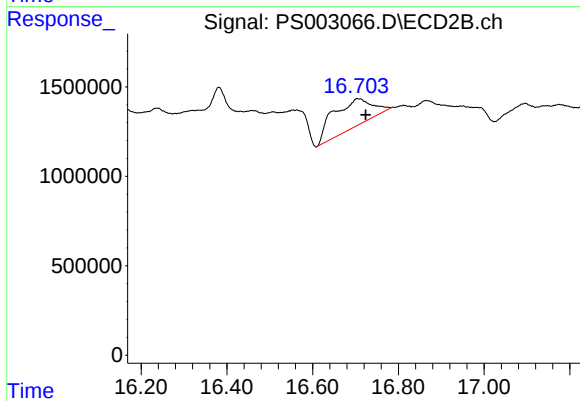

#15 Picloram


R.T.: 16.706 min
Delta R.T.: -0.019 min
Response: 9962470
Conc: 3.31 ng/ml

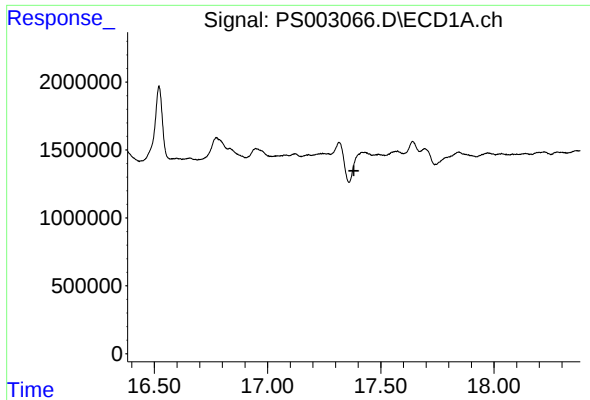

#16 DCPA

R.T.: 17.424 min
Delta R.T.: 0.042 min
Response: -4711713
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

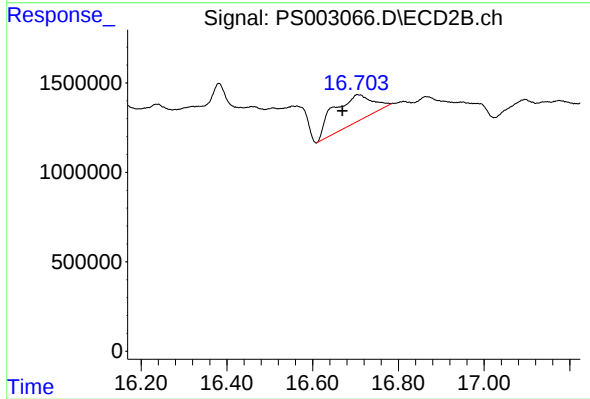

#16 DCPA

R.T.: 16.706 min
Delta R.T.: 0.036 min
Response: 9962470
Conc: 3.22 ng/ml