

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2019 00:14
 Operator : EI\SJ
 Sample : K1356-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 02:16:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.310	10.810	213.8E6	220.1E6	563.247	514.904
Target Compounds							
1) T	Dalapon	2.831	2.321	15186558	75084151	27.529	140.103 #
2) T	3,5-DICHL...	0.000	8.978	0	7876840	N.D.	13.977 #
3) T	4-Nitroph...	0.000	9.997	0	2500146	N.D.	11.961 #
6) T	MCP	11.982	0.000	8316804	0	6.942	N.D. #
7) T	MCPA	0.000	11.762	0	138.8E6	N.D.	88.213 #
9) T	2,4-D	13.169	0.000	6726082	0	14.588	N.D. #
12) T	2,4,5-T	0.000	14.412	0	3548034	N.D.	1.854 #
14) T	DINOSEB	0.000	15.517	0	8525208	N.D.	4.863 #
15) T	Picloram	16.796	16.736	6939764	13355091	2.194	4.442 #
16) T	DCPA	0.000	16.736	0	13355091	N.D.	4.311 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2019 00:14
Operator : EI\SJ
Sample : K1356-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 02:16:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

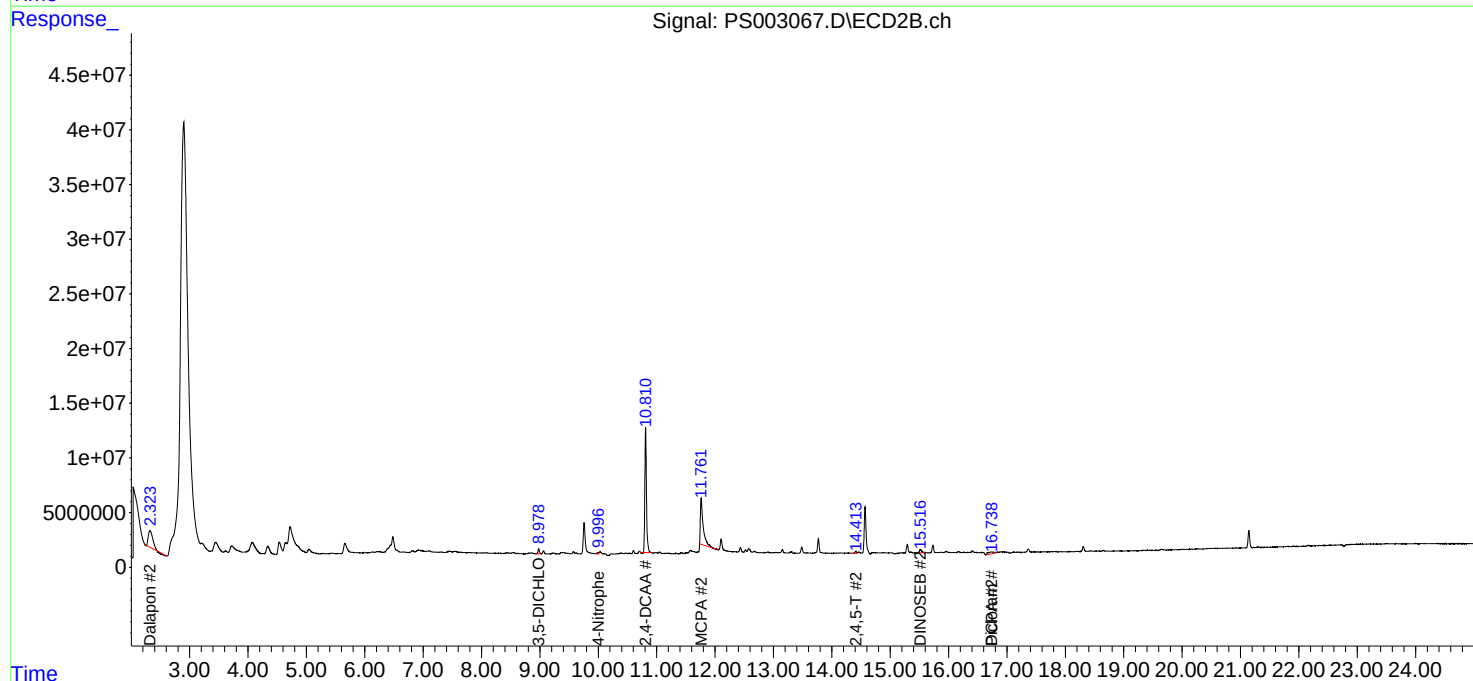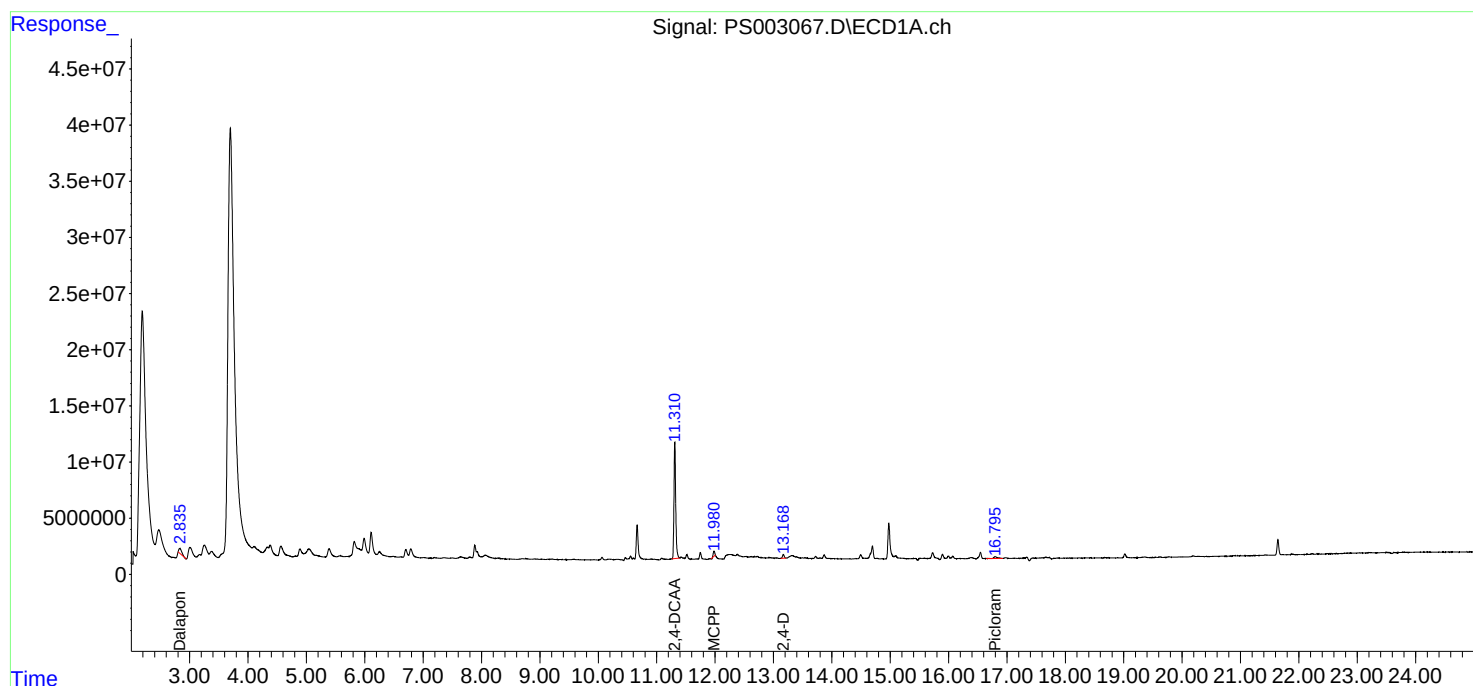


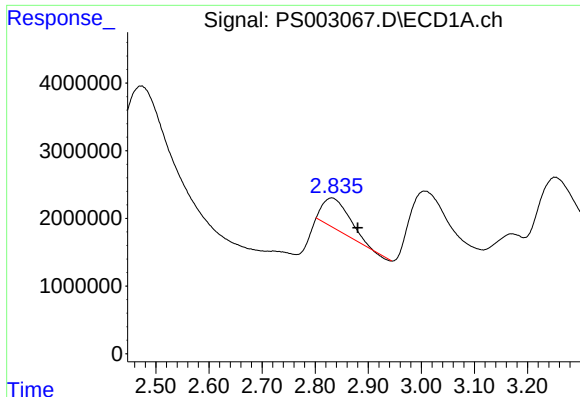

#1 Dalapon


R.T.: 2.831 min
Delta R.T.: -0.049 min
Response: 15186558
Conc: 27.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

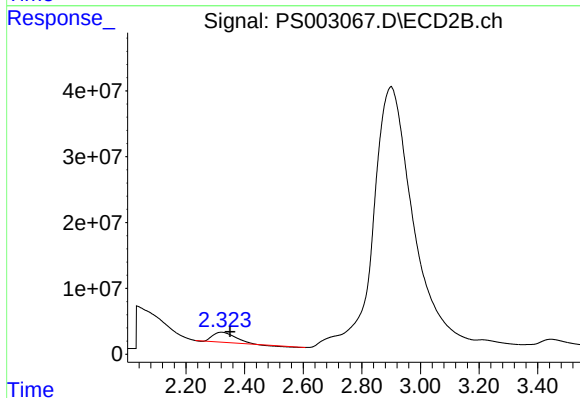


#1 Dalapon

R.T.: 2.321 min
Delta R.T.: -0.030 min
Response: 75084151
Conc: 140.10 ng/ml

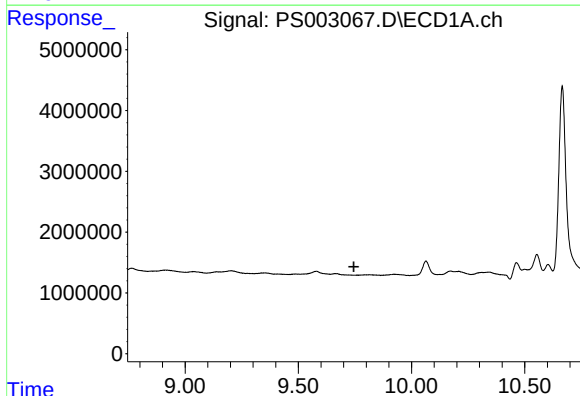


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

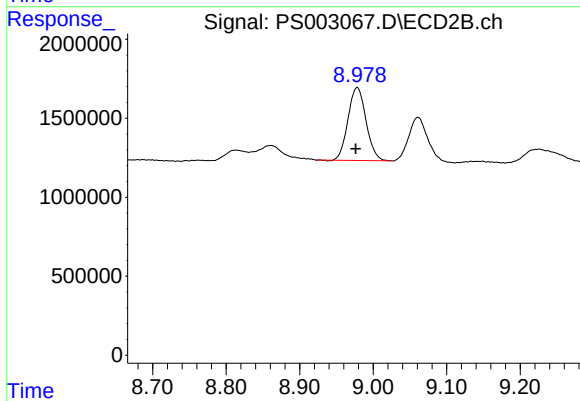

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.978 min
Delta R.T.: 0.002 min
Response: 7876840
Conc: 13.98 ng/ml

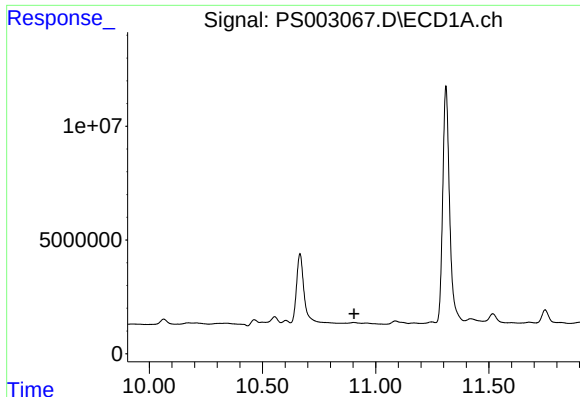

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

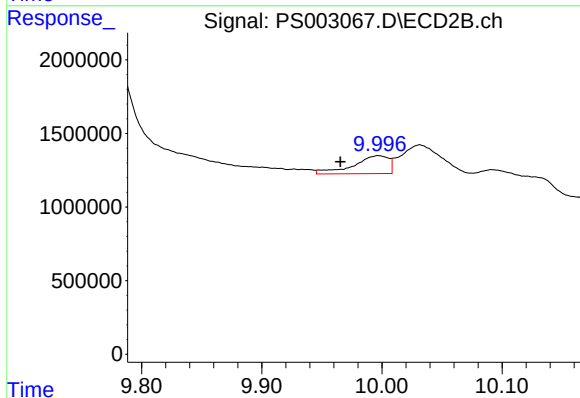


#3 4-Nitrophenol

R.T.: 9.997 min
Delta R.T.: 0.032 min
Response: 2500146
Conc: 11.96 ng/ml

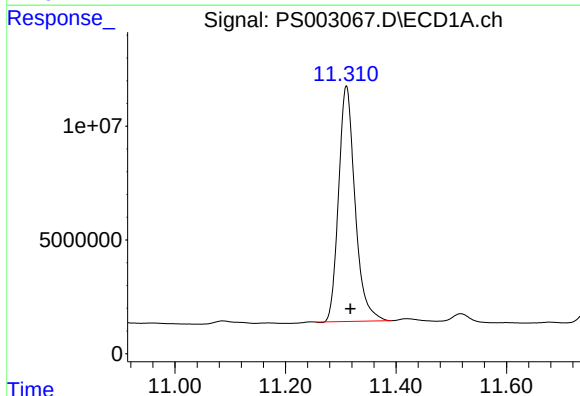


#4 2,4-DCAA

R.T.: 11.310 min
Delta R.T.: -0.008 min
Response: 213831460
Conc: 563.25 ng/ml

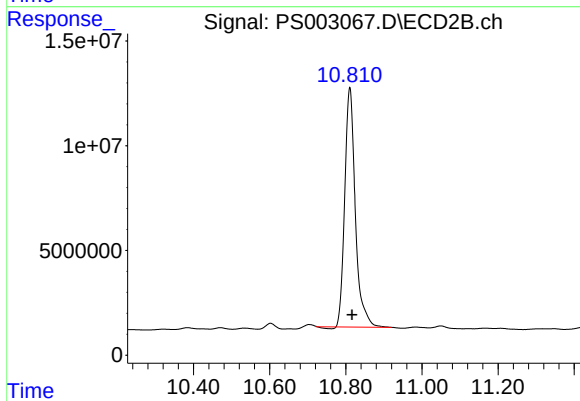

#4 2,4-DCAA


R.T.: 10.810 min
Delta R.T.: -0.006 min
Response: 220145130
Conc: 514.90 ng/ml

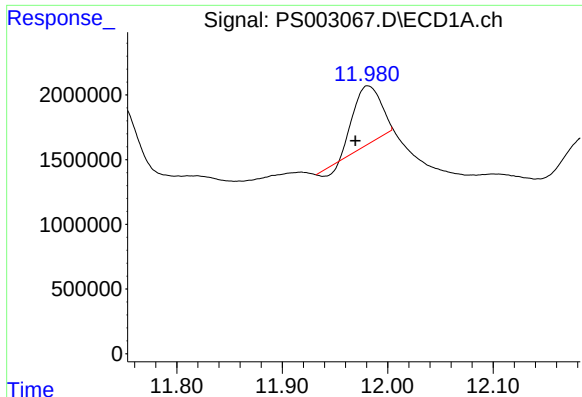

#6 MCPP


R.T.: 11.982 min
Delta R.T.: 0.013 min
Response: 8316804
Conc: 6.94 ug/ml

Instrument :
ECD_S
ClientSampleId :

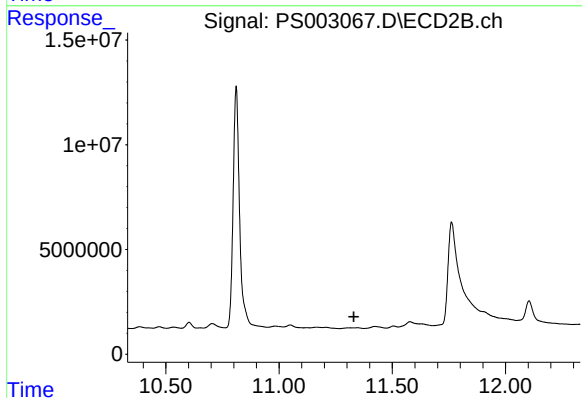


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

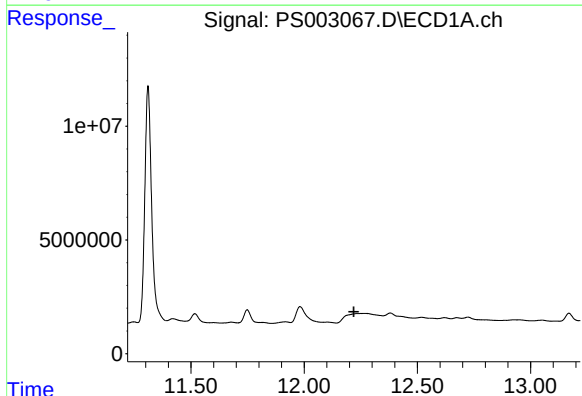


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.219 min
Response: 0
Conc: N.D.

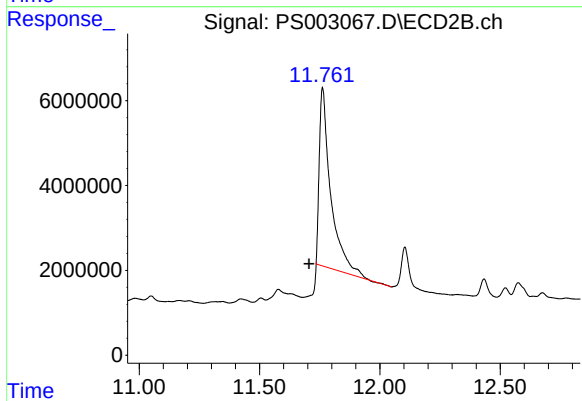

#7 MCPA


R.T.: 11.762 min
Delta R.T.: 0.056 min
Response: 138763978
Conc: 88.21 ug/ml

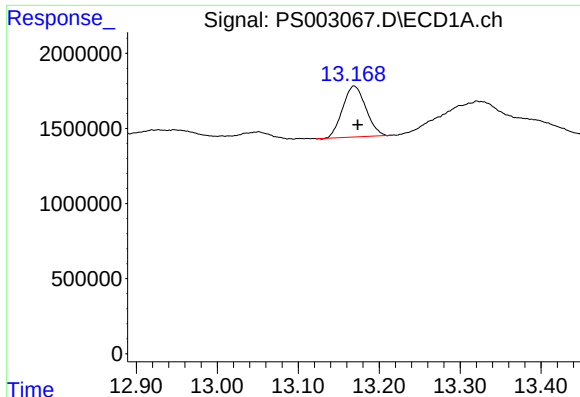

#9 2,4-D


R.T.: 13.169 min
Delta R.T.: -0.004 min
Response: 6726082
Conc: 14.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

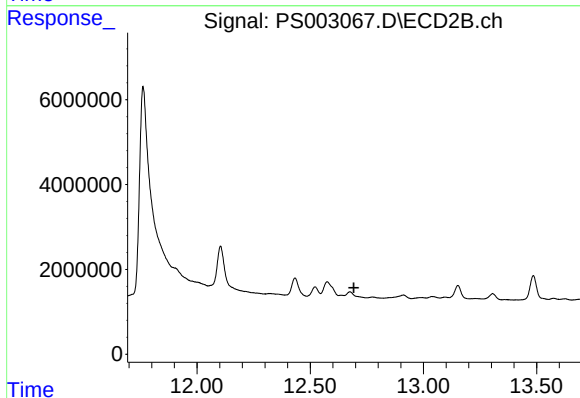


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

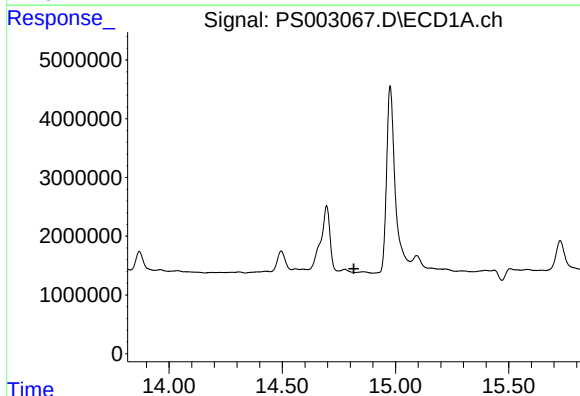


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

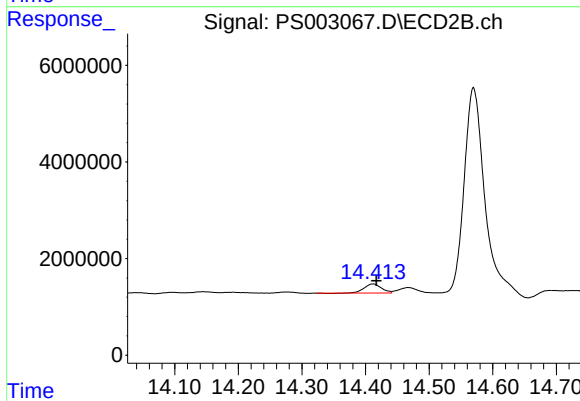

#12 2,4,5-T


R.T.: 14.412 min
Delta R.T.: -0.005 min
Response: 3548034
Conc: 1.85 ng/ml

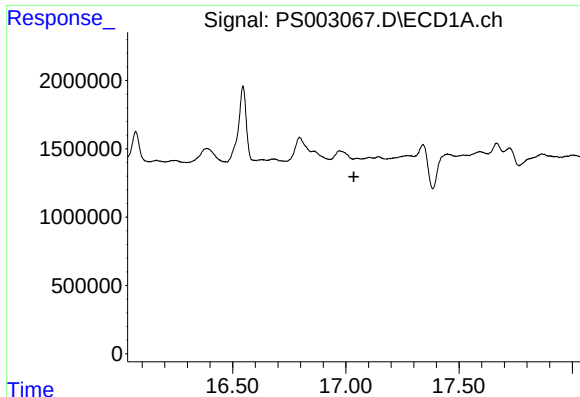

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

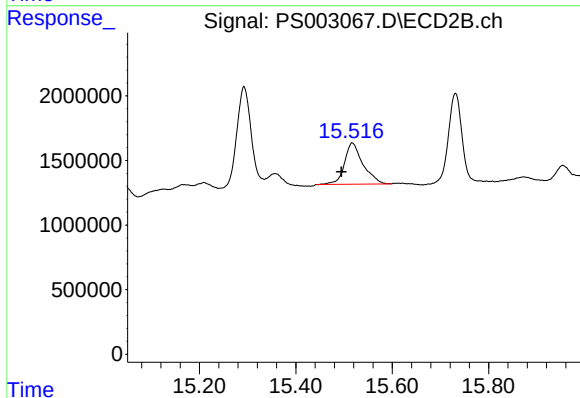


#14 DINOSEB

R.T.: 15.517 min
Delta R.T.: 0.022 min
Response: 8525208
Conc: 4.86 ng/ml

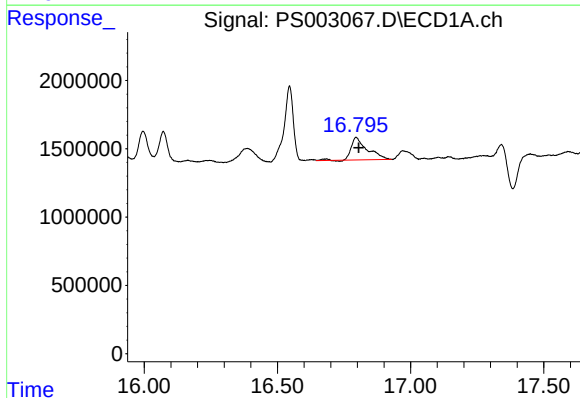


#15 Picloram

R.T.: 16.796 min
Delta R.T.: -0.010 min
Response: 6939764
Conc: 2.19 ng/ml

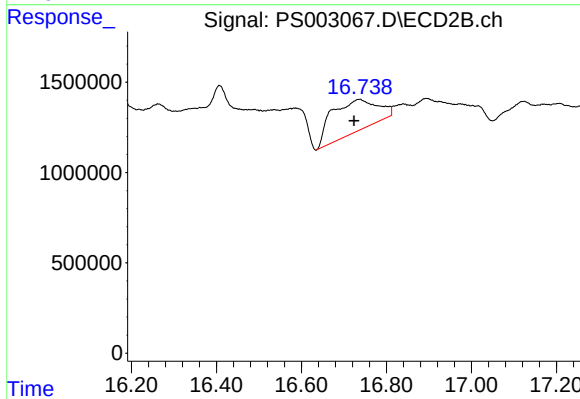

#15 Picloram


R.T.: 16.736 min
Delta R.T.: 0.012 min
Response: 13355091
Conc: 4.44 ng/ml

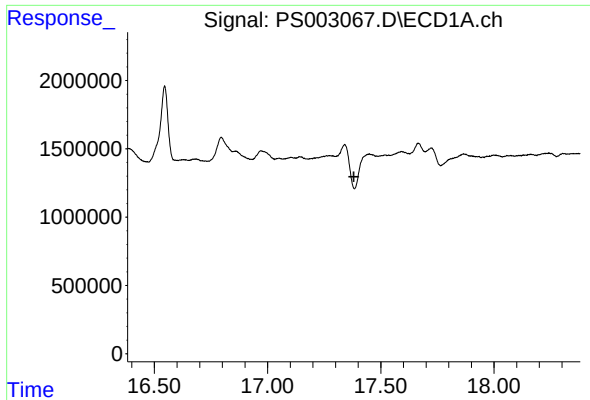

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

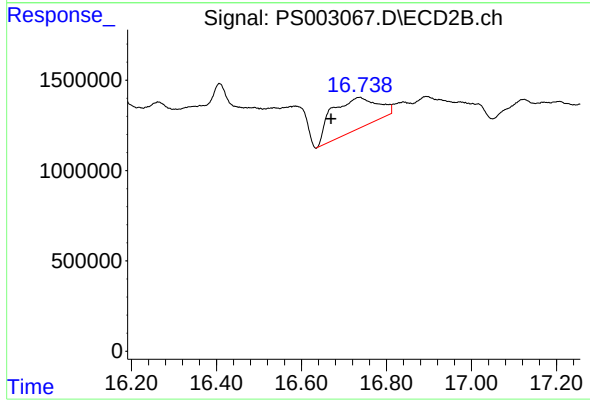

#16 DCPA

R.T.: 16.736 min
Delta R.T.: 0.066 min
Response: 13355091
Conc: 4.31 ng/ml