

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003068.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2019 00:45
 Operator : EI\SJ
 Sample : K1358-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 02:17:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.291	10.773	201.4E6	219.4E6	530.370	513.113
Target Compounds							
2) T	3,5-DICHL...	0.000	8.940	0	7009278	N.D.	12.437 #
3) T	4-Nitroph...	0.000	9.959	0	3839138	N.D.	18.367 #
6) T	MCP	11.961	0.000	14236913	0	11.883	N.D. #
7) T	MCPA	0.000	11.724	0	16151264	N.D.	10.267 #
9) T	2,4-D	13.151	0.000	5870808	0	12.733	N.D. #
10) T	Pentachlo...	0.000	13.270	0	2443964	N.D.	0.395 #
11) T	2,4,5-TP ...	14.477	0.000	4514421	0	1.793	N.D. #
12) T	2,4,5-T	0.000	14.430	0	2304022	N.D.	1.204 #
14) T	DINOSEB	17.054	15.480	6388554	7041470	3.396	4.017
15) T	Picloram	16.779	16.700	6952209	12430921	2.198	4.135 #
16) T	DCPA	17.440	16.700	-6279691	12430921	N.D.	4.013



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003068.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2019 00:45
Operator : EI\SJ
Sample : K1358-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 02:17:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

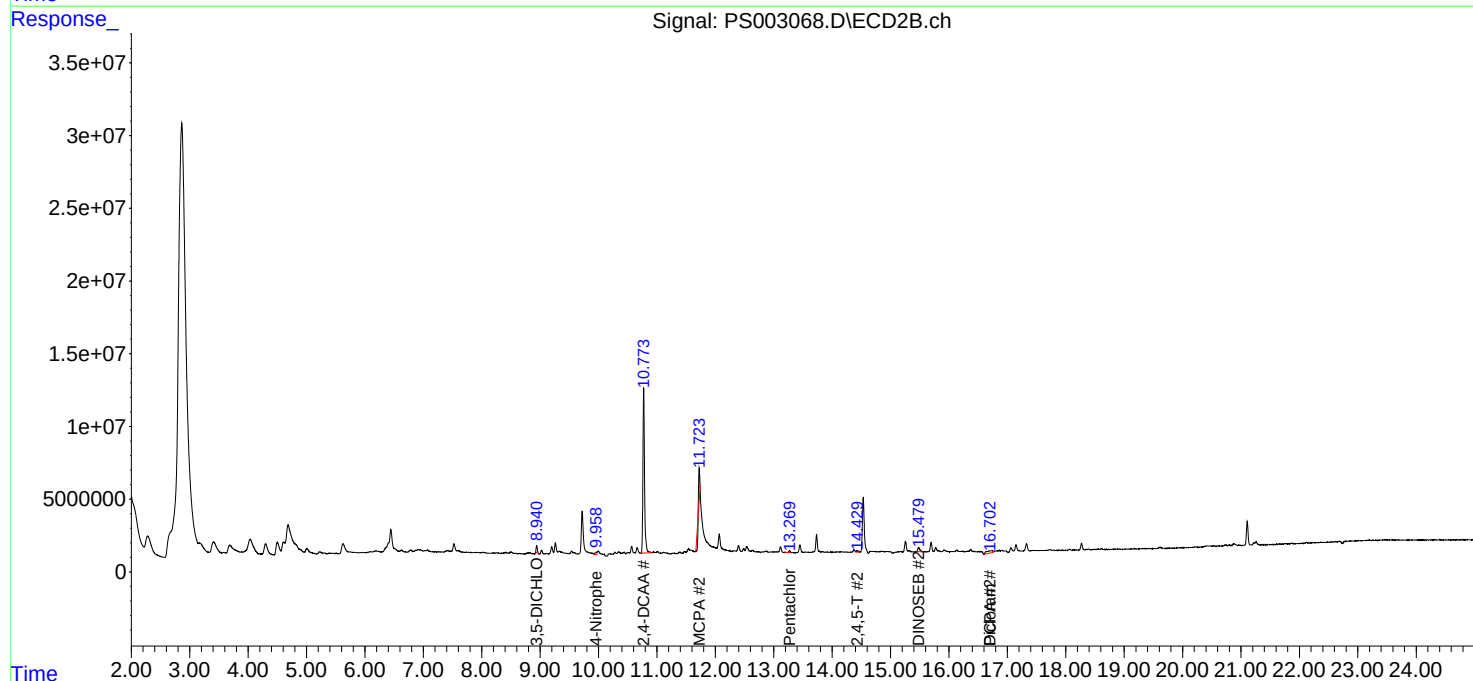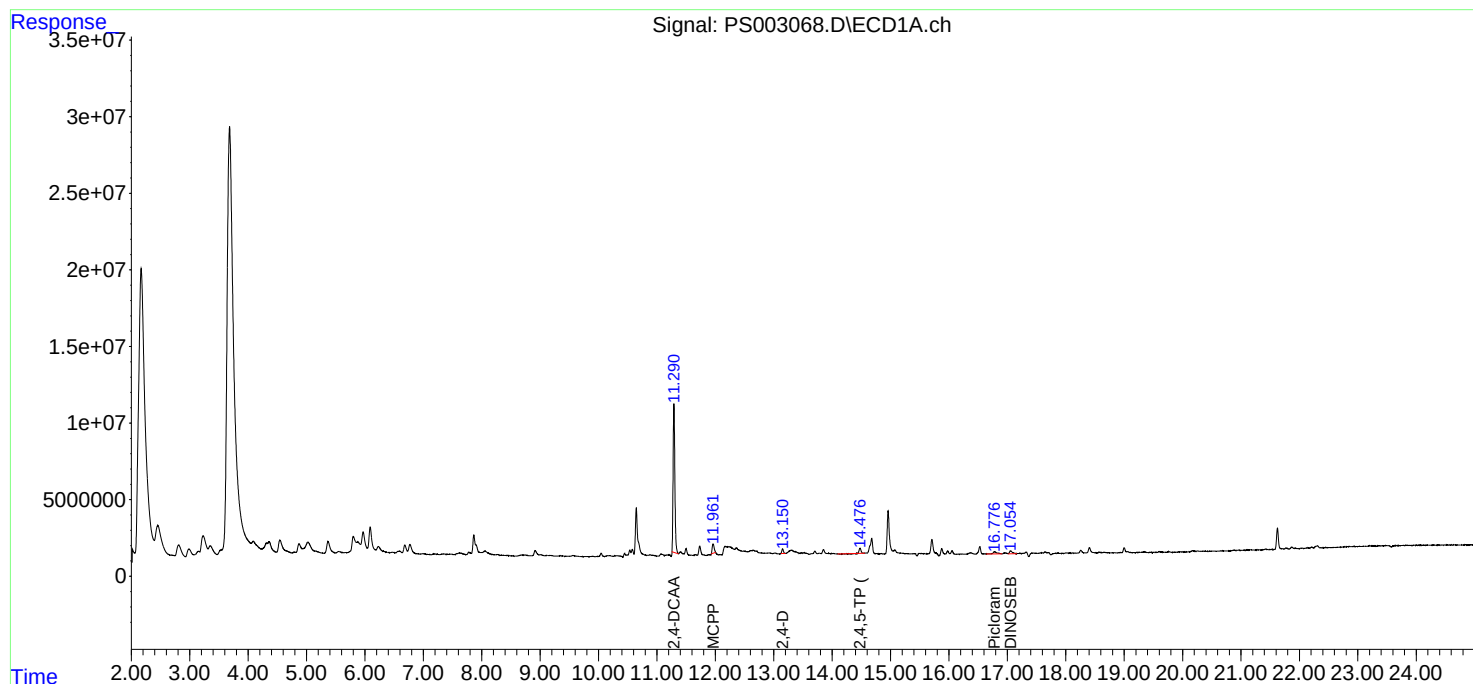


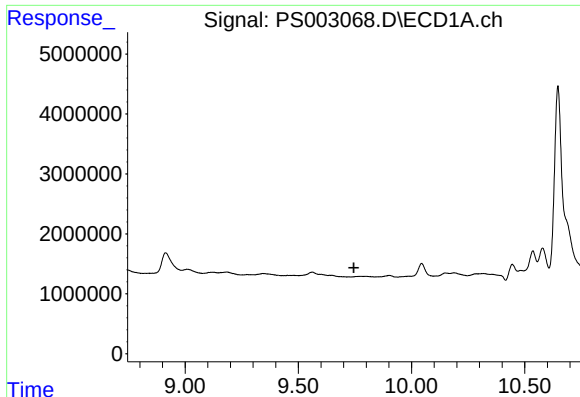

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

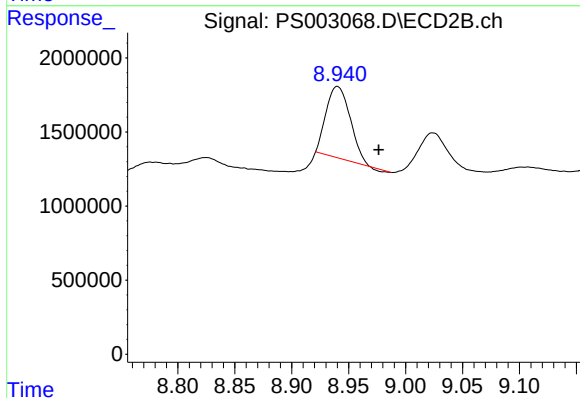


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.940 min
Delta R.T.: -0.036 min
Response: 7009278
Conc: 12.44 ng/ml

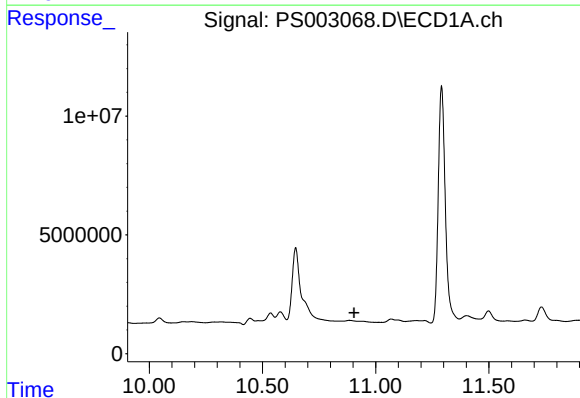


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

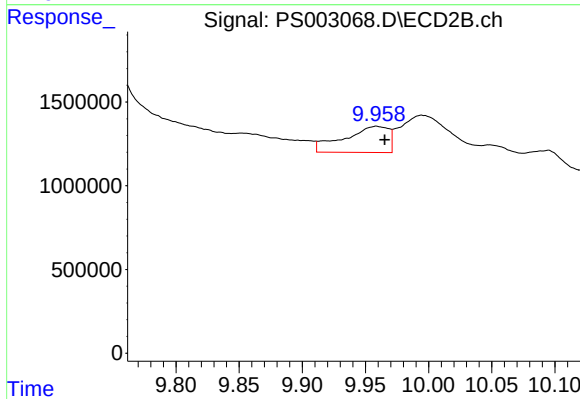

#3 4-Nitrophenol


R.T.: 9.959 min
Delta R.T.: -0.006 min
Response: 3839138
Conc: 18.37 ng/ml

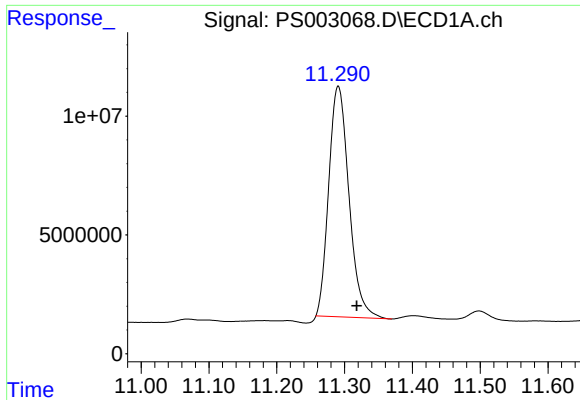

#4 2,4-DCAA


R.T.: 11.291 min
Delta R.T.: -0.027 min
Response: 201350158
Conc: 530.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

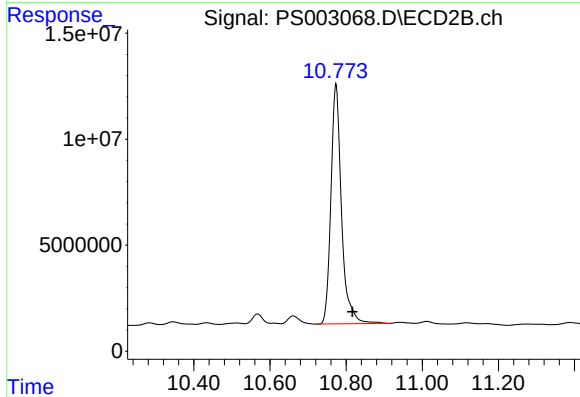


#4 2,4-DCAA

R.T.: 10.773 min
Delta R.T.: -0.044 min
Response: 219379434
Conc: 513.11 ng/ml

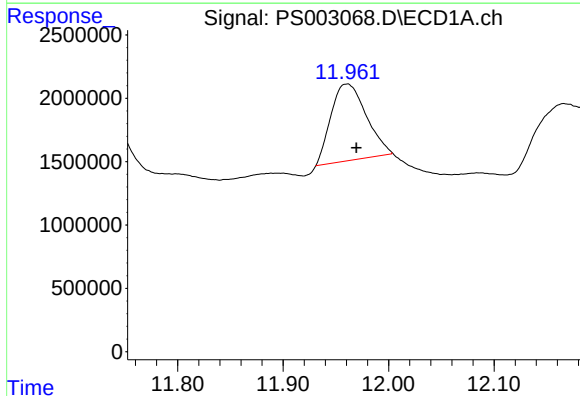


#6 MCP

R.T.: 11.961 min
Delta R.T.: -0.008 min
Response: 14236913
Conc: 11.88 ug/ml

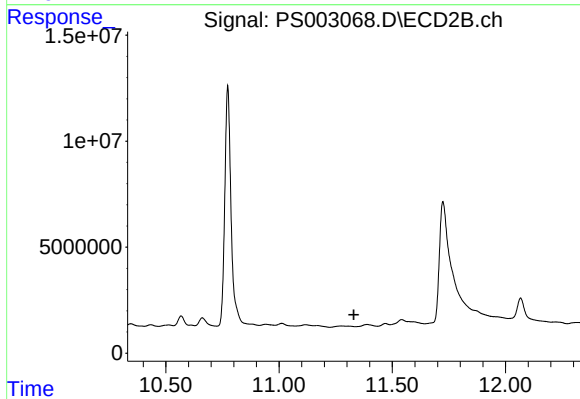

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

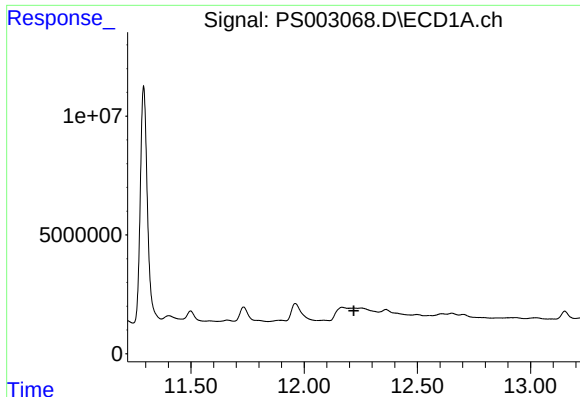

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

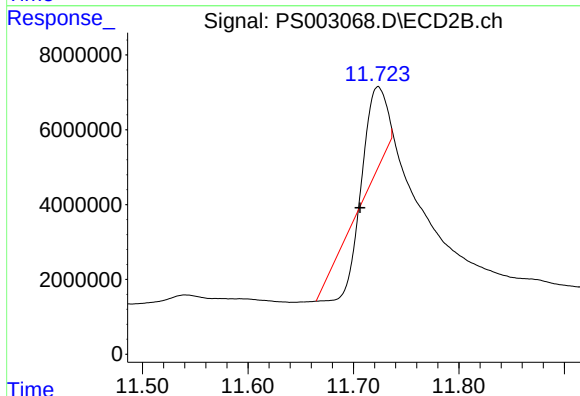


#7 MCPA

R.T.: 11.724 min
Delta R.T.: 0.018 min
Response: 16151264
Conc: 10.27 ug/ml

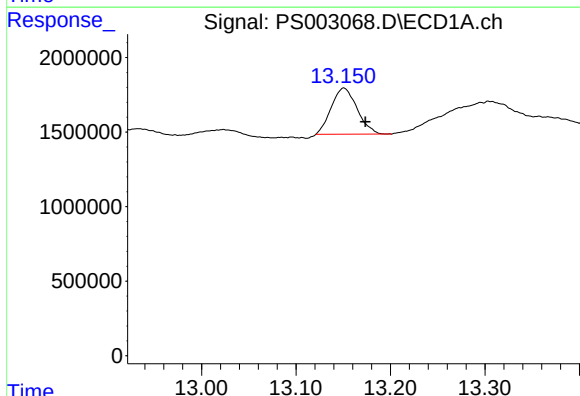


#9 2,4-D

R.T.: 13.151 min
Delta R.T.: -0.023 min
Response: 5870808
Conc: 12.73 ng/ml

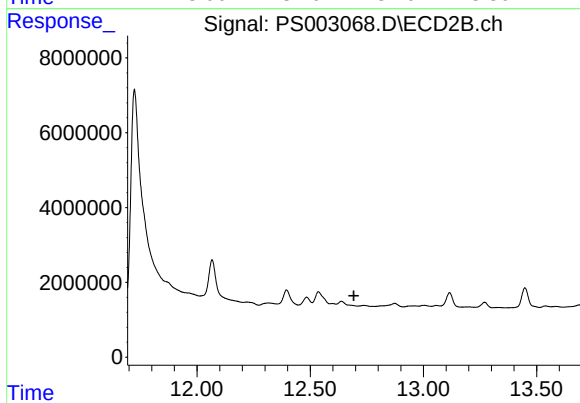

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.693 min
Response: 0
Conc: N.D.

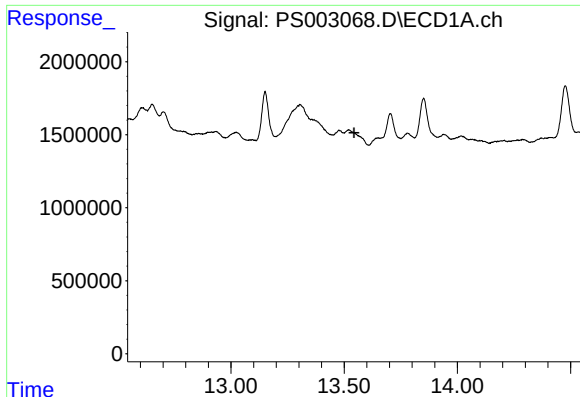

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

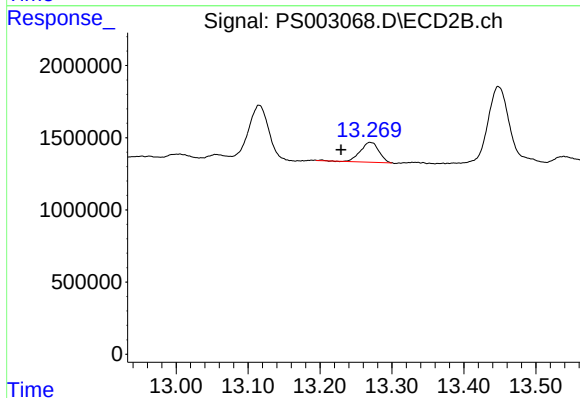


#10 Pentachlorophenol

R.T.: 13.270 min
Delta R.T.: 0.041 min
Response: 2443964
Conc: 0.40 ng/ml

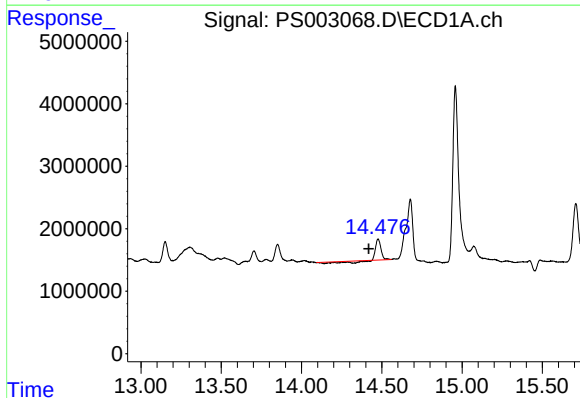


#11 2,4,5-TP (SILVEX)

R.T.: 14.477 min
Delta R.T.: 0.057 min
Response: 4514421
Conc: 1.79 ng/ml

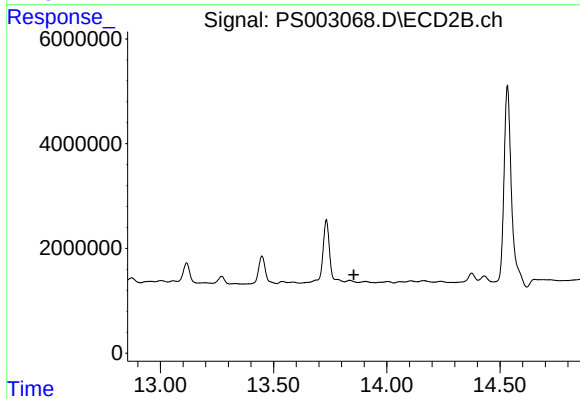

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.854 min
Response: 0
Conc: N.D.

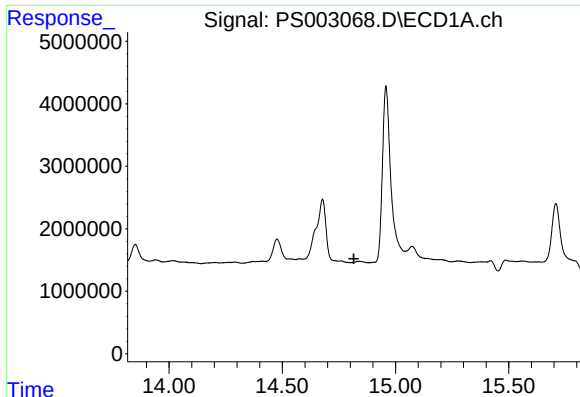

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

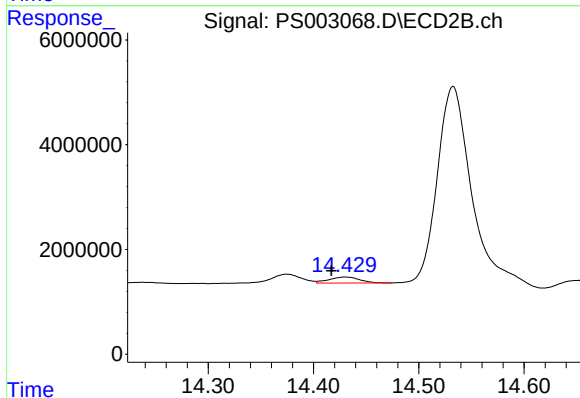


#12 2,4,5-T

R.T.: 14.430 min
Delta R.T.: 0.013 min
Response: 2304022
Conc: 1.20 ng/ml

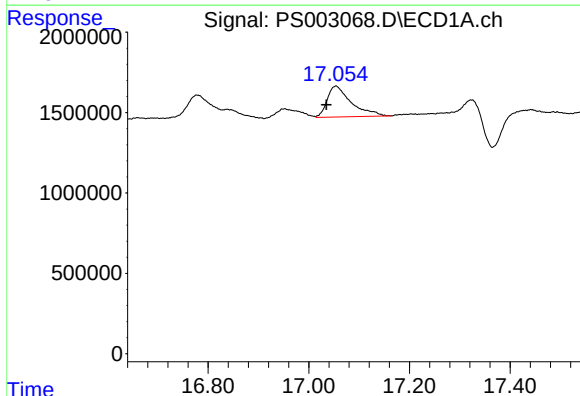


#14 DINOSEB

R.T.: 17.054 min
Delta R.T.: 0.019 min
Response: 6388554
Conc: 3.40 ng/ml

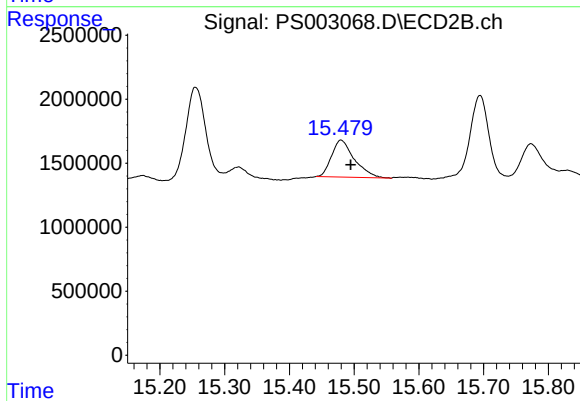

#14 DINOSEB


R.T.: 15.480 min
Delta R.T.: -0.015 min
Response: 7041470
Conc: 4.02 ng/ml

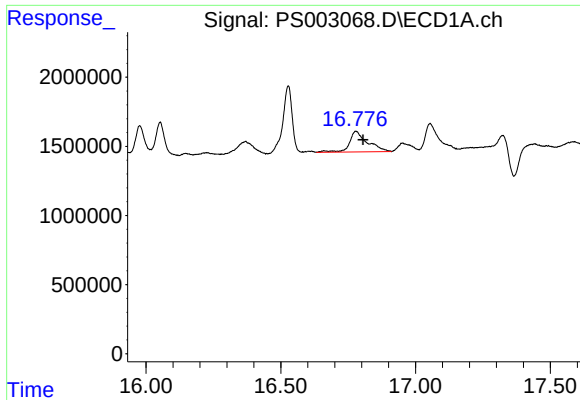

#15 Picloram


R.T.: 16.779 min
Delta R.T.: -0.027 min
Response: 6952209
Conc: 2.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

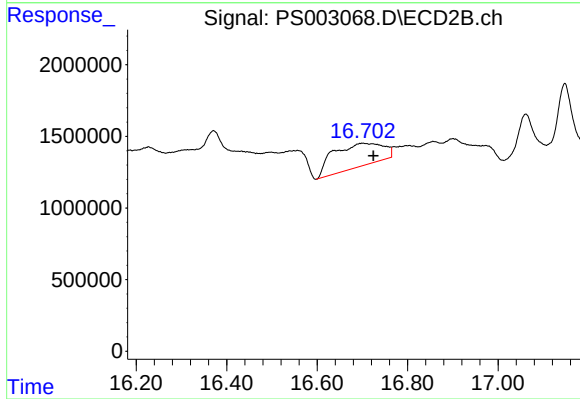


#15 Picloram

R.T.: 16.700 min
Delta R.T.: -0.024 min
Response: 12430921
Conc: 4.13 ng/ml

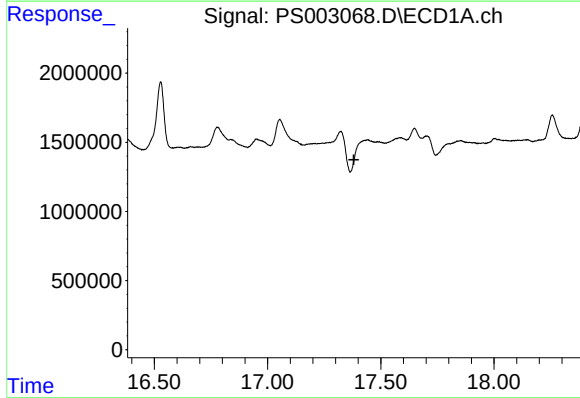

#16 DCPA

R.T.: 17.440 min
Delta R.T.: 0.059 min
Response: -6279691
Conc: N.D.

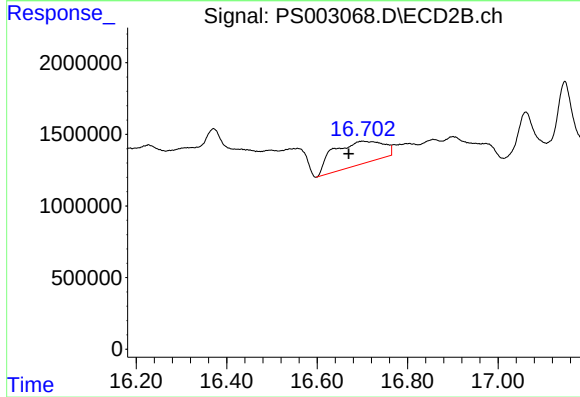

#16 DCPA

R.T.: 16.700 min
Delta R.T.: 0.031 min
Response: 12430921
Conc: 4.01 ng/ml