

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2019 01:16
 Operator : EI\SJ
 Sample : K1379-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 02:17:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.309	10.808	201.5E6	203.8E6	530.736	476.716
Target Compounds							
1) T	Dalapon	2.829	2.316	13654664	53732117	24.753	100.261 #
2) T	3,5-DICHL...	0.000	8.975	0	10613381	N.D.	18.832 #
3) T	4-Nitroph...	0.000	10.029	0	6885802	N.D.	32.943 #
6) T	MCP	11.979	0.000	10254710	0	8.559	N.D. #
7) T	MCPA	0.000	11.758	0	105.9E6	N.D.	67.318 #
9) T	2,4-D	13.168	0.000	6393646	0	13.867	N.D. #
11) T	2,4,5-TP ...	14.384	0.000	4518258	0	1.794	N.D. #
12) T	2,4,5-T	0.000	14.409	0	2320522	N.D.	1.213 #
14) T	DINOSEB	0.000	15.515	0	8904076	N.D.	5.079 #
15) T	Picloram	16.811	16.728	9511821	12048861	3.007	4.008 #
16) T	DCPA	17.451	16.728	-6195645	12048861	N.D.	3.890



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2019 01:16
Operator : EI\SJ
Sample : K1379-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 02:17:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

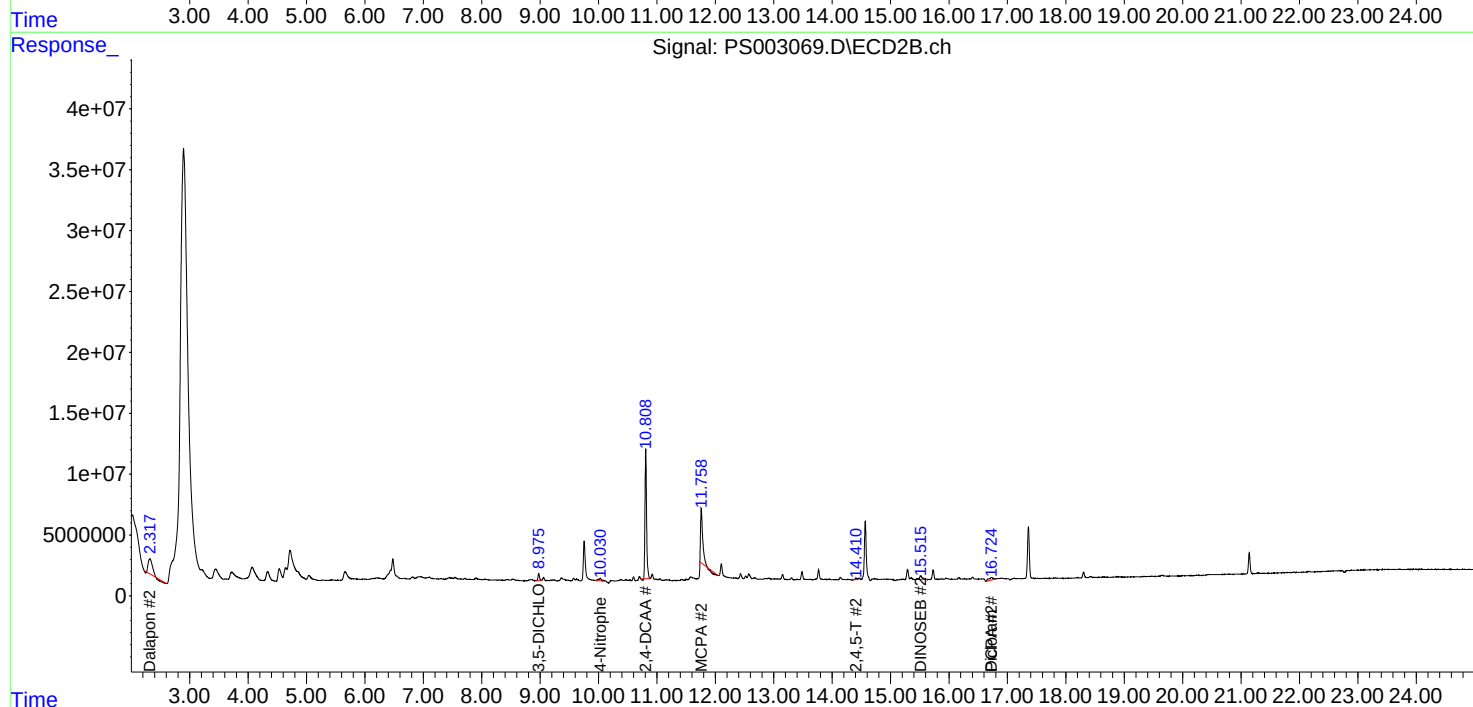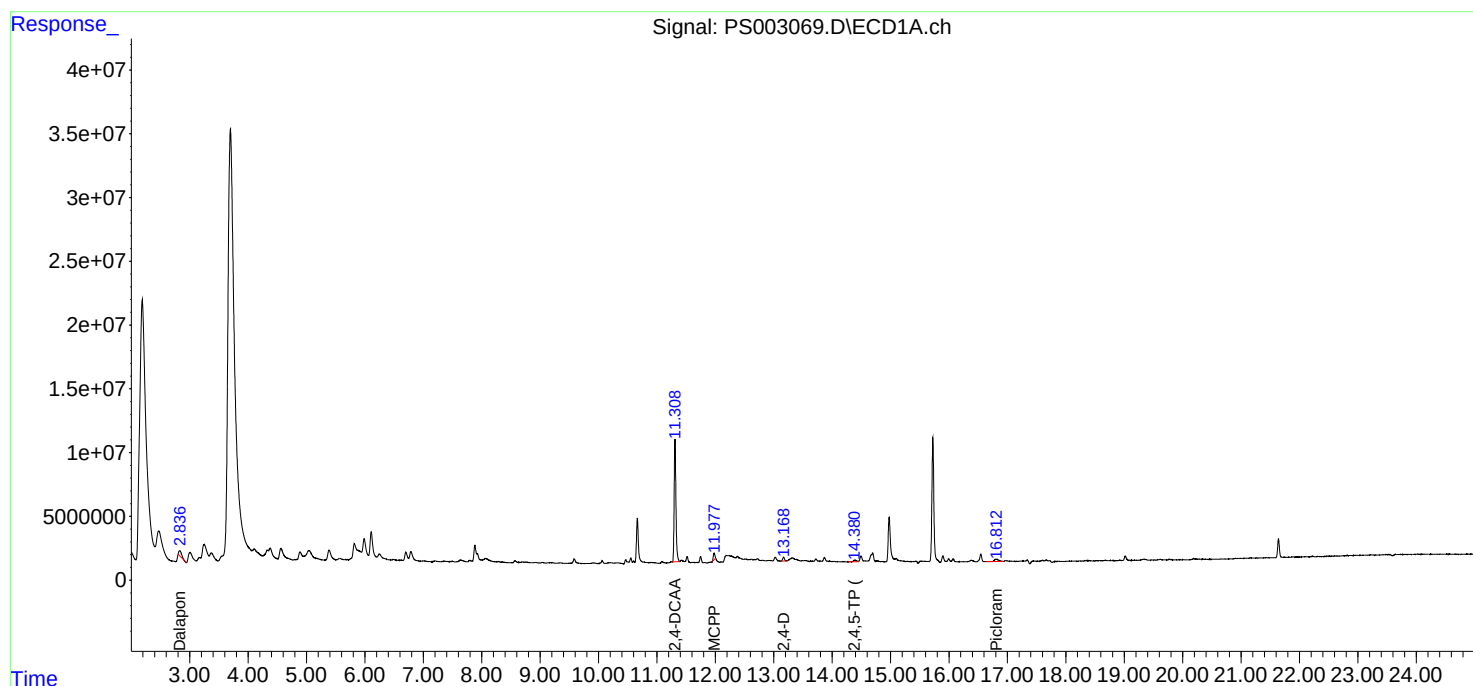


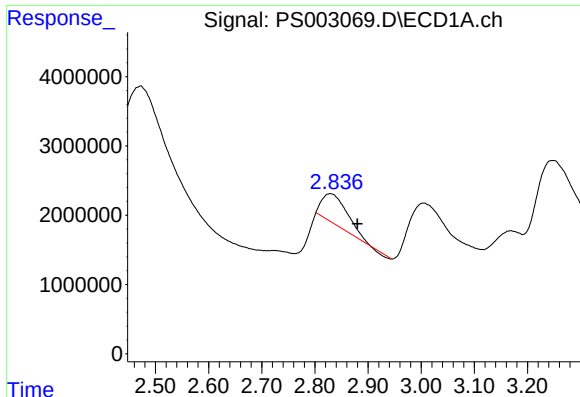

#1 Dalapon


R.T.: 2.829 min
Delta R.T.: -0.051 min
Response: 13654664
Conc: 24.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

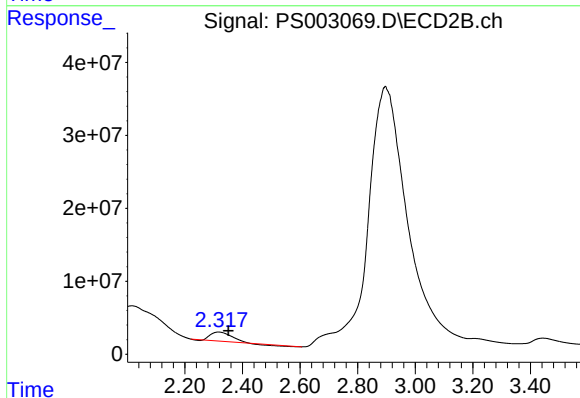


#1 Dalapon

R.T.: 2.316 min
Delta R.T.: -0.034 min
Response: 53732117
Conc: 100.26 ng/ml

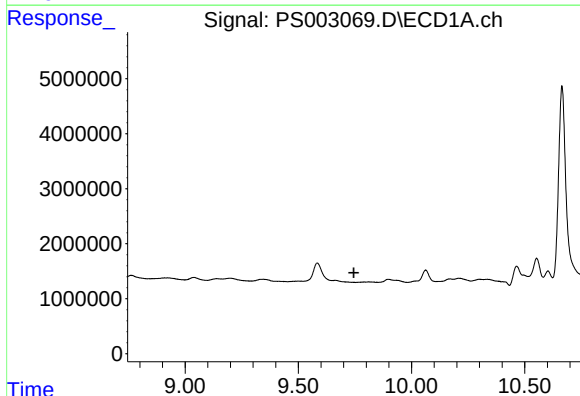


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

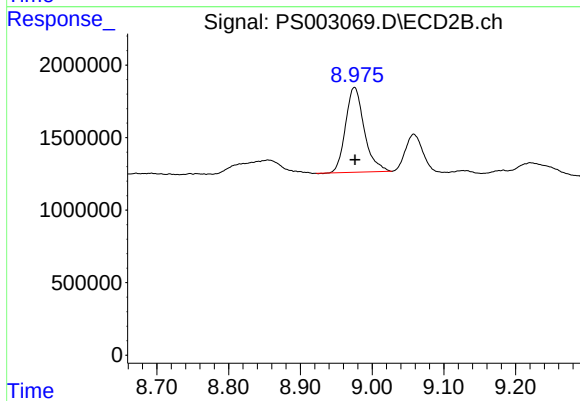

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 10613381
Conc: 18.83 ng/ml

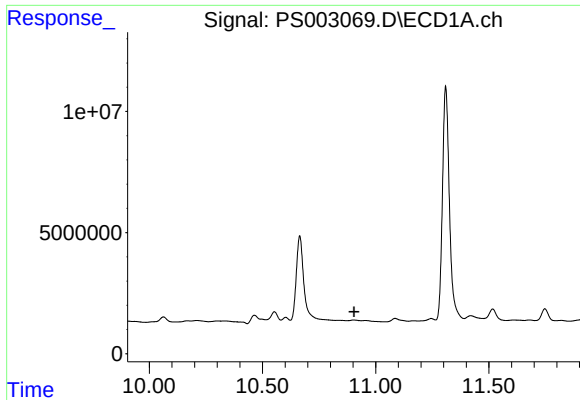

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

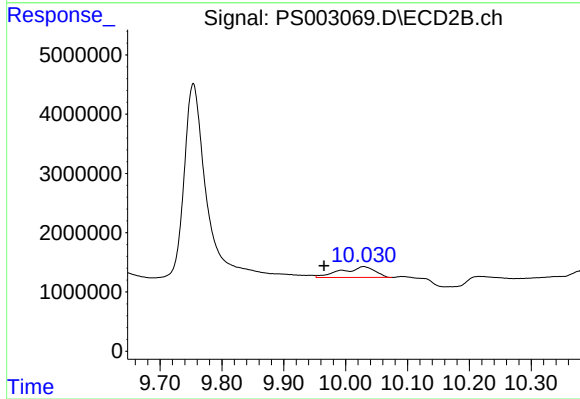


#3 4-Nitrophenol

R.T.: 10.029 min
Delta R.T.: 0.064 min
Response: 6885802
Conc: 32.94 ng/ml

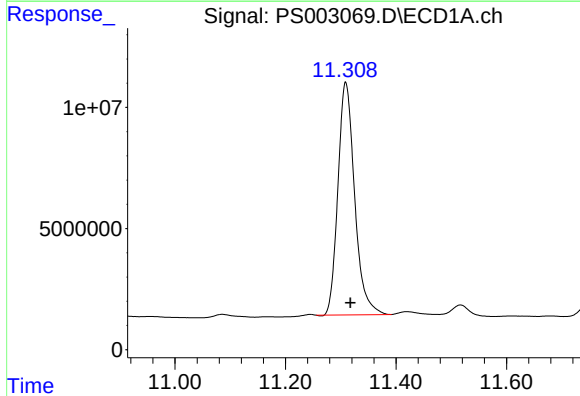


#4 2,4-DCAA

R.T.: 11.309 min
Delta R.T.: -0.008 min
Response: 201488963
Conc: 530.74 ng/ml

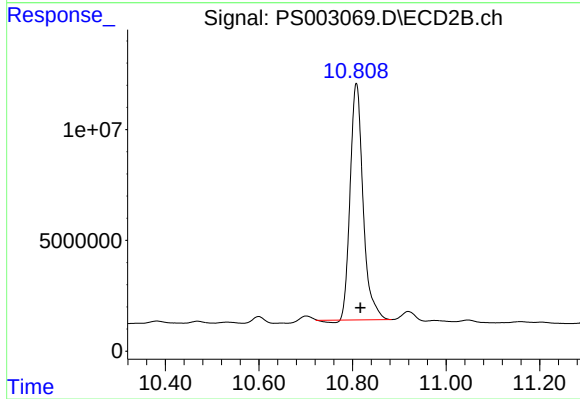

#4 2,4-DCAA


R.T.: 10.808 min
Delta R.T.: -0.008 min
Response: 203818070
Conc: 476.72 ng/ml

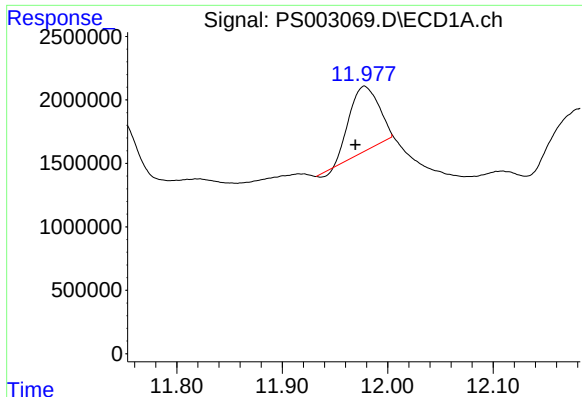

#6 MCPP


R.T.: 11.979 min
Delta R.T.: 0.009 min
Response: 10254710
Conc: 8.56 ug/ml

Instrument :
ECD_S
ClientSampleId :

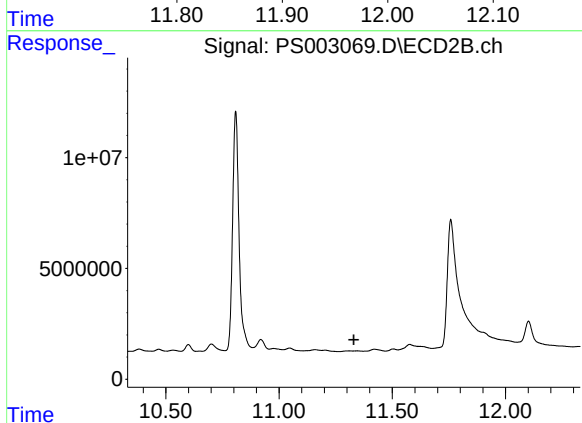


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

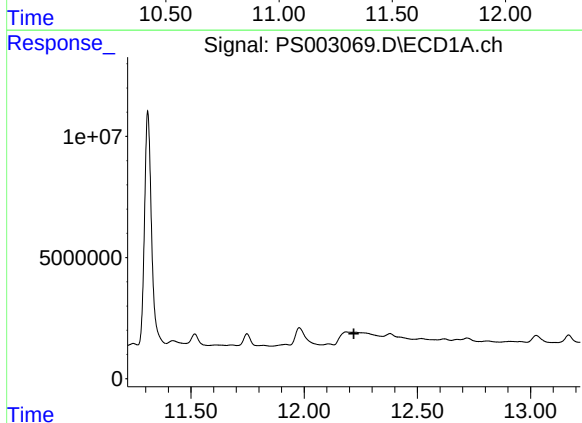


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.219 min
Response: 0
Conc: N.D.

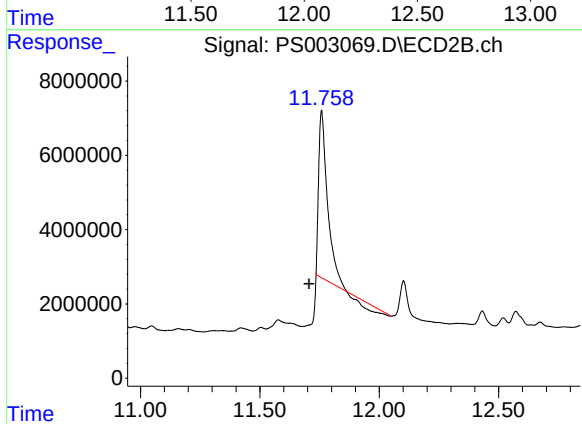

#7 MCPA


R.T.: 11.758 min
Delta R.T.: 0.052 min
Response: 105895519
Conc: 67.32 ug/ml

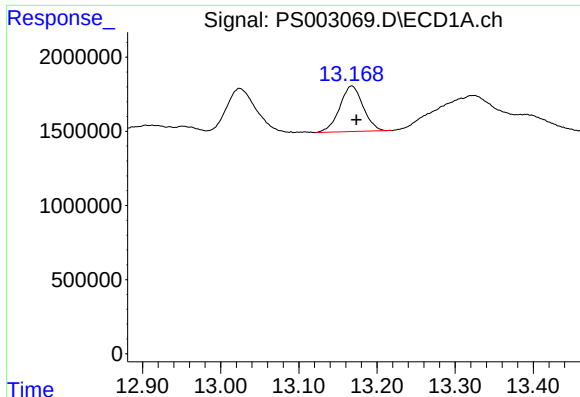

#9 2,4-D


R.T.: 13.168 min
Delta R.T.: -0.006 min
Response: 6393646
Conc: 13.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

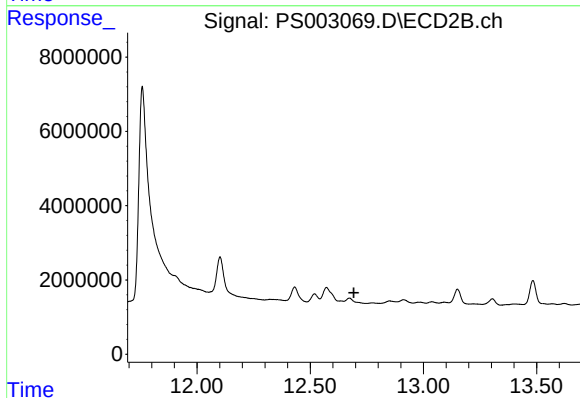


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.693 min
Response: 0
Conc: N.D.

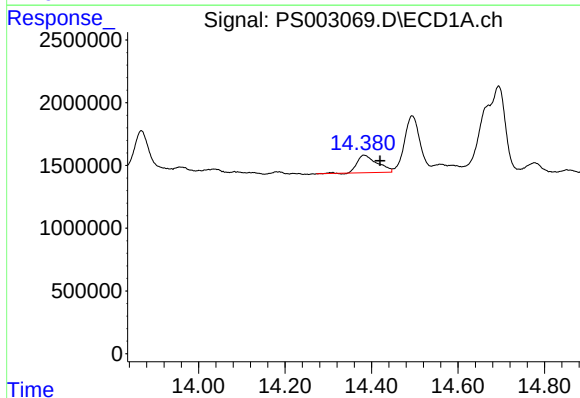


#11 2,4,5-TP (SILVEX)

R.T.: 14.384 min
Delta R.T.: -0.036 min
Response: 4518258
Conc: 1.79 ng/ml

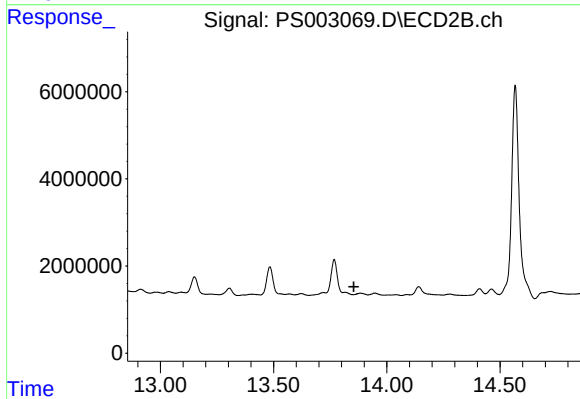

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

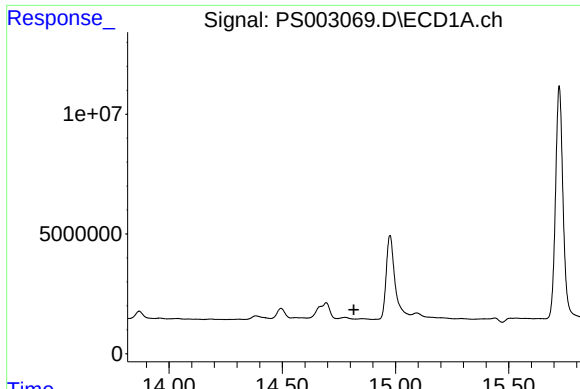

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

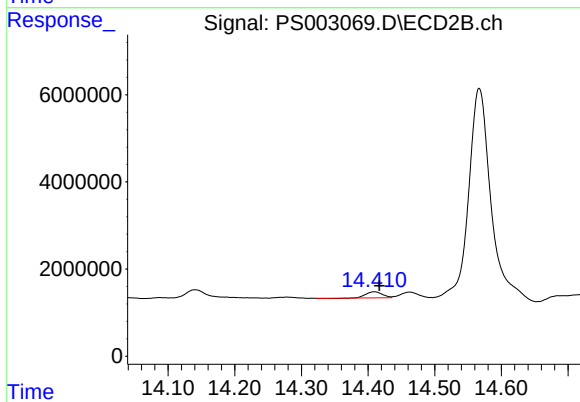


#12 2,4,5-T

R.T.: 14.409 min
Delta R.T.: -0.008 min
Response: 2320522
Conc: 1.21 ng/ml

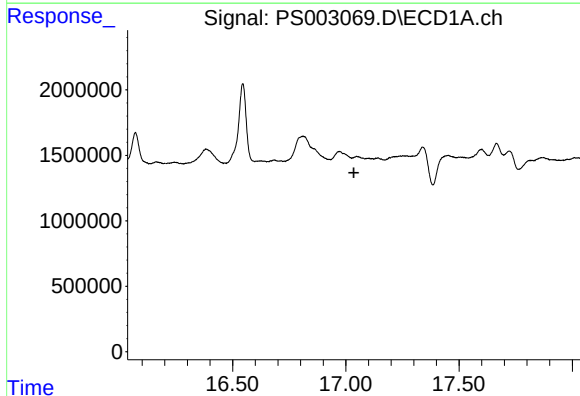


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

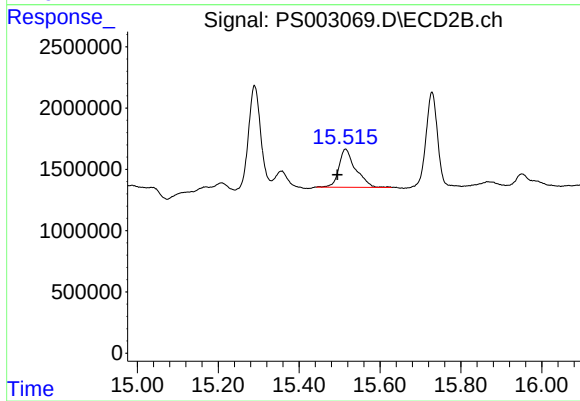

#14 DINOSEB


R.T.: 15.515 min
Delta R.T.: 0.020 min
Response: 8904076
Conc: 5.08 ng/ml

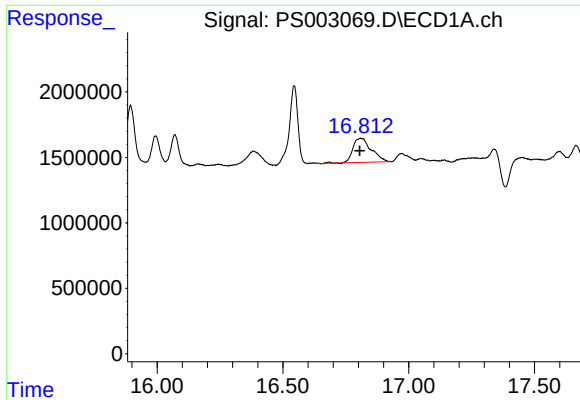

#15 Picloram


R.T.: 16.811 min
Delta R.T.: 0.005 min
Response: 9511821
Conc: 3.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

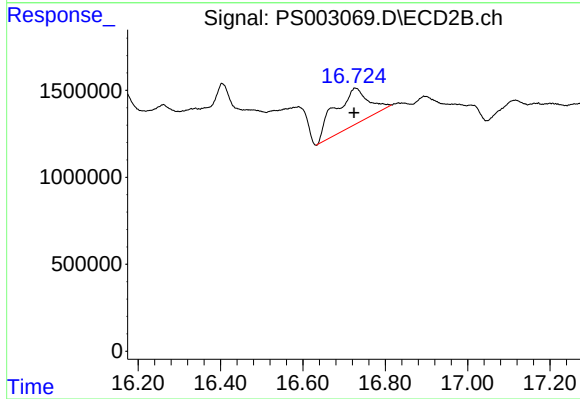


#15 Picloram

R.T.: 16.728 min
Delta R.T.: 0.004 min
Response: 12048861
Conc: 4.01 ng/ml

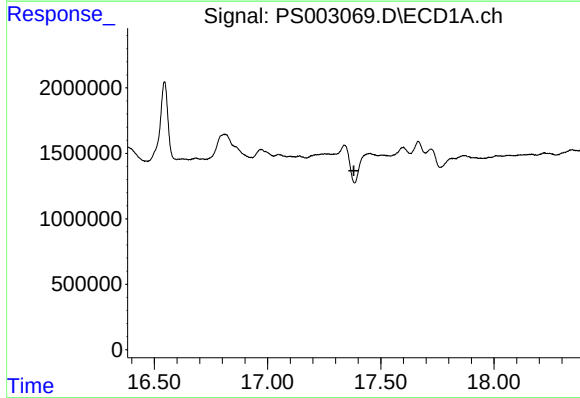

#16 DCPA

R.T.: 17.451 min
Delta R.T.: 0.069 min
Response: -6195645
Conc: N.D.

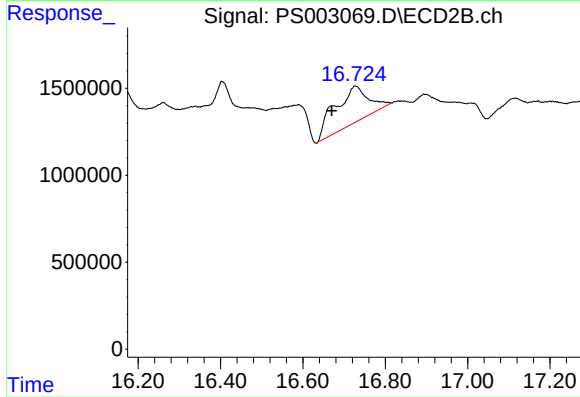

#16 DCPA

R.T.: 16.728 min
Delta R.T.: 0.058 min
Response: 12048861
Conc: 3.89 ng/ml