

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 20:37
 Operator : EI\SJ
 Sample : K1338-02MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-06-020519-AMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 01:12:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.294	10.779	157.0E6	164.6E6	413.544	384.956
Target Compounds							
1) T	Dalapon	2.861	2.312	257.8E6	324.5E6	467.393m	605.408 #
2) T	3,5-DICHL...	9.721	8.939	295.7E6	289.4E6	513.494m	513.503m
5) T	DICAMBA	11.600	11.059	894.1E6	866.3E6	557.800m	546.013m
6) T	MCPD	11.945	11.290	99110602	64586295	82.722m	58.558m#
7) T	MCPA	12.192	11.666	108.8E6	87600550	61.498m	55.688m
8) T	DICHLORPROP	12.789	12.184	232.6E6	226.8E6	606.389m	593.275
9) T	2,4-D	13.148	12.655	288.0E6	309.8E6	624.720m	617.896m
10) T	Pentachlo...	13.518	13.190	2883.5E6	2768.0E6	449.640m	447.849m
11) T	2,4,5-TP ...	14.395	13.816	1432.2E6	1359.1E6	568.708	547.929m
12) T	2,4,5-T	14.791	14.380	1355.9E6	881.2E6	555.820	460.544m
13) T	2,4-DB	15.538	15.031	166.6E6	153.6E6	637.221m	604.824m
14) T	DINOSEB	17.010	15.456	688.4E6	632.2E6	365.899	360.635m
15) T	Picloram	16.781	16.686	1600.7E6	1498.0E6	505.975	498.282
16) T	DCPA	17.355	16.631	1132.1E6	1195.4E6	376.455m	385.899m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : X:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 20:37
Operator : EI\SJ
Sample : K1338-02MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 01:12:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

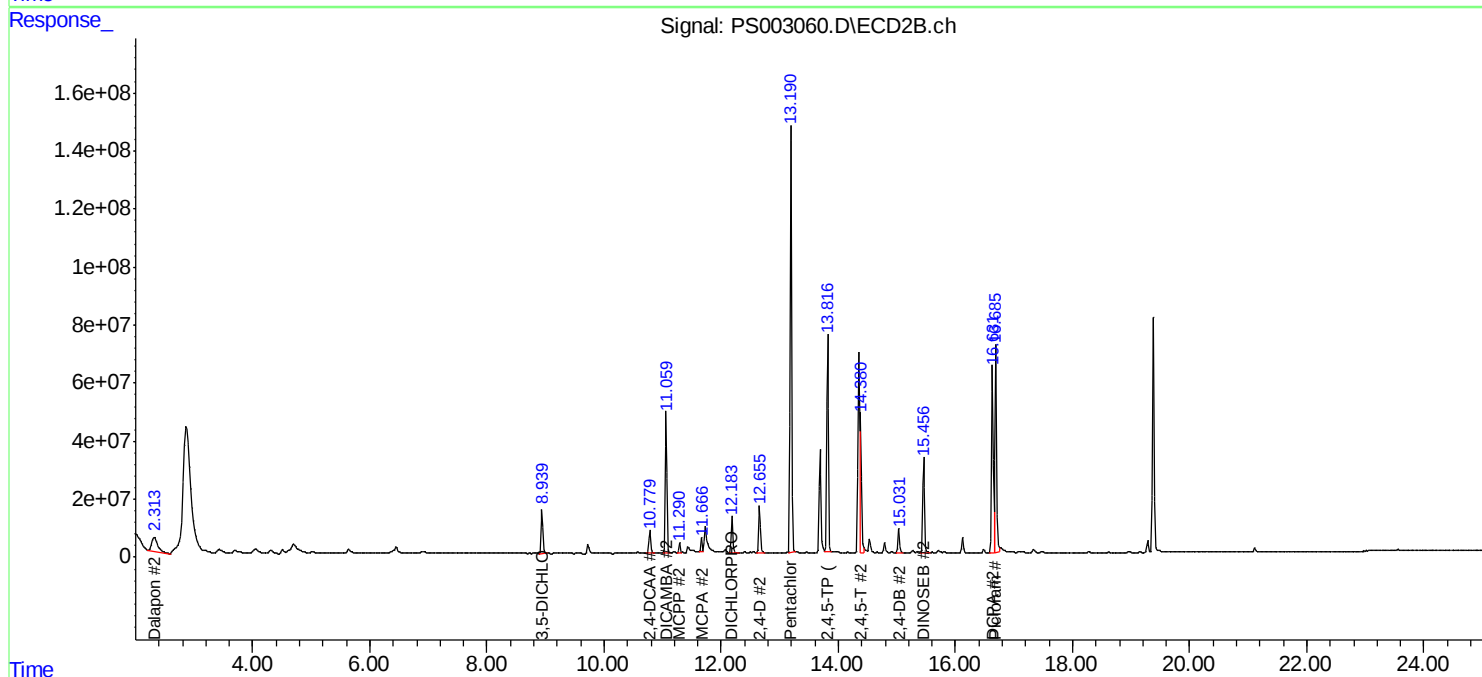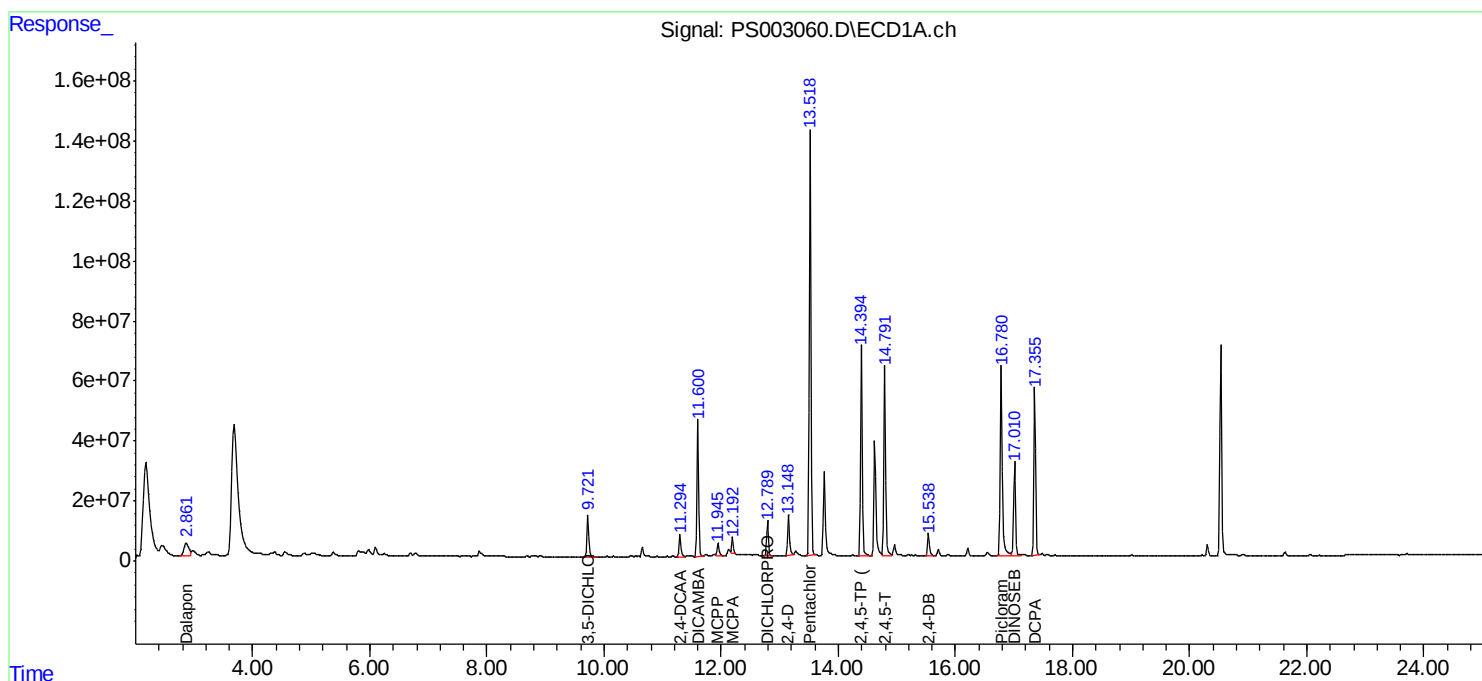


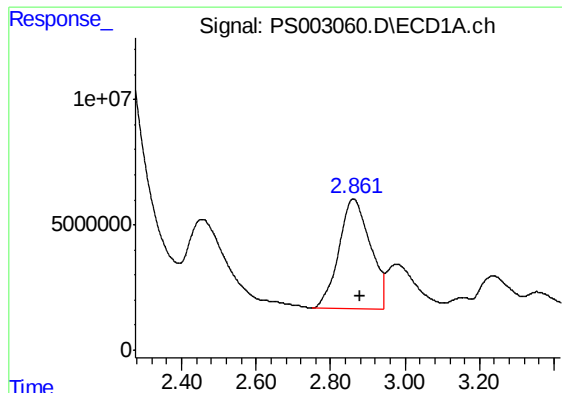

#1 Dalapon


R.T.: 2.861 min
Delta R.T.: -0.019 min
Response: 257836450
Conc: 467.39 ng/ml m

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMS

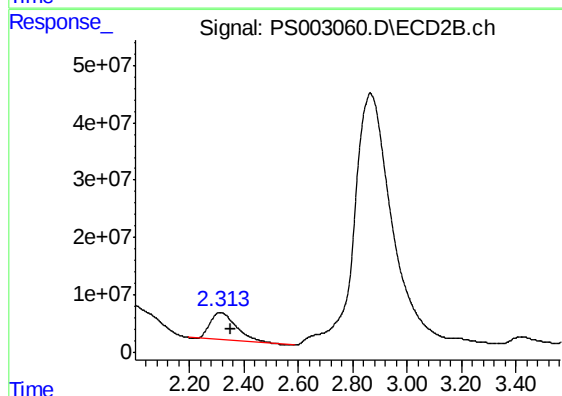


#1 Dalapon

R.T.: 2.312 min
Delta R.T.: -0.038 min
Response: 324451048
Conc: 605.41 ng/ml

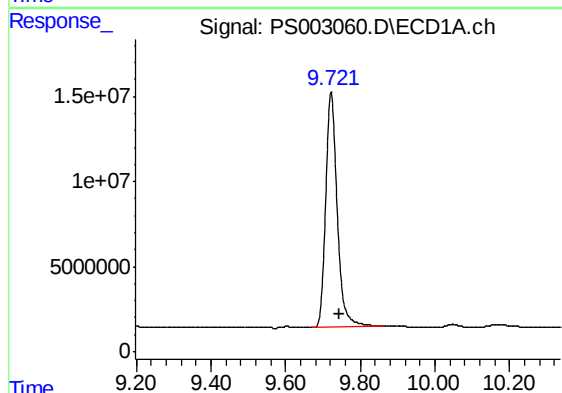


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.721 min
Delta R.T.: -0.024 min
Response: 295691593
Conc: 513.49 ng/ml m

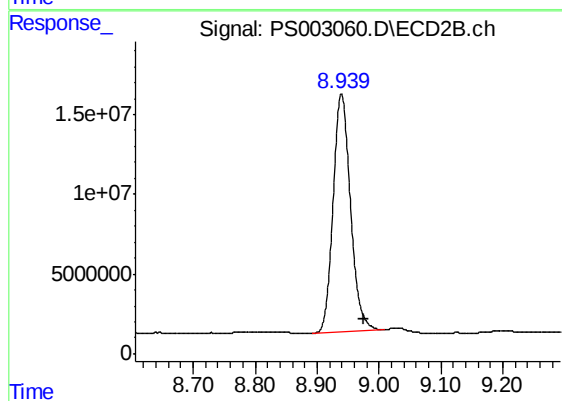

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.939 min
Delta R.T.: -0.037 min
Response: 289393906
Conc: 513.50 ng/ml m

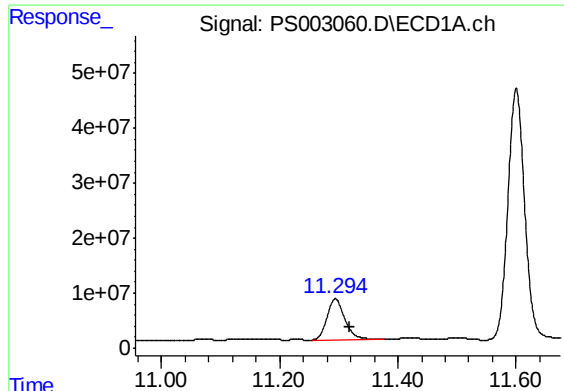

#4 2,4-DCAA


R.T.: 11.294 min
Delta R.T.: -0.023 min
Response: 156998122
Conc: 413.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMS

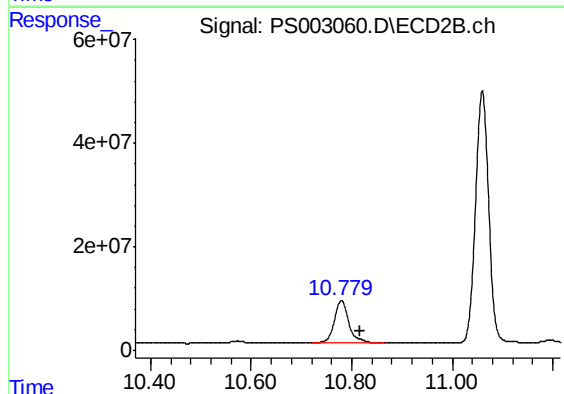


#4 2,4-DCAA

R.T.: 10.779 min
Delta R.T.: -0.037 min
Response: 164586381
Conc: 384.96 ng/ml

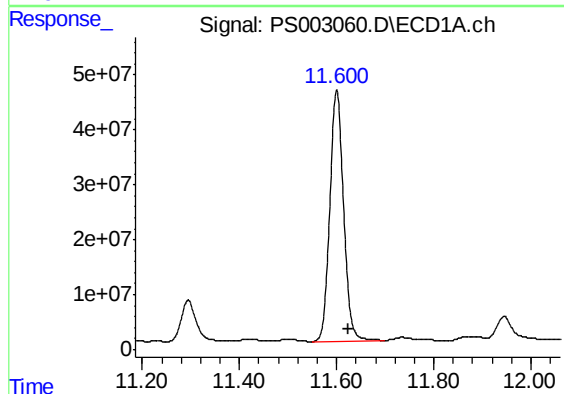


#5 DICAMBA

R.T.: 11.600 min
Delta R.T.: -0.024 min
Response: 894091622
Conc: 557.80 ng/ml m

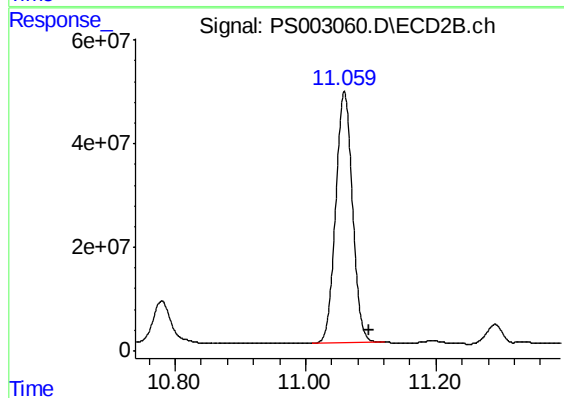

#5 DICAMBA


R.T.: 11.059 min
Delta R.T.: -0.038 min
Response: 866340516
Conc: 546.01 ng/ml m

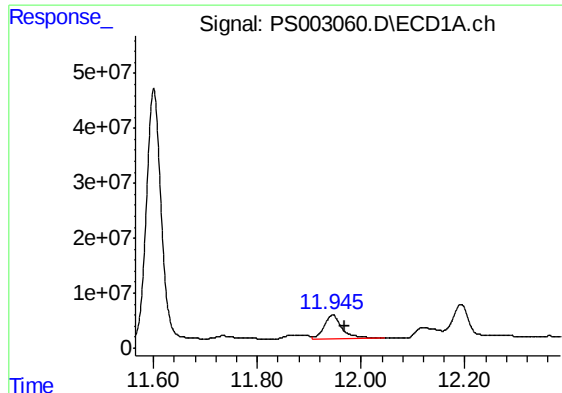

#6 MCPP


R.T.: 11.945 min
Delta R.T.: -0.024 min
Response: 99110602
Conc: 82.72 ug/ml m

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMS

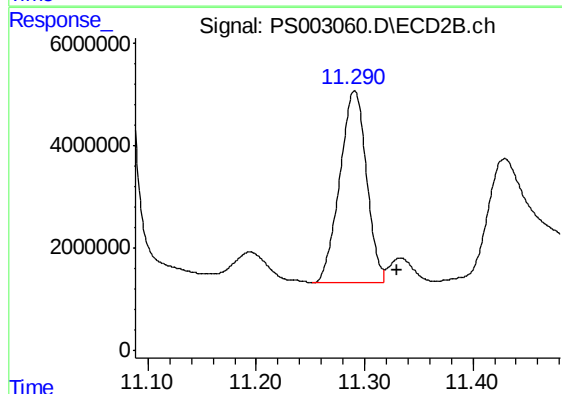


#6 MCPP

R.T.: 11.290 min
Delta R.T.: -0.040 min
Response: 64586295
Conc: 58.56 ug/ml m

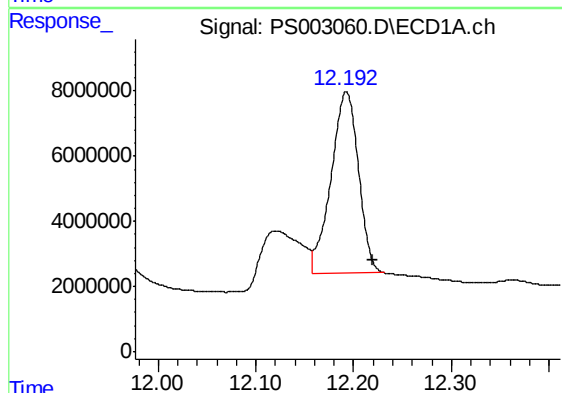


#7 MCPA

R.T.: 12.192 min
Delta R.T.: -0.027 min
Response: 108849758
Conc: 61.50 ug/ml m

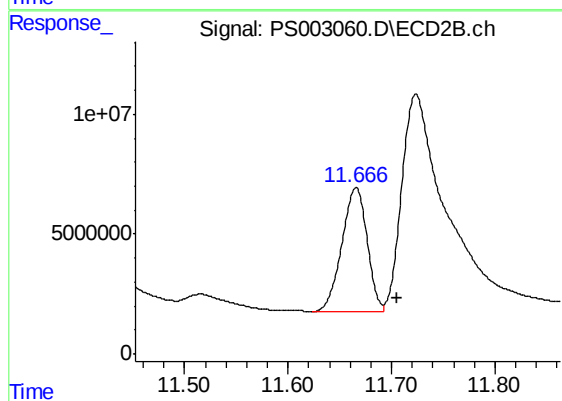

#7 MCPA


R.T.: 11.666 min
Delta R.T.: -0.041 min
Response: 87600550
Conc: 55.69 ug/ml m

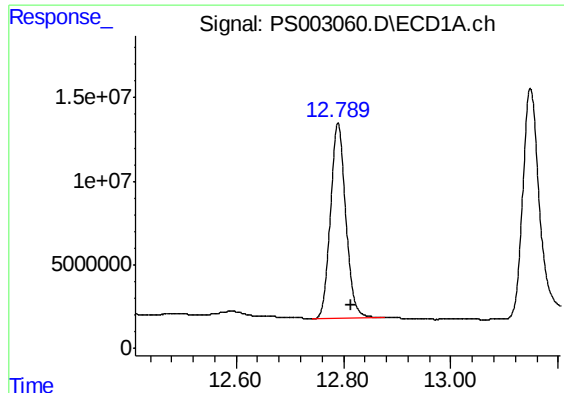

#8 DICHLORPROP


R.T.: 12.789 min
Delta R.T.: -0.025 min
Response: 232568450
Conc: 606.39 ng/ml m

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMS

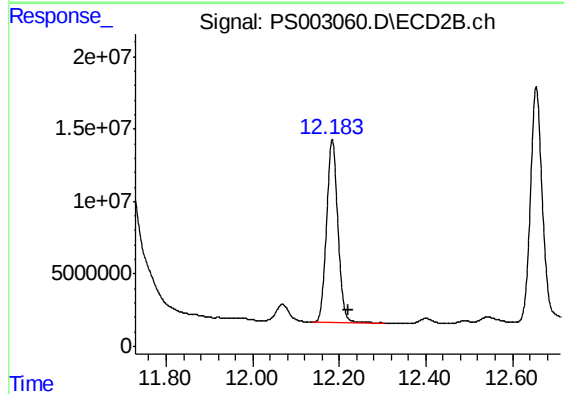


#8 DICHLORPROP

R.T.: 12.184 min
Delta R.T.: -0.038 min
Response: 226833377
Conc: 593.27 ng/ml

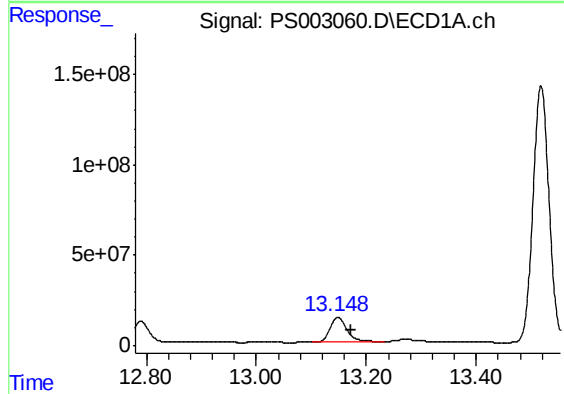


#9 2,4-D

R.T.: 13.148 min
Delta R.T.: -0.026 min
Response: 288032384
Conc: 624.72 ng/ml m

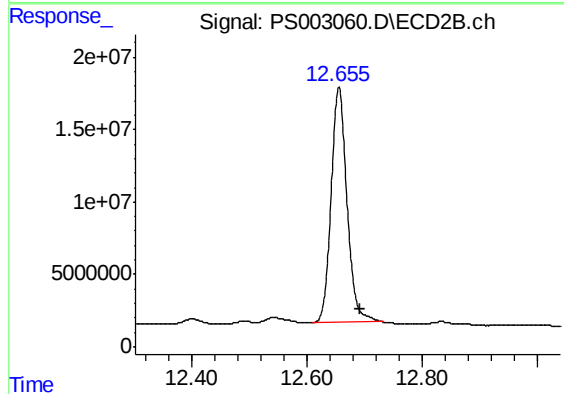

#9 2,4-D


R.T.: 12.655 min
Delta R.T.: -0.038 min
Response: 309804263
Conc: 617.90 ng/ml m

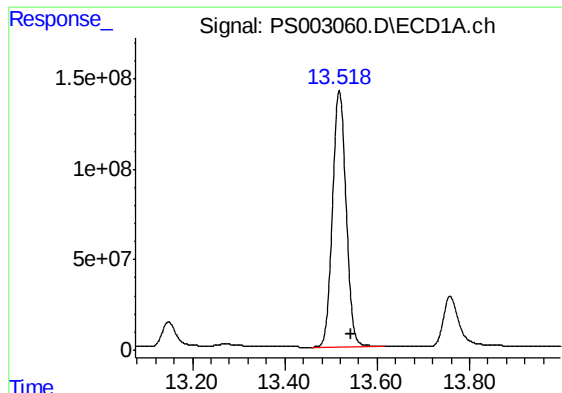

#10 Pentachlorophenol


R.T.: 13.518 min
Delta R.T.: -0.026 min
Response: 2883537617
Conc: 449.64 ng/ml m

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMS

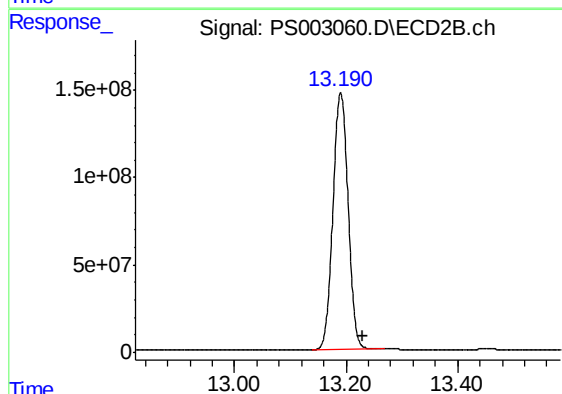


#10 Pentachlorophenol

R.T.: 13.190 min
Delta R.T.: -0.040 min
Response: 2767981998
Conc: 447.85 ng/ml m

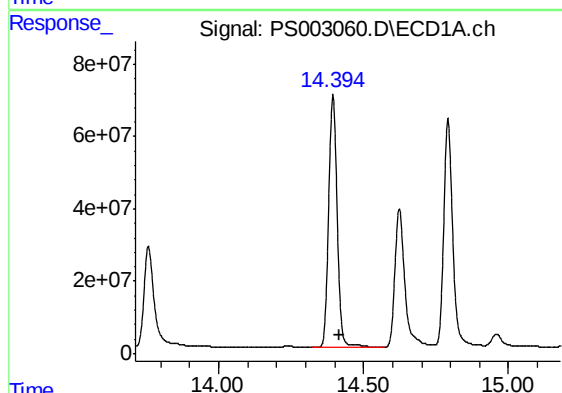


#11 2,4,5-TP (SILVEX)

R.T.: 14.395 min
Delta R.T.: -0.025 min
Response: 1432218760
Conc: 568.71 ng/ml

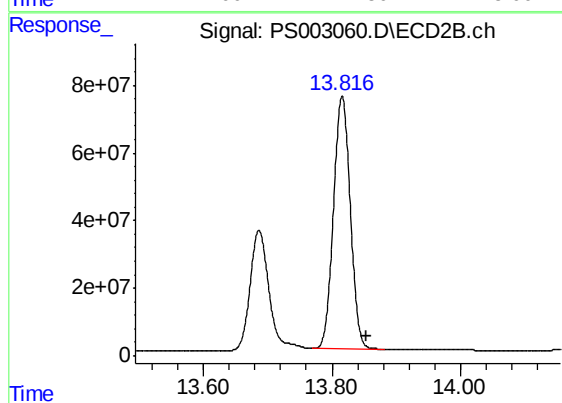

#11 2,4,5-TP (SILVEX)


R.T.: 13.816 min
Delta R.T.: -0.039 min
Response: 1359058214
Conc: 547.93 ng/ml m

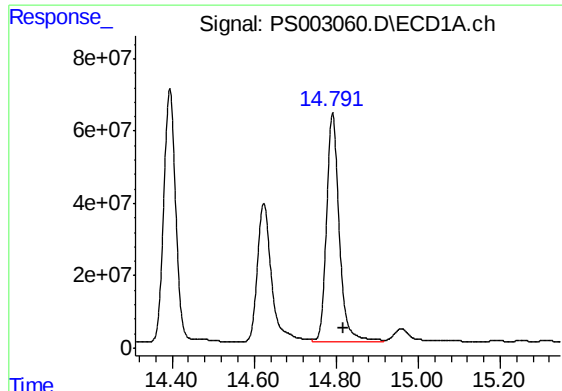

#12 2,4,5-T


R.T.: 14.791 min
Delta R.T.: -0.025 min
Response: 1355869834
Conc: 555.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMS

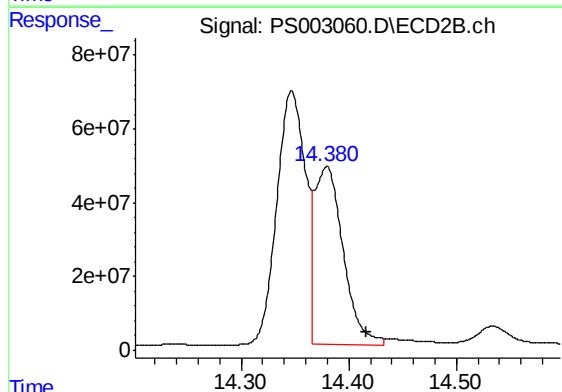


#12 2,4,5-T

R.T.: 14.380 min
Delta R.T.: -0.037 min
Response: 881245235
Conc: 460.54 ng/ml m

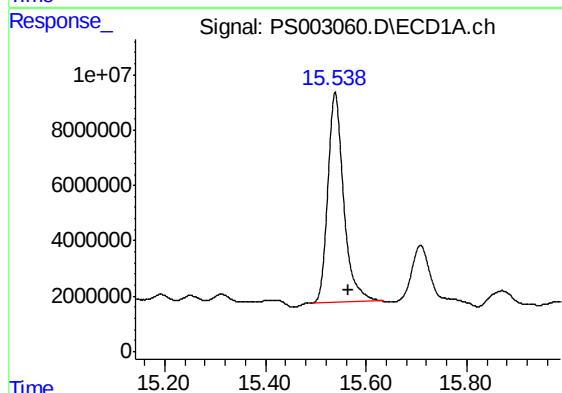


#13 2,4-DB

R.T.: 15.538 min
Delta R.T.: -0.027 min
Response: 166587580
Conc: 637.22 ng/ml m

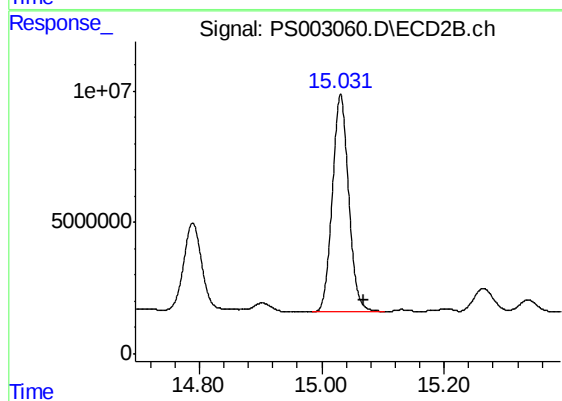

#13 2,4-DB


R.T.: 15.031 min
Delta R.T.: -0.038 min
Response: 153624791
Conc: 604.82 ng/ml m

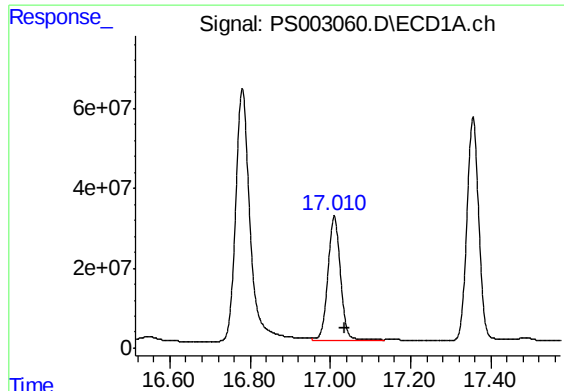

#14 DINOSEB


R.T.: 17.010 min
Delta R.T.: -0.026 min
Response: 688375333
Conc: 365.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMS

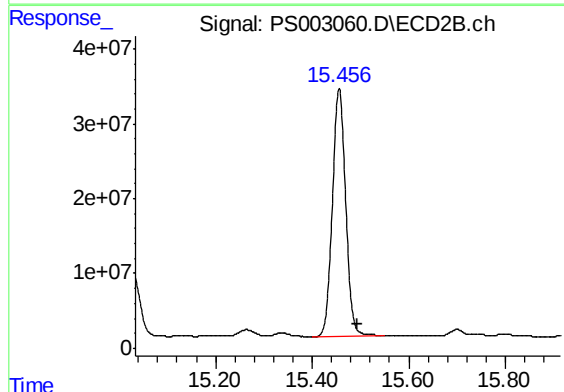


#14 DINOSEB

R.T.: 15.456 min
Delta R.T.: -0.039 min
Response: 632192524
Conc: 360.64 ng/ml m

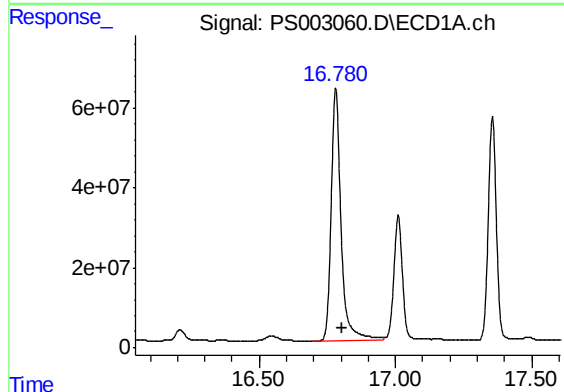


#15 Picloram

R.T.: 16.781 min
Delta R.T.: -0.025 min
Response: 1600718501
Conc: 505.97 ng/ml

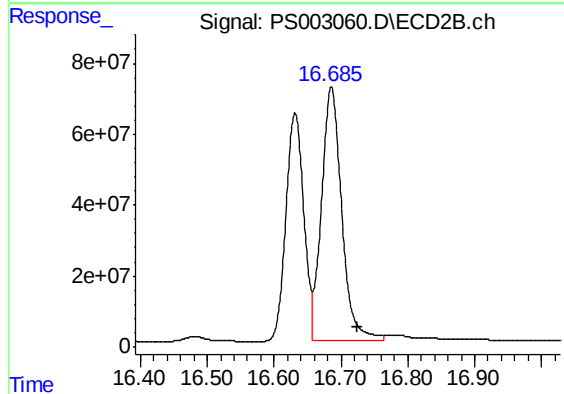

#15 Picloram


R.T.: 16.686 min
Delta R.T.: -0.039 min
Response: 1498036520
Conc: 498.28 ng/ml

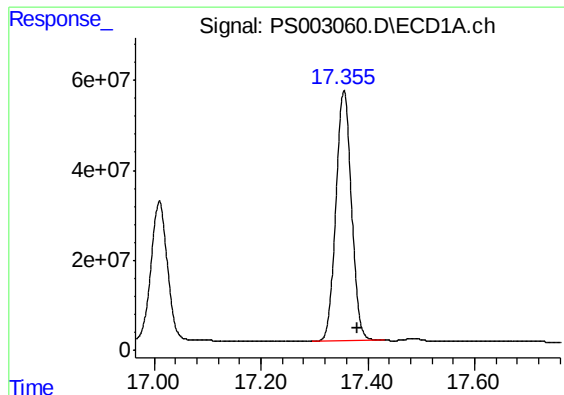

#16 DCPA

R.T.: 17.355 min
Delta R.T.: -0.026 min
Response: 1132110682
Conc: 376.45 ng/ml m

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMS

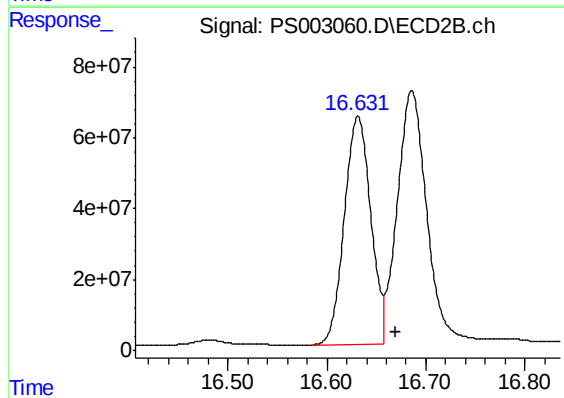

#16 DCPA

R.T.: 16.631 min
Delta R.T.: -0.039 min
Response: 1195355563
Conc: 385.90 ng/ml m