

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
 Data File : PS003061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 21:08
 Operator : EI\SJ
 Sample : K1338-02MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-06-020519-AMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:53:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.302	10.786	157.8E6	166.7E6	415.637	389.797
Target Compounds							
1) T	Dalapon	2.864	2.317	261.5E6	335.2E6	474.054m	625.551 #
2) T	3,5-DICHL...	9.729	8.945	295.3E6	288.2E6	512.859m	511.462m
5) T	DICAMBA	11.608	11.066	883.8E6	873.6E6	551.376	550.611m
6) T	MCP	11.953	11.297	81562434	64175037	68.075m	58.185m
7) T	MCPA	12.201	11.673	110.2E6	87063584	62.234m	55.347m
8) T	DICHLORPROP	12.798	12.191	226.6E6	226.1E6	590.765	591.247
9) T	2,4-D	13.157	12.661	295.5E6	311.5E6	640.965	621.293m
10) T	Pentachlo...	13.527	13.197	2874.4E6	2768.8E6	448.207	447.984m
11) T	2,4,5-TP ...	14.403	13.822	1430.5E6	1359.0E6	568.023	547.908m
12) T	2,4,5-T	14.800	14.387	1356.6E6	902.7E6	556.134	471.780m
13) T	2,4-DB	15.547	15.037	162.6E6	153.9E6	621.886	605.962m
14) T	DINOSEB	17.018	15.463	688.2E6	624.7E6	365.815	356.337m
15) T	Picloram	16.789	16.692	1620.9E6	1515.9E6	512.347	504.211
16) T	DCPA	17.362	16.638	1140.1E6	1200.1E6	379.095m	387.425m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : X:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020619\
Data File : PS003061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 21:08
Operator : EI\SJ
Sample : K1338-02MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 23:53:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

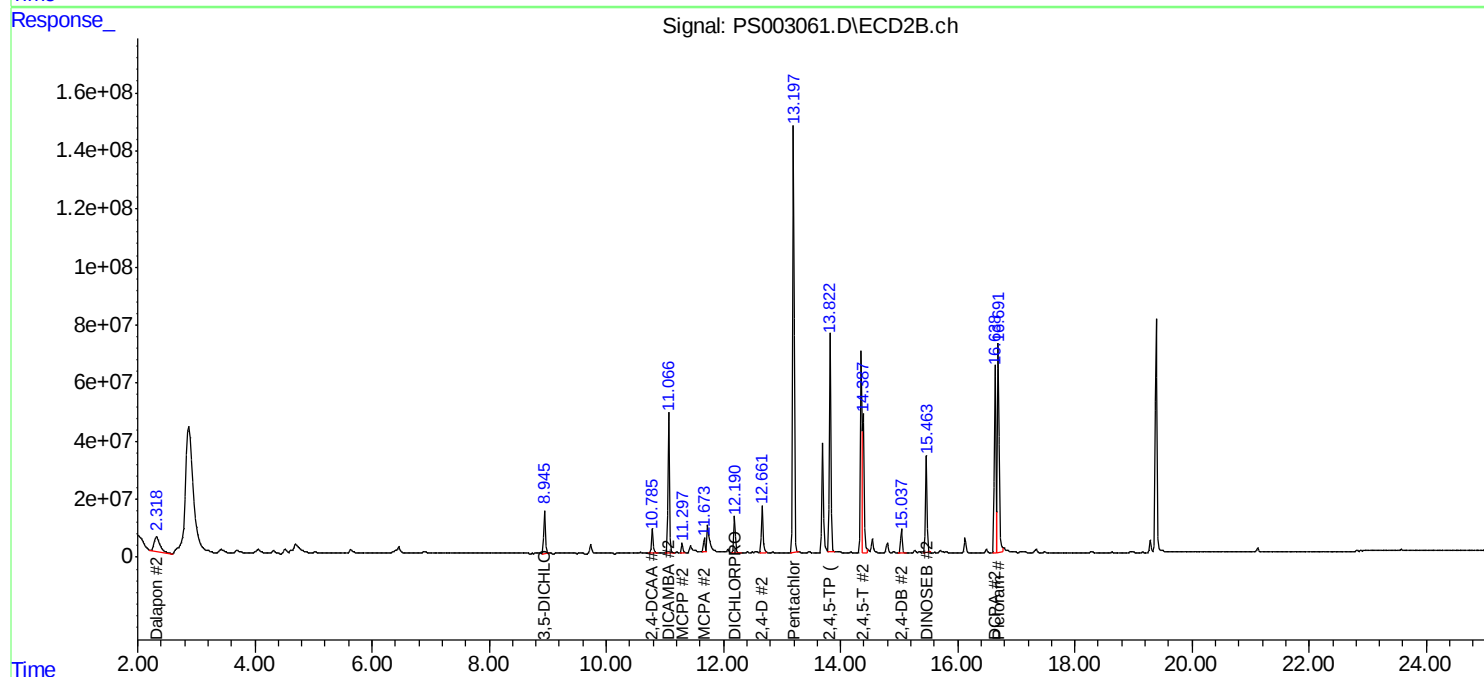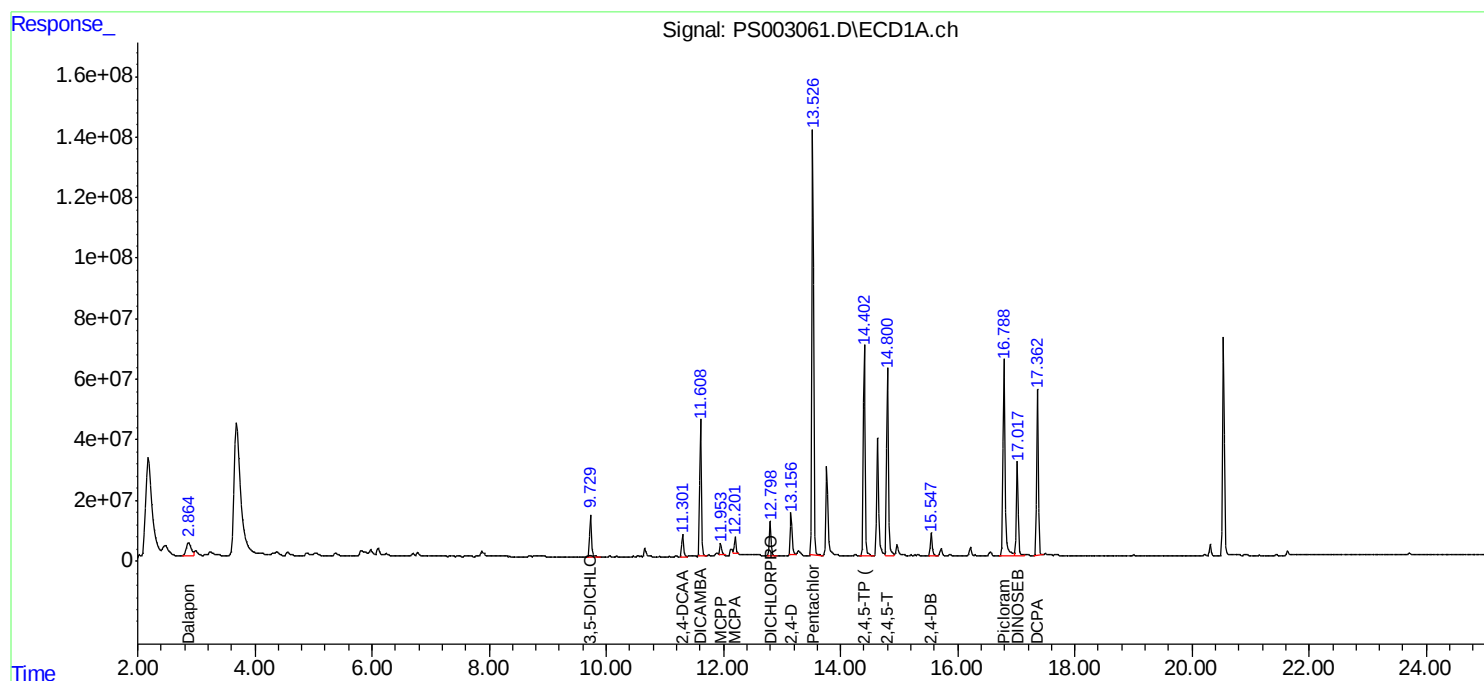


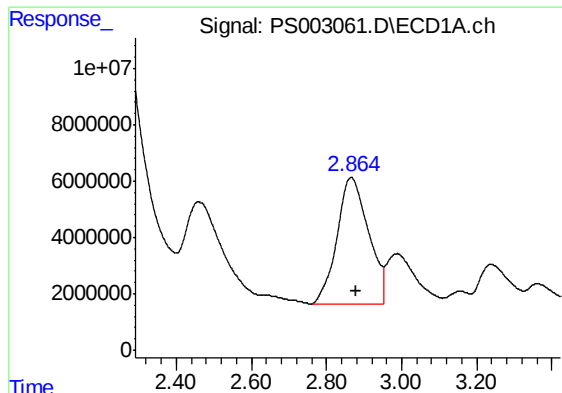

#1 Dalapon


R.T.: 2.864 min
Delta R.T.: -0.016 min
Response: 261510618
Conc: 474.05 ng/ml m

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMSD

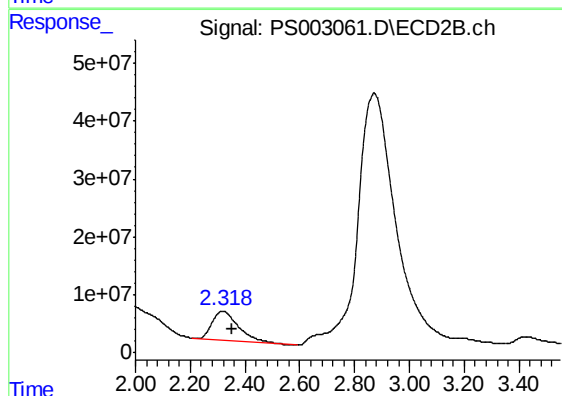


#1 Dalapon

R.T.: 2.317 min
Delta R.T.: -0.034 min
Response: 335245918
Conc: 625.55 ng/ml

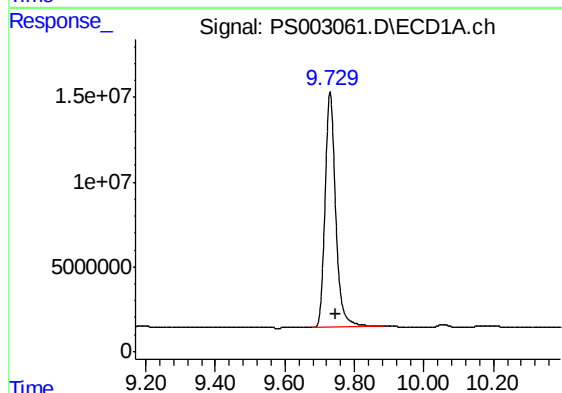


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.729 min
Delta R.T.: -0.016 min
Response: 295326020
Conc: 512.86 ng/ml m

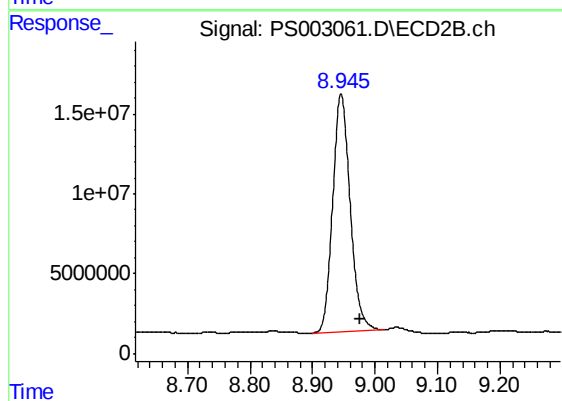

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.945 min
Delta R.T.: -0.031 min
Response: 288243921
Conc: 511.46 ng/ml m

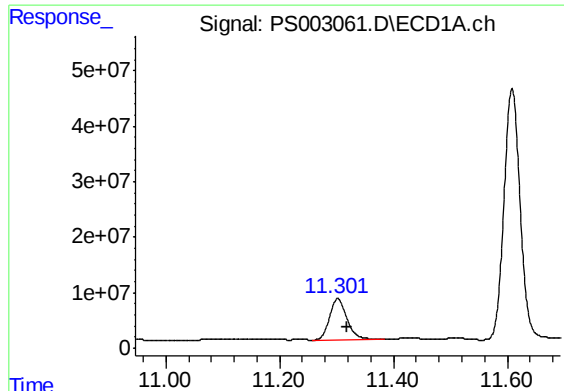

#4 2,4-DCAA


R.T.: 11.302 min
Delta R.T.: -0.015 min
Response: 157792889
Conc: 415.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMSD

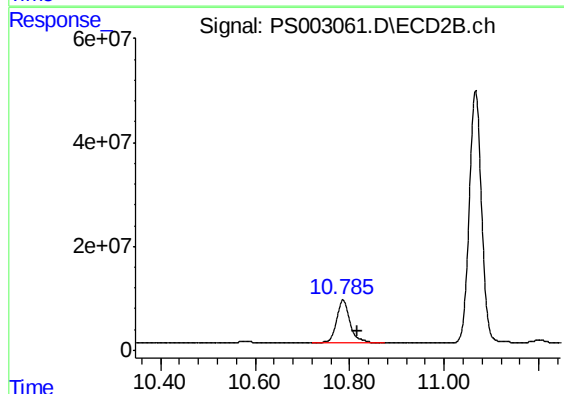


#4 2,4-DCAA

R.T.: 10.786 min
Delta R.T.: -0.031 min
Response: 166656132
Conc: 389.80 ng/ml

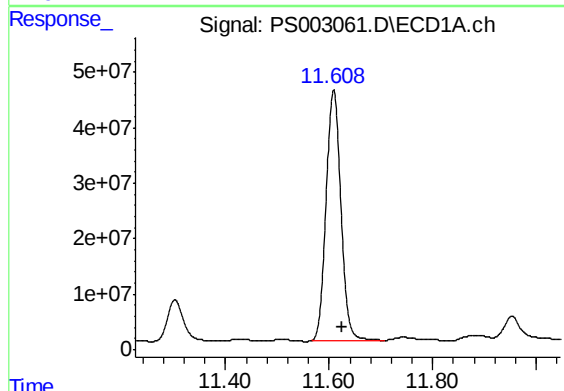


#5 DICAMBA

R.T.: 11.608 min
Delta R.T.: -0.016 min
Response: 883793309
Conc: 551.38 ng/ml

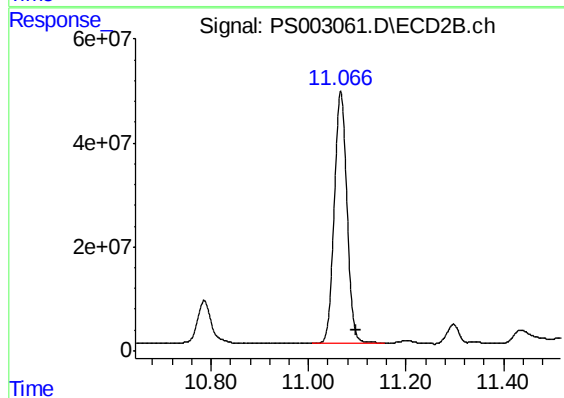

#5 DICAMBA


R.T.: 11.066 min
Delta R.T.: -0.031 min
Response: 873636066
Conc: 550.61 ng/ml m

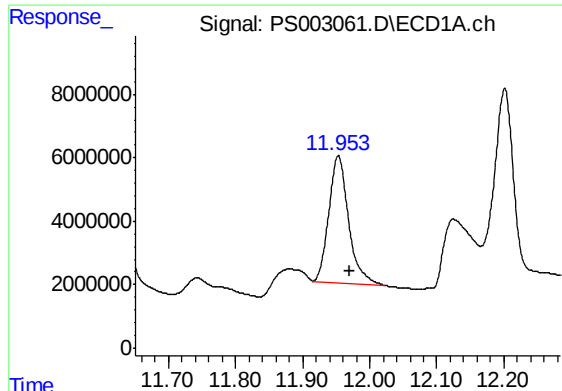

#6 MCPP


R.T.: 11.953 min
Delta R.T.: -0.016 min
Response: 81562434
Conc: 68.08 ug/ml m

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMSD

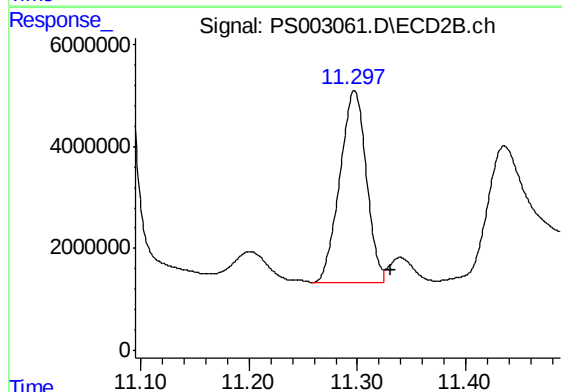


#6 MCPP

R.T.: 11.297 min
Delta R.T.: -0.033 min
Response: 64175037
Conc: 58.18 ug/ml m

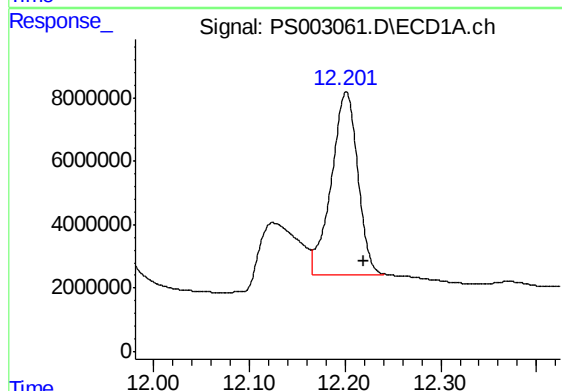


#7 MCPA

R.T.: 12.201 min
Delta R.T.: -0.018 min
Response: 110151876
Conc: 62.23 ug/ml m

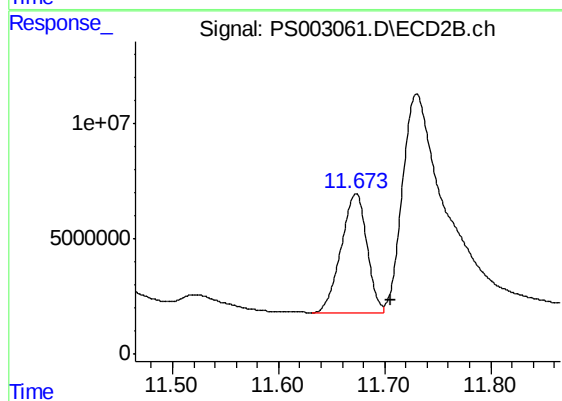

#7 MCPA


R.T.: 11.673 min
Delta R.T.: -0.033 min
Response: 87063584
Conc: 55.35 ug/ml m

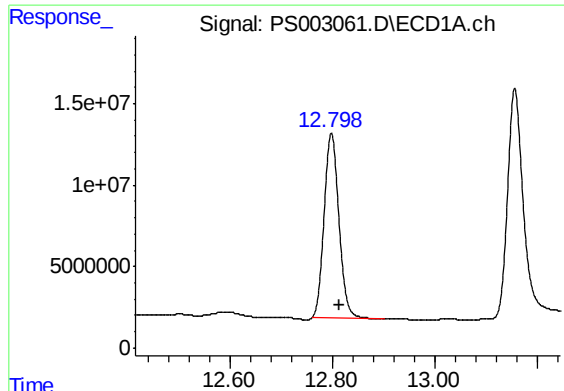

#8 DICHLORPROP


R.T.: 12.798 min
Delta R.T.: -0.017 min
Response: 226576382
Conc: 590.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMSD

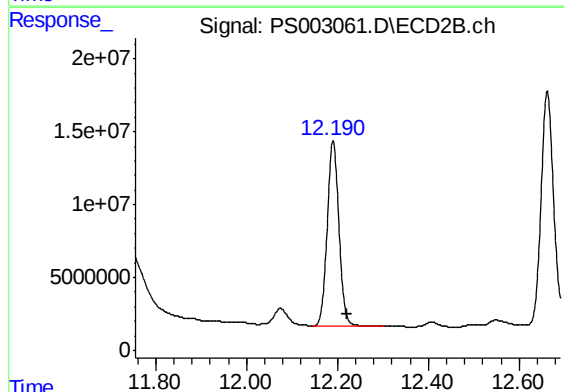


#8 DICHLORPROP

R.T.: 12.191 min
Delta R.T.: -0.031 min
Response: 226058215
Conc: 591.25 ng/ml

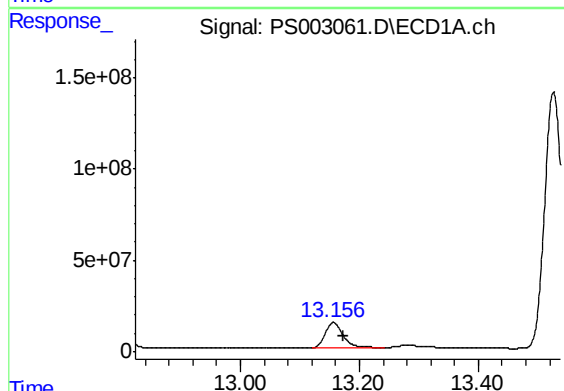


#9 2,4-D

R.T.: 13.157 min
Delta R.T.: -0.017 min
Response: 295522281
Conc: 640.97 ng/ml

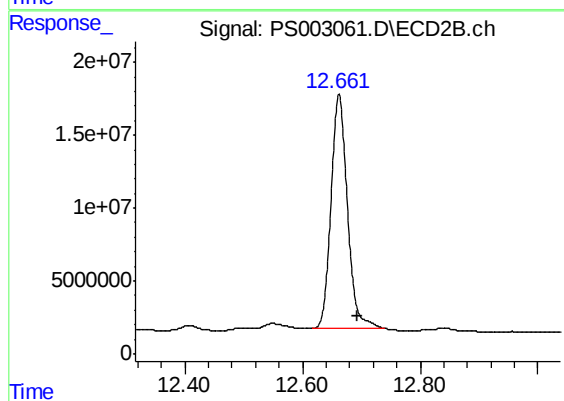

#9 2,4-D


R.T.: 12.661 min
Delta R.T.: -0.031 min
Response: 311507505
Conc: 621.29 ng/ml m

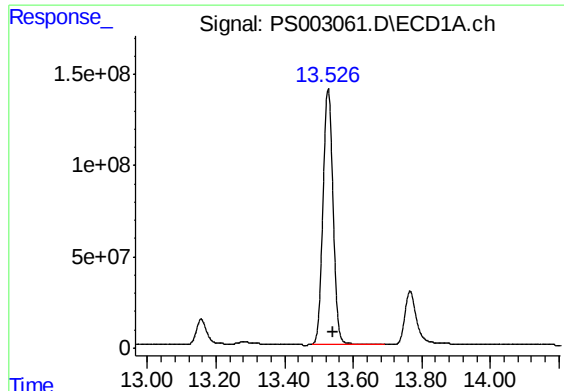

#10 Pentachlorophenol


R.T.: 13.527 min
Delta R.T.: -0.017 min
Response: 2874351769
Conc: 448.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMSD

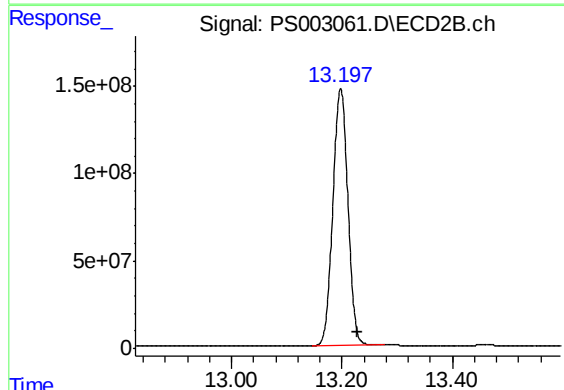


#10 Pentachlorophenol

R.T.: 13.197 min
Delta R.T.: -0.032 min
Response: 2768815546
Conc: 447.98 ng/ml m

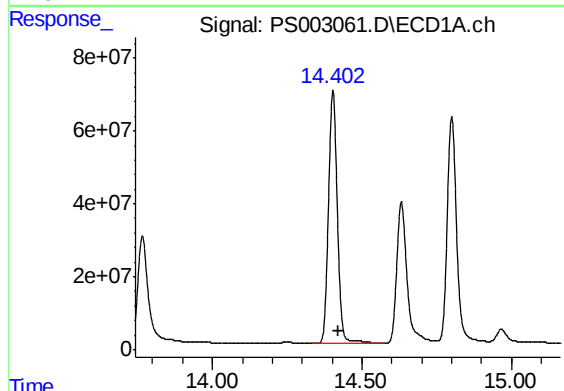


#11 2,4,5-TP (SILVEX)

R.T.: 14.403 min
Delta R.T.: -0.017 min
Response: 1430494252
Conc: 568.02 ng/ml

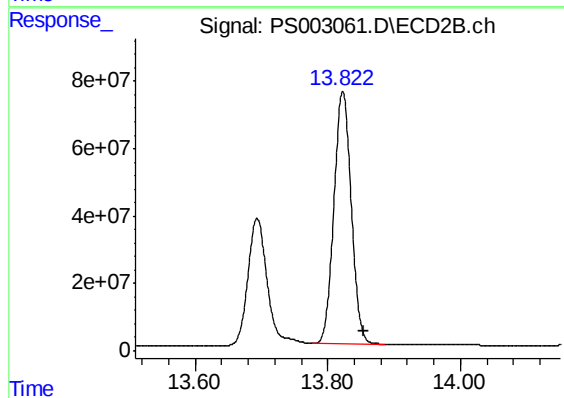

#11 2,4,5-TP (SILVEX)


R.T.: 13.822 min
Delta R.T.: -0.032 min
Response: 1359006831
Conc: 547.91 ng/ml m

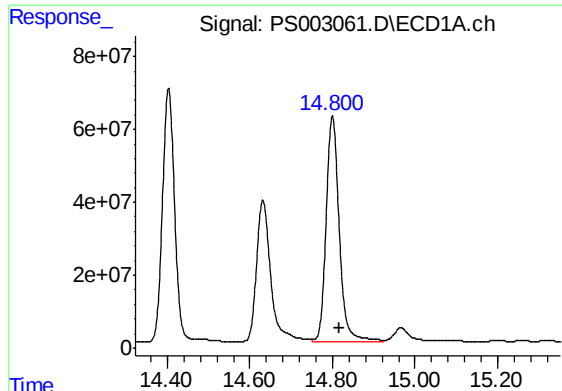

#12 2,4,5-T


R.T.: 14.800 min
Delta R.T.: -0.017 min
Response: 1356637197
Conc: 556.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMSD

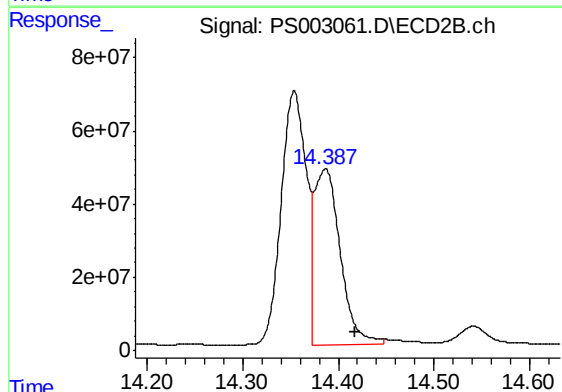


#12 2,4,5-T

R.T.: 14.387 min
Delta R.T.: -0.030 min
Response: 902745918
Conc: 471.78 ng/ml m

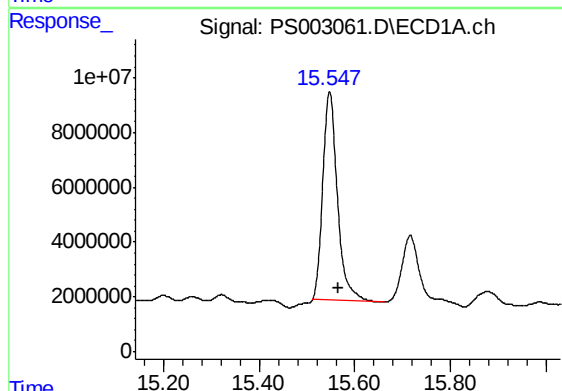


#13 2,4-DB

R.T.: 15.547 min
Delta R.T.: -0.017 min
Response: 162578607
Conc: 621.89 ng/ml

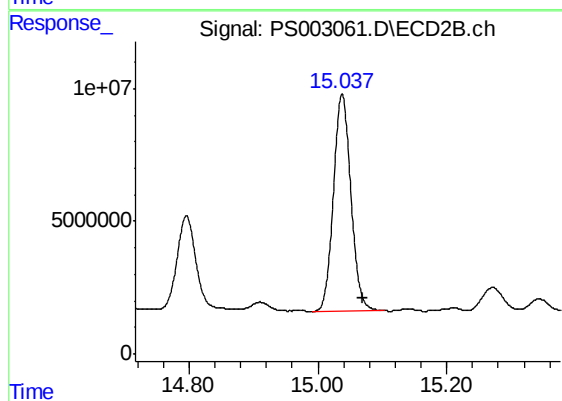

#13 2,4-DB


R.T.: 15.037 min
Delta R.T.: -0.032 min
Response: 153913896
Conc: 605.96 ng/ml m

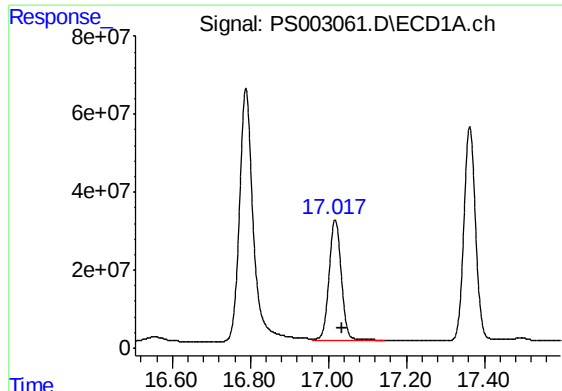

#14 DINOSEB


R.T.: 17.018 min
Delta R.T.: -0.017 min
Response: 688218227
Conc: 365.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMSD

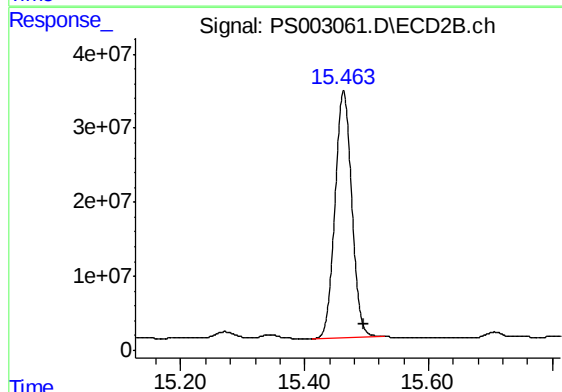


#14 DINOSEB

R.T.: 15.463 min
Delta R.T.: -0.032 min
Response: 624657153
Conc: 356.34 ng/ml m

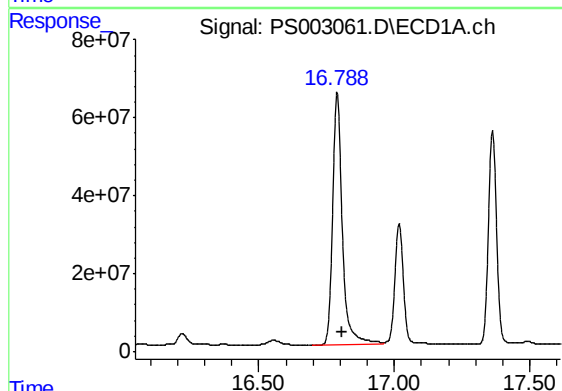


#15 Picloram

R.T.: 16.789 min
Delta R.T.: -0.017 min
Response: 1620877592
Conc: 512.35 ng/ml

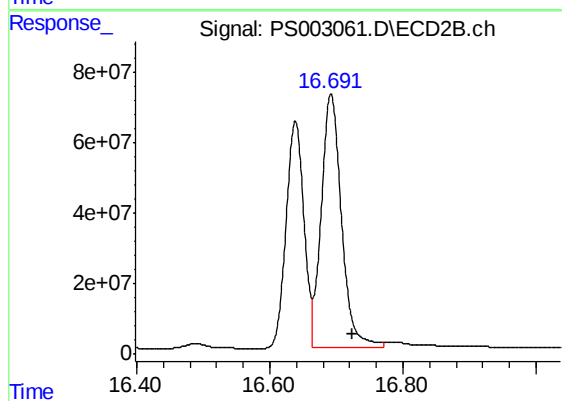

#15 Picloram


R.T.: 16.692 min
Delta R.T.: -0.032 min
Response: 1515862464
Conc: 504.21 ng/ml

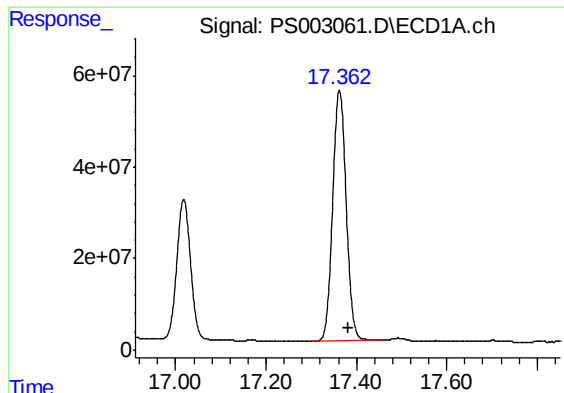

#16 DCPA

R.T.: 17.362 min
Delta R.T.: -0.020 min
Response: 1140051705
Conc: 379.10 ng/ml m

Instrument :
ECD_S
ClientSampleId :
AU-06-020519-AMSD

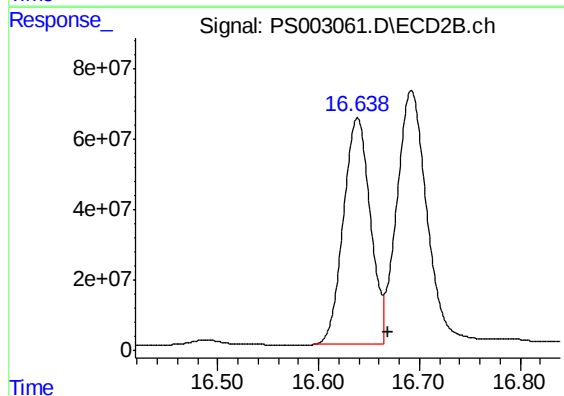

#16 DCPA

R.T.: 16.638 min
Delta R.T.: -0.032 min
Response: 1200083922
Conc: 387.43 ng/ml m