

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
 Data File : PS025768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 13:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 15:38:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.347	6.754	728.8E6	363.6E6	516.449	516.835
Target Compounds							
1) T	Dalapon	0.000	2.555	0	1685725	N.D.	1.520
6) T	MCP	6.704f	0.000	17226135	0	4.735	N.D. #
7) T	MCPA	6.704f	7.229	17226135	1470631	3.200	<MDL #
8) T	DICHLORPROP	0.000	7.546	0	6157174	N.D.	7.710
9) T	2,4-D	0.000	7.757f	0	353270	N.D.	<MDL
10) T	Pentachlo...	0.000	8.227	0	8748155	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.588	0	1076858	N.D.	<MDL
12) T	2,4,5-T	0.000	8.970	0	1017919	N.D.	<MDL
14) T	DINOSEB	0.000	9.785	0	1093469	N.D.	<MDL
15) T	Picloram	0.000	10.760	0	5099268	N.D.	<MDL
16) T	DCPA	0.000	10.705	0	2006574	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
Data File : PS025768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 13:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 15:38:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

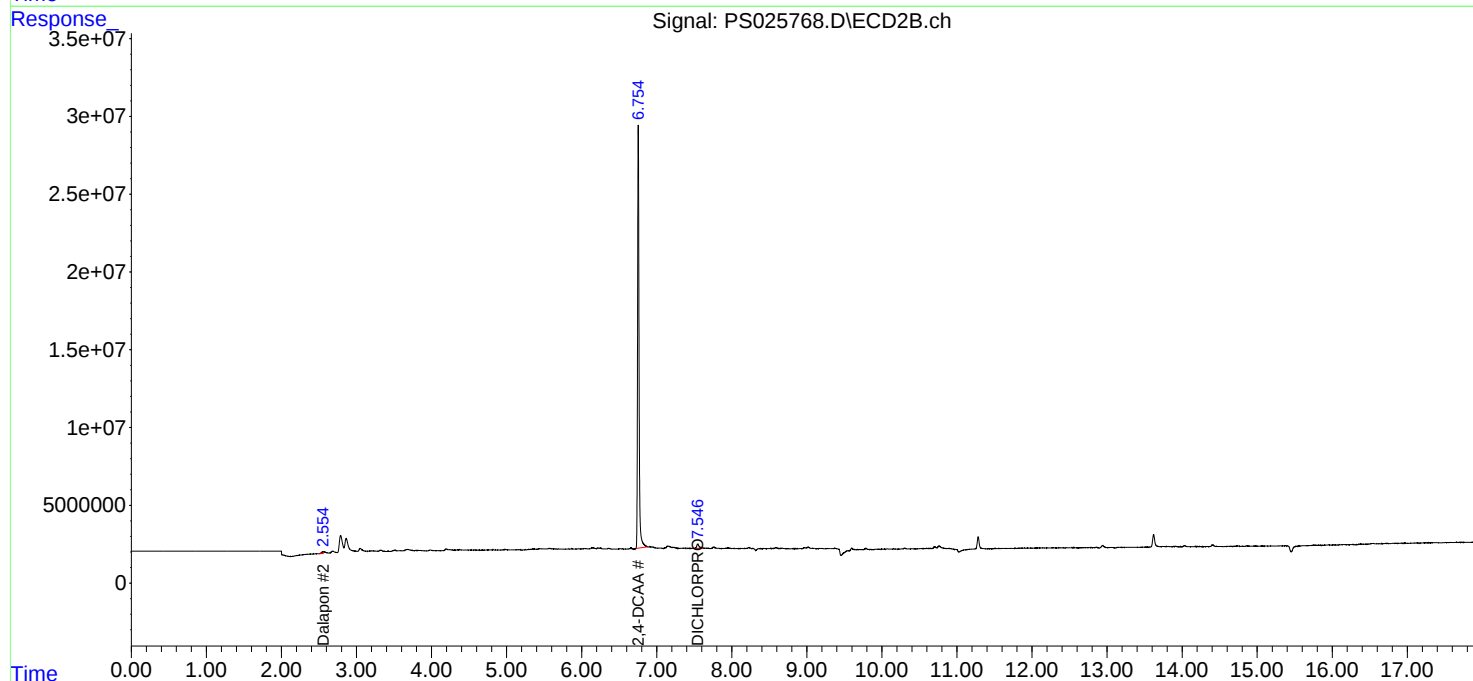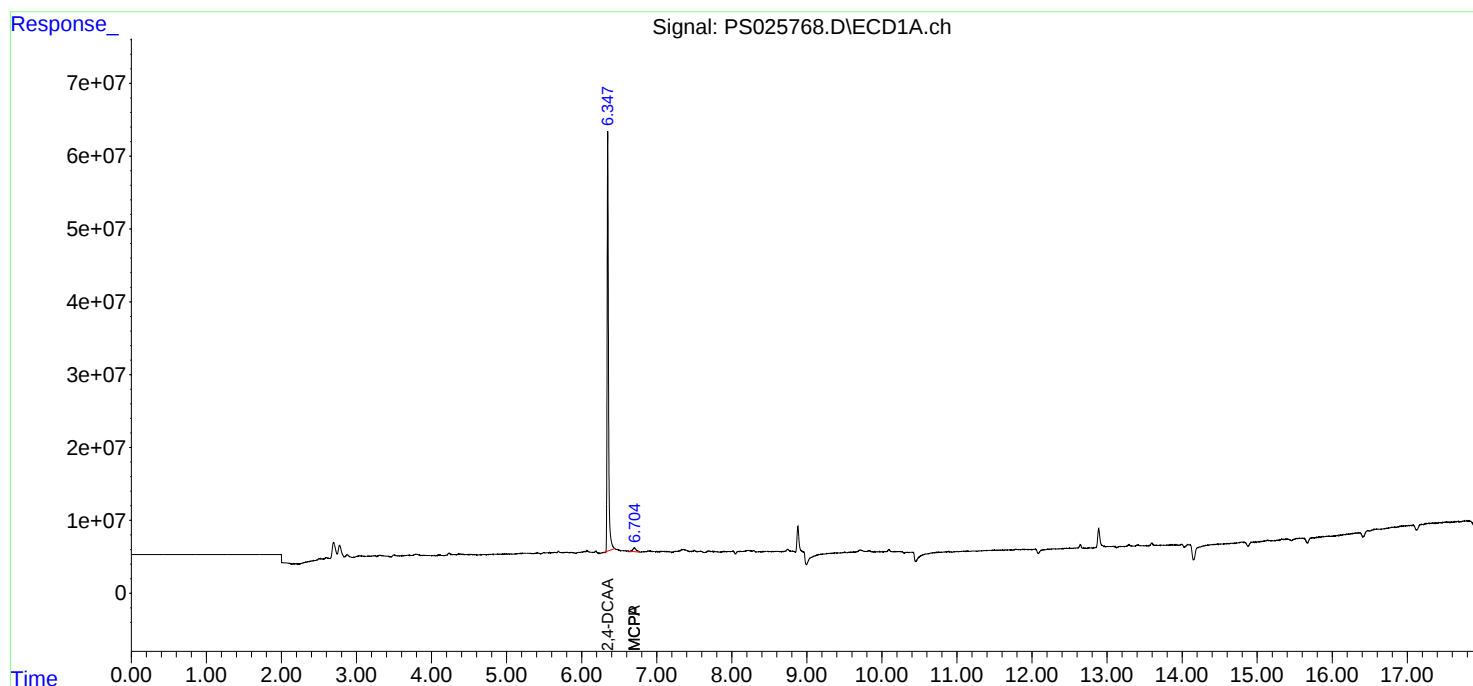


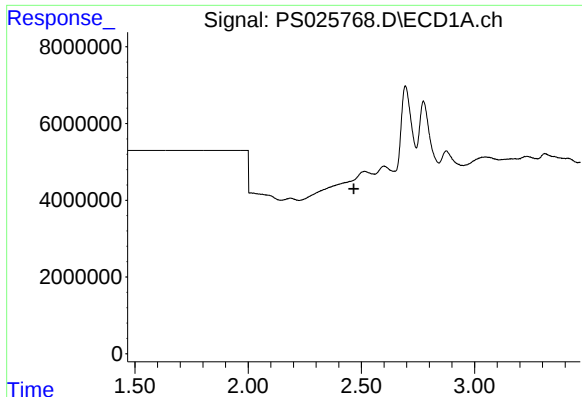

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

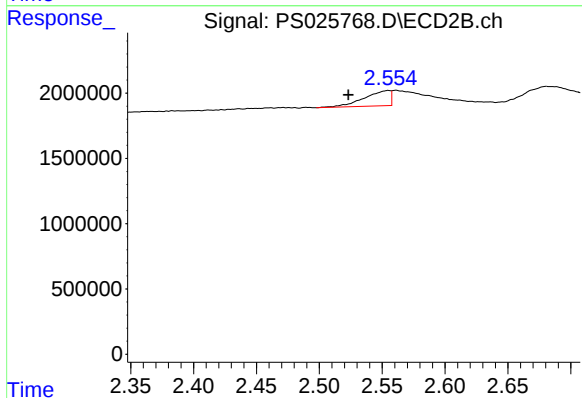


#1 Dalapon

R.T.: 2.555 min
Delta R.T.: 0.032 min
Response: 1685725
Conc: 1.52 ng/ml

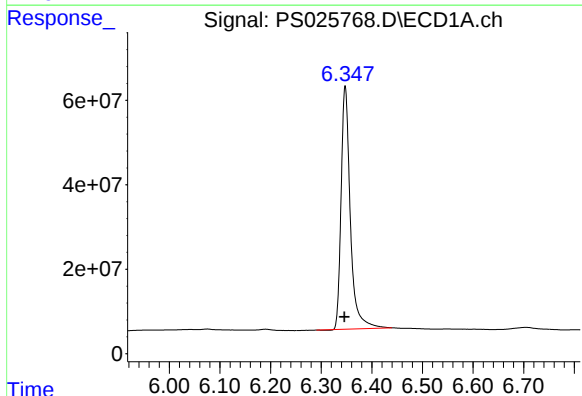


#4 2,4-DCAA

R.T.: 6.347 min
Delta R.T.: 0.002 min
Response: 728839025
Conc: 516.45 ng/ml

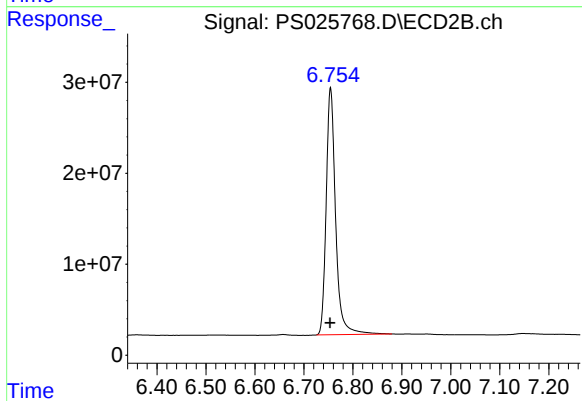

#4 2,4-DCAA


R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 363564462
Conc: 516.84 ng/ml

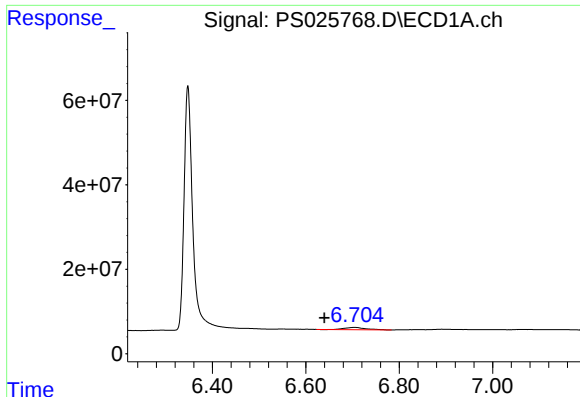

#6 MCPP


R.T.: 6.704 min
Delta R.T.: 0.064 min
Response: 17226135
Conc: 4.74 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

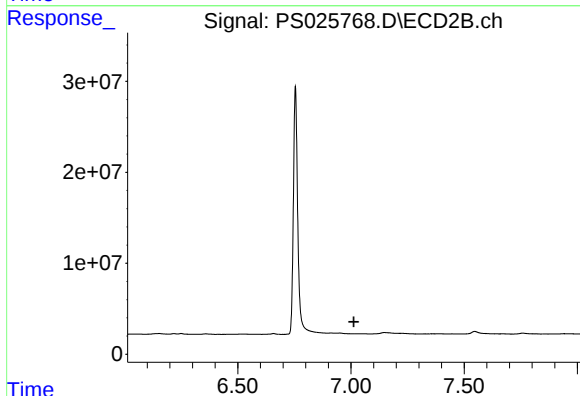


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.013 min
Response: 0
Conc: N.D.

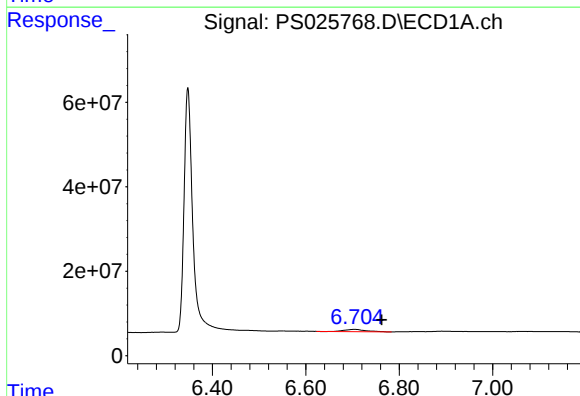


#7 MCPA

R.T.: 6.704 min
Delta R.T.: -0.059 min
Response: 17226135
Conc: 3.20 ug/ml

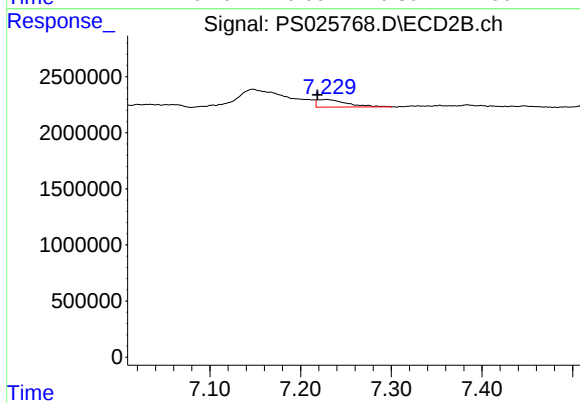

#7 MCPA


R.T.: 7.229 min
Delta R.T.: 0.011 min
Response: 1470631
Conc: N.D.

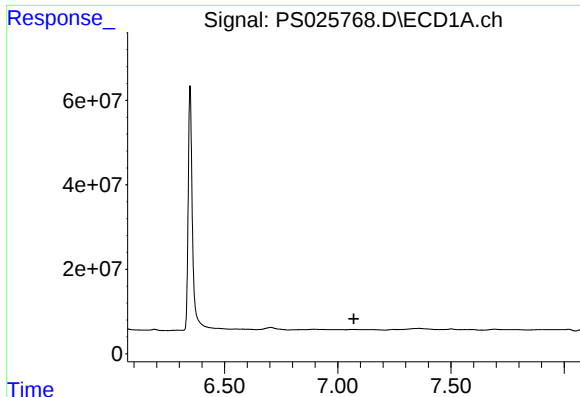

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

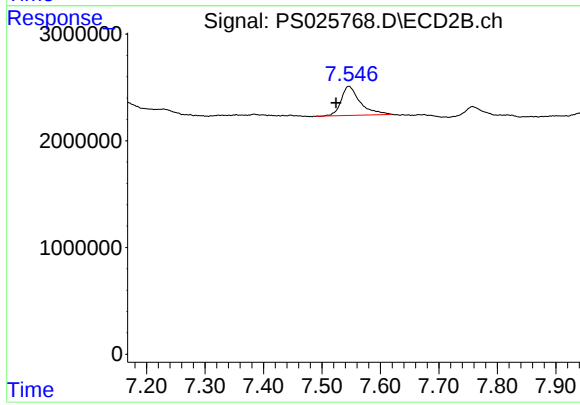

#8 DICHLORPROP

R.T.: 7.546 min
Delta R.T.: 0.022 min
Response: 6157174
Conc: 7.71 ng/ml