

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
 Data File : PS025775.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 16:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 16:25:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.349	6.755	730.4E6	366.6E6	517.522	521.174
Target Compounds							
1) T	Dalapon	0.000	2.557	0	1663108	N.D.	1.499
5) T	DICAMBA	0.000	6.952	0	1589091	N.D.	<MDL
6) T	MCP	0.000	6.952f	0	1589091	N.D.	<MDL
7) T	MCPA	6.714f	7.149f	18685824	6956653	3.471	2.233 #
8) T	DICHLORPROP	0.000	7.555	0	7548993	N.D.	9.453
10) T	Pentachlo...	0.000	8.229	0	4796554	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.594	0	934179	N.D.	<MDL
12) T	2,4,5-T	0.000	8.978	0	622194	N.D.	<MDL
14) T	DINOSEB	0.000	9.789	0	1750827	N.D.	<MDL
15) T	Picloram	0.000	10.706	0	1781538	N.D.	<MDL
16) T	DCPA	0.000	10.706	0	1781538	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
Data File : PS025775.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 16:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 16:25:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

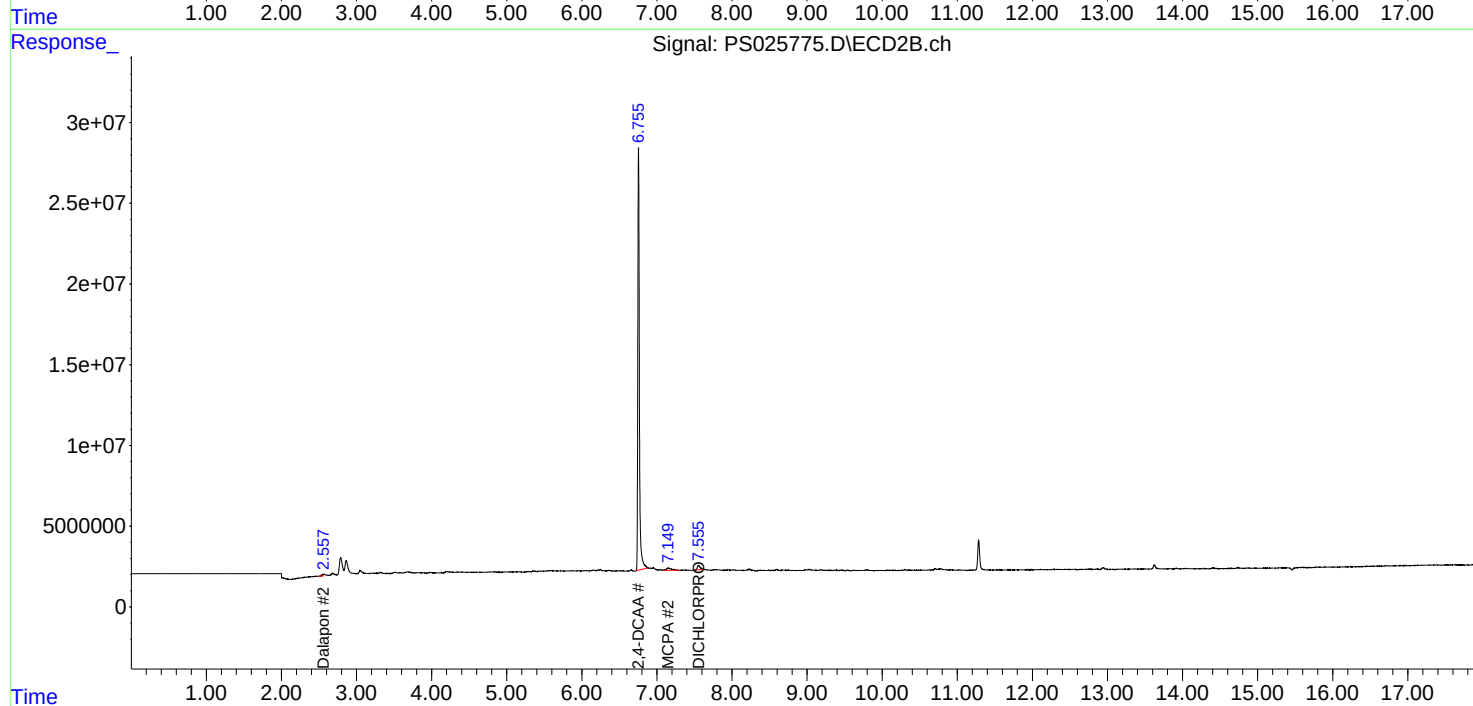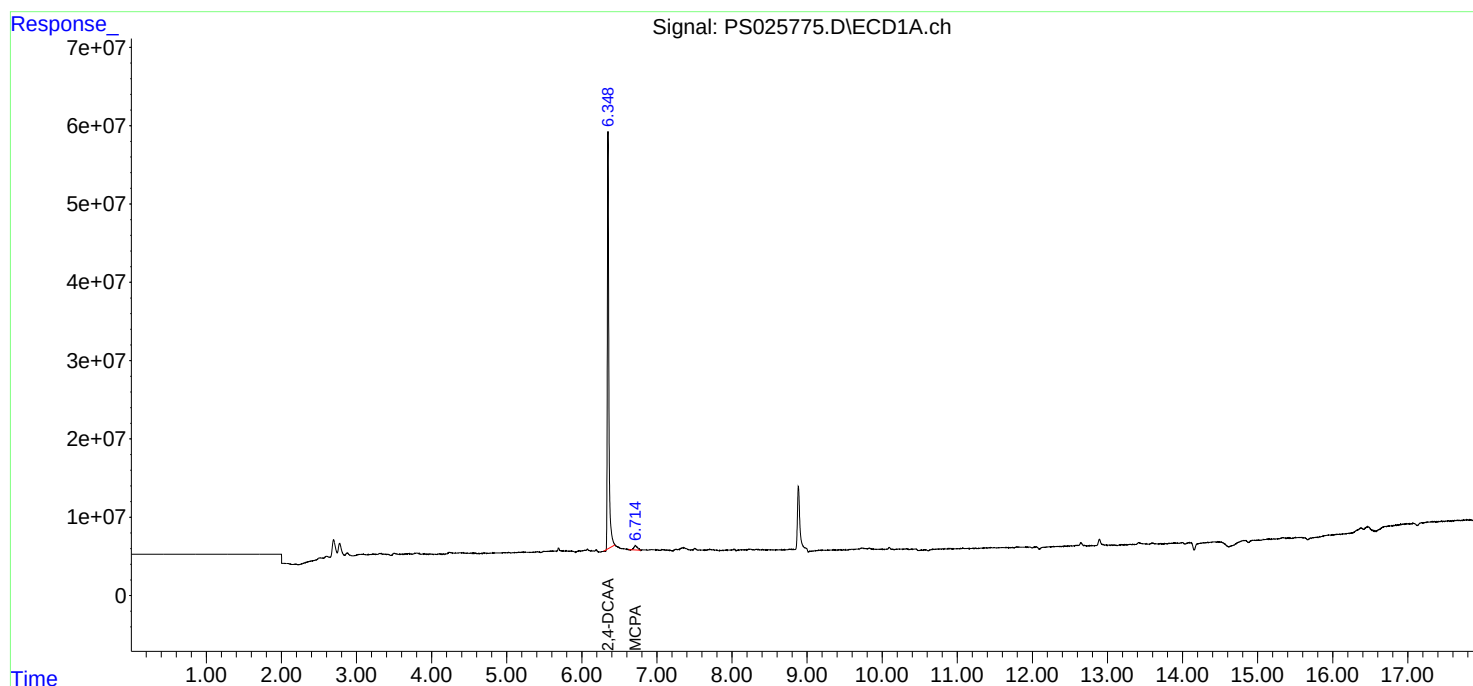


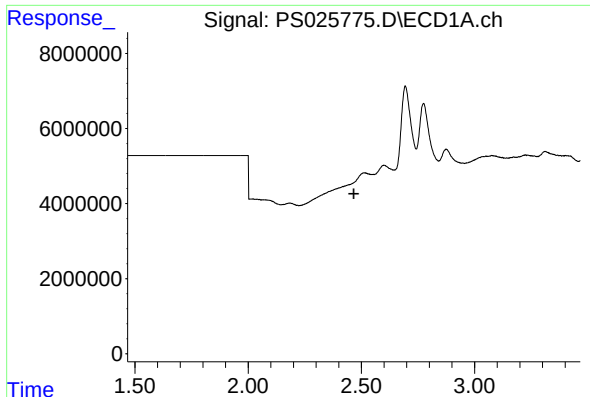

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

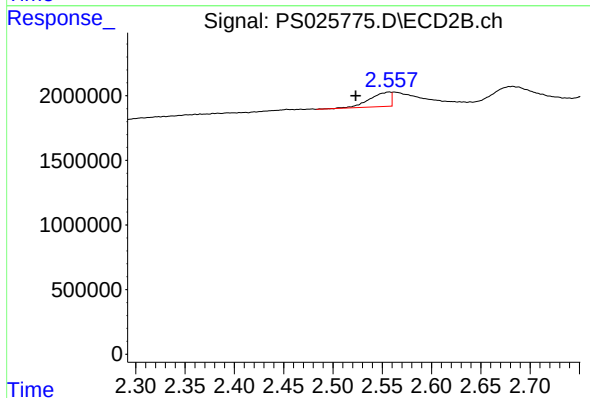


#1 Dalapon

R.T.: 2.557 min
Delta R.T.: 0.034 min
Response: 1663108
Conc: 1.50 ng/ml

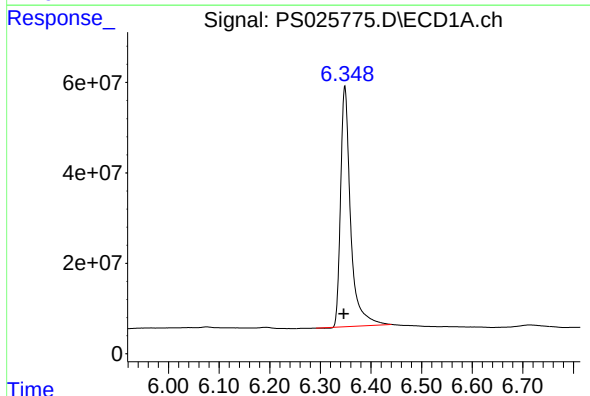


#4 2,4-DCAA

R.T.: 6.349 min
Delta R.T.: 0.003 min
Response: 730353863
Conc: 517.52 ng/ml

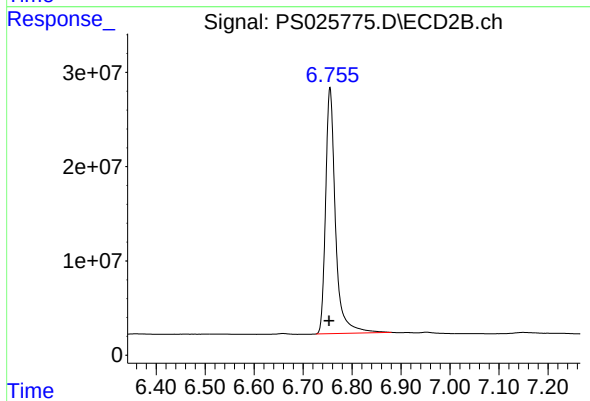

#4 2,4-DCAA


R.T.: 6.755 min
Delta R.T.: 0.002 min
Response: 366616703
Conc: 521.17 ng/ml

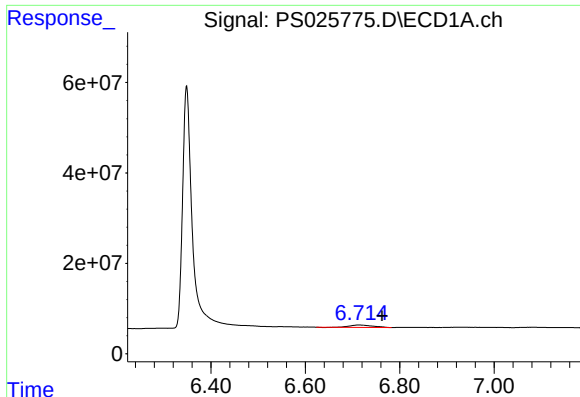

#7 MCPA


R.T.: 6.714 min
Delta R.T.: -0.049 min
Response: 18685824
Conc: 3.47 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

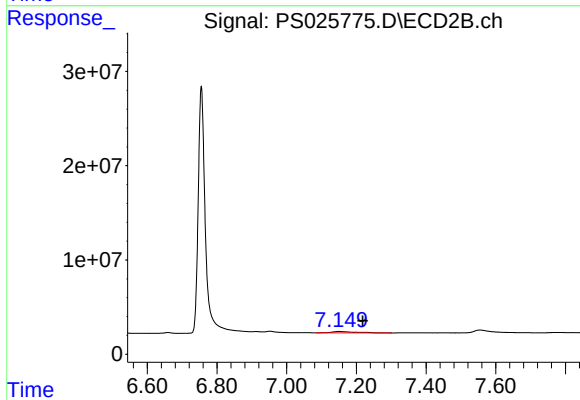


#7 MCPA

R.T.: 7.149 min
Delta R.T.: -0.069 min
Response: 6956653
Conc: 2.23 ug/ml

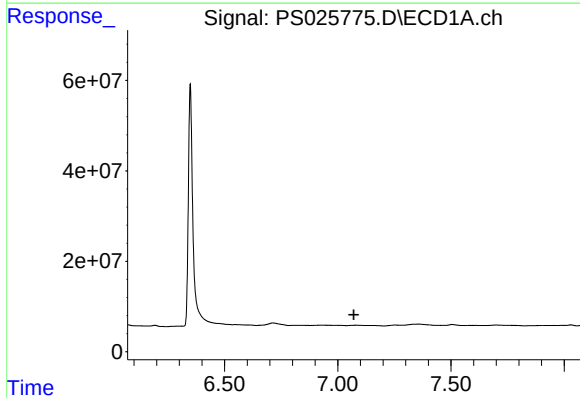

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.071 min
Response: 0
Conc: N.D.

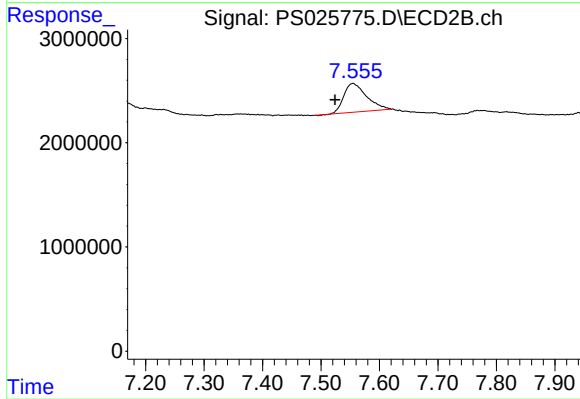

#8 DICHLORPROP

R.T.: 7.555 min
Delta R.T.: 0.031 min
Response: 7548993
Conc: 9.45 ng/ml