

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
 Data File : PS025795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2024 00:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 04:15:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.349	6.753	725.0E6	366.3E6	513.732	520.661
Target Compounds							
1) T	Dalapon	0.000	2.552	0	3272904	N.D.	2.951
2) T	3,5-DICHL...	5.691	0.000	4570449	0	2.121	N.D. #
3) T	4-Nitroph...	0.000	6.360	0	373387	N.D.	<MDL
5) T	DICAMBA	0.000	6.912	0	254137	N.D.	<MDL
6) T	MCP	6.684f	7.020	72831553	1356271	20.020	<MDL #
8) T	DICHLORPROP	0.000	7.540	0	36484866	N.D.	45.688
9) T	2,4-D	7.244	7.756f	53615986	754125	30.169	<MDL #
10) T	Pentachlo...	0.000	8.224	0	2796013	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.589	0	521186	N.D.	<MDL
12) T	2,4,5-T	0.000	8.964	0	592172	N.D.	<MDL
13) T	2,4-DB	0.000	9.455	0	954014	N.D.	2.154
14) T	DINOSEB	0.000	9.782	0	848870	N.D.	<MDL
15) T	Picloram	0.000	10.758	0	1964338	N.D.	<MDL
16) T	DCPA	0.000	10.701	0	1631917	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
Data File : PS025795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2024 00:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 04:15:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

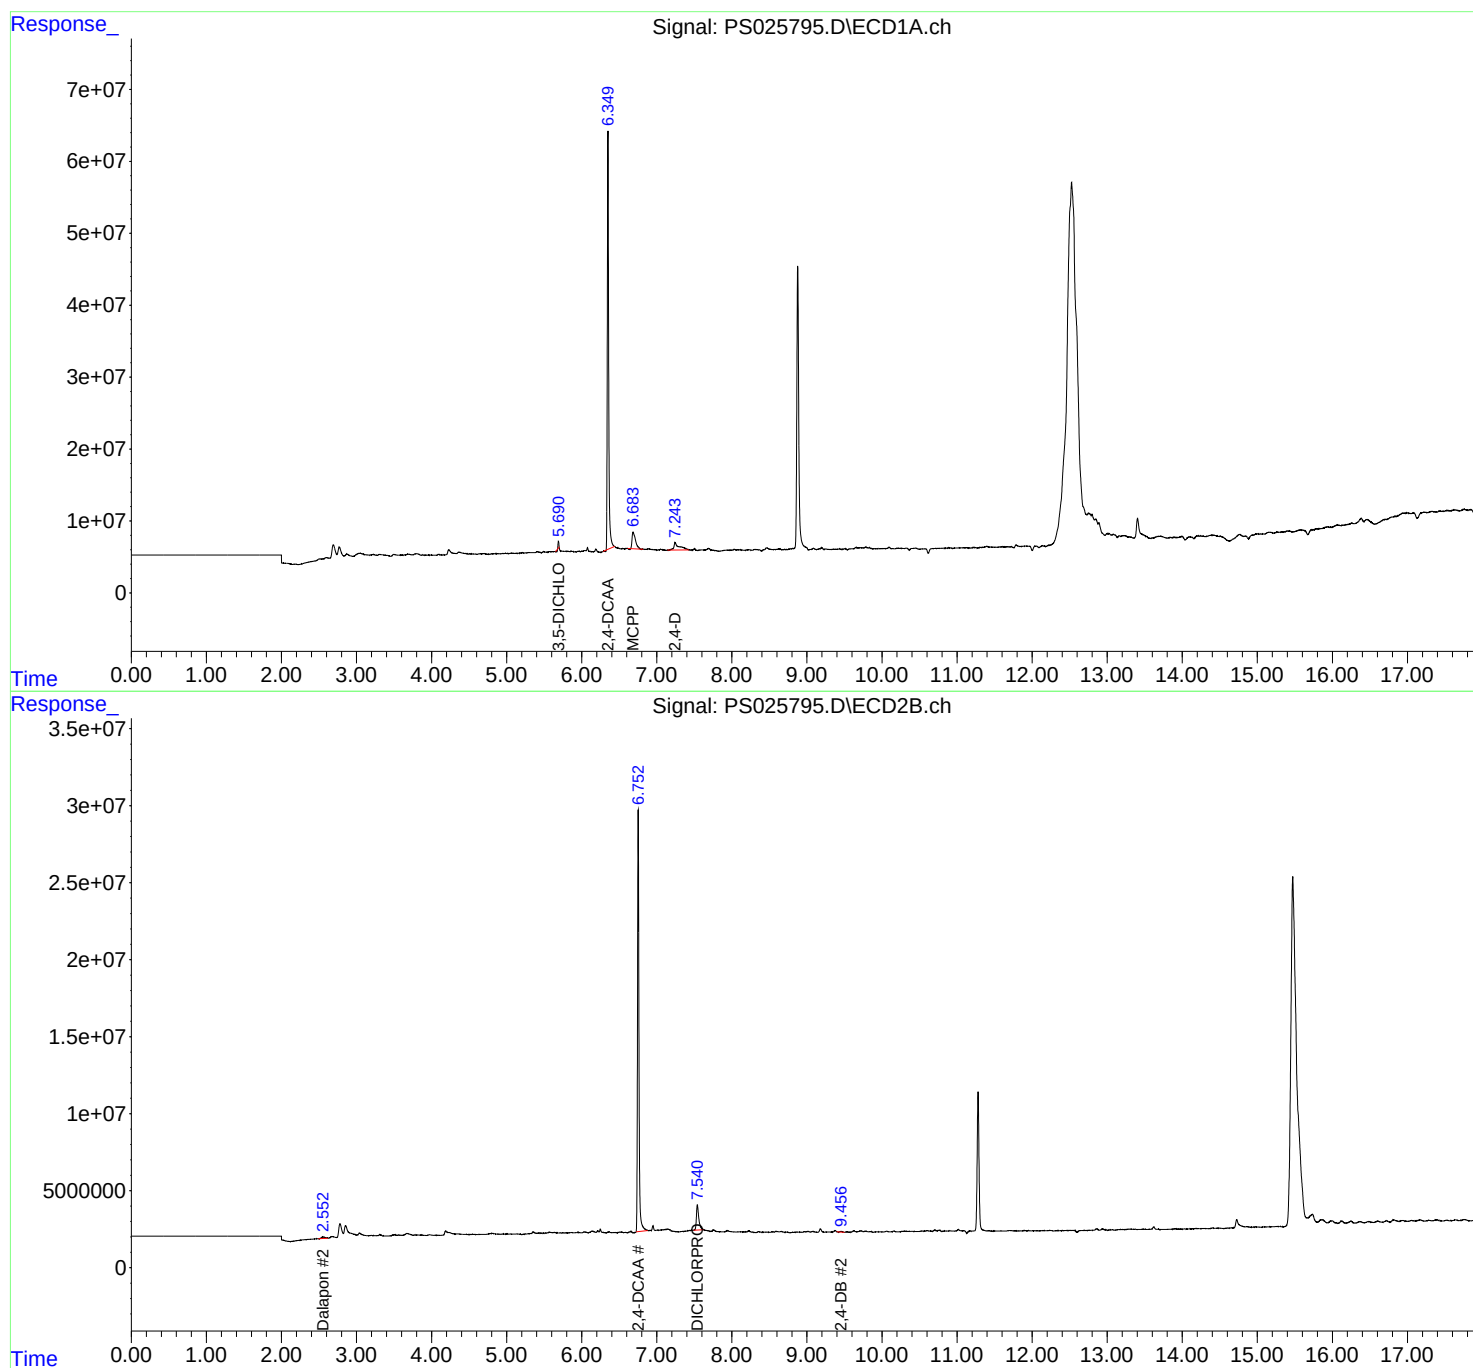


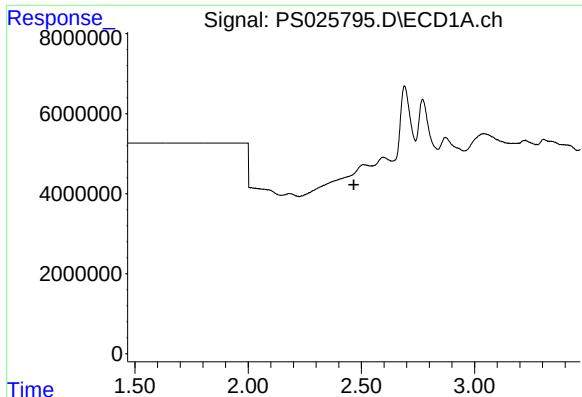

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

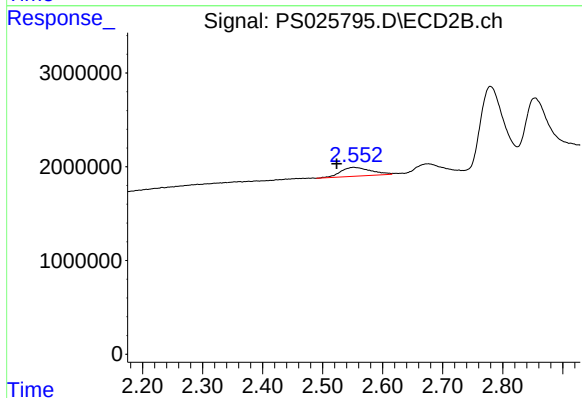


#1 Dalapon

R.T.: 2.552 min
Delta R.T.: 0.029 min
Response: 3272904
Conc: 2.95 ng/ml

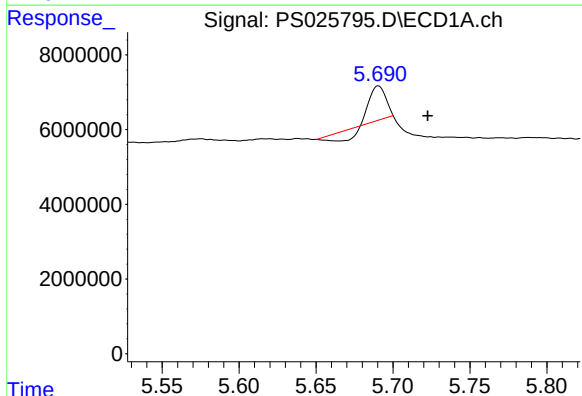


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.032 min
Response: 4570449
Conc: 2.12 ng/ml

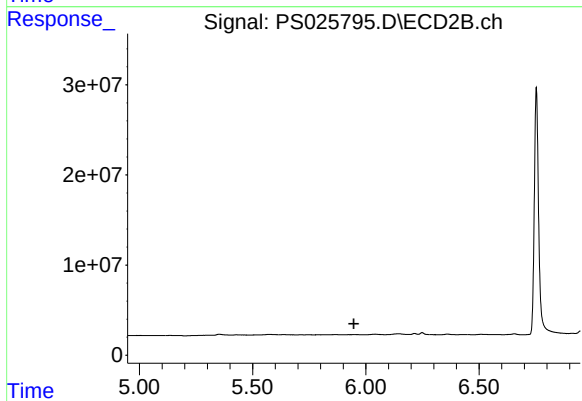

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

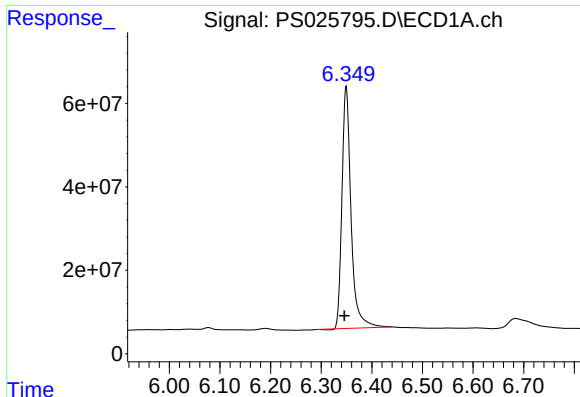

#4 2,4-DCAA


R.T.: 6.349 min
Delta R.T.: 0.003 min
Response: 725005585
Conc: 513.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

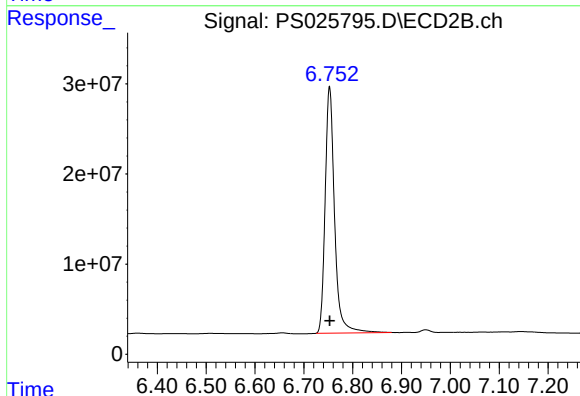


#4 2,4-DCAA

R.T.: 6.753 min
Delta R.T.: 0.000 min
Response: 366255560
Conc: 520.66 ng/ml

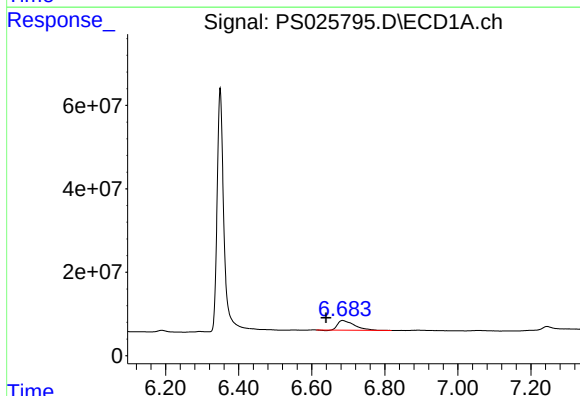


#6 MCP

R.T.: 6.684 min
Delta R.T.: 0.045 min
Response: 72831553
Conc: 20.02 ug/ml

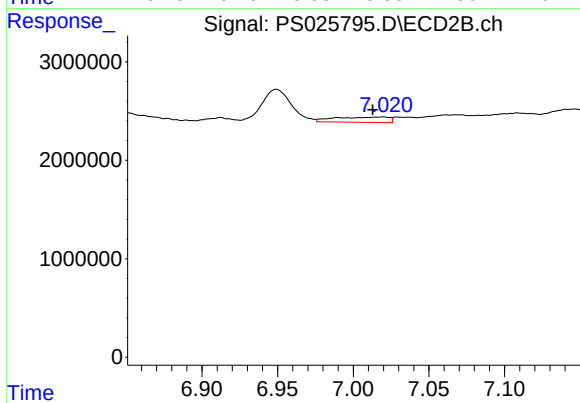

#6 MCP


R.T.: 7.020 min
Delta R.T.: 0.007 min
Response: 1356271
Conc: N.D.

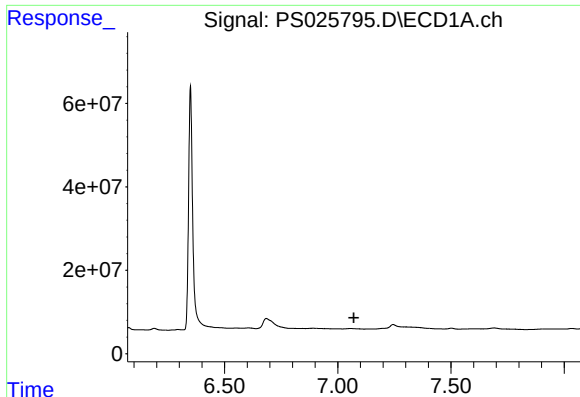

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

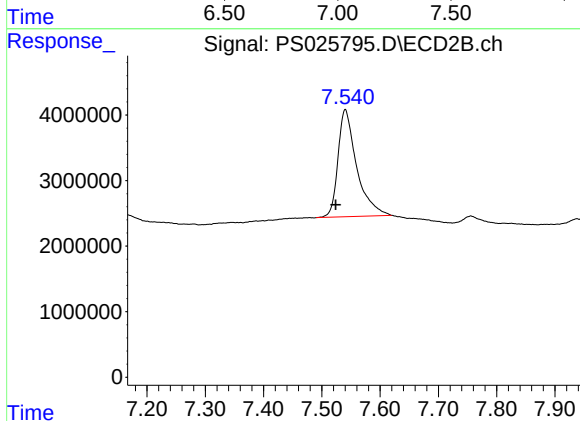


#8 DICHLORPROP

R.T.: 7.540 min
Delta R.T.: 0.016 min
Response: 36484866
Conc: 45.69 ng/ml

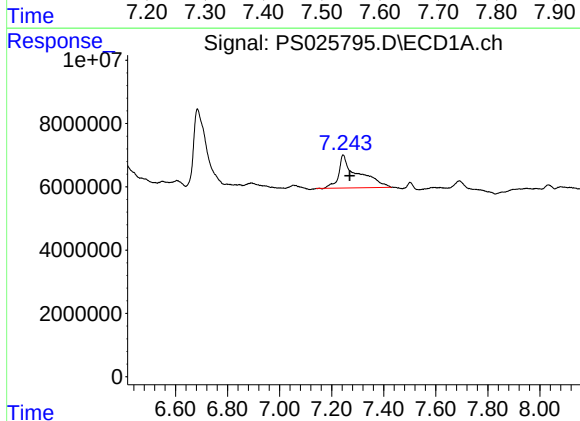


#9 2,4-D

R.T.: 7.244 min
Delta R.T.: -0.025 min
Response: 53615986
Conc: 30.17 ng/ml

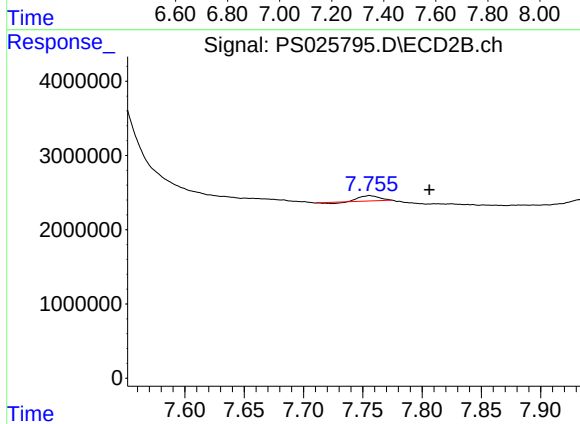

#9 2,4-D


R.T.: 7.756 min
Delta R.T.: -0.050 min
Response: 754125
Conc: N.D.

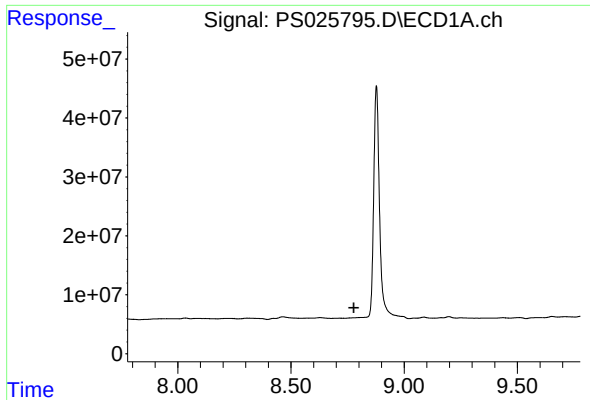

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.778 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

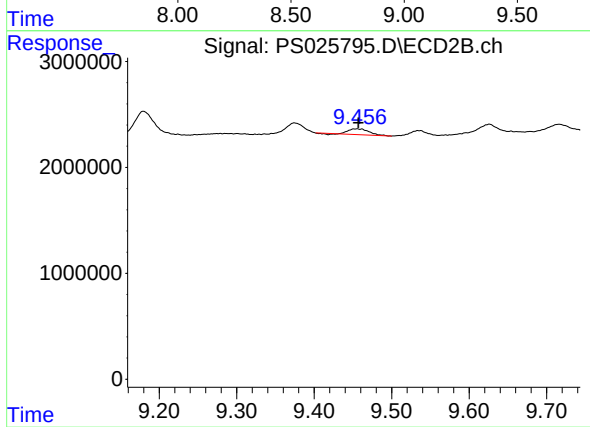

#13 2,4-DB

R.T.: 9.455 min
Delta R.T.: -0.002 min
Response: 954014
Conc: 2.15 ng/ml