

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
 Data File : PS025805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2024 05:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 10:40:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.348	6.755	728.7E6	369.6E6	516.375	525.362
Target Compounds							
1) T	Dalapon	0.000	2.560	0	2879201	N.D.	2.596
2) T	3,5-DICHL...	5.691	0.000	5121497	0	2.376	N.D. #
5) T	DICAMBA	0.000	6.952	0	4610357	N.D.	1.519
6) T	MCP	0.000	6.952f	0	4610357	N.D.	2.254
7) T	MCPA	6.711f	7.229	20584307	938887	3.823	<MDL #
8) T	DICHLORPROP	0.000	7.551	0	9524888	N.D.	11.928
9) T	2,4-D	7.246	0.000	5529882	0	3.112	N.D. #
10) T	Pentachlo...	0.000	8.228	0	1660223	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.594	0	142456	N.D.	<MDL
12) T	2,4,5-T	0.000	8.976	0	227287	N.D.	<MDL
14) T	DINOSEB	0.000	9.788	0	616303	N.D.	<MDL
15) T	Picloram	0.000	10.707	0	1324576	N.D.	<MDL
16) T	DCPA	0.000	10.707	0	1324576	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
Data File : PS025805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2024 05:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 10:40:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

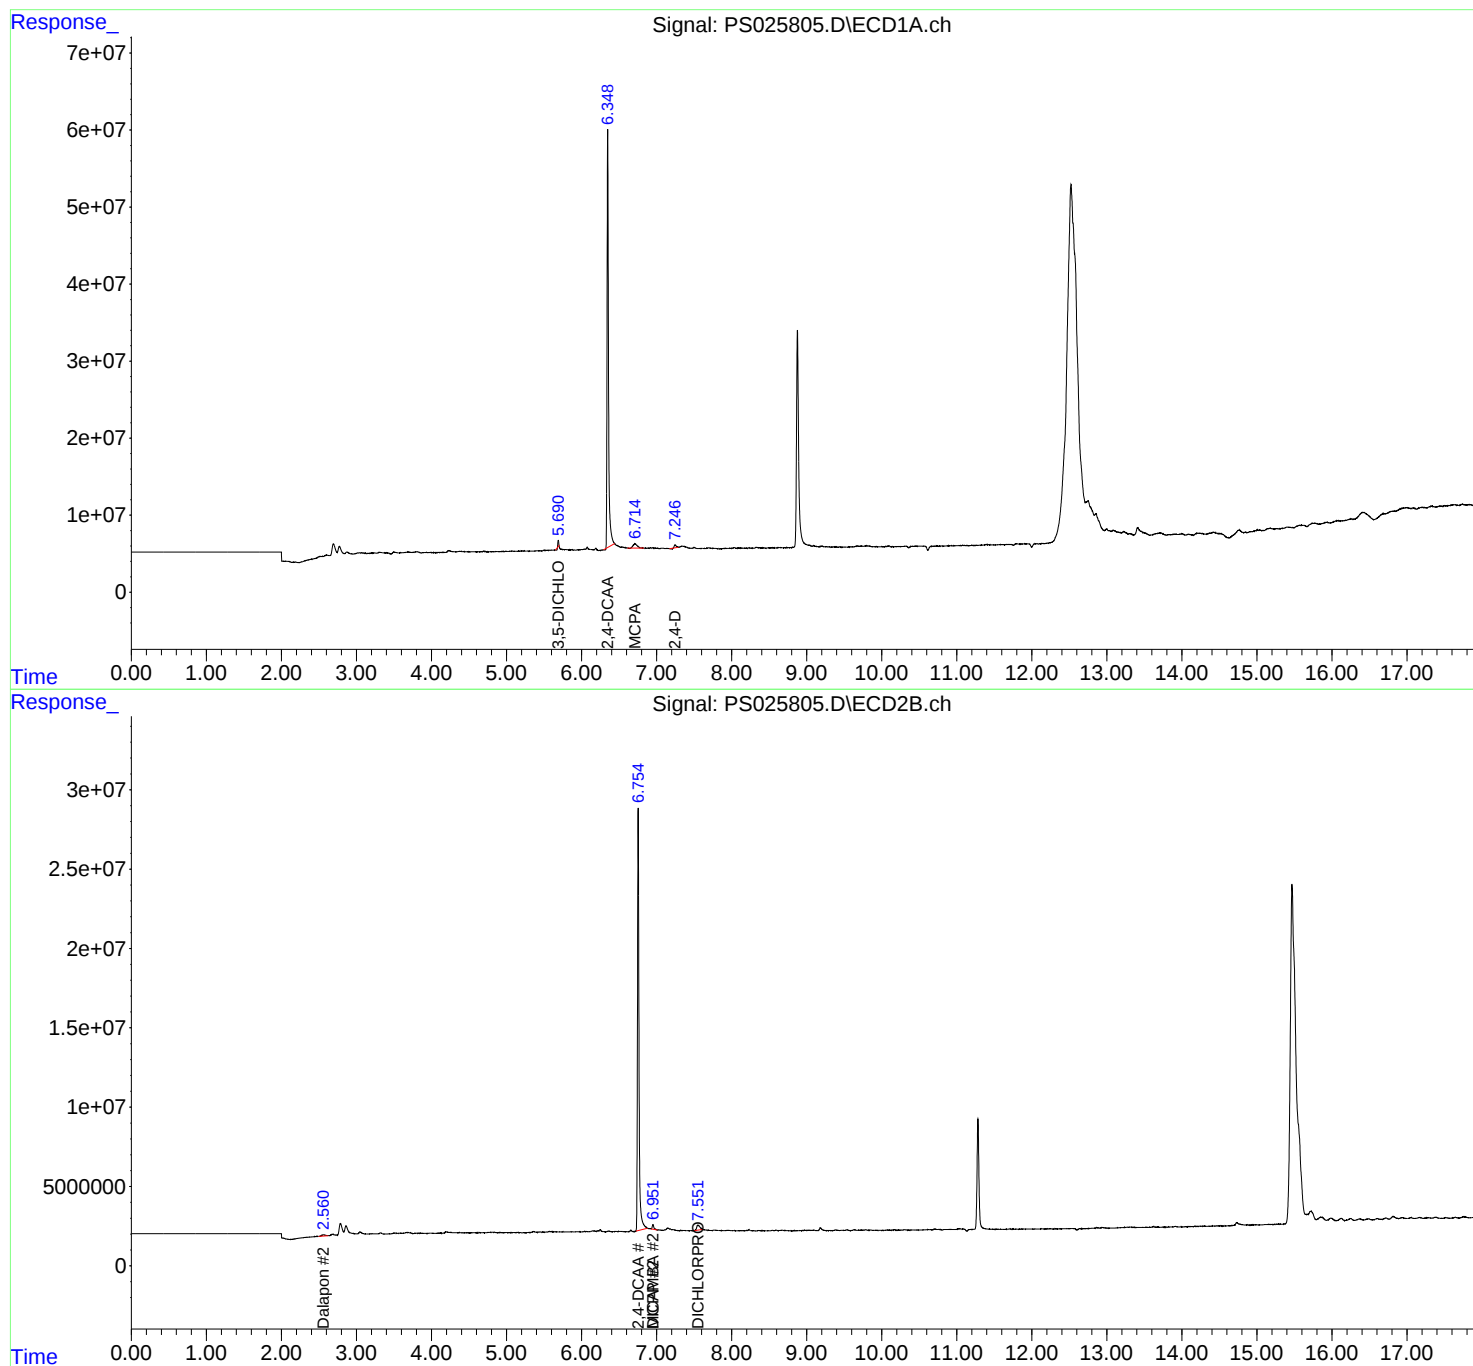


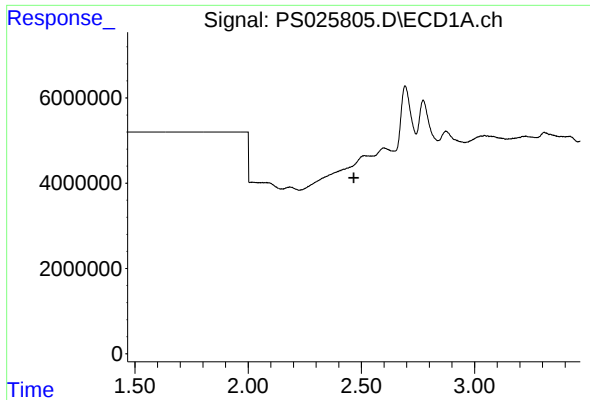

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

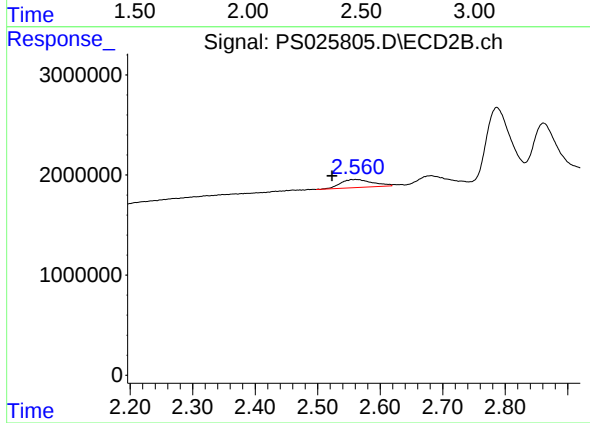


#1 Dalapon

R.T.: 2.560 min
Delta R.T.: 0.037 min
Response: 2879201
Conc: 2.60 ng/ml

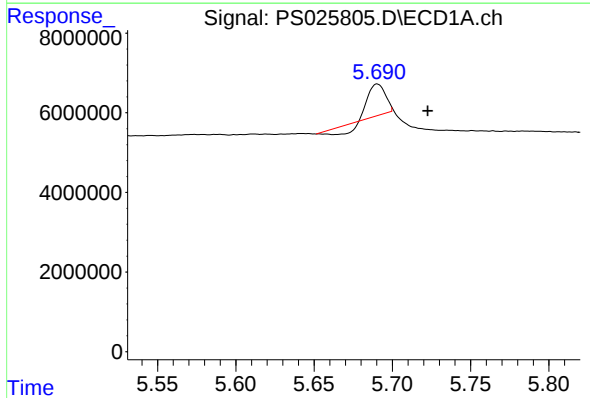


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.032 min
Response: 5121497
Conc: 2.38 ng/ml

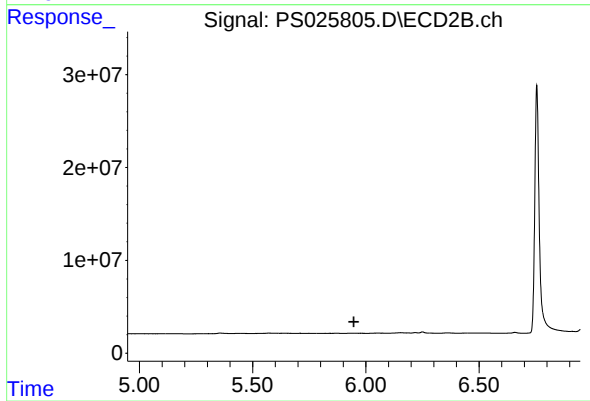

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

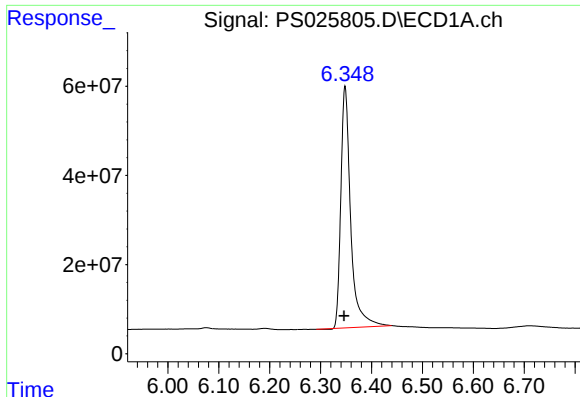

#4 2,4-DCAA


R.T.: 6.348 min
Delta R.T.: 0.002 min
Response: 728735091
Conc: 516.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

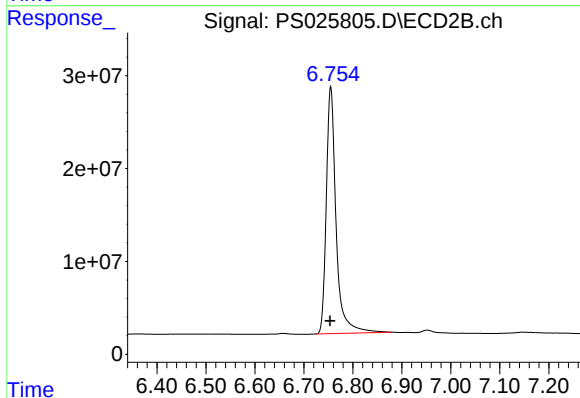


#4 2,4-DCAA

R.T.: 6.755 min
Delta R.T.: 0.001 min
Response: 369562167
Conc: 525.36 ng/ml

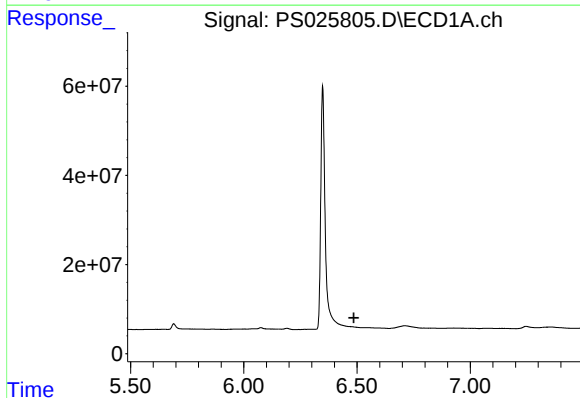


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

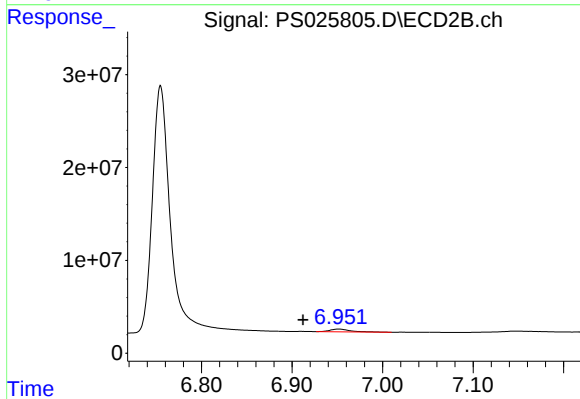

#5 DICAMBA


R.T.: 6.952 min
Delta R.T.: 0.040 min
Response: 4610357
Conc: 1.52 ng/ml

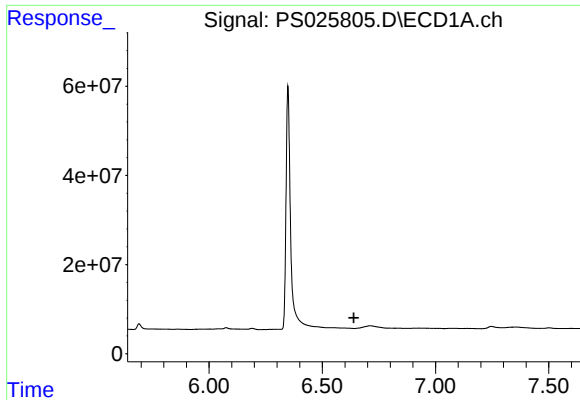

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

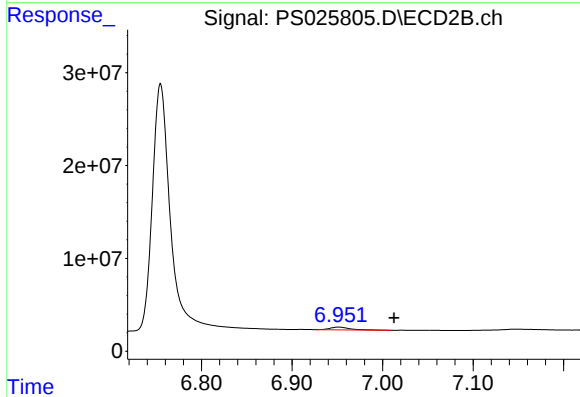


#6 MCPP

R.T.: 6.952 min
Delta R.T.: -0.061 min
Response: 4610357
Conc: 2.25 ug/ml

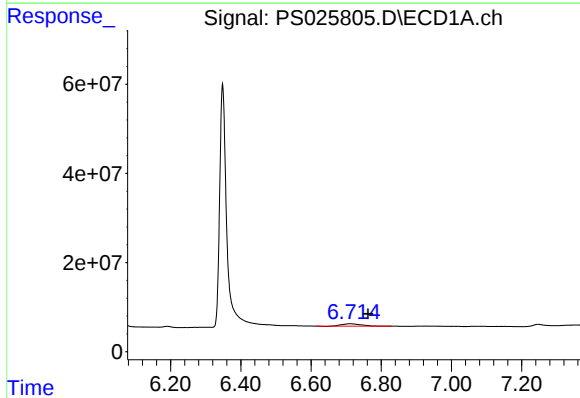


#7 MCPA

R.T.: 6.711 min
Delta R.T.: -0.051 min
Response: 20584307
Conc: 3.82 ug/ml

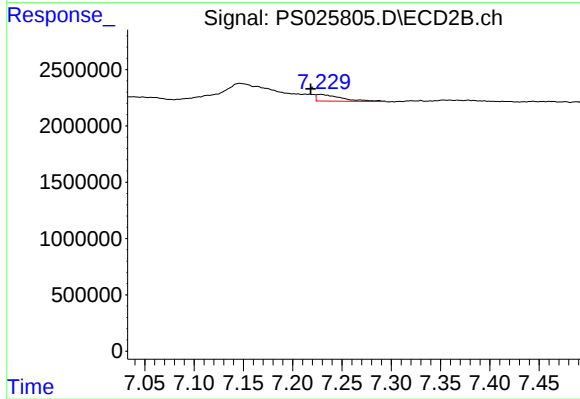

#7 MCPA


R.T.: 7.229 min
Delta R.T.: 0.010 min
Response: 938887
Conc: N.D.

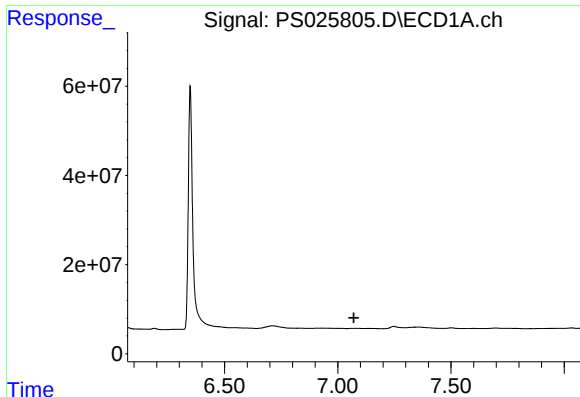

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

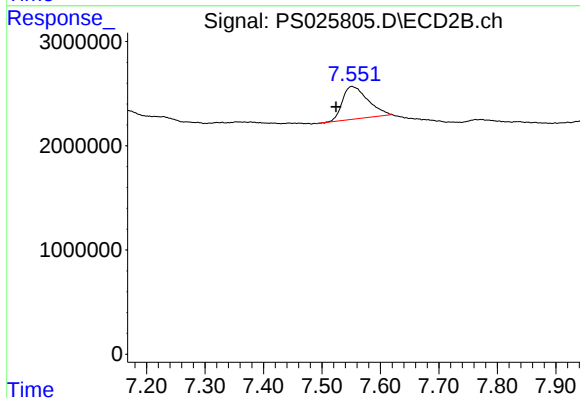


#8 DICHLORPROP

R.T.: 7.551 min
Delta R.T.: 0.027 min
Response: 9524888
Conc: 11.93 ng/ml

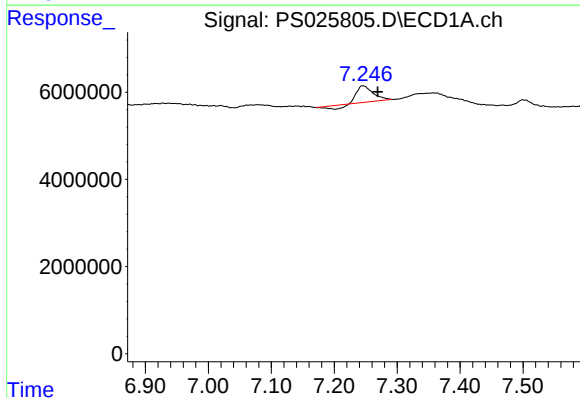

#9 2,4-D

R.T.: 7.246 min
Delta R.T.: -0.023 min
Response: 5529882
Conc: 3.11 ng/ml

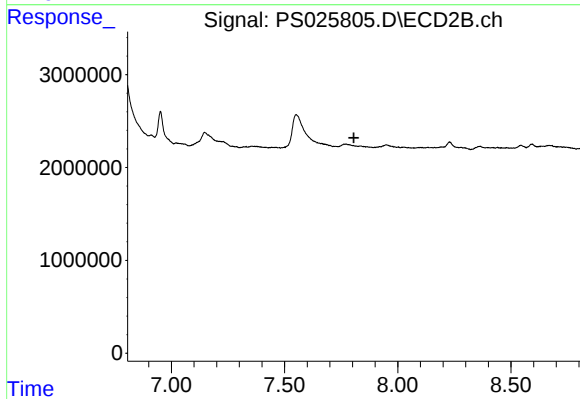

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.806 min
Response: 0
Conc: N.D.