

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
 Data File : PS025815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2024 09:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 10:45:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.348	6.754	729.7E6	370.4E6	517.073	526.602
Target Compounds							
1) T	Dalapon	0.000	2.557	0	1472538	N.D.	1.328
2) T	3,5-DICHL...	5.691	0.000	5254290	0	2.438	N.D. #
5) T	DICAMBA	0.000	6.951	0	6214859	N.D.	2.048
6) T	MCP	0.000	6.951f	0	6214859	N.D.	3.038
7) T	MCPA	6.712f	0.000	28275692	0	5.252	N.D. #
8) T	DICHLORPROP	0.000	7.553	0	12590517	N.D.	15.767
9) T	2,4-D	7.247	7.767	9982430	72807	5.617	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
Data File : PS025815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2024 09:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 10:45:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

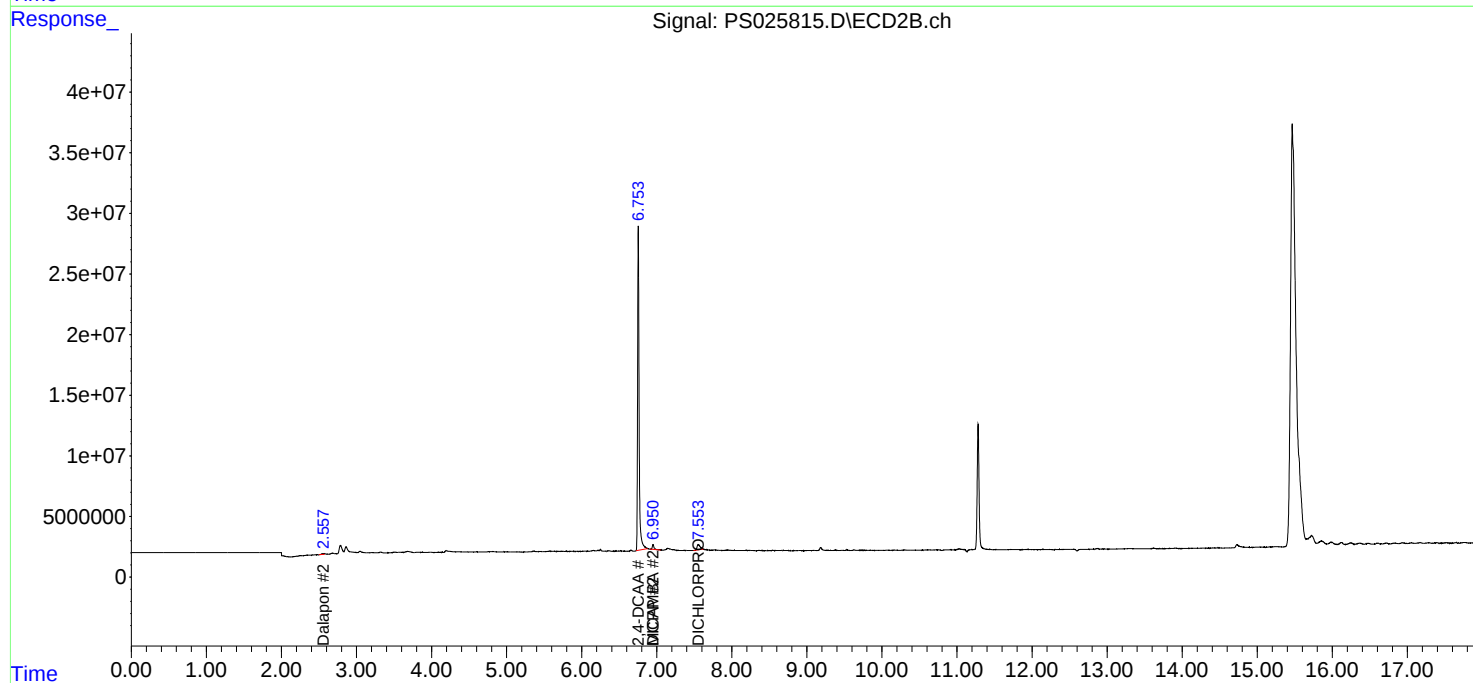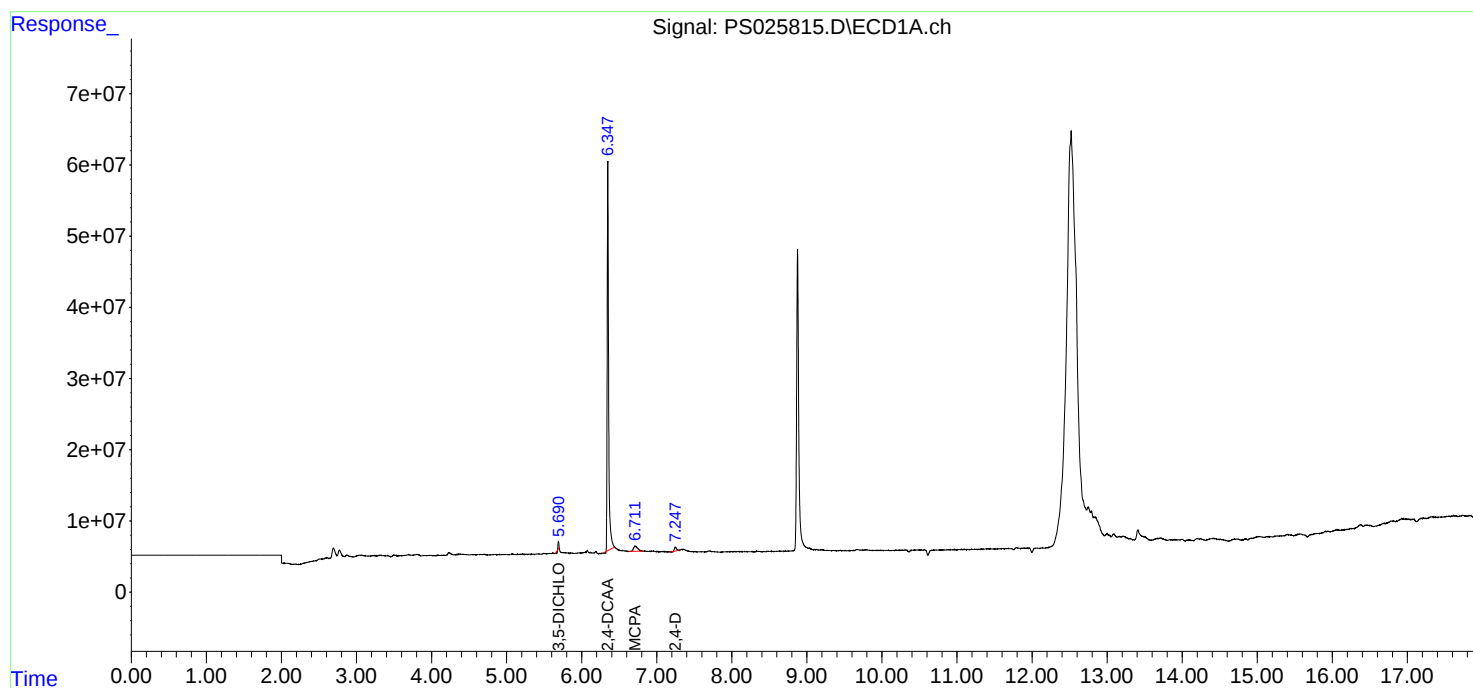


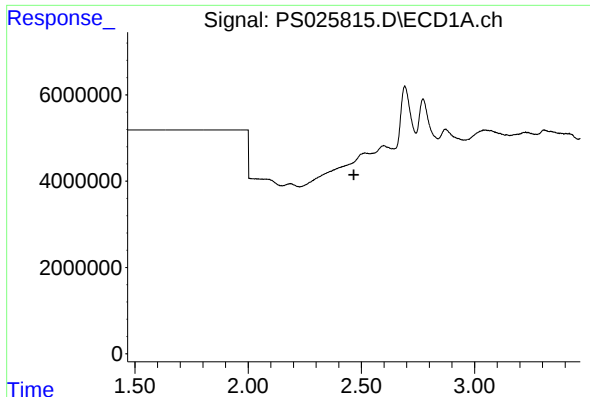

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

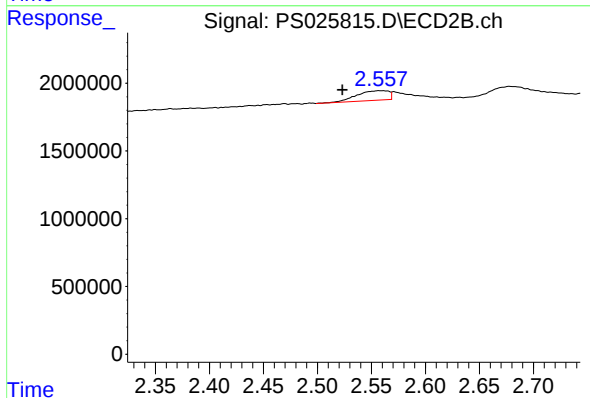


#1 Dalapon

R.T.: 2.557 min
Delta R.T.: 0.034 min
Response: 1472538
Conc: 1.33 ng/ml

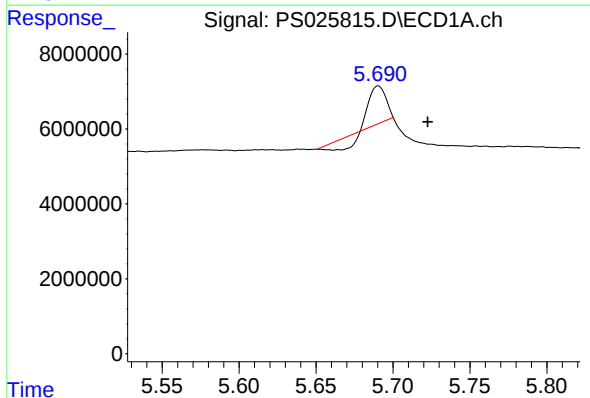


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.032 min
Response: 5254290
Conc: 2.44 ng/ml

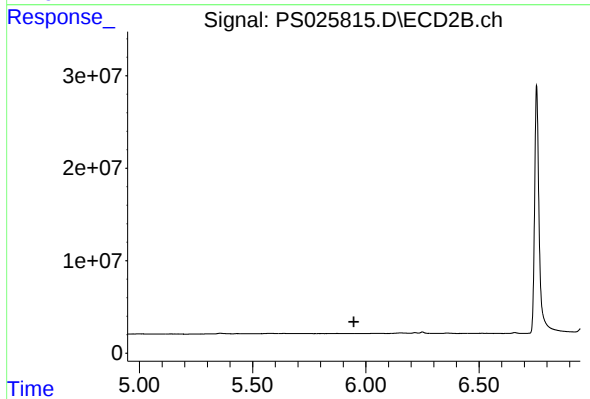

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

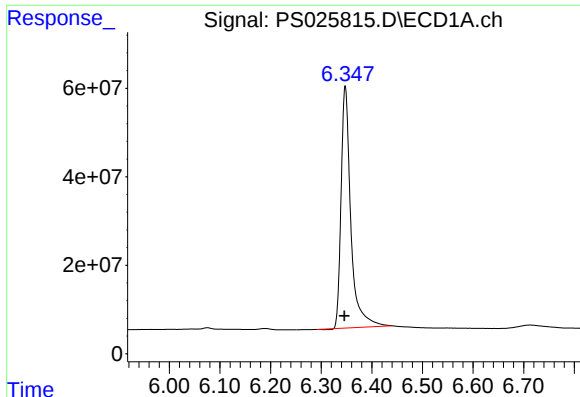

#4 2,4-DCAA


R.T.: 6.348 min
Delta R.T.: 0.002 min
Response: 729720821
Conc: 517.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

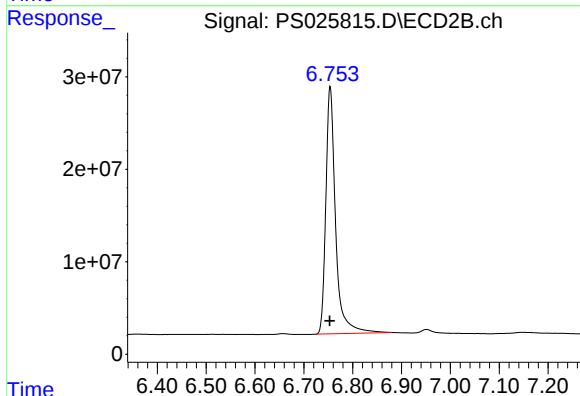


#4 2,4-DCAA

R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 370434546
Conc: 526.60 ng/ml

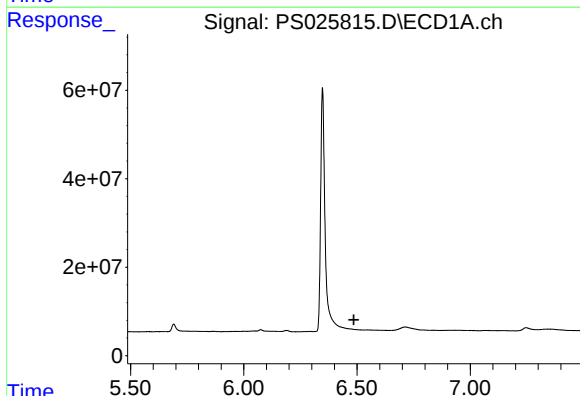


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

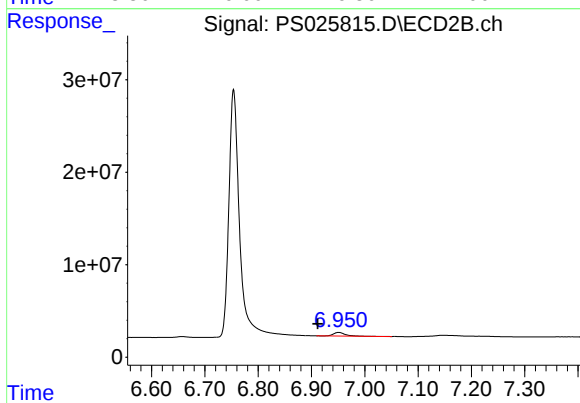

#5 DICAMBA


R.T.: 6.951 min
Delta R.T.: 0.039 min
Response: 6214859
Conc: 2.05 ng/ml

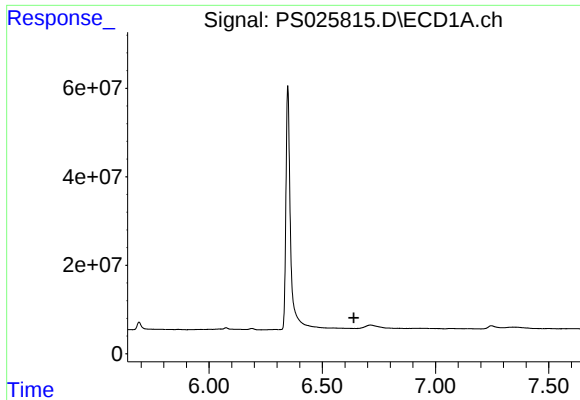

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

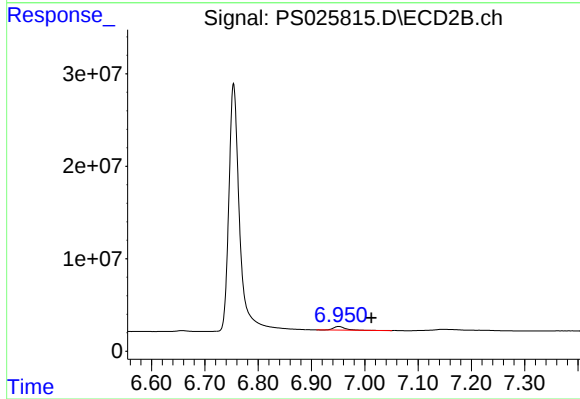


#6 MCPP

R.T.: 6.951 min
Delta R.T.: -0.062 min
Response: 6214859
Conc: 3.04 ug/ml

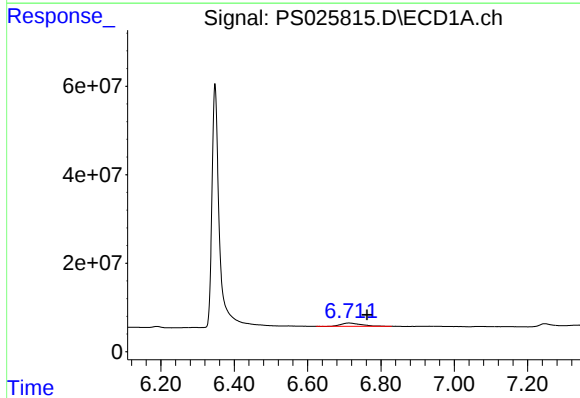


#7 MCPA

R.T.: 6.712 min
Delta R.T.: -0.050 min
Response: 28275692
Conc: 5.25 ug/ml

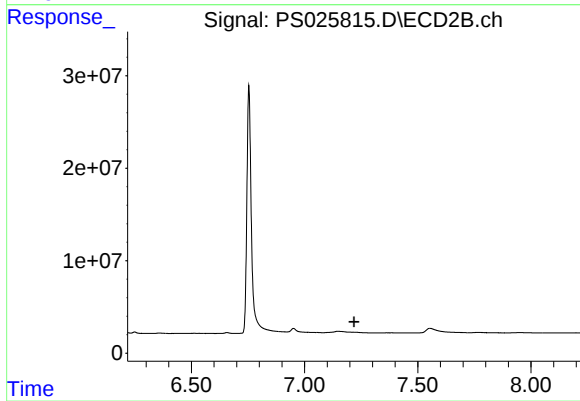

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.218 min
Response: 0
Conc: N.D.

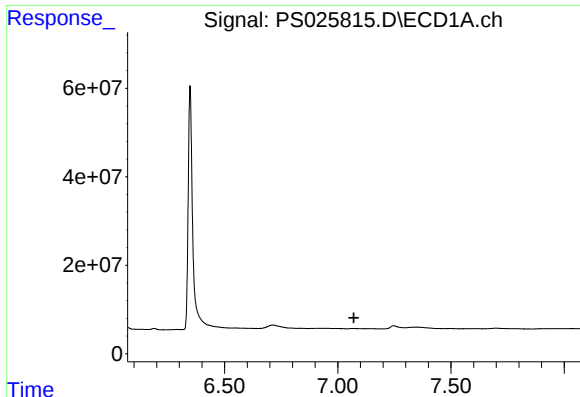

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

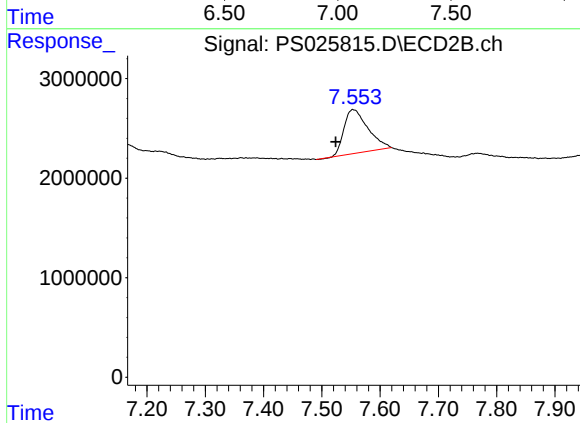


#8 DICHLORPROP

R.T.: 7.553 min
Delta R.T.: 0.029 min
Response: 12590517
Conc: 15.77 ng/ml

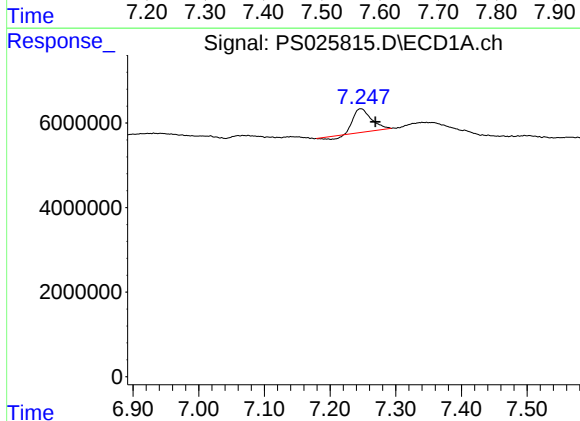

#9 2,4-D

R.T.: 7.247 min
Delta R.T.: -0.022 min
Response: 9982430
Conc: 5.62 ng/ml

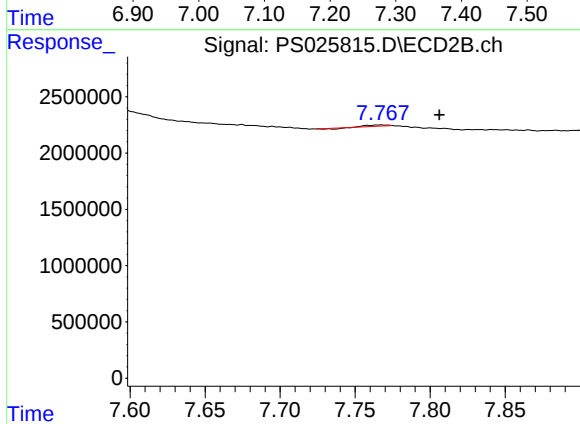

#9 2,4-D

R.T.: 7.767 min
Delta R.T.: -0.040 min
Response: 72807
Conc: N.D.