

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
 Data File : PS025787.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 20:54
 Operator : AR\AJ
 Sample : P1307-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-614-COMP-03

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/07/2024
 Supervised By : Ankita Jodhani 02/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 04:50:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.346	6.753	1074.0E6	402.2E6	761.051m	571.784
Target Compounds							
13) T	2,4-DB	8.790	9.461	355.2E6	152.4E6	306.913	343.970m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
Data File : PS025787.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 20:54
Operator : AR\AJ
Sample : P1307-16
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TR-614-COMP-03


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/07/2024
Supervised By : Ankita Jodhani 02/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 04:50:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

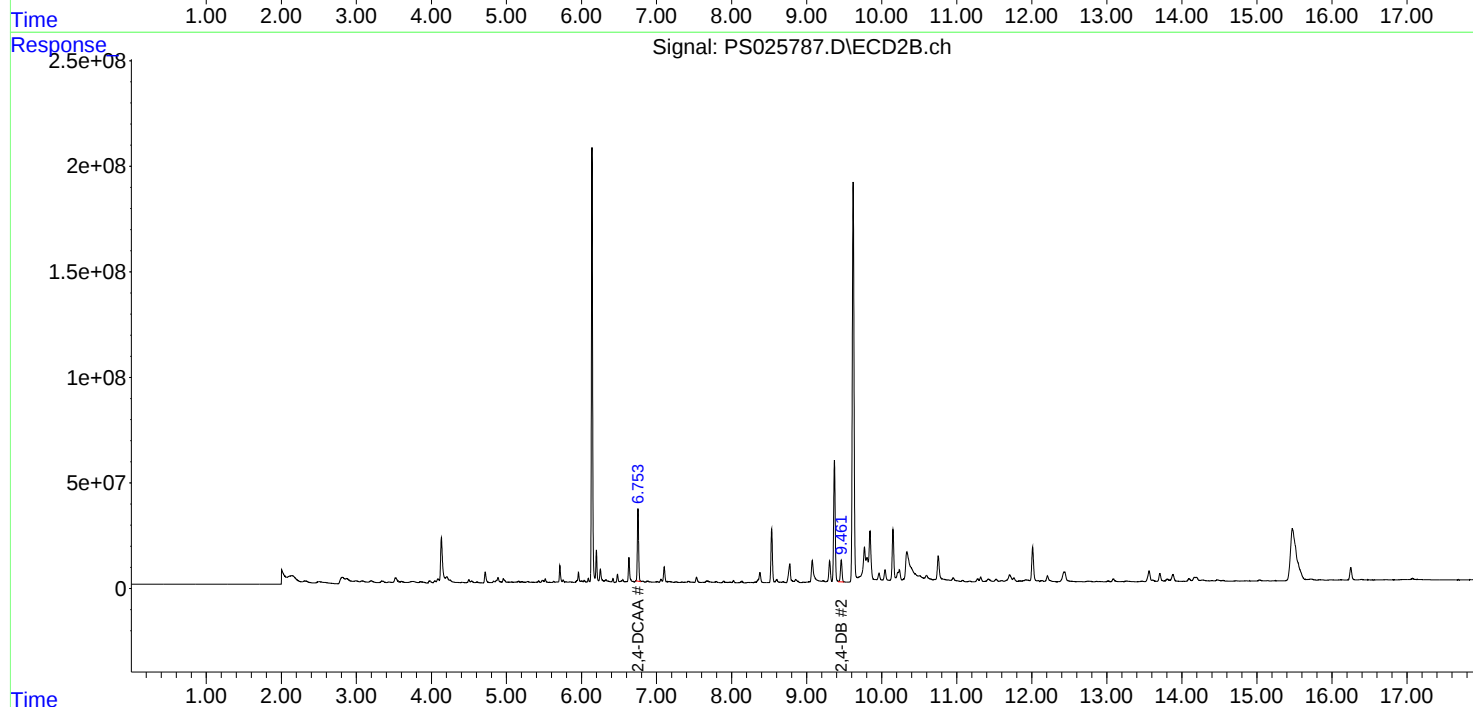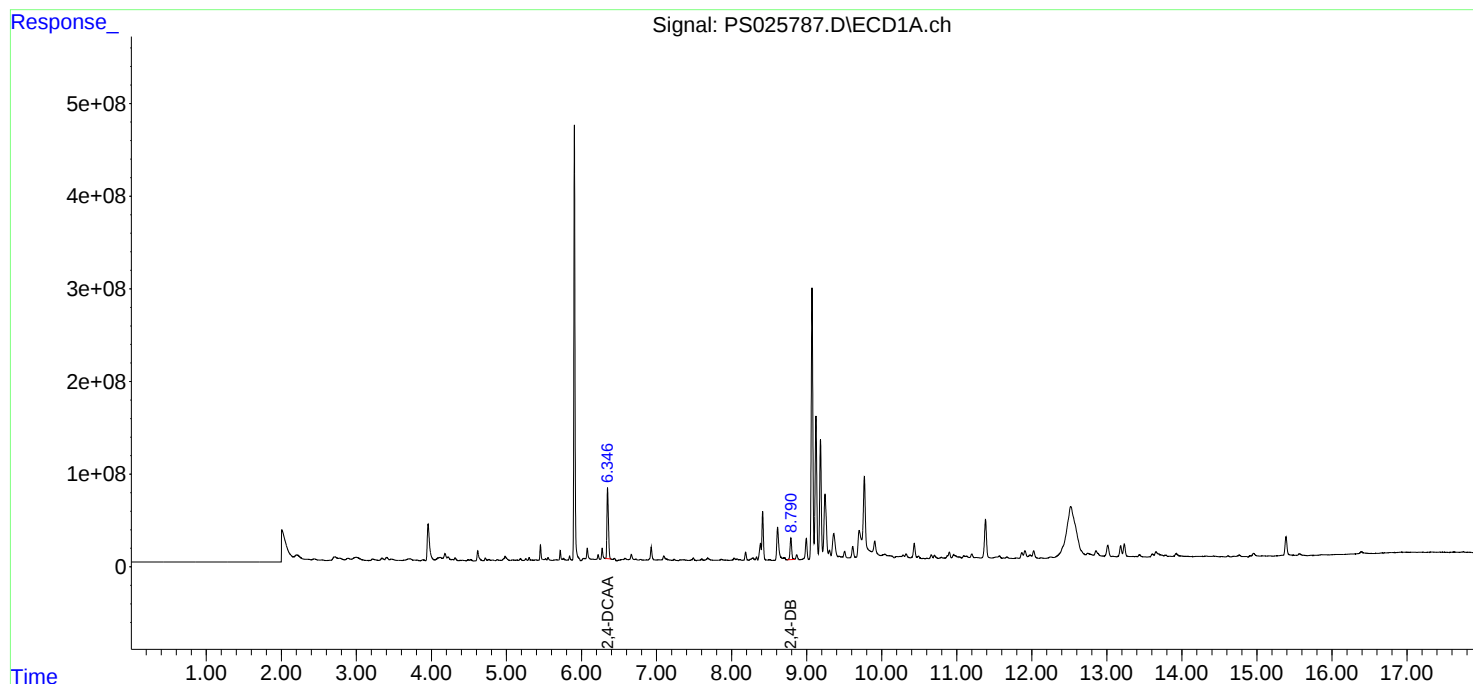

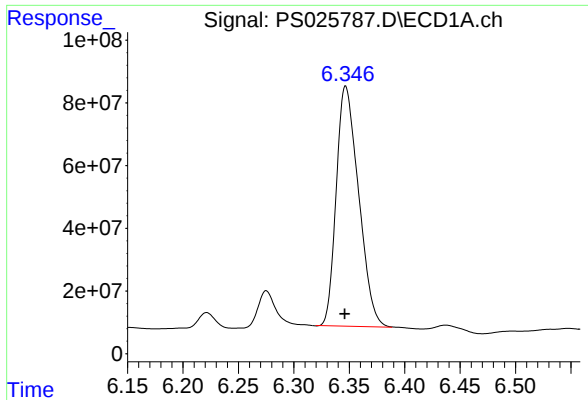


#4 2,4-DCAA

R.T.: 6.346 min
Delta R.T.: 0.000 min
Response: 1074034892
Conc: 761.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-614-COMP-03


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/07/2024
Supervised By :Ankita Jodhani 02/07/2024

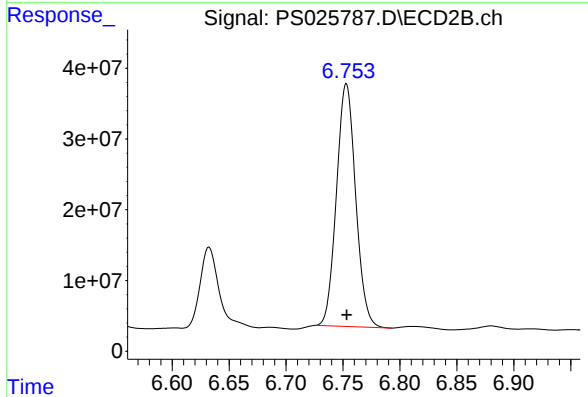


#4 2,4-DCAA

R.T.: 6.753 min
Delta R.T.: 0.000 min
Response: 402217808
Conc: 571.78 ng/ml

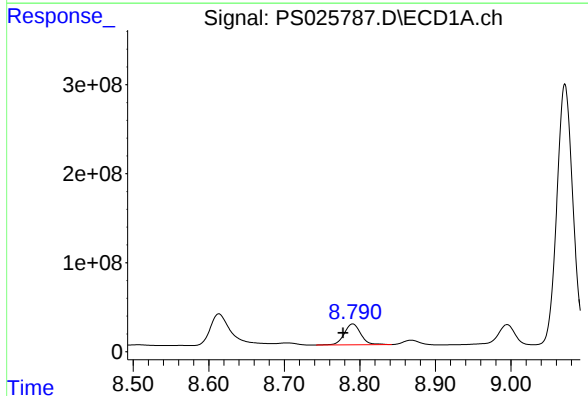

#13 2,4-DB

R.T.: 8.790 min
Delta R.T.: 0.013 min
Response: 355243262
Conc: 306.91 ng/ml

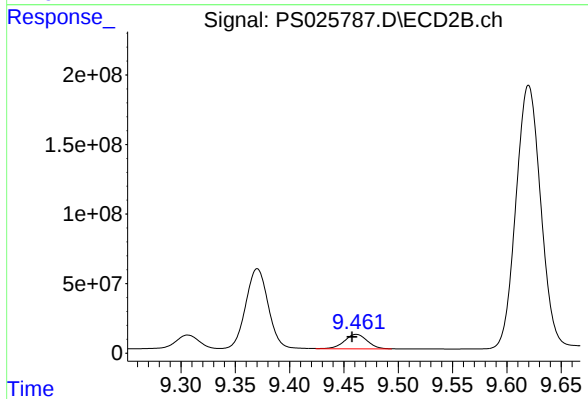

#13 2,4-DB

R.T.: 9.461 min
Delta R.T.: 0.004 min
Response: 152366158
Conc: 343.97 ng/ml m