

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
 Data File : PS025813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2024 09:11
 Operator : AR\AJ
 Sample : PB158779TB
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB158779TB

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/07/2024
 Supervised By : Ankita Jodhani 02/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 10:44:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.347	6.753	1234.1E6	389.0E6	874.470m	553.036 #
Target Compounds							
13) T	2,4-DB	8.790	9.460	431.8E6	107.3E6	373.071	242.287 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020624\
Data File : PS025813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2024 09:11
Operator : AR\AJ
Sample : PB158779TB
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PB158779TB


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/07/2024
Supervised By : Ankita Jodhani 02/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 10:44:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

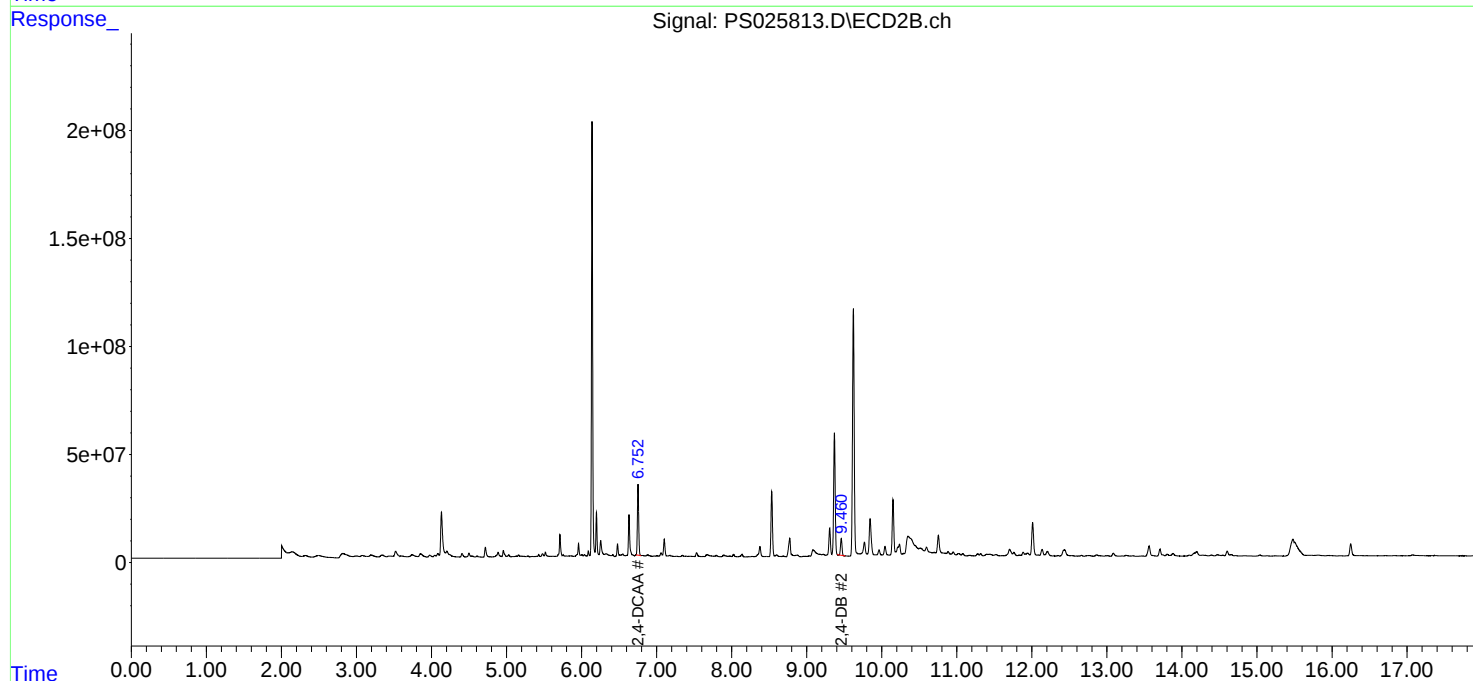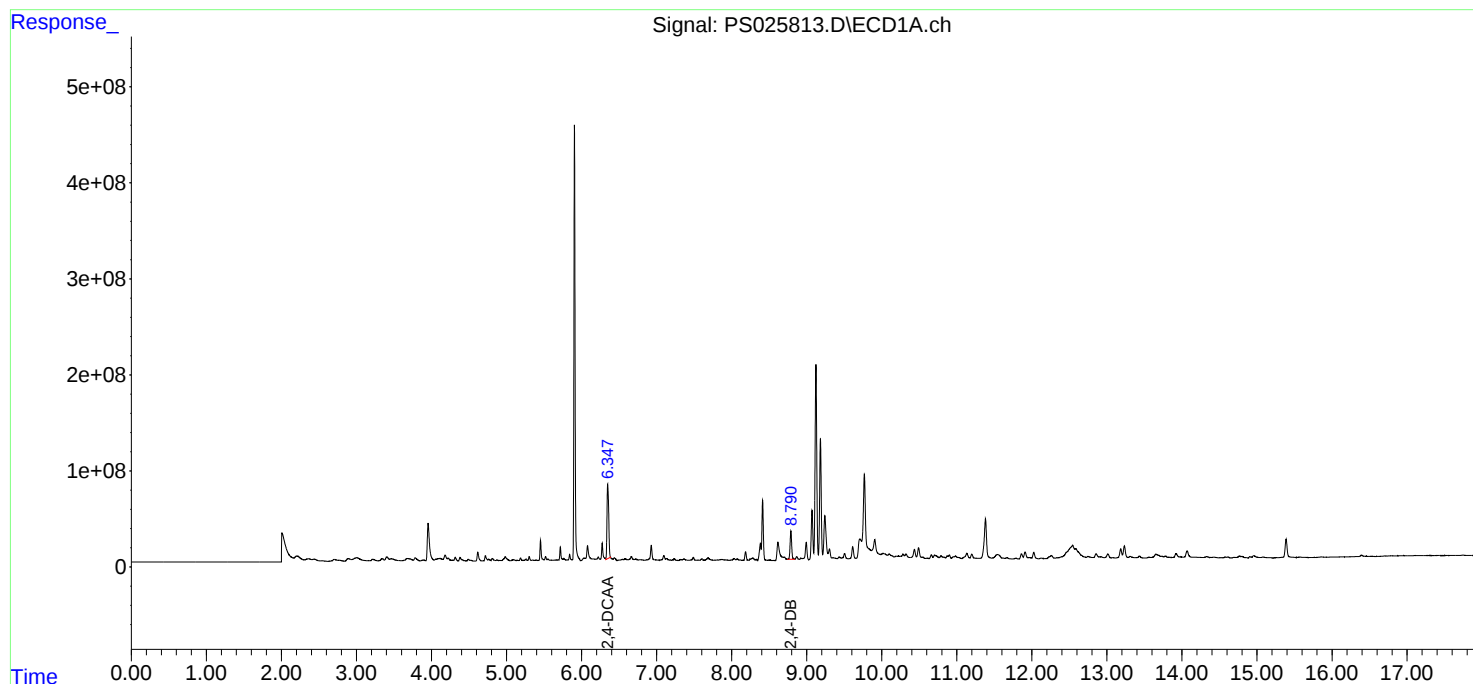

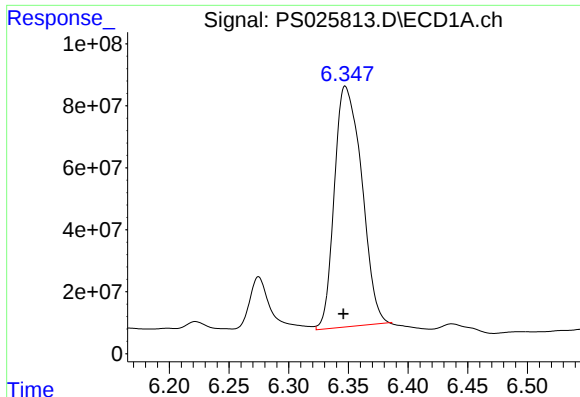

#4 2,4-DCAA

R.T.: 6.347 min
Delta R.T.: 0.000 min
Response: 1234096827
Conc: 874.47 ng/ml

Instrument :

ECD_S


ClientSampleId :

PB158779TB

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 02/07/2024
Supervised By :Ankita Jodhani 02/07/2024

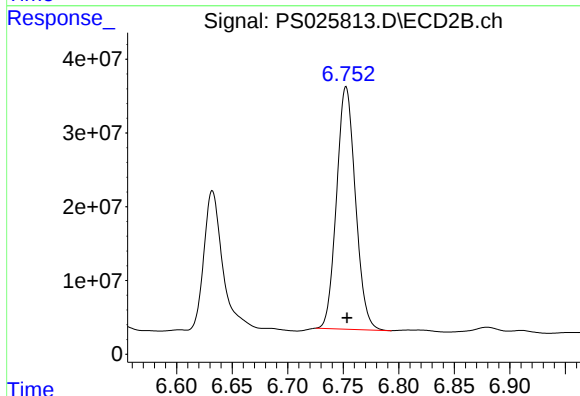


#4 2,4-DCAA

R.T.: 6.753 min
Delta R.T.: 0.000 min
Response: 389029346
Conc: 553.04 ng/ml

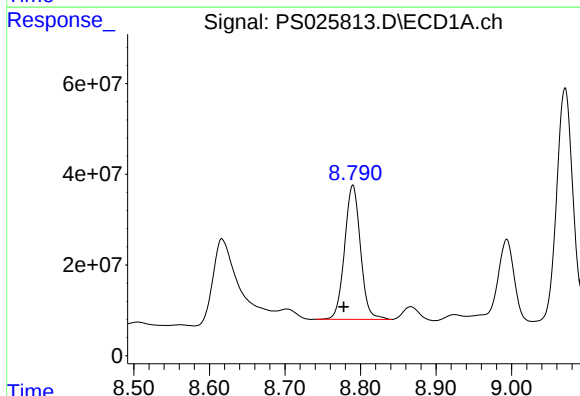

#13 2,4-DB

R.T.: 8.790 min
Delta R.T.: 0.012 min
Response: 431819474
Conc: 373.07 ng/ml

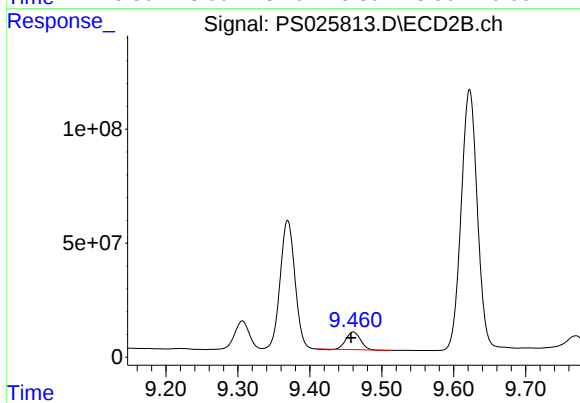

#13 2,4-DB

R.T.: 9.460 min
Delta R.T.: 0.003 min
Response: 107324119
Conc: 242.29 ng/ml