

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
 Data File : PS008750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2020 12:36
 Operator : DD\AJ
 Sample : L1394-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 22:42:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.253	6.947	771.3E6	347.6E6	359.341	375.068
Target Compounds							
1) T	Dalapon	0.000	2.594	0	280.3E6	N.D.	233.740
2) T	3,5-DICHL...	0.000	6.120	0	105.7E6	N.D.	76.852
7) T	MCPA	7.806	7.416	95839819	61185692	11.157	14.660 #
11) T	2,4,5-TP ...	0.000	8.806	0	117.9E6	N.D.	23.007
13) T	2,4-DB	10.117	0.000	193.5E6	0	118.932	N.D. #
15) T	Picloram	0.000	11.039	0	52447585	N.D.	6.948
16) T	DCPA	11.571	11.039	256.8E6	52447585	18.321	8.064 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
Data File : PS008750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2020 12:36
Operator : DD\AJ
Sample : L1394-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 22:42:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

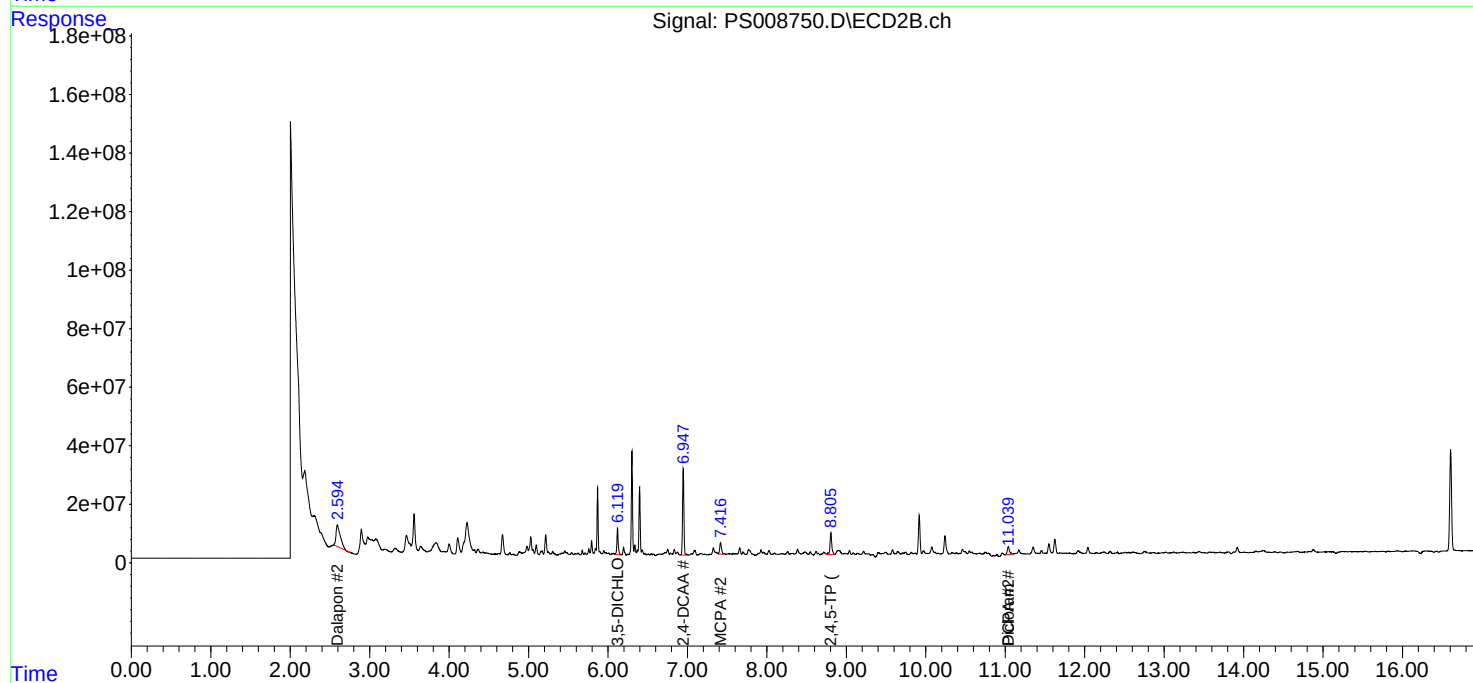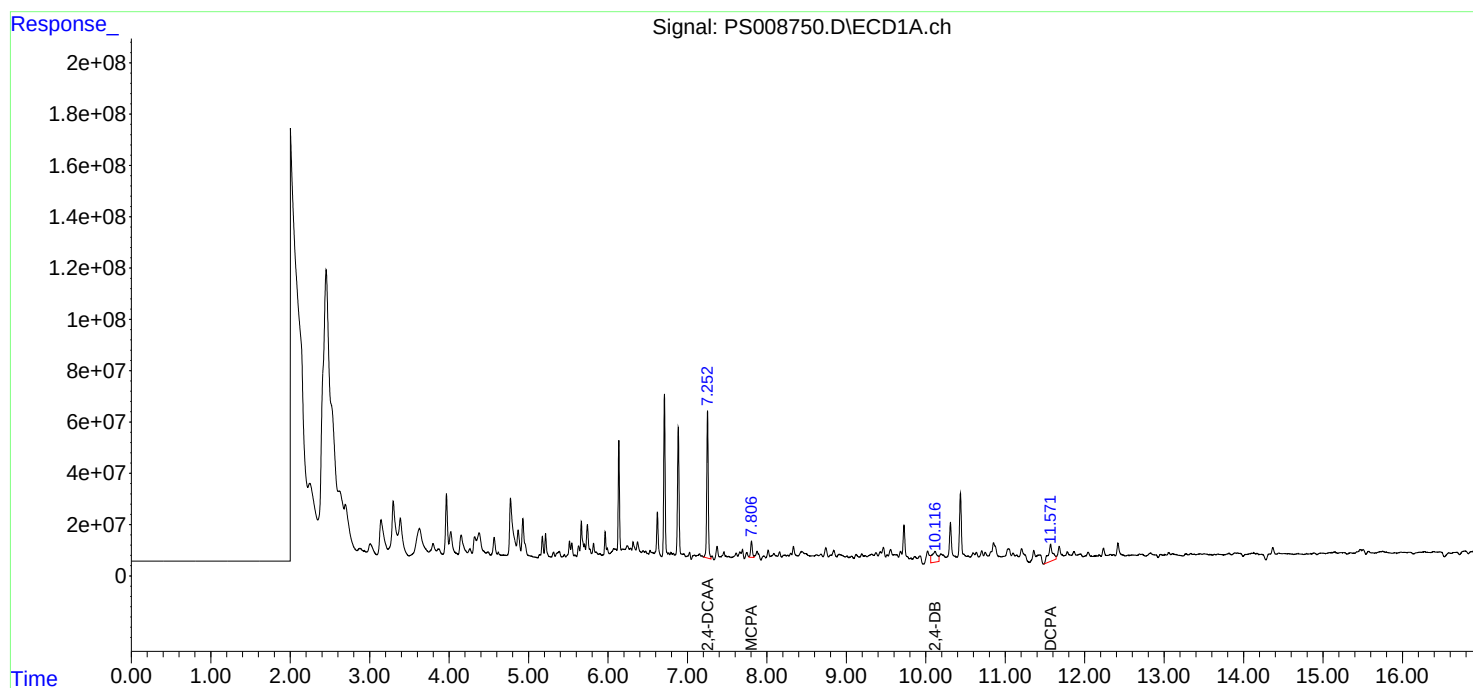


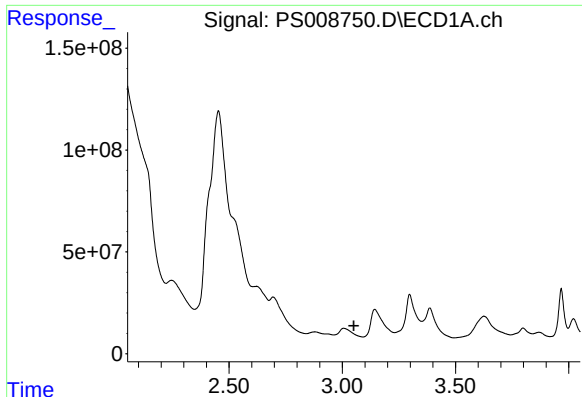

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

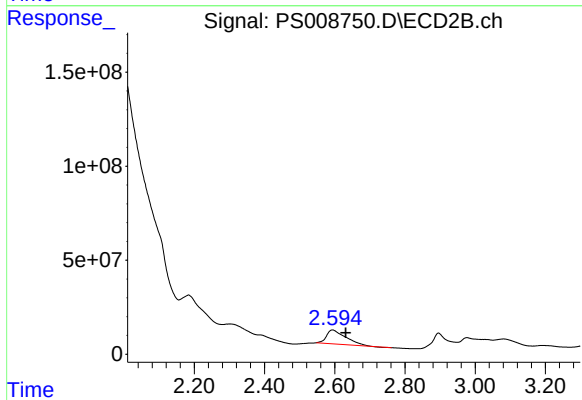


#1 Dalapon

R.T.: 2.594 min
Delta R.T.: -0.038 min
Response: 280328538
Conc: 233.74 ng/ml

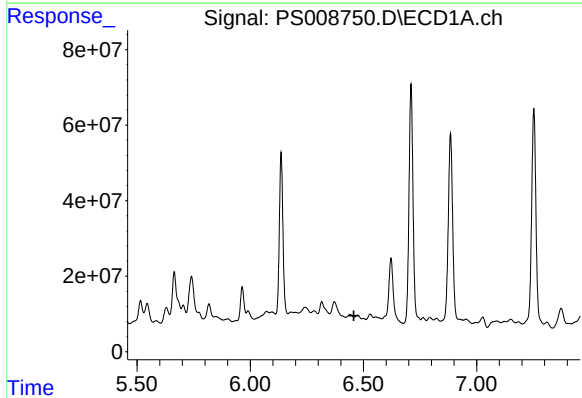


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.458 min
Response: 0
Conc: N.D.

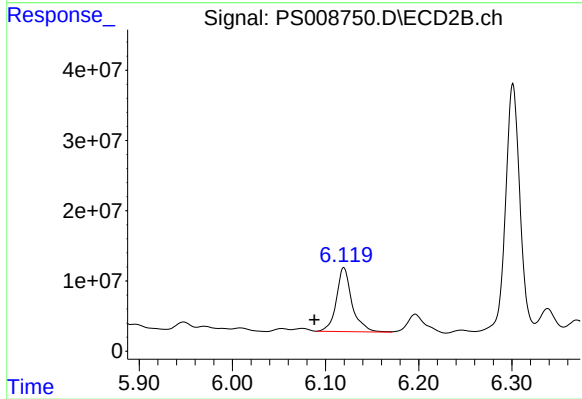

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.120 min
Delta R.T.: 0.032 min
Response: 105739464
Conc: 76.85 ng/ml

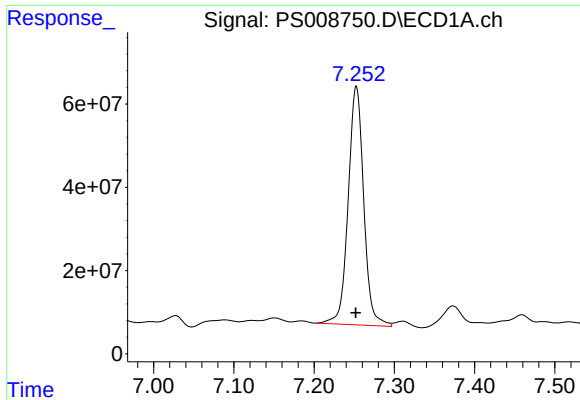

#4 2,4-DCAA


R.T.: 7.253 min
Delta R.T.: 0.000 min
Response: 771256675
Conc: 359.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

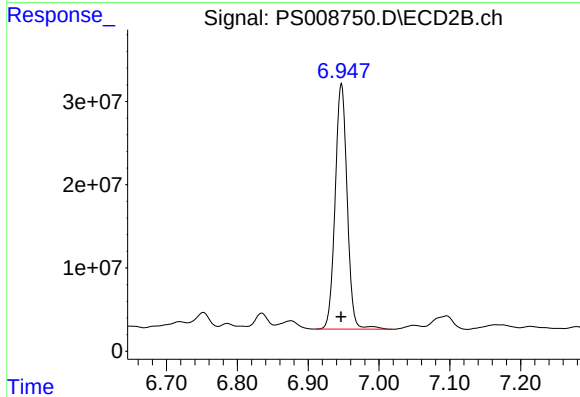


#4 2,4-DCAA

R.T.: 6.947 min
Delta R.T.: 0.000 min
Response: 347622198
Conc: 375.07 ng/ml

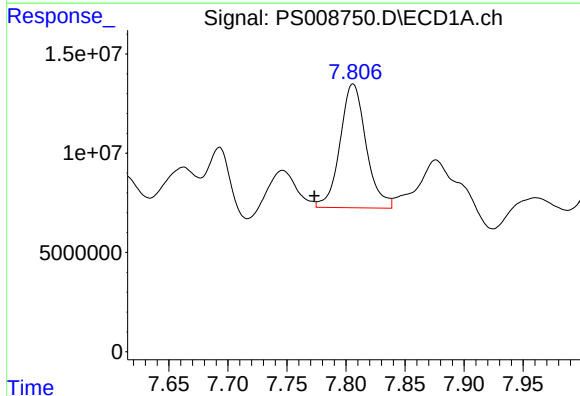


#7 MCPA

R.T.: 7.806 min
Delta R.T.: 0.033 min
Response: 95839819
Conc: 11.16 ug/ml

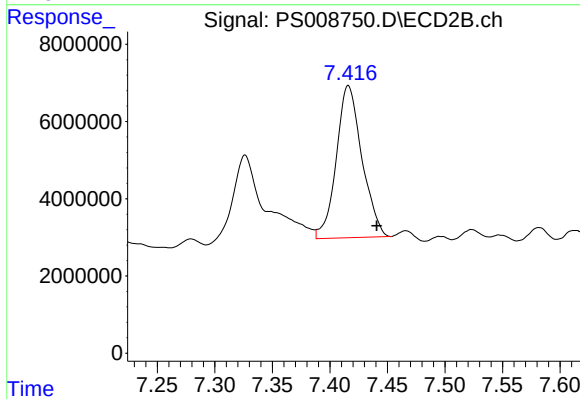

#7 MCPA


R.T.: 7.416 min
Delta R.T.: -0.025 min
Response: 61185692
Conc: 14.66 ug/ml

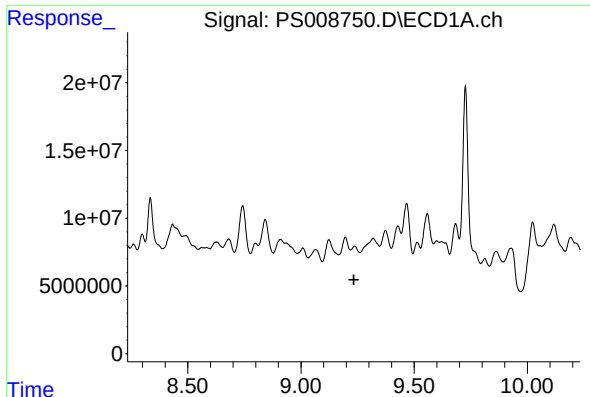

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

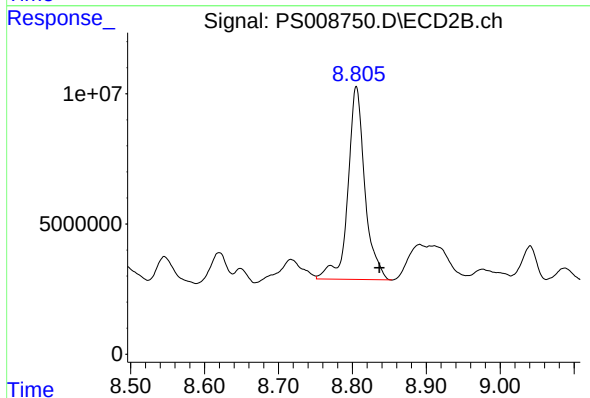


#11 2,4,5-TP (SILVEX)

R.T.: 8.806 min
Delta R.T.: -0.031 min
Response: 117917732
Conc: 23.01 ng/ml

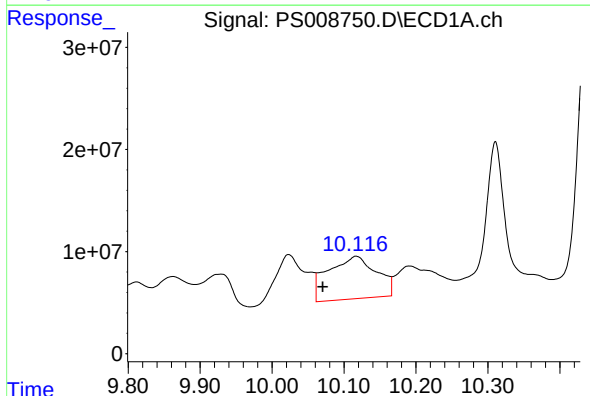


#13 2,4-DB

R.T.: 10.117 min
Delta R.T.: 0.046 min
Response: 193453584
Conc: 118.93 ng/ml

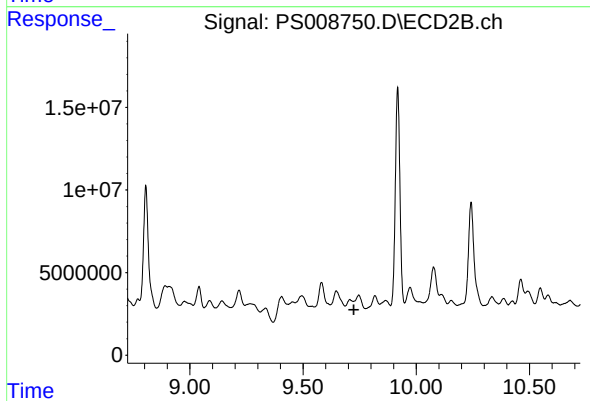

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.724 min
Response: 0
Conc: N.D.

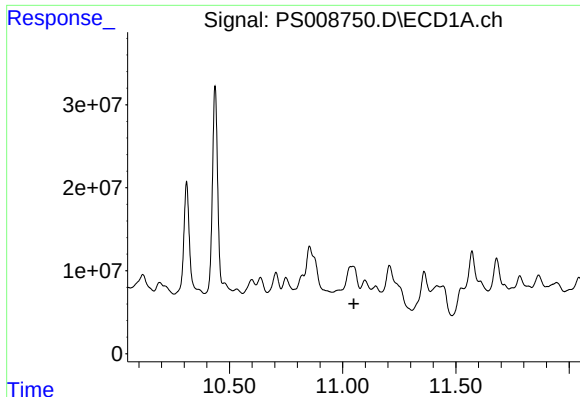

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

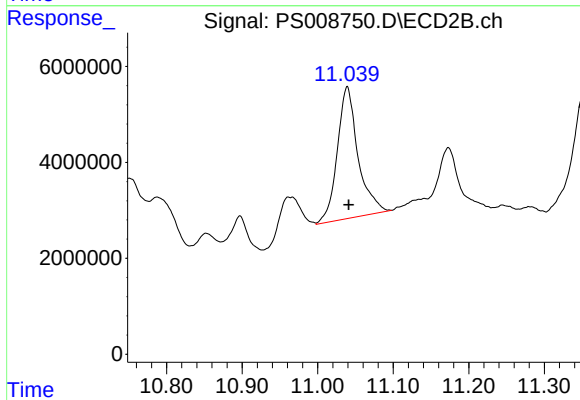


#15 Picloram

R.T.: 11.039 min
Delta R.T.: -0.002 min
Response: 52447585
Conc: 6.95 ng/ml

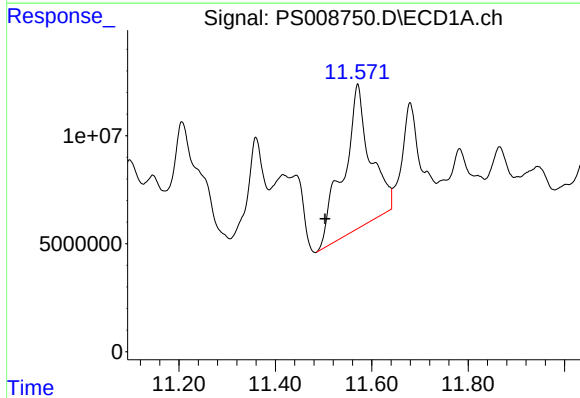

#16 DCPA

R.T.: 11.571 min
Delta R.T.: 0.068 min
Response: 256838619
Conc: 18.32 ng/ml

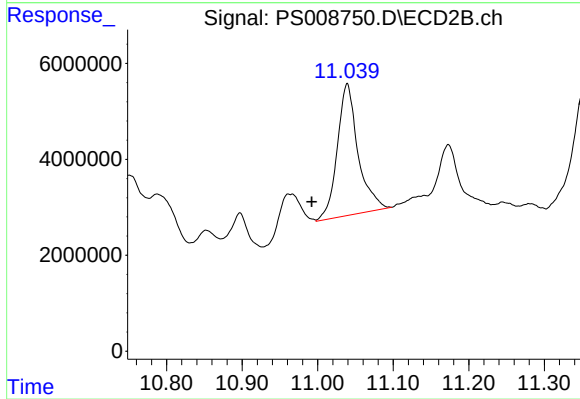

#16 DCPA

R.T.: 11.039 min
Delta R.T.: 0.047 min
Response: 52447585
Conc: 8.06 ng/ml