

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
 Data File : PS008751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2020 12:59
 Operator : DD\AJ
 Sample : L1408-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 22:43:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.252	6.947	675.7E6	253.0E6	314.808	272.985
Target Compounds							
2) T	3,5-DICHL...	0.000	6.119	0	145.7E6	N.D.	105.915
5) T	DICAMBA	7.380	0.000	138.6E6	0	17.185	N.D. #
6) T	MCP	7.690	7.211	123.0E6	44344650	20.013	15.111
7) T	MCPA	7.806	7.438	128.9E6	51040252	15.003	12.229
8) T	DICHLORPROP	8.157	0.000	95337760	0	48.187	N.D. #
10) T	Pentachlo...	8.719	0.000	67974426	0	2.391	N.D. #
11) T	2,4,5-TP ...	0.000	8.806	0	101.8E6	N.D.	19.858
12) T	2,4,5-T	9.465	9.207	123.4E6	54205994	11.214	10.490
13) T	2,4-DB	10.133	9.745	112.4E6	75261780	69.128	107.629 #
14) T	DINOSEB	0.000	10.076	0	125.9E6	N.D.	34.274
16) T	DCPA	11.523	0.000	155.1E6	0	11.066	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
Data File : PS008751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2020 12:59
Operator : DD\AJ
Sample : L1408-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 22:43:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

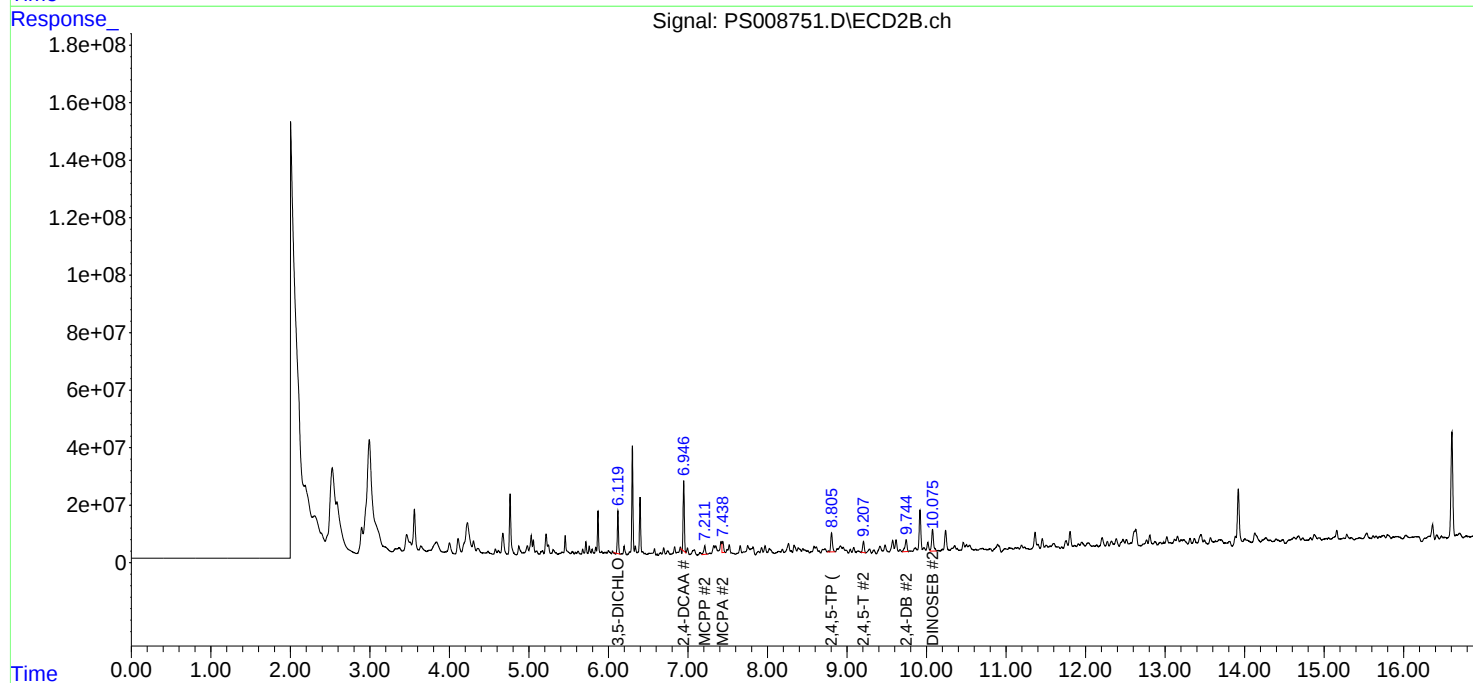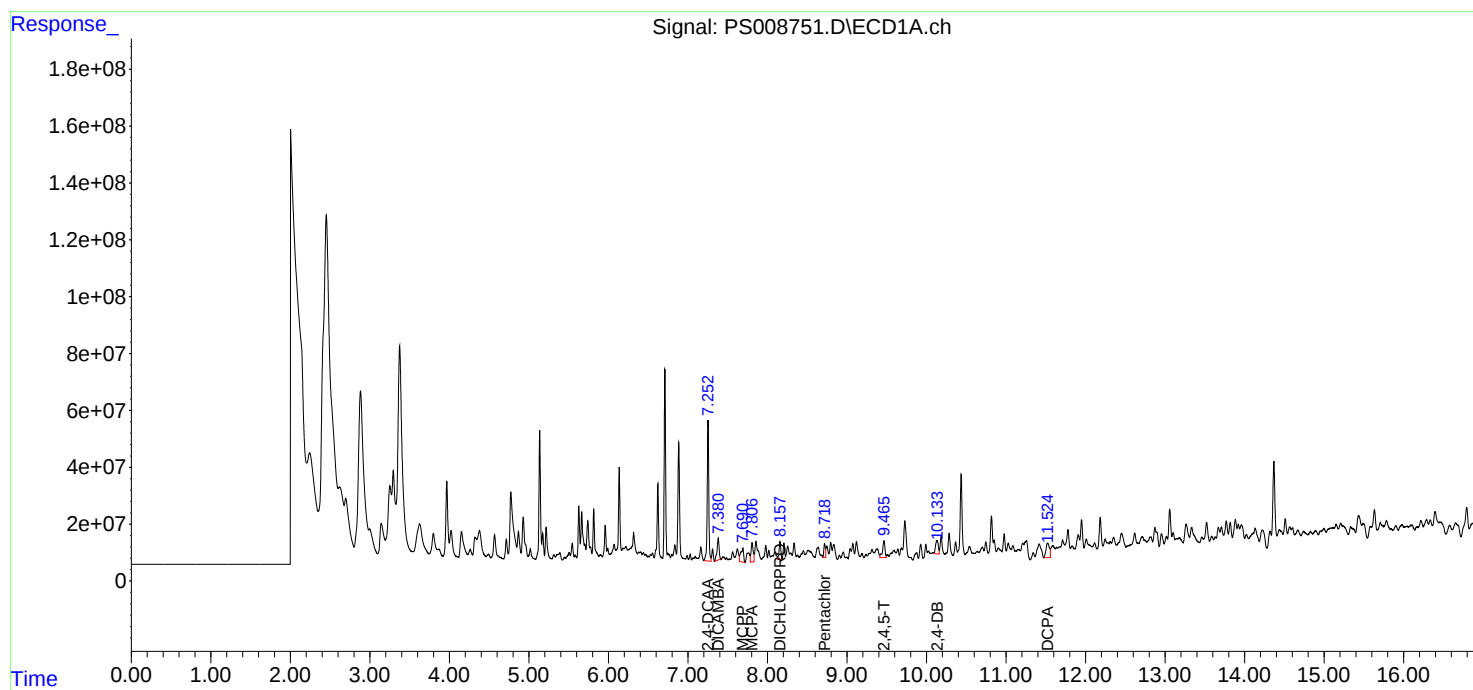


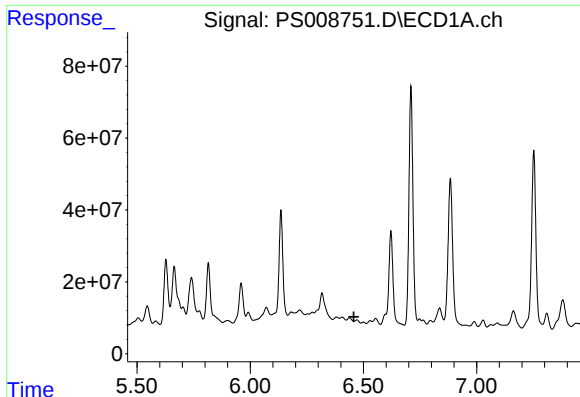

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

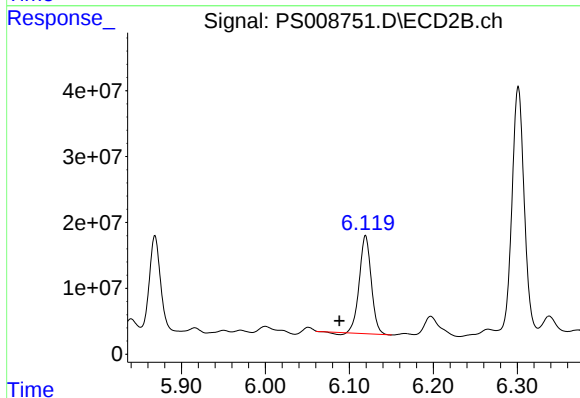


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.119 min
Delta R.T.: 0.031 min
Response: 145727336
Conc: 105.92 ng/ml

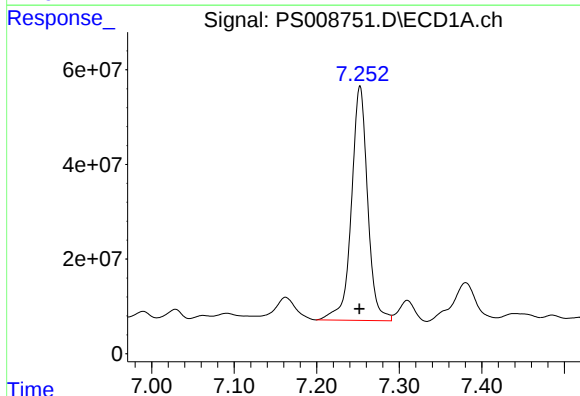


#4 2,4-DCAA

R.T.: 7.252 min
Delta R.T.: 0.000 min
Response: 675674264
Conc: 314.81 ng/ml

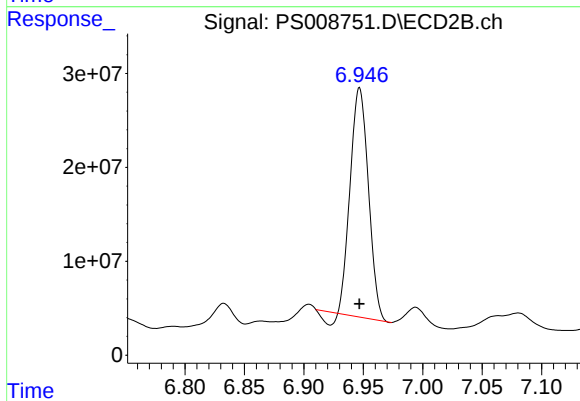

#4 2,4-DCAA


R.T.: 6.947 min
Delta R.T.: 0.000 min
Response: 253009073
Conc: 272.98 ng/ml

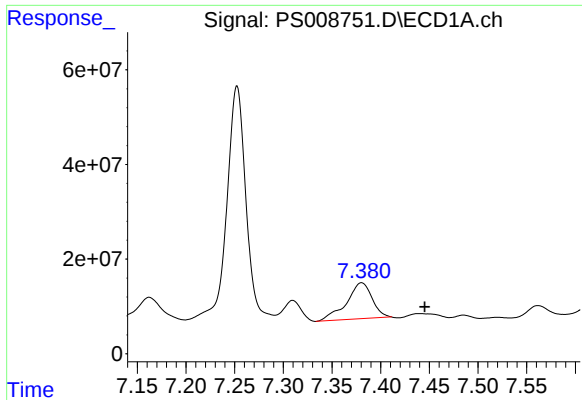

#5 DICAMBA


R.T.: 7.380 min
Delta R.T.: -0.065 min
Response: 138612474
Conc: 17.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

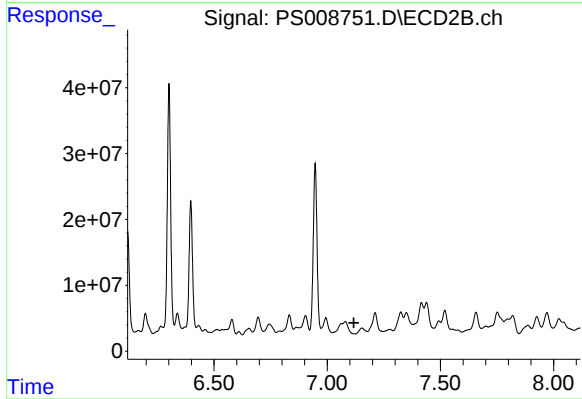


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.118 min
Response: 0
Conc: N.D.

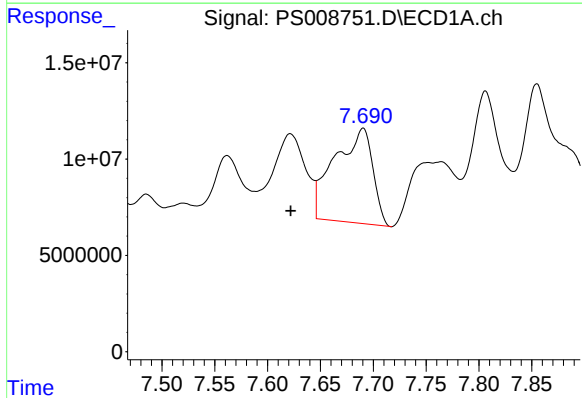


#6 MCP

R.T.: 7.690 min
Delta R.T.: 0.068 min
Response: 123017301
Conc: 20.01 ug/ml

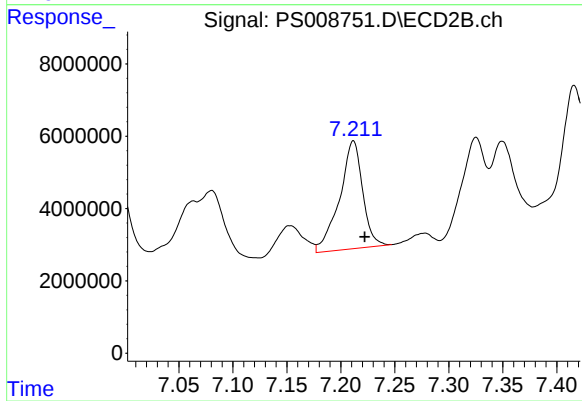

#6 MCP


R.T.: 7.211 min
Delta R.T.: -0.011 min
Response: 44344650
Conc: 15.11 ug/ml

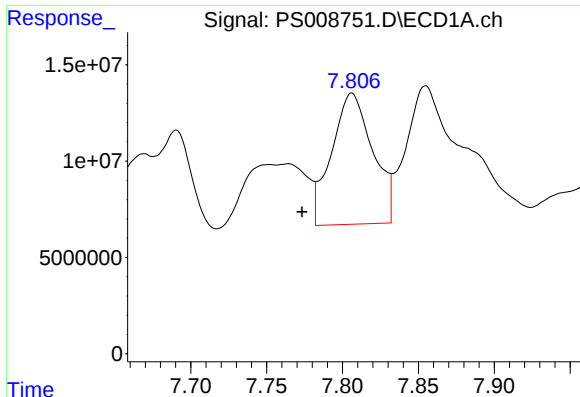

#7 MCPA


R.T.: 7.806 min
Delta R.T.: 0.033 min
Response: 128882573
Conc: 15.00 ug/ml

Instrument :
ECD_S
ClientSampleId :

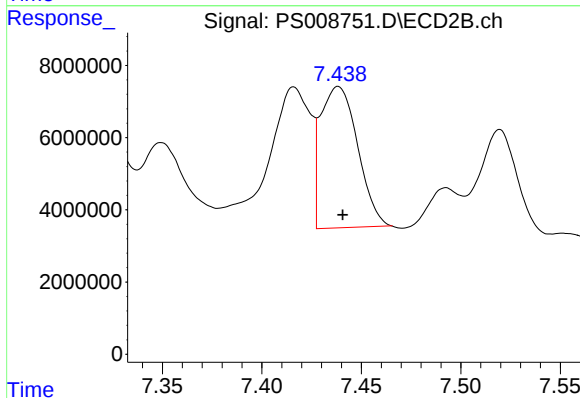


#7 MCPA

R.T.: 7.438 min
Delta R.T.: -0.002 min
Response: 51040252
Conc: 12.23 ug/ml

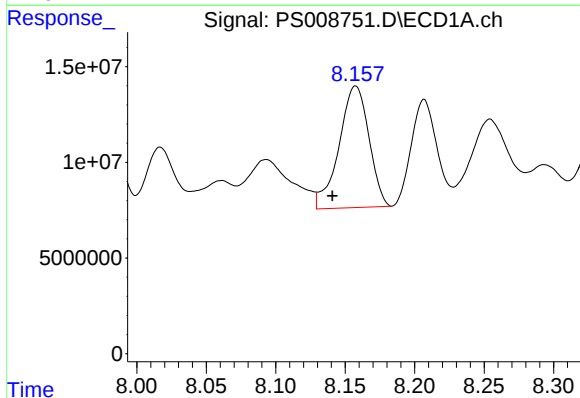


#8 DICHLORPROP

R.T.: 8.157 min
Delta R.T.: 0.017 min
Response: 95337760
Conc: 48.19 ng/ml

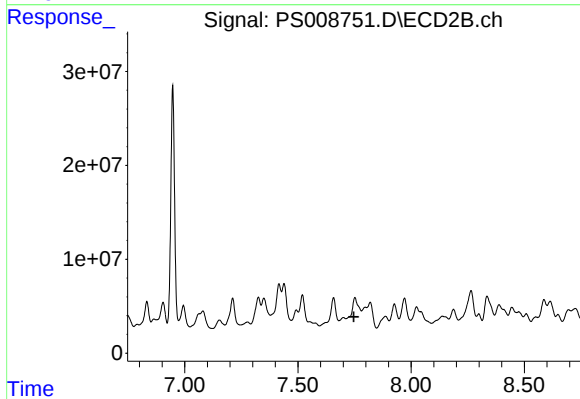

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.747 min
Response: 0
Conc: N.D.

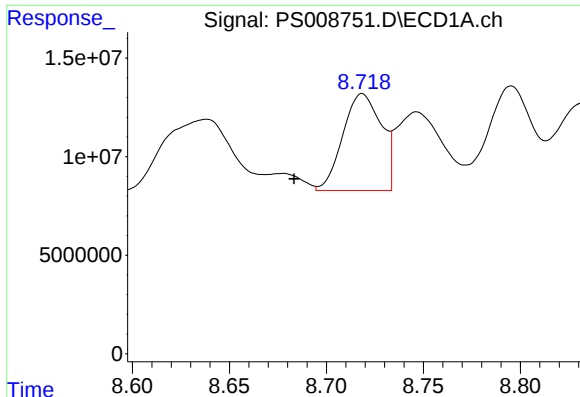

#10 Pentachlorophenol


R.T.: 8.719 min
Delta R.T.: 0.035 min
Response: 67974426
Conc: 2.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

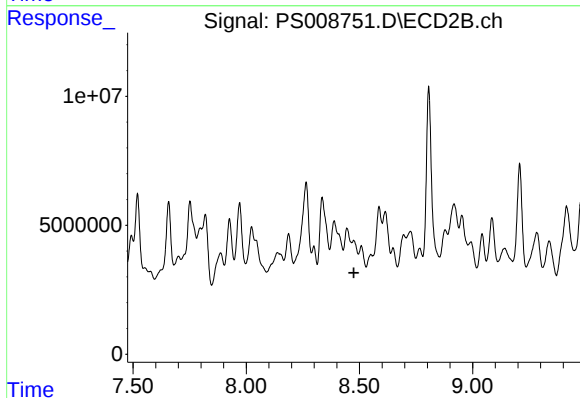


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.475 min
Response: 0
Conc: N.D.

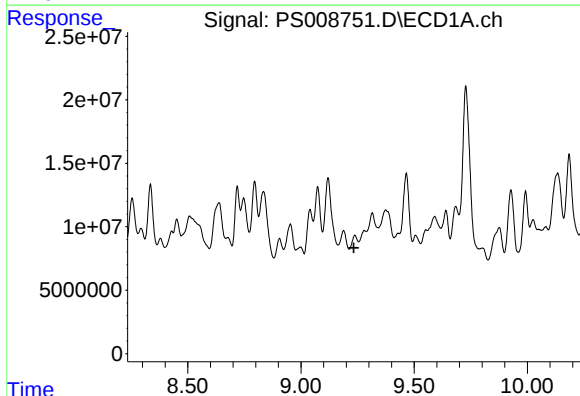


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.234 min
Response: 0
Conc: N.D.

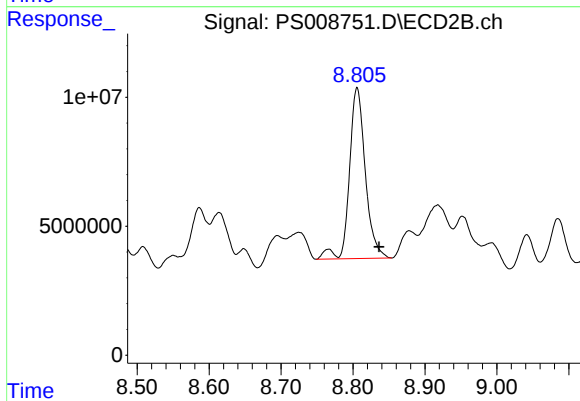

#11 2,4,5-TP (SILVEX)


R.T.: 8.806 min
Delta R.T.: -0.031 min
Response: 101773687
Conc: 19.86 ng/ml

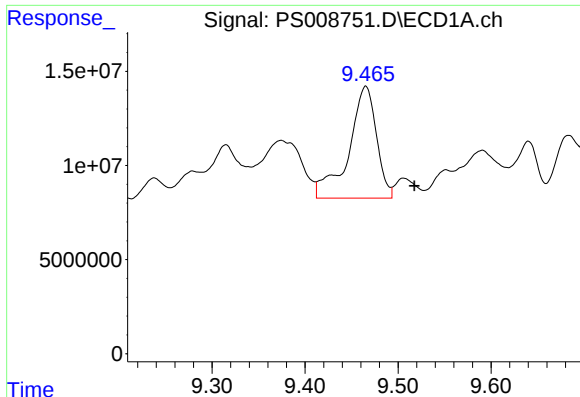

#12 2,4,5-T


R.T.: 9.465 min
Delta R.T.: -0.052 min
Response: 123417343
Conc: 11.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

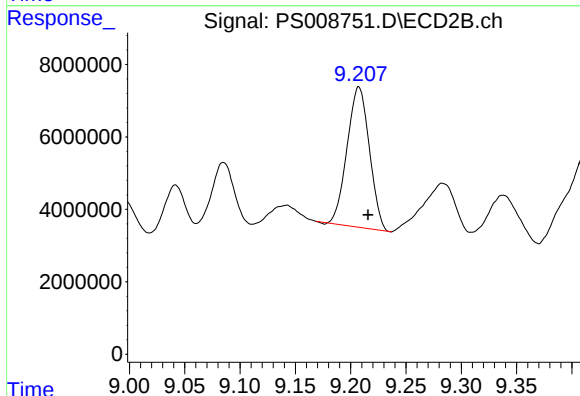


#12 2,4,5-T

R.T.: 9.207 min
Delta R.T.: -0.008 min
Response: 54205994
Conc: 10.49 ng/ml

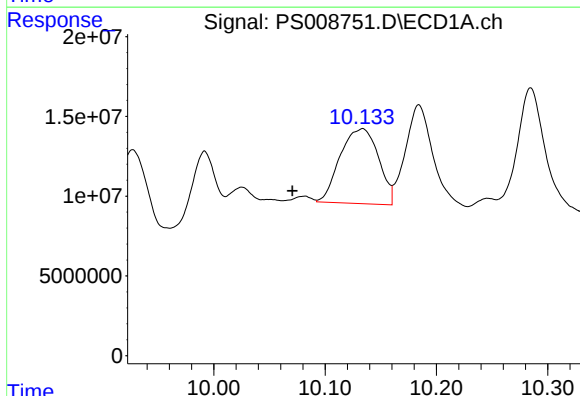


#13 2,4-DB

R.T.: 10.133 min
Delta R.T.: 0.062 min
Response: 112442748
Conc: 69.13 ng/ml

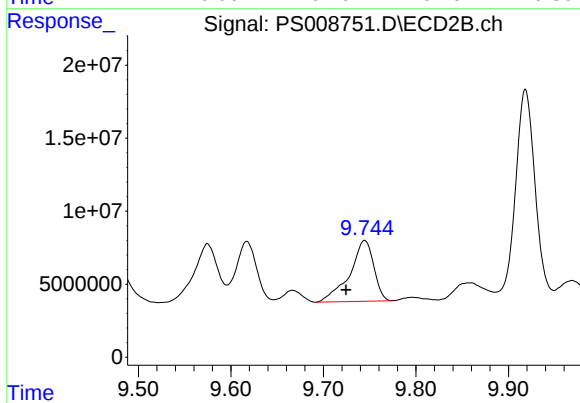

#13 2,4-DB


R.T.: 9.745 min
Delta R.T.: 0.020 min
Response: 75261780
Conc: 107.63 ng/ml

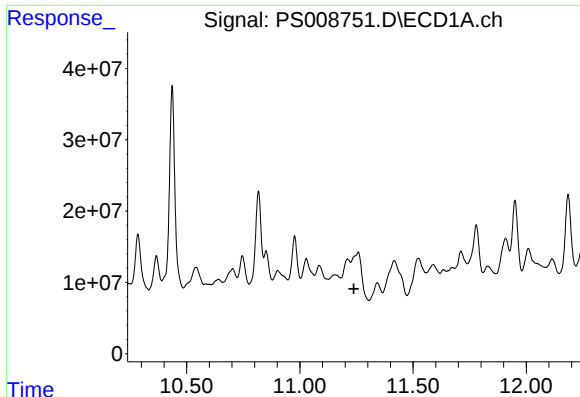

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

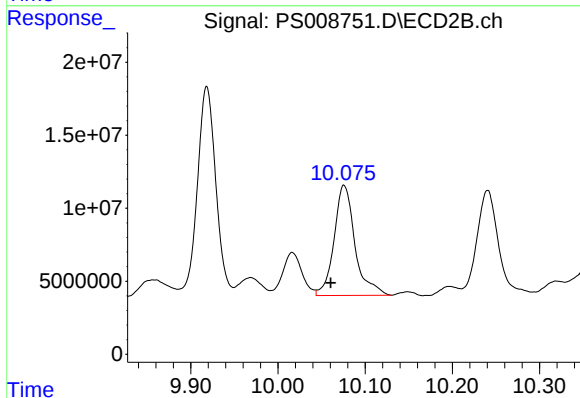


#14 DINOSEB

R.T.: 10.076 min
Delta R.T.: 0.015 min
Response: 125889357
Conc: 34.27 ng/ml

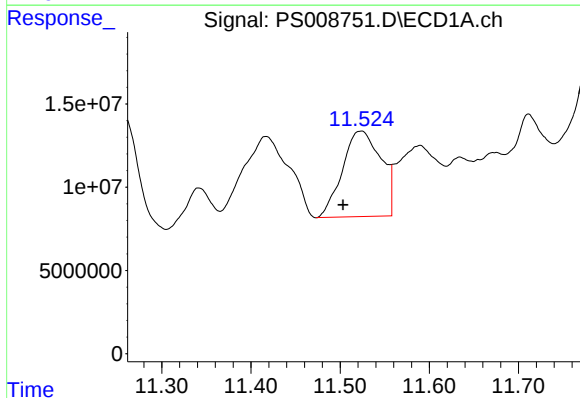

#16 DCPA

R.T.: 11.523 min
Delta R.T.: 0.020 min
Response: 155133635
Conc: 11.07 ng/ml

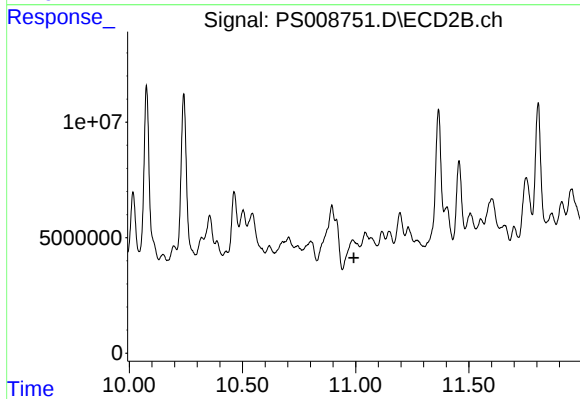

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.992 min
Response: 0
Conc: N.D.