

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
 Data File : PS008753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2020 13:44
 Operator : DD\AJ
 Sample : L1408-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 22:43:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.252	6.947	793.7E6	321.0E6	369.801	346.384
Target Compounds							
2) T	3,5-DICHL...	0.000	6.119	0	124.3E6	N.D.	90.367
5) T	DICAMBA	7.377	0.000	88272894	0	10.944	N.D. #
7) T	MCPA	7.805	7.416	84480830	69860910	9.834	16.739 #
11) T	2,4,5-TP ...	0.000	8.805	0	113.5E6	N.D.	22.154
12) T	2,4,5-T	9.464	0.000	92392312	0	8.395	N.D. #
14) T	DINOSEB	0.000	10.075	0	103.7E6	N.D.	28.220
16) T	DCPA	11.521	0.000	52026091	0	3.711	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
Data File : PS008753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2020 13:44
Operator : DD\AJ
Sample : L1408-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 22:43:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

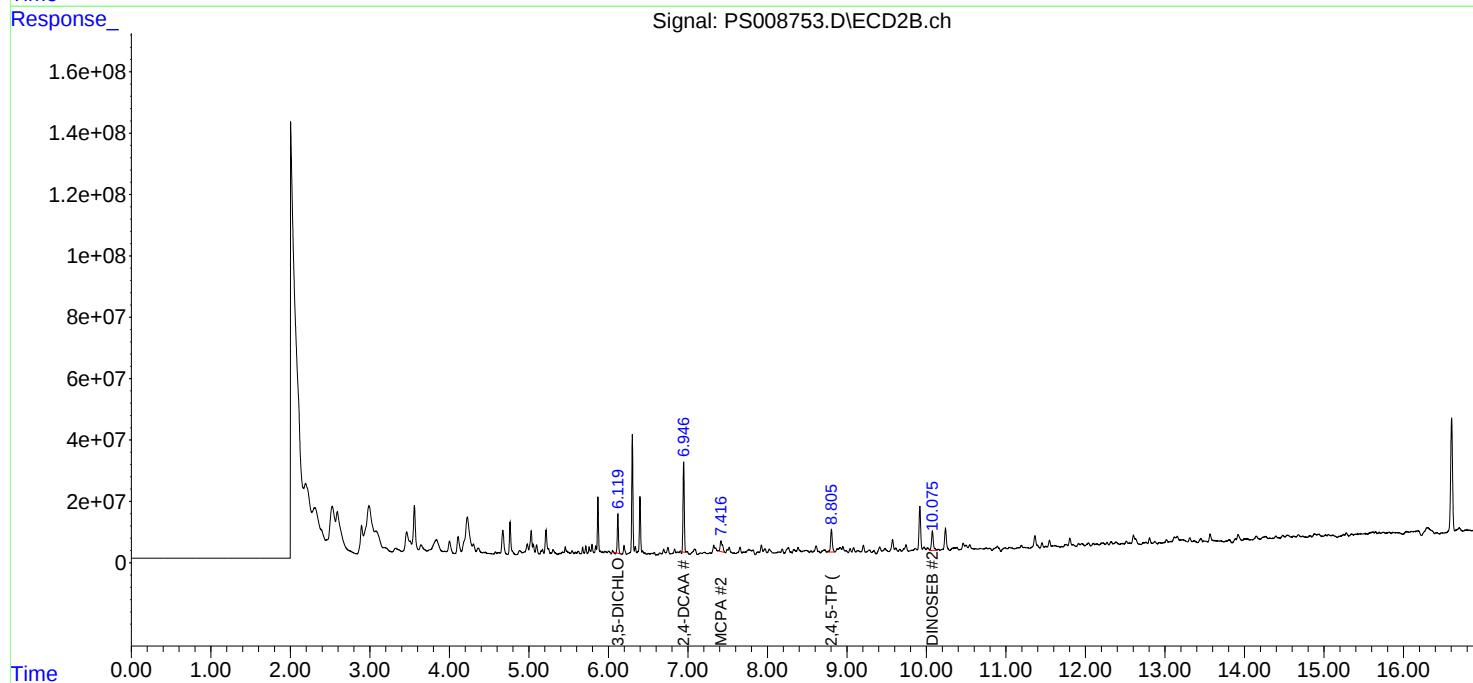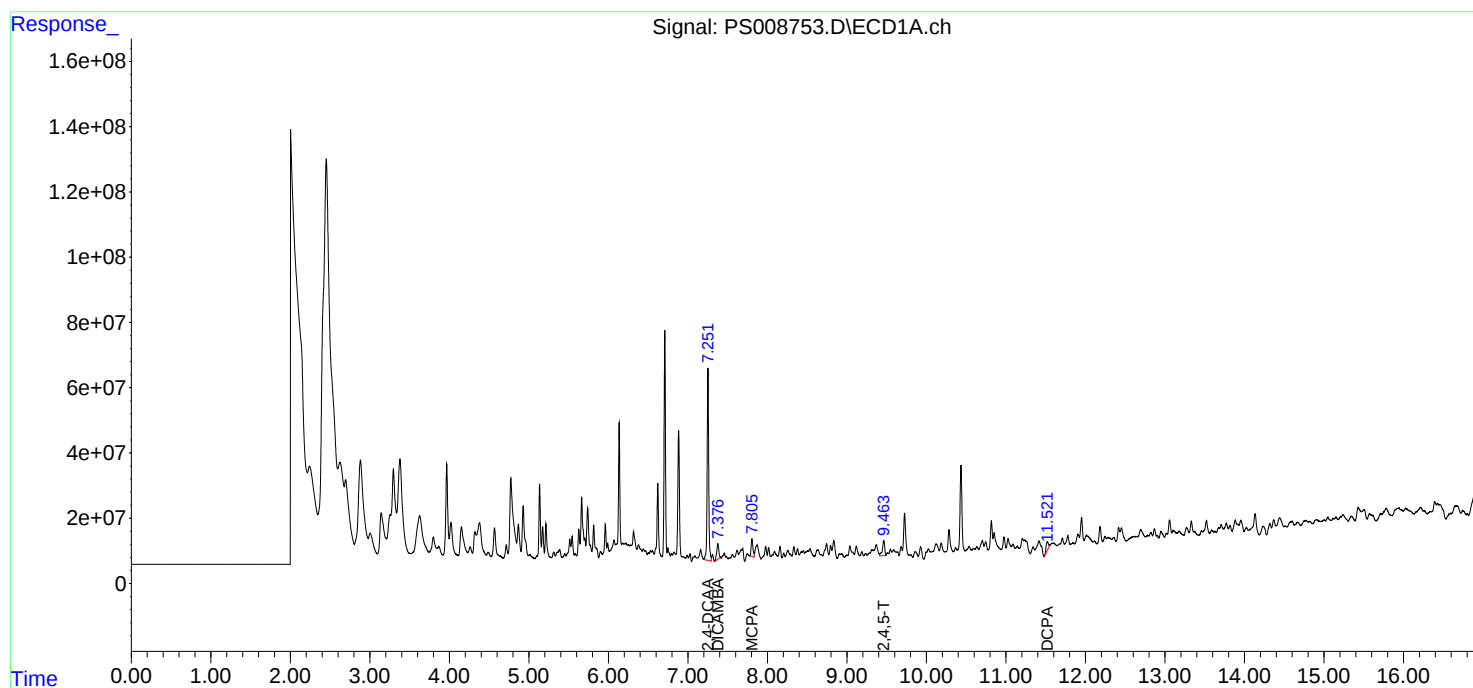


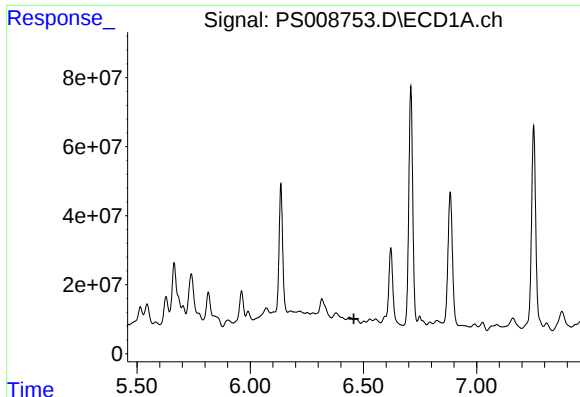

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

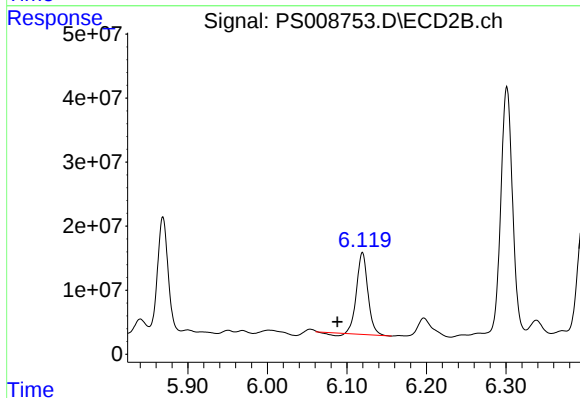


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.119 min
Delta R.T.: 0.031 min
Response: 124334237
Conc: 90.37 ng/ml

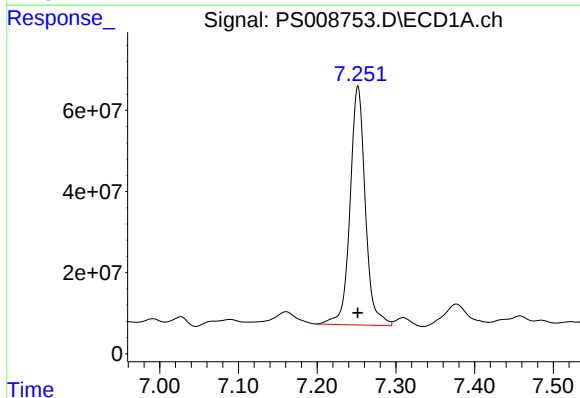


#4 2,4-DCAA

R.T.: 7.252 min
Delta R.T.: 0.000 min
Response: 793707968
Conc: 369.80 ng/ml

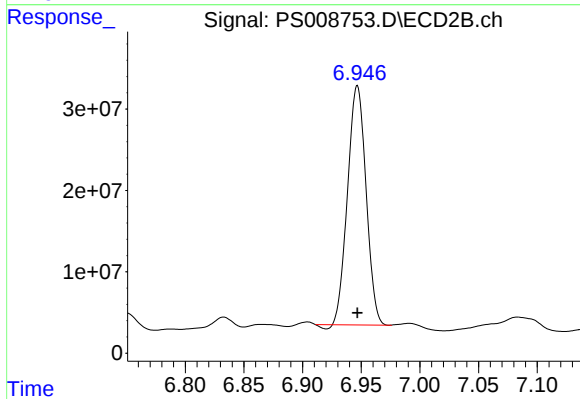

#4 2,4-DCAA


R.T.: 6.947 min
Delta R.T.: 0.000 min
Response: 321036659
Conc: 346.38 ng/ml

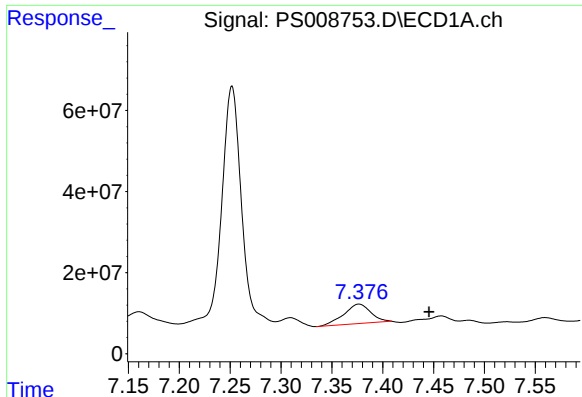

#5 DICAMBA


R.T.: 7.377 min
Delta R.T.: -0.069 min
Response: 88272894
Conc: 10.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

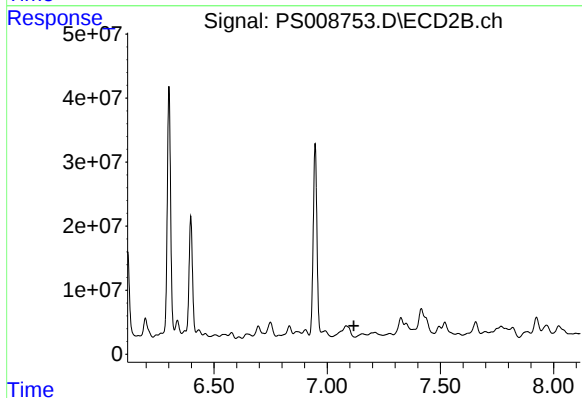


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.118 min
Response: 0
Conc: N.D.

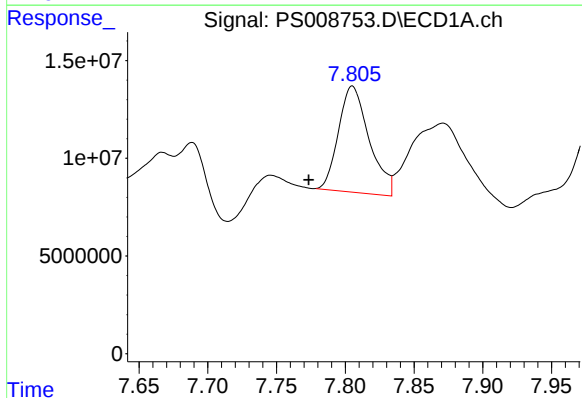


#7 MCPA

R.T.: 7.805 min
Delta R.T.: 0.032 min
Response: 84480830
Conc: 9.83 ug/ml

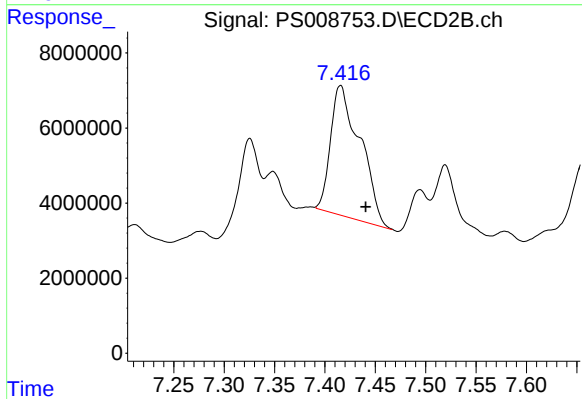

#7 MCPA


R.T.: 7.416 min
Delta R.T.: -0.025 min
Response: 69860910
Conc: 16.74 ug/ml

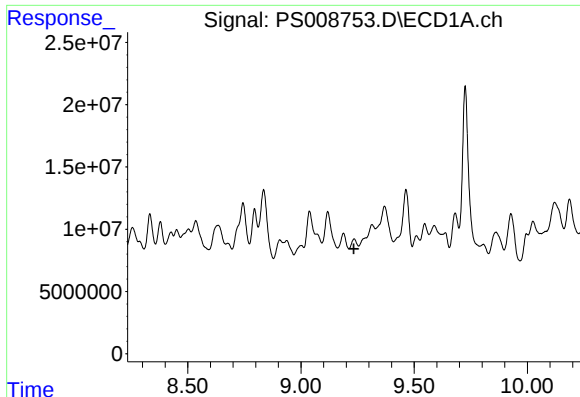

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

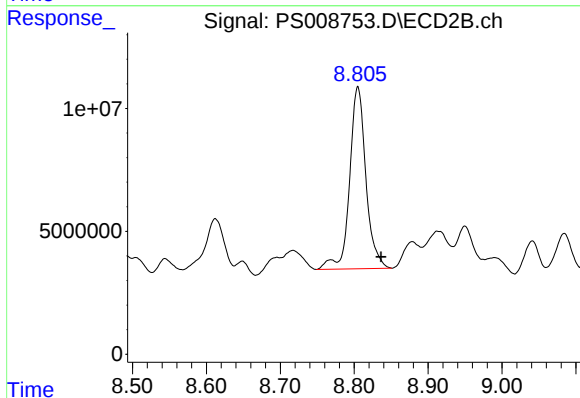


#11 2,4,5-TP (SILVEX)

R.T.: 8.805 min
Delta R.T.: -0.031 min
Response: 113544633
Conc: 22.15 ng/ml

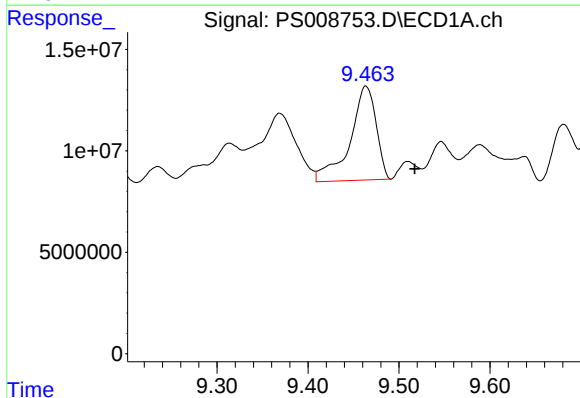


#12 2,4,5-T

R.T.: 9.464 min
Delta R.T.: -0.054 min
Response: 92392312
Conc: 8.39 ng/ml

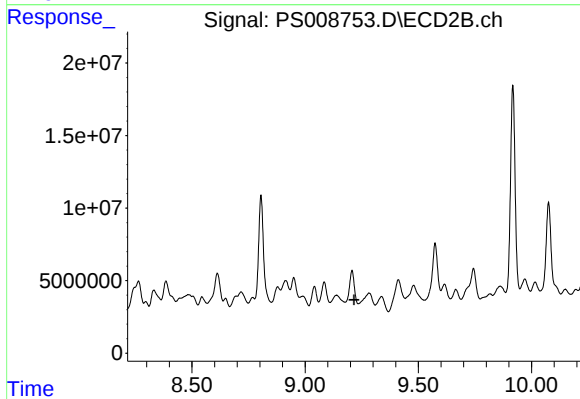

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.216 min
Response: 0
Conc: N.D.

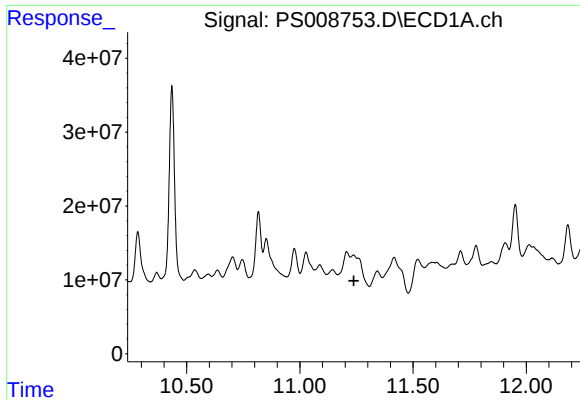

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

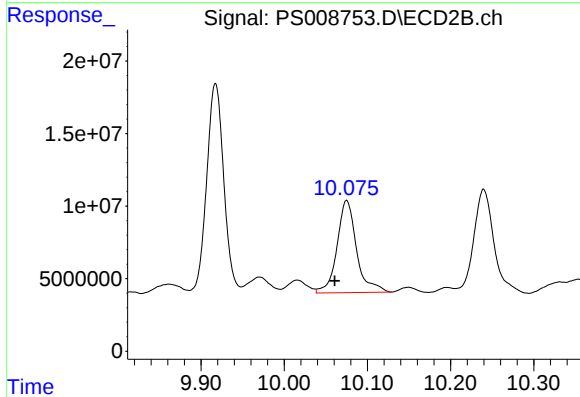


#14 DINOSEB

R.T.: 10.075 min
Delta R.T.: 0.014 min
Response: 103652265
Conc: 28.22 ng/ml

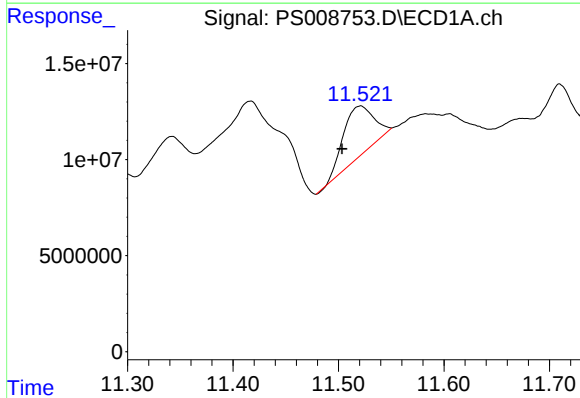

#16 DCPA

R.T.: 11.521 min
Delta R.T.: 0.017 min
Response: 52026091
Conc: 3.71 ng/ml

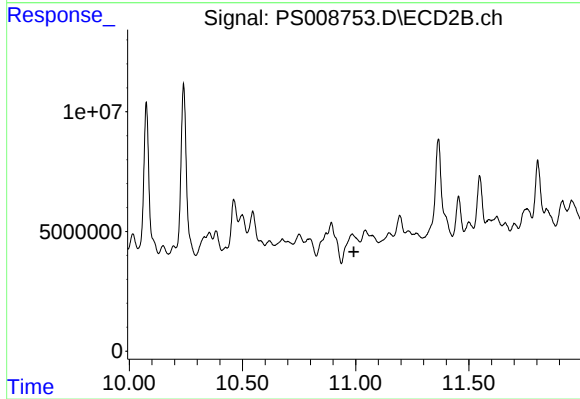

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.992 min
Response: 0
Conc: N.D.