

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
 Data File : PS008755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2020 14:30
 Operator : DD\AJ
 Sample : L1409-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 22:44:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.251	6.946	860.1E6	310.7E6	400.734	335.243
Target Compounds							
2) T	3,5-DICHL...	0.000	6.119	0	76456907	N.D.	55.569
5) T	DICAMBA	7.380	0.000	170.2E6	0	21.102	N.D. #
7) T	MCPA	7.804	7.439	159.6E6	52641053	18.576	12.613 #
8) T	DICHLORPROP	8.156	0.000	134.7E6	0	68.095	N.D. #
10) T	Pentachlo...	8.745	0.000	88009533	0	3.096	N.D. #
11) T	2,4,5-TP ...	0.000	8.804	0	100.4E6	N.D.	19.587
12) T	2,4,5-T	9.464	0.000	90724321	0	8.243	N.D. #
13) T	2,4-DB	10.117	0.000	301.7E6	0	185.501	N.D. #
16) T	DCPA	11.569	0.000	160.1E6	0	11.417	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
Data File : PS008755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2020 14:30
Operator : DD\AJ
Sample : L1409-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 22:44:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

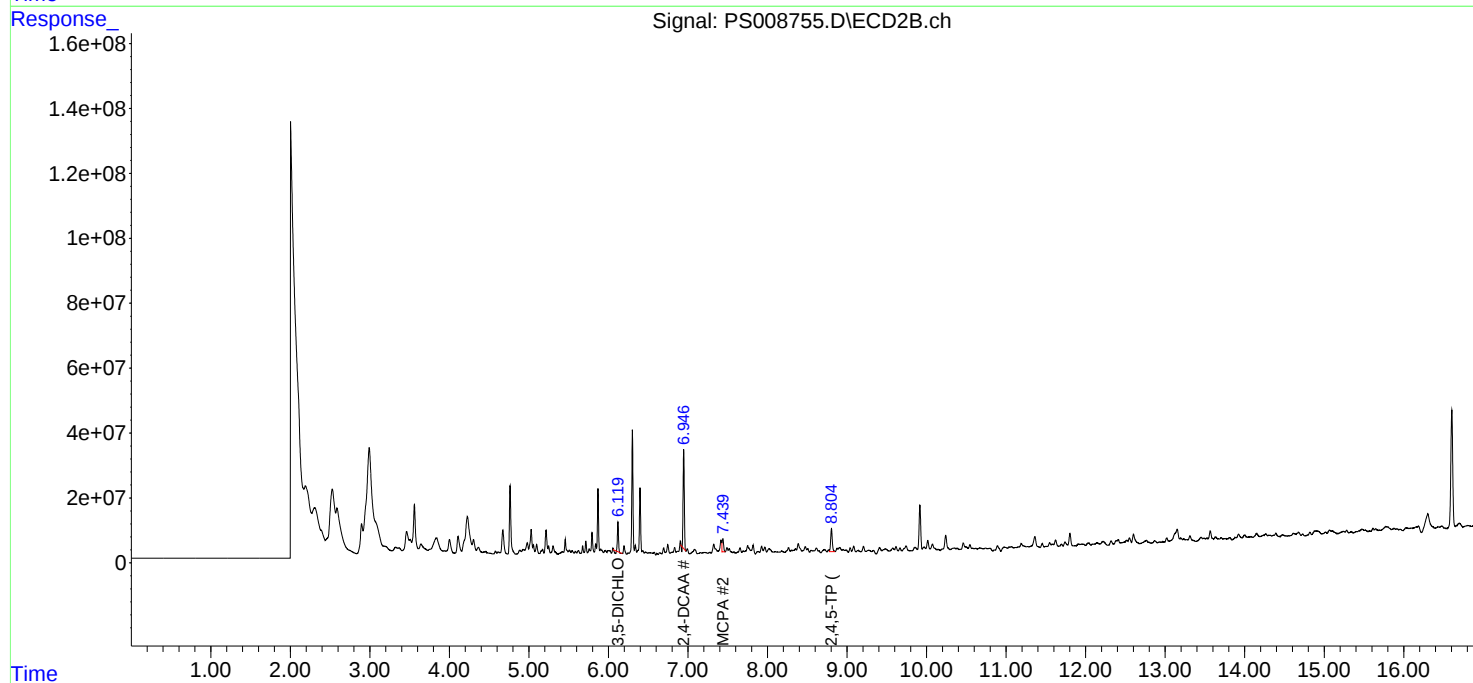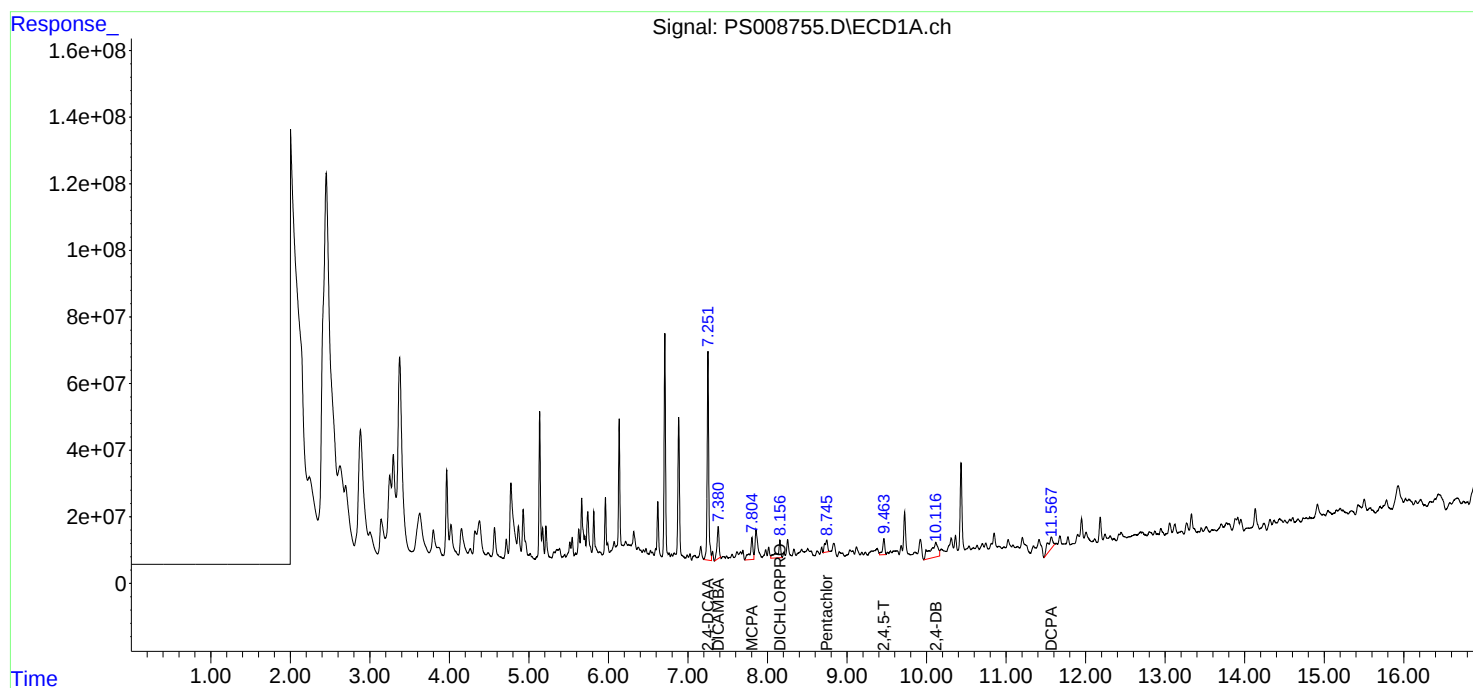


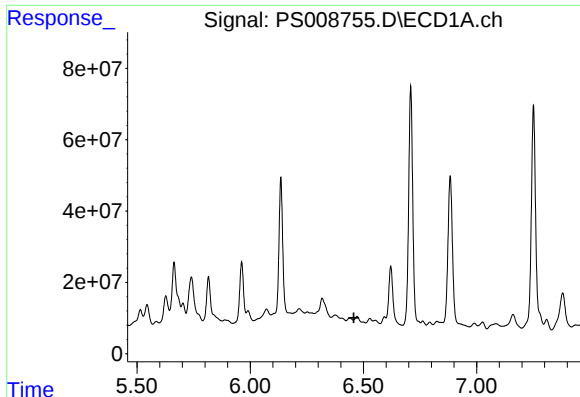

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

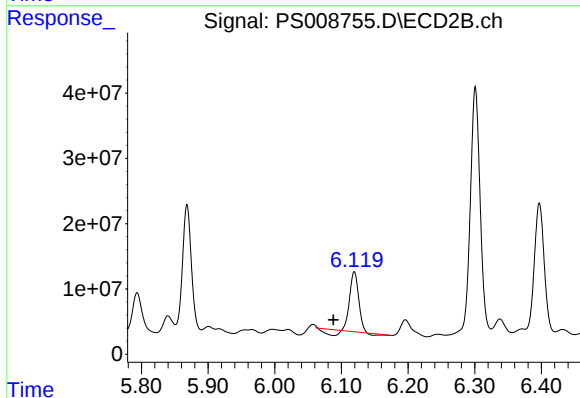


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.119 min
Delta R.T.: 0.031 min
Response: 76456907
Conc: 55.57 ng/ml

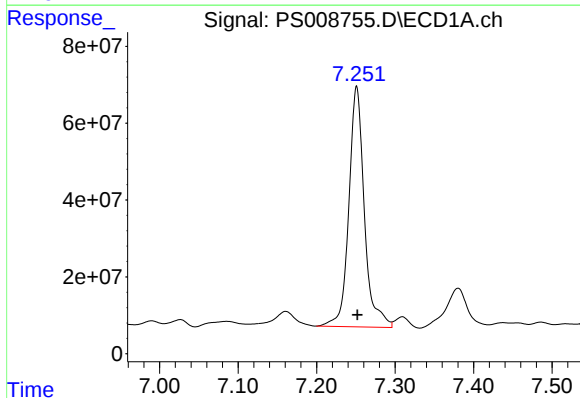


#4 2,4-DCAA

R.T.: 7.251 min
Delta R.T.: 0.000 min
Response: 860098067
Conc: 400.73 ng/ml

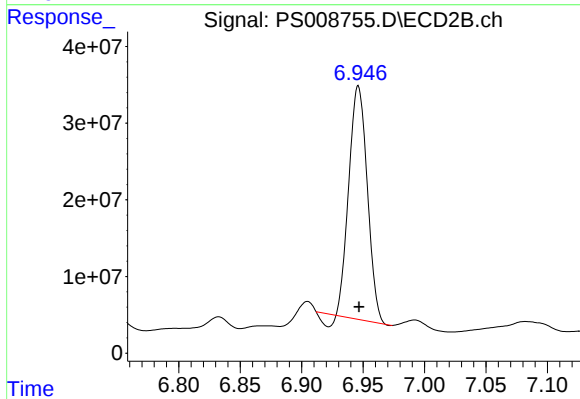

#4 2,4-DCAA


R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 310711403
Conc: 335.24 ng/ml

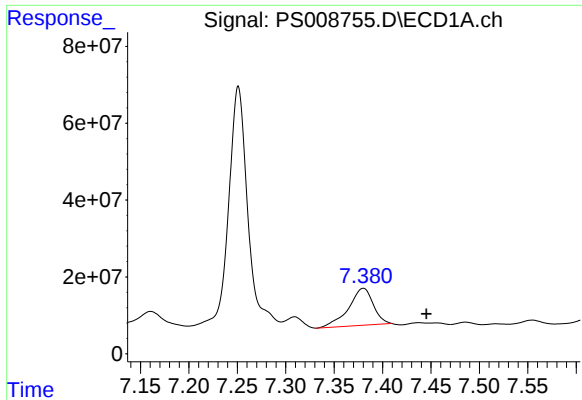

#5 DICAMBA


R.T.: 7.380 min
Delta R.T.: -0.065 min
Response: 170207490
Conc: 21.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

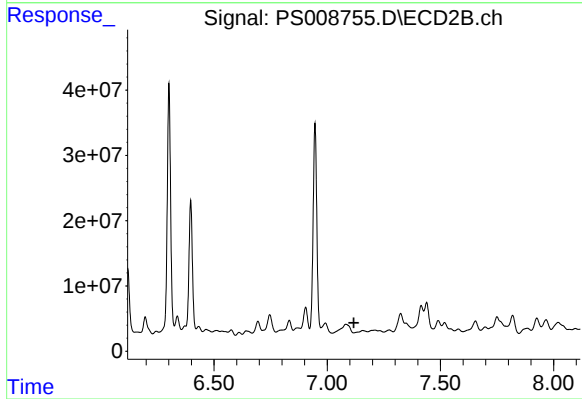


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

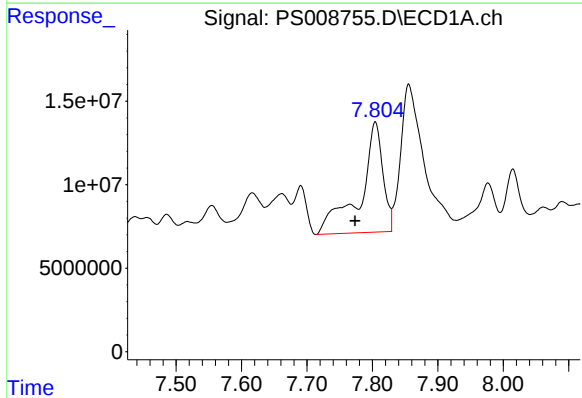


#7 MCPA

R.T.: 7.804 min
Delta R.T.: 0.031 min
Response: 159577733
Conc: 18.58 ug/ml

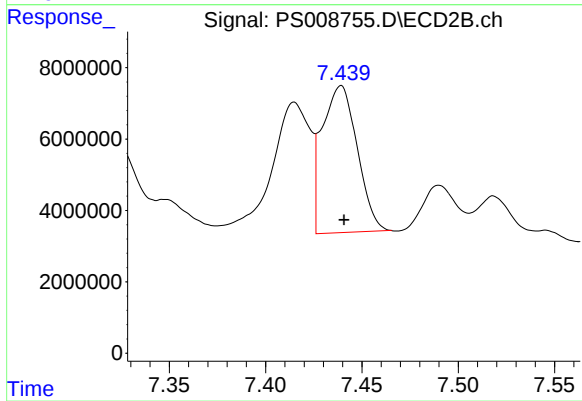

#7 MCPA


R.T.: 7.439 min
Delta R.T.: -0.002 min
Response: 52641053
Conc: 12.61 ug/ml

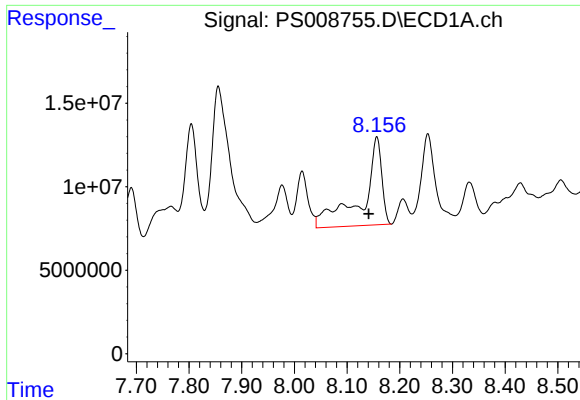

#8 DICHLORPROP


R.T.: 8.156 min
Delta R.T.: 0.016 min
Response: 134724782
Conc: 68.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

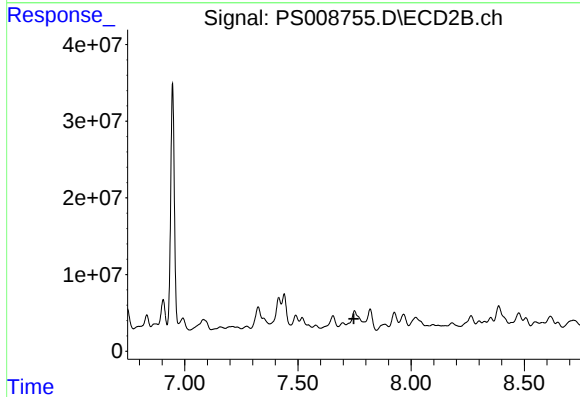


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.747 min
Response: 0
Conc: N.D.

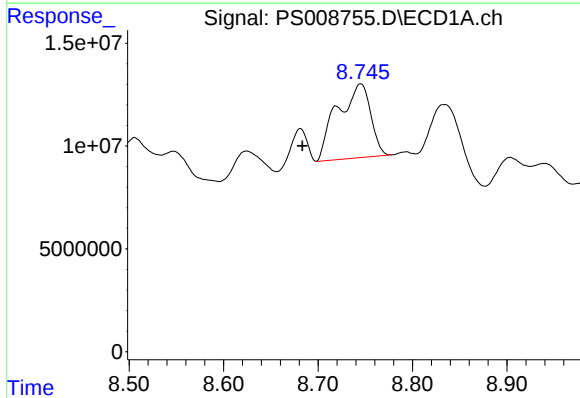


#10 Pentachlorophenol

R.T.: 8.745 min
Delta R.T.: 0.062 min
Response: 88009533
Conc: 3.10 ng/ml

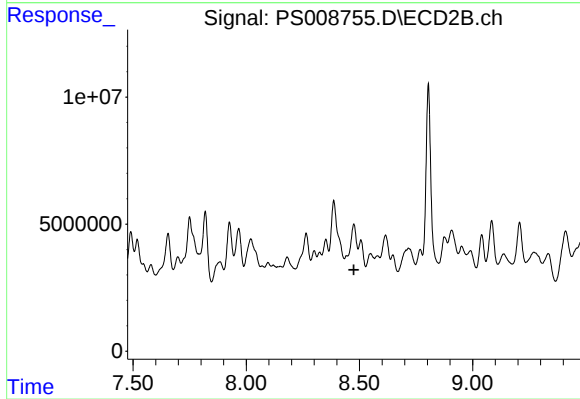

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 8.475 min
Response: 0
Conc: N.D.

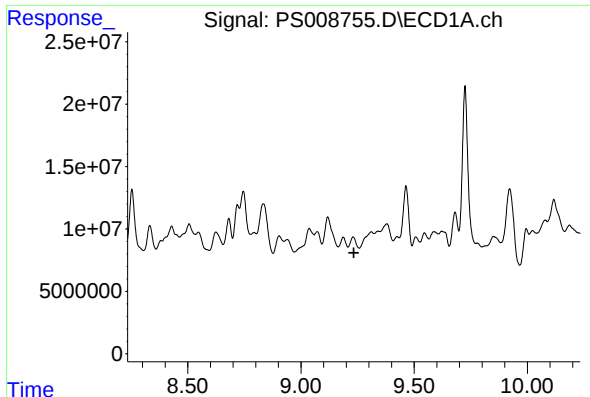

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

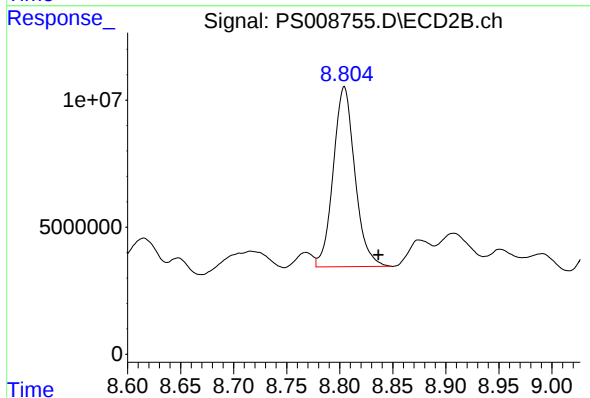


#11 2,4,5-TP (SILVEX)

R.T.: 8.804 min
Delta R.T.: -0.032 min
Response: 100386954
Conc: 19.59 ng/ml

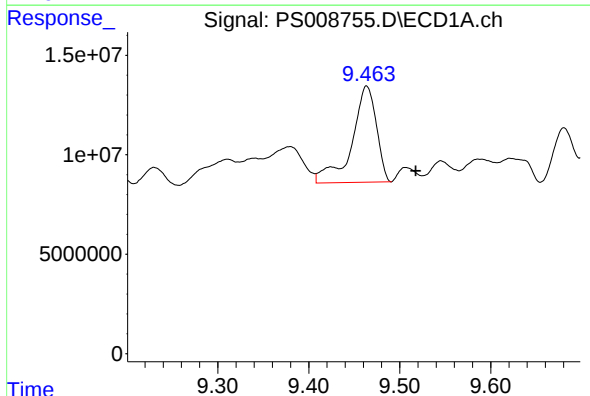


#12 2,4,5-T

R.T.: 9.464 min
Delta R.T.: -0.054 min
Response: 90724321
Conc: 8.24 ng/ml

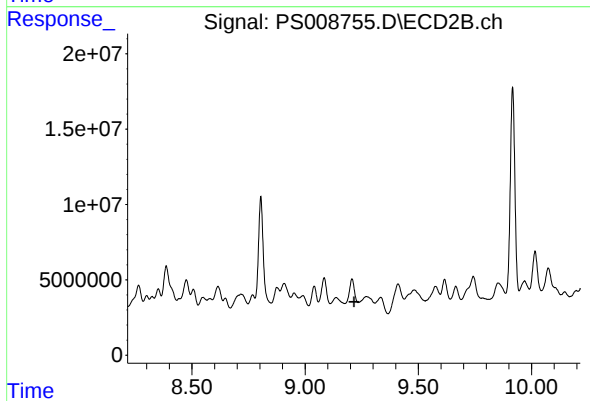

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.216 min
Response: 0
Conc: N.D.

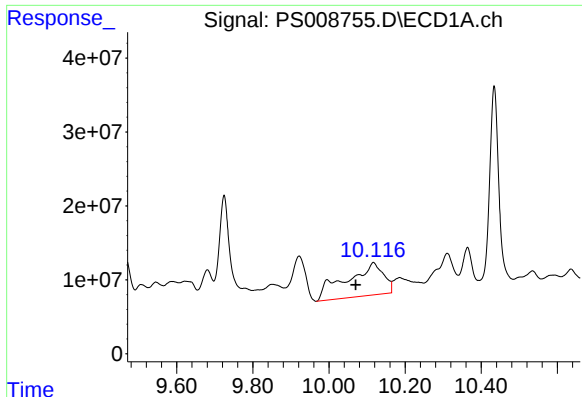

#13 2,4-DB


R.T.: 10.117 min
Delta R.T.: 0.046 min
Response: 301734126
Conc: 185.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

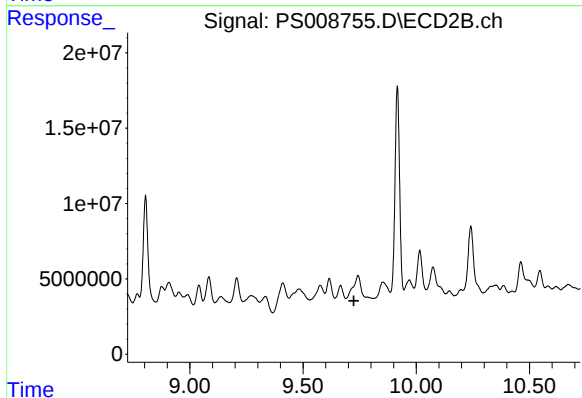


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.724 min
Response: 0
Conc: N.D.

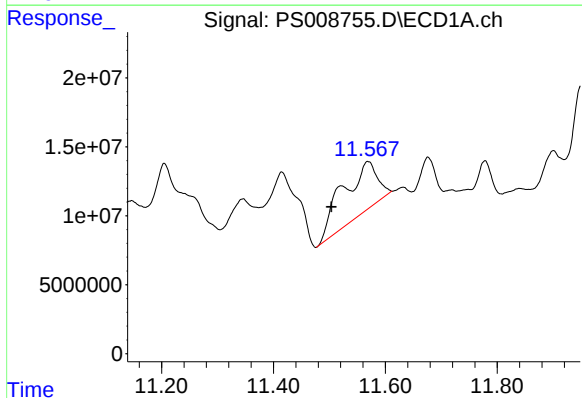

#16 DCPA

R.T.: 11.569 min
Delta R.T.: 0.066 min
Response: 160055334
Conc: 11.42 ng/ml

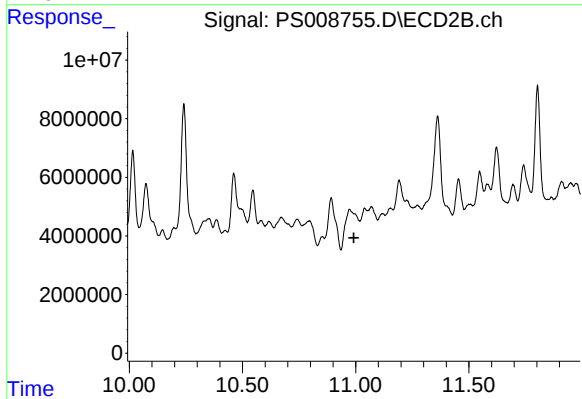

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.992 min
Response: 0
Conc: N.D.