

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
 Data File : PS008760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2020 16:47
 Operator : DD\AJ
 Sample : PB126666BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 22:45:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.251	6.946	1276.2E6	607.4E6	594.598	655.309
Target Compounds							
1) T	Dalapon	0.000	2.595	0	281.0E6	N.D.	234.276
2) T	3,5-DICHL...	0.000	6.119	0	57152872	N.D.	41.539
7) T	MCPA	7.804	7.414	75936810	40772946	8.840	9.769
12) T	2,4,5-T	0.000	9.267	0	75865005	N.D.	14.681
15) T	Picloram	11.050	11.040	602.1E6	322.4E6	39.756	42.712
16) T	DCPA	0.000	11.040	0	322.4E6	N.D.	49.567



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
Data File : PS008760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2020 16:47
Operator : DD\AJ
Sample : PB126666BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 22:45:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

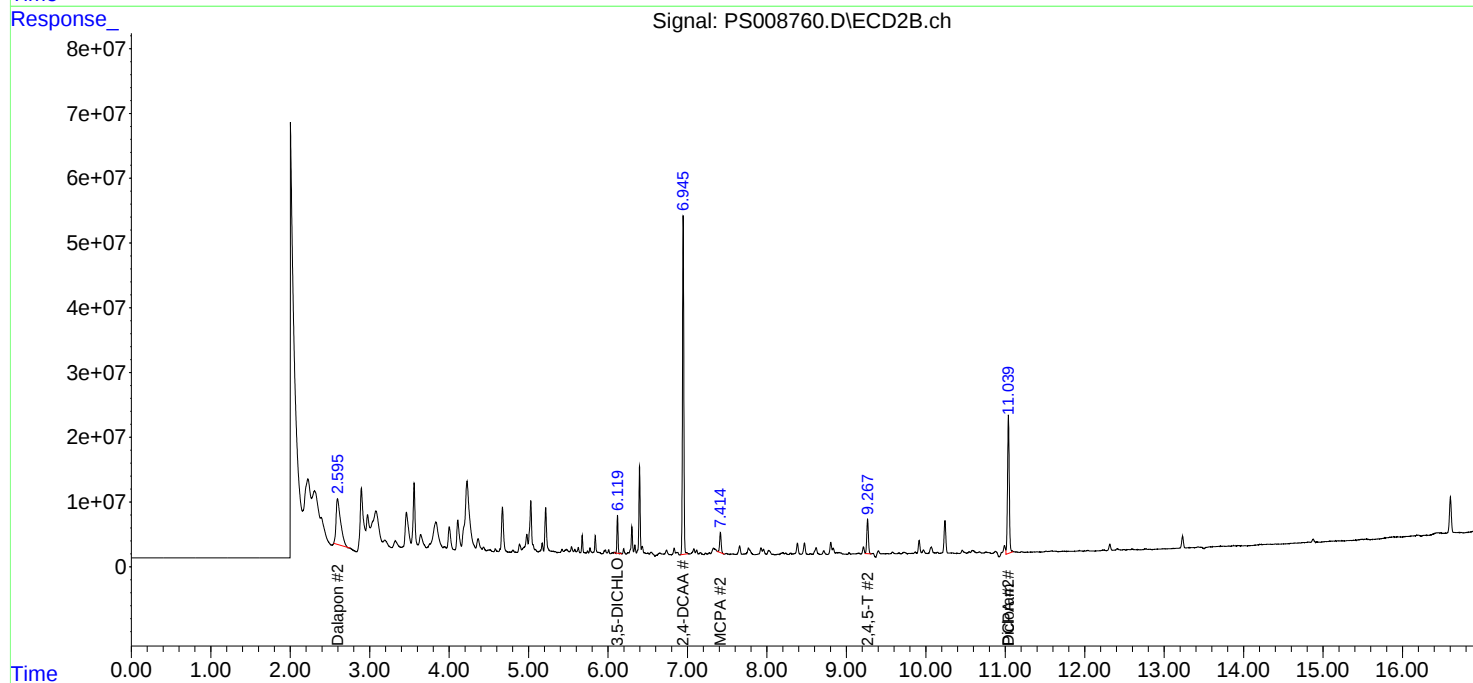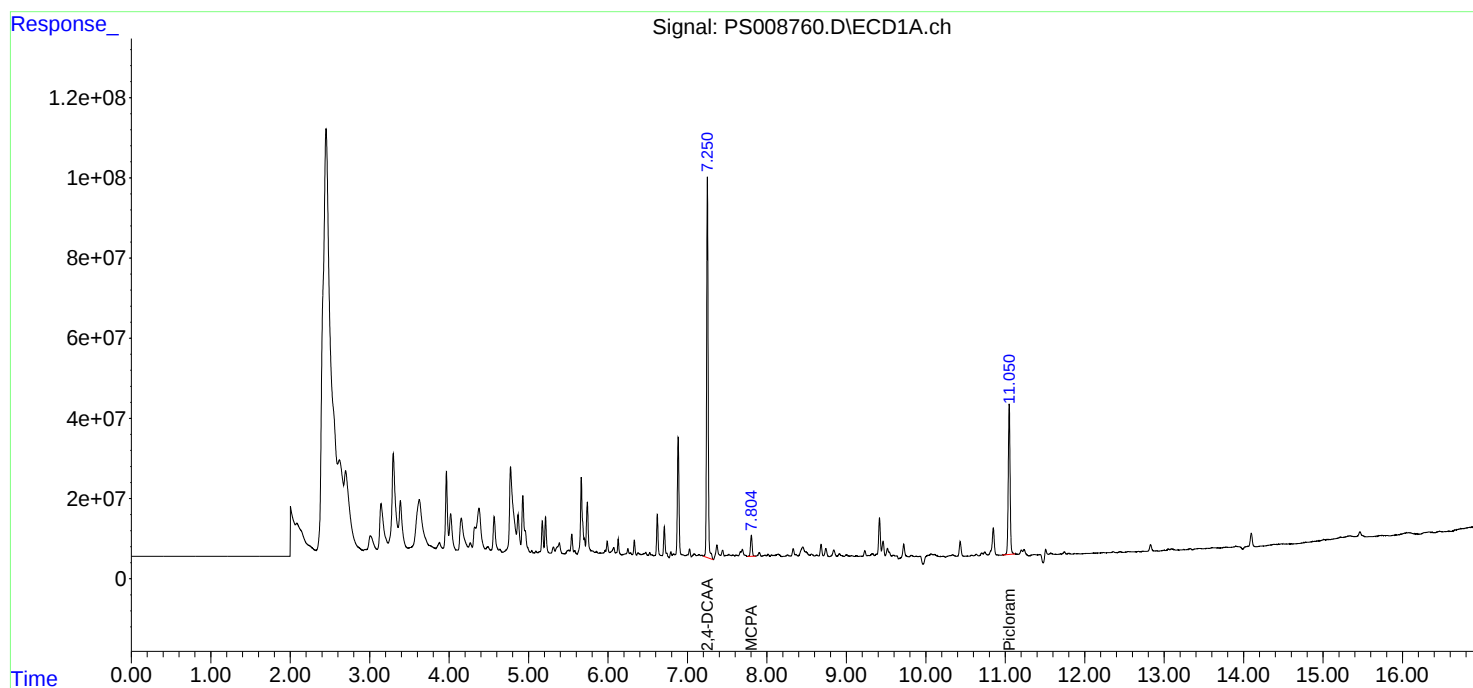


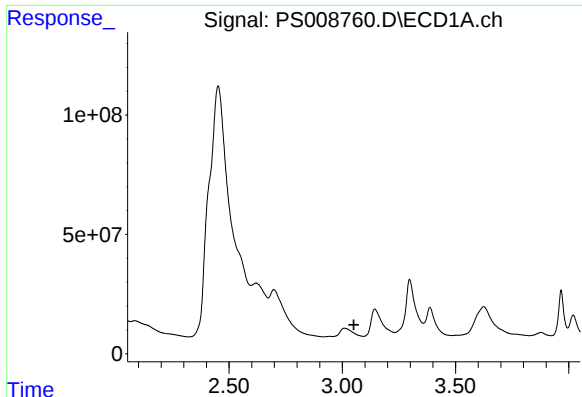

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

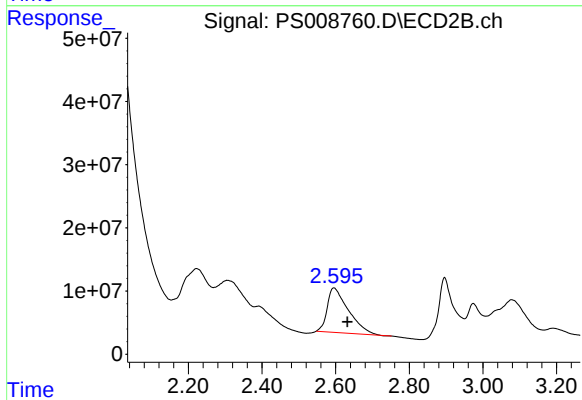


#1 Dalapon

R.T.: 2.595 min
Delta R.T.: -0.036 min
Response: 280970883
Conc: 234.28 ng/ml

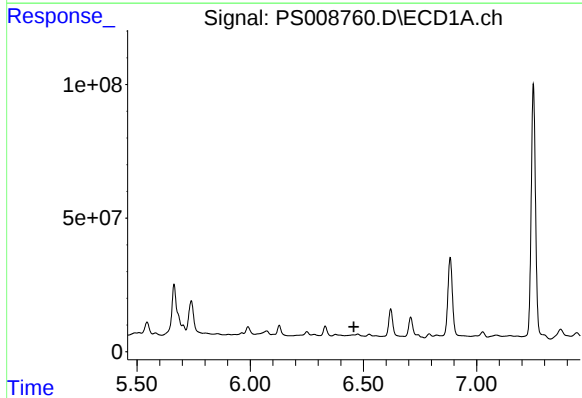


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

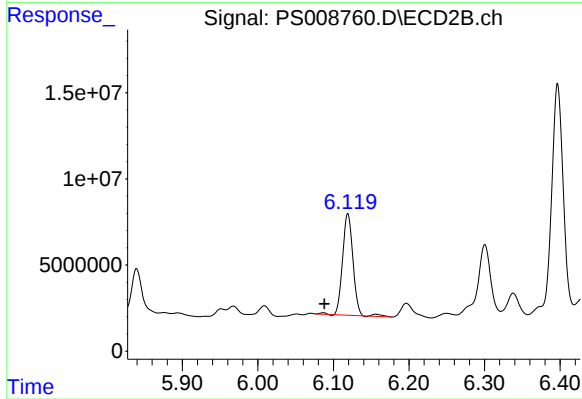

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.119 min
Delta R.T.: 0.031 min
Response: 57152872
Conc: 41.54 ng/ml

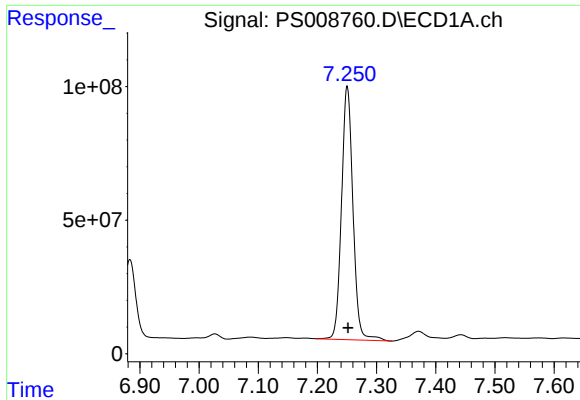

#4 2,4-DCAA


R.T.: 7.251 min
Delta R.T.: -0.001 min
Response: 1276191079
Conc: 594.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

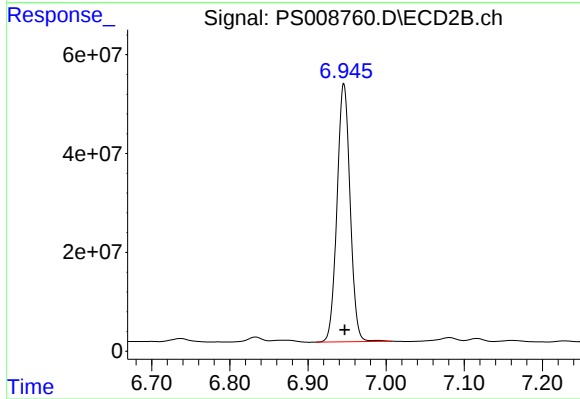


#4 2,4-DCAA

R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 607356542
Conc: 655.31 ng/ml

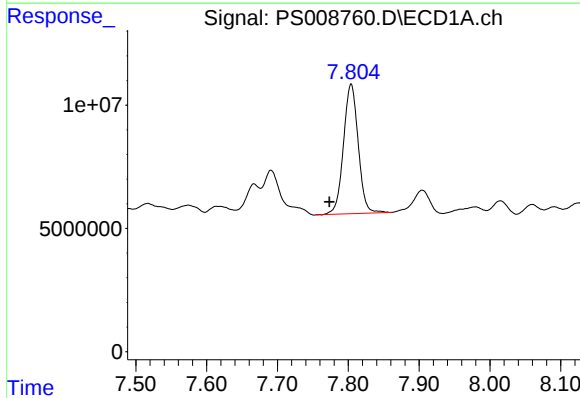


#7 MCPA

R.T.: 7.804 min
Delta R.T.: 0.031 min
Response: 75936810
Conc: 8.84 ug/ml

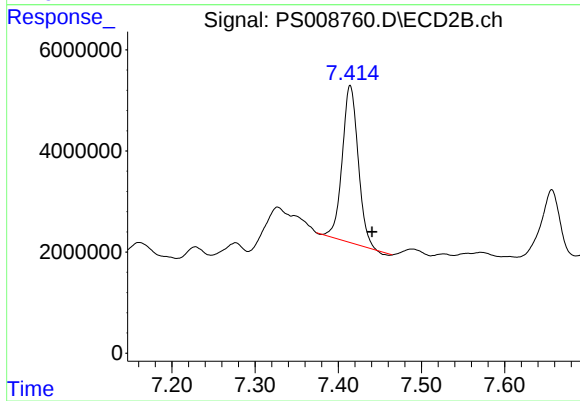

#7 MCPA


R.T.: 7.414 min
Delta R.T.: -0.026 min
Response: 40772946
Conc: 9.77 ug/ml

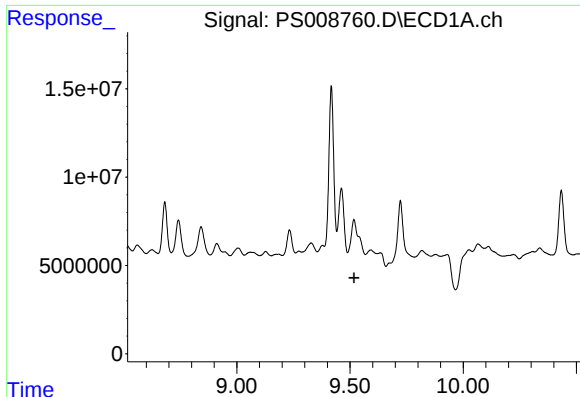

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.517 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

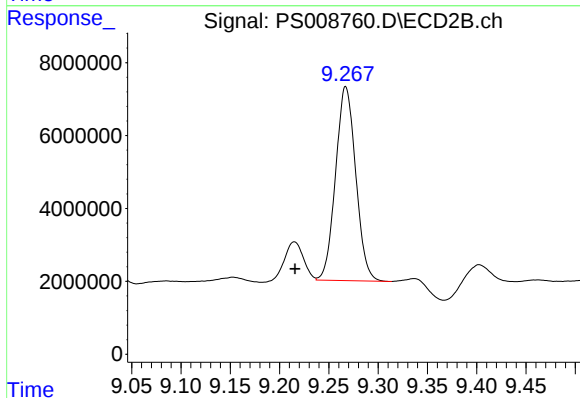


#12 2,4,5-T

R.T.: 9.267 min
Delta R.T.: 0.052 min
Response: 75865005
Conc: 14.68 ng/ml

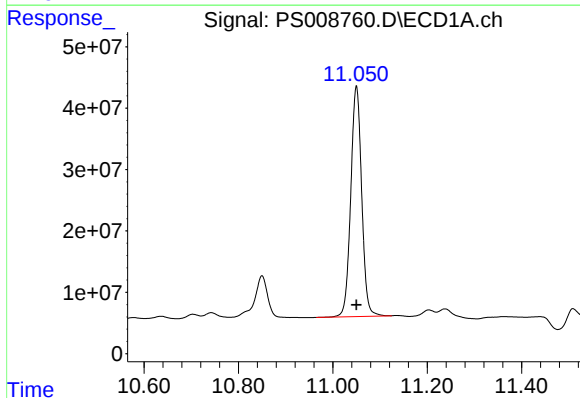


#15 Picloram

R.T.: 11.050 min
Delta R.T.: 0.000 min
Response: 602060910
Conc: 39.76 ng/ml

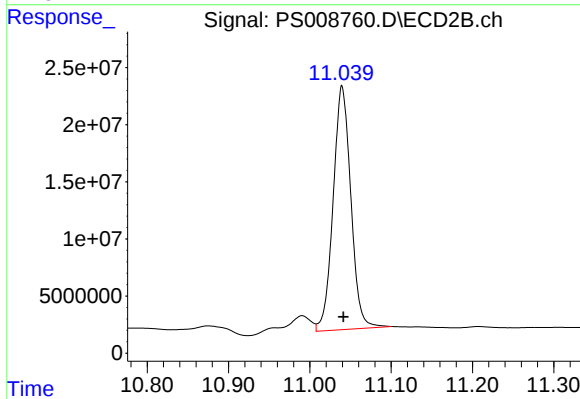

#15 Picloram


R.T.: 11.040 min
Delta R.T.: -0.001 min
Response: 322393176
Conc: 42.71 ng/ml

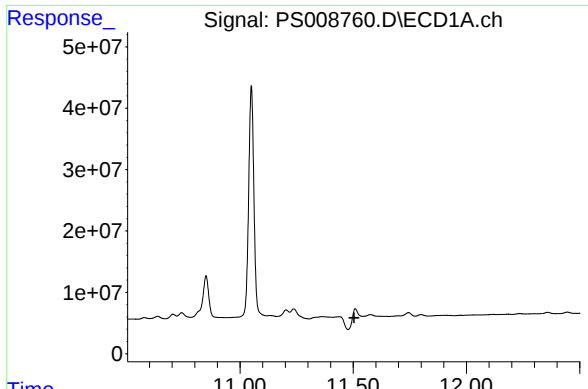

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

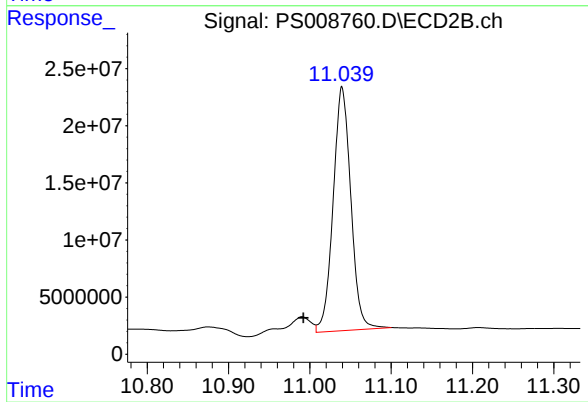

#16 DCPA

R.T.: 11.040 min
Delta R.T.: 0.048 min
Response: 322393176
Conc: 49.57 ng/ml