

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
 Data File : PS008772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2020 21:22
 Operator : DD\AJ
 Sample : L1433-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 22:49:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
 Quant Title : 8080.M
 QLast Update : Wed Feb 05 02:36:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.249	6.945	815.1E6	364.1E6	379.755	392.875
Target Compounds							
1) T	Dalapon	0.000	2.595	0	155.8E6	N.D.	129.868
2) T	3,5-DICHL...	0.000	6.118	0	149.4E6	N.D.	108.580
10) T	Pentachlo...	8.681	0.000	63750232	0	2.242	N.D. #
11) T	2,4,5-TP ...	0.000	8.802	0	89028557	N.D.	17.371
12) T	2,4,5-T	0.000	9.266	0	52635070	N.D.	10.186
14) T	DINOSEB	0.000	10.104	0	82689168	N.D.	22.512
15) T	Picloram	11.048	11.038	374.2E6	180.0E6	24.711	23.841
16) T	DCPA	0.000	11.038	0	180.0E6	N.D.	27.668



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020720\
Data File : PS008772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2020 21:22
Operator : DD\AJ
Sample : L1433-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 22:49:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020420.M
Quant Title : 8080.M
QLast Update : Wed Feb 05 02:36:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

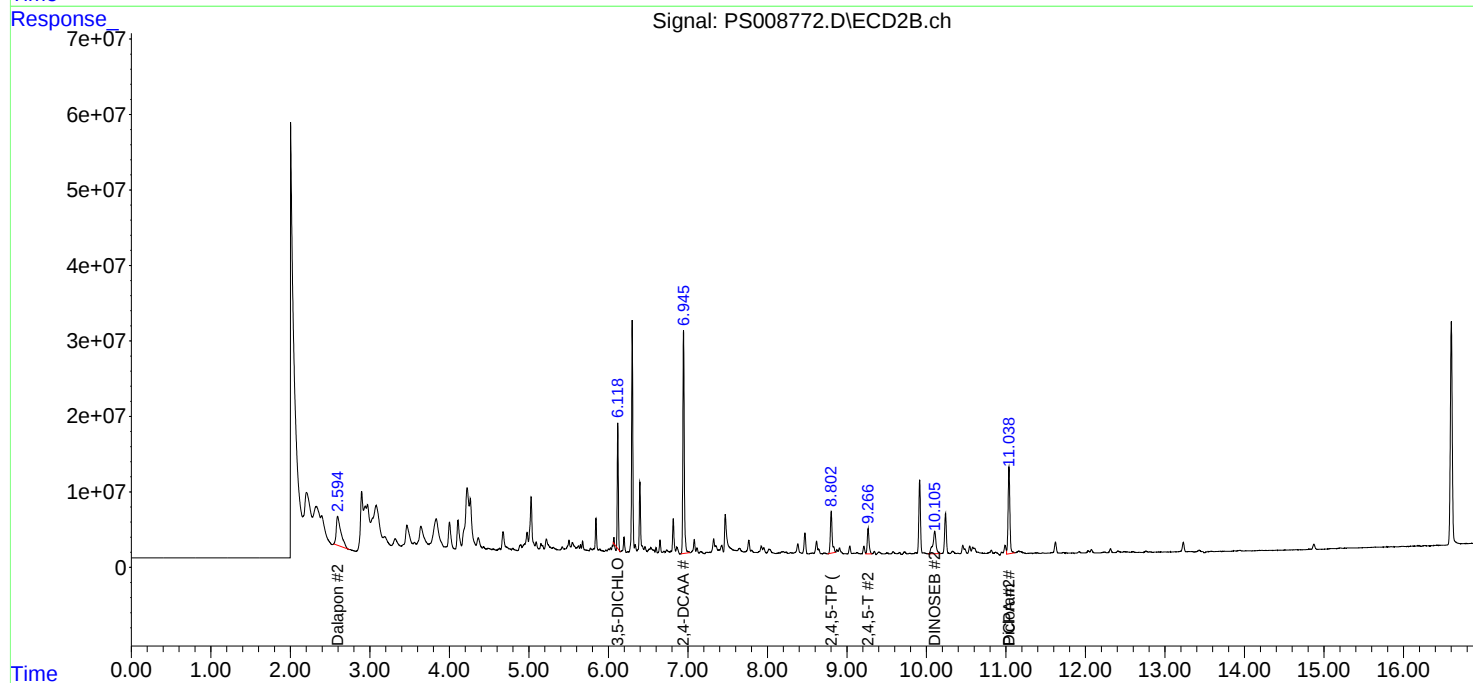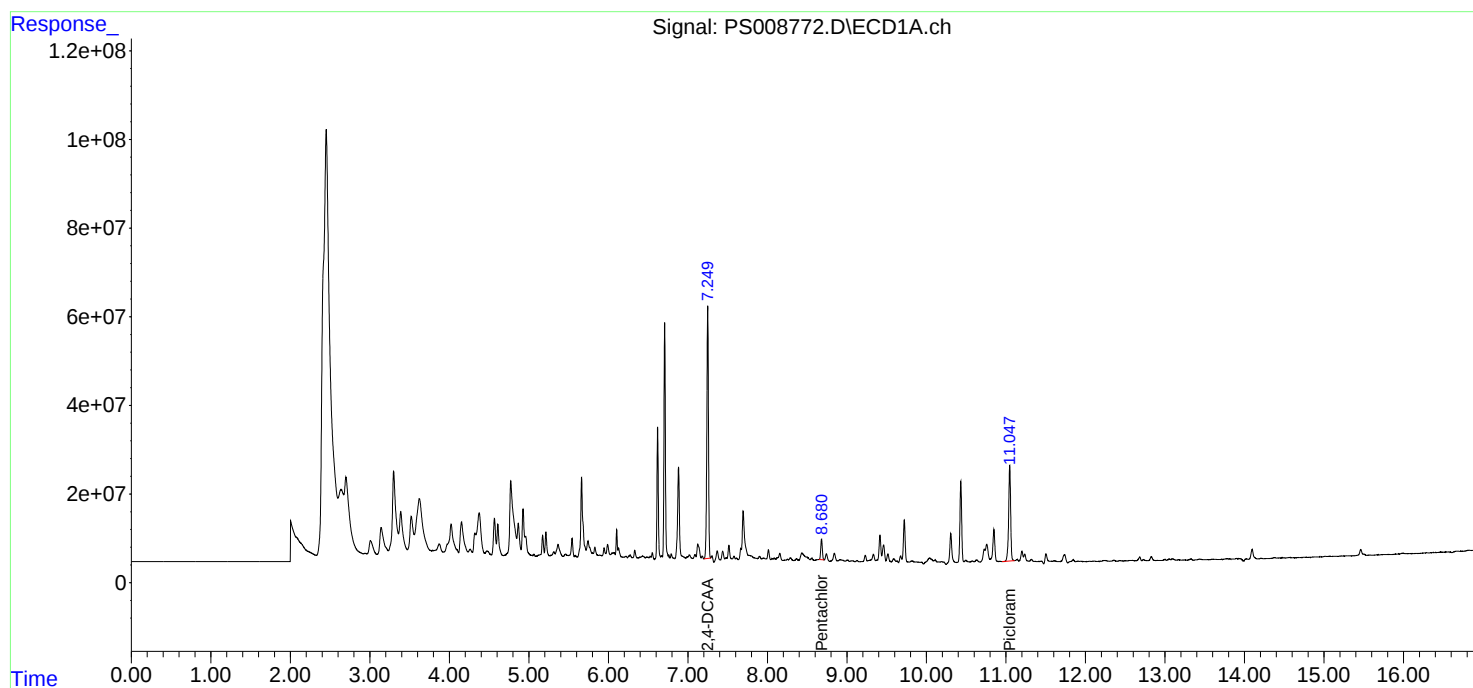


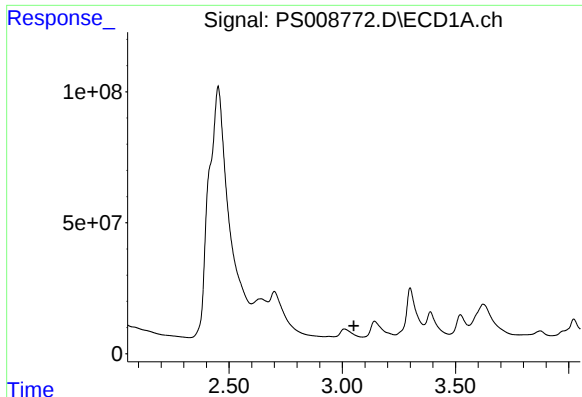

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

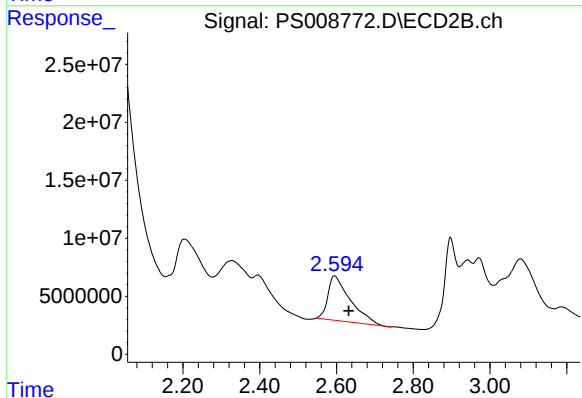


#1 Dalapon

R.T.: 2.595 min
Delta R.T.: -0.037 min
Response: 155753006
Conc: 129.87 ng/ml

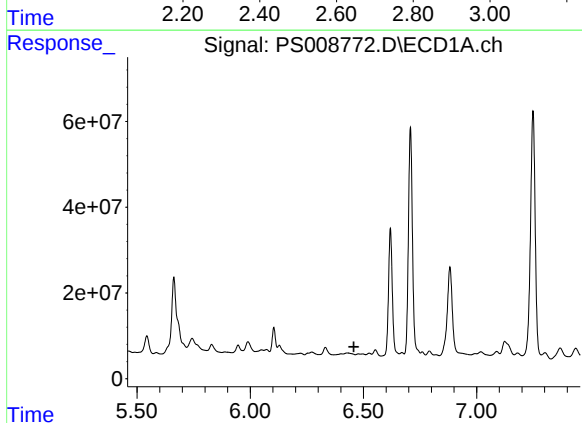


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

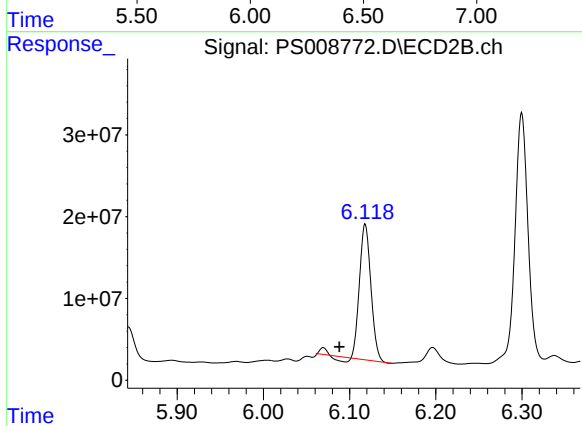

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.118 min
Delta R.T.: 0.030 min
Response: 149393903
Conc: 108.58 ng/ml

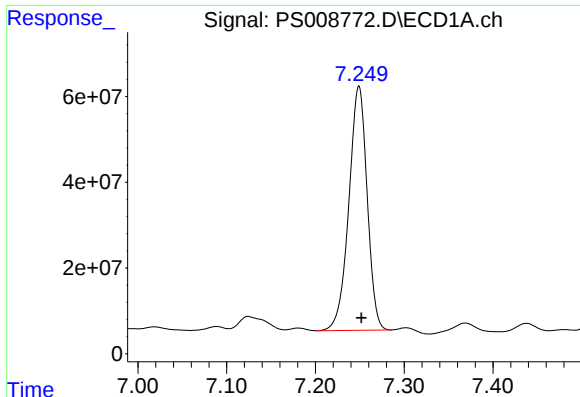

#4 2,4-DCAA


R.T.: 7.249 min
Delta R.T.: -0.003 min
Response: 815071979
Conc: 379.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

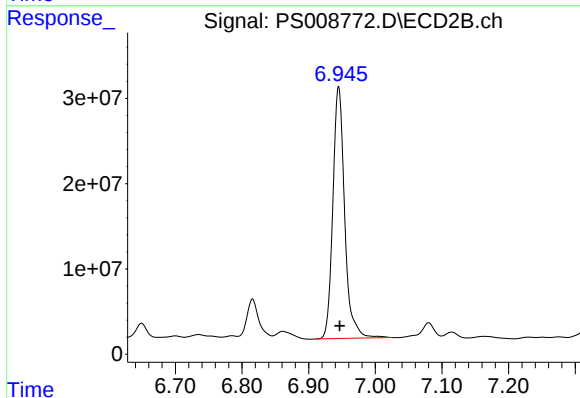


#4 2,4-DCAA

R.T.: 6.945 min
Delta R.T.: -0.002 min
Response: 364126234
Conc: 392.88 ng/ml

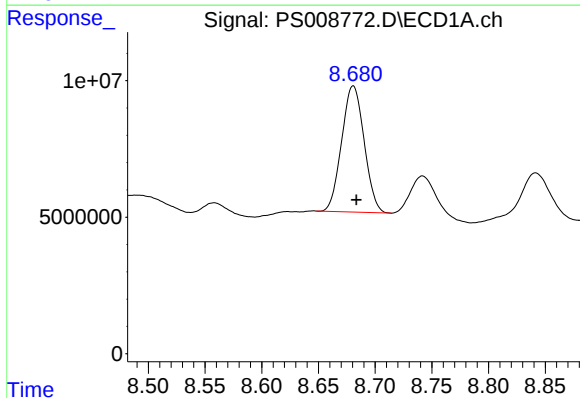


#10 Pentachlorophenol

R.T.: 8.681 min
Delta R.T.: -0.003 min
Response: 63750232
Conc: 2.24 ng/ml

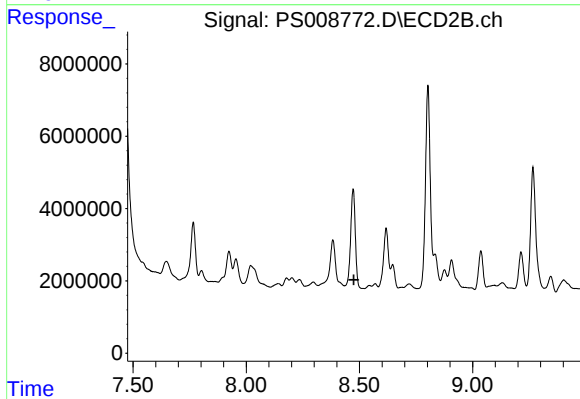

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 8.475 min
Response: 0
Conc: N.D.

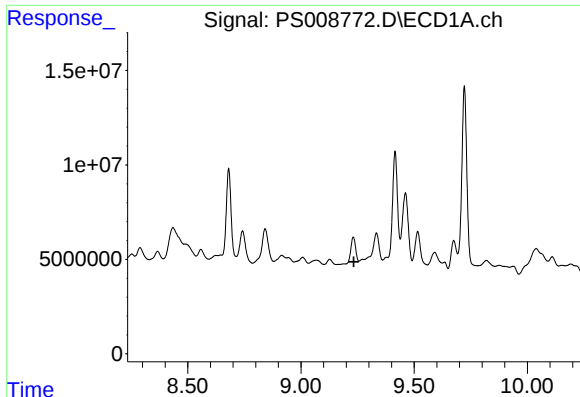

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.234 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

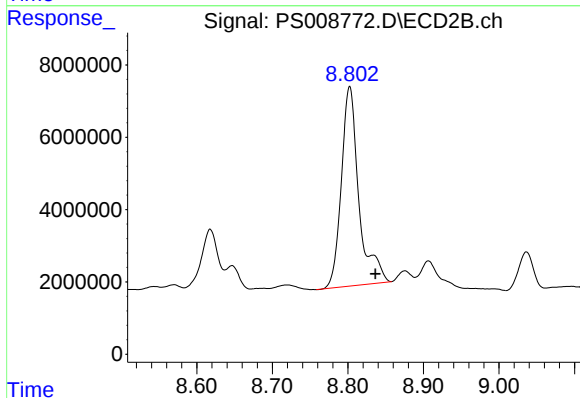


#11 2,4,5-TP (SILVEX)

R.T.: 8.802 min
Delta R.T.: -0.034 min
Response: 89028557
Conc: 17.37 ng/ml

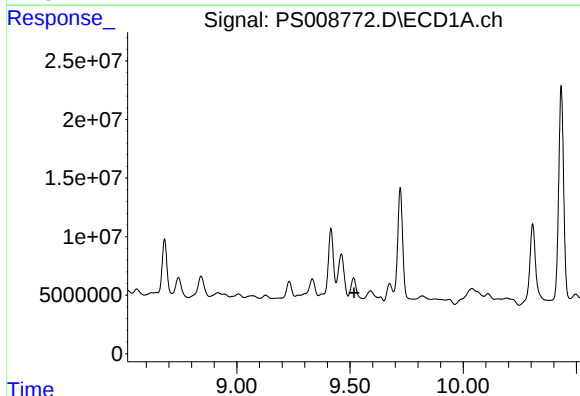


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.517 min
Response: 0
Conc: N.D.

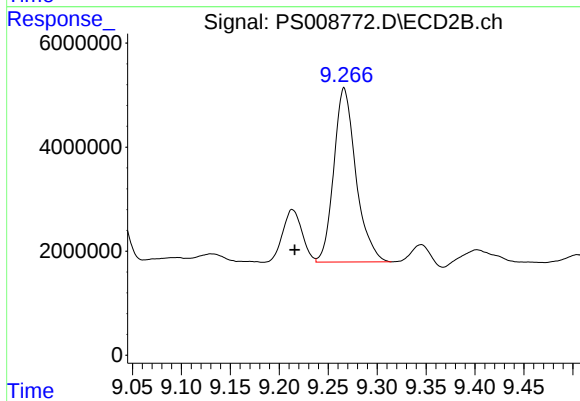

#12 2,4,5-T


R.T.: 9.266 min
Delta R.T.: 0.051 min
Response: 52635070
Conc: 10.19 ng/ml

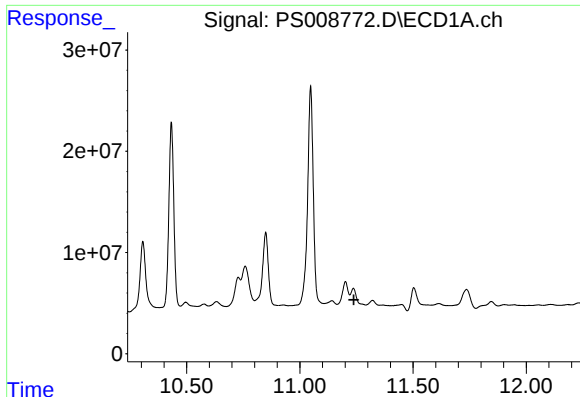

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

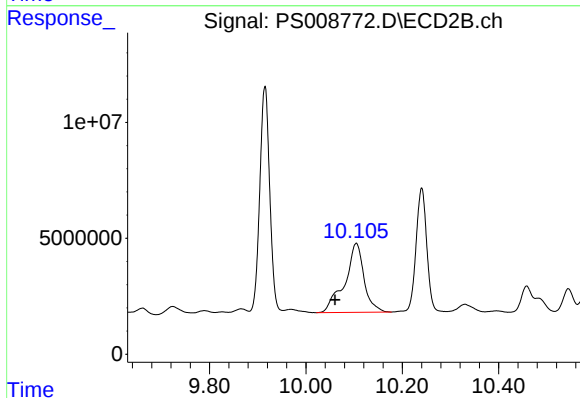


#14 DINOSEB

R.T.: 10.104 min
Delta R.T.: 0.044 min
Response: 82689168
Conc: 22.51 ng/ml

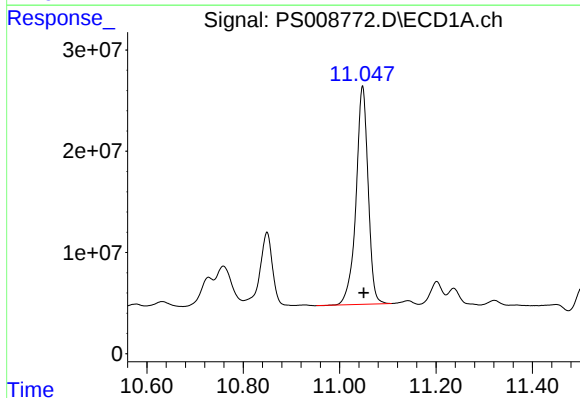


#15 Picloram

R.T.: 11.048 min
Delta R.T.: -0.002 min
Response: 374220806
Conc: 24.71 ng/ml

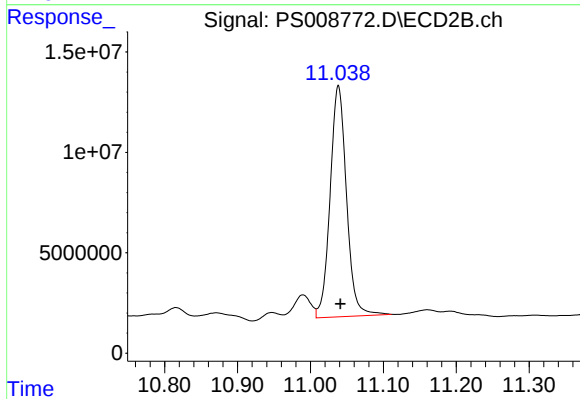

#15 Picloram


R.T.: 11.038 min
Delta R.T.: -0.003 min
Response: 179956844
Conc: 23.84 ng/ml

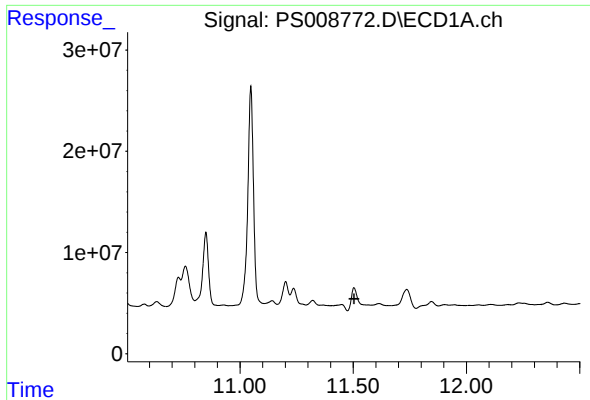

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

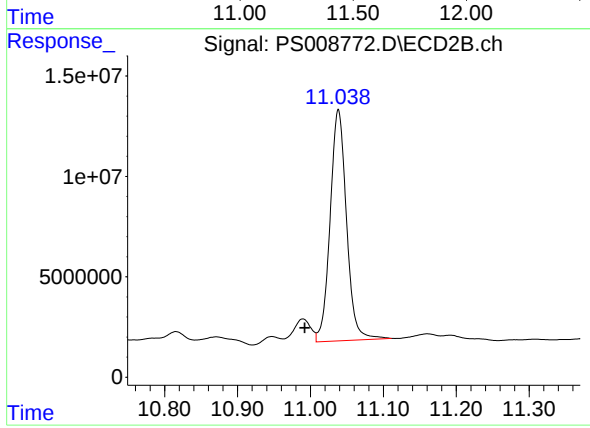

#16 DCPA

R.T.: 11.038 min
Delta R.T.: 0.046 min
Response: 179956844
Conc: 27.67 ng/ml