

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020724\
 Data File : PS025829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2024 17:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 00:42:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 06 15:37:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.348	6.754	743.8E6	381.0E6	527.018	541.615
Target Compounds							
1) T	Dalapon	0.000	2.560	0	3248467	N.D.	2.929
2) T	3,5-DICHL...	5.691	0.000	5127968	0	2.379	N.D. #
5) T	DICAMBA	0.000	6.952	0	7682976	N.D.	2.532
6) T	MCP	0.000	6.952f	0	7682976	N.D.	3.755
7) T	MCPA	6.718f	7.210	18014609	66708	3.346	<MDL #
8) T	DICHLORPROP	0.000	7.560	0	8006671	N.D.	10.026
9) T	2,4-D	7.247	7.769	13900533	80447	7.822	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS020724\
Data File : PS025829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2024 17:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 00:42:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS020624.M
Quant Title : 8080.M
QLast Update : Tue Feb 06 15:37:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

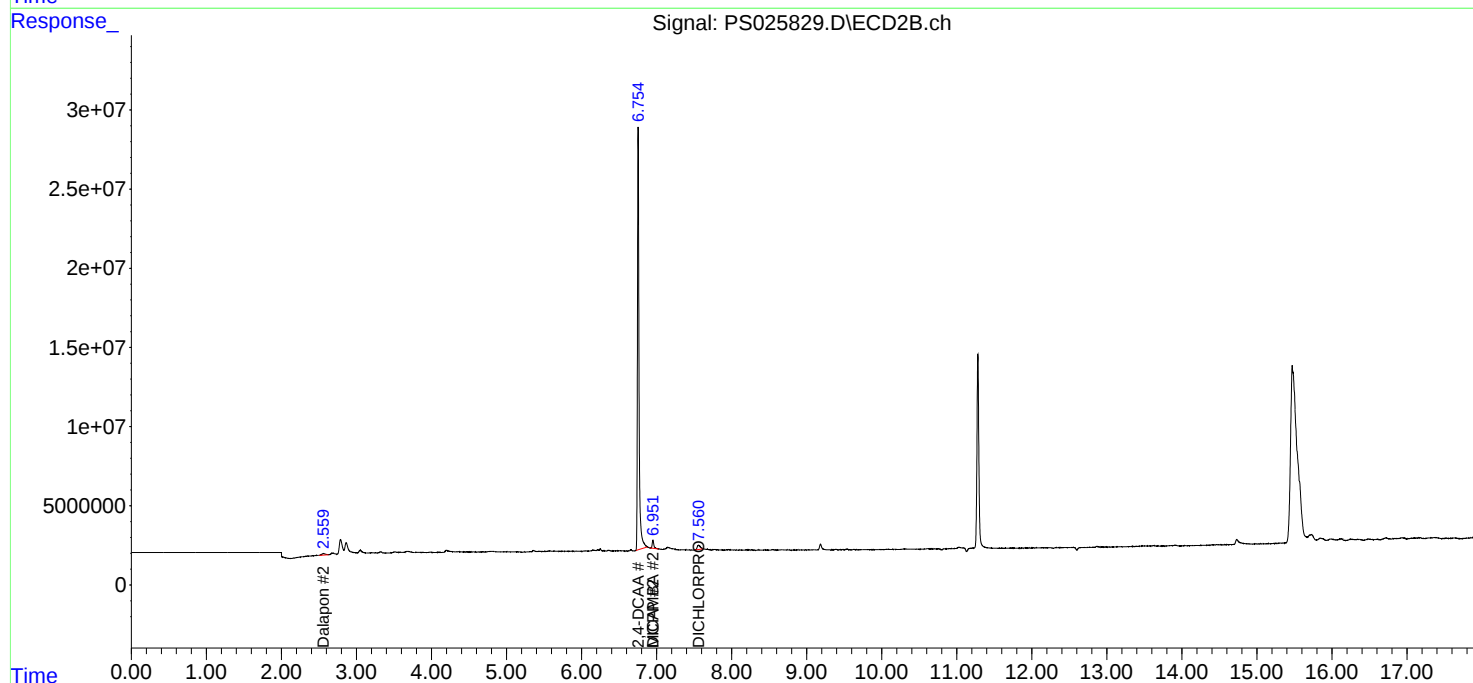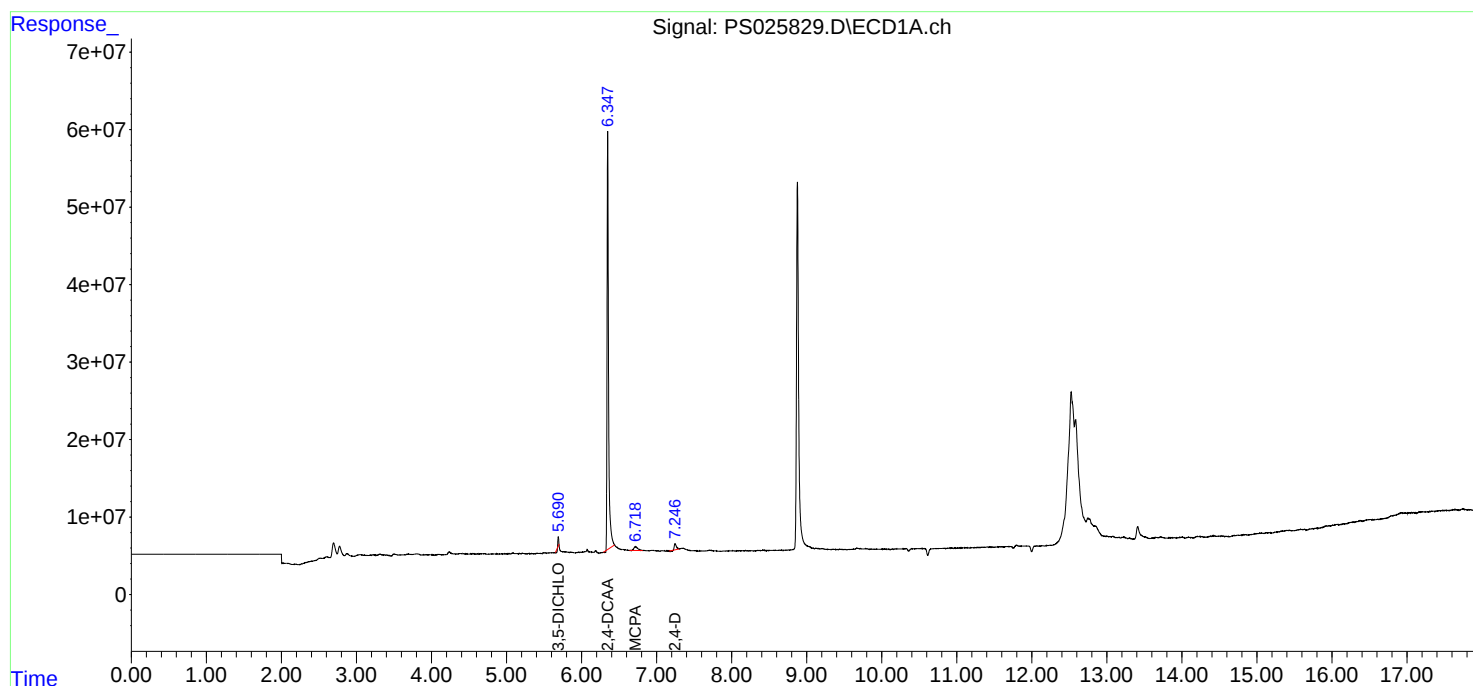


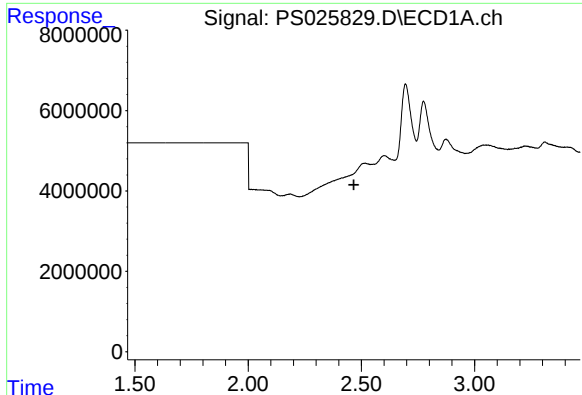

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

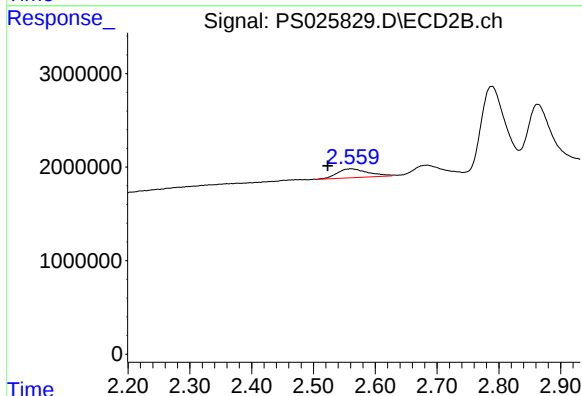


#1 Dalapon

R.T.: 2.560 min
Delta R.T.: 0.037 min
Response: 3248467
Conc: 2.93 ng/ml

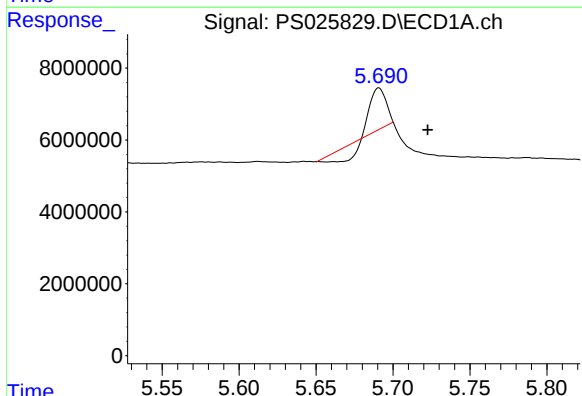


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.691 min
Delta R.T.: -0.032 min
Response: 5127968
Conc: 2.38 ng/ml

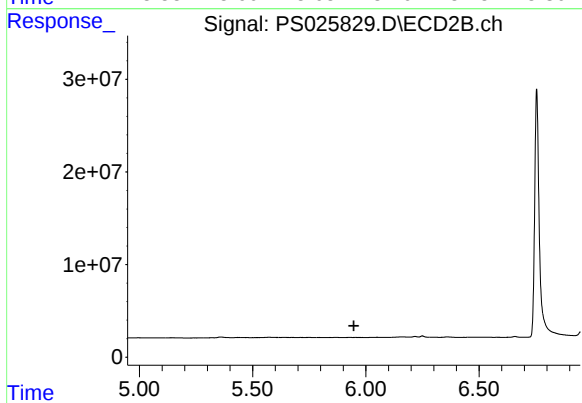

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

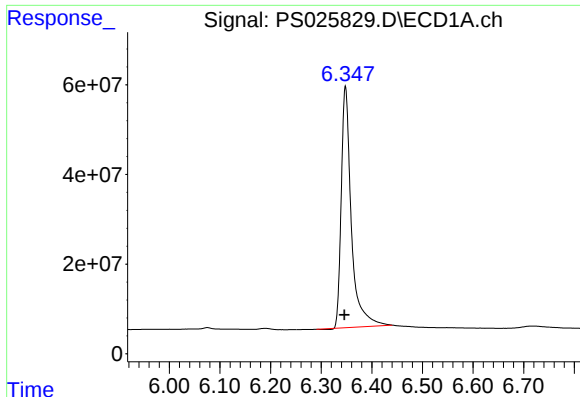

#4 2,4-DCAA


R.T.: 6.348 min
Delta R.T.: 0.002 min
Response: 743755019
Conc: 527.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

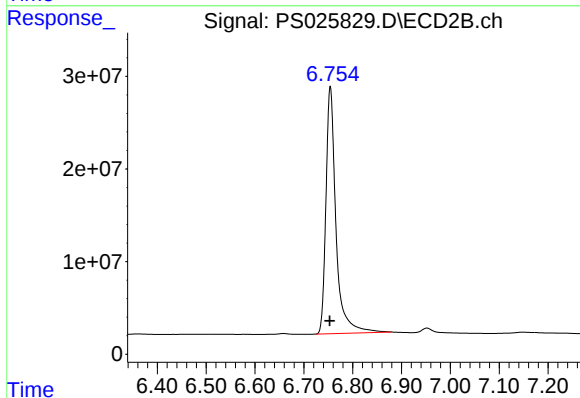


#4 2,4-DCAA

R.T.: 6.754 min
Delta R.T.: 0.000 min
Response: 380995805
Conc: 541.62 ng/ml

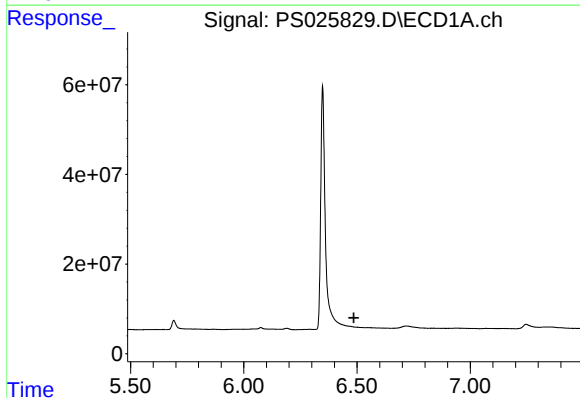


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

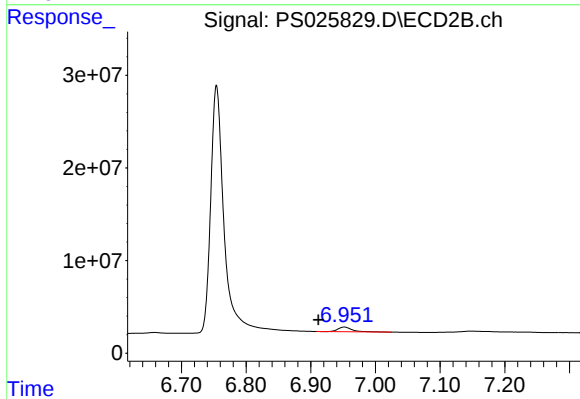

#5 DICAMBA


R.T.: 6.952 min
Delta R.T.: 0.040 min
Response: 7682976
Conc: 2.53 ng/ml

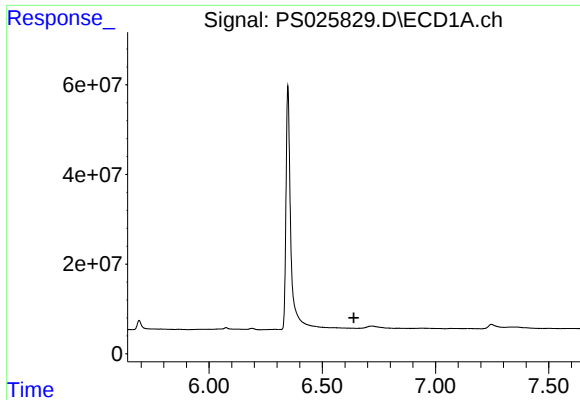

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

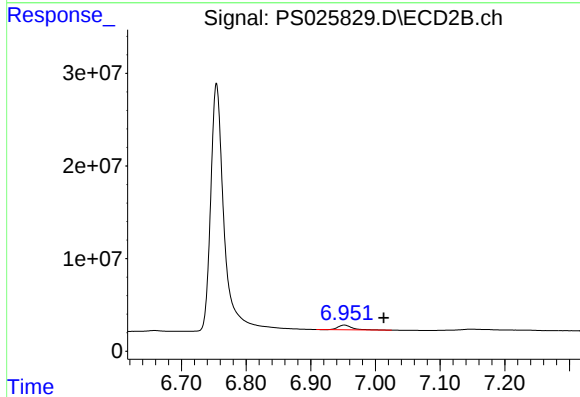


#6 MCPP

R.T.: 6.952 min
Delta R.T.: -0.061 min
Response: 7682976
Conc: 3.76 ug/ml

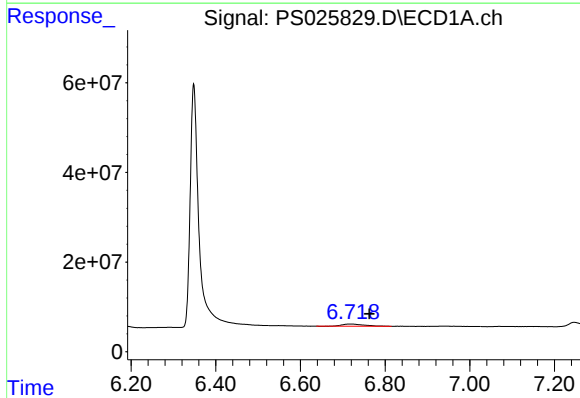


#7 MCPA

R.T.: 6.718 min
Delta R.T.: -0.045 min
Response: 18014609
Conc: 3.35 ug/ml

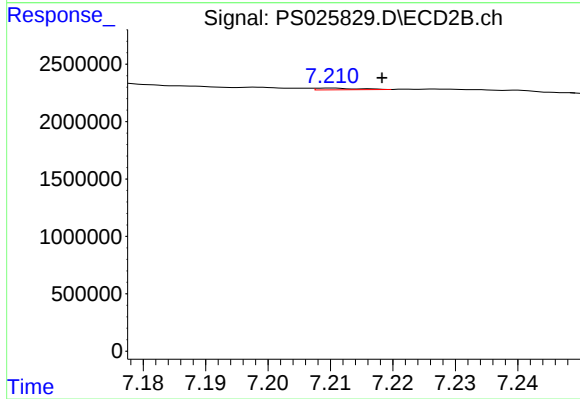

#7 MCPA


R.T.: 7.210 min
Delta R.T.: -0.008 min
Response: 66708
Conc: N.D.

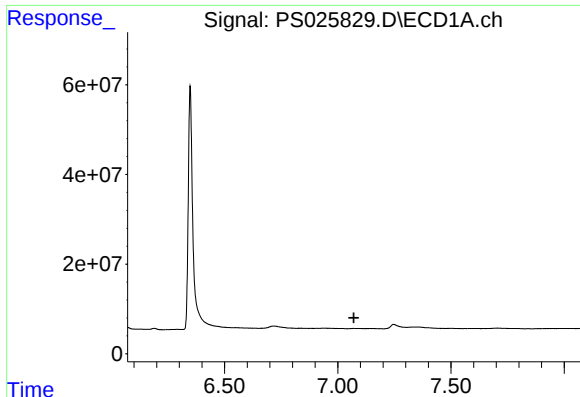

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

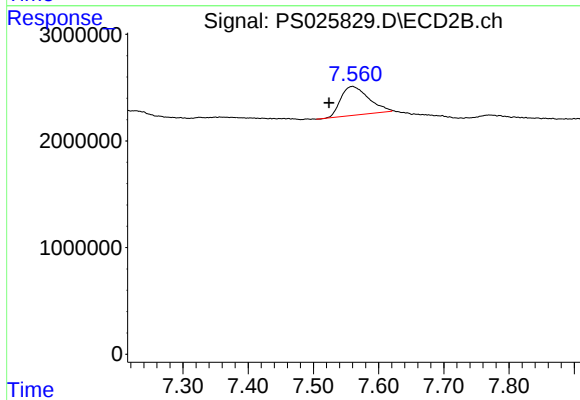


#8 DICHLORPROP

R.T.: 7.560 min
Delta R.T.: 0.037 min
Response: 8006671
Conc: 10.03 ng/ml

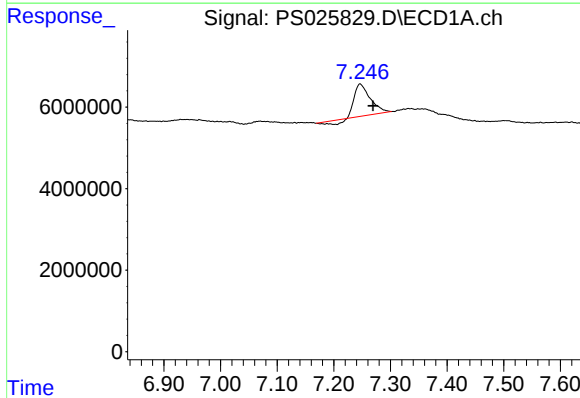

#9 2,4-D

R.T.: 7.247 min
Delta R.T.: -0.022 min
Response: 13900533
Conc: 7.82 ng/ml

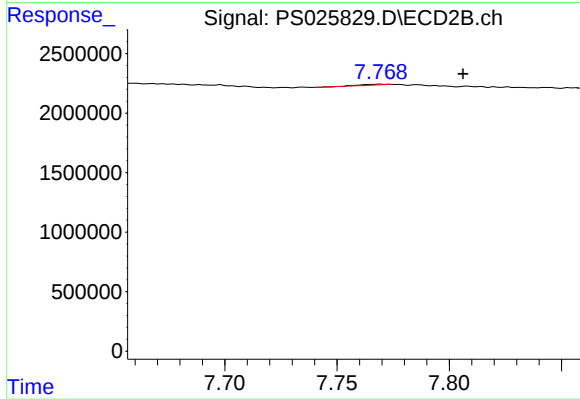

#9 2,4-D

R.T.: 7.769 min
Delta R.T.: -0.037 min
Response: 80447
Conc: N.D.